

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120425\
 Data File : PL097779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 16:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 01:02:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 26 07:07:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	2.801	111.9E6	155.3E6	21.830	21.717
28)	SA Decachlor...	8.967	7.952	75308894	130.2E6	23.463	27.657
Target Compounds							
15)	B Endosulfa...	6.701f	0.000	15819625	0	3.118	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120425\
Data File : PL097779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 16:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 01:02:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Wed Nov 26 07:07:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

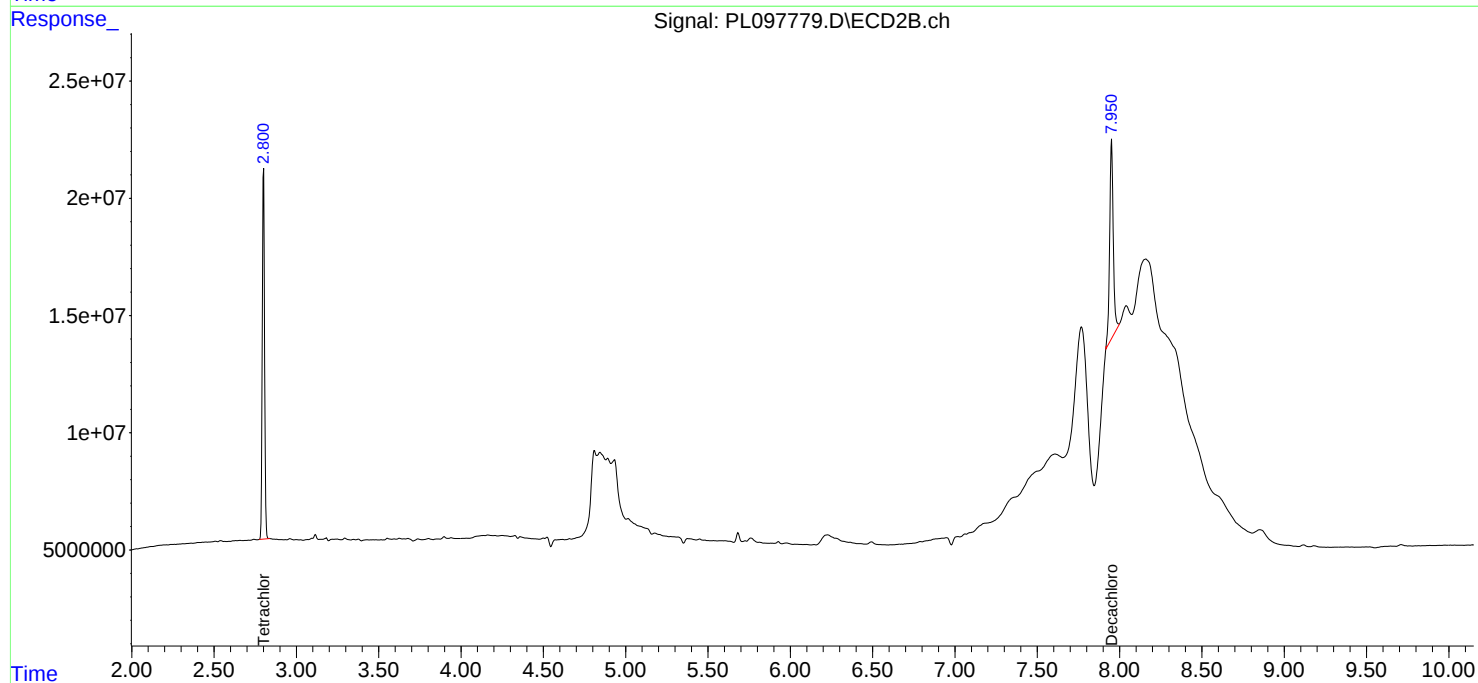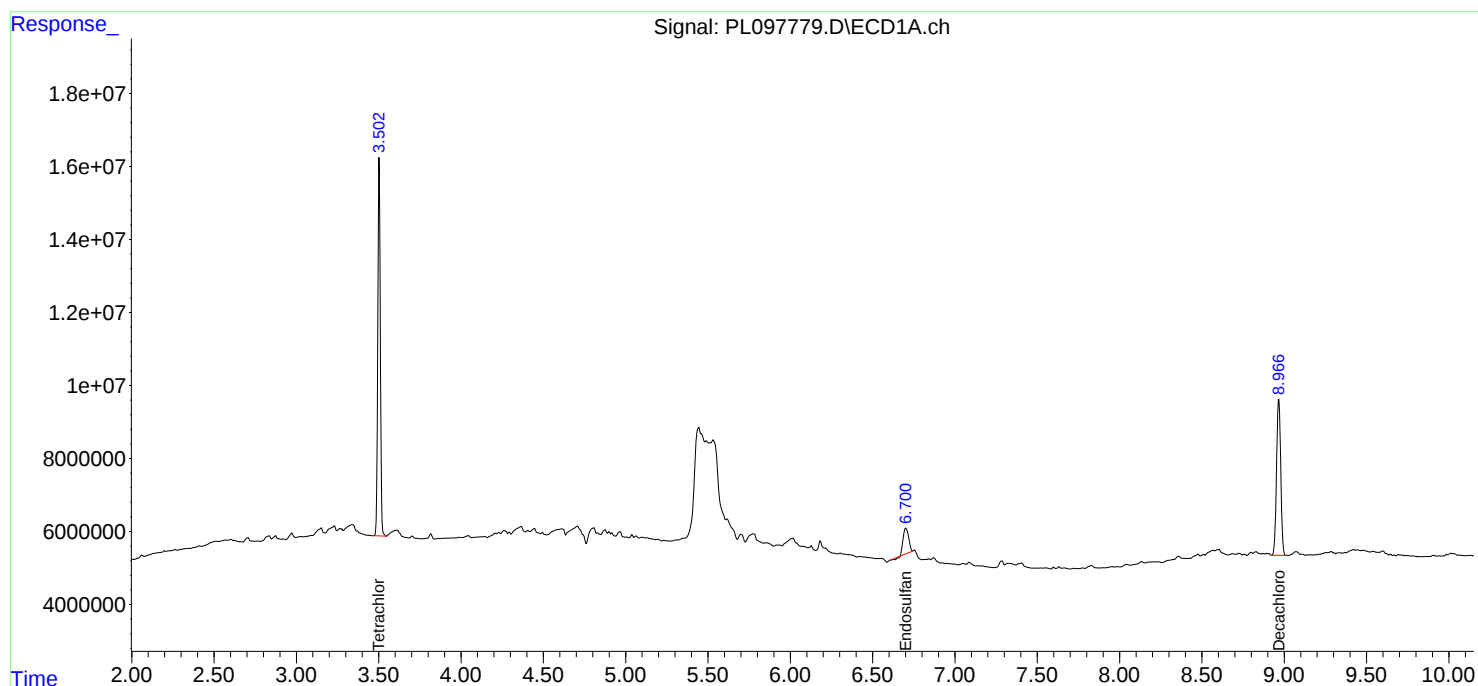


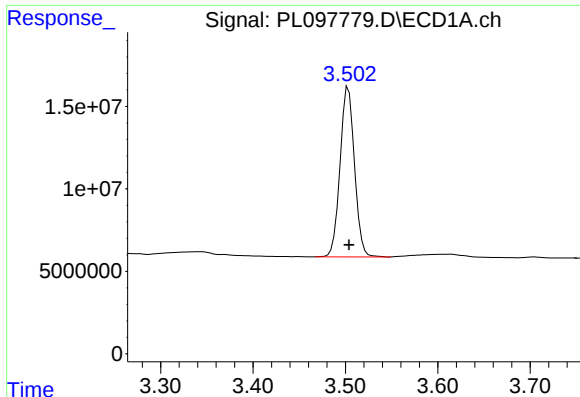

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 111850230
Conc: 21.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

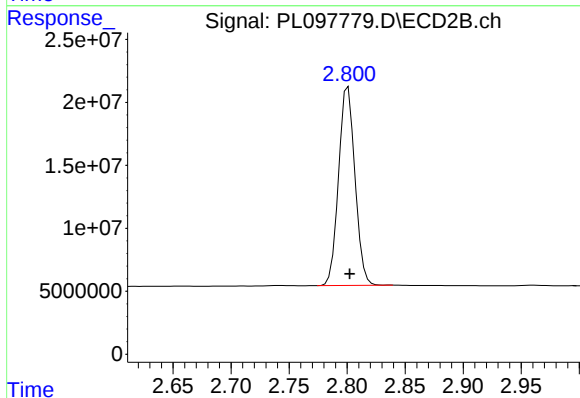


#1 Tetrachloro-m-xylene

R.T.: 2.801 min
Delta R.T.: -0.001 min
Response: 155338342
Conc: 21.72 ng/ml

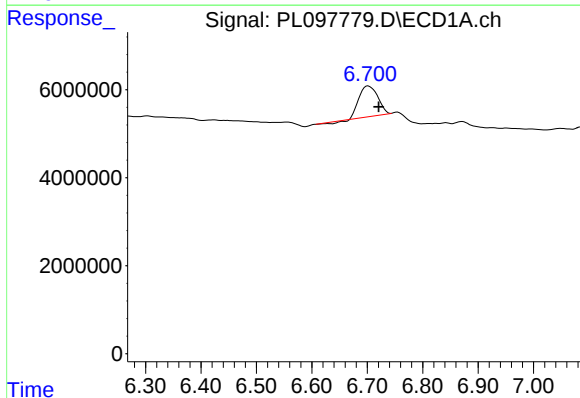


#15 Endosulfan II

R.T.: 6.701 min
Delta R.T.: -0.019 min
Response: 15819625
Conc: 3.12 ng/ml

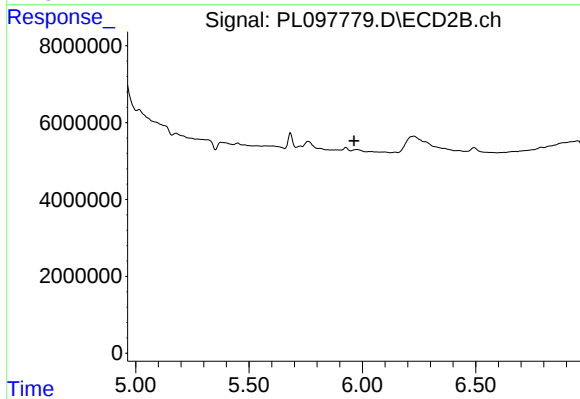

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.963 min
Response: 0
Conc: N.D.

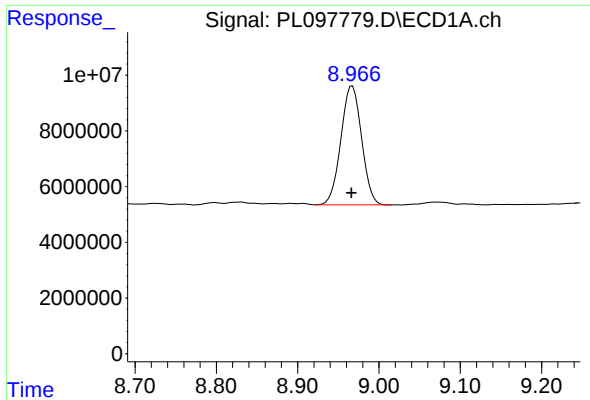

#28 Decachlorobiphenyl

R.T.: 8.967 min
Delta R.T.: 0.001 min
Response: 75308894
Conc: 23.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

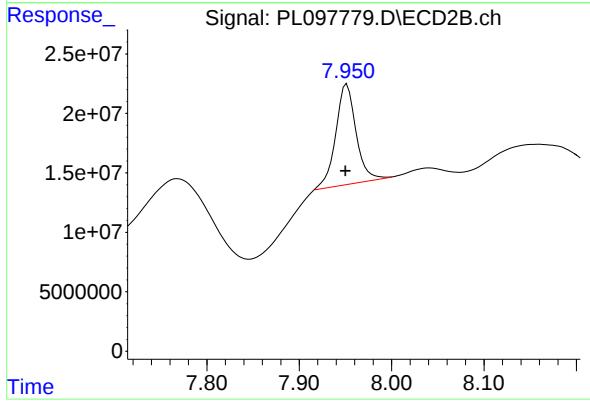

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: 0.002 min
Response: 130174750
Conc: 27.66 ng/ml