

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120425\
 Data File : PL097776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 15:12
 Operator : AR\AJ
 Sample : Q3768-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20071

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/05/2025
 Supervised By : mohammad ahmed 12/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 15:32:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 26 07:07:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530f	2.844f	23098497	28676042	4.508m	4.009m
28)	SA Decachlor...	8.967	7.951	38240938	56883003	11.914	12.085

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120425\
Data File : PL097776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 15:12
Operator : AR\AJ
Sample : Q3768-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20071


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/05/2025
Supervised By : mohammad ahmed 12/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 15:32:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Wed Nov 26 07:07:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

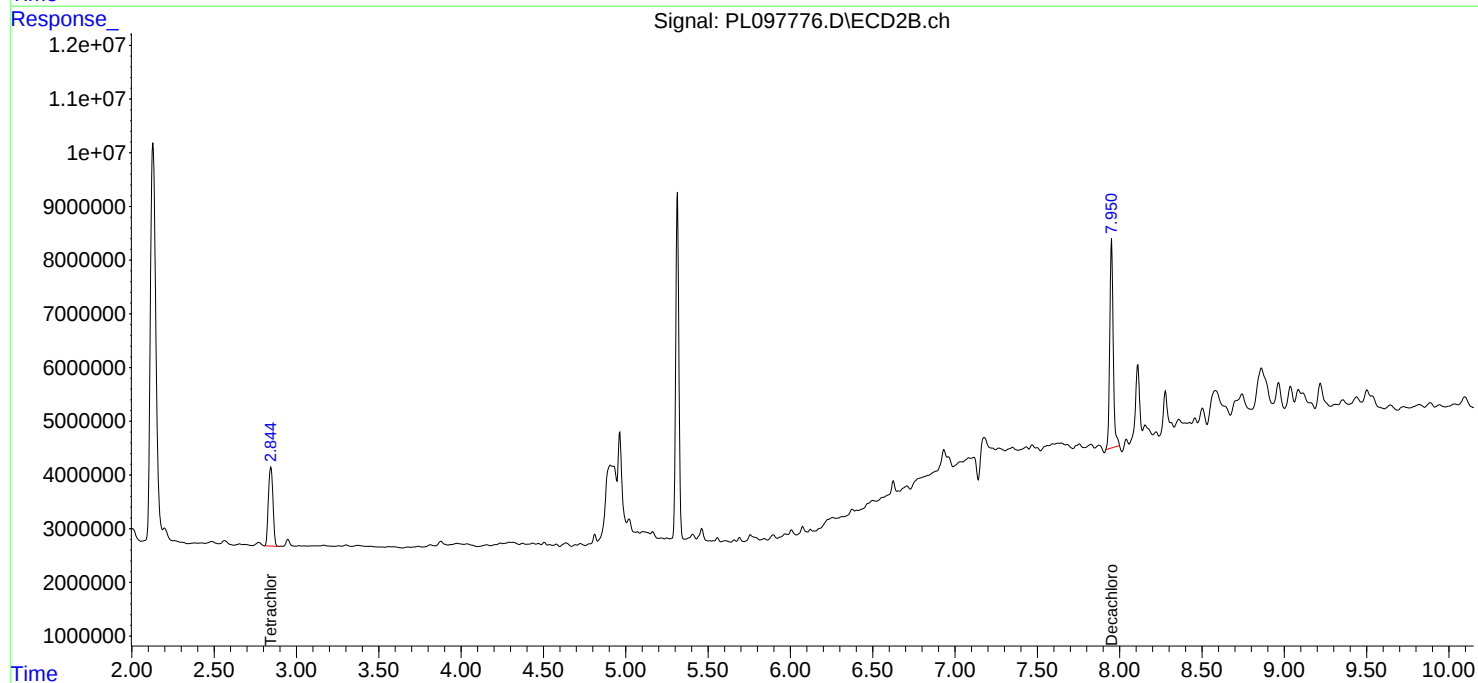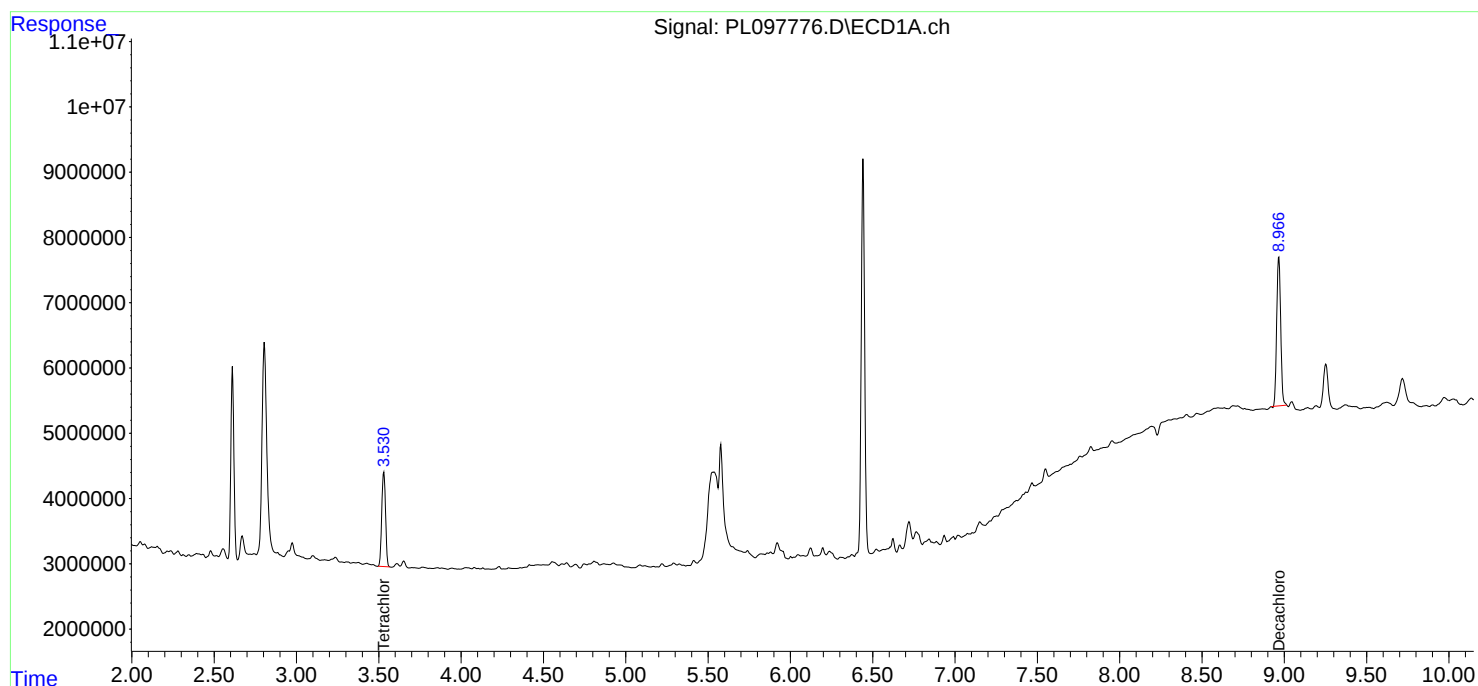

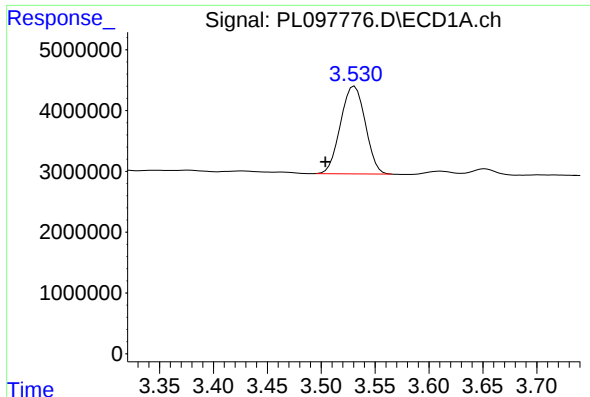


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.026 min
Response: 23098497
Conc: 4.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
20071


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/05/2025
Supervised By :mohammad ahmed 12/08/2025

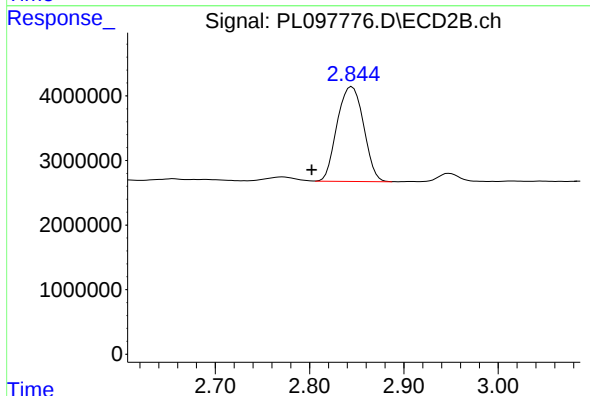


#1 Tetrachloro-m-xylene

R.T.: 2.844 min
Delta R.T.: 0.041 min
Response: 28676042
Conc: 4.01 ng/ml m

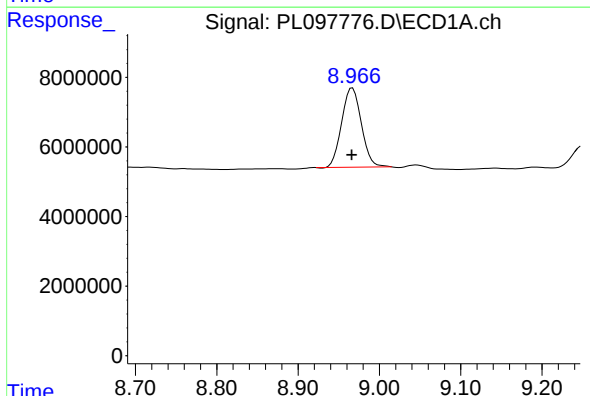

#28 Decachlorobiphenyl

R.T.: 8.967 min
Delta R.T.: 0.000 min
Response: 38240938
Conc: 11.91 ng/ml

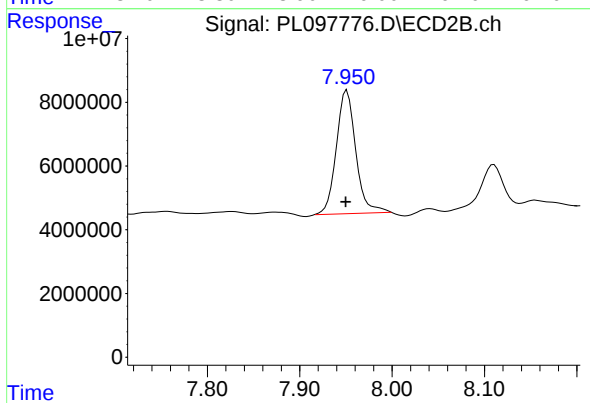

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.001 min
Response: 56883003
Conc: 12.09 ng/ml