

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 09:26
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:07:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.408f	0.000	2561388	0	0.723	N.D.	#
9) A	Endosulfan I	0.000	6.307f	0	10288584	N.D.	3.258	#
10) B	gamma-Chl...	0.000	6.166f	0	9854082	N.D.	2.895	#
11) B	alpha-Chl...	0.000	6.307	0	10288584	N.D.	3.077	#
14) MA	Endrin	5.959f	0.000	1817401	0	0.278	N.D.	#
18) B	Endrin al...	0.000	7.119f	0	2231723	N.D.	0.973	#
19) B	Endosulfa...	6.703	7.324f	-2617477	2332539	N.D.	0.839	
25)	Chlordane-3	0.000	6.166	0	9854082	N.D.	20.969	#
26)	Chlordane-4	0.000	6.307	0	10288584	N.D.	18.804	#
27)	Chlordane-5	0.000	7.119	0	2231723	N.D.	23.200	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 09:26
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:07:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

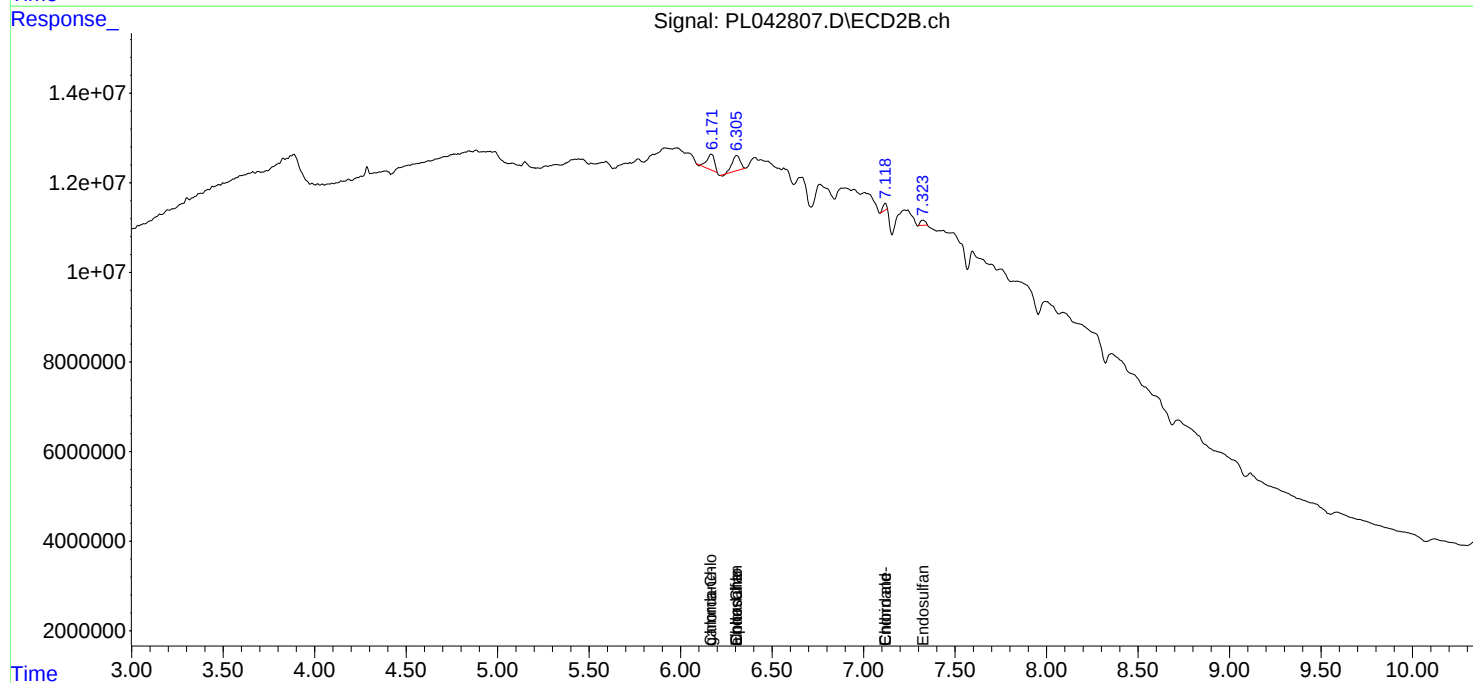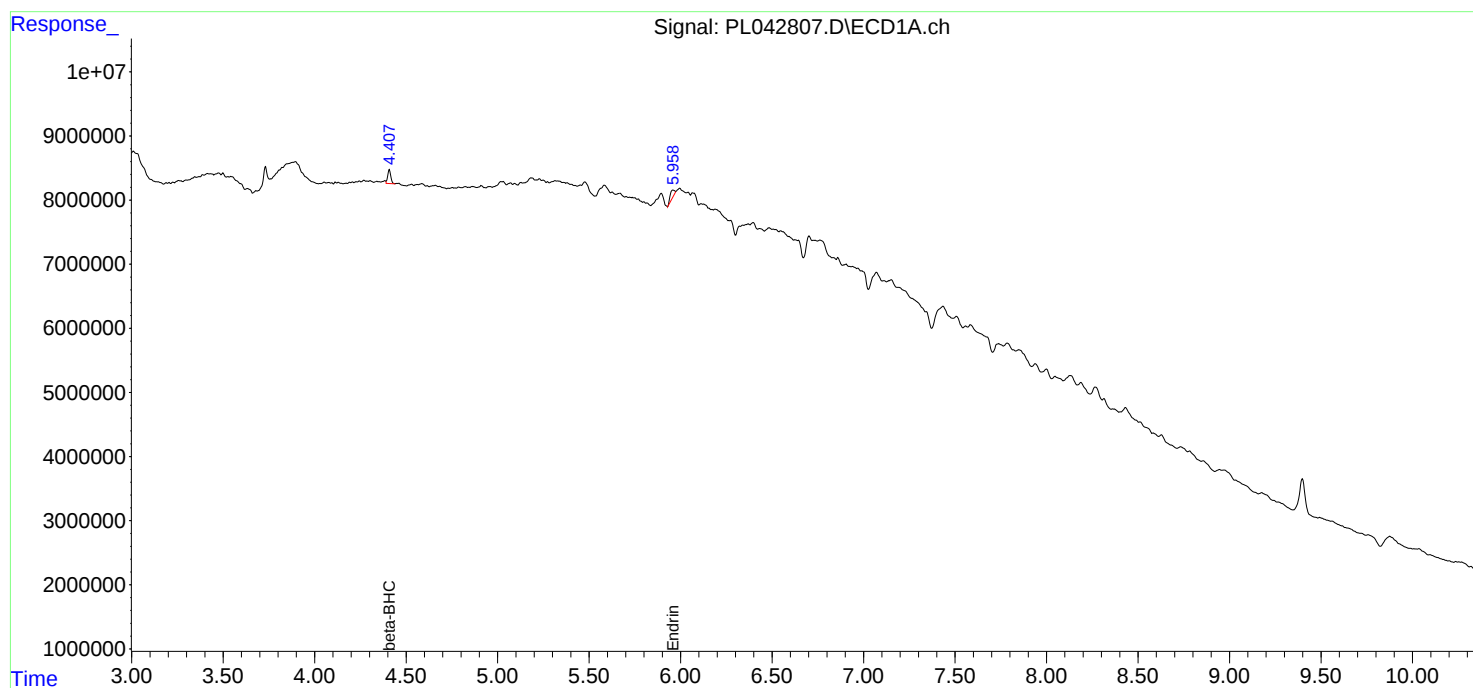


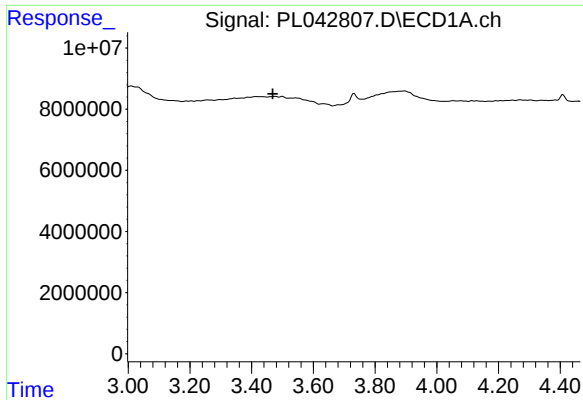

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

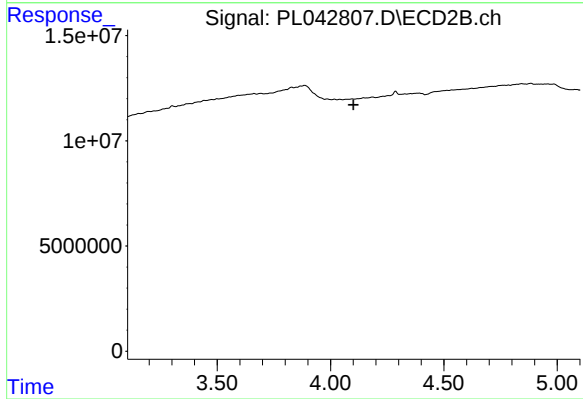


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.102 min
Response: 0
Conc: N.D.

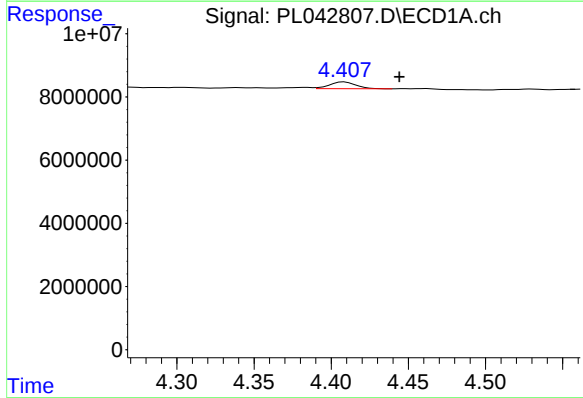


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: -0.036 min
Response: 2561388
Conc: 0.72 ng/ml

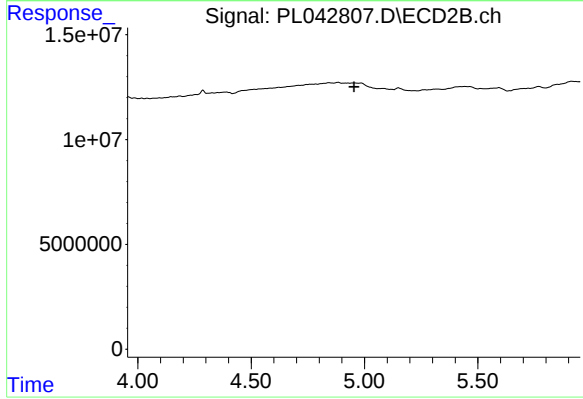

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.954 min
Response: 0
Conc: N.D.

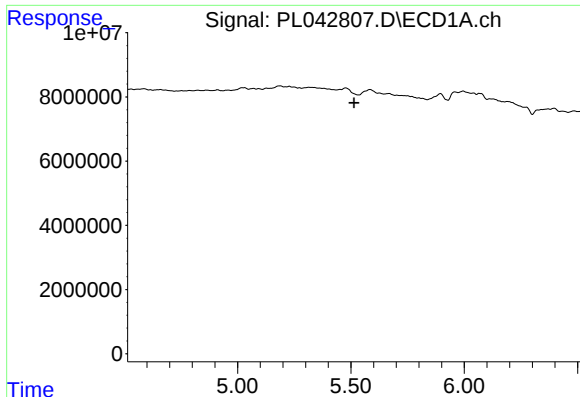

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

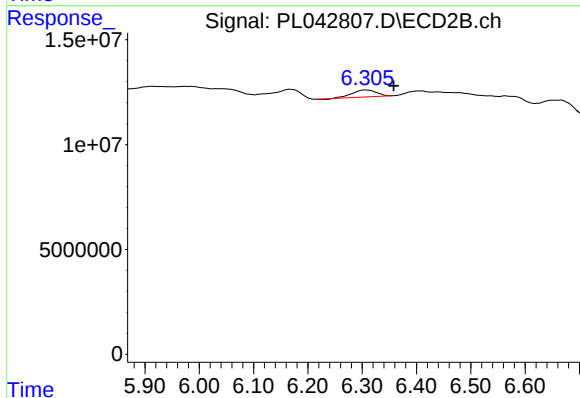


#9 Endosulfan I

R.T.: 6.307 min
Delta R.T.: -0.052 min
Response: 10288584
Conc: 3.26 ng/ml

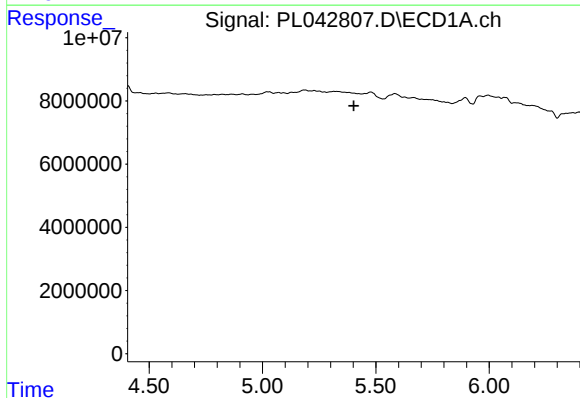


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

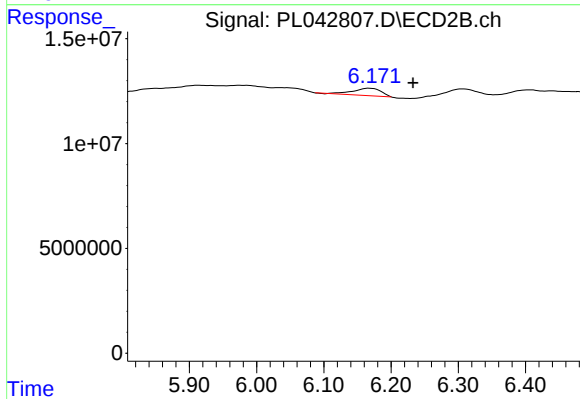

#10 gamma-Chlordane


R.T.: 6.166 min
Delta R.T.: -0.067 min
Response: 9854082
Conc: 2.89 ng/ml

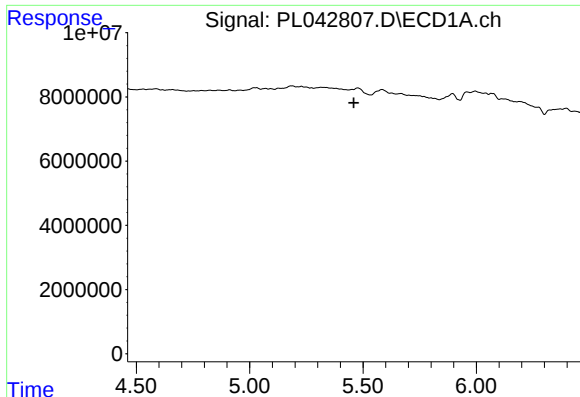

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

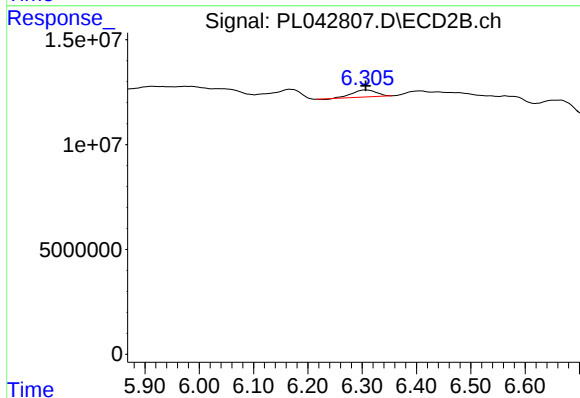


#11 alpha-Chlordane

R.T.: 6.307 min
Delta R.T.: 0.000 min
Response: 10288584
Conc: 3.08 ng/ml

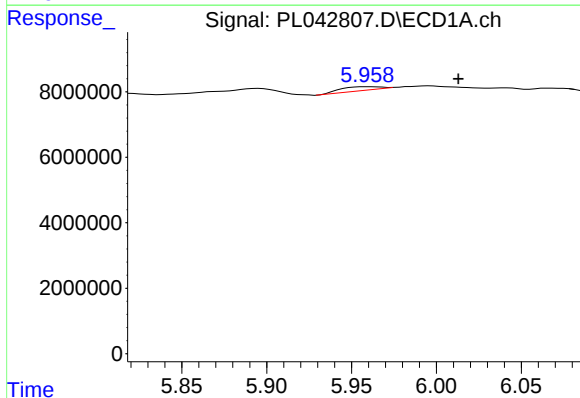


#14 Endrin

R.T.: 5.959 min
Delta R.T.: -0.054 min
Response: 1817401
Conc: 0.28 ng/ml

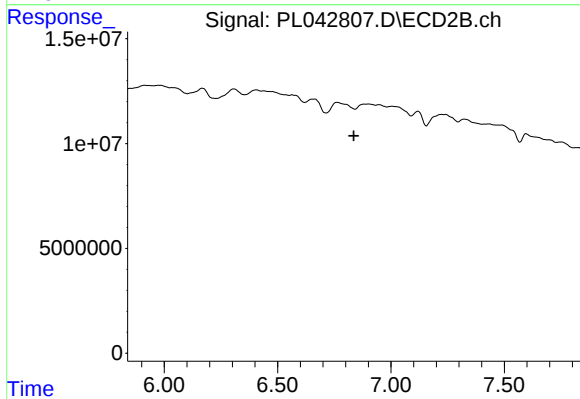

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.836 min
Response: 0
Conc: N.D.

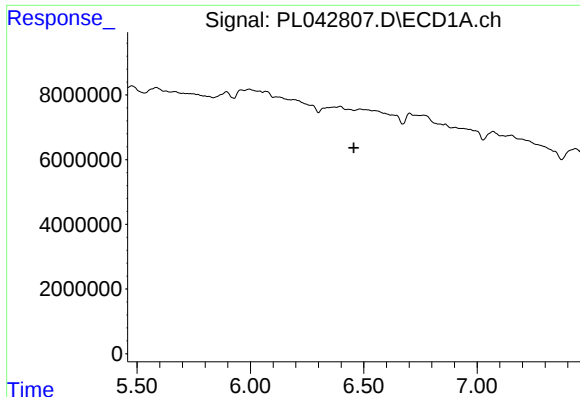

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

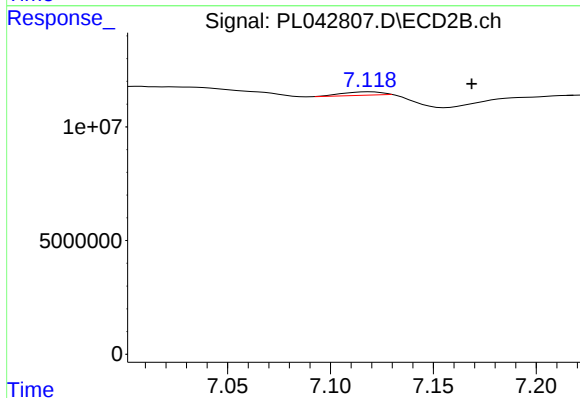


#18 Endrin aldehyde

R.T.: 7.119 min
Delta R.T.: -0.049 min
Response: 2231723
Conc: 0.97 ng/ml

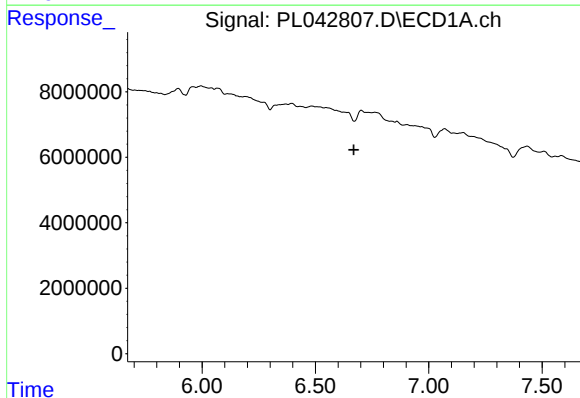


#19 Endosulfan Sulfate

R.T.: 6.703 min
Delta R.T.: 0.034 min
Response: -2617477
Conc: N.D.

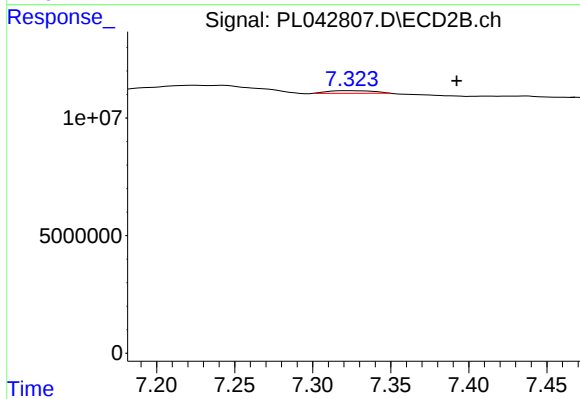

#19 Endosulfan Sulfate


R.T.: 7.324 min
Delta R.T.: -0.068 min
Response: 2332539
Conc: 0.84 ng/ml

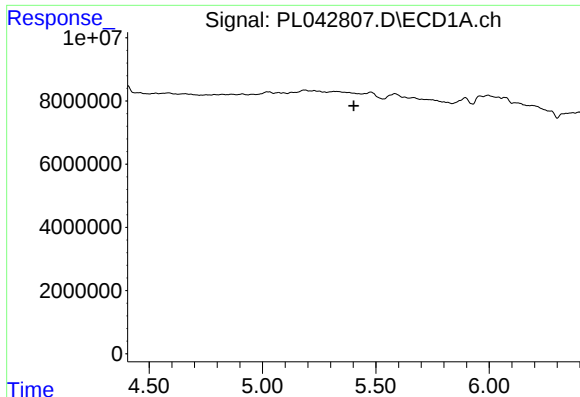

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

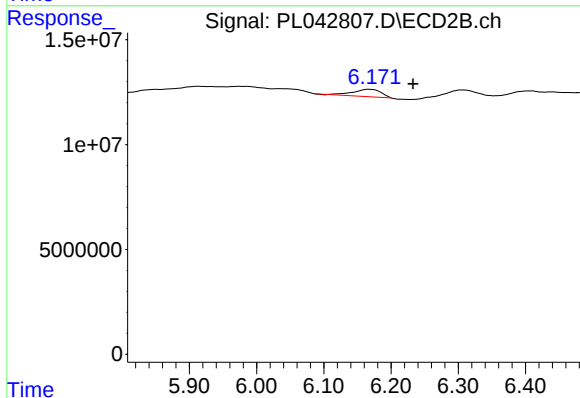


#25 Chlordane-3

R.T.: 6.166 min
Delta R.T.: -0.066 min
Response: 9854082
Conc: 20.97 ng/ml

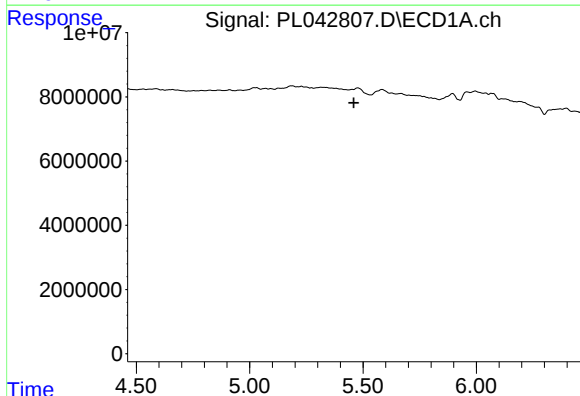


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

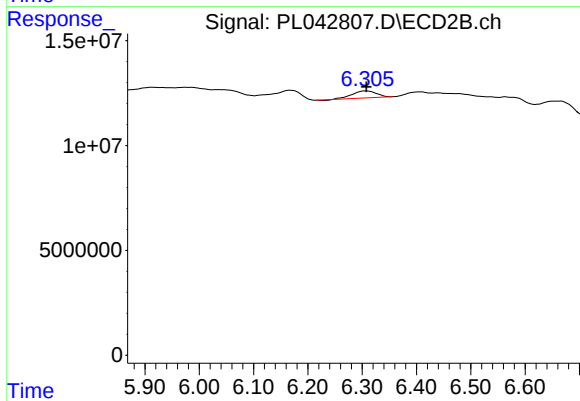

#26 Chlordane-4


R.T.: 6.307 min
Delta R.T.: -0.001 min
Response: 10288584
Conc: 18.80 ng/ml

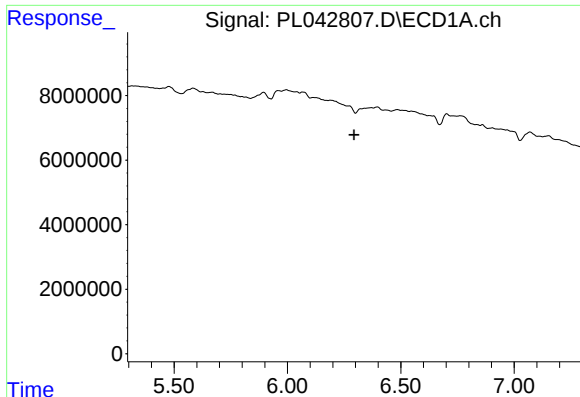

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

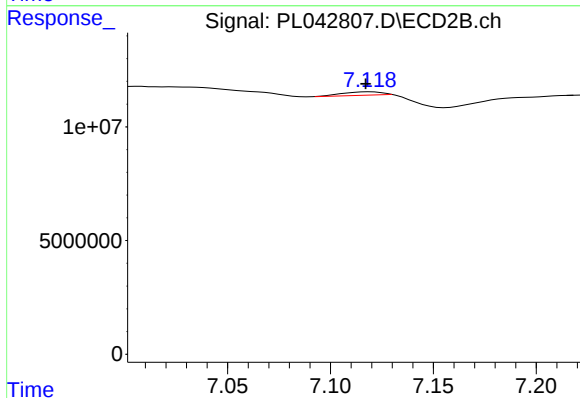


#27 Chlordane-5

R.T.: 7.119 min
Delta R.T.: 0.002 min
Response: 2231723
Conc: 23.20 ng/ml

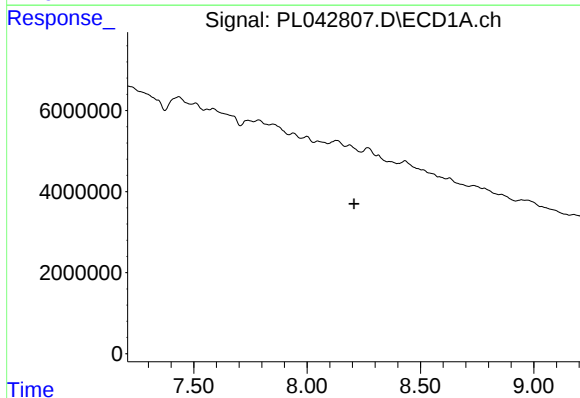

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.207 min
Response: 0
Conc: N.D.

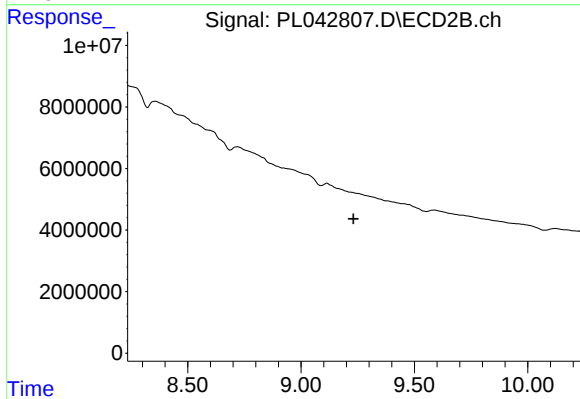

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.232 min
Response: 0
Conc: N.D.