

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 13:33
 Operator : AJ\SJ
 Sample : J6208-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:08:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	48823799	26771591	8.298	9.308
28)	SA Decachlor...	8.203	9.232	63146507	23986721	10.020	9.945
Target Compounds							
6)	B beta-BHC	4.400f	4.907f	8116891	-547349	2.291	N.D. #
9)	A Endosulfan I	0.000	6.307f	0	1147541	N.D.	0.363 #
11)	B alpha-Chl...	0.000	6.307	0	1147541	N.D.	0.343 #
12)	B 4,4'-DDE	5.622	0.000	2003268	0	0.306	N.D. #
17)	MA 4,4'-DDT	6.372	0.000	3298993	0	0.593	N.D. #
18)	B Endrin al...	6.414f	0.000	580363	0	0.112	N.D. #
19)	B Endosulfa...	6.658	0.000	1824762	0	0.292	N.D. #
20)	A Methoxychlor	6.902	0.000	2174461	0	0.689	N.D. #
21)	B Endrin ke...	7.175	7.824f	2058533	1884386	0.297	0.682 #
23)	Chlordane-1	4.400	0.000	8116891	0	29.359	N.D. #
26)	Chlordane-4	0.000	6.307	0	1147541	N.D.	2.097 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 13:33
Operator : AJ\SJ
Sample : J6208-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:08:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

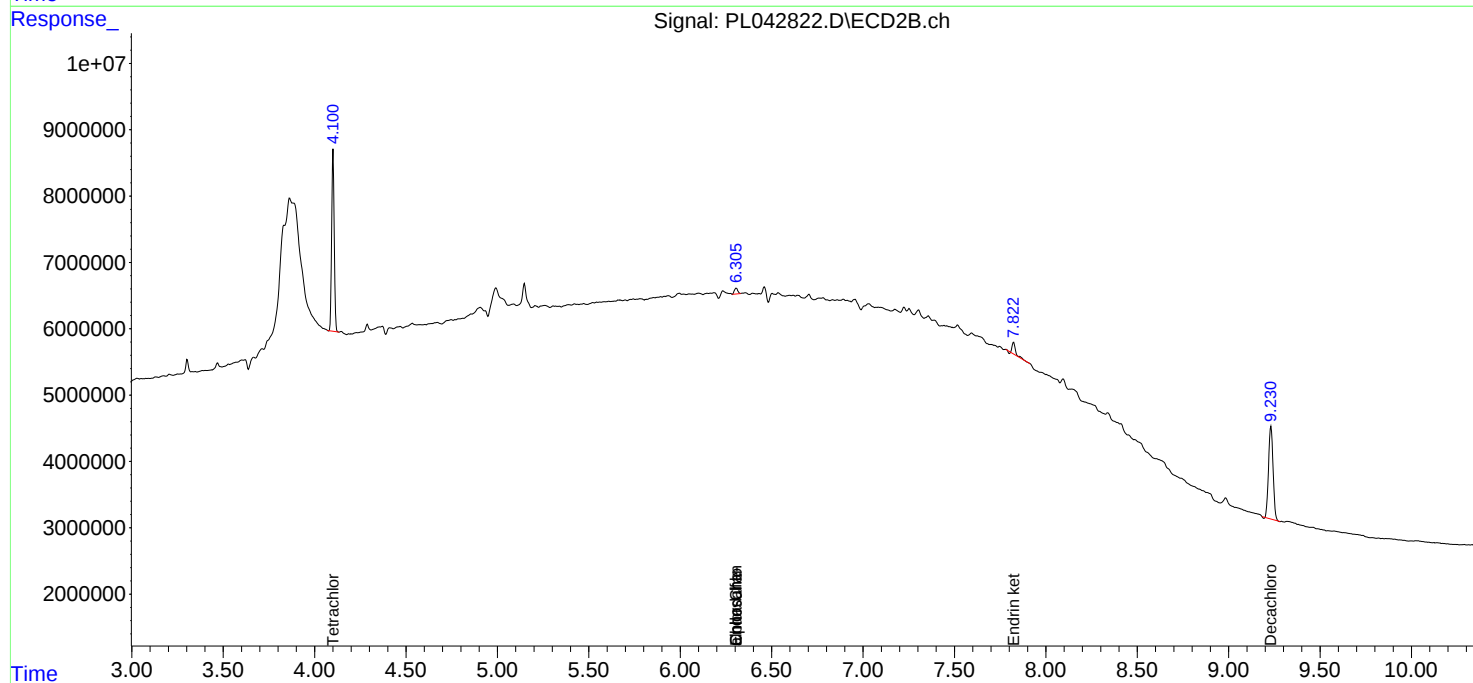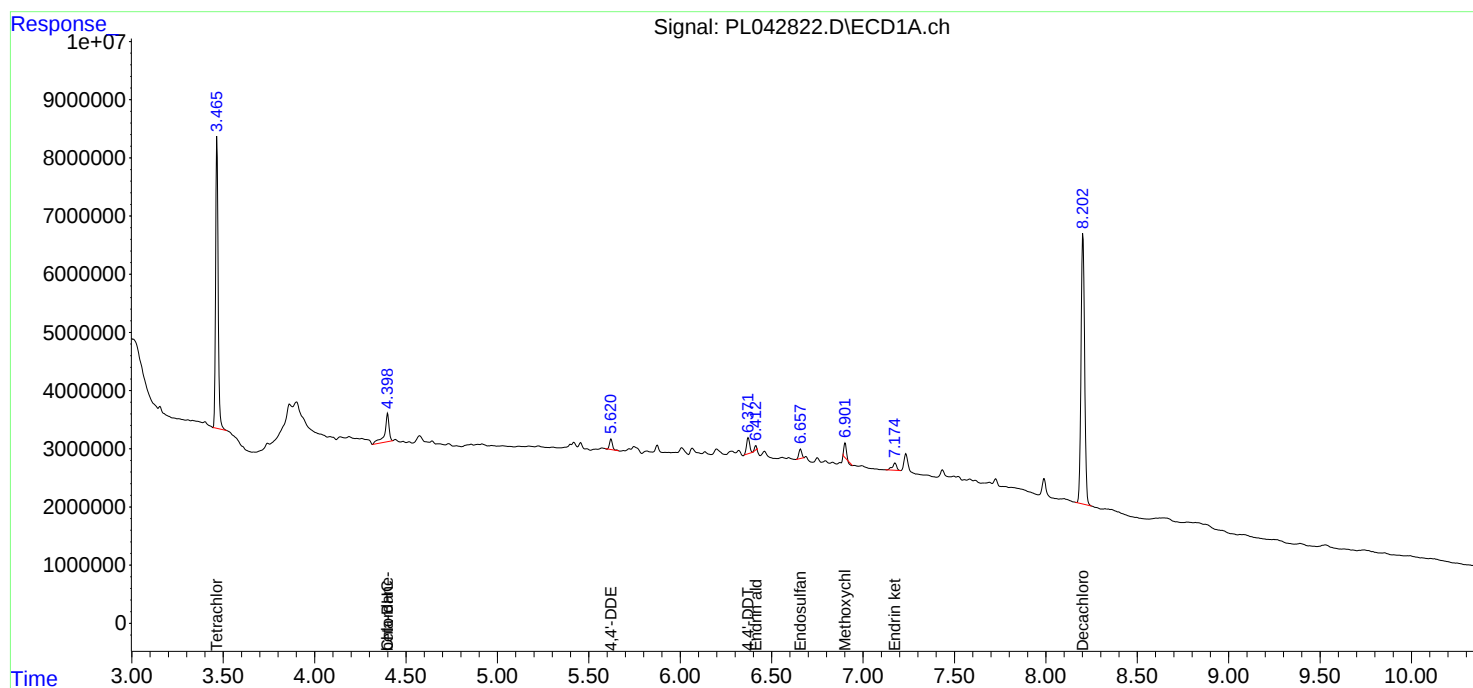


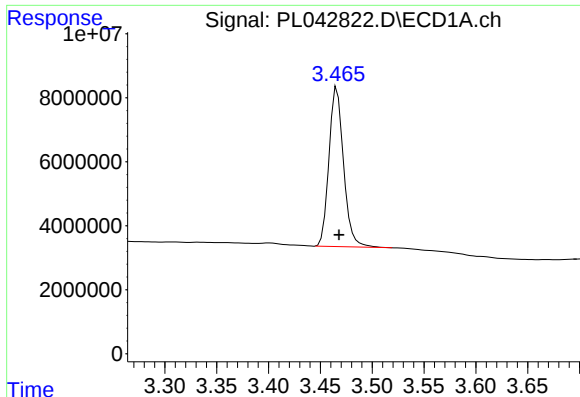

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 48823799
Conc: 8.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

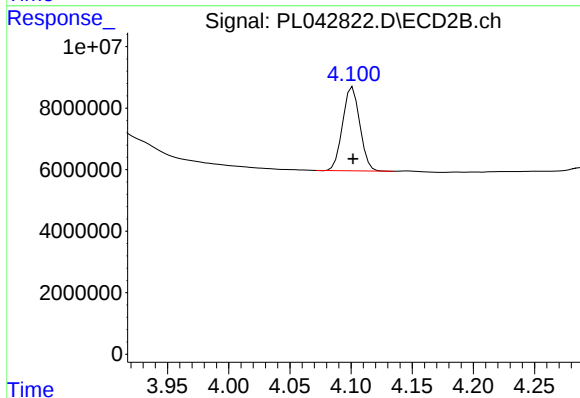


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 26771591
Conc: 9.31 ng/ml

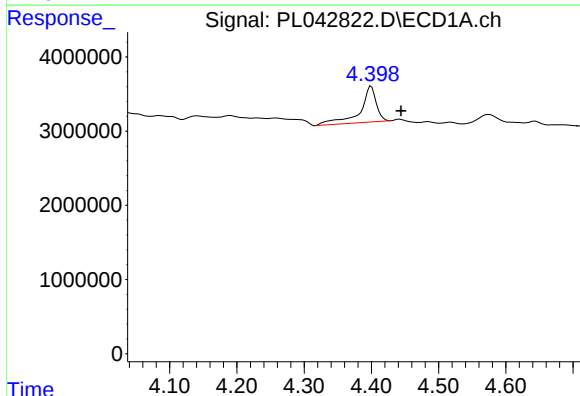


#6 beta-BHC

R.T.: 4.400 min
Delta R.T.: -0.045 min
Response: 8116891
Conc: 2.29 ng/ml

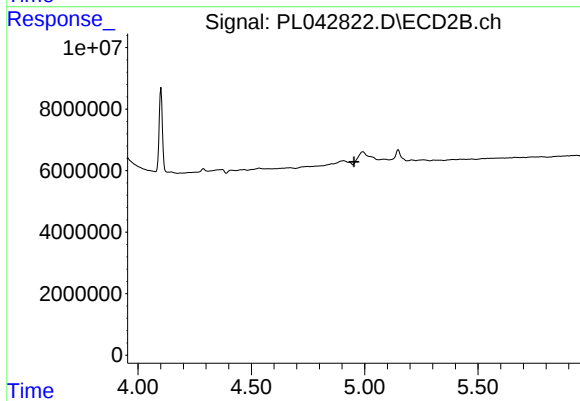

#6 beta-BHC


R.T.: 4.907 min
Delta R.T.: -0.047 min
Response: -547349
Conc: N.D.

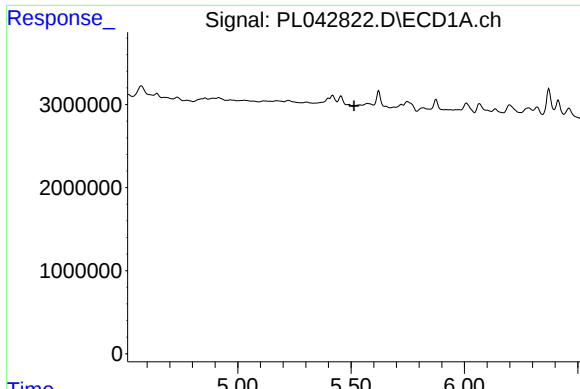

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

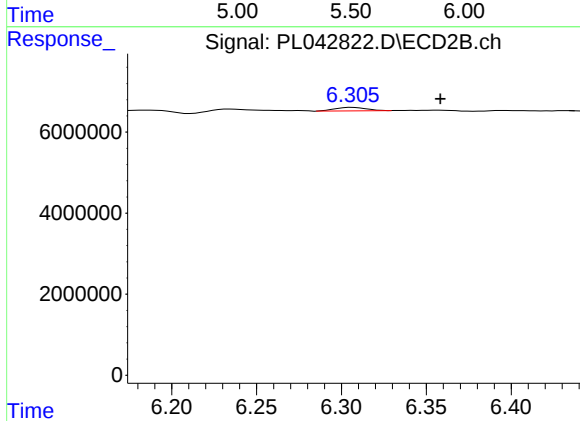


#9 Endosulfan I

R.T.: 6.307 min
Delta R.T.: -0.052 min
Response: 1147541
Conc: 0.36 ng/ml

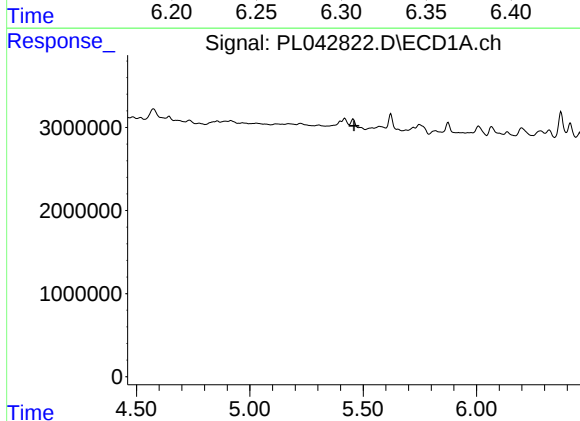


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

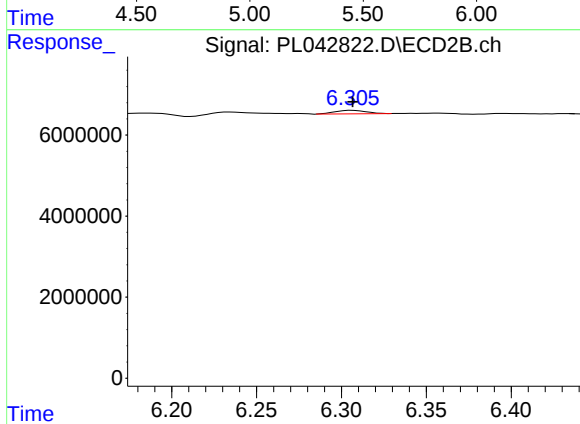

#11 alpha-Chlordane


R.T.: 6.307 min
Delta R.T.: 0.000 min
Response: 1147541
Conc: 0.34 ng/ml

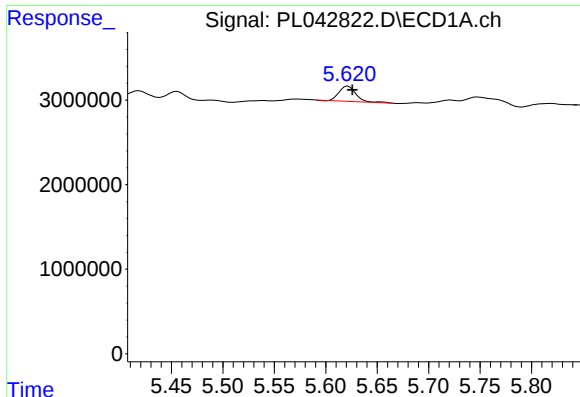

#12 4,4'-DDE


R.T.: 5.622 min
Delta R.T.: -0.004 min
Response: 2003268
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

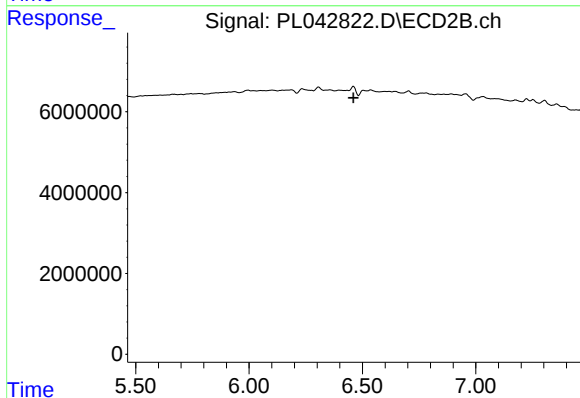


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

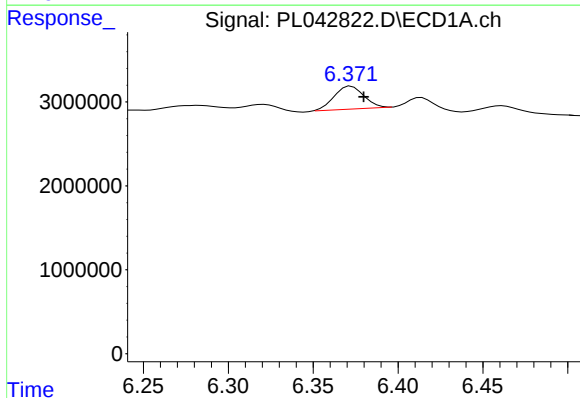


#17 4,4'-DDT

R.T.: 6.372 min
Delta R.T.: -0.007 min
Response: 3298993
Conc: 0.59 ng/ml

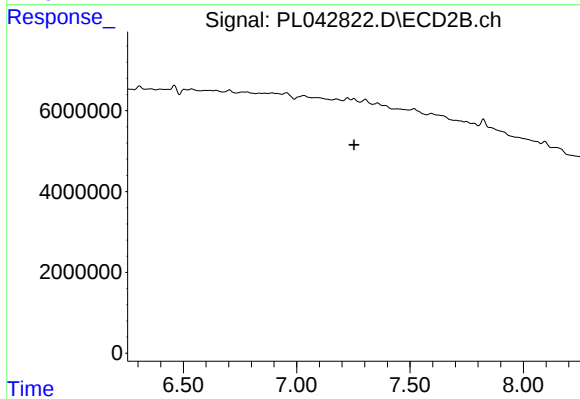

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

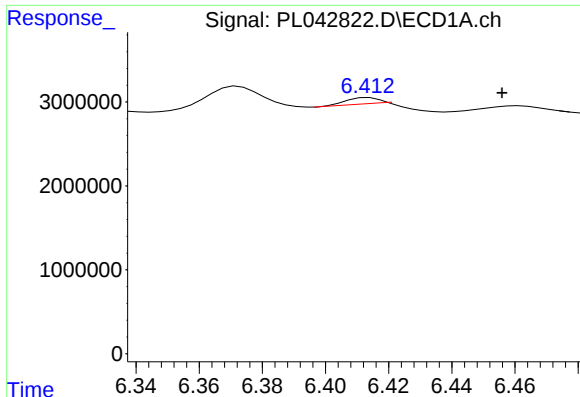

#18 Endrin aldehyde


R.T.: 6.414 min
Delta R.T.: -0.042 min
Response: 580363
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

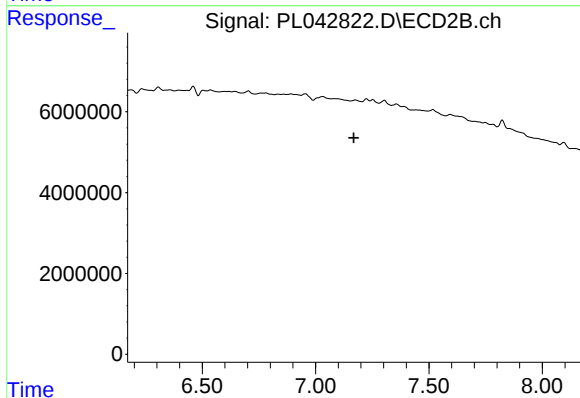


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.169 min
Response: 0
Conc: N.D.

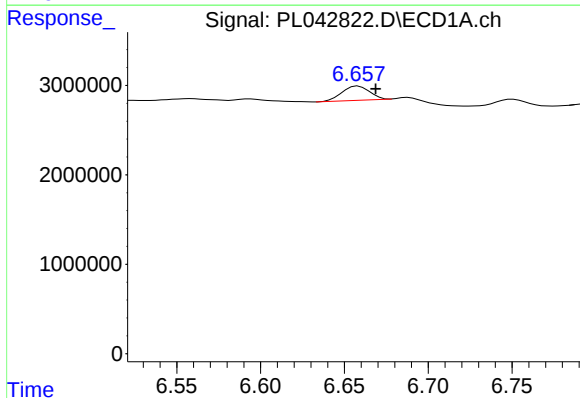


#19 Endosulfan Sulfate

R.T.: 6.658 min
Delta R.T.: -0.011 min
Response: 1824762
Conc: 0.29 ng/ml

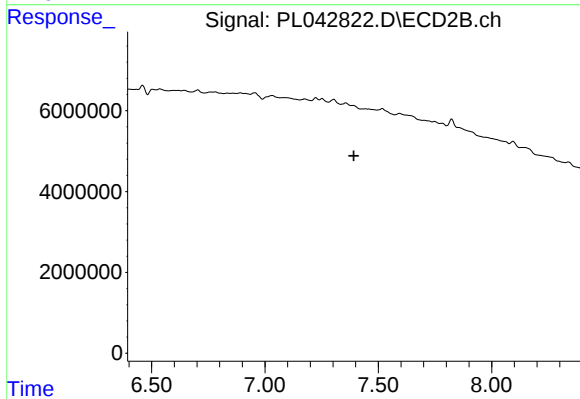

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

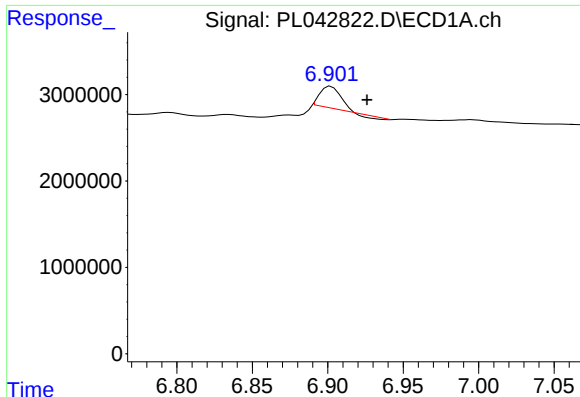

#20 Methoxychlor


R.T.: 6.902 min
Delta R.T.: -0.024 min
Response: 2174461
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

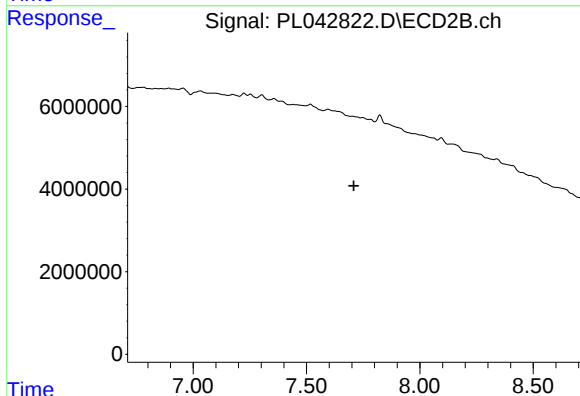


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

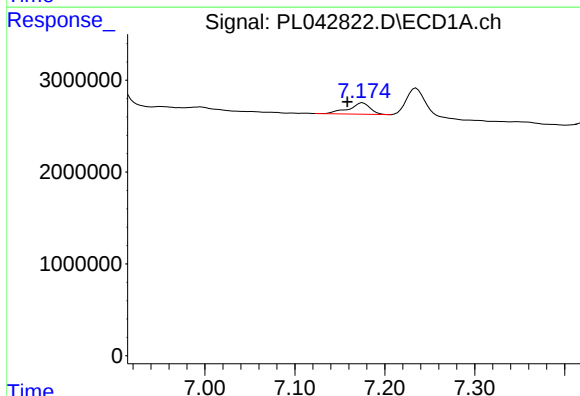


#21 Endrin ketone

R.T.: 7.175 min
Delta R.T.: 0.017 min
Response: 2058533
Conc: 0.30 ng/ml

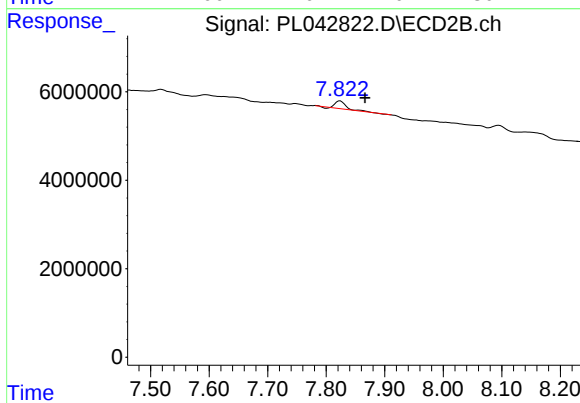

#21 Endrin ketone


R.T.: 7.824 min
Delta R.T.: -0.043 min
Response: 1884386
Conc: 0.68 ng/ml

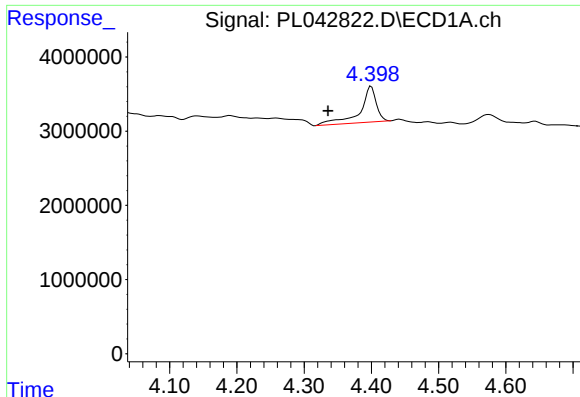

#23 Chlordane-1


R.T.: 4.400 min
Delta R.T.: 0.064 min
Response: 8116891
Conc: 29.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

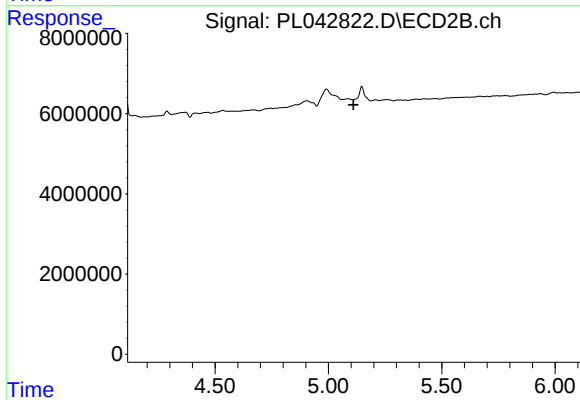


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

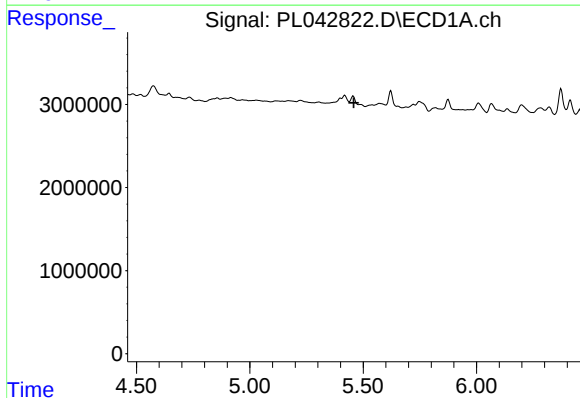


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

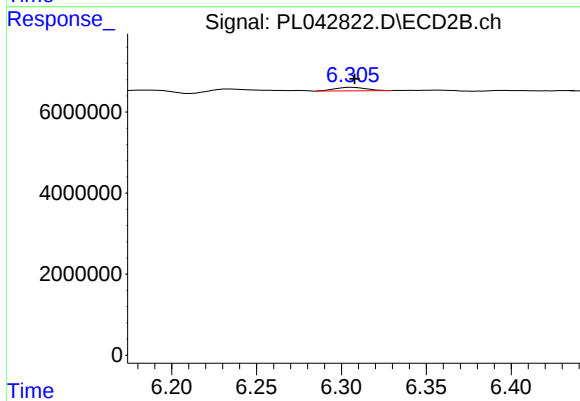

#26 Chlordane-4


R.T.: 6.307 min
Delta R.T.: -0.001 min
Response: 1147541
Conc: 2.10 ng/ml

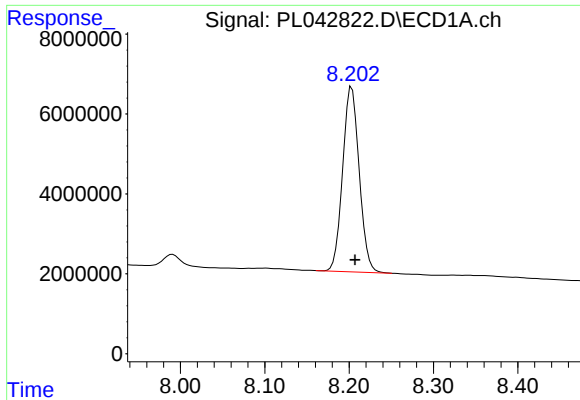

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 63146507
Conc: 10.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

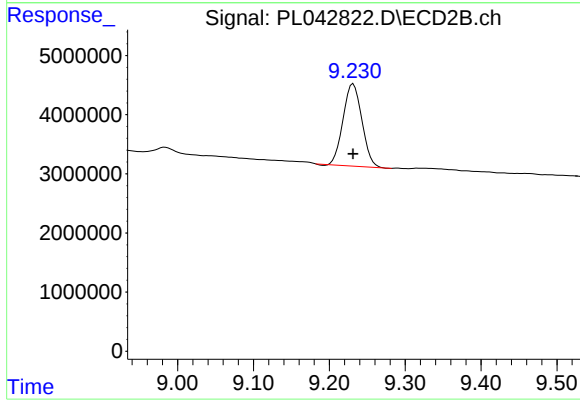

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 23986721
Conc: 9.95 ng/ml