

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 13:47
 Operator : AJ\SJ
 Sample : J6208-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:08:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	44324638	24066439	7.534	8.368
28)	SA Decachlor...	8.203	9.231	49842916	19513767	7.909	8.091
Target Compounds							
6)	B beta-BHC	4.399f	0.000	5635949	0	1.591	N.D. #
8)	B Heptachlo...	0.000	5.994	0	1685844	N.D.	0.470 #
13)	MA Dieldrin	5.747	0.000	2636423	0	0.358	N.D. #
14)	MA Endrin	6.016	0.000	2946386	0	0.450	N.D. #
15)	B Endosulfa...	6.322	0.000	829817	0	0.133	N.D. #
16)	A 4,4'-DDD	6.198f	6.957	2697905	2468020	0.510	0.938 #
17)	MA 4,4'-DDT	6.372	0.000	5174255	0	0.929	N.D. #
19)	B Endosulfa...	6.658	0.000	4152362	0	0.666	N.D. #
20)	A Methoxychlor	6.902	0.000	4682228	0	1.485	N.D. #
21)	B Endrin ke...	7.177	7.824f	4423675	4237979	0.639	1.533 #
23)	Chlordane-1	4.399	0.000	5635949	0	20.385	N.D. #
27)	Chlordane-5	6.322	0.000	829817	0	2.785	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 13:47
Operator : AJ\SJ
Sample : J6208-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:08:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

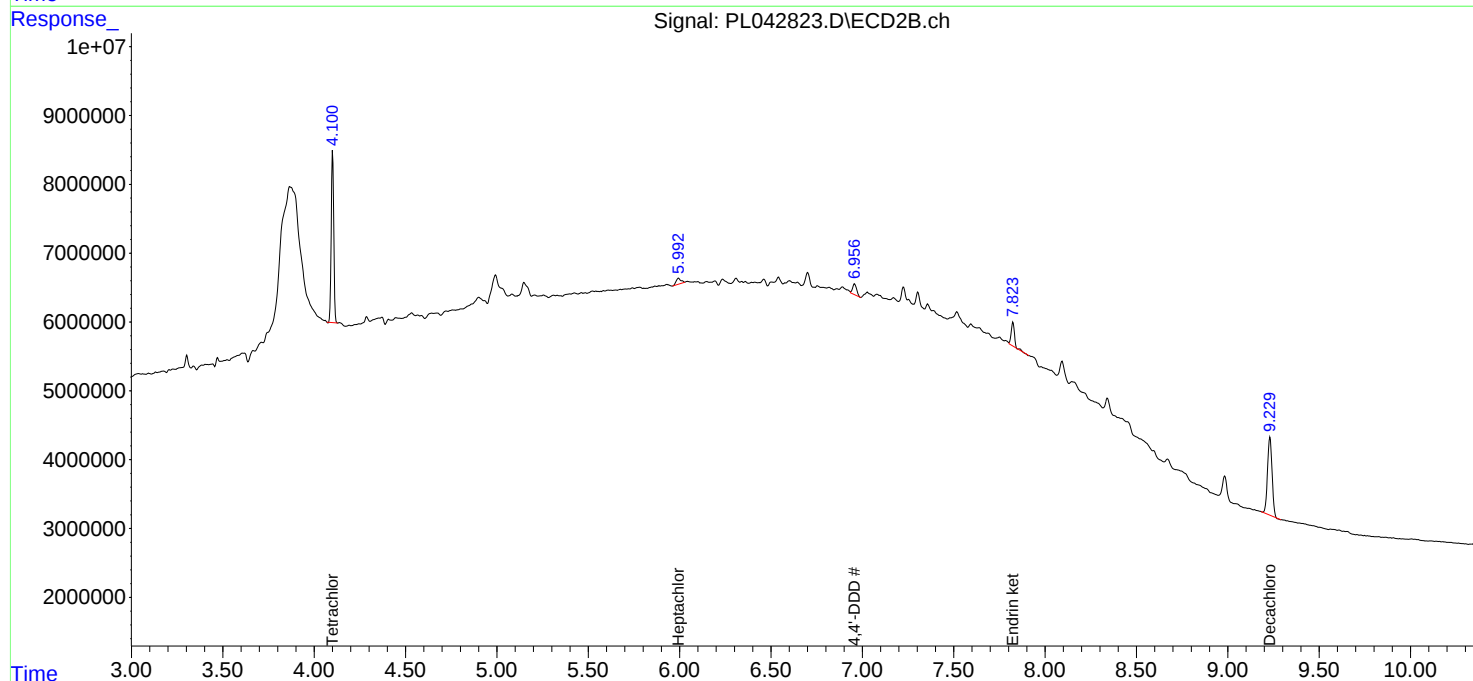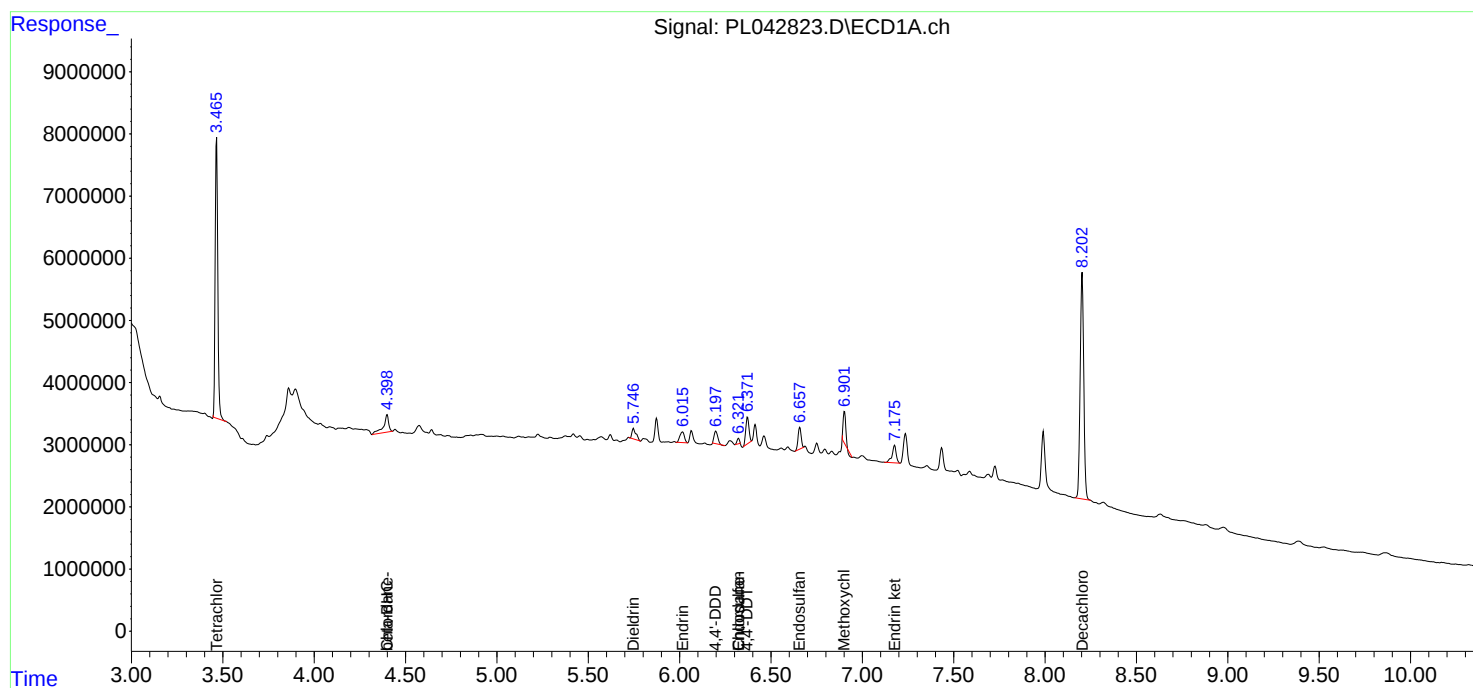


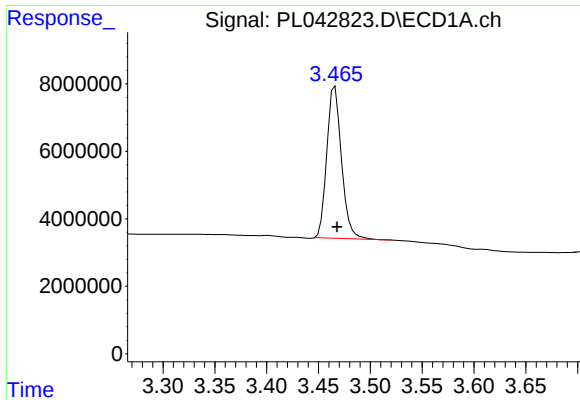

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 44324638
Conc: 7.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

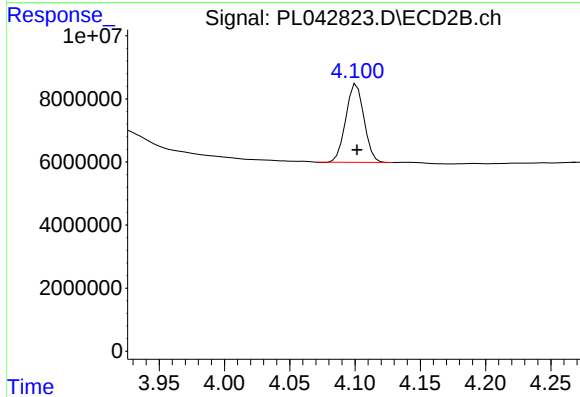


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 24066439
Conc: 8.37 ng/ml

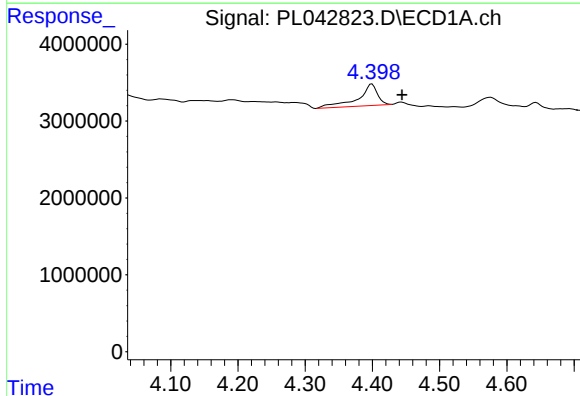


#6 beta-BHC

R.T.: 4.399 min
Delta R.T.: -0.045 min
Response: 5635949
Conc: 1.59 ng/ml

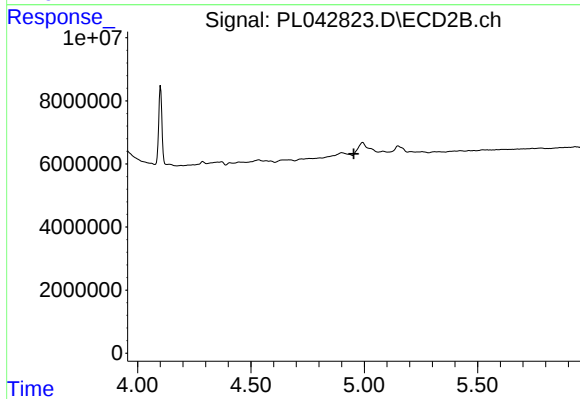

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

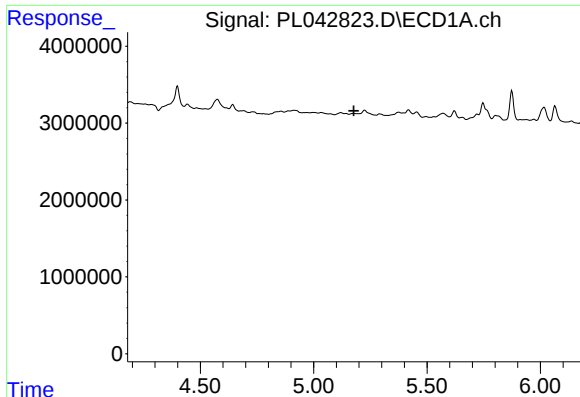

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

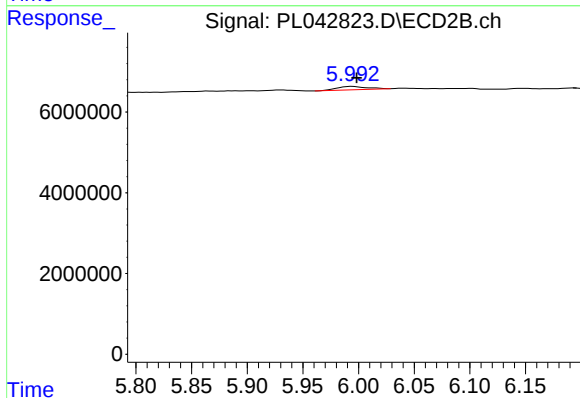


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 1685844
Conc: 0.47 ng/ml

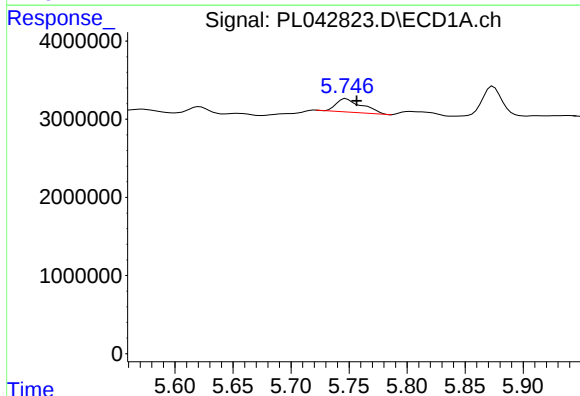


#13 Dieldrin

R.T.: 5.747 min
Delta R.T.: -0.009 min
Response: 2636423
Conc: 0.36 ng/ml

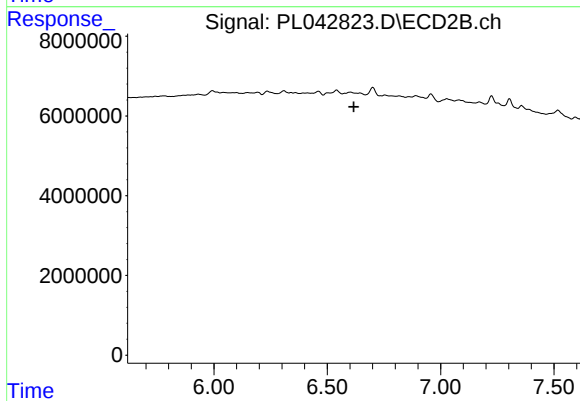

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

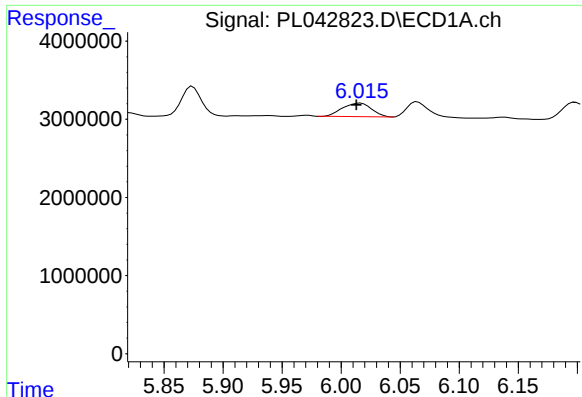

#14 Endrin


R.T.: 6.016 min
Delta R.T.: 0.003 min
Response: 2946386
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

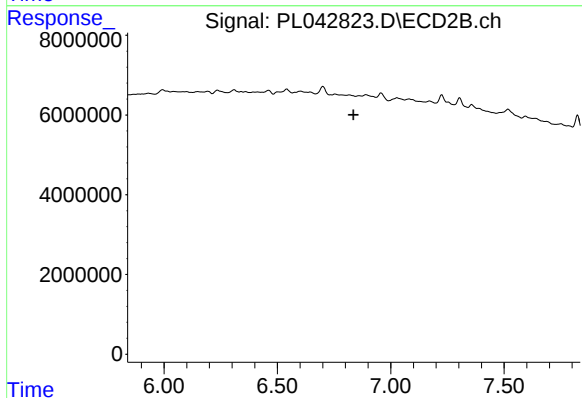


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

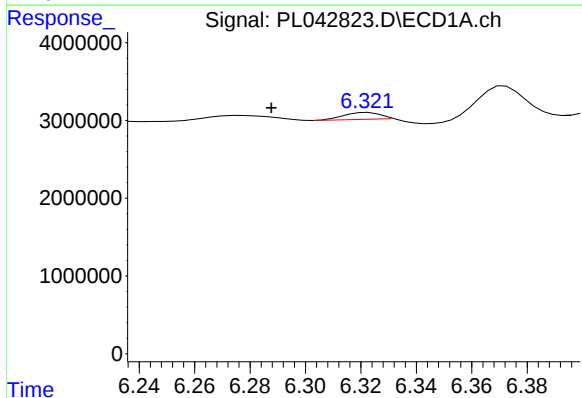


#15 Endosulfan II

R.T.: 6.322 min
Delta R.T.: 0.035 min
Response: 829817
Conc: 0.13 ng/ml

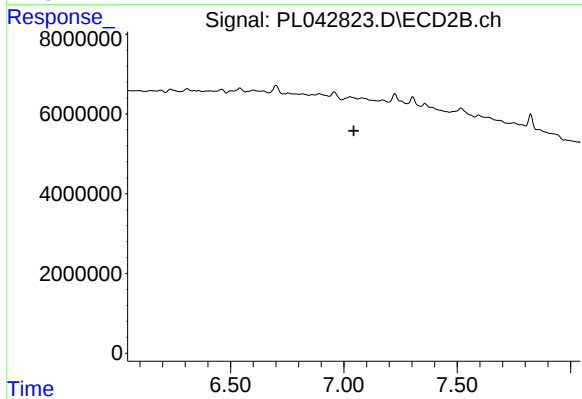

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

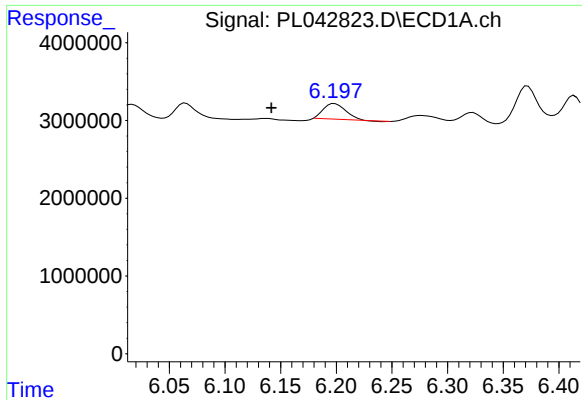

#16 4,4'-DDD


R.T.: 6.198 min
Delta R.T.: 0.057 min
Response: 2697905
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

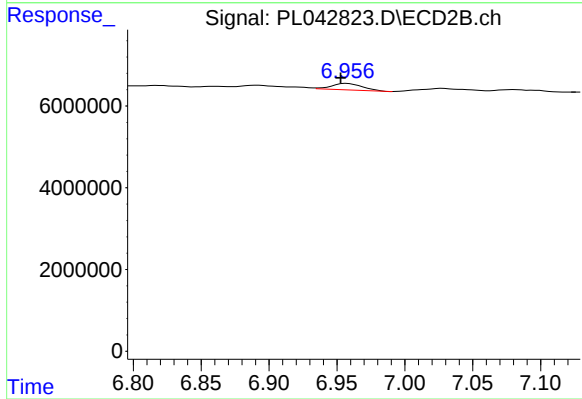


#16 4,4'-DDD

R.T.: 6.957 min
Delta R.T.: 0.005 min
Response: 2468020
Conc: 0.94 ng/ml

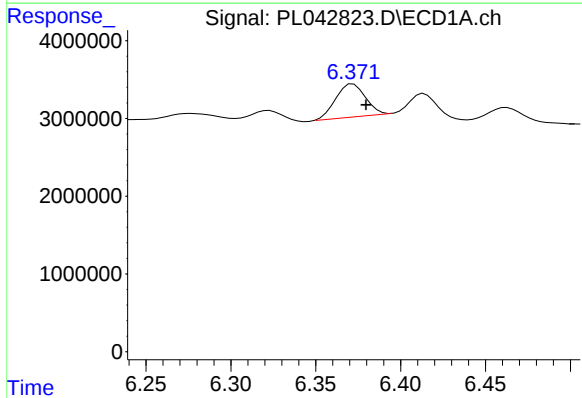


#17 4,4'-DDT

R.T.: 6.372 min
Delta R.T.: -0.008 min
Response: 5174255
Conc: 0.93 ng/ml

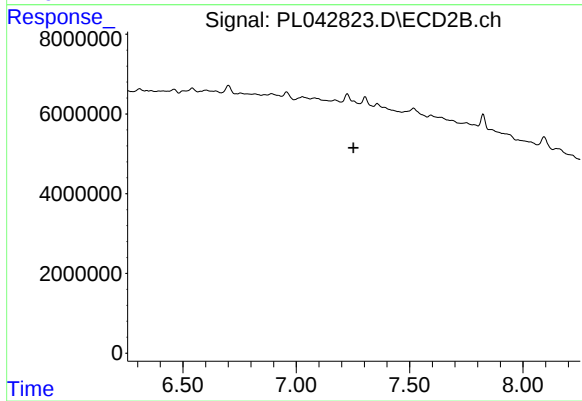

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

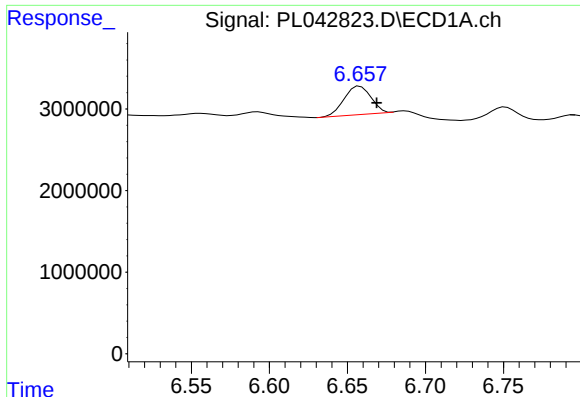

#19 Endosulfan Sulfate


R.T.: 6.658 min
Delta R.T.: -0.011 min
Response: 4152362
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

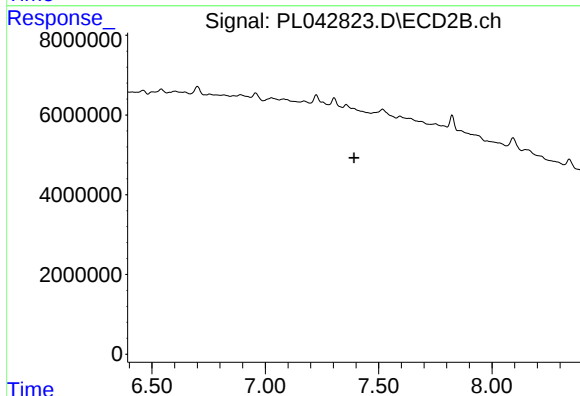


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

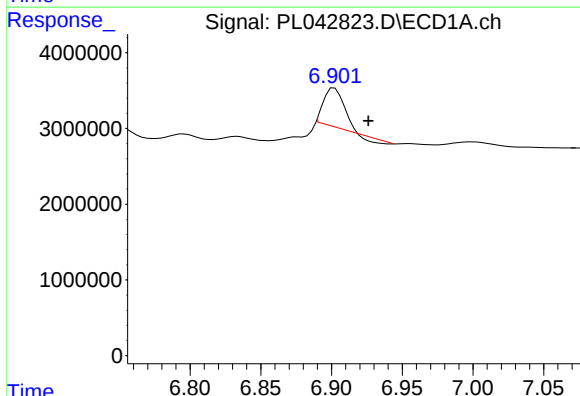


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: -0.024 min
Response: 4682228
Conc: 1.48 ng/ml

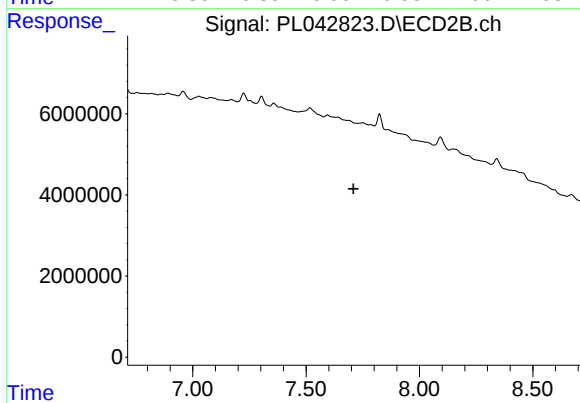

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

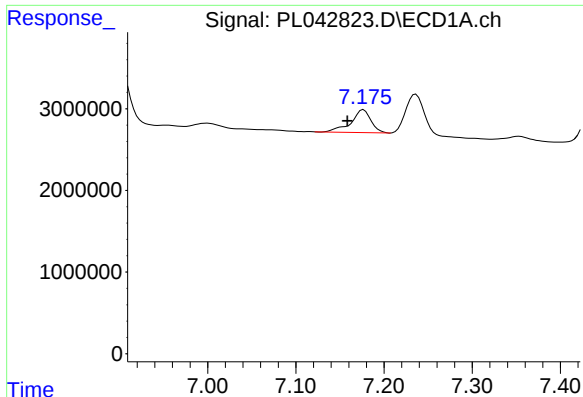

#21 Endrin ketone


R.T.: 7.177 min
Delta R.T.: 0.018 min
Response: 4423675
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

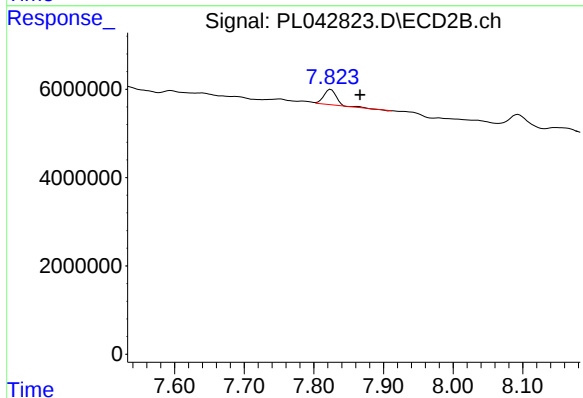


#21 Endrin ketone

R.T.: 7.824 min
Delta R.T.: -0.042 min
Response: 4237979
Conc: 1.53 ng/ml

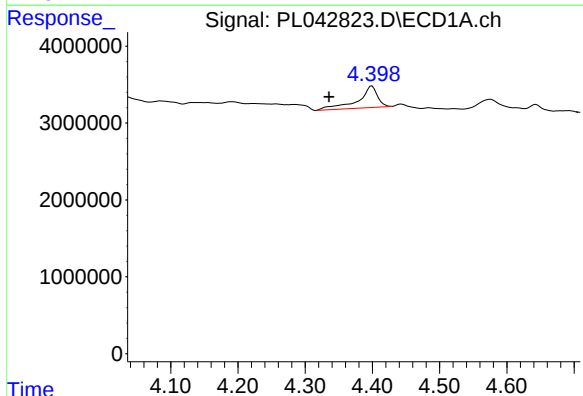


#23 Chlordane-1

R.T.: 4.399 min
Delta R.T.: 0.064 min
Response: 5635949
Conc: 20.39 ng/ml

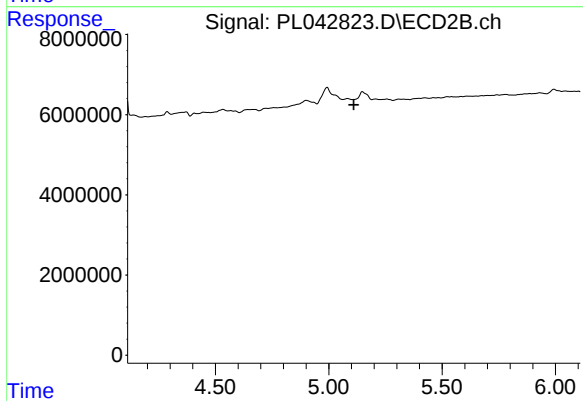

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.111 min
Response: 0
Conc: N.D.

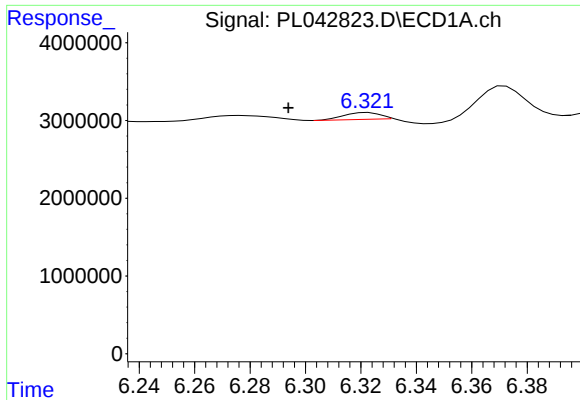

#27 Chlordane-5


R.T.: 6.322 min
Delta R.T.: 0.029 min
Response: 829817
Conc: 2.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

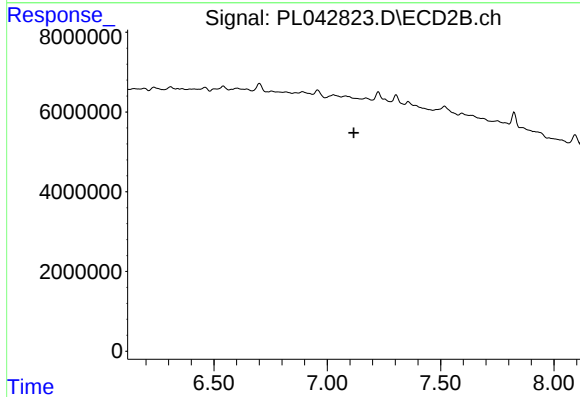


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

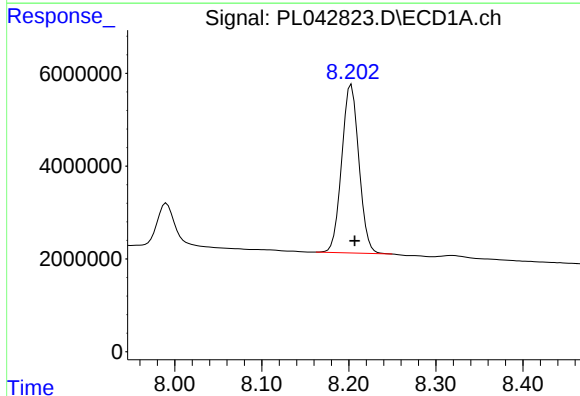

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 49842916
Conc: 7.91 ng/ml

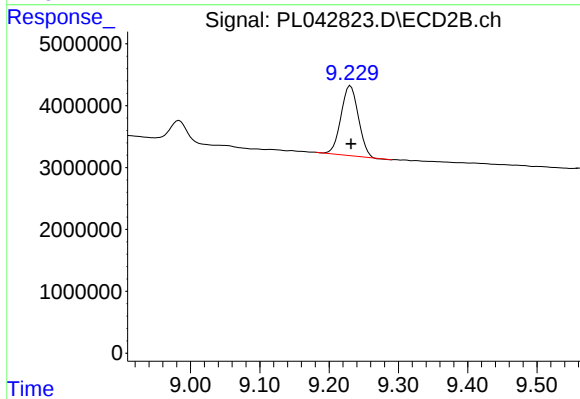

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 19513767
Conc: 8.09 ng/ml