

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 19:53
 Operator : AJ\SJ
 Sample : J6201-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:09:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	106.0E6	57183761	18.015	19.882
28)	SA Decachlor...	8.203	9.230	80360307	33680663	12.751	13.965
Target Compounds							
2)	A alpha-BHC	3.899	0.000	3727326	0	0.413	N.D. #
6)	B beta-BHC	4.400f	0.000	15087082	0	4.259	N.D. #
8)	B Heptachlo...	0.000	5.995	0	2200499	N.D.	0.614 #
23)	Chlordane-1	4.335	0.000	1825010	0	6.601	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 19:53
Operator : AJ\SJ
Sample : J6201-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:09:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

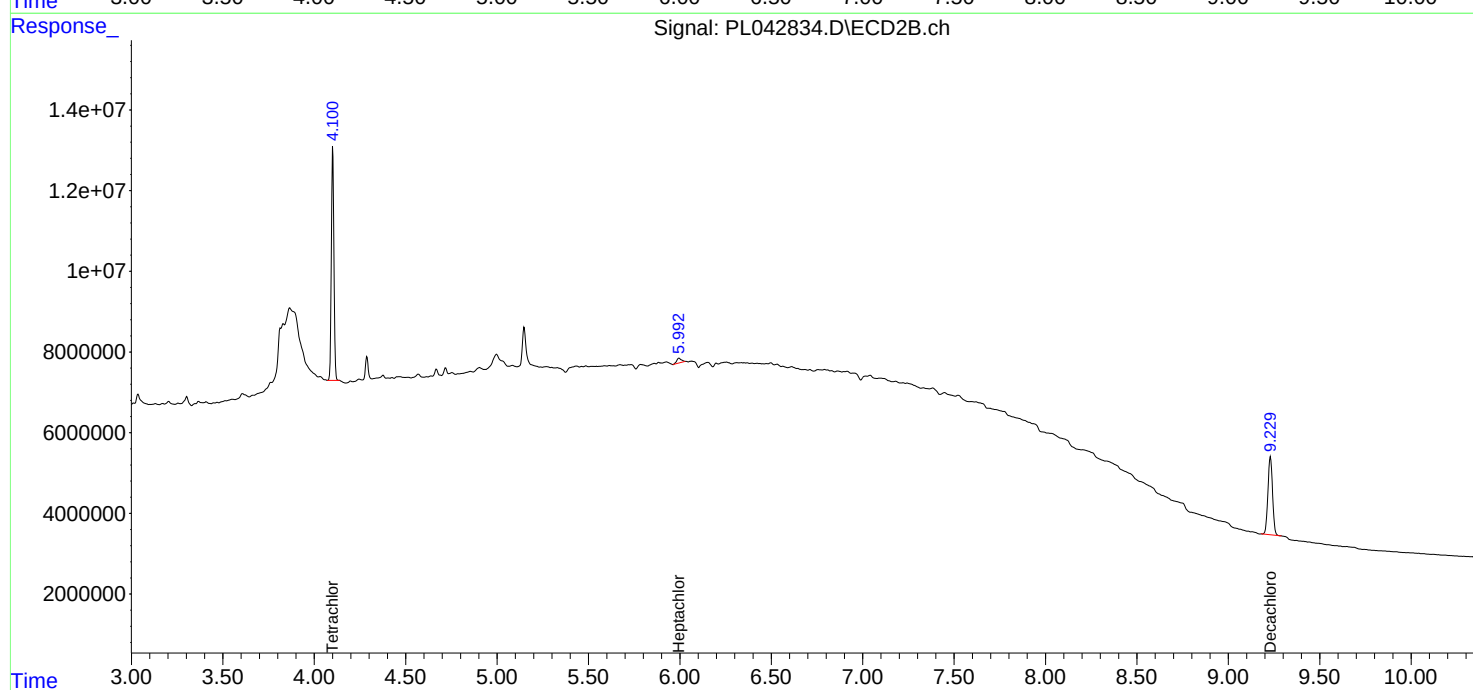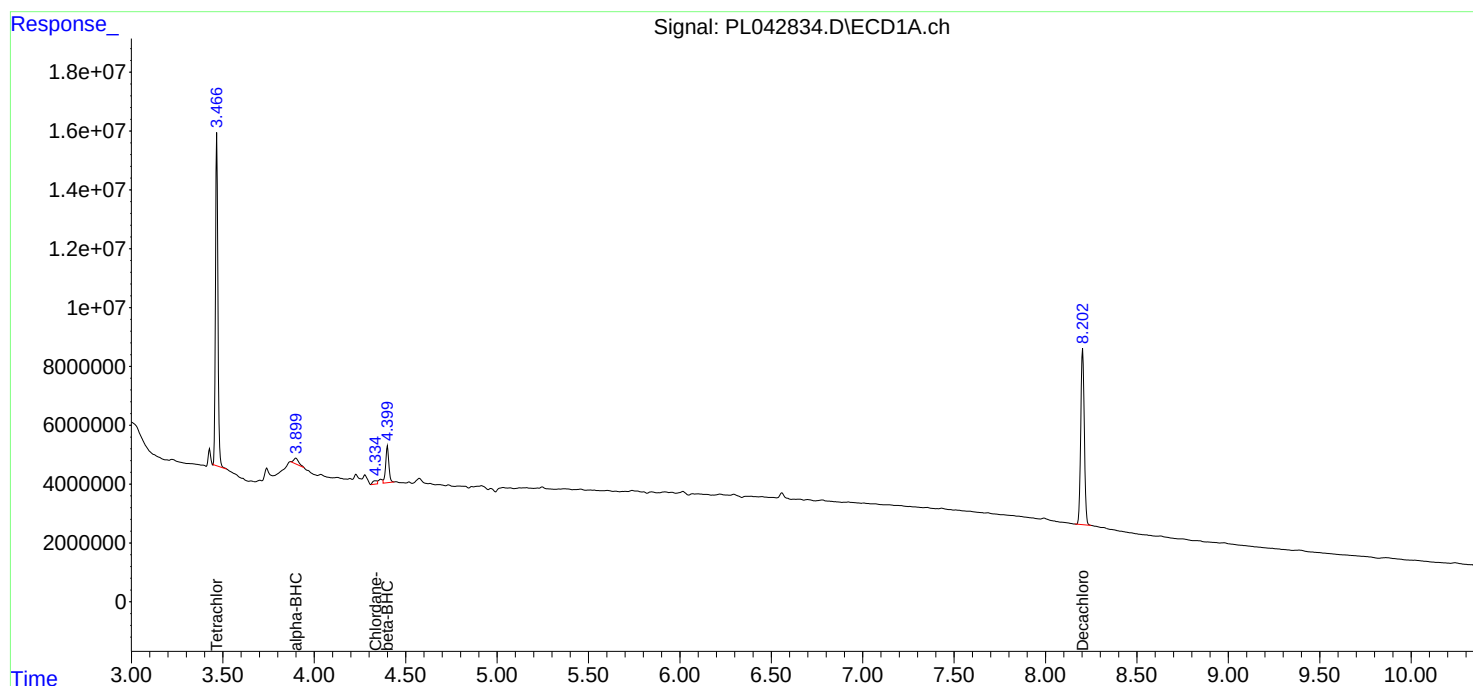


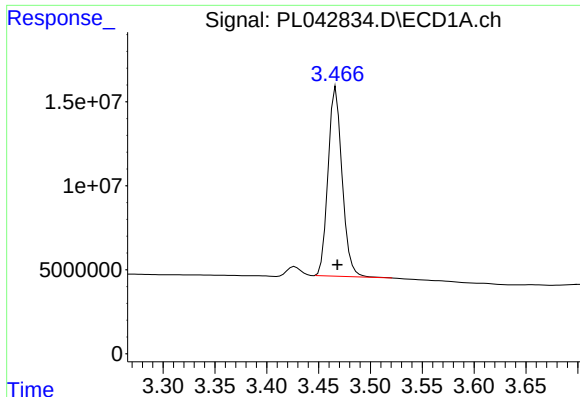

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 105992144
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

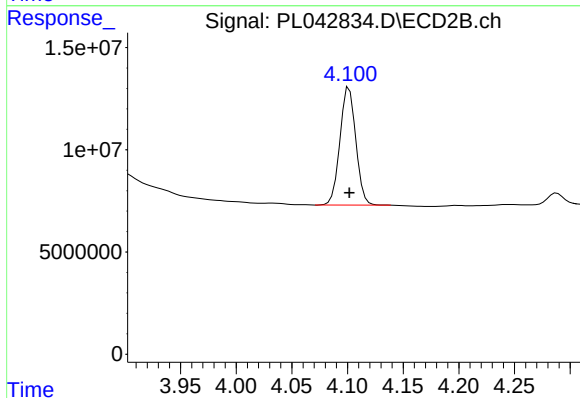


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 57183761
Conc: 19.88 ng/ml

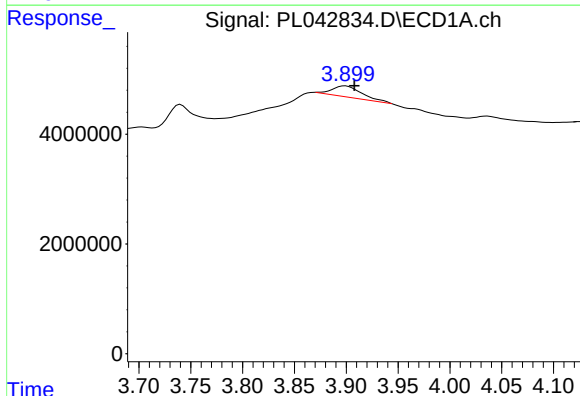


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: -0.008 min
Response: 3727326
Conc: 0.41 ng/ml

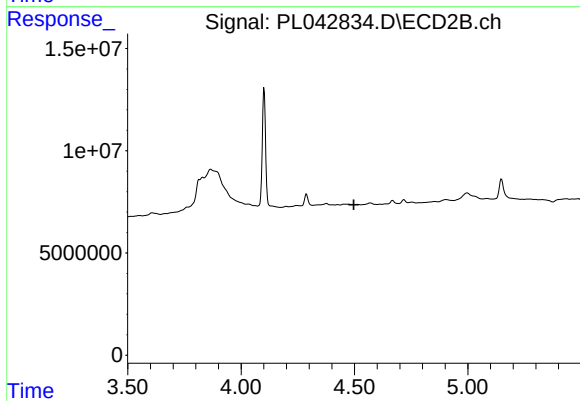

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

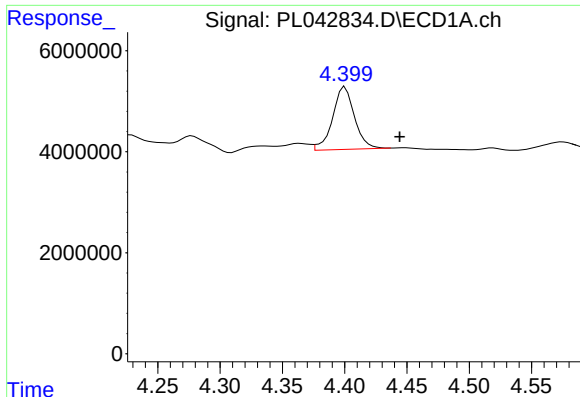

#6 beta-BHC


R.T.: 4.400 min
Delta R.T.: -0.044 min
Response: 15087082
Conc: 4.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

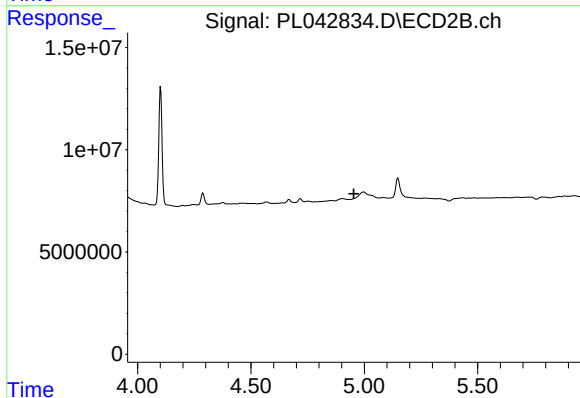


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

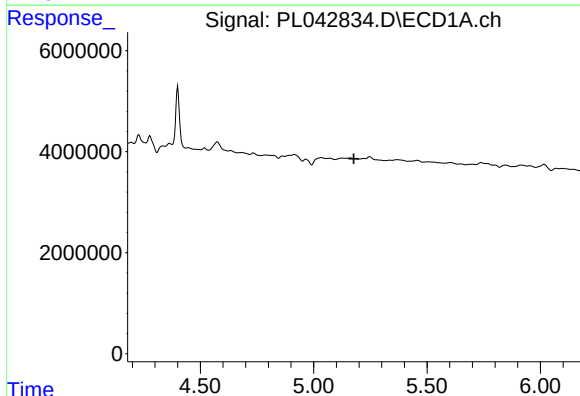


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

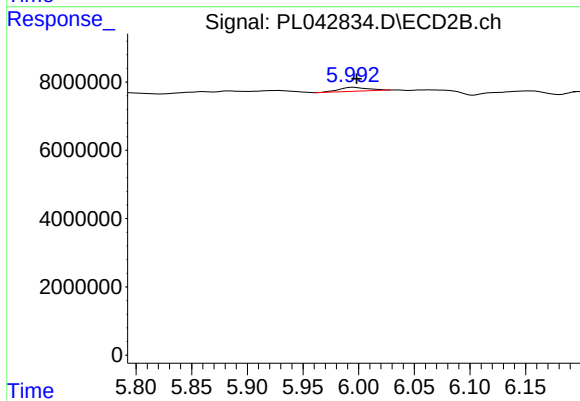

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 2200499
Conc: 0.61 ng/ml

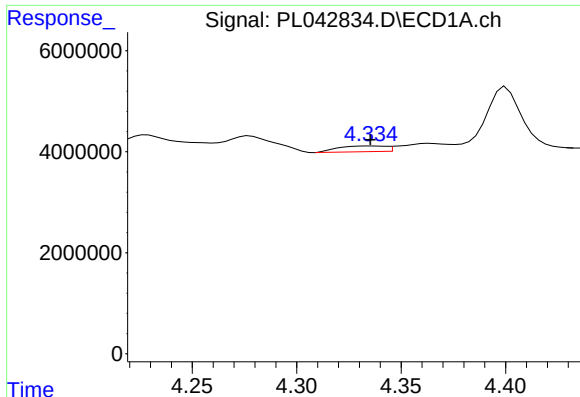

#23 Chlordane-1


R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 1825010
Conc: 6.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

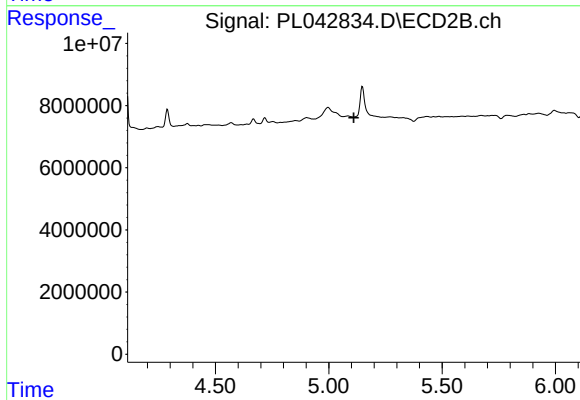


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

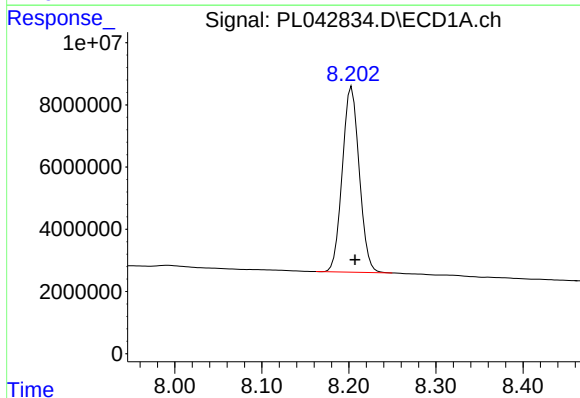

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 80360307
Conc: 12.75 ng/ml

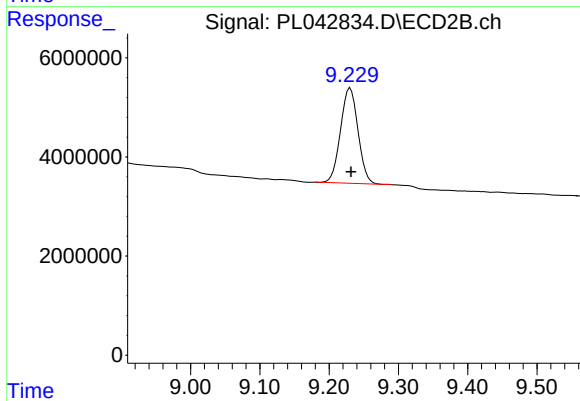

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.001 min
Response: 33680663
Conc: 13.96 ng/ml