

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 20:07
 Operator : AJ\SJ
 Sample : J6214-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:09:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	78313061	41842335	13.311	14.548
28)	SA Decachlor...	8.204	9.232	69691737	28259794	11.058	11.717
Target Compounds							
6)	B beta-BHC	4.401f	4.906f	5232785	812637	1.477	0.515 #
8)	B Heptachlo...	0.000	5.995	0	3543959	N.D.	0.988 #
9)	A Endosulfan I	5.540	6.344	2435742	830270	0.352	0.263 #
10)	B gamma-Chl...	0.000	6.255	0	1011274	N.D.	0.297 #
11)	B alpha-Chl...	0.000	6.344f	0	830270	N.D.	0.248 #
20)	A Methoxychlor	6.965f	0.000	3320532	0	1.053	N.D. #
23)	Chlordane-1	4.356	0.000	2656388	0	9.608	N.D. #
25)	Chlordane-3	0.000	6.255	0	1011274	N.D.	2.152 #
26)	Chlordane-4	0.000	6.344	0	830270	N.D.	1.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 20:07
Operator : AJ\SJ
Sample : J6214-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:09:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

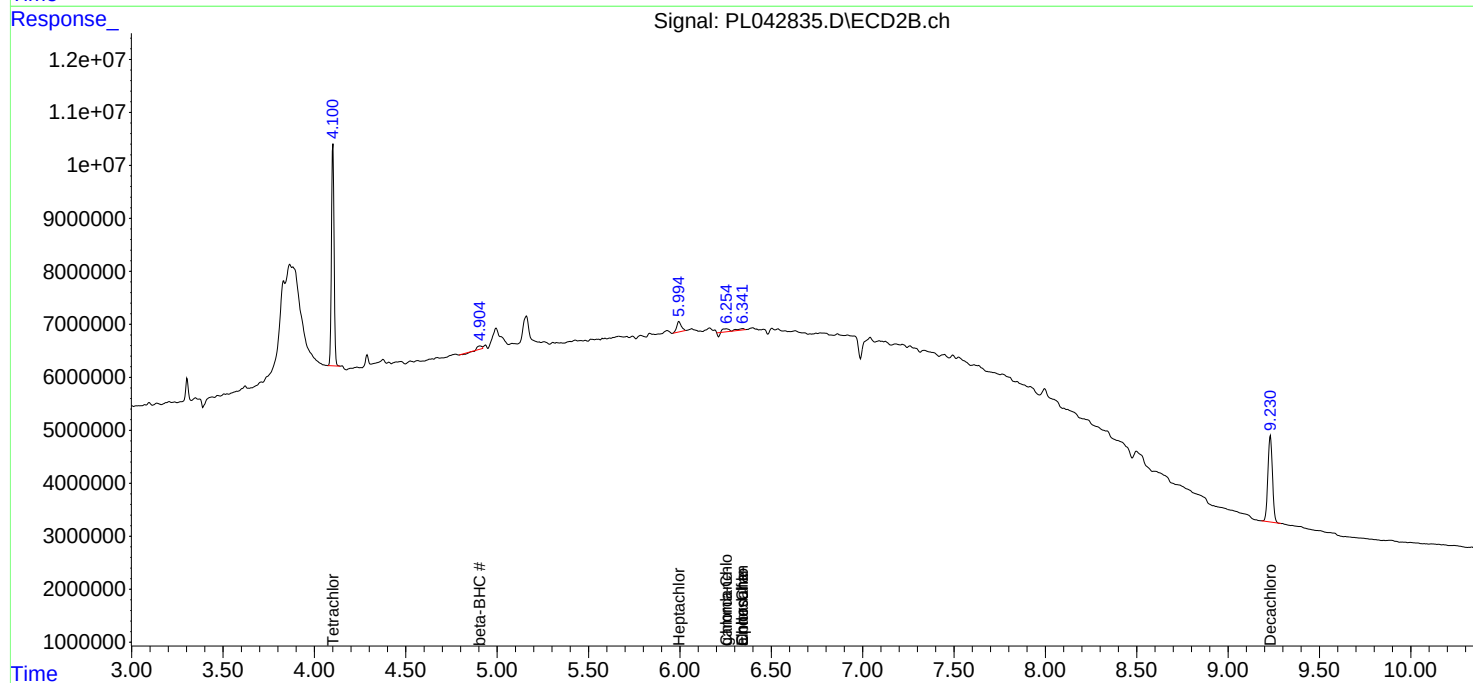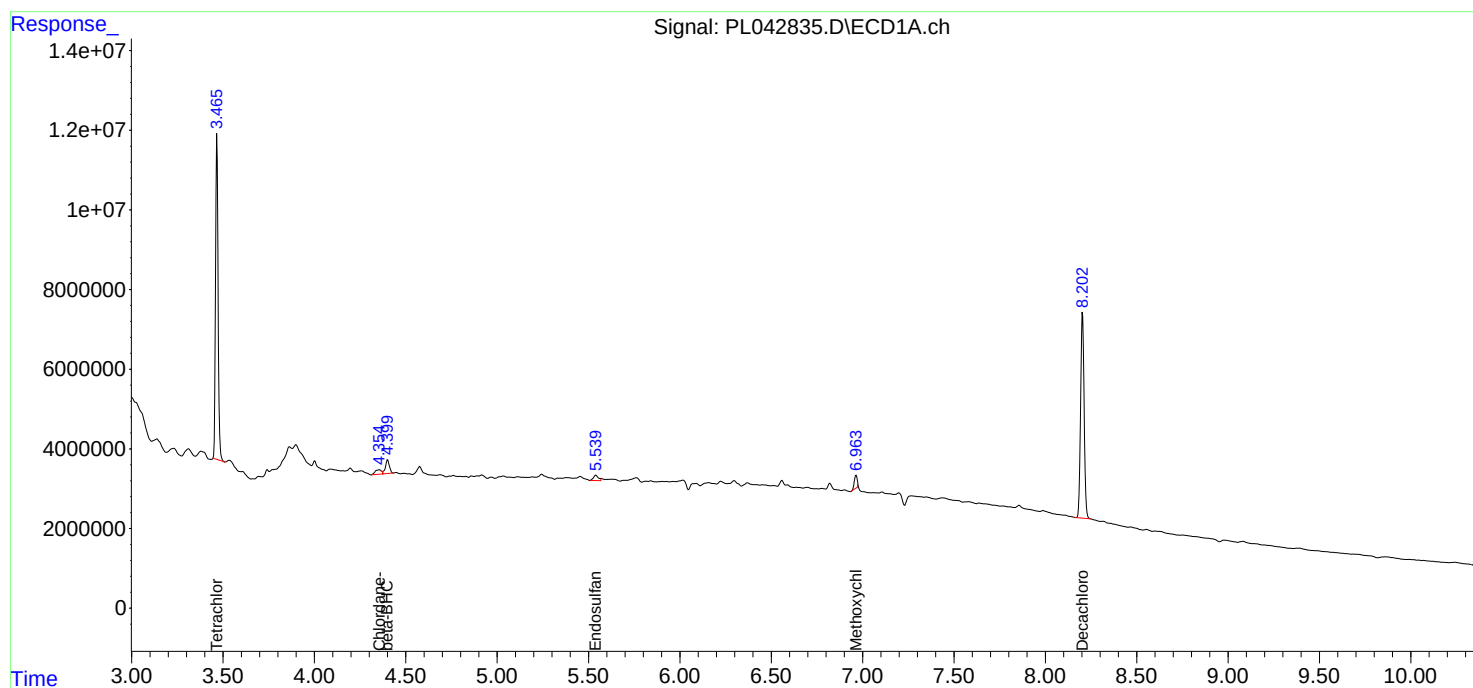


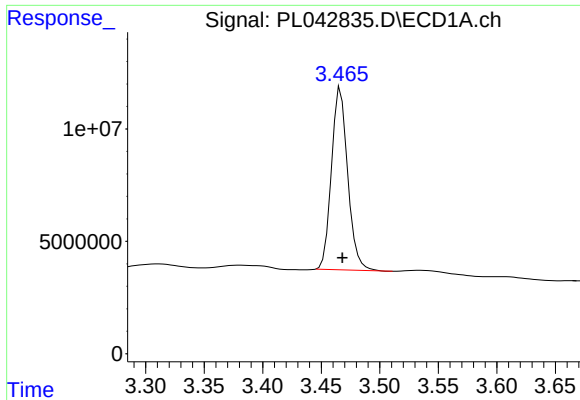

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 78313061
Conc: 13.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

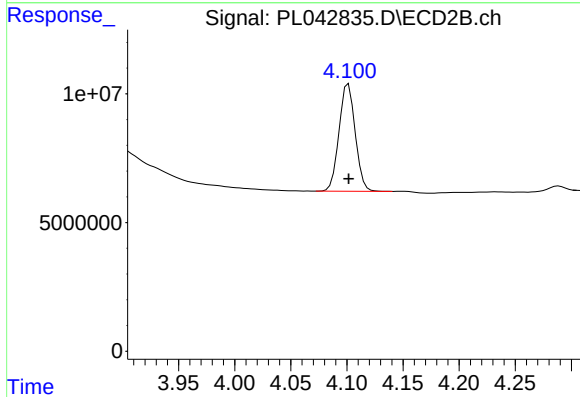


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 41842335
Conc: 14.55 ng/ml

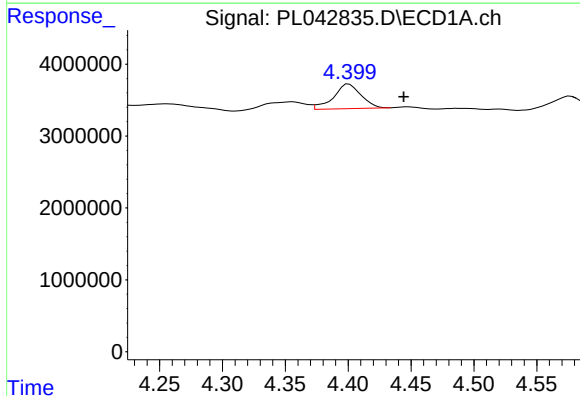


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.044 min
Response: 5232785
Conc: 1.48 ng/ml

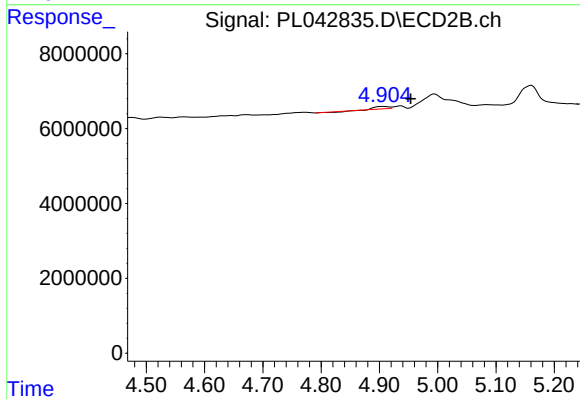

#6 beta-BHC


R.T.: 4.906 min
Delta R.T.: -0.048 min
Response: 812637
Conc: 0.52 ng/ml

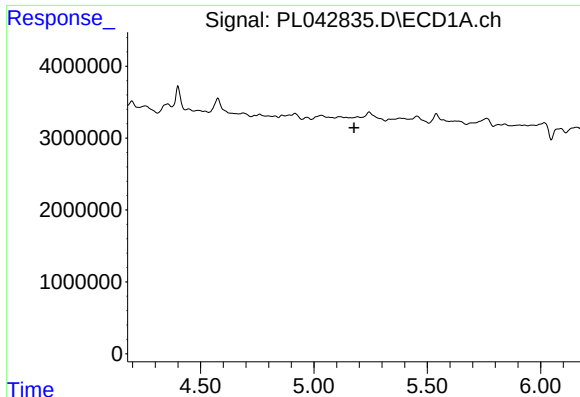

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

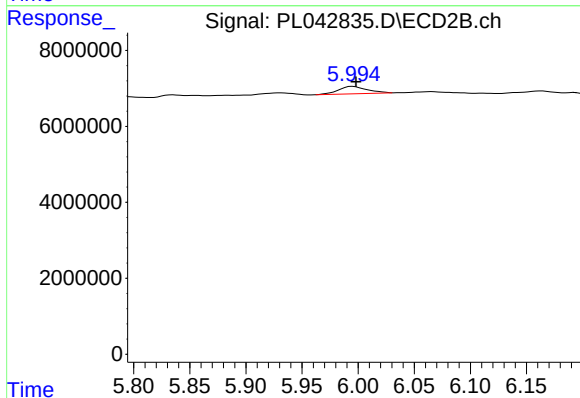


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 3543959
Conc: 0.99 ng/ml

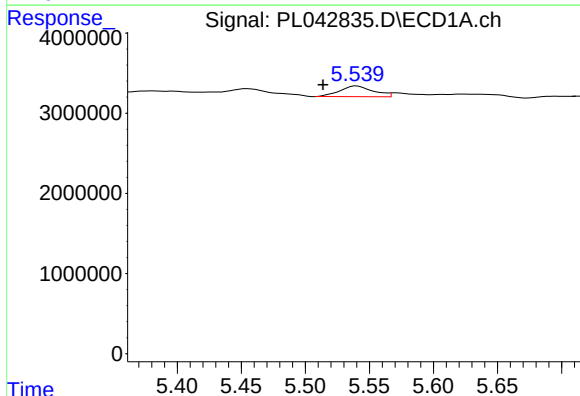


#9 Endosulfan I

R.T.: 5.540 min
Delta R.T.: 0.026 min
Response: 2435742
Conc: 0.35 ng/ml

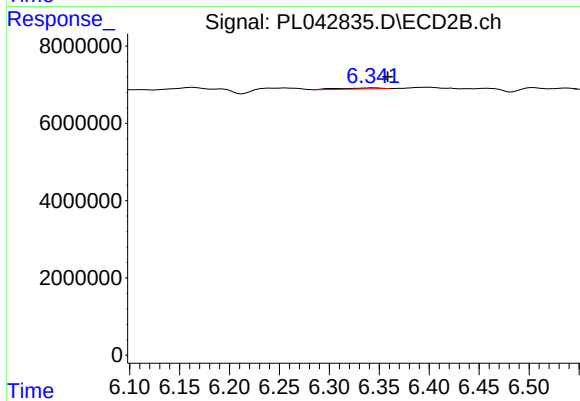

#9 Endosulfan I


R.T.: 6.344 min
Delta R.T.: -0.014 min
Response: 830270
Conc: 0.26 ng/ml

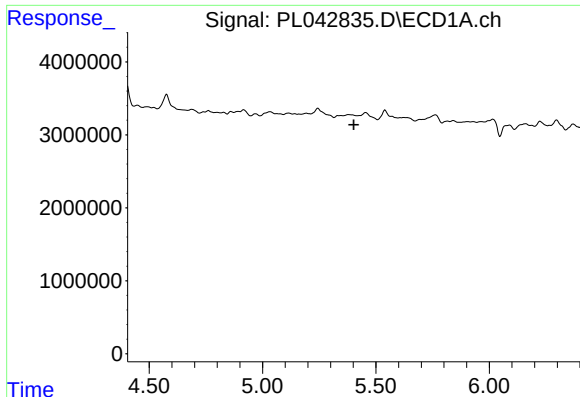

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

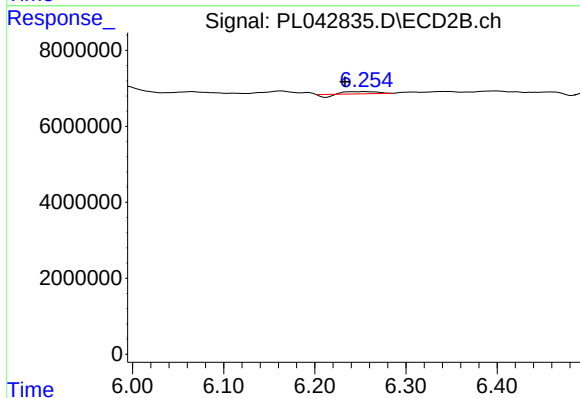


#10 gamma-Chlordane

R.T.: 6.255 min
Delta R.T.: 0.022 min
Response: 1011274
Conc: 0.30 ng/ml

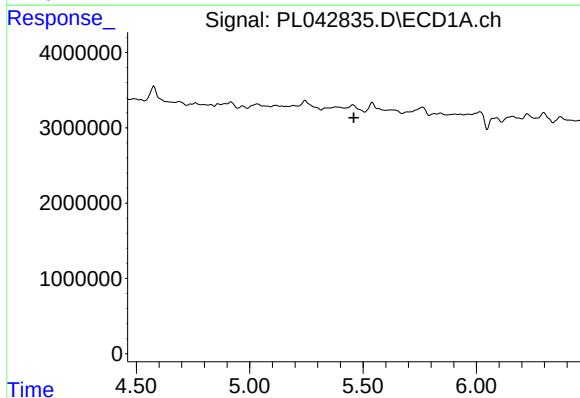


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

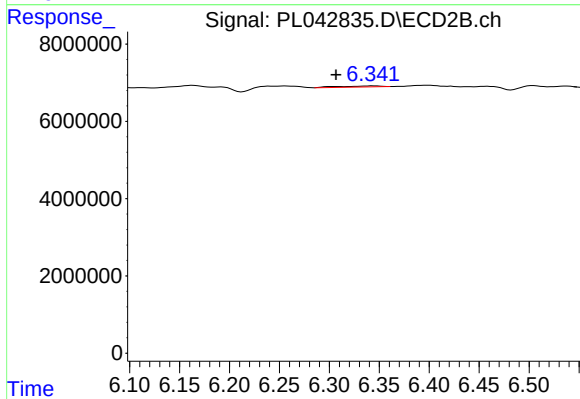

#11 alpha-Chlordane


R.T.: 6.344 min
Delta R.T.: 0.037 min
Response: 830270
Conc: 0.25 ng/ml

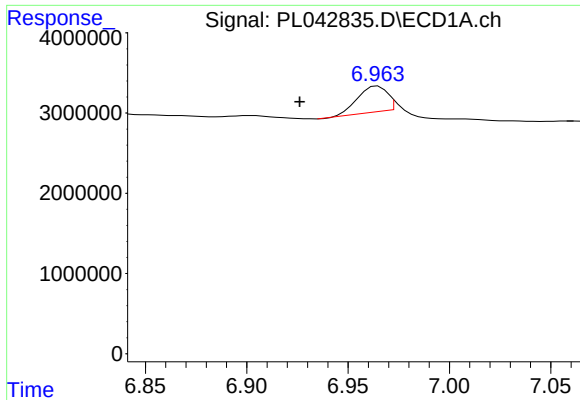

#20 Methoxychlor


R.T.: 6.965 min
Delta R.T.: 0.039 min
Response: 3320532
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

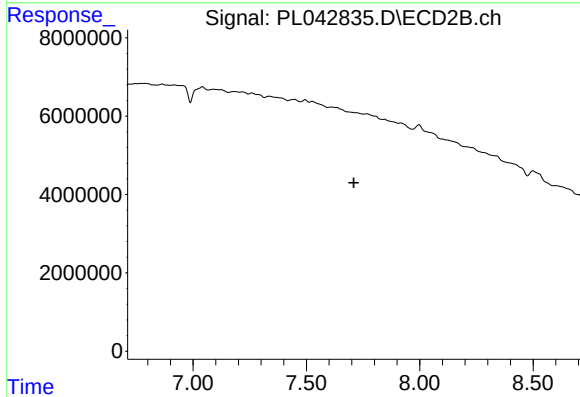


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

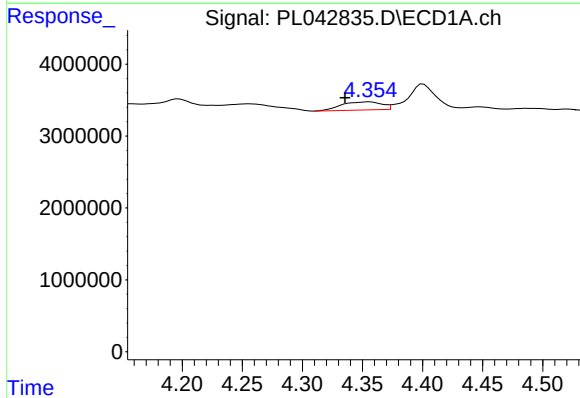


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.020 min
Response: 2656388
Conc: 9.61 ng/ml

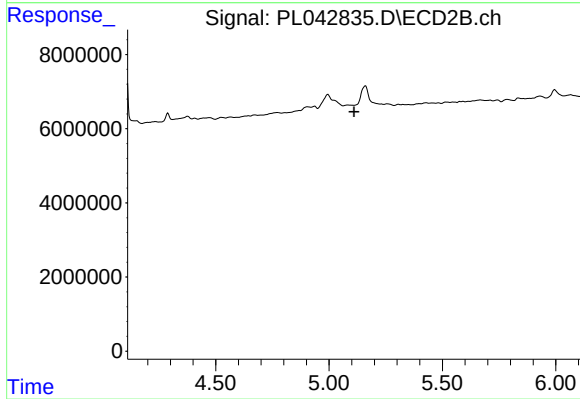

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

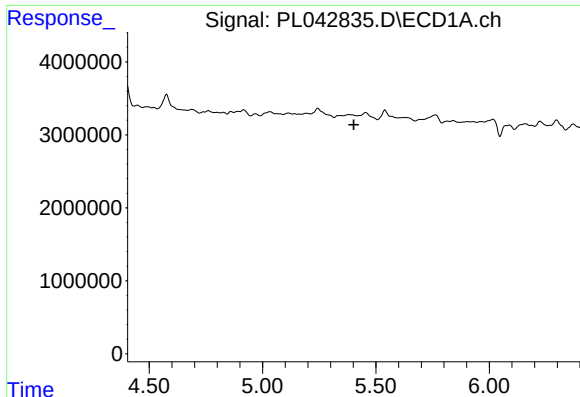

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

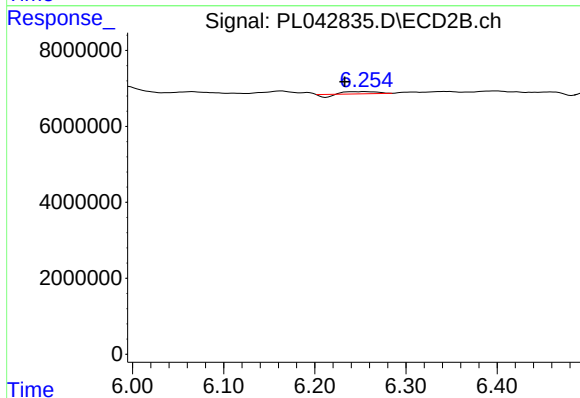


#25 Chlordane-3

R.T.: 6.255 min
Delta R.T.: 0.023 min
Response: 1011274
Conc: 2.15 ng/ml

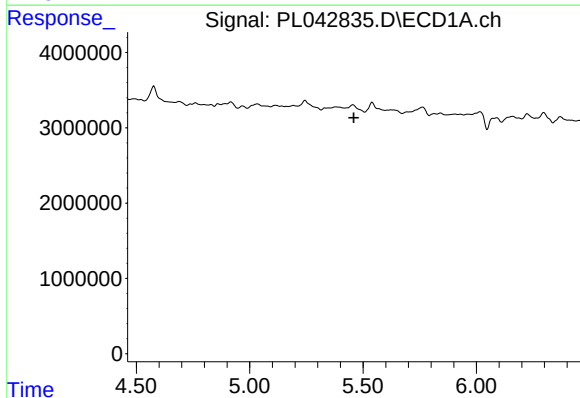


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

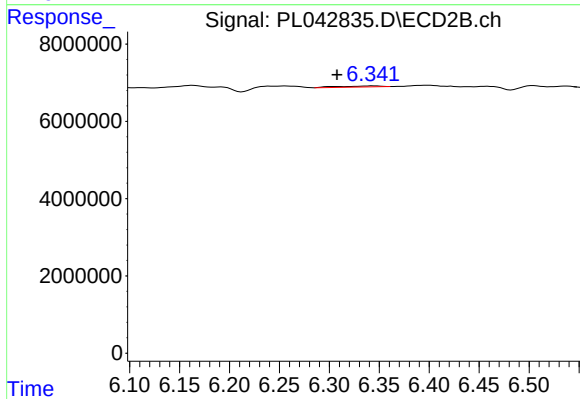

#26 Chlordane-4


R.T.: 6.344 min
Delta R.T.: 0.036 min
Response: 830270
Conc: 1.52 ng/ml

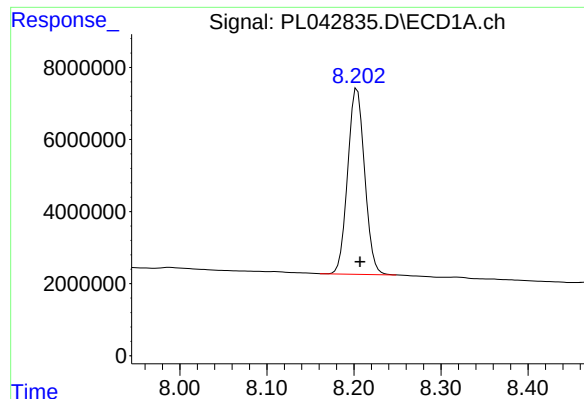

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 69691737
Conc: 11.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

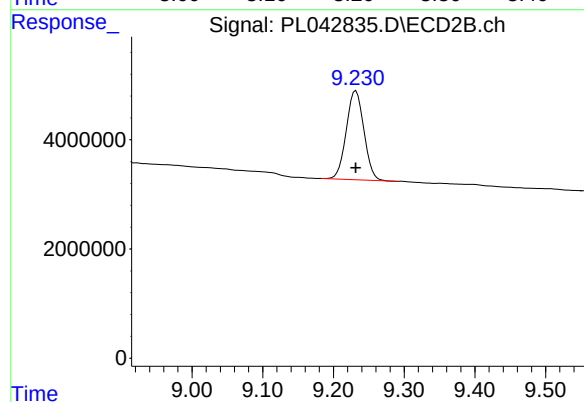

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 28259794
Conc: 11.72 ng/ml