

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 20:36
 Operator : AJ\SJ
 Sample : J6214-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:10:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	108.3E6	58131722	18.413	20.212
28)	SA Decachlor...	8.203	9.231	97100672	40591096	15.408	16.830
Target Compounds							
6)	B beta-BHC	4.400f	0.000	4131990	0	1.166	N.D. #
7)	B delta-BHC	0.000	5.163	0	2976834	N.D.	0.809 #
8)	B Heptachlo...	0.000	5.995	0	3696436	N.D.	1.031 #
10)	B gamma-Chl...	0.000	6.248	0	799106	N.D.	0.235 #
11)	B alpha-Chl...	0.000	6.248f	0	799106	N.D.	0.239 #
15)	B Endosulfa...	6.295	0.000	2118289	0	0.339	N.D. #
20)	A Methoxychlor	6.963f	0.000	1108597	0	0.352	N.D. #
23)	Chlordane-1	4.356	5.163	2420564	2976834	8.755	22.394 #
25)	Chlordane-3	0.000	6.248	0	799106	N.D.	1.700 #
26)	Chlordane-4	0.000	6.248	0	799106	N.D.	1.460 #
27)	Chlordane-5	6.295	0.000	2118289	0	7.109	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 20:36
Operator : AJ\SJ
Sample : J6214-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:10:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

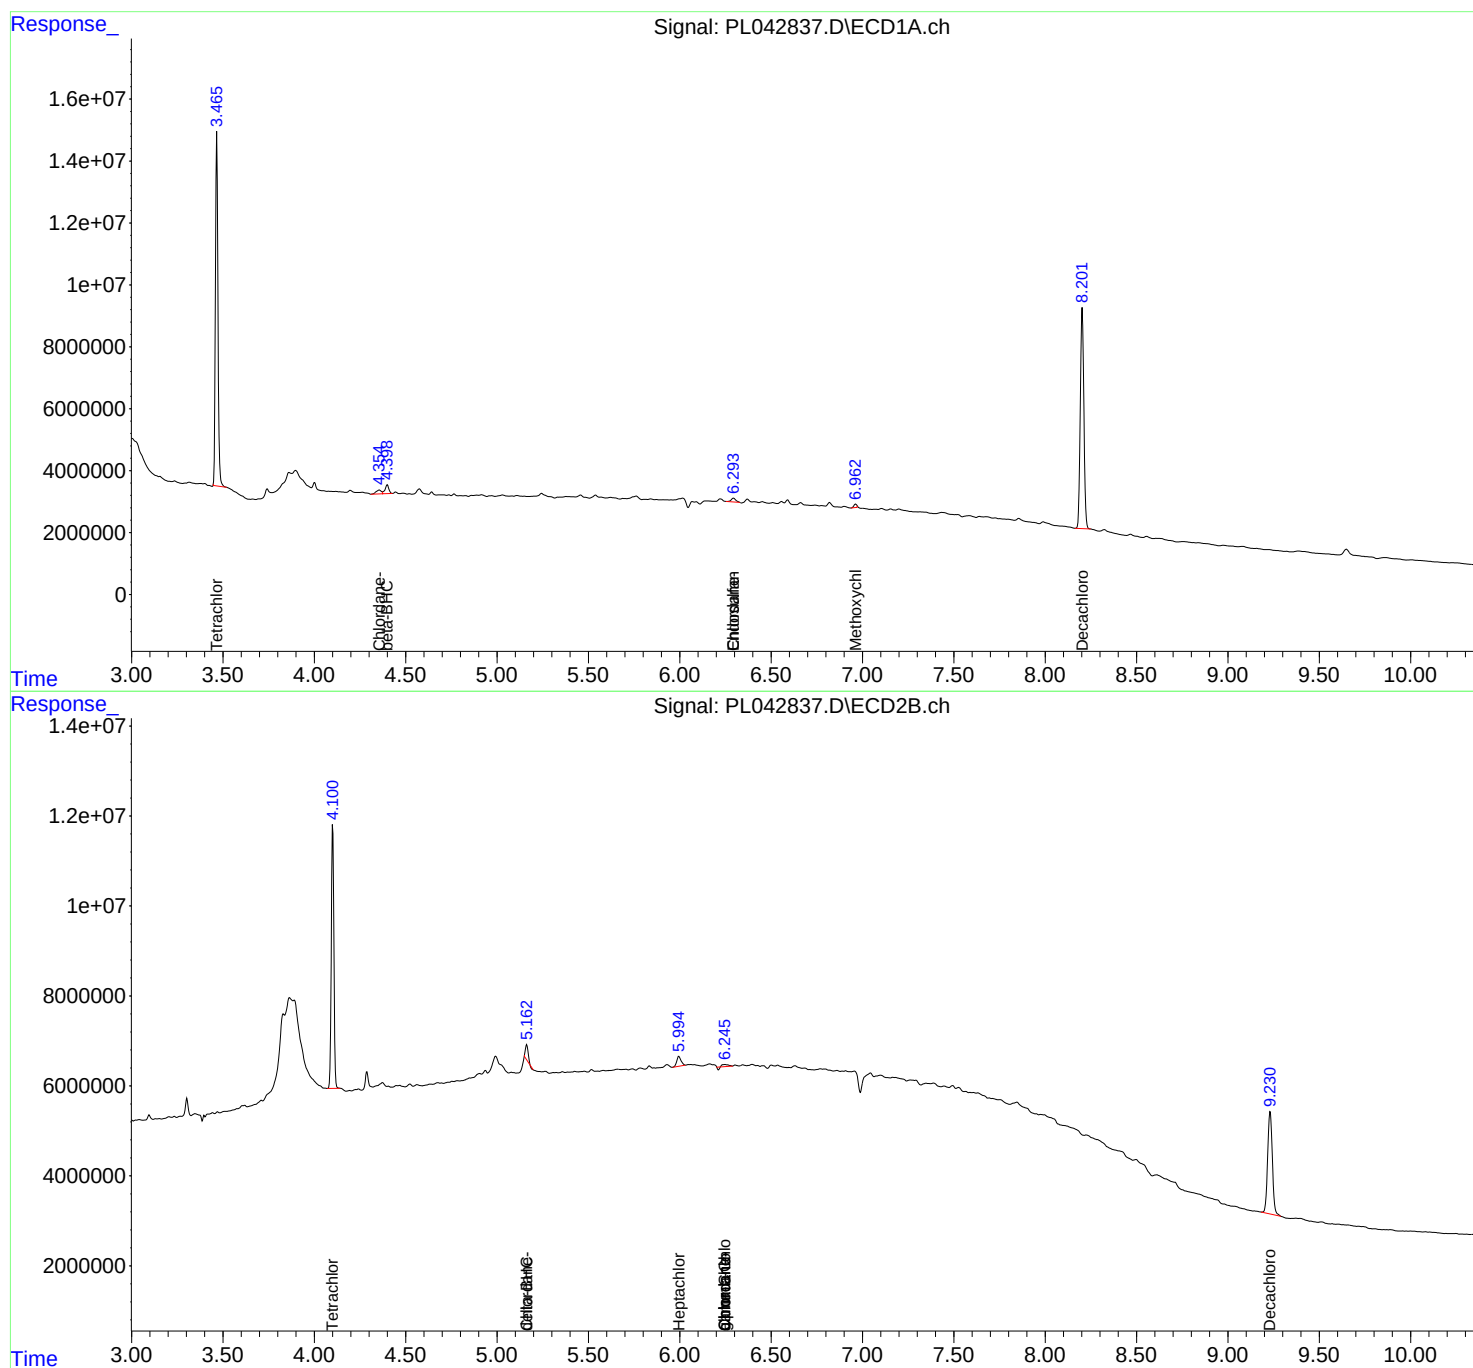


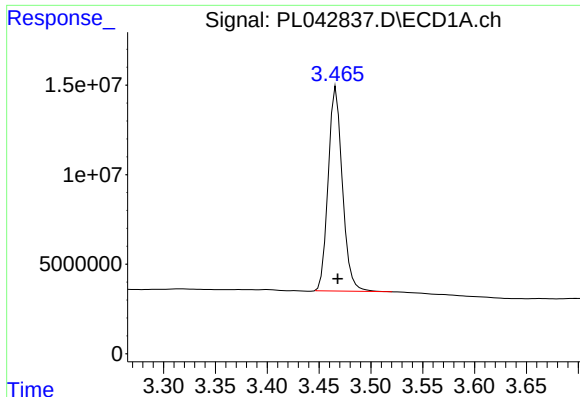

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 108330946
Conc: 18.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

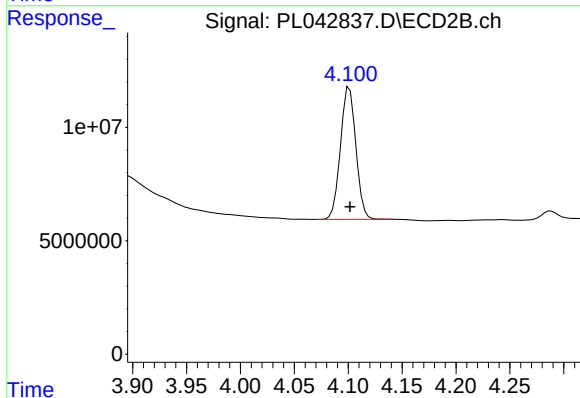


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 58131722
Conc: 20.21 ng/ml

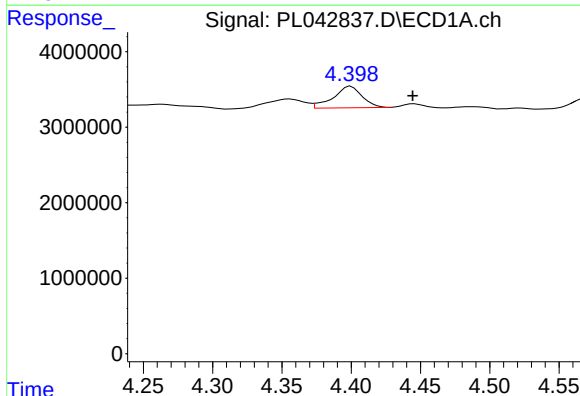


#6 beta-BHC

R.T.: 4.400 min
Delta R.T.: -0.045 min
Response: 4131990
Conc: 1.17 ng/ml

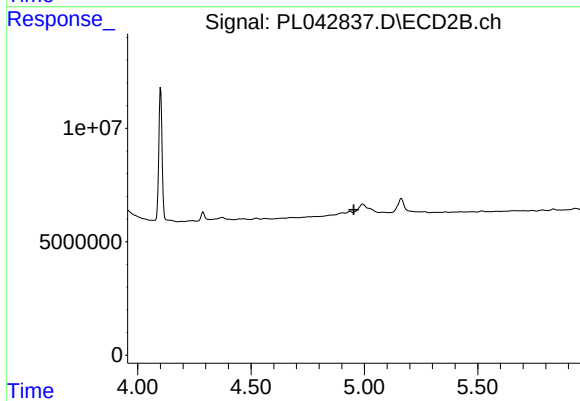

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

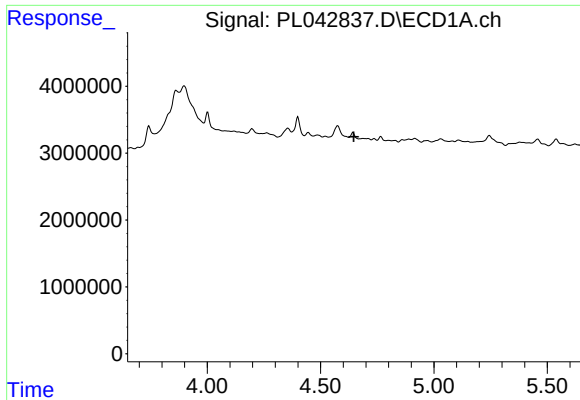

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

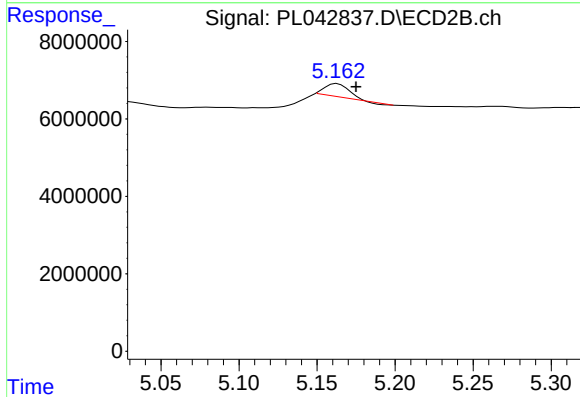


#7 delta-BHC

R.T.: 5.163 min
Delta R.T.: -0.012 min
Response: 2976834
Conc: 0.81 ng/ml

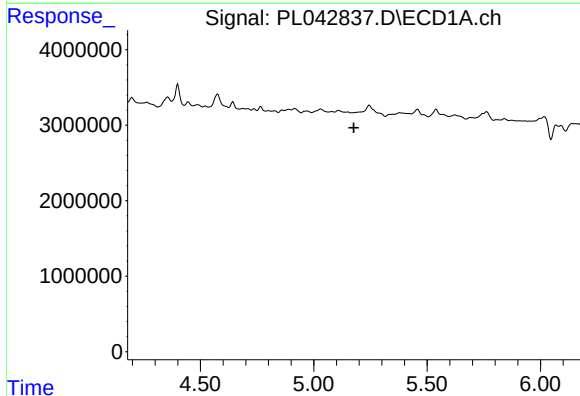


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

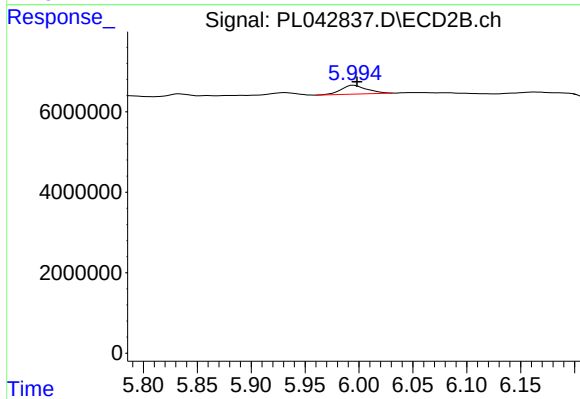

#8 Heptachlor epoxide


R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 3696436
Conc: 1.03 ng/ml

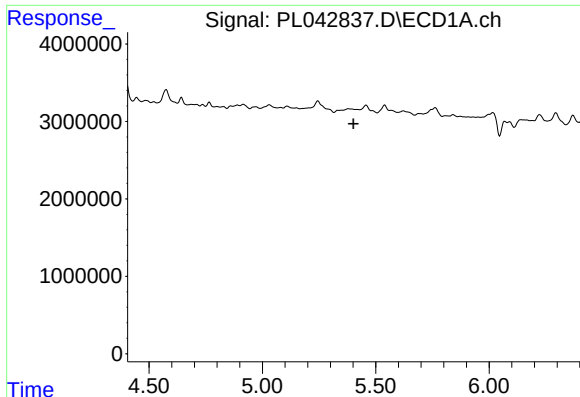

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

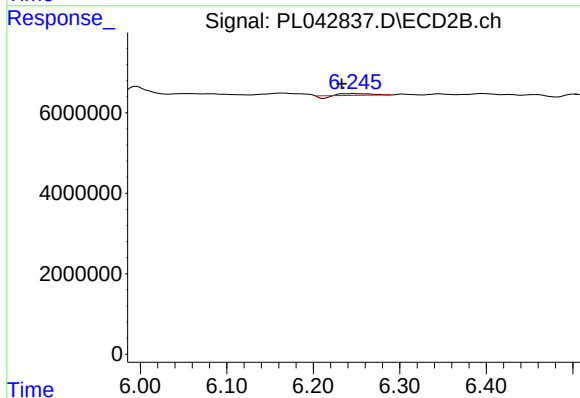


#10 gamma-Chlordane

R.T.: 6.248 min
Delta R.T.: 0.015 min
Response: 799106
Conc: 0.23 ng/ml

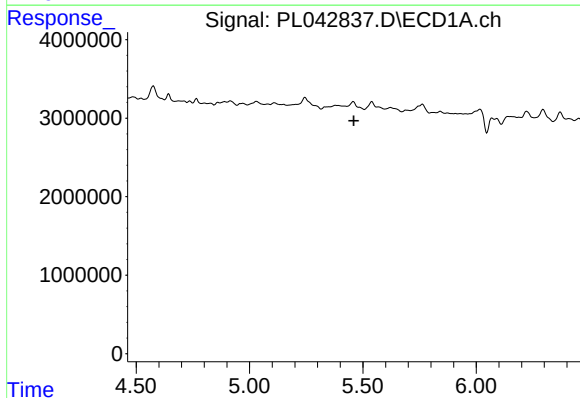


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

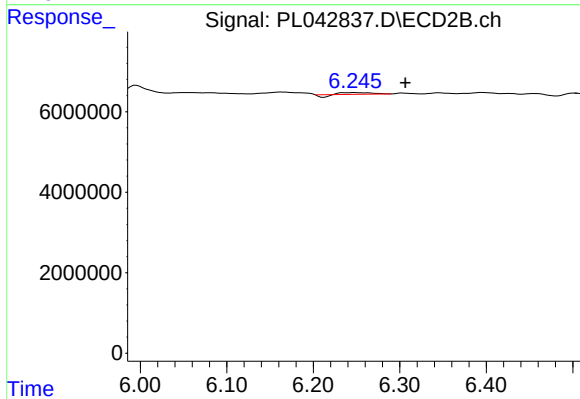

#11 alpha-Chlordane


R.T.: 6.248 min
Delta R.T.: -0.059 min
Response: 799106
Conc: 0.24 ng/ml

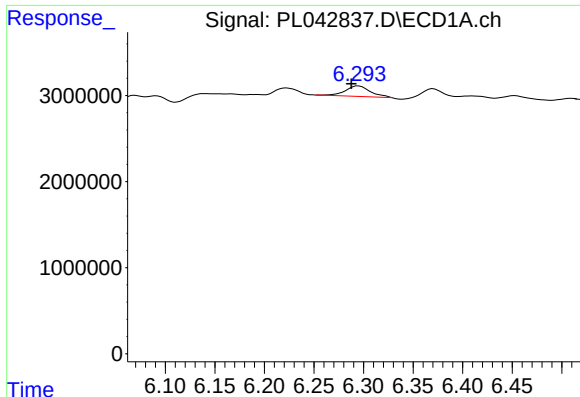

#15 Endosulfan II


R.T.: 6.295 min
Delta R.T.: 0.007 min
Response: 2118289
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

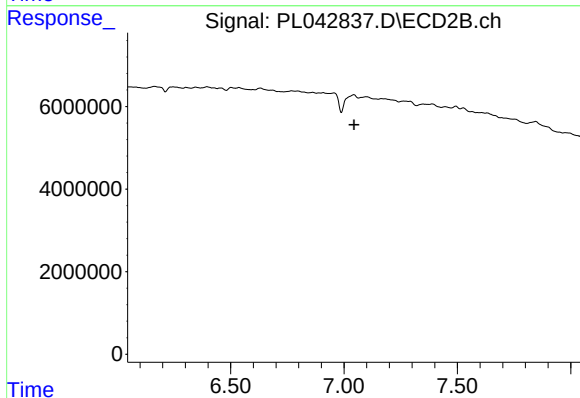


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

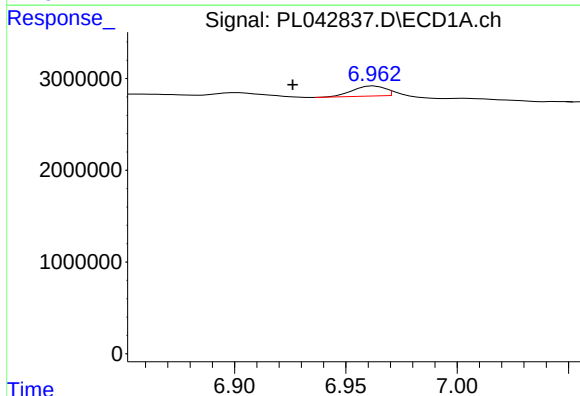


#20 Methoxychlor

R.T.: 6.963 min
Delta R.T.: 0.037 min
Response: 1108597
Conc: 0.35 ng/ml

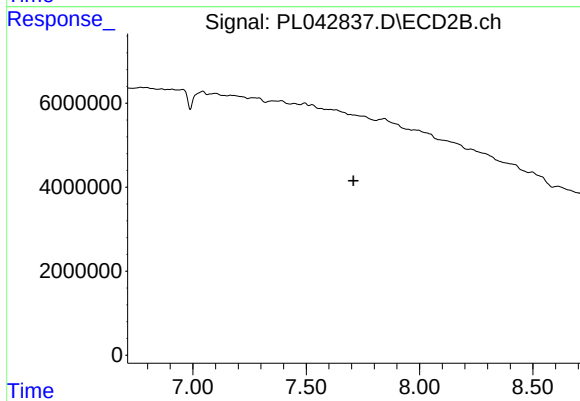

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

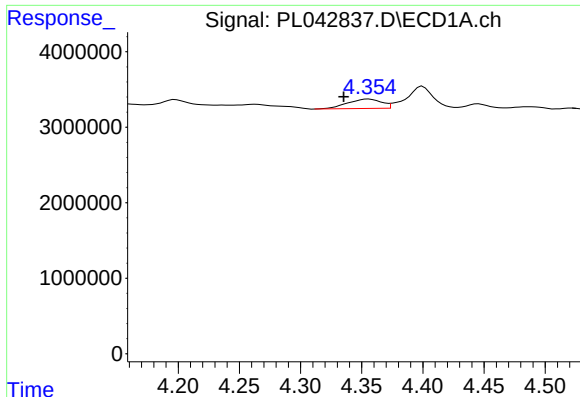

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.021 min
Response: 2420564
Conc: 8.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

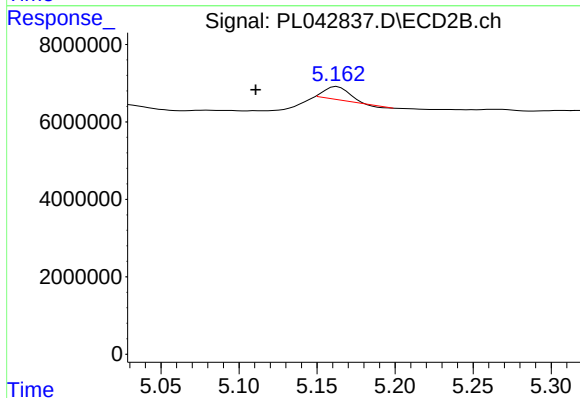


#23 Chlordane-1

R.T.: 5.163 min
Delta R.T.: 0.052 min
Response: 2976834
Conc: 22.39 ng/ml

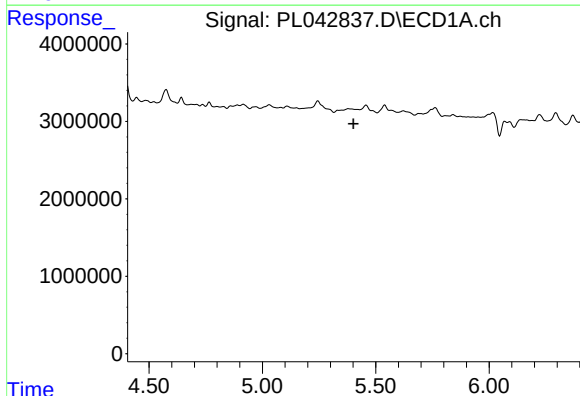


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

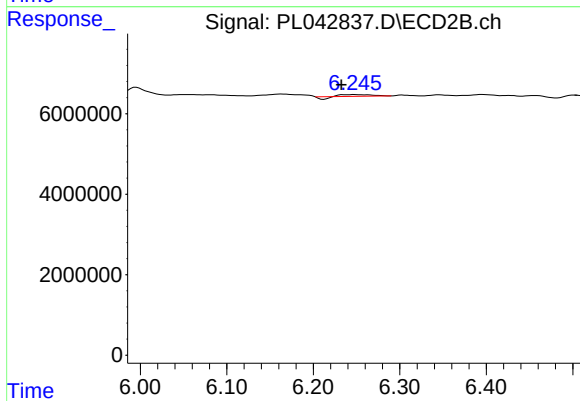

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: 0.015 min
Response: 799106
Conc: 1.70 ng/ml

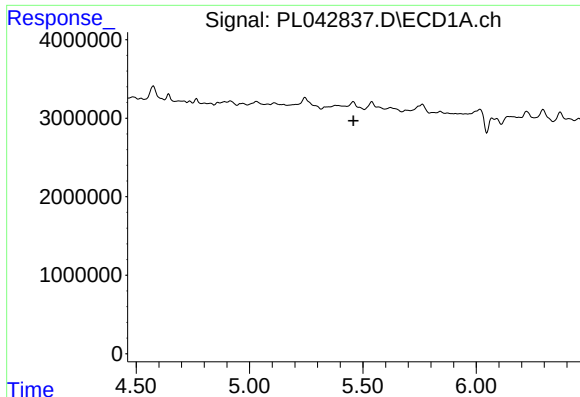

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

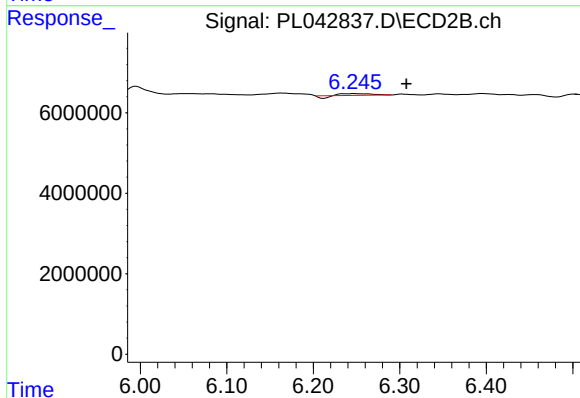


#26 Chlordane-4

R.T.: 6.248 min
Delta R.T.: -0.060 min
Response: 799106
Conc: 1.46 ng/ml

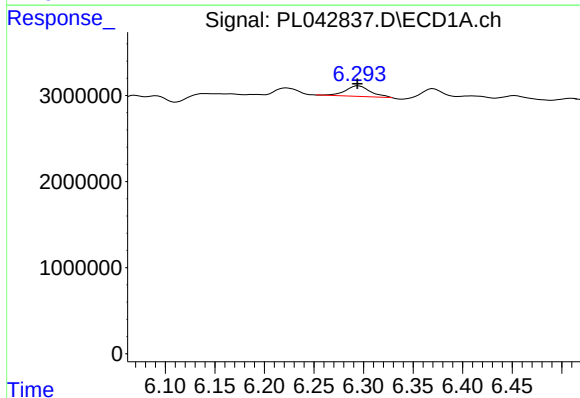


#27 Chlordane-5

R.T.: 6.295 min
Delta R.T.: 0.001 min
Response: 2118289
Conc: 7.11 ng/ml

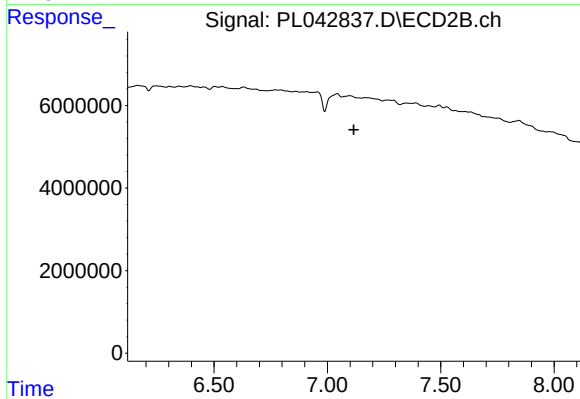

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.117 min
Response: 0
Conc: N.D.

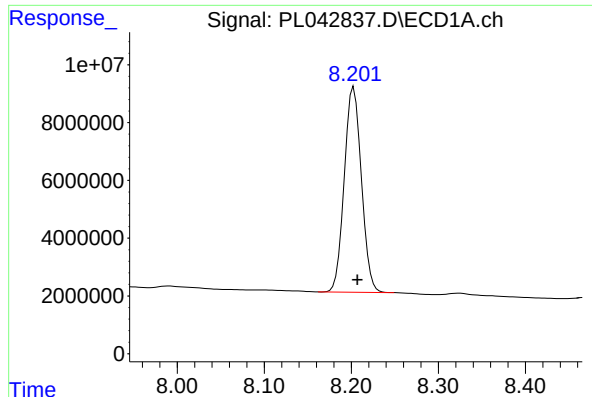

#28 Decachlorobiphenyl


R.T.: 8.203 min

Delta R.T.: -0.004 min

Response: 97100672

Conc: 15.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

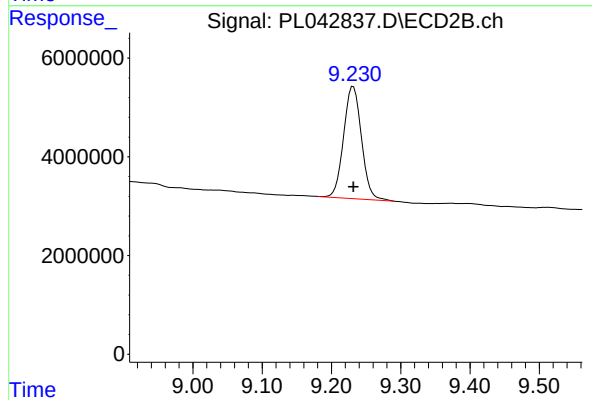

#28 Decachlorobiphenyl

R.T.: 9.231 min

Delta R.T.: 0.000 min

Response: 40591096

Conc: 16.83 ng/ml