

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2018 21:18
 Operator : AJ\SJ
 Sample : J6214-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:10:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	59939017	30160636	10.188	10.487
28)	SA Decachlor...	8.203	9.232	73690571	30658622	11.693	12.712
Target Compounds							
4)	MA Heptachlor	4.519	0.000	712227	0	0.082	N.D. #
9)	A Endosulfan I	0.000	6.357	0	1723382	N.D.	0.546 #
10)	B gamma-Chl...	0.000	6.247	0	3321161	N.D.	0.976 #
11)	B alpha-Chl...	0.000	6.302	0	4764973	N.D.	1.425 #
23)	Chlordane-1	4.343	0.000	5067683	0	18.330	N.D. #
24)	Chlordane-2	0.000	5.544	0	1482594	N.D.	10.632 #
25)	Chlordane-3	0.000	6.247	0	3321161	N.D.	7.067 #
26)	Chlordane-4	0.000	6.302	0	4764973	N.D.	8.709 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2018 21:18
Operator : AJ\SJ
Sample : J6214-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:10:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

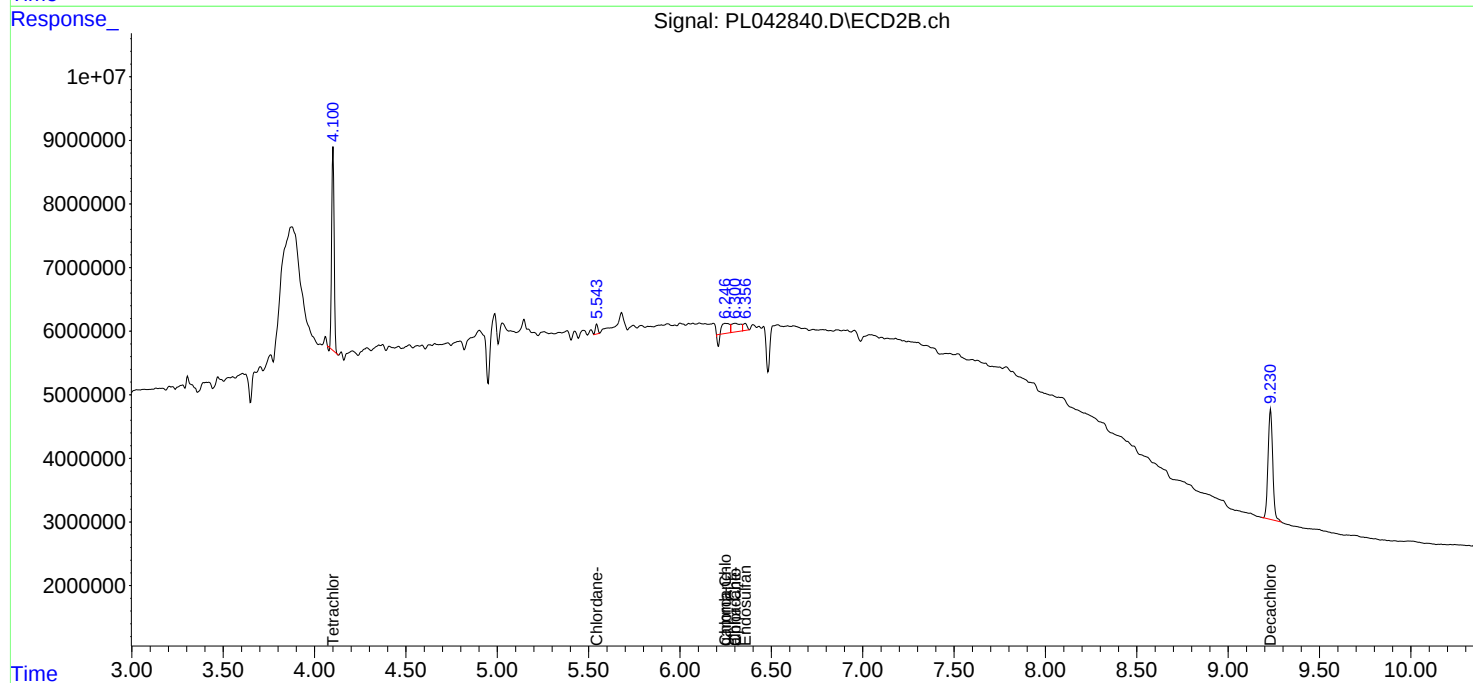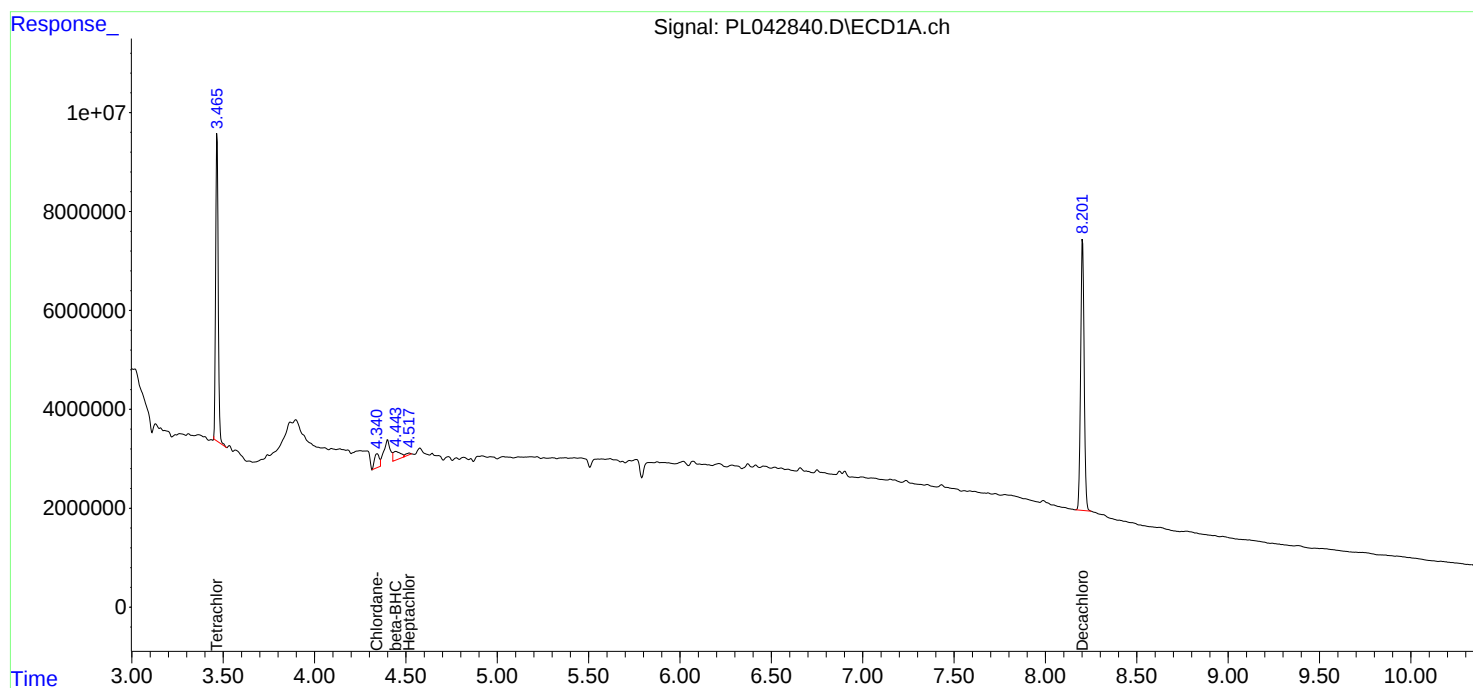


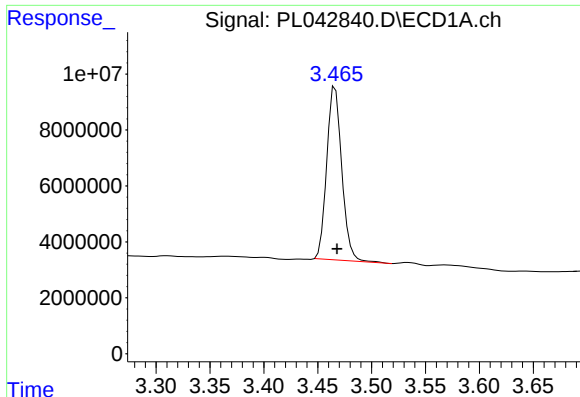

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 59939017
Conc: 10.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

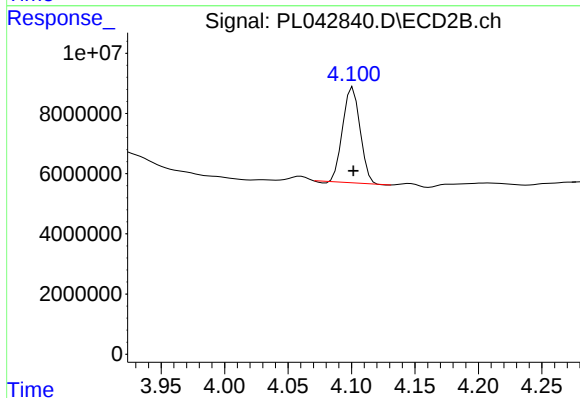


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 30160636
Conc: 10.49 ng/ml

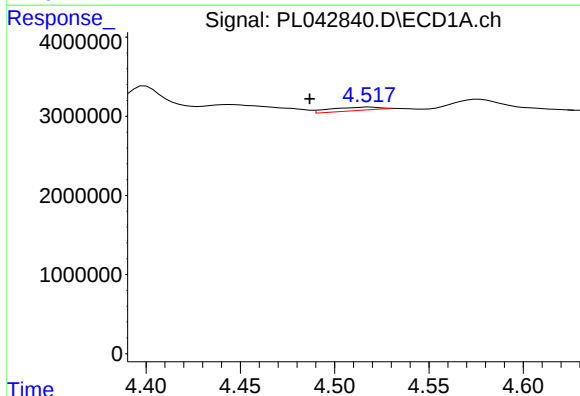


#4 Heptachlor

R.T.: 4.519 min
Delta R.T.: 0.032 min
Response: 712227
Conc: 0.08 ng/ml

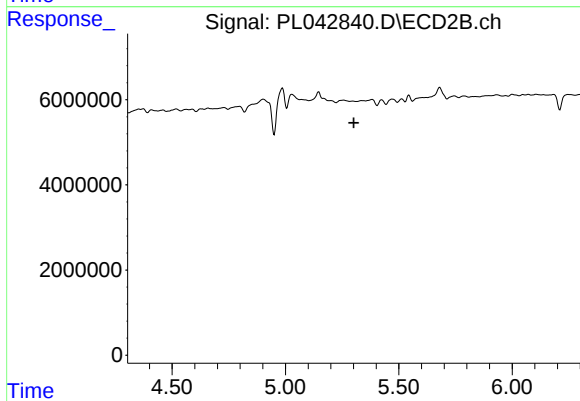

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.301 min
Response: 0
Conc: N.D.

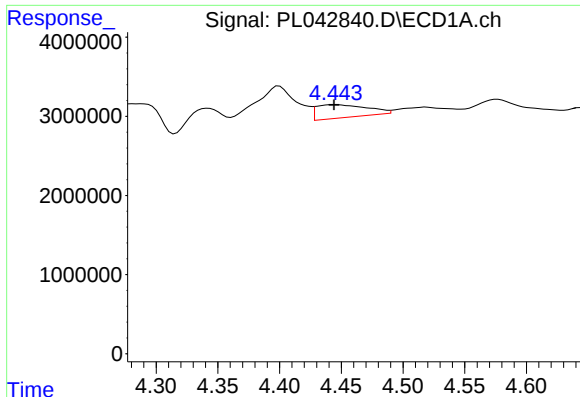

#6 beta-BHC


R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 4684781
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

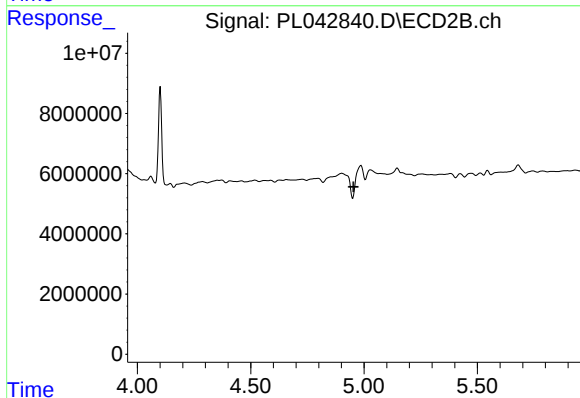


#6 beta-BHC

R.T.: 4.986 min
Delta R.T.: 0.033 min
Response: -4892288
Conc: N.D.

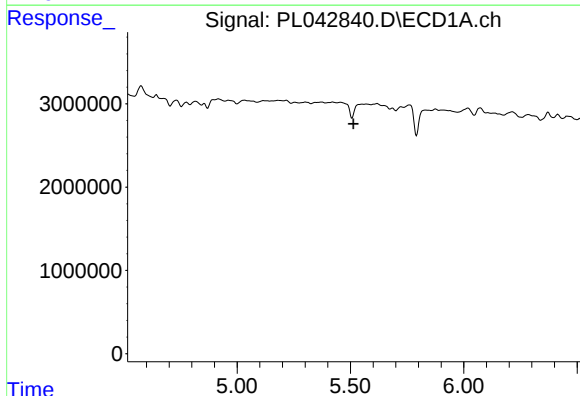


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.514 min
Response: 0
Conc: N.D.

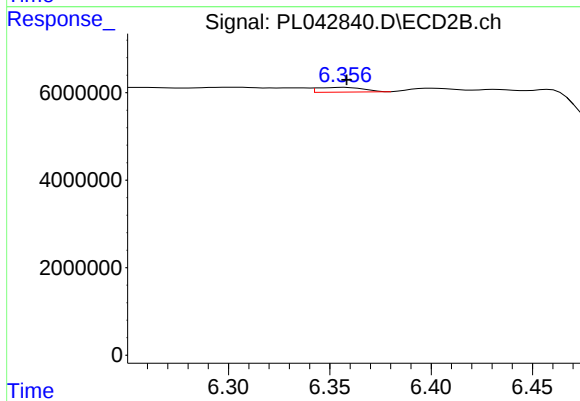

#9 Endosulfan I


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1723382
Conc: 0.55 ng/ml

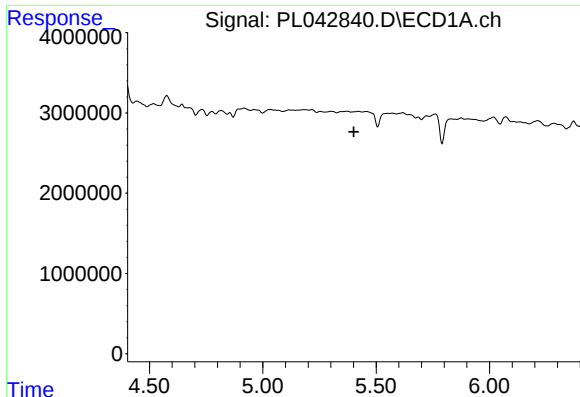

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

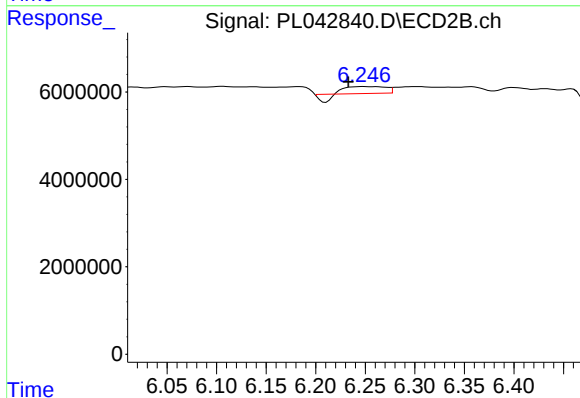


#10 gamma-Chlordane

R.T.: 6.247 min
Delta R.T.: 0.014 min
Response: 3321161
Conc: 0.98 ng/ml

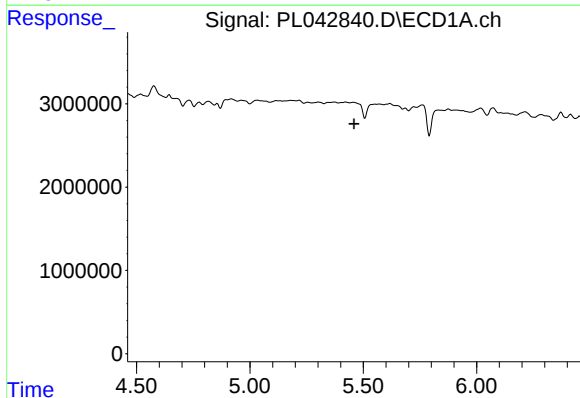


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

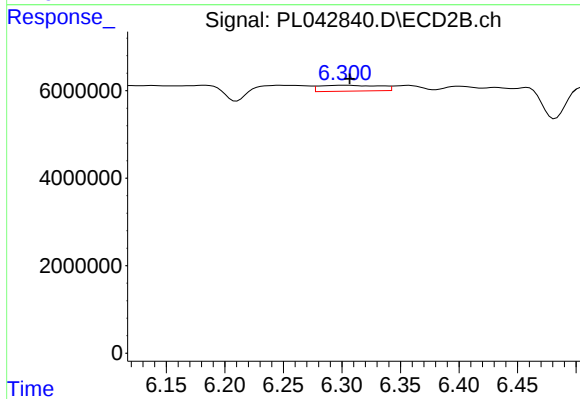

#11 alpha-Chlordane


R.T.: 6.302 min
Delta R.T.: -0.004 min
Response: 4764973
Conc: 1.43 ng/ml

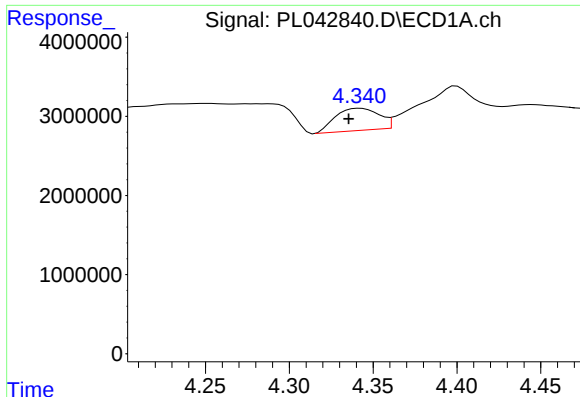

#23 Chlordane-1


R.T.: 4.343 min
Delta R.T.: 0.007 min
Response: 5067683
Conc: 18.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

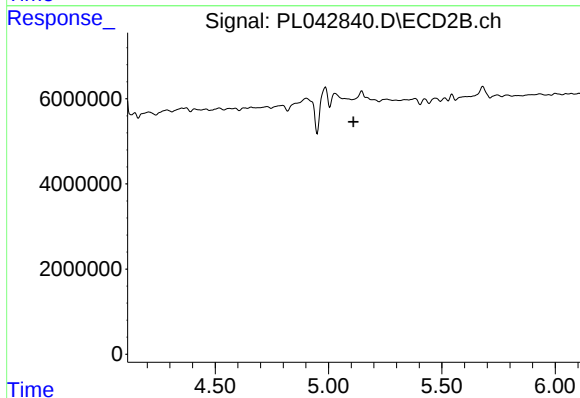


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

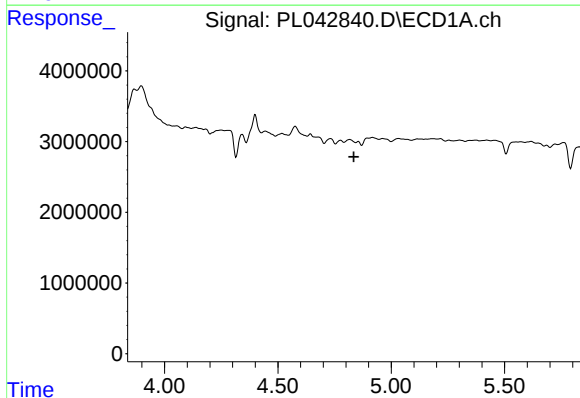


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.835 min
Response: 0
Conc: N.D.

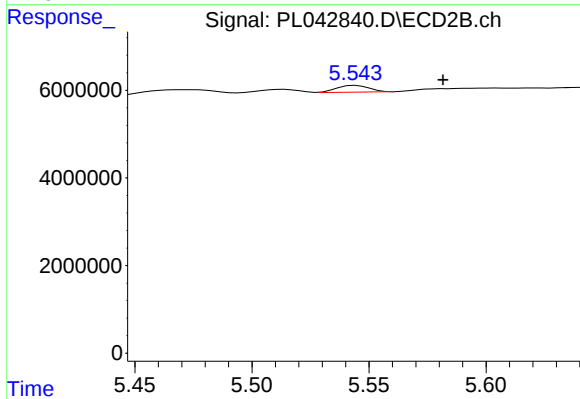

#24 Chlordane-2


R.T.: 5.544 min
Delta R.T.: -0.037 min
Response: 1482594
Conc: 10.63 ng/ml

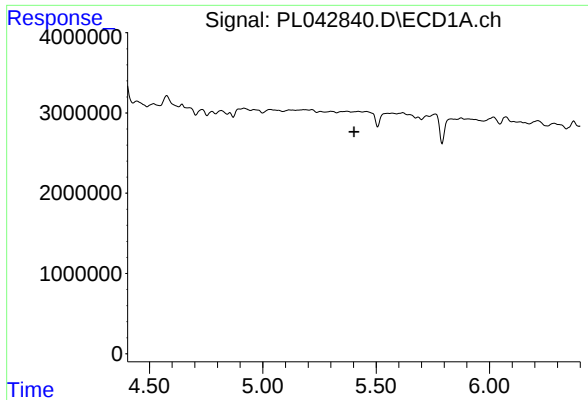

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

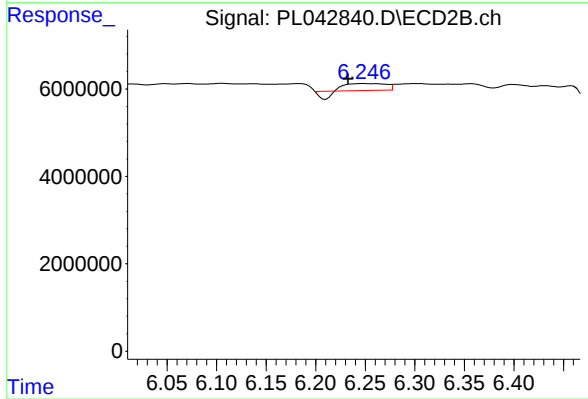


#25 Chlordane-3

R.T.: 6.247 min
Delta R.T.: 0.015 min
Response: 3321161
Conc: 7.07 ng/ml

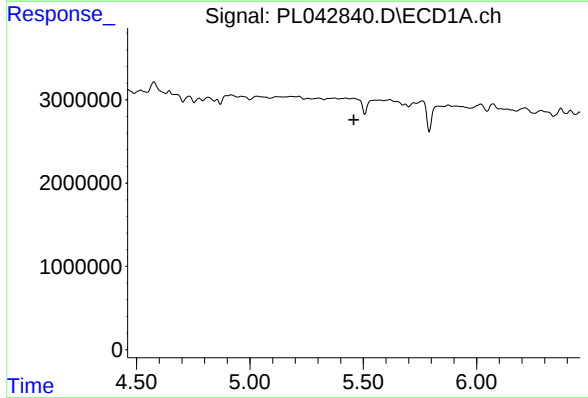


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

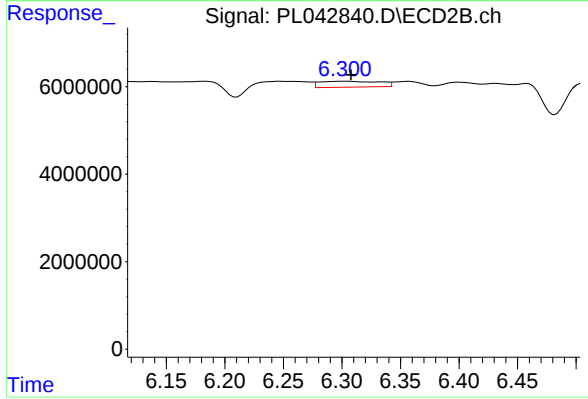

#26 Chlordane-4


R.T.: 6.302 min
Delta R.T.: -0.006 min
Response: 4764973
Conc: 8.71 ng/ml

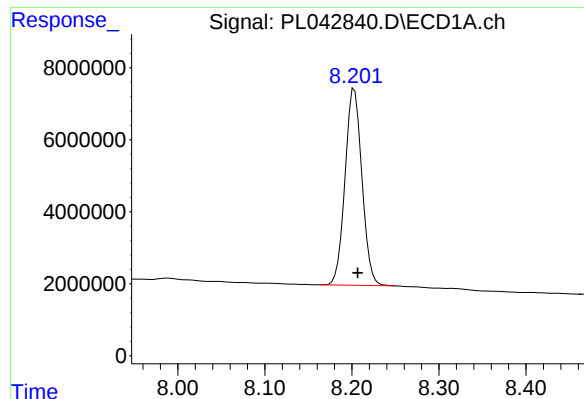

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 73690571
Conc: 11.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

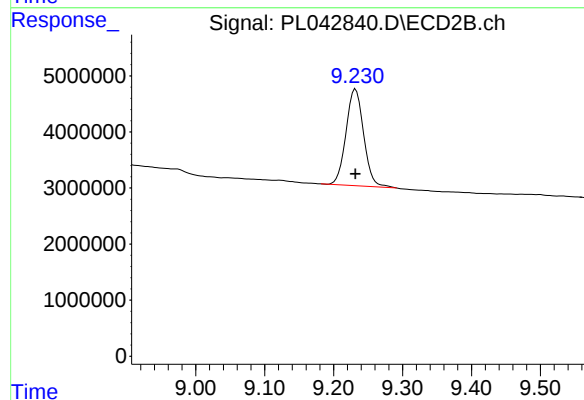

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 30658622
Conc: 12.71 ng/ml