

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2018 03:11
 Operator : AJ\SJ
 Sample : J6214-25
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 04:12:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	59610534	28949665	10.132	10.065
28)	SA Decachlor...	8.204	9.231	68875632	30195714	10.929	12.520
Target Compounds							
4)	MA Heptachlor	0.000	5.328	0	1858592	N.D.	0.474 #
8)	B Heptachlo...	0.000	5.998	0	2309382	N.D.	0.644 #
9)	A Endosulfan I	0.000	6.309 ^f	0	4232498	N.D.	1.340 #
10)	B gamma-Chl...	0.000	6.240	0	3287670	N.D.	0.966 #
11)	B alpha-Chl...	0.000	6.309	0	4232498	N.D.	1.266 #
14)	MA Endrin	0.000	6.856	0	1707057	N.D.	0.620 #
23)	Chlordane-1	4.346	5.065	1730284	767375	6.258	5.773
24)	Chlordane-2	0.000	5.542	0	10332369	N.D.	74.097 #
25)	Chlordane-3	0.000	6.240	0	3287670	N.D.	6.996 #
26)	Chlordane-4	0.000	6.309	0	4232498	N.D.	7.735 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2018 03:11
Operator : AJ\SJ
Sample : J6214-25
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 04:12:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

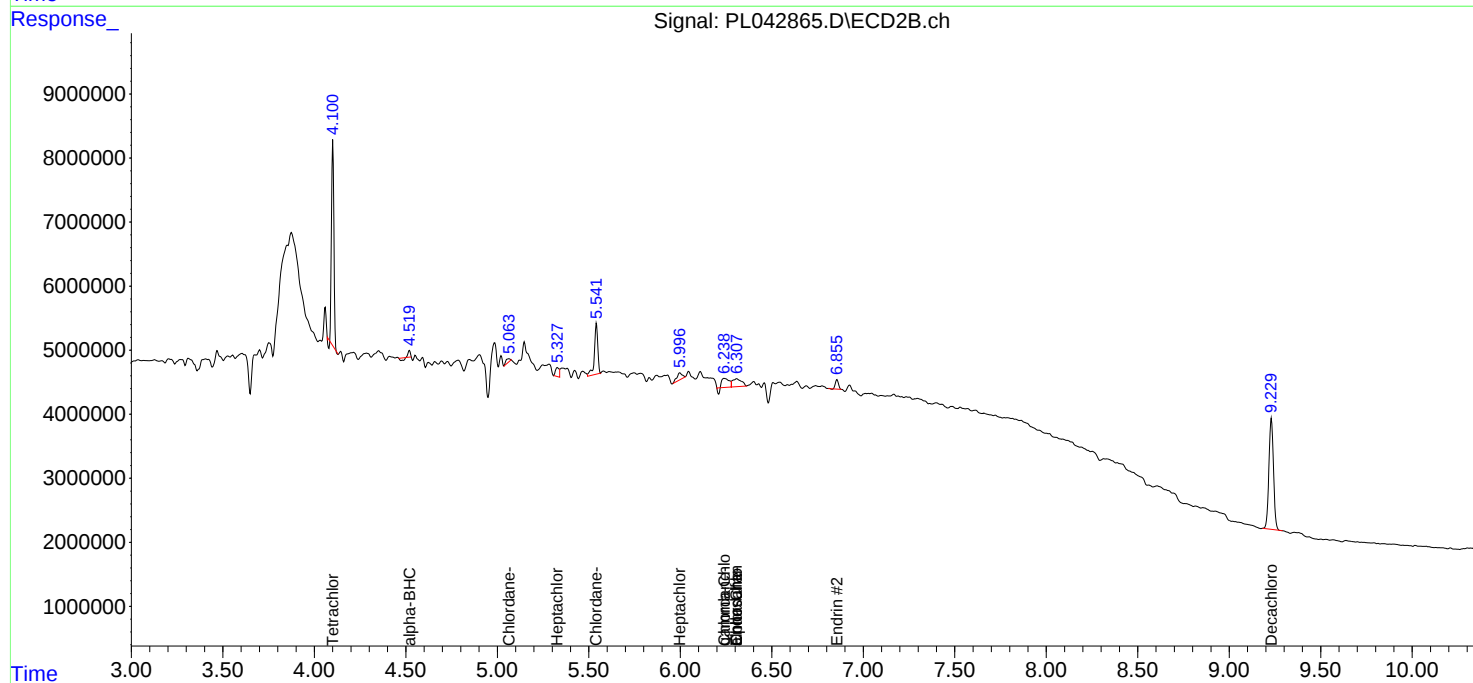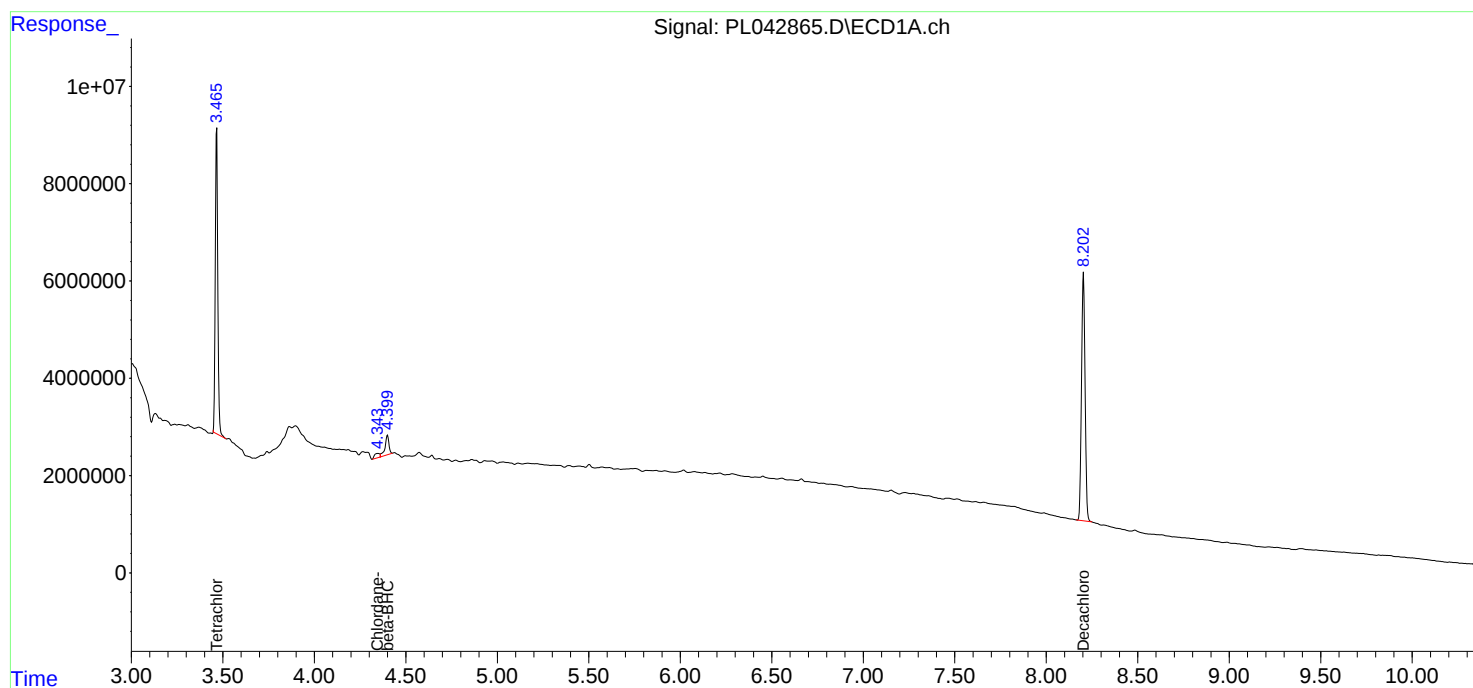


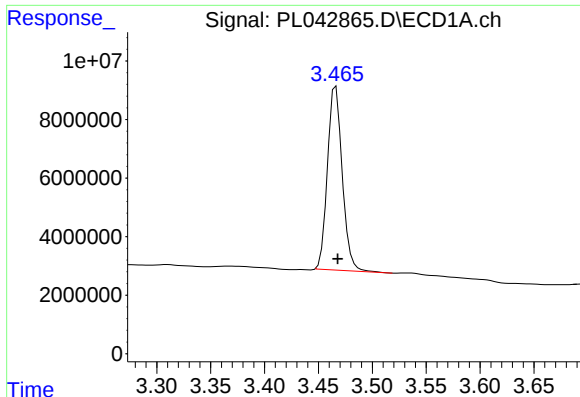

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 59610534
Conc: 10.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

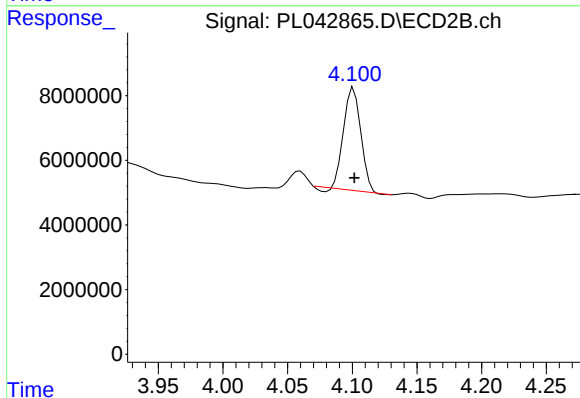


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 28949665
Conc: 10.07 ng/ml

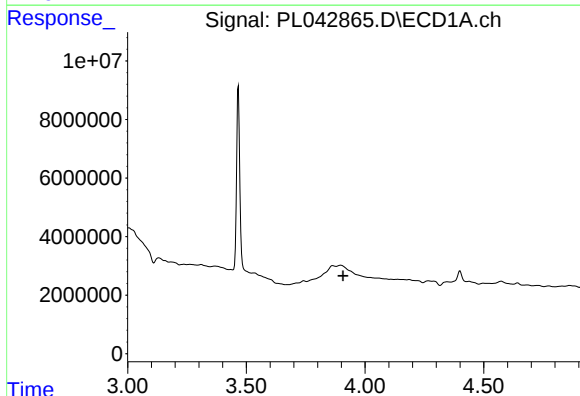


#2 alpha-BHC

R.T.: 3.864 min
Delta R.T.: -0.044 min
Response: -2667138
Conc: N.D.

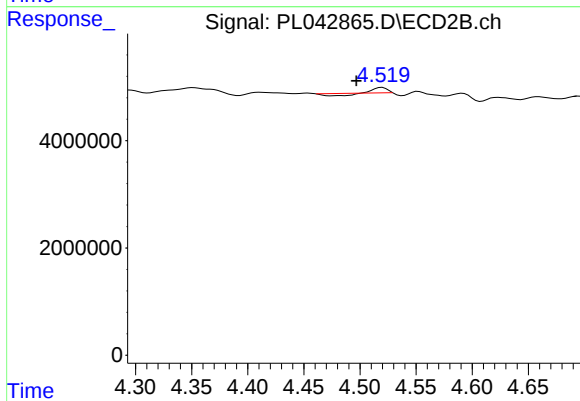

#2 alpha-BHC


R.T.: 4.520 min
Delta R.T.: 0.023 min
Response: 292087
Conc: 0.07 ng/ml

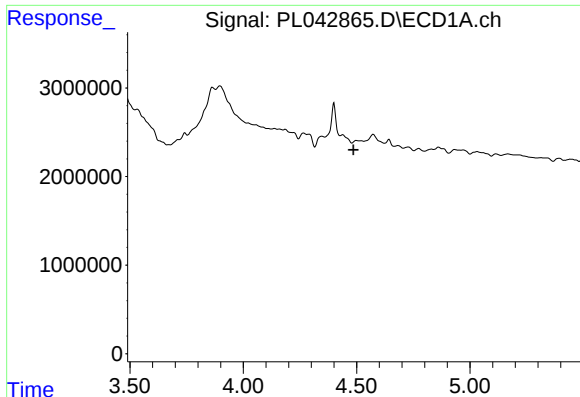

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

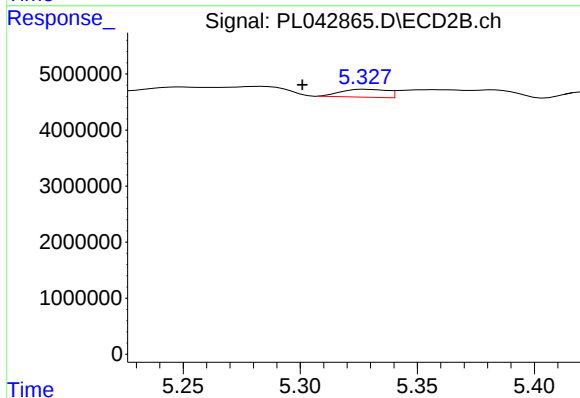


#4 Heptachlor

R.T.: 5.328 min
Delta R.T.: 0.027 min
Response: 1858592
Conc: 0.47 ng/ml

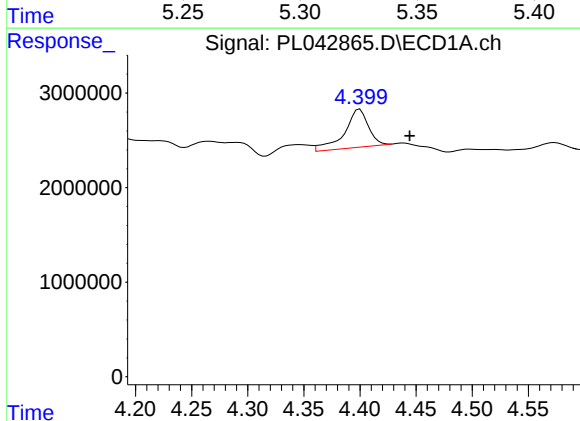


#6 beta-BHC

R.T.: 4.400 min
Delta R.T.: -0.044 min
Response: 5960882
Conc: 1.68 ng/ml

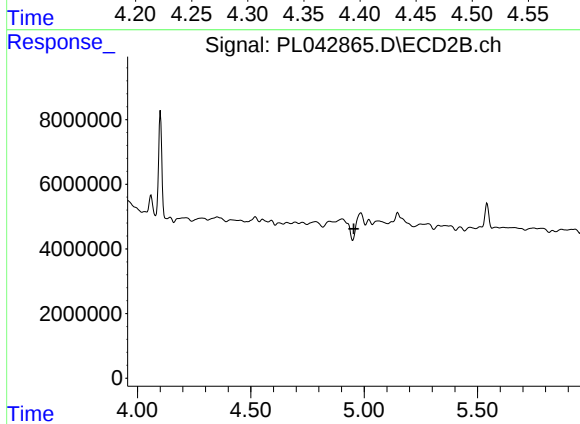

#6 beta-BHC


R.T.: 4.986 min
Delta R.T.: 0.032 min
Response: -3214152
Conc: N.D.

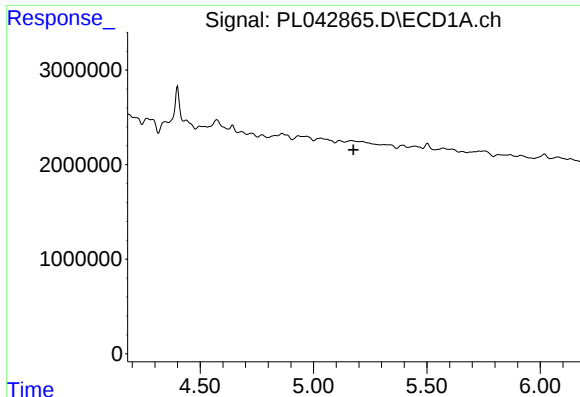

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

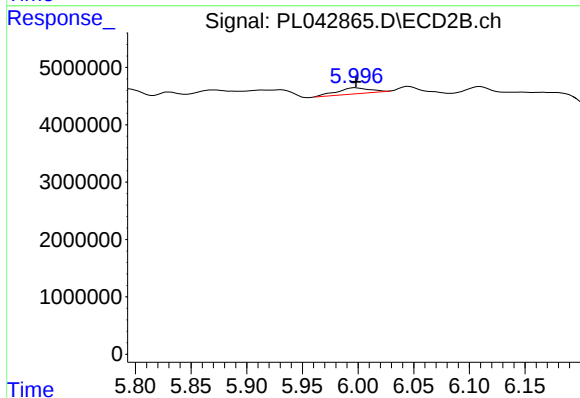


#8 Heptachlor epoxide

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 2309382
Conc: 0.64 ng/ml

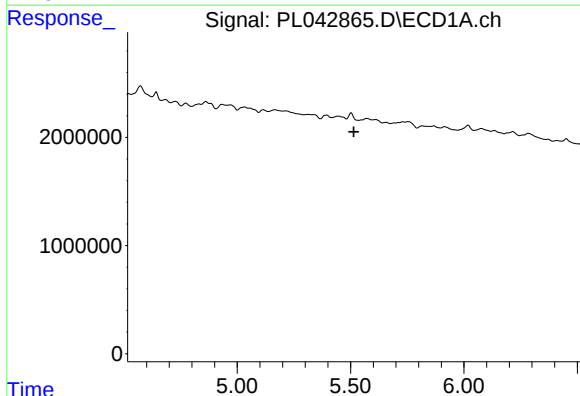


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.514 min
Response: 0
Conc: N.D.

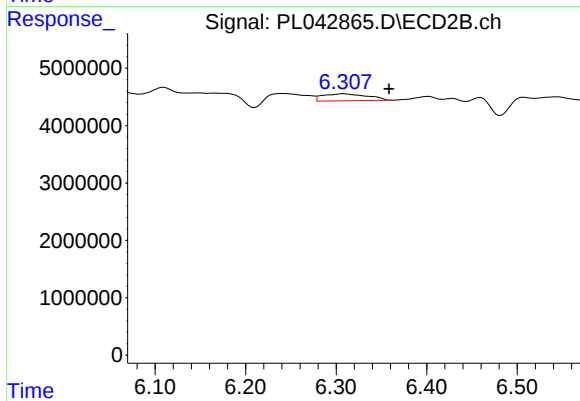

#9 Endosulfan I


R.T.: 6.309 min
Delta R.T.: -0.050 min
Response: 4232498
Conc: 1.34 ng/ml

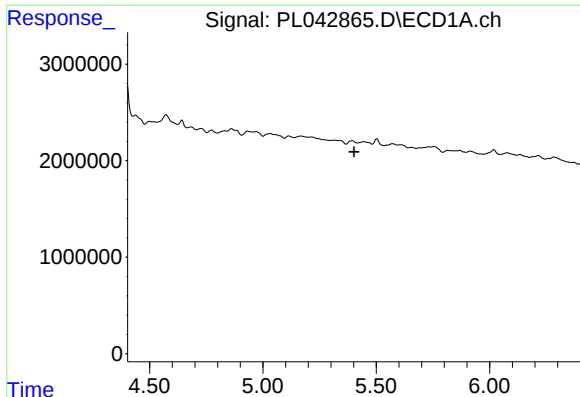

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

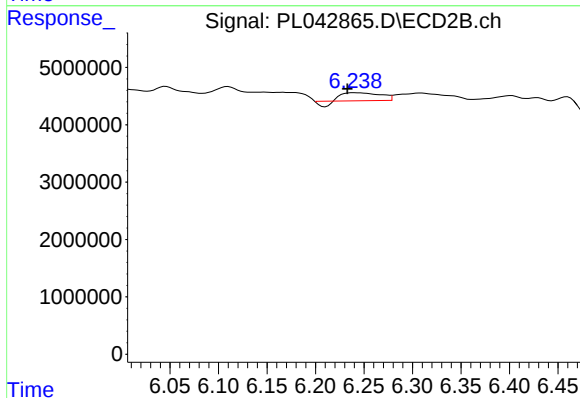


#10 gamma-Chlordane

R.T.: 6.240 min
Delta R.T.: 0.007 min
Response: 3287670
Conc: 0.97 ng/ml

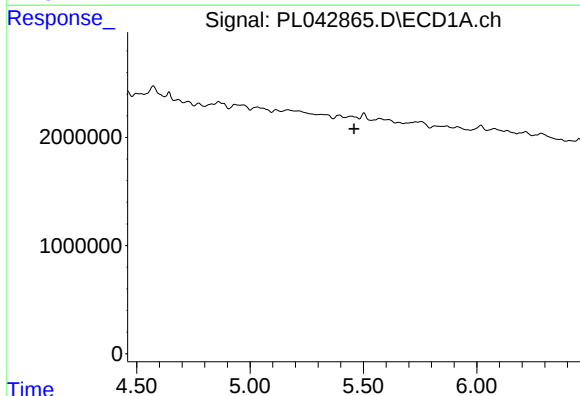


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

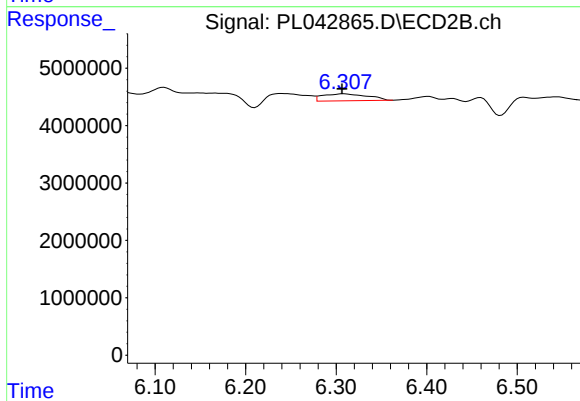

#11 alpha-Chlordane


R.T.: 6.309 min
Delta R.T.: 0.002 min
Response: 4232498
Conc: 1.27 ng/ml

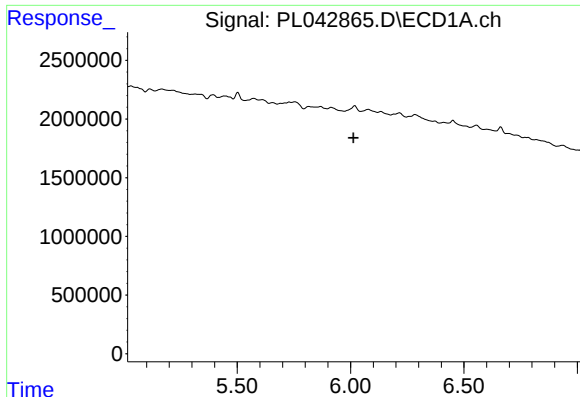

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

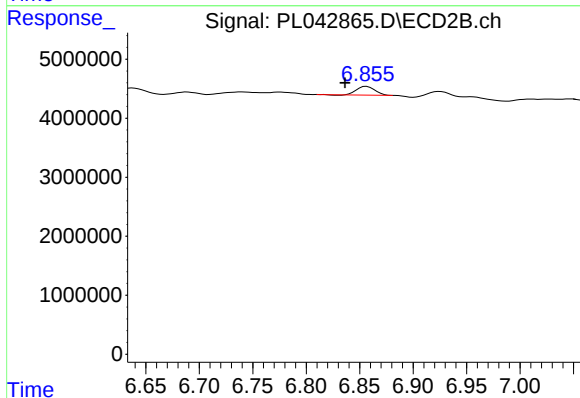


#14 Endrin

R.T.: 6.856 min
Delta R.T.: 0.020 min
Response: 1707057
Conc: 0.62 ng/ml

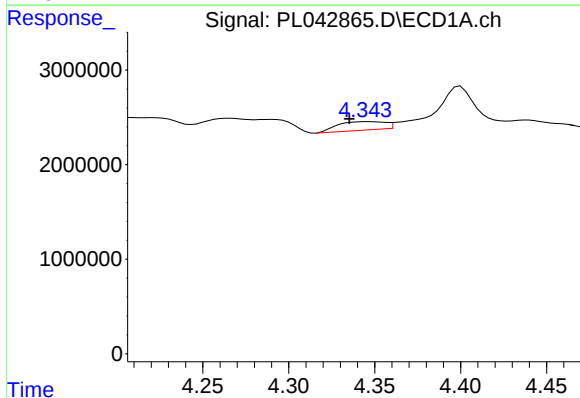


#23 Chlordane-1

R.T.: 4.346 min
Delta R.T.: 0.011 min
Response: 1730284
Conc: 6.26 ng/ml

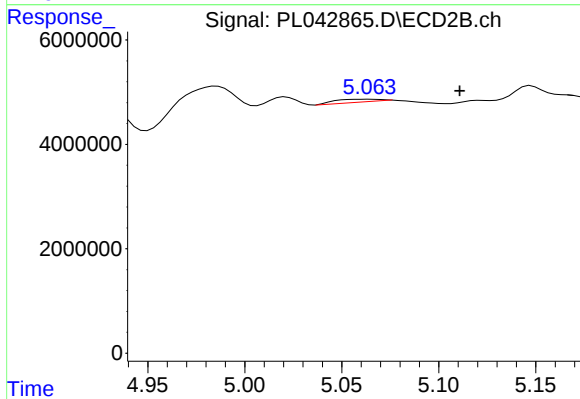

#23 Chlordane-1


R.T.: 5.065 min
Delta R.T.: -0.046 min
Response: 767375
Conc: 5.77 ng/ml

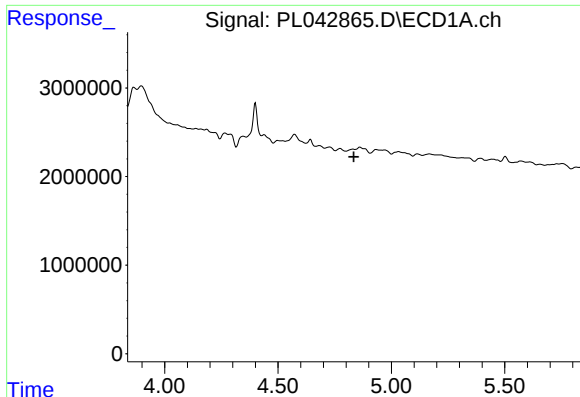

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

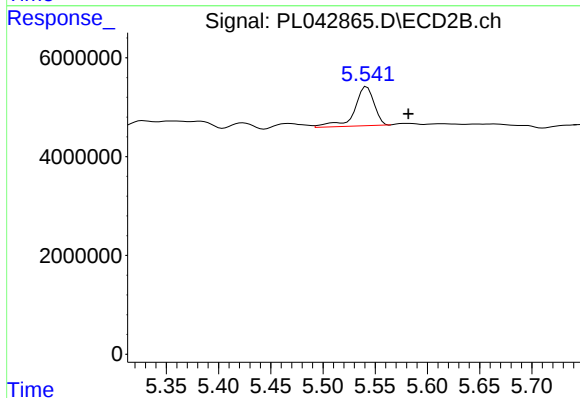


#24 Chlordane-2

R.T.: 5.542 min
Delta R.T.: -0.040 min
Response: 10332369
Conc: 74.10 ng/ml

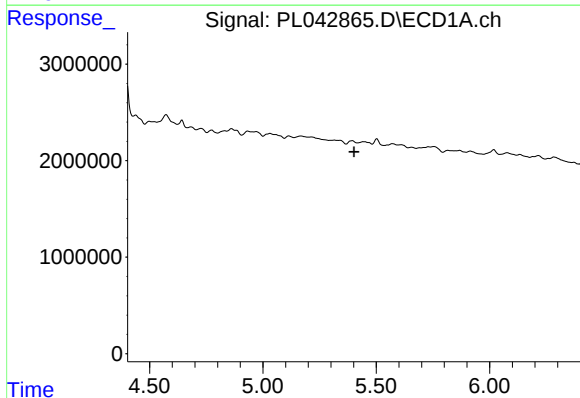


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

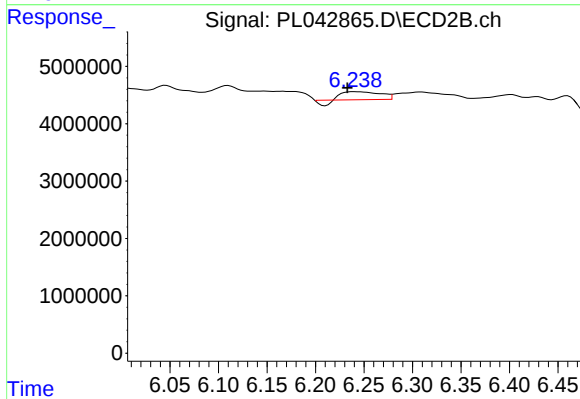

#25 Chlordane-3


R.T.: 6.240 min
Delta R.T.: 0.007 min
Response: 3287670
Conc: 7.00 ng/ml

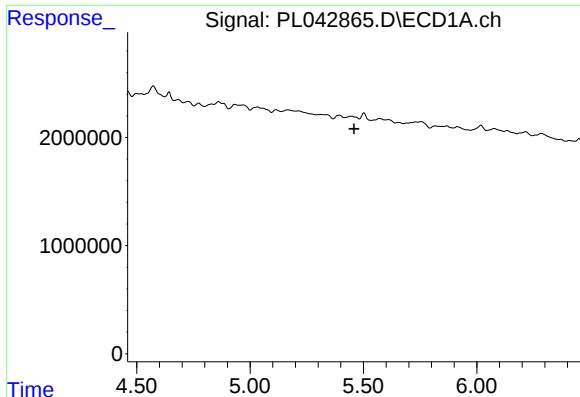

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

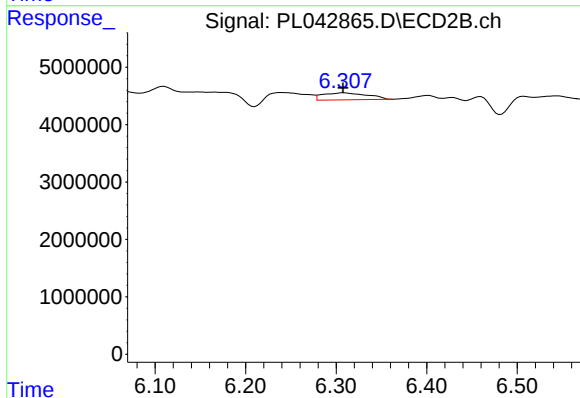


#26 Chlordane-4

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 4232498
Conc: 7.74 ng/ml

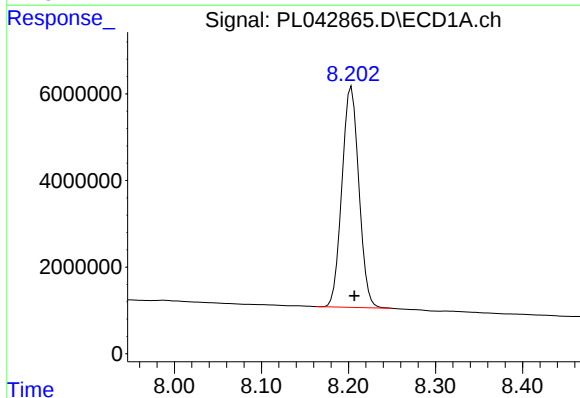

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 68875632
Conc: 10.93 ng/ml

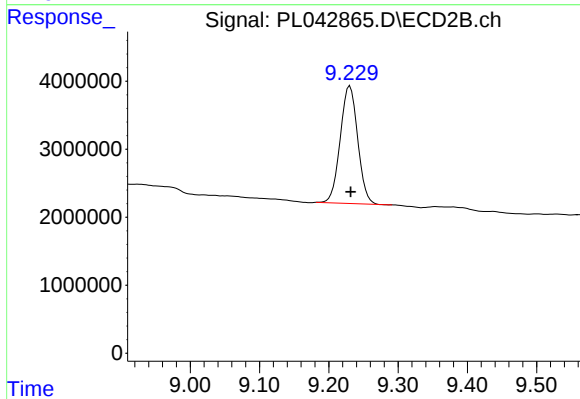

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 30195714
Conc: 12.52 ng/ml