

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
 Data File : PL042867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2018 03:39
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 04:13:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	111.2E6	58078975	18.903	20.193
28)	SA Decachlor...	8.202	9.230	113.0E6	47835235	17.923	19.833
Target Compounds							
6)	B beta-BHC	4.399f	0.000	3464639	0	0.978	N.D. #
8)	B Heptachlo...	0.000	5.995	0	2943213	N.D.	0.821 #
14)	MA Endrin	6.019	0.000	1550623	0	0.237	N.D. #
15)	B Endosulfa...	6.301	0.000	3418612	0	0.547	N.D. #
23)	Chlordane-1	4.399	0.000	3464639	0	12.532	N.D. #
27)	Chlordane-5	6.301	0.000	3418612	0	11.473	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120518\
Data File : PL042867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2018 03:39
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 04:13:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

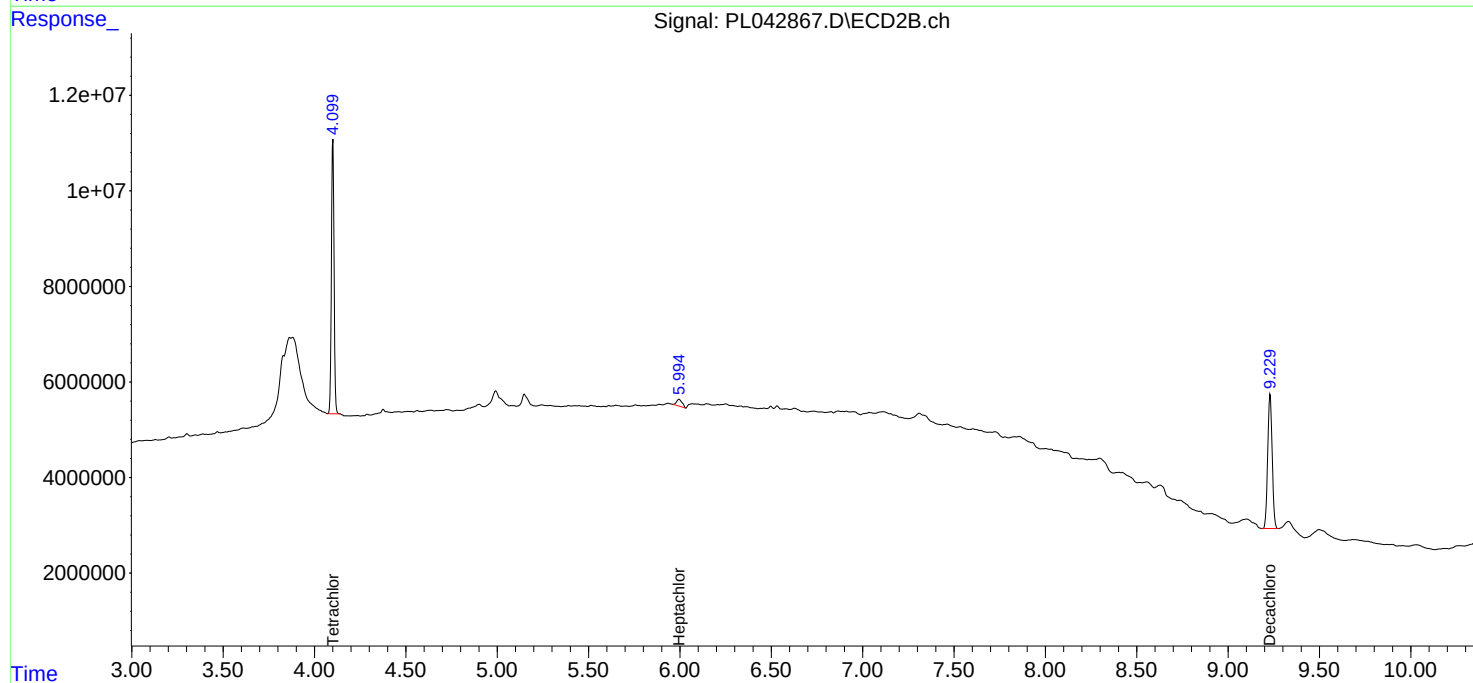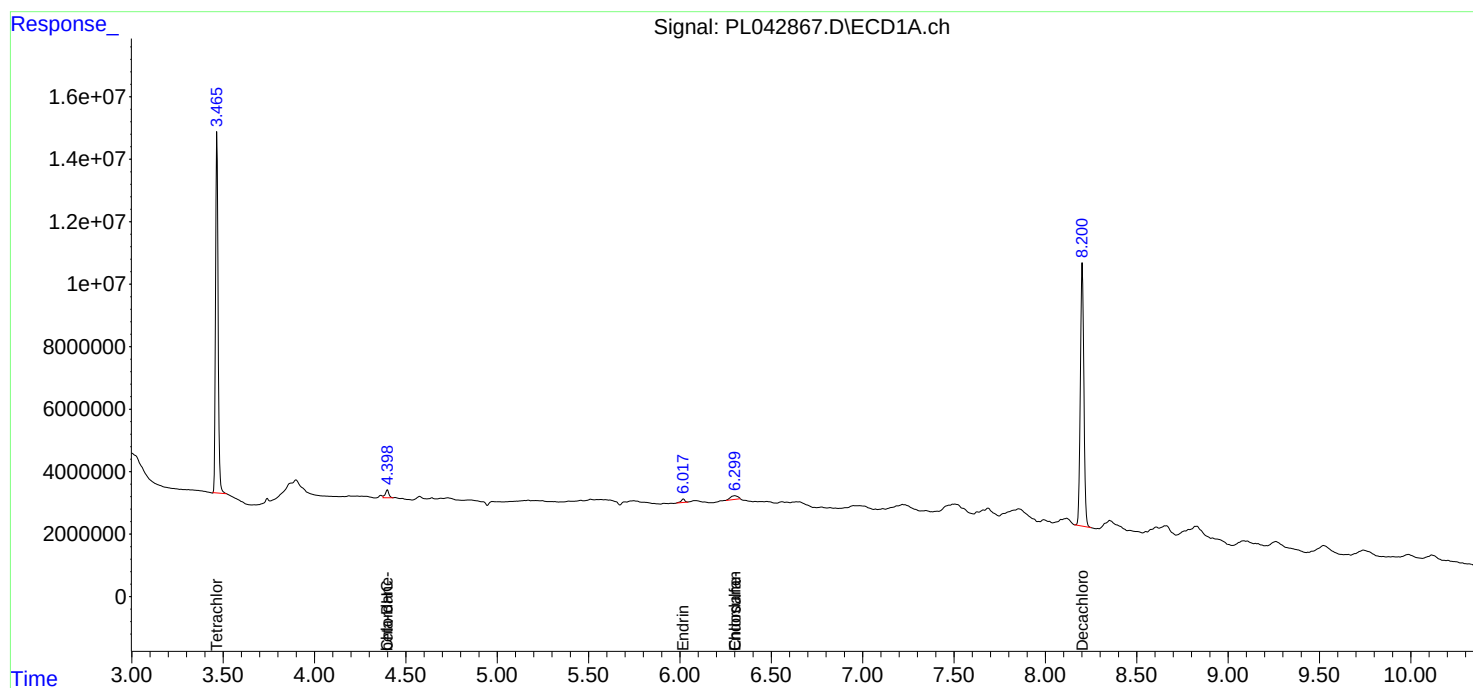


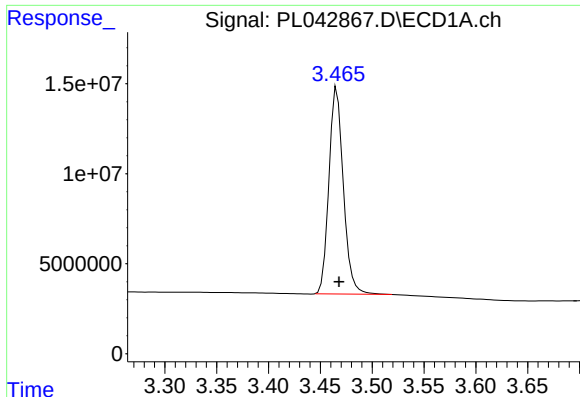

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 111215293
Conc: 18.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

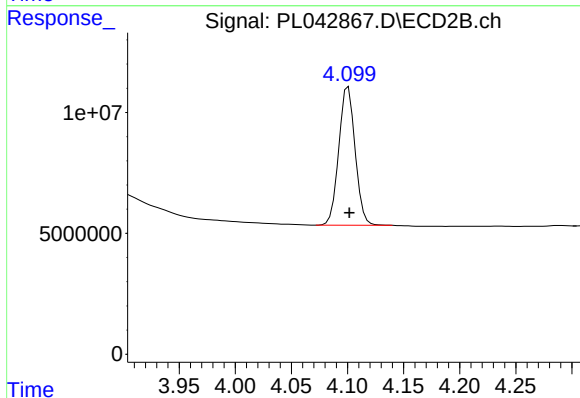


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 58078975
Conc: 20.19 ng/ml

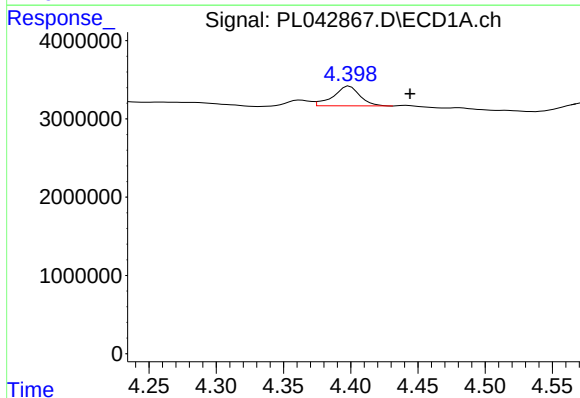


#6 beta-BHC

R.T.: 4.399 min
Delta R.T.: -0.045 min
Response: 3464639
Conc: 0.98 ng/ml

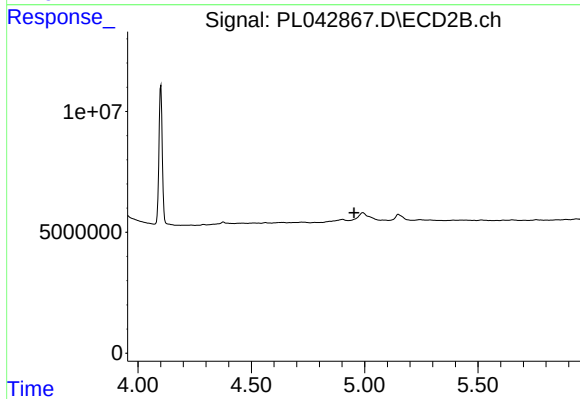

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

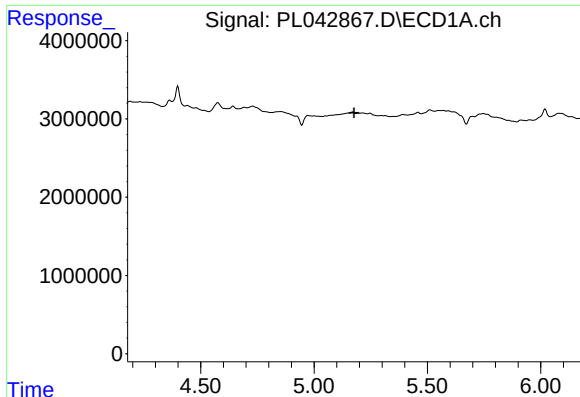

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

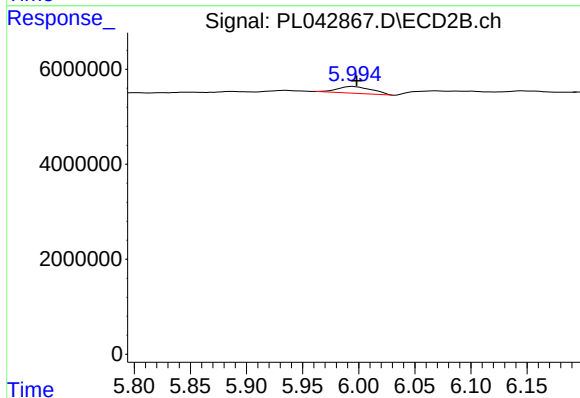


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: -0.003 min
Response: 2943213
Conc: 0.82 ng/ml

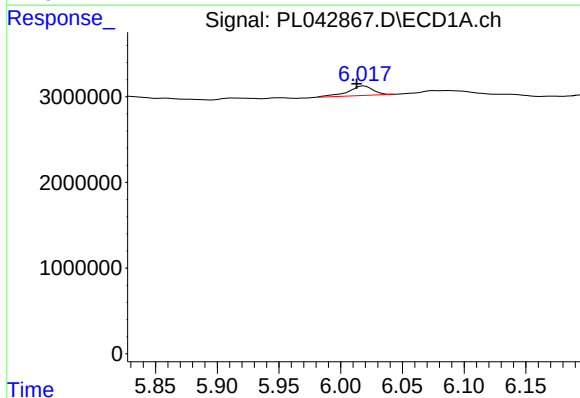


#14 Endrin

R.T.: 6.019 min
Delta R.T.: 0.006 min
Response: 1550623
Conc: 0.24 ng/ml

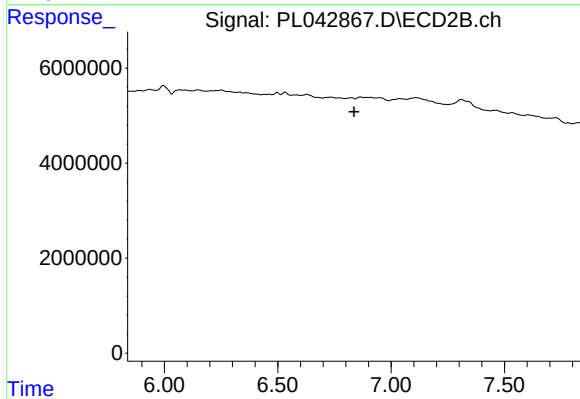

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.836 min
Response: 0
Conc: N.D.

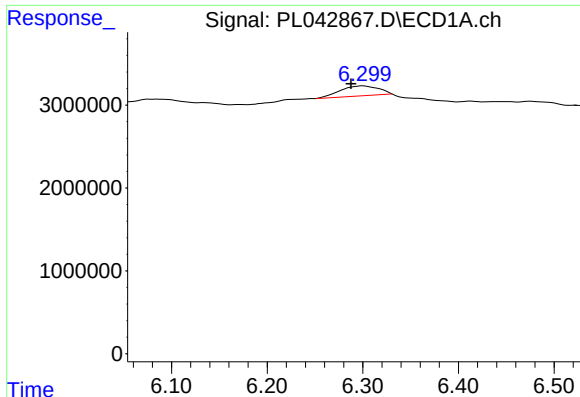

#15 Endosulfan II


R.T.: 6.301 min
Delta R.T.: 0.013 min
Response: 3418612
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

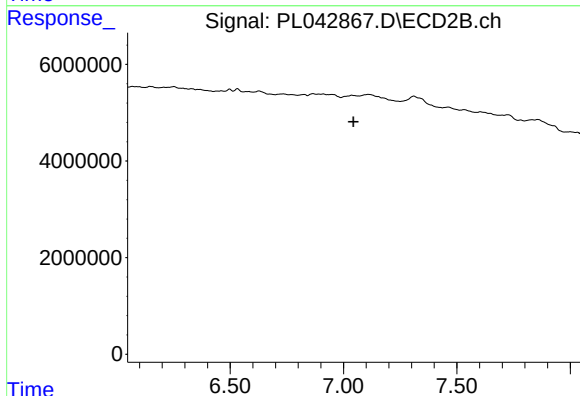


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

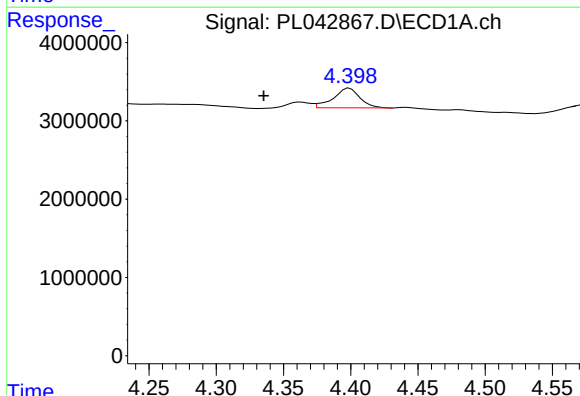


#23 Chlordane-1

R.T.: 4.399 min
Delta R.T.: 0.064 min
Response: 3464639
Conc: 12.53 ng/ml

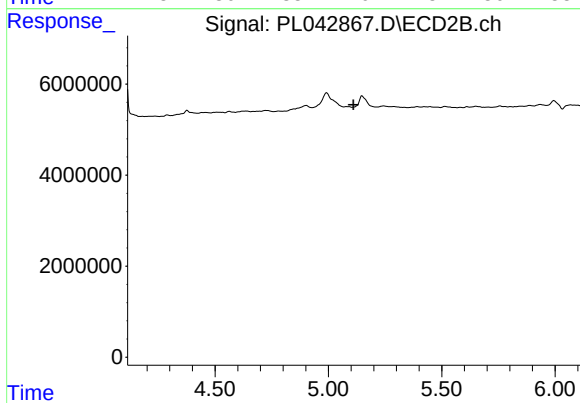

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

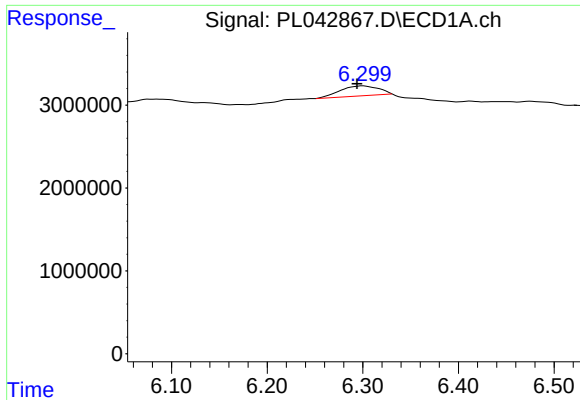

#27 Chlordane-5


R.T.: 6.301 min
Delta R.T.: 0.007 min
Response: 3418612
Conc: 11.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

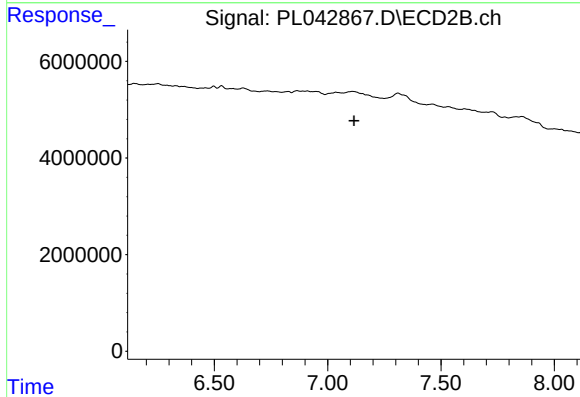


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.117 min
Response: 0
Conc: N.D.

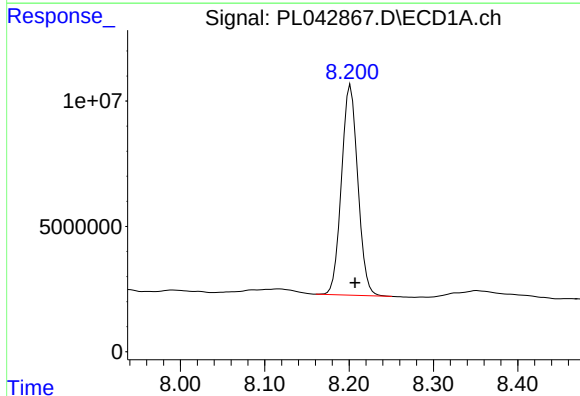

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 112953520
Conc: 17.92 ng/ml

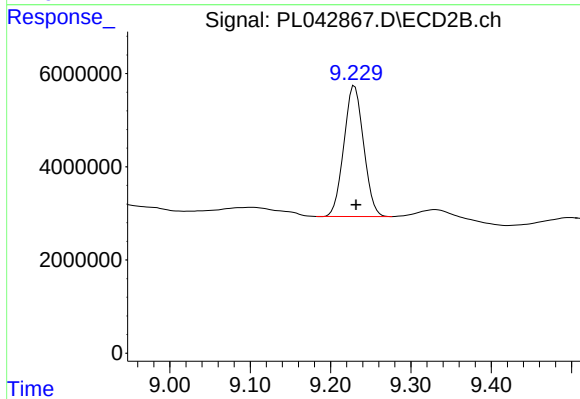

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.002 min
Response: 47835235
Conc: 19.83 ng/ml