

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120519\
 Data File : PL054778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 08:04
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 04:41:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.492f	0.000	10433559	0	1.407	N.D.	#
8) B	Heptachlo...	0.000	5.930	0	8533718	N.D.	3.416	#
9) A	Endosulfan I	5.622	0.000	36711502	0	2.692	N.D.	#
10) B	gamma-Chl...	5.516f	0.000	44643134	0	2.944	N.D.	#
11) B	alpha-Chl...	5.568	0.000	50304780	0	3.411	N.D.	#
13) MA	Dieldrin	5.862	0.000	1534726	0	0.108	N.D.	#
14) MA	Endrin	0.000	6.765	0	273265	N.D.	0.123	#
24)	Chlordane-2	4.933	0.000	19439680	0	44.765	N.D.	#
25)	Chlordane-3	5.516f	0.000	44643134	0	34.765	N.D.	#
26)	Chlordane-4	5.568	0.000	50304780	0	47.624	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120519\
Data File : PL054778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 08:04
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 04:41:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

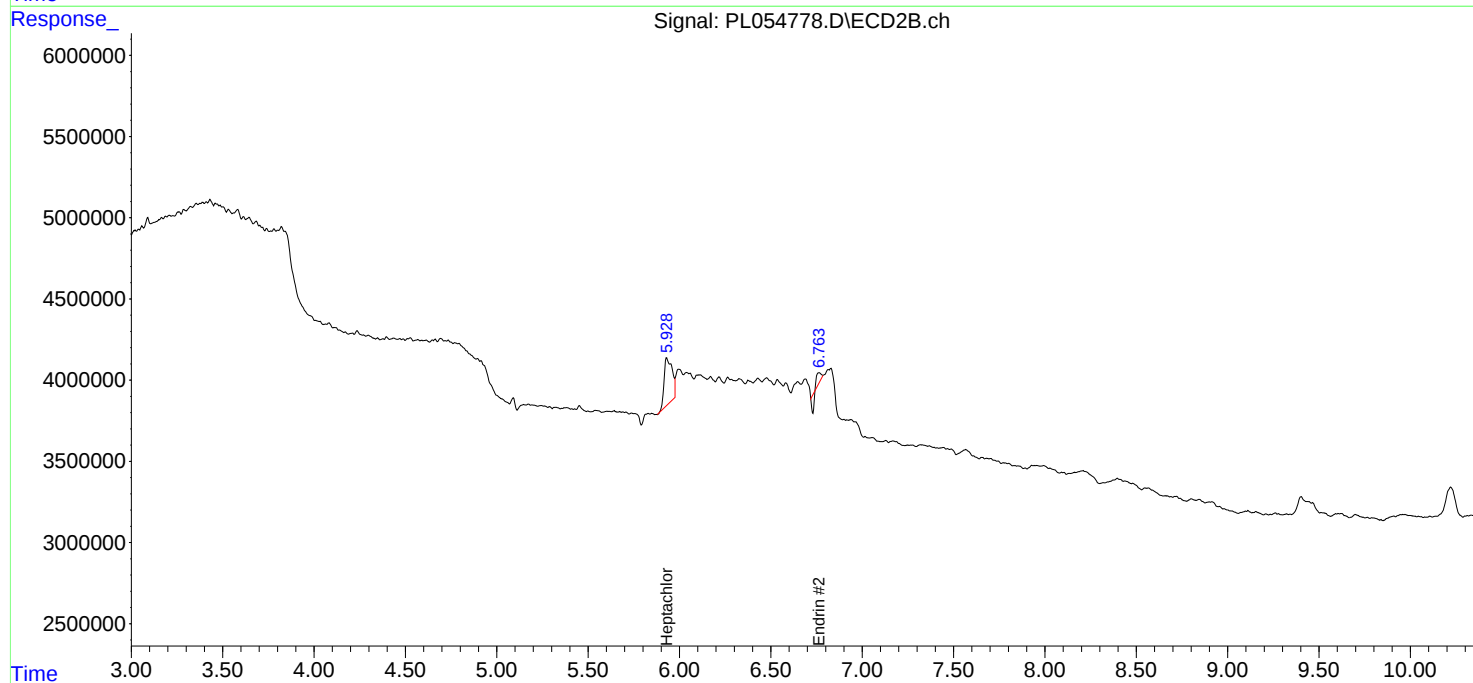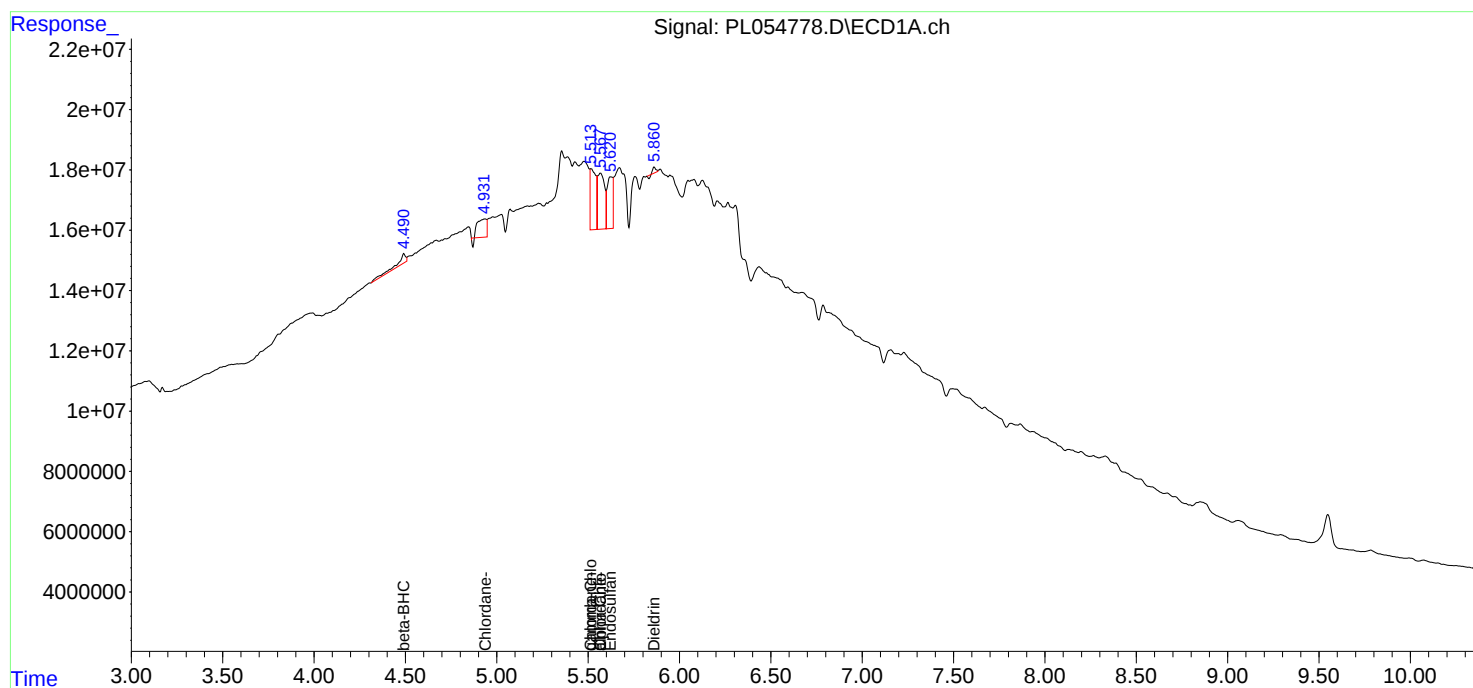


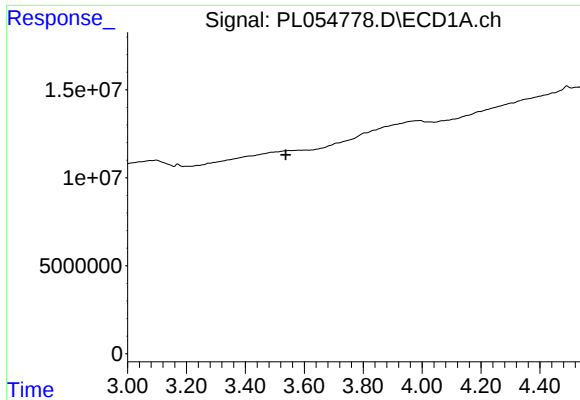

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

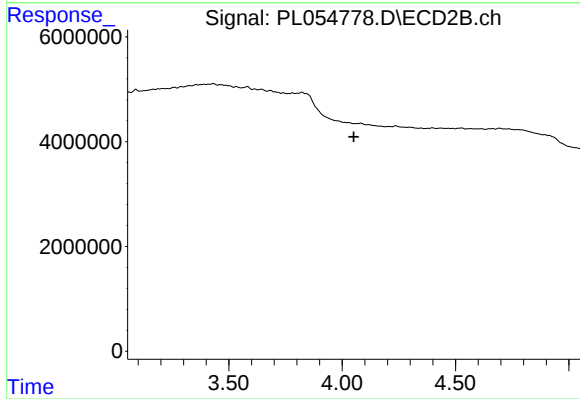


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.052 min
Response: 0
Conc: N.D.

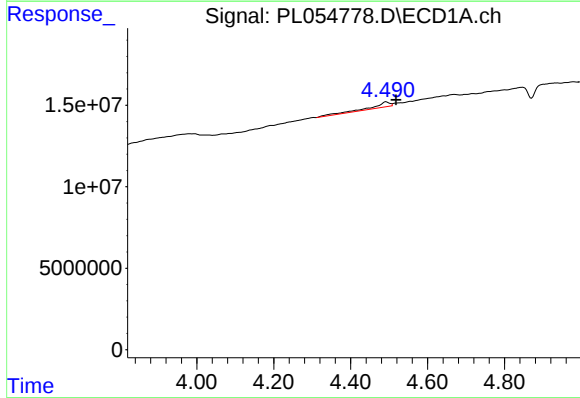


#6 beta-BHC

R.T.: 4.492 min
Delta R.T.: -0.026 min
Response: 10433559
Conc: 1.41 ng/ml

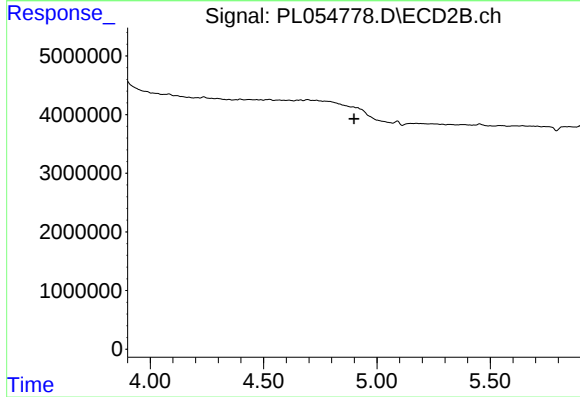

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.899 min
Response: 0
Conc: N.D.

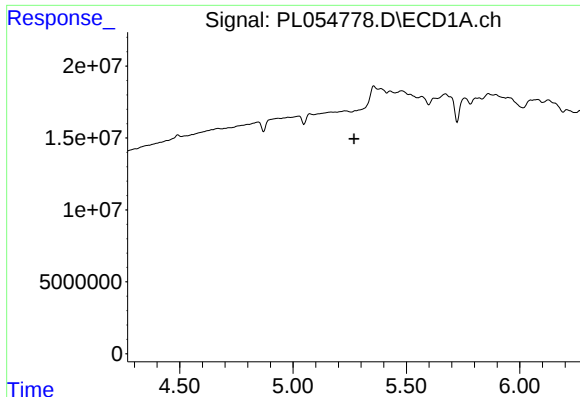

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

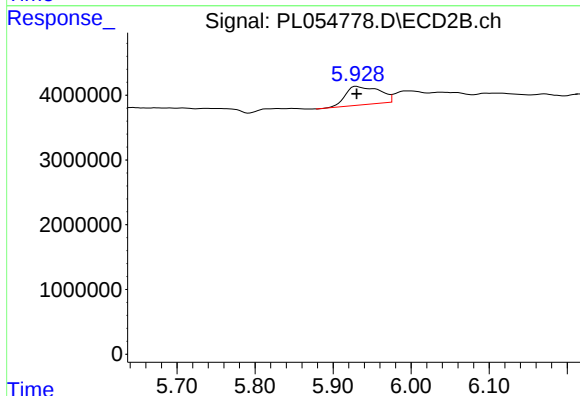


#8 Heptachlor epoxide

R.T.: 5.930 min
Delta R.T.: 0.000 min
Response: 8533718
Conc: 3.42 ng/ml

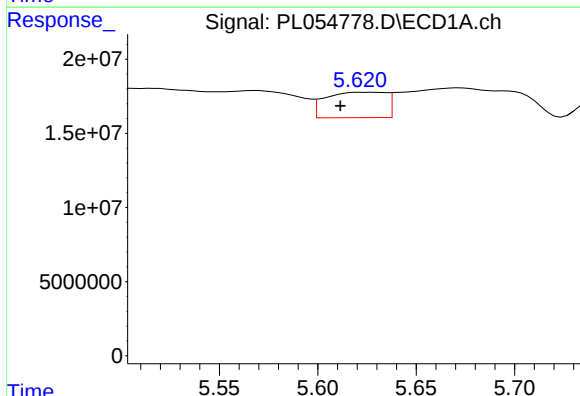


#9 Endosulfan I

R.T.: 5.622 min
Delta R.T.: 0.011 min
Response: 36711502
Conc: 2.69 ng/ml

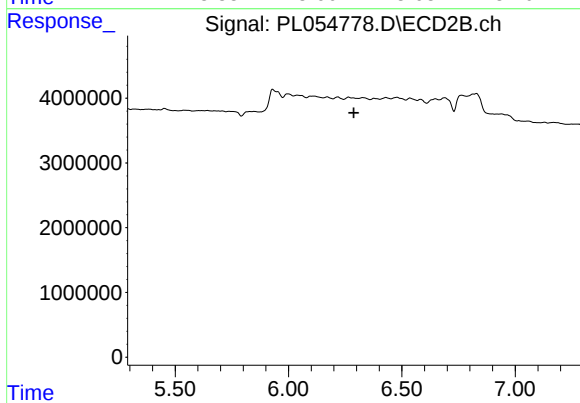

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.288 min
Response: 0
Conc: N.D.

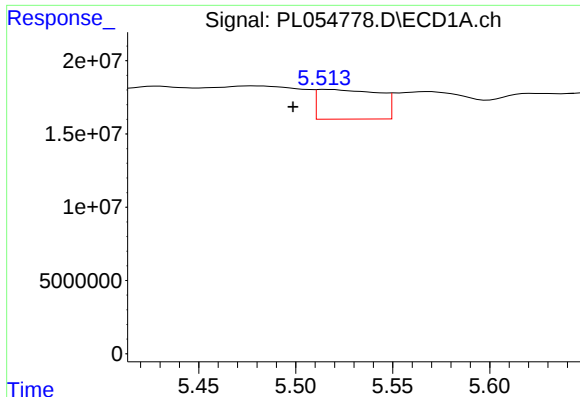

#10 gamma-Chlordane


R.T.: 5.516 min
Delta R.T.: 0.018 min
Response: 44643134
Conc: 2.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

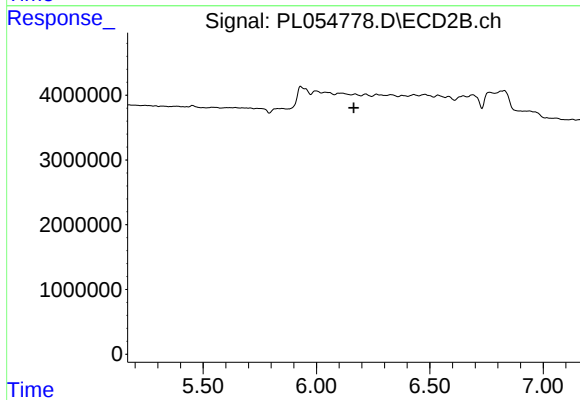


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

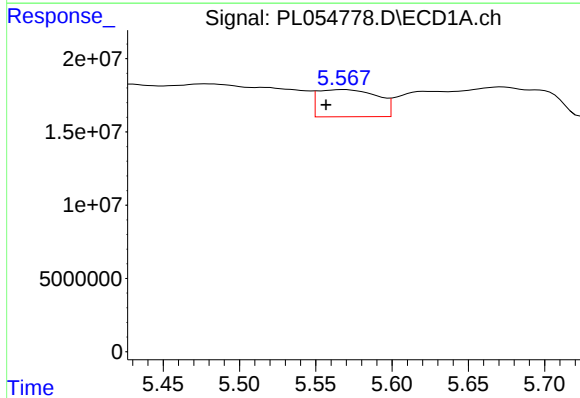


#11 alpha-Chlordane

R.T.: 5.568 min
Delta R.T.: 0.011 min
Response: 50304780
Conc: 3.41 ng/ml

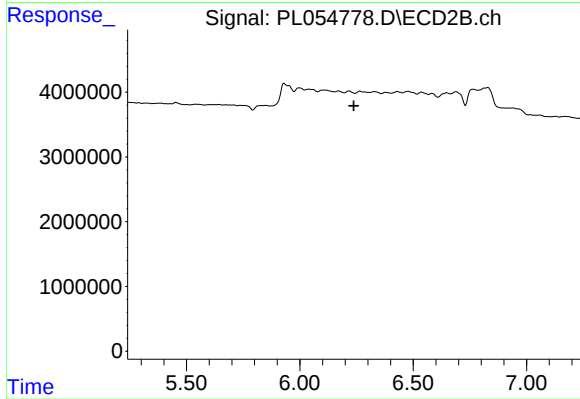

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

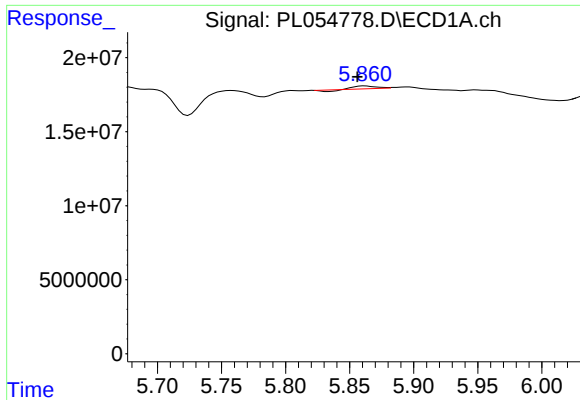

#13 Dieldrin


R.T.: 5.862 min
Delta R.T.: 0.006 min
Response: 1534726
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

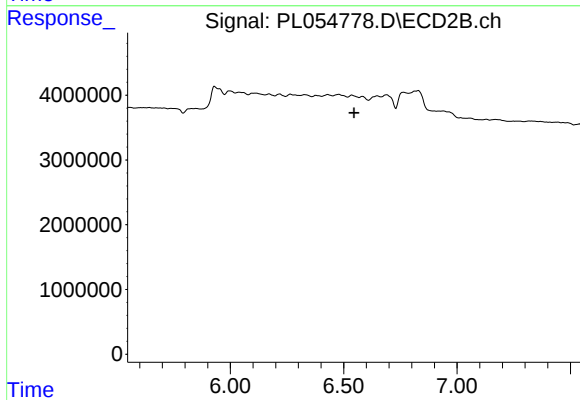


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.545 min
Response: 0
Conc: N.D.

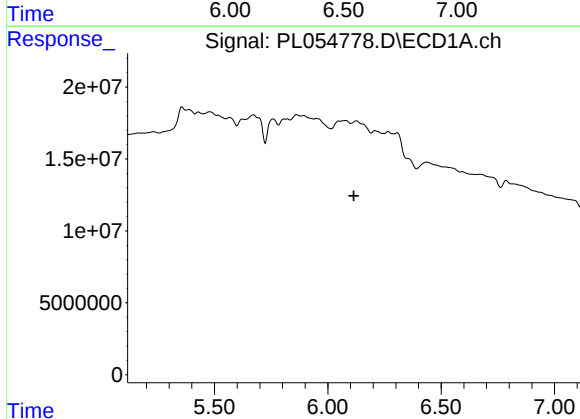


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

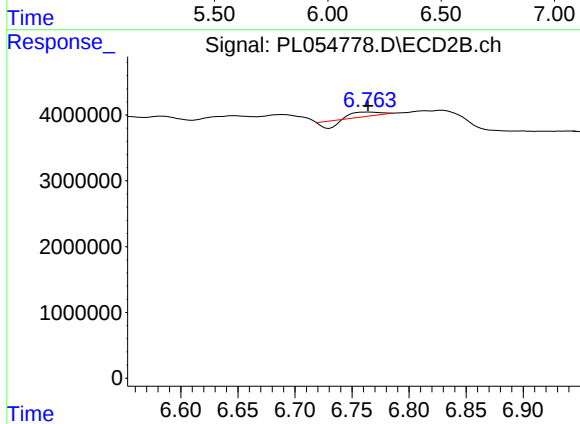

#14 Endrin


R.T.: 6.765 min
Delta R.T.: 0.001 min
Response: 273265
Conc: 0.12 ng/ml

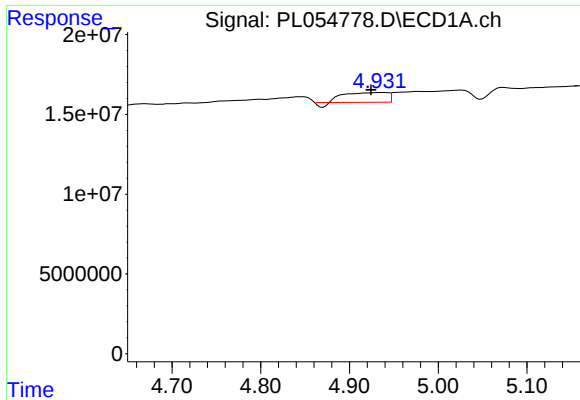

#24 Chlordane-2


R.T.: 4.933 min
Delta R.T.: 0.008 min
Response: 19439680
Conc: 44.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

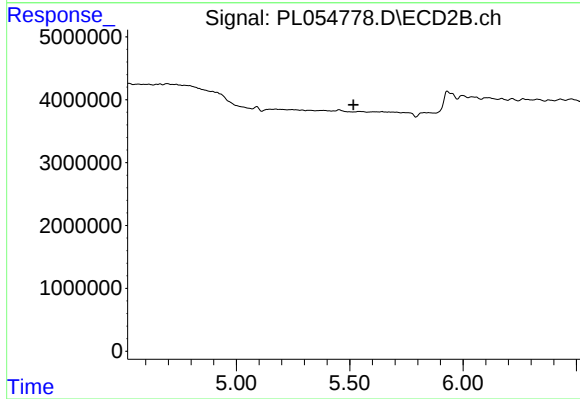


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.517 min
Response: 0
Conc: N.D.

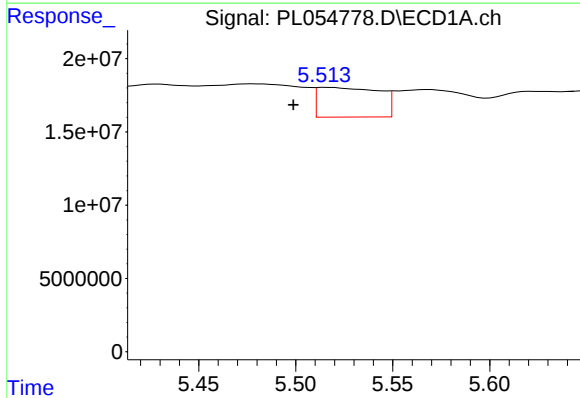


#25 Chlordane-3

R.T.: 5.516 min
Delta R.T.: 0.017 min
Response: 44643134
Conc: 34.77 ng/ml

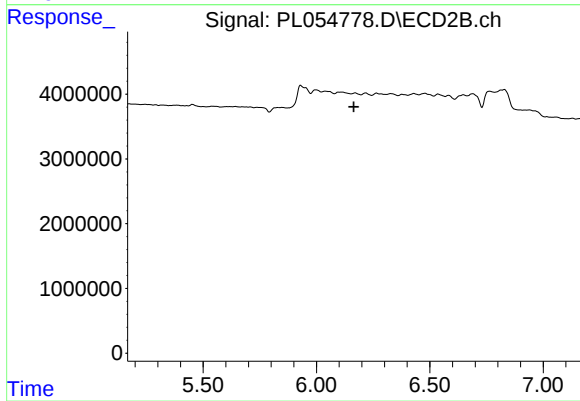

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

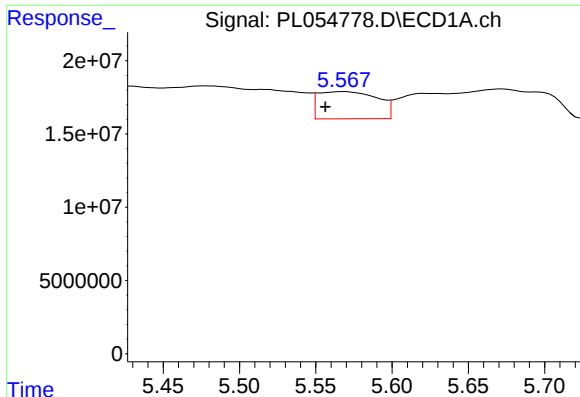

#26 Chlordane-4


R.T.: 5.568 min
Delta R.T.: 0.012 min
Response: 50304780
Conc: 47.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

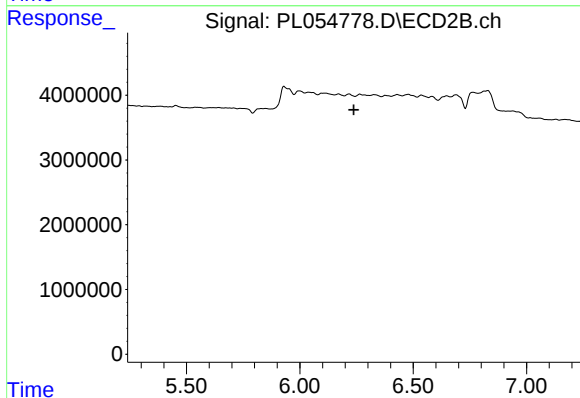


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

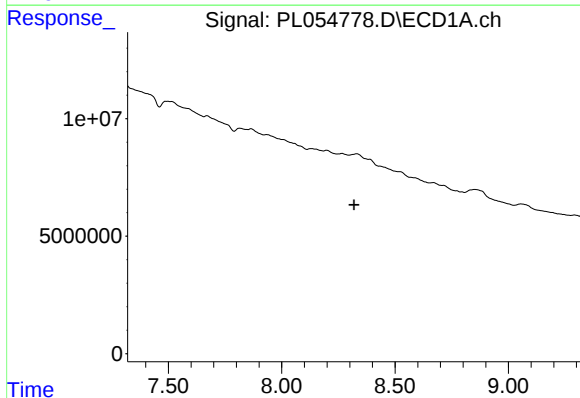

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.320 min
Response: 0
Conc: N.D.

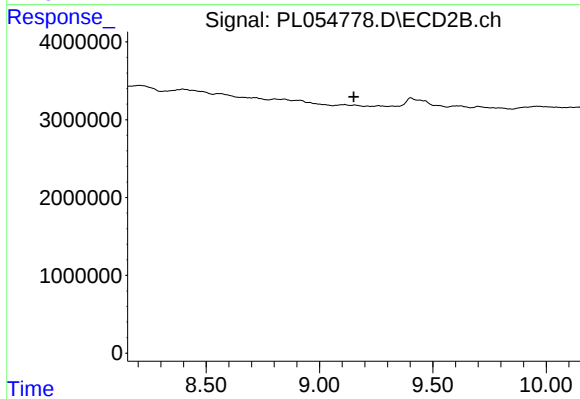

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.152 min
Response: 0
Conc: N.D.