

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\pl120522\
 Data File : PL079574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2022 15:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:25:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	2.567	47785538	56694129	21.153	20.828
28)	SA Decachlor...	8.769	7.634	48932784	41845449	25.196	17.812 #
Target Compounds							
4)	MA Heptachlor	0.000	3.676f	0	496574	N.D.	0.129 #
5)	MB Aldrin	0.000	3.992f	0	526377	N.D.	0.142 #
6)	B beta-BHC	0.000	3.676	0	496574	N.D.	0.328 #
8)	B Heptachlo...	0.000	4.458	0	494758	N.D.	0.147 #
11)	B alpha-Chl...	0.000	4.774	0	31414663	N.D.	9.380 #
13)	MA Dieldrin	0.000	5.084	0	1043171	N.D.	0.309 #
14)	MA Endrin	0.000	5.390f	0	1044381	N.D.	0.345 #
23)	Chlordane-1	0.000	3.536	0	197017	N.D.	1.852 #
24)	Chlordane-2	0.000	4.087	0	1620575	N.D.	13.841 #
26)	Chlordane-4	0.000	4.774	0	31414663	N.D.	86.694 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\p1120522\
Data File : PL079574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2022 15:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:25:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

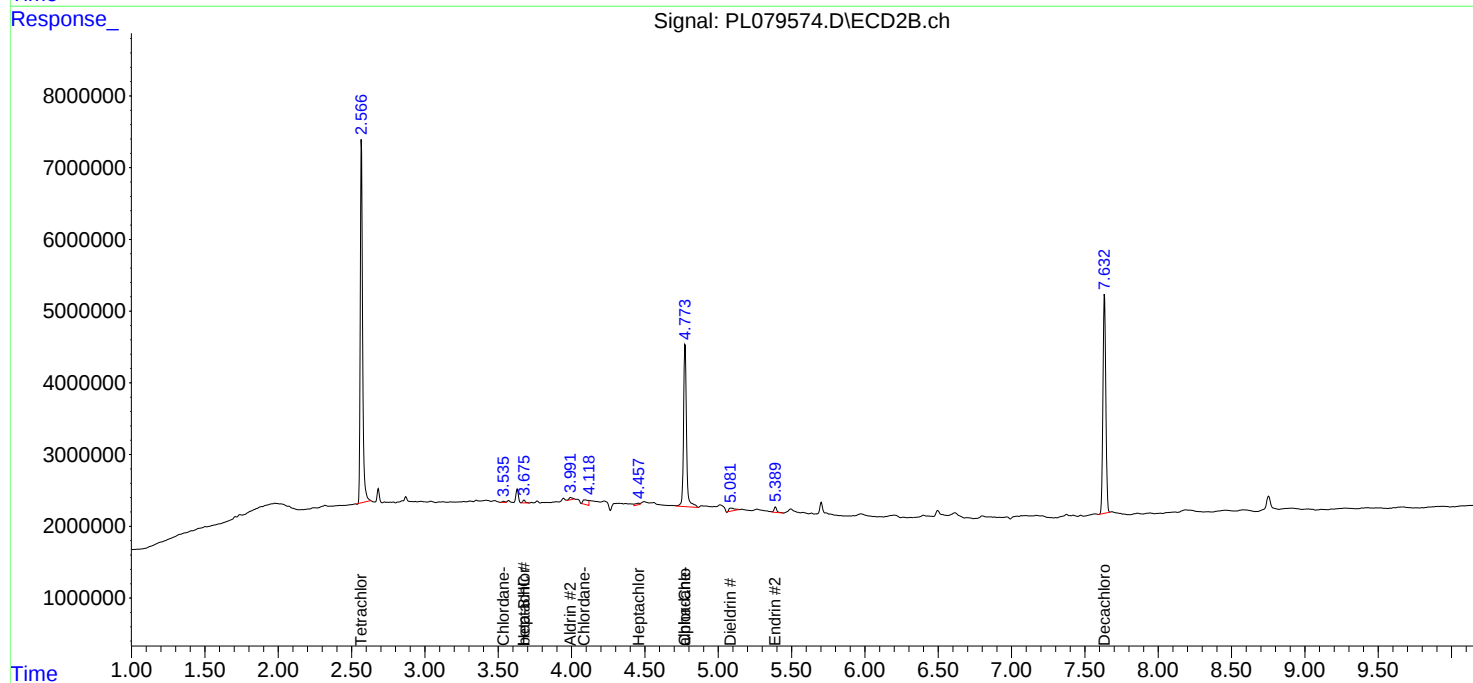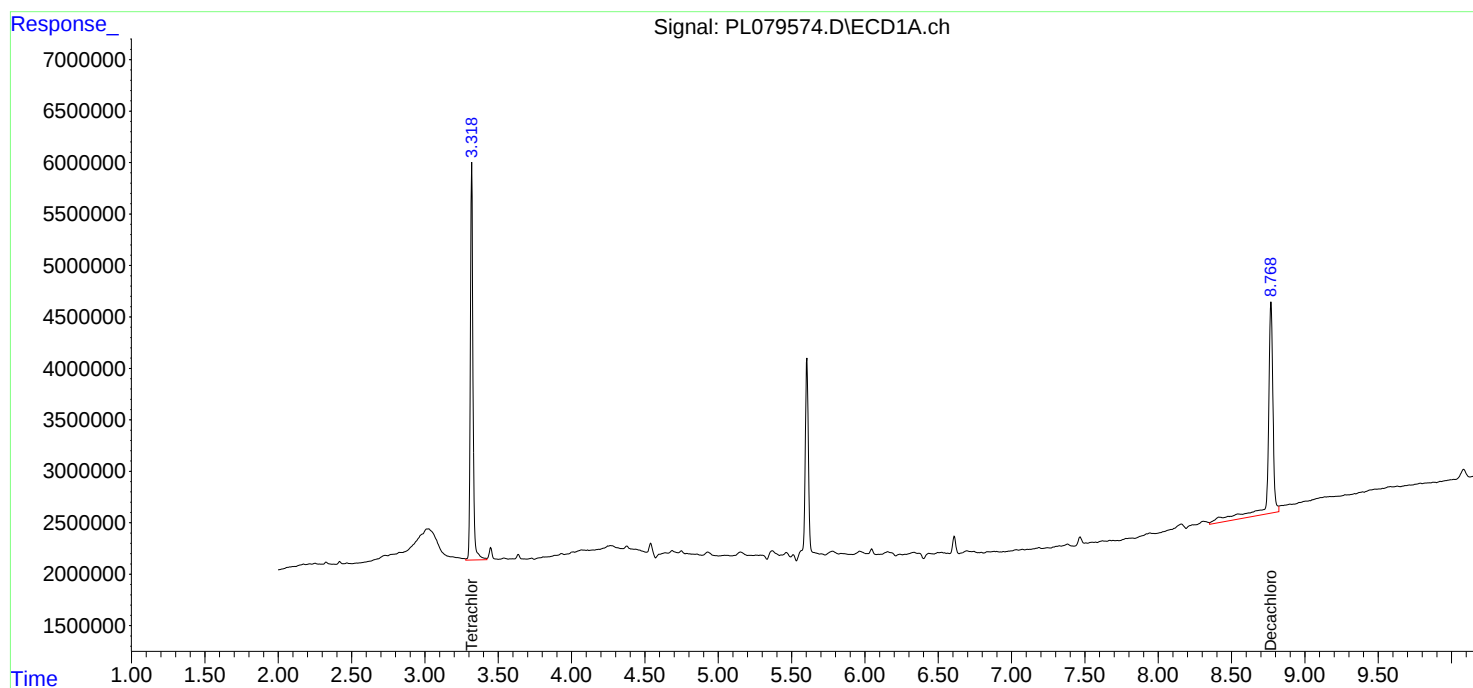


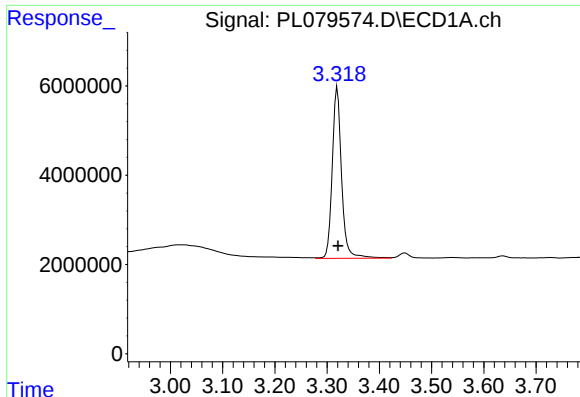

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.002 min
Response: 47785538
Conc: 21.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

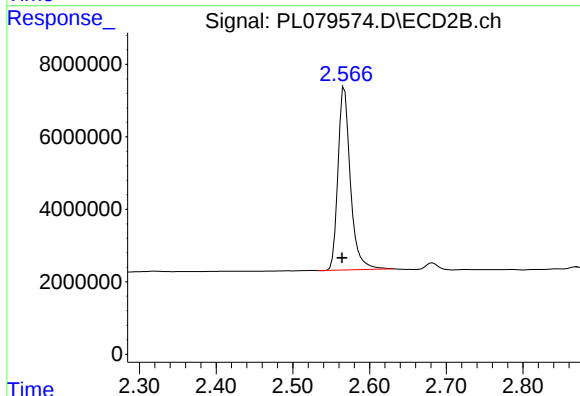


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: 0.003 min
Response: 56694129
Conc: 20.83 ng/ml

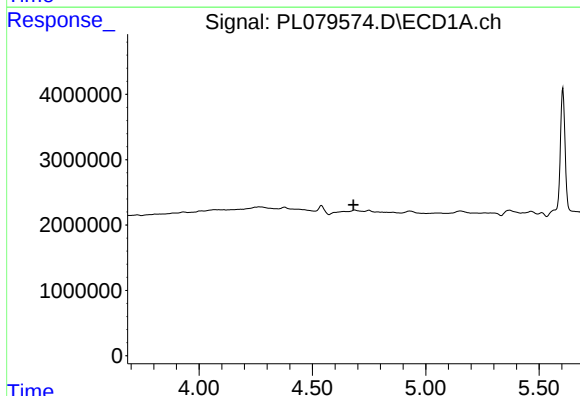


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.681 min
Response: 0
Conc: N.D.

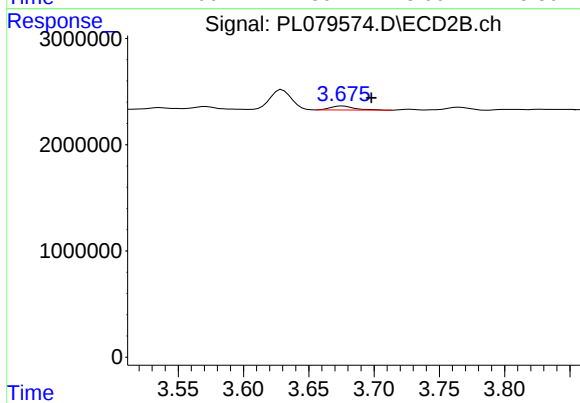

#4 Heptachlor


R.T.: 3.676 min
Delta R.T.: -0.022 min
Response: 496574
Conc: 0.13 ng/ml

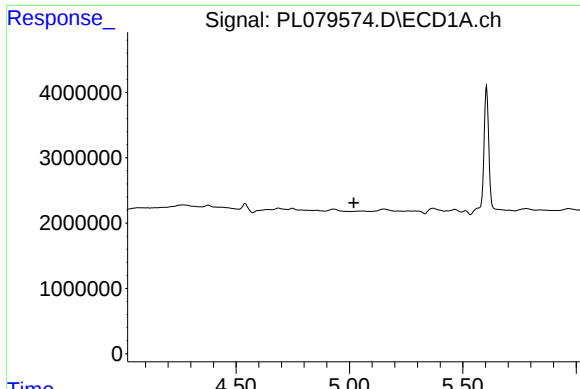

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

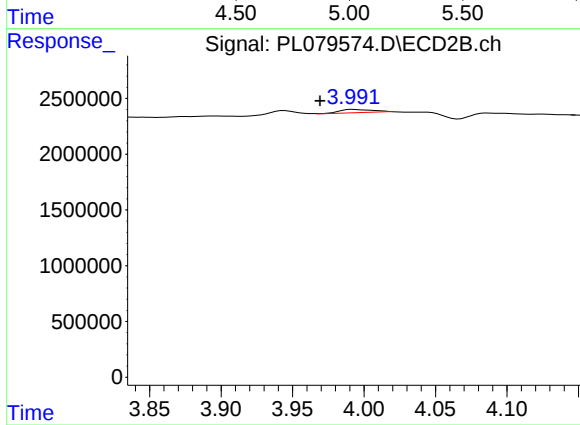


#5 Aldrin

R.T.: 3.992 min
Delta R.T.: 0.023 min
Response: 526377
Conc: 0.14 ng/ml

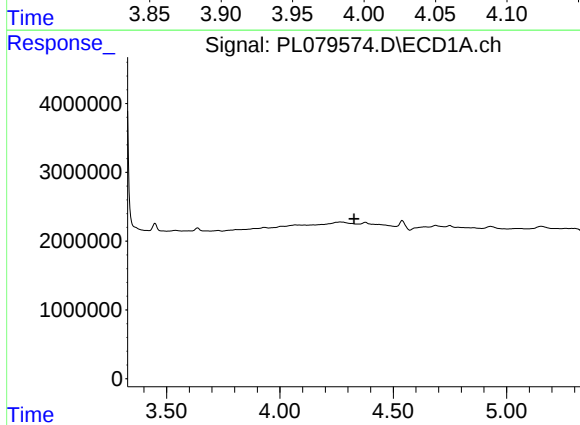


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.327 min
Response: 0
Conc: N.D.

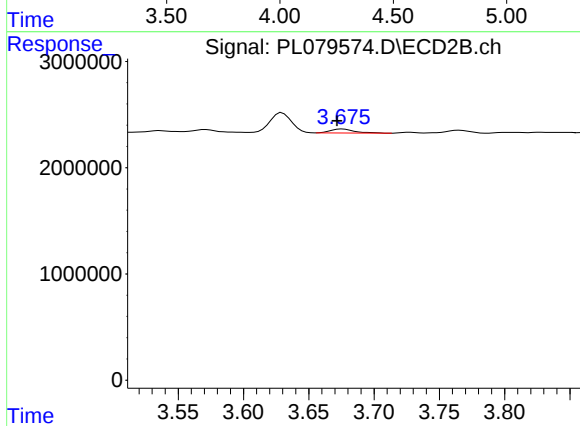

#6 beta-BHC


R.T.: 3.676 min
Delta R.T.: 0.004 min
Response: 496574
Conc: 0.33 ng/ml

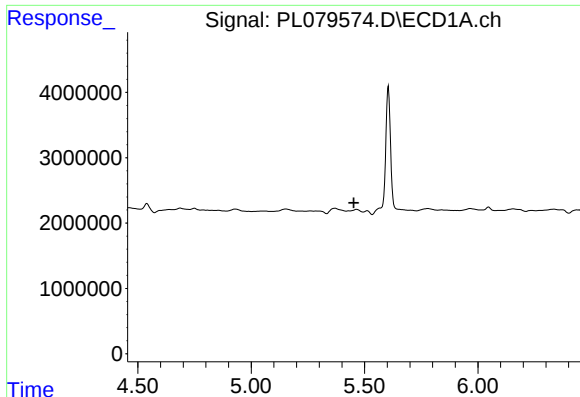

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

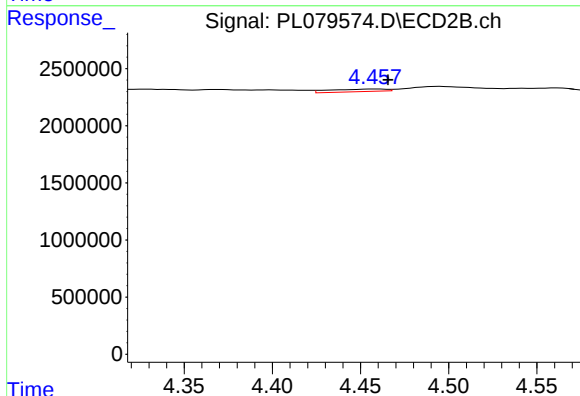


#8 Heptachlor epoxide

R.T.: 4.458 min
Delta R.T.: -0.007 min
Response: 494758
Conc: 0.15 ng/ml

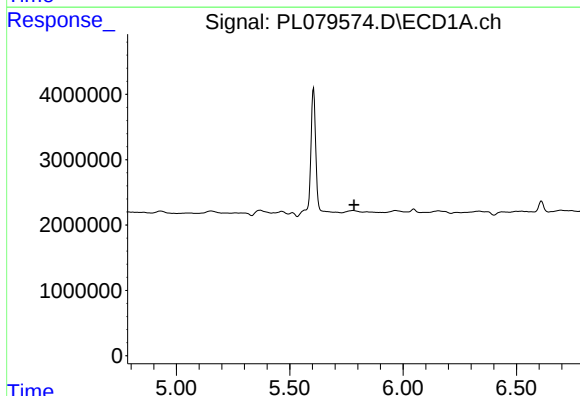


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.784 min
Response: 0
Conc: N.D.

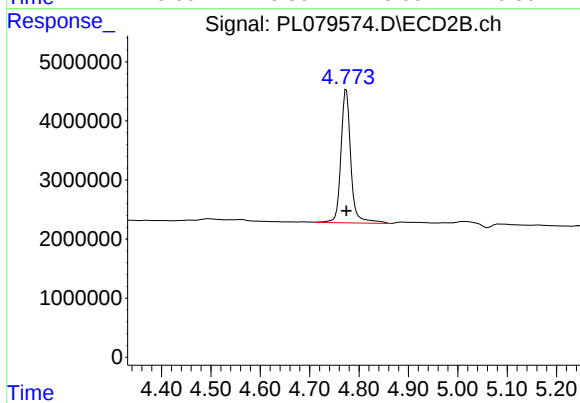

#11 alpha-Chlordane


R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 31414663
Conc: 9.38 ng/ml

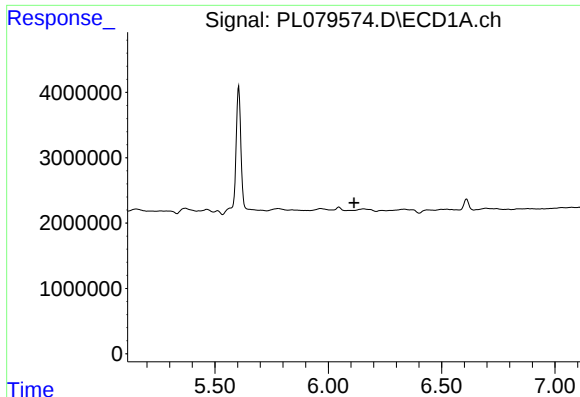

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

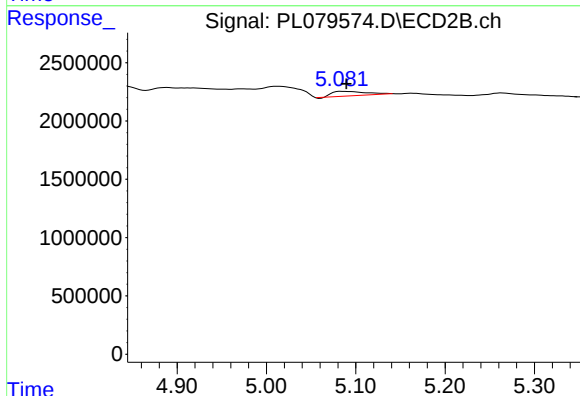


#13 Dieldrin

R.T.: 5.084 min
Delta R.T.: -0.005 min
Response: 1043171
Conc: 0.31 ng/ml

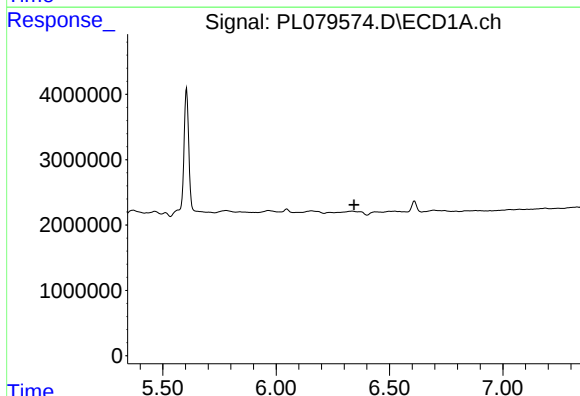


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

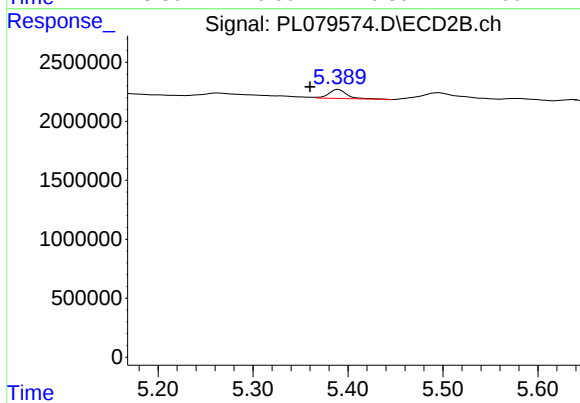

#14 Endrin


R.T.: 5.390 min
Delta R.T.: 0.030 min
Response: 1044381
Conc: 0.35 ng/ml

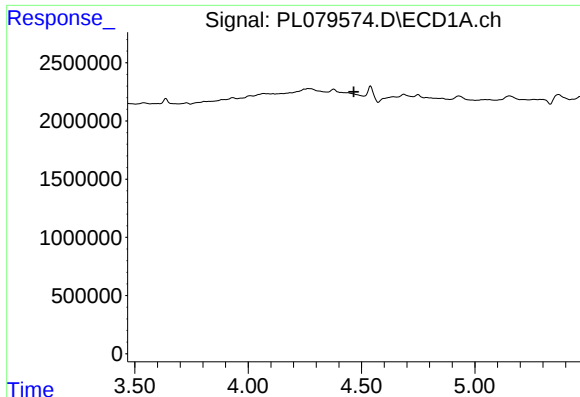

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

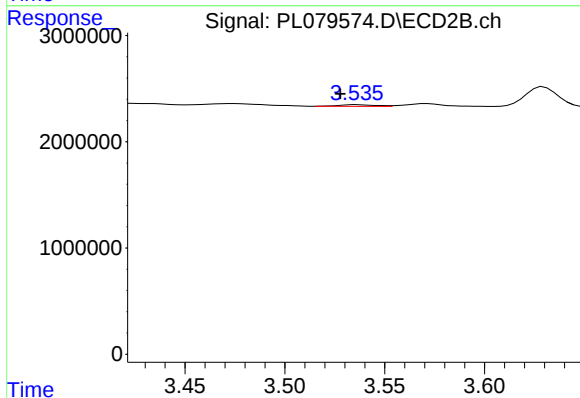


#23 Chlordane-1

R.T.: 3.536 min
Delta R.T.: 0.008 min
Response: 197017
Conc: 1.85 ng/ml

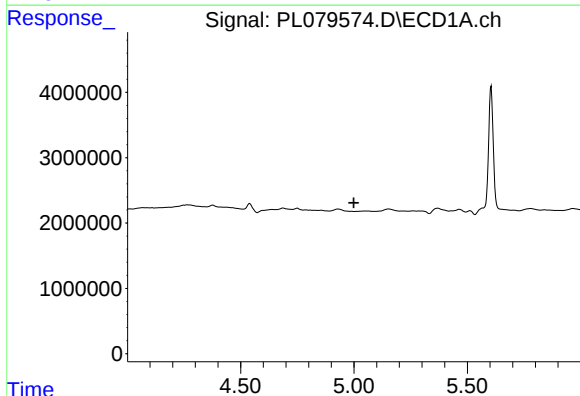


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.999 min
Response: 0
Conc: N.D.

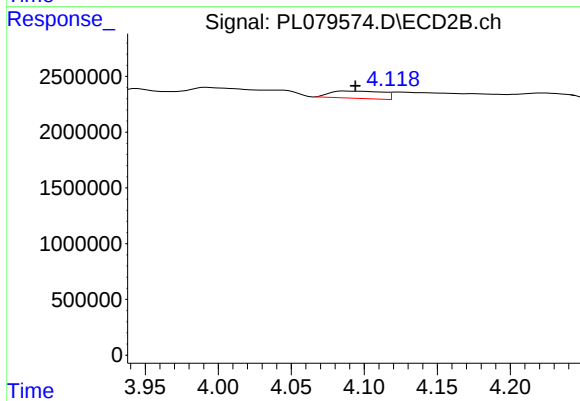

#24 Chlordane-2


R.T.: 4.087 min
Delta R.T.: -0.007 min
Response: 1620575
Conc: 13.84 ng/ml

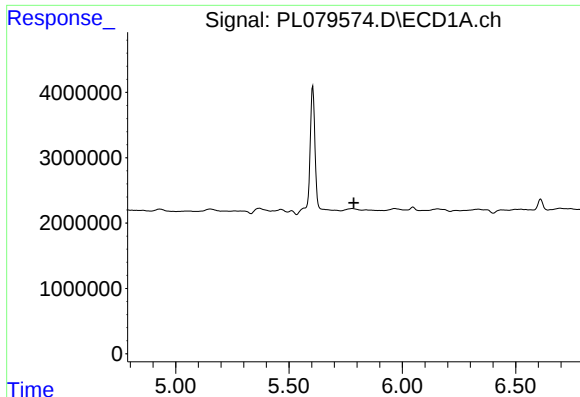

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

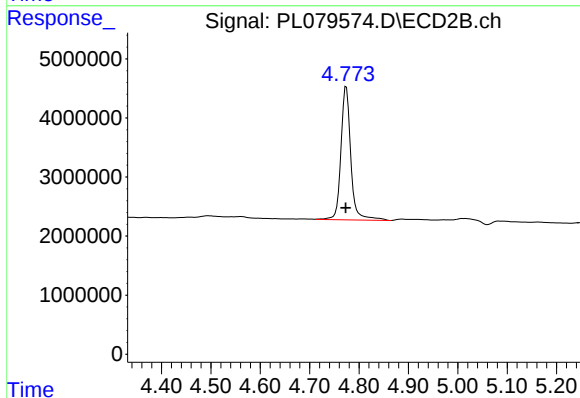


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 31414663
Conc: 86.69 ng/ml

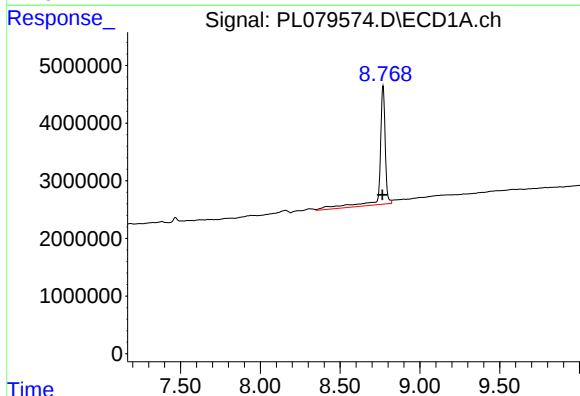

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: 0.004 min
Response: 48932784
Conc: 25.20 ng/ml

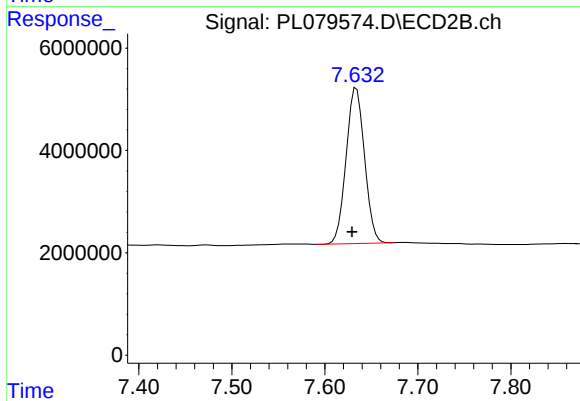

#28 Decachlorobiphenyl

R.T.: 7.634 min
Delta R.T.: 0.005 min
Response: 41845449
Conc: 17.81 ng/ml