

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\pl120522\
 Data File : PL079577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2022 16:38
 Operator : AR\AJ
 Sample : N5863-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:26:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.567	22663875	27741669	10.033	10.192
28)	SA Decachlor...	8.765	7.632	27013368	26689077	13.909	11.361
Target Compounds							
5)	MB Aldrin	0.000	3.949f	0	222848	N.D.	0.060 #
10)	B gamma-Chl...	0.000	4.741f	0	2309406	N.D.	0.682 #
11)	B alpha-Chl...	5.787	4.772	2168998	1489239	0.753	0.445 #
12)	B 4,4'-DDE	0.000	4.972	0	242765	N.D.	0.079 #
14)	MA Endrin	0.000	5.388f	0	332588	N.D.	0.110 #
15)	B Endosulfa...	0.000	5.659	0	470566	N.D.	0.168 #
17)	MA 4,4'-DDT	0.000	5.765	0	434770	N.D.	0.166 #
23)	Chlordane-1	0.000	3.533	0	319782	N.D.	3.007 #
25)	Chlordane-3	0.000	4.741f	0	2309406	N.D.	6.908 #
26)	Chlordane-4	5.787	4.772	2168998	1489239	4.263	4.110
27)	Chlordane-5	0.000	5.460f	0	58050	N.D.	0.646 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\p1120522\
Data File : PL079577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2022 16:38
Operator : AR\AJ
Sample : N5863-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:26:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

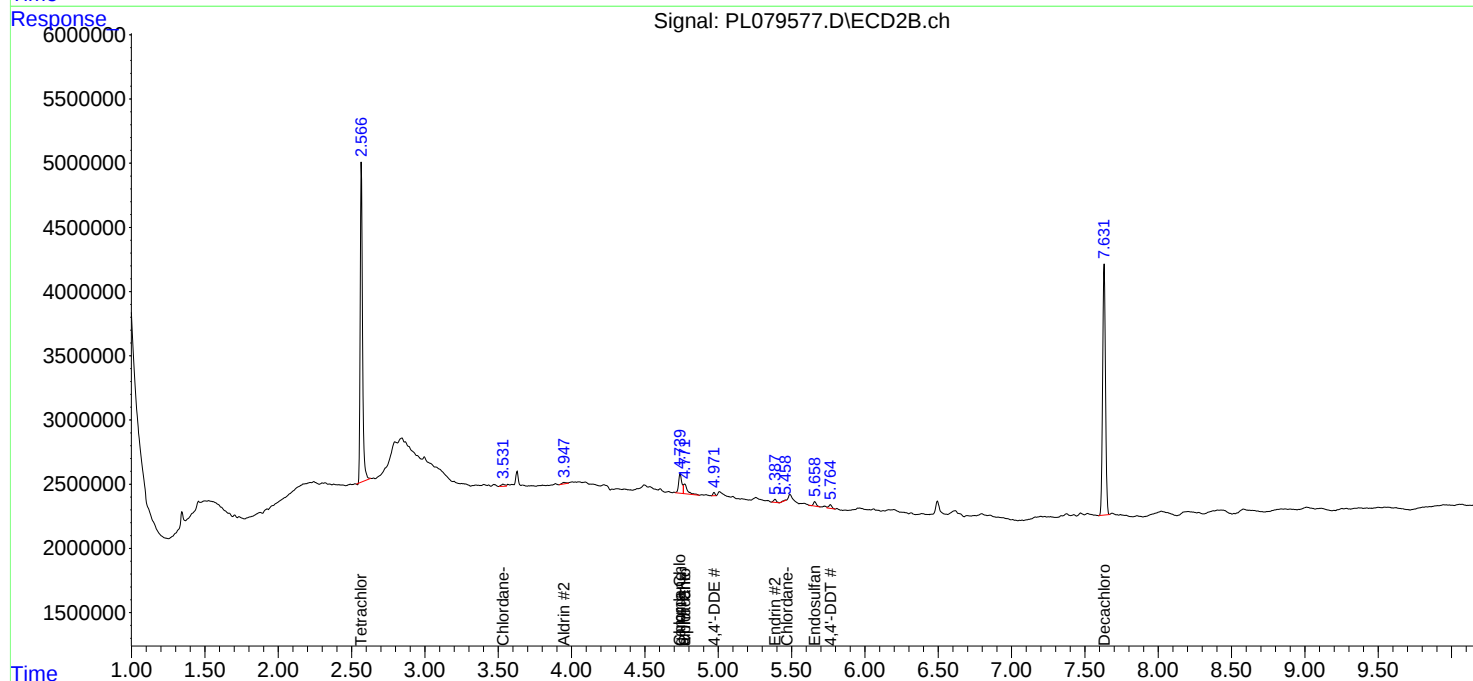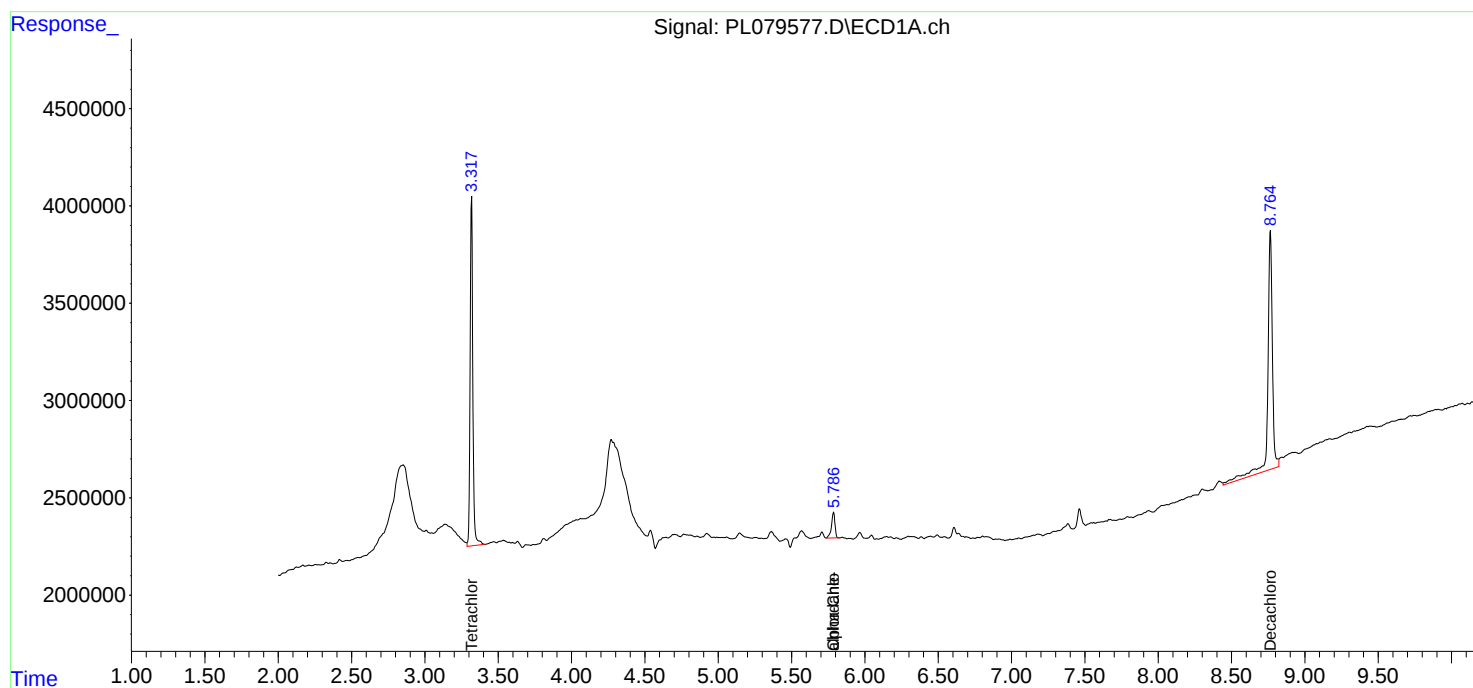


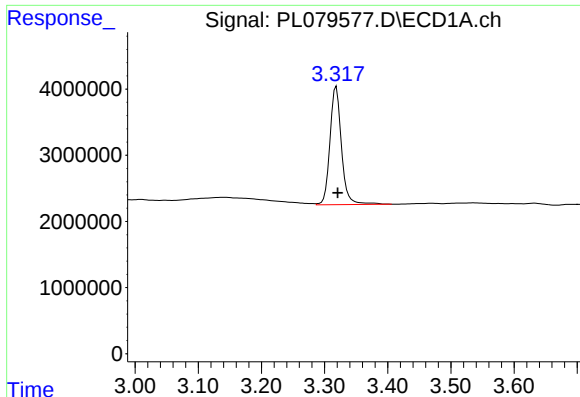

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.003 min
Response: 22663875
Conc: 10.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

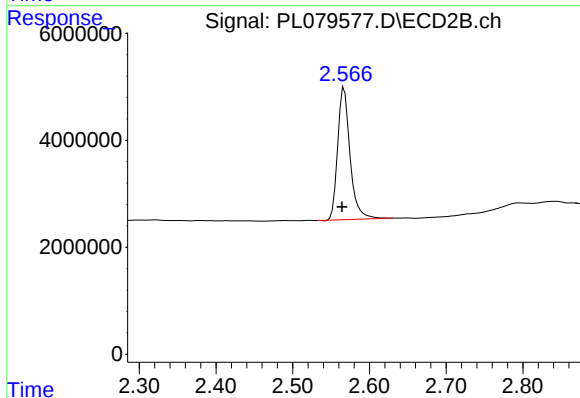


#1 Tetrachloro-m-xylene

R.T.: 2.567 min
Delta R.T.: 0.003 min
Response: 27741669
Conc: 10.19 ng/ml

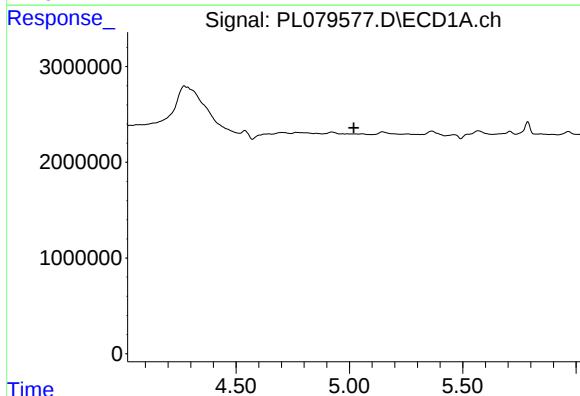


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

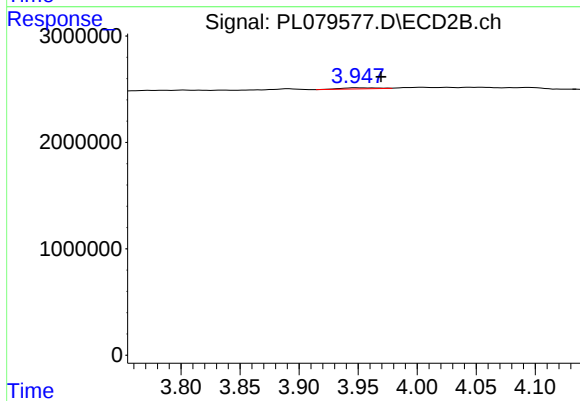

#5 Aldrin


R.T.: 3.949 min
Delta R.T.: -0.021 min
Response: 222848
Conc: 0.06 ng/ml

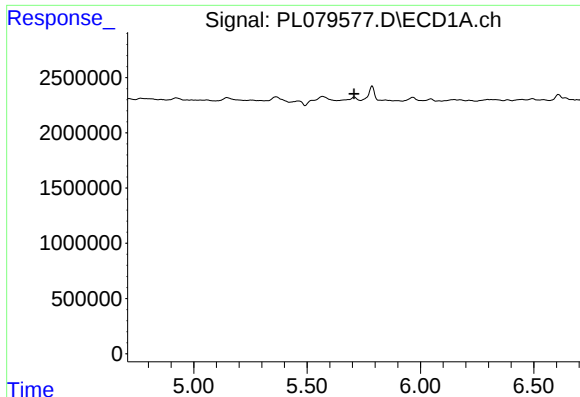

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

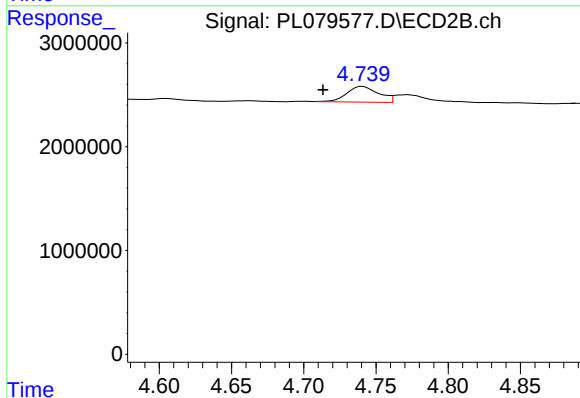


#10 gamma-Chlordane

R.T.: 4.741 min
Delta R.T.: 0.028 min
Response: 2309406
Conc: 0.68 ng/ml

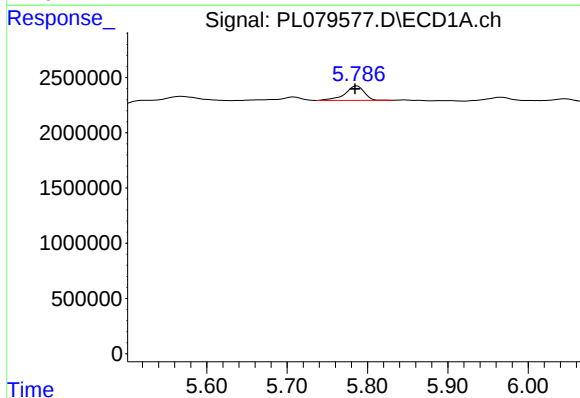


#11 alpha-Chlordane

R.T.: 5.787 min
Delta R.T.: 0.002 min
Response: 2168998
Conc: 0.75 ng/ml

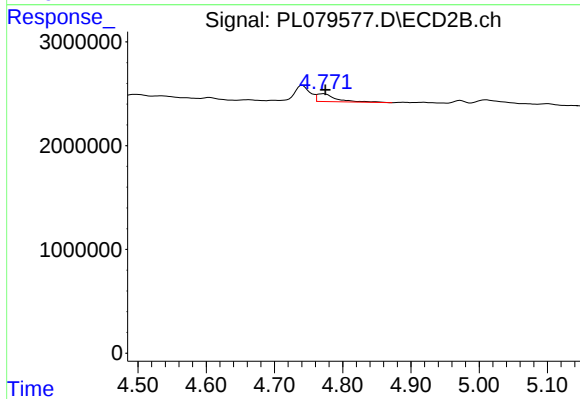

#11 alpha-Chlordane


R.T.: 4.772 min
Delta R.T.: -0.002 min
Response: 1489239
Conc: 0.44 ng/ml

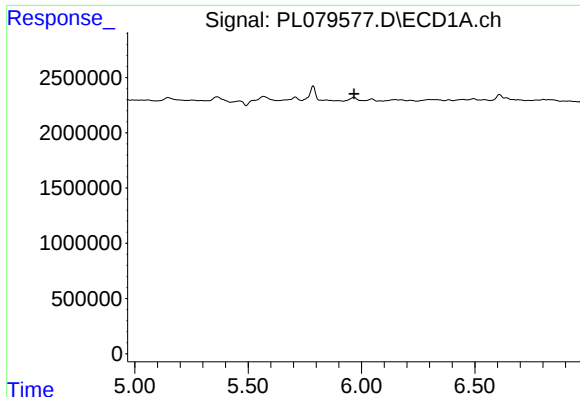

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.968 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

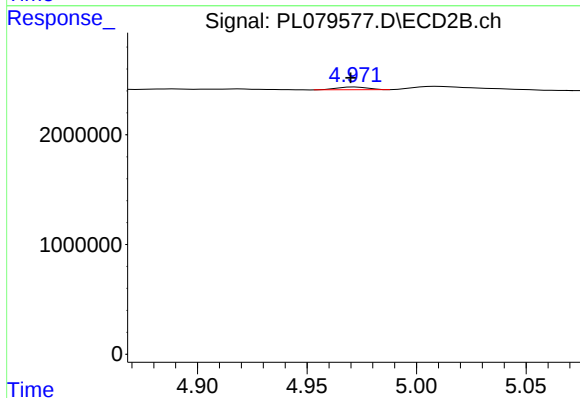


#12 4,4'-DDE

R.T.: 4.972 min
Delta R.T.: 0.002 min
Response: 242765
Conc: 0.08 ng/ml

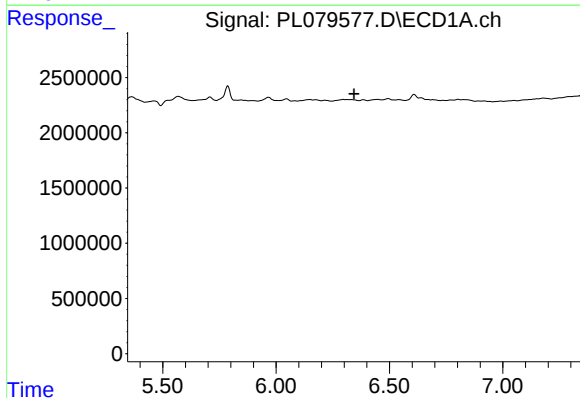


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

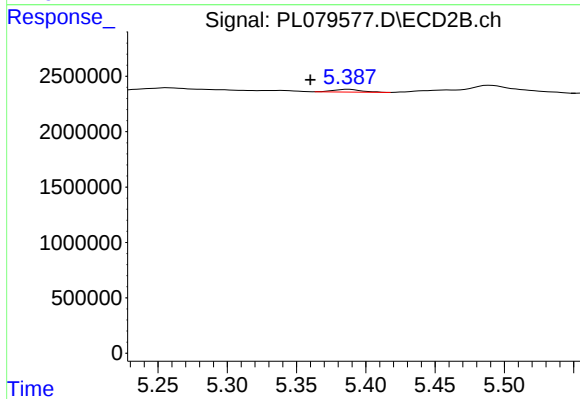

#14 Endrin


R.T.: 5.388 min
Delta R.T.: 0.028 min
Response: 332588
Conc: 0.11 ng/ml

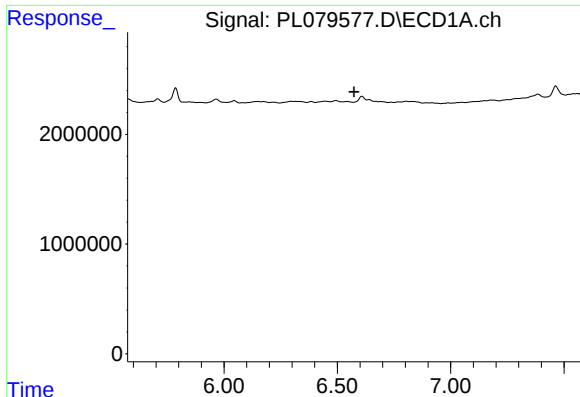

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

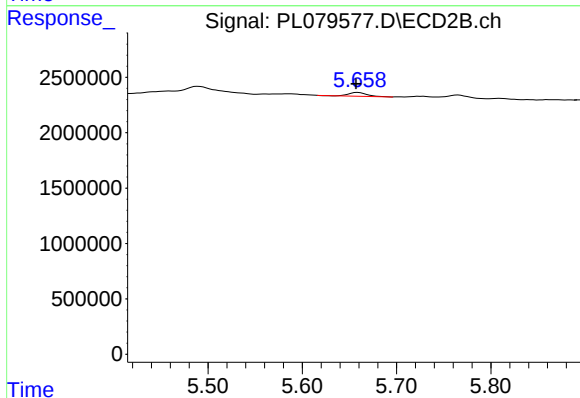


#15 Endosulfan II

R.T.: 5.659 min
Delta R.T.: 0.002 min
Response: 470566
Conc: 0.17 ng/ml

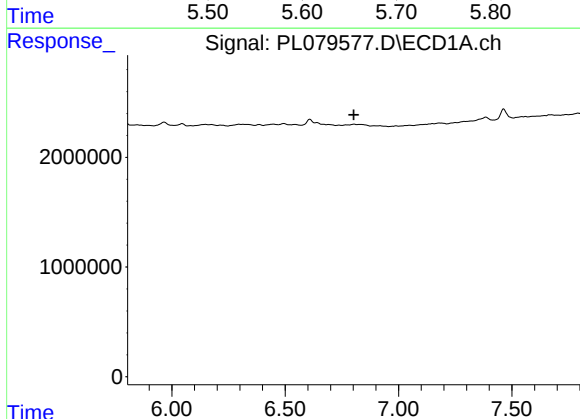


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.802 min
Response: 0
Conc: N.D.

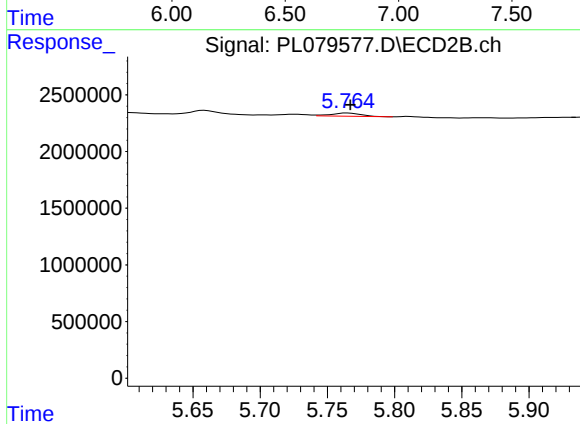

#17 4,4'-DDT


R.T.: 5.765 min
Delta R.T.: -0.002 min
Response: 434770
Conc: 0.17 ng/ml

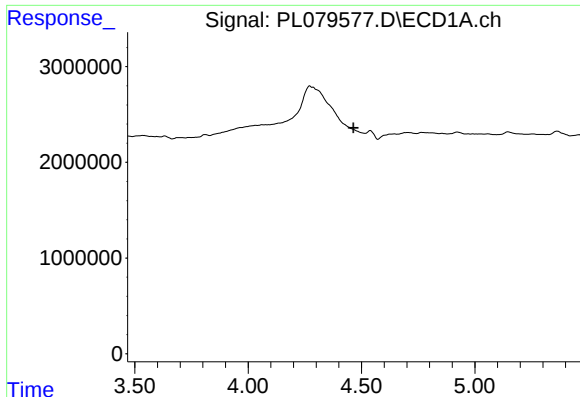

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

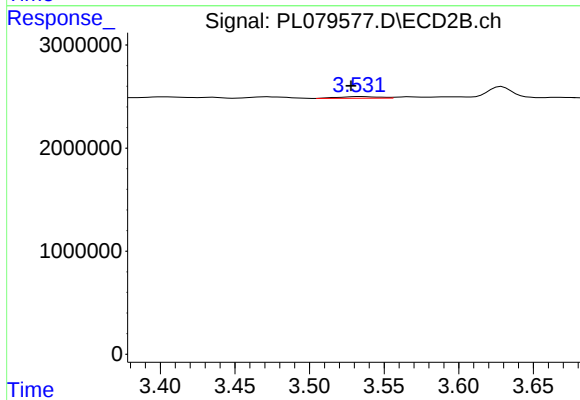


#23 Chlordane-1

R.T.: 3.533 min
Delta R.T.: 0.006 min
Response: 319782
Conc: 3.01 ng/ml

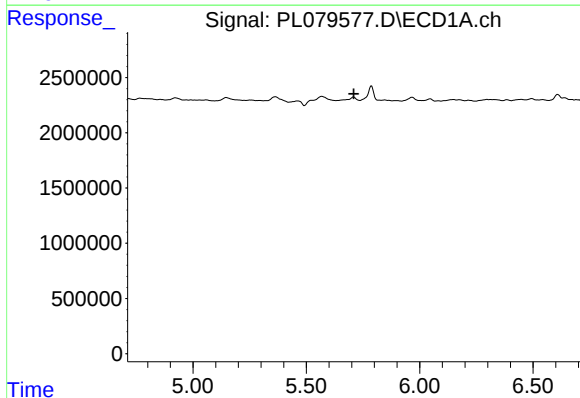


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.709 min
Response: 0
Conc: N.D.

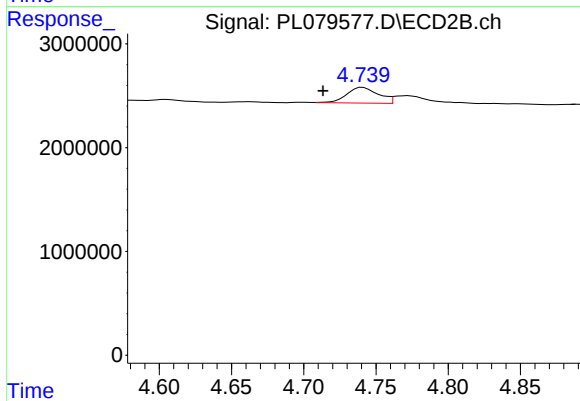

#25 Chlordane-3


R.T.: 4.741 min
Delta R.T.: 0.028 min
Response: 2309406
Conc: 6.91 ng/ml

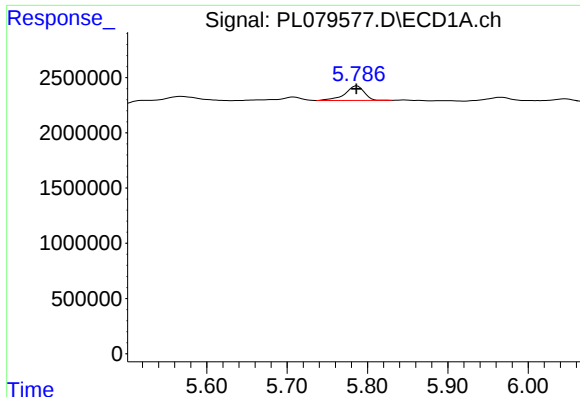

#26 Chlordane-4


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 2168998
Conc: 4.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

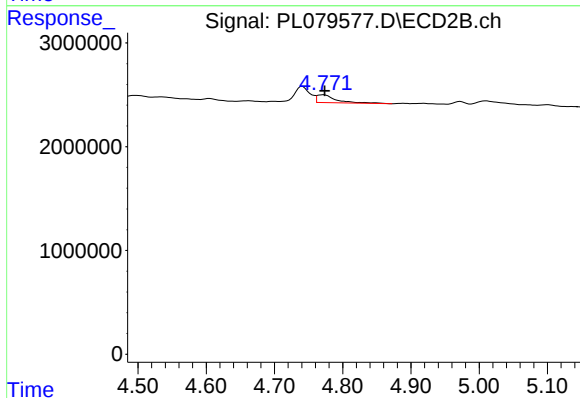


#26 Chlordane-4

R.T.: 4.772 min
Delta R.T.: -0.001 min
Response: 1489239
Conc: 4.11 ng/ml

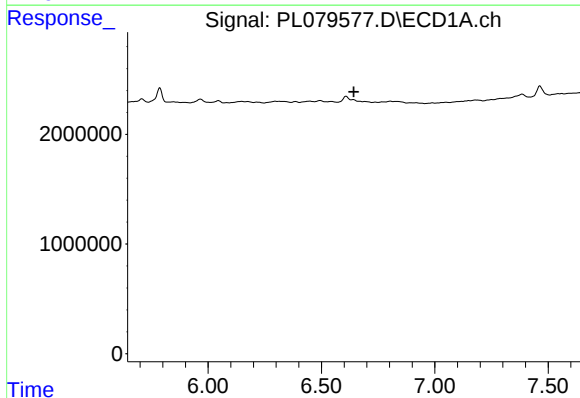


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

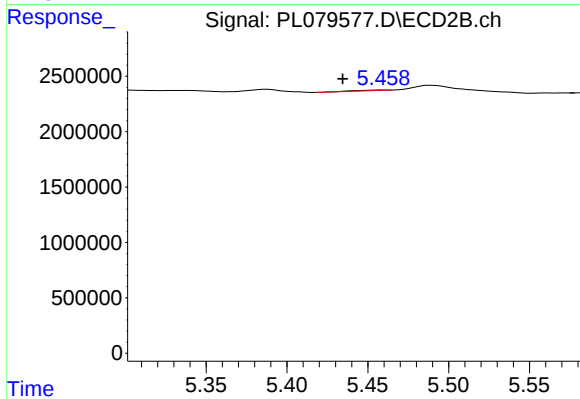

#27 Chlordane-5


R.T.: 5.460 min
Delta R.T.: 0.025 min
Response: 58050
Conc: 0.65 ng/ml

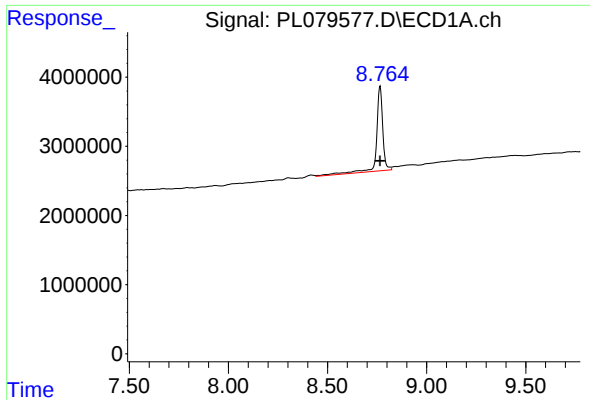

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 27013368
Conc: 13.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

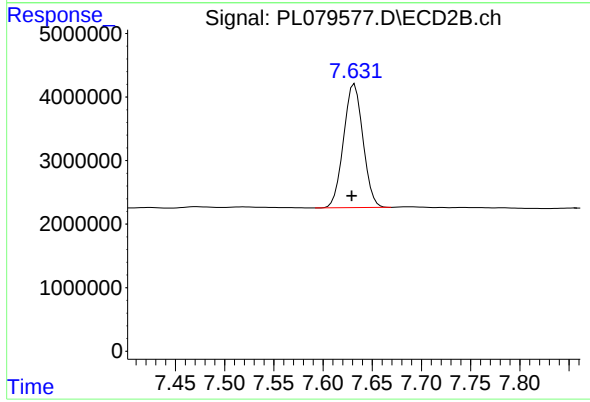

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: 0.003 min
Response: 26689077
Conc: 11.36 ng/ml