

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\pl120522\
 Data File : PL079579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2022 17:05
 Operator : AR\AJ
 Sample : N5868-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:27:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.566	21840987	25626662	9.668	9.415
28)	SA Decachlor...	8.765	7.632	17904944	20949192	9.219	8.917
Target Compounds							
4)	MA Heptachlor	4.699f	0.000	3841154	0	1.166	N.D. #
5)	MB Aldrin	0.000	3.949f	0	244244	N.D.	0.066 #
11)	B alpha-Chl...	0.000	4.761	0	2821550	N.D.	0.842 #
12)	B 4,4'-DDE	0.000	4.972	0	501157	N.D.	0.163 #
14)	MA Endrin	0.000	5.384f	0	516167	N.D.	0.171 #
17)	MA 4,4'-DDT	0.000	5.768	0	1875697	N.D.	0.718 #
23)	Chlordane-1	0.000	3.539	0	468905	N.D.	4.409 #
26)	Chlordane-4	0.000	4.761	0	2821550	N.D.	7.787 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\pl120522\
Data File : PL079579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2022 17:05
Operator : AR\AJ
Sample : N5868-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:27:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

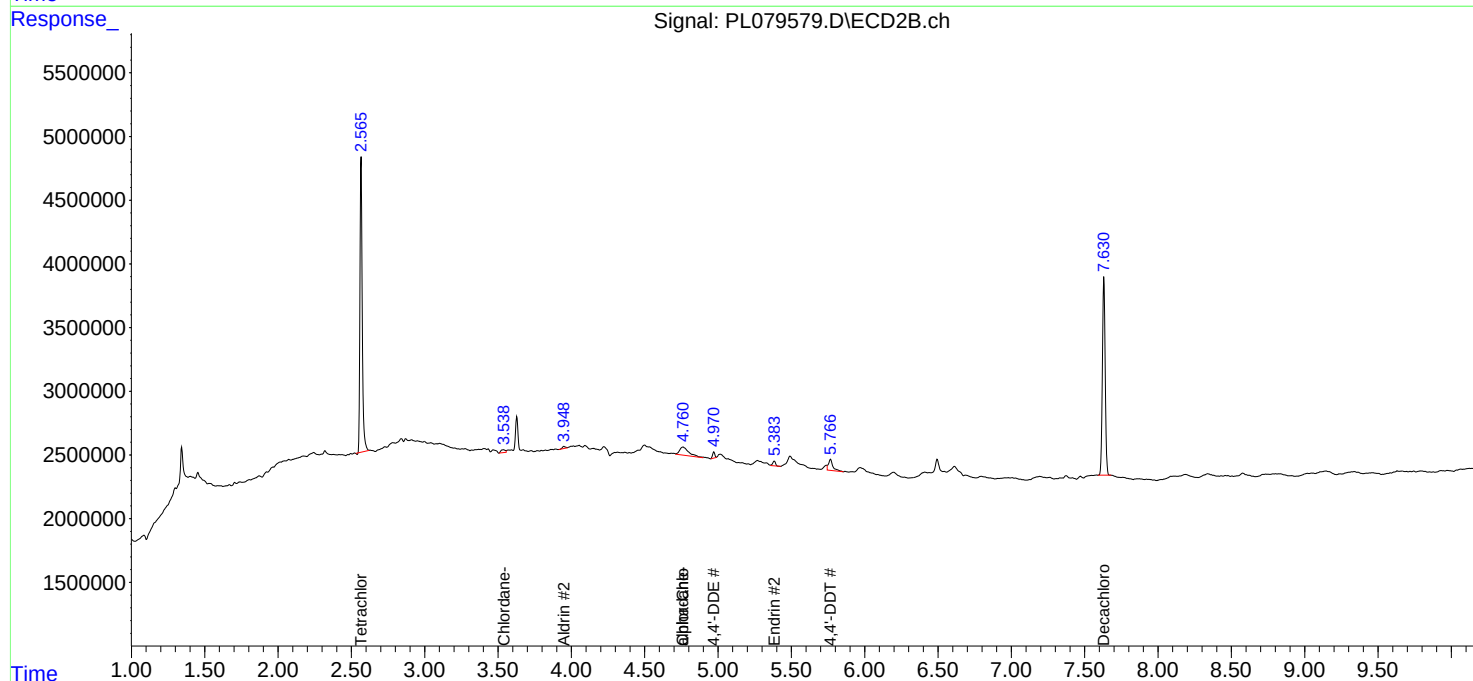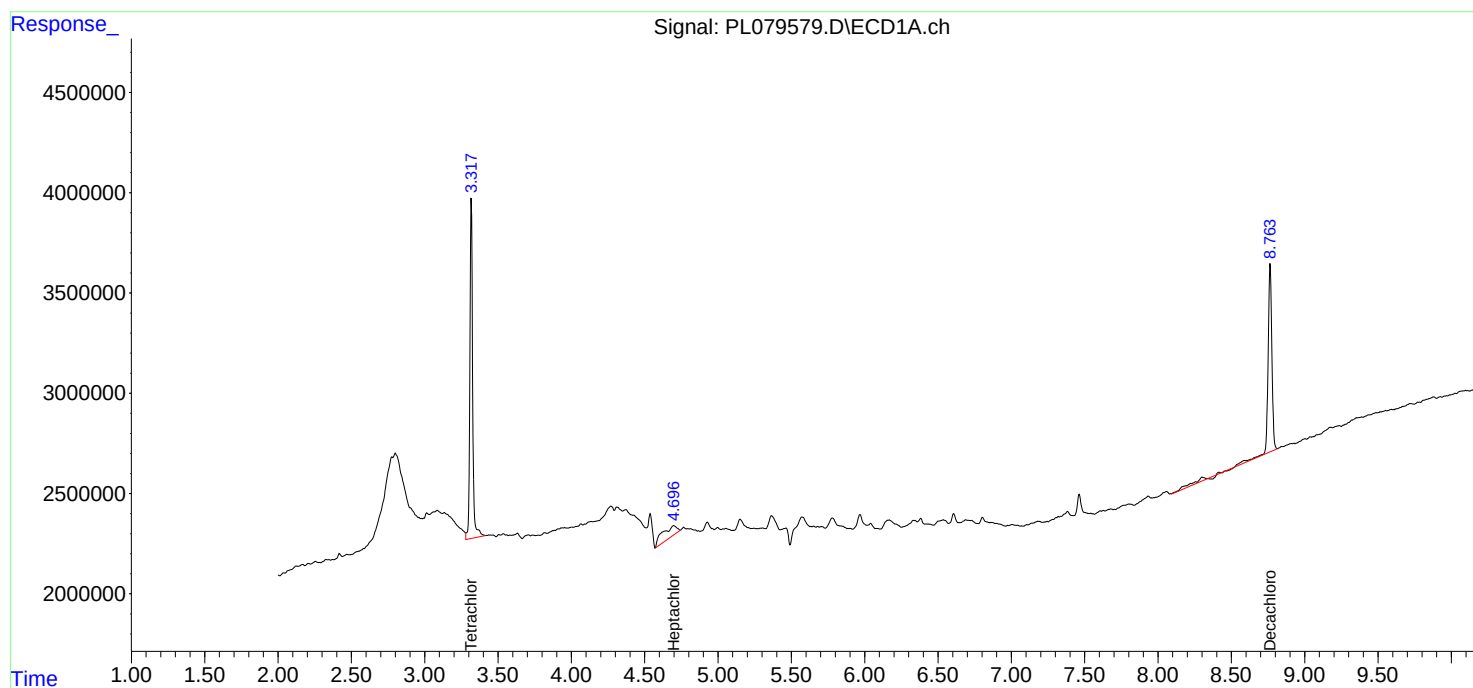


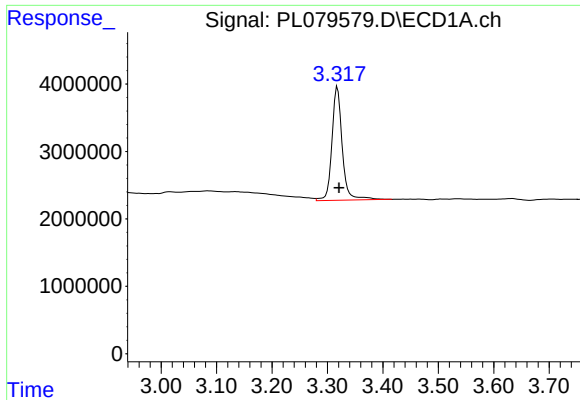

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.003 min
Response: 21840987
Conc: 9.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

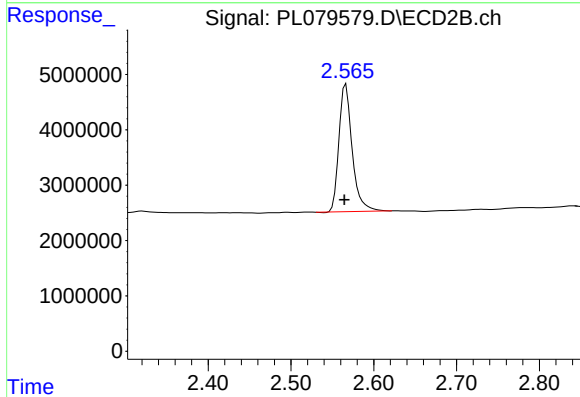


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: 0.002 min
Response: 25626662
Conc: 9.41 ng/ml

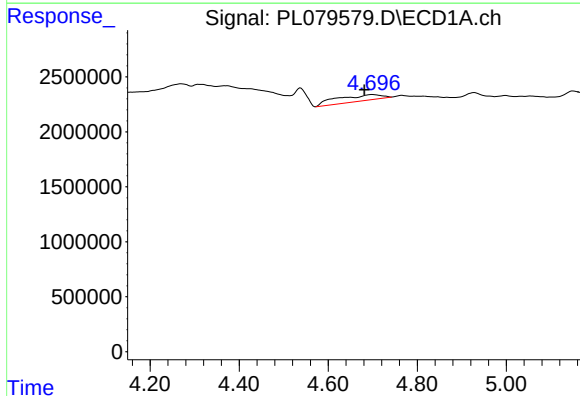


#4 Heptachlor

R.T.: 4.699 min
Delta R.T.: 0.018 min
Response: 3841154
Conc: 1.17 ng/ml

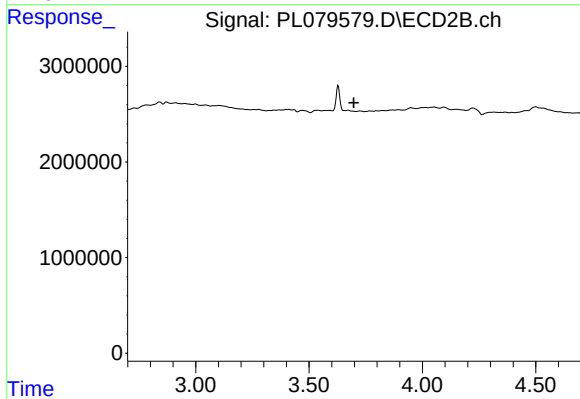

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.698 min
Response: 0
Conc: N.D.

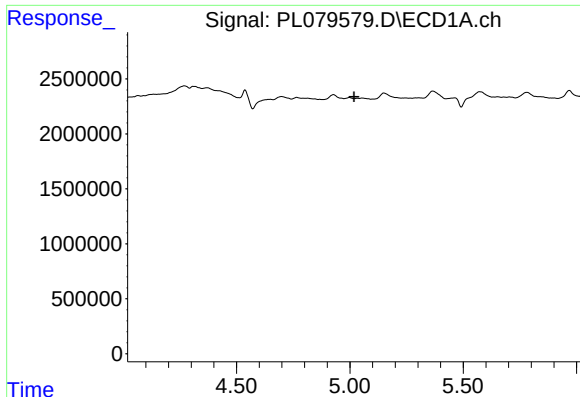

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

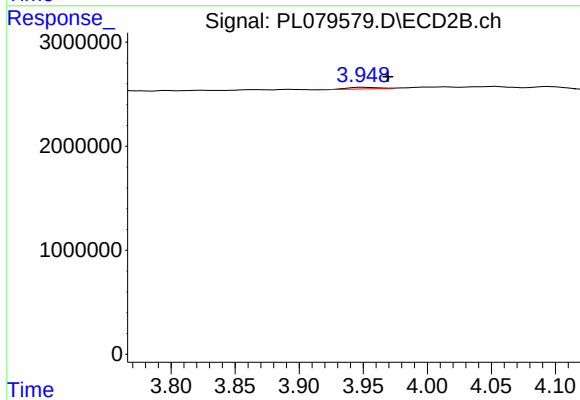


#5 Aldrin

R.T.: 3.949 min
Delta R.T.: -0.020 min
Response: 244244
Conc: 0.07 ng/ml

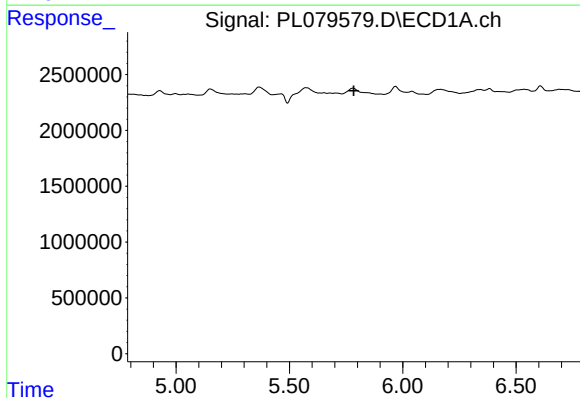


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.784 min
Response: 0
Conc: N.D.

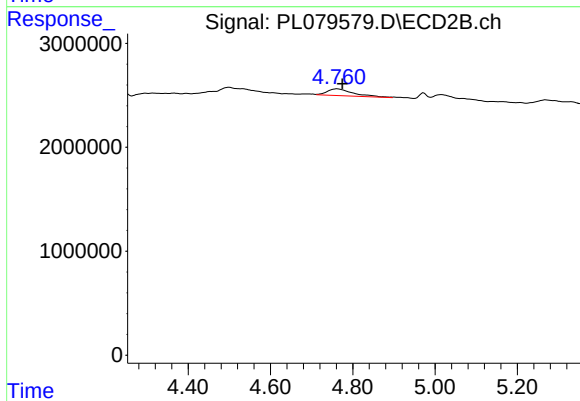

#11 alpha-Chlordane


R.T.: 4.761 min
Delta R.T.: -0.013 min
Response: 2821550
Conc: 0.84 ng/ml

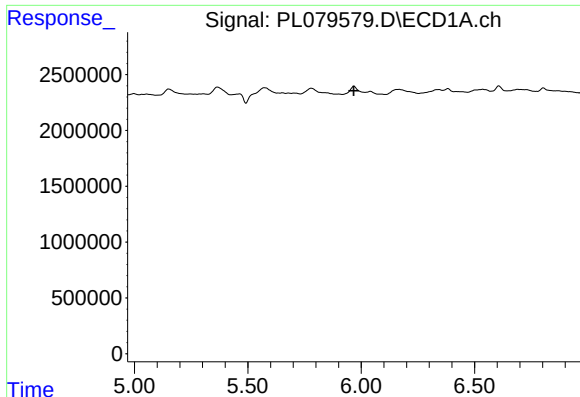

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.968 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

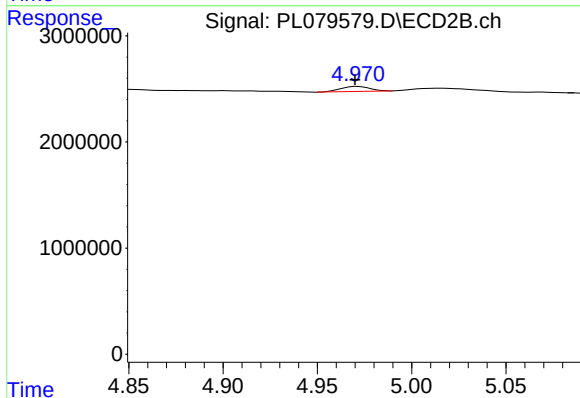


#12 4,4'-DDE

R.T.: 4.972 min
Delta R.T.: 0.002 min
Response: 501157
Conc: 0.16 ng/ml

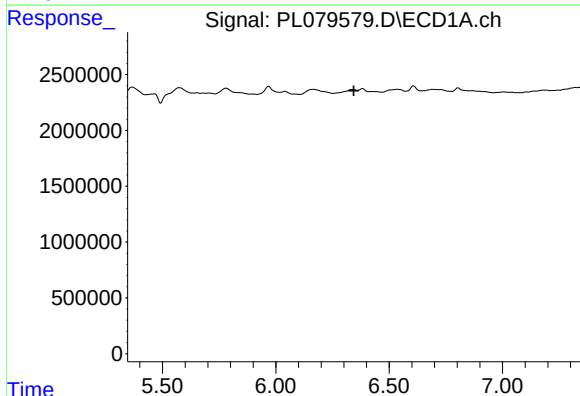


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

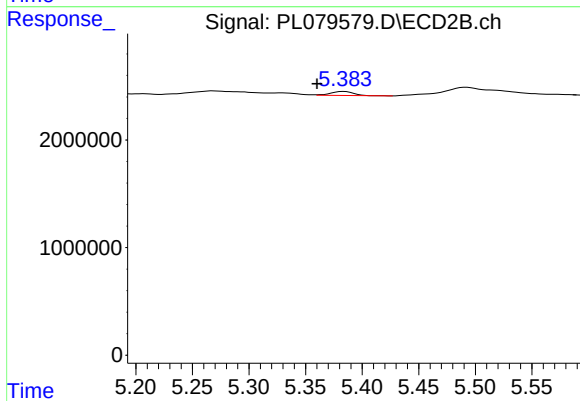

#14 Endrin


R.T.: 5.384 min
Delta R.T.: 0.024 min
Response: 516167
Conc: 0.17 ng/ml

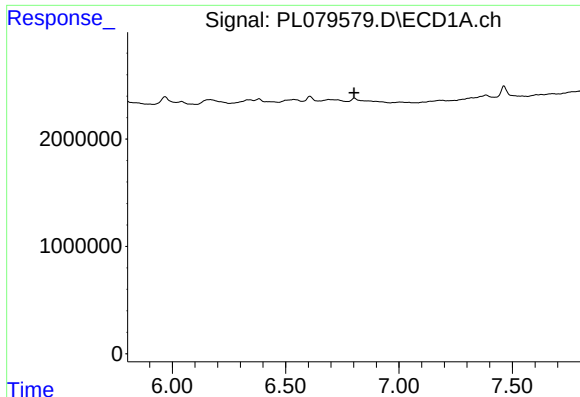

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

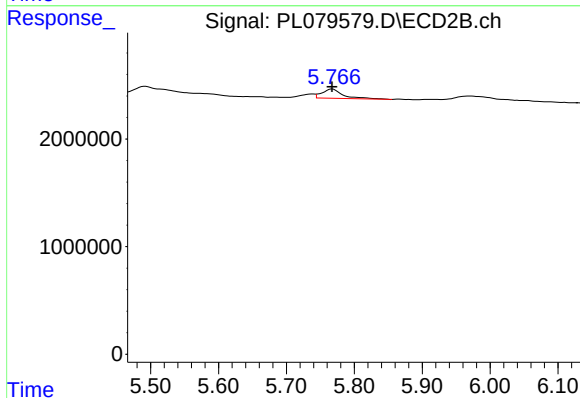


#17 4,4'-DDT

R.T.: 5.768 min
Delta R.T.: 0.000 min
Response: 1875697
Conc: 0.72 ng/ml

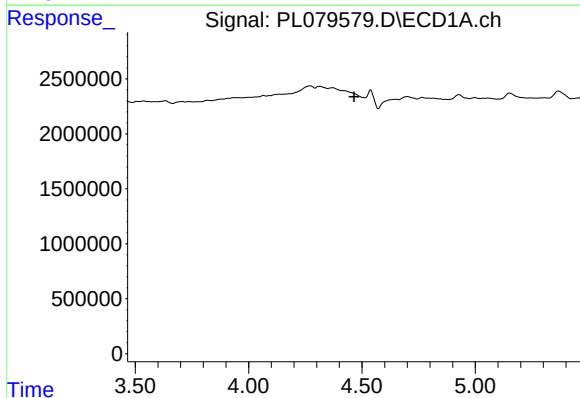


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

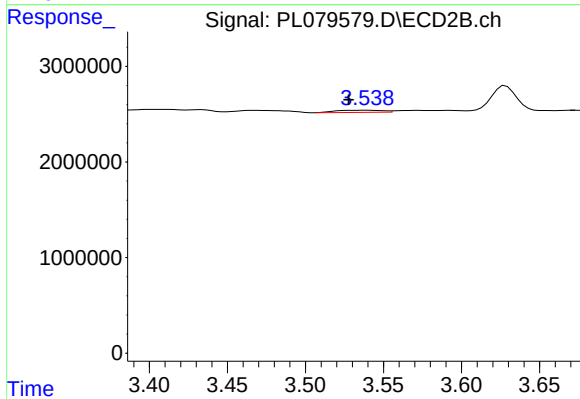

#23 Chlordane-1


R.T.: 3.539 min
Delta R.T.: 0.011 min
Response: 468905
Conc: 4.41 ng/ml

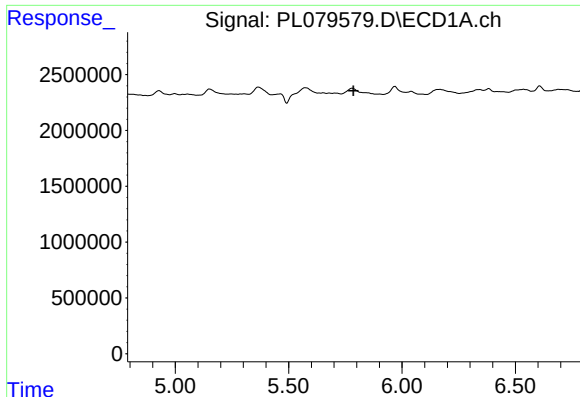

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

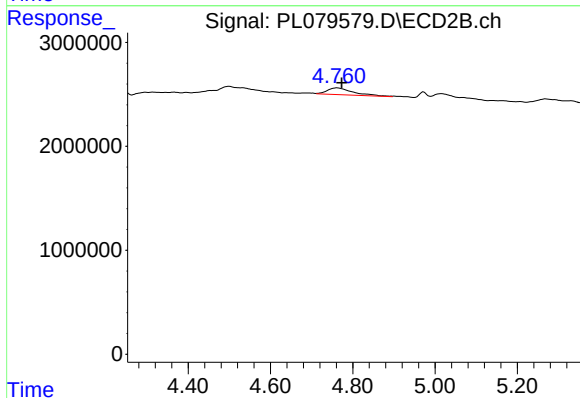


#26 Chlordane-4

R.T.: 4.761 min
Delta R.T.: -0.012 min
Response: 2821550
Conc: 7.79 ng/ml

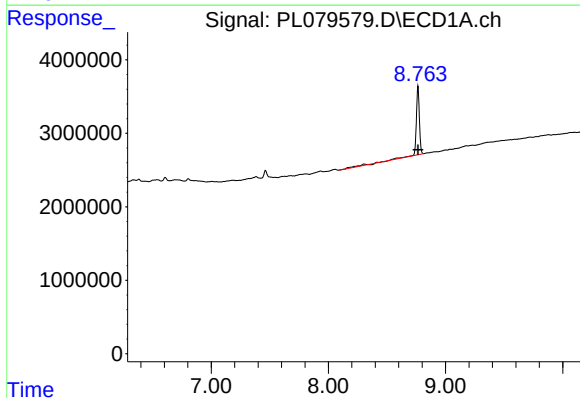

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 17904944
Conc: 9.22 ng/ml

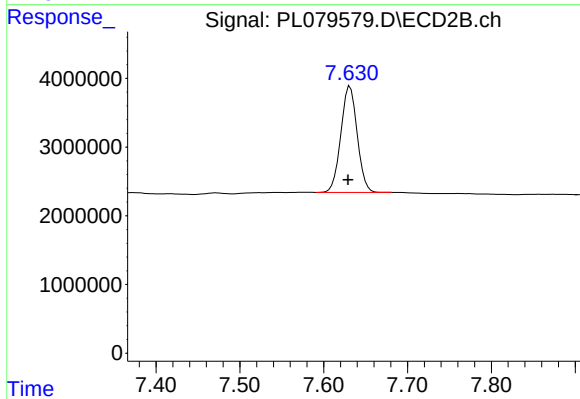

#28 Decachlorobiphenyl

R.T.: 7.632 min
Delta R.T.: 0.002 min
Response: 20949192
Conc: 8.92 ng/ml