

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120525\
 Data File : PL097785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2025 10:49
 Operator : AR\AJ
 Sample : Q3753-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:16:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 26 07:07:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	2.803	57285831	71697647	11.180	10.024
28)	SA Decachlor...	8.964	7.950	73662795	108.3E6	22.950	23.013
Target Compounds							
7)	B delta-BHC	4.720	0.000	4810579	0	0.689	N.D. #
10)	B gamma-Chl...	0.000	4.990f	0	13882631	N.D.	1.551 #
11)	B alpha-Chl...	5.960	0.000	6298222	0	1.053	N.D. #
12)	B 4,4'-DDE	6.130	5.267	54199282	65855026	10.117	8.091
13)	MA Dieldrin	6.279	5.397	49400124	58239271	8.832	6.740
14)	MA Endrin	0.000	5.682	0	6474255	N.D.	0.842 #
16)	A 4,4'-DDD	6.639	5.819	40238581	40963934	9.451	6.055 #
17)	MA 4,4'-DDT	6.953	6.071	29574894	25607890	8.105	5.196 #
18)	B Endrin al...	0.000	6.165f	0	23573778	N.D.	0.551 #
25)	Chlordane-3	0.000	4.990f	0	13882631	N.D.	16.971 #
26)	Chlordane-4	5.960	0.000	6298222	0	6.624	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120525\
Data File : PL097785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2025 10:49
Operator : AR\AJ
Sample : Q3753-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:16:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Wed Nov 26 07:07:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

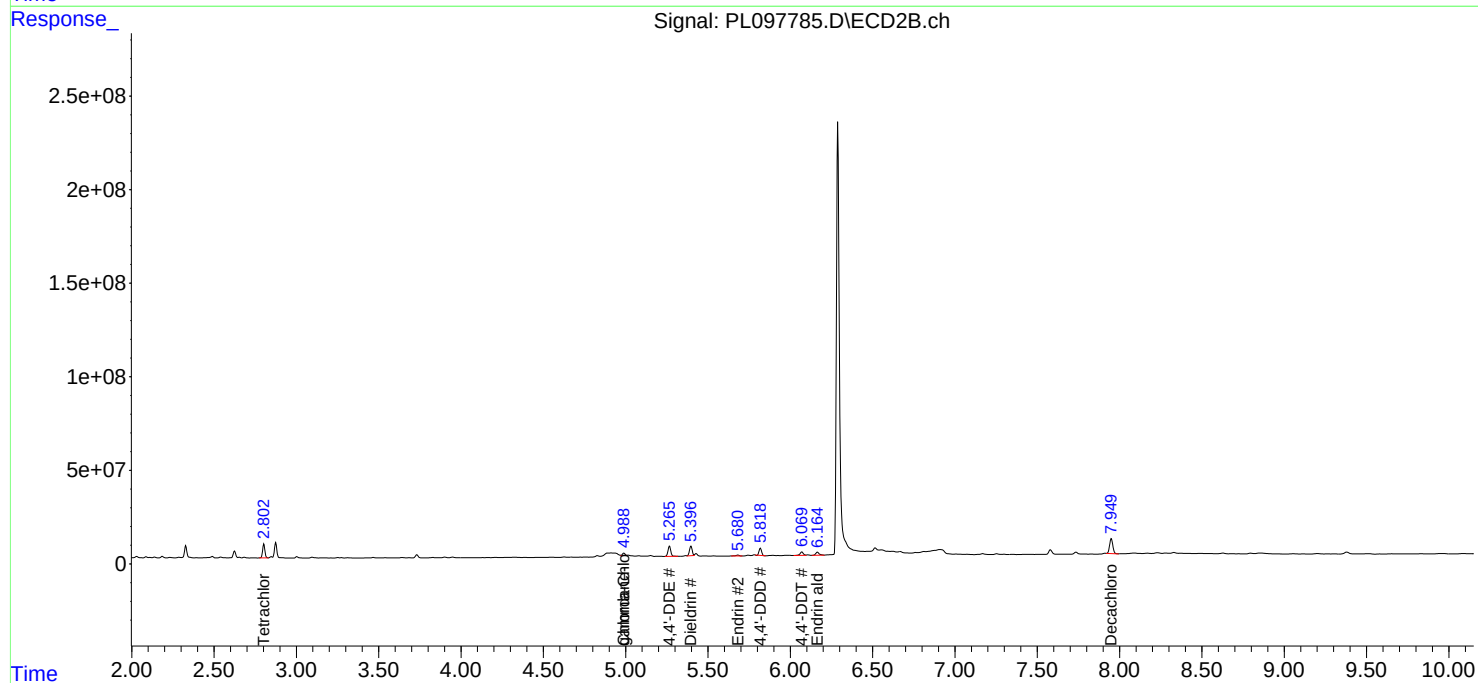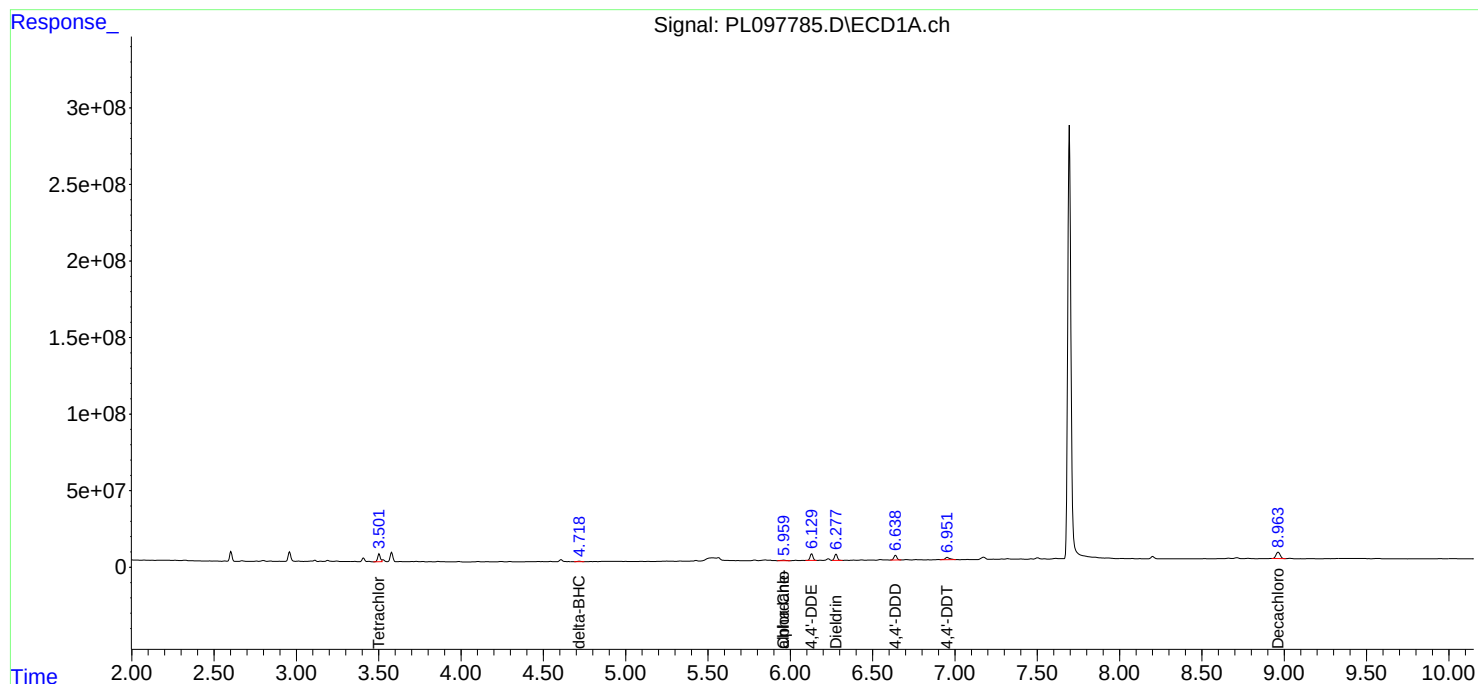


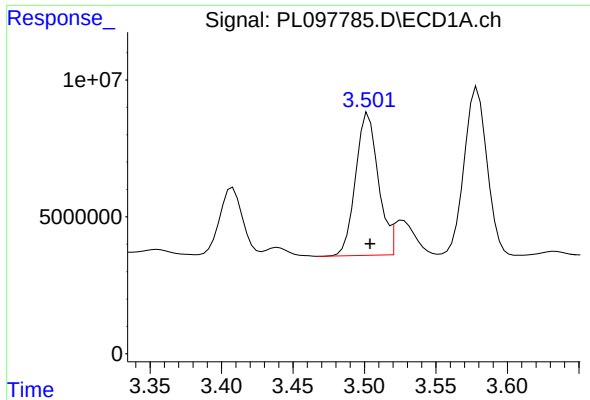

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: -0.001 min
Response: 57285831
Conc: 11.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

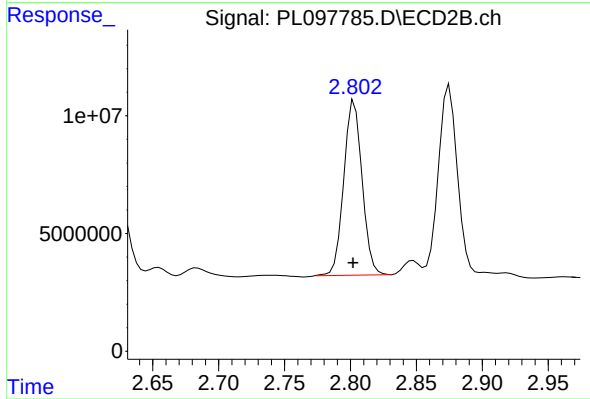


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 71697647
Conc: 10.02 ng/ml

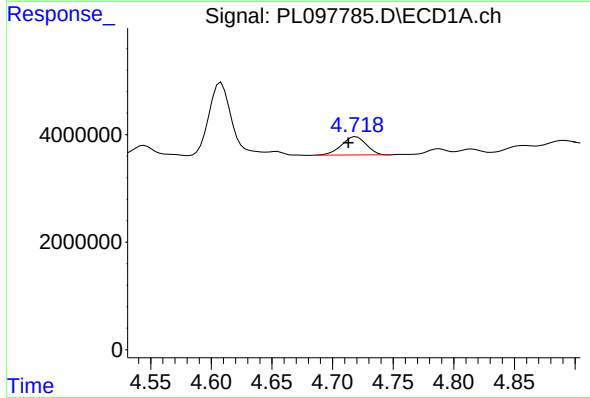


#7 delta-BHC

R.T.: 4.720 min
Delta R.T.: 0.007 min
Response: 4810579
Conc: 0.69 ng/ml

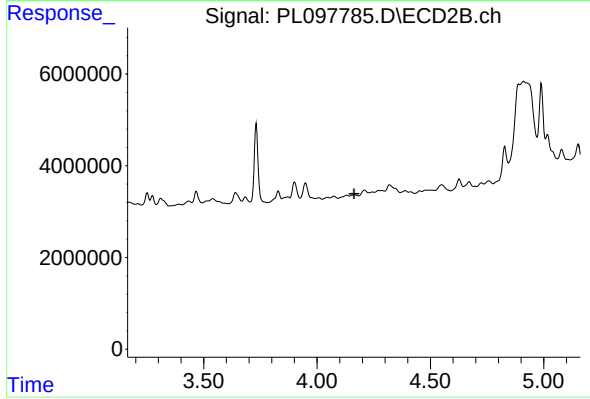

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.163 min
Response: 0
Conc: N.D.

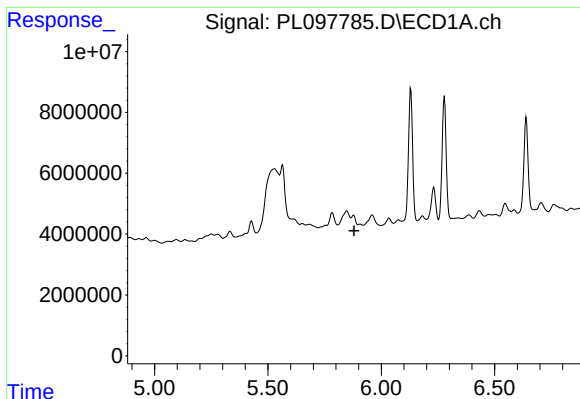

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.881 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

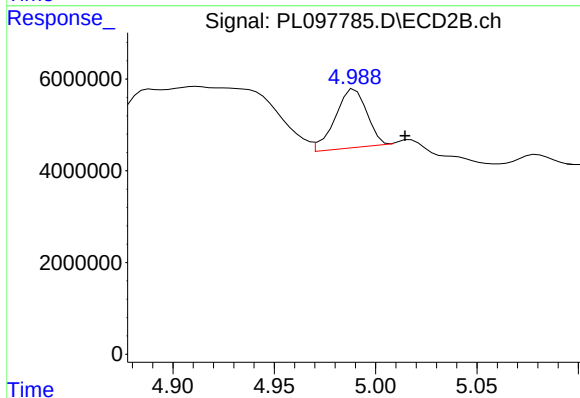


#10 gamma-Chlordane

R.T.: 4.990 min
Delta R.T.: -0.025 min
Response: 13882631
Conc: 1.55 ng/ml

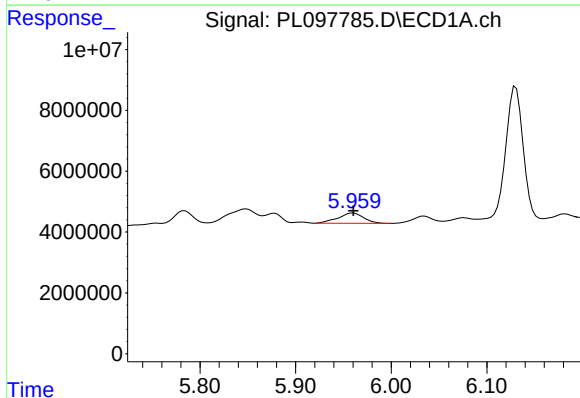


#11 alpha-Chlordane

R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 6298222
Conc: 1.05 ng/ml

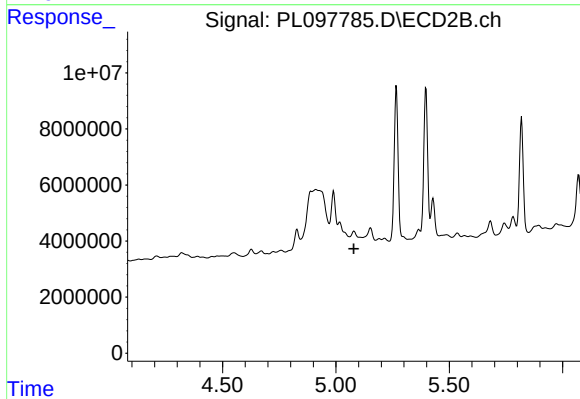

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.078 min
Response: 0
Conc: N.D.

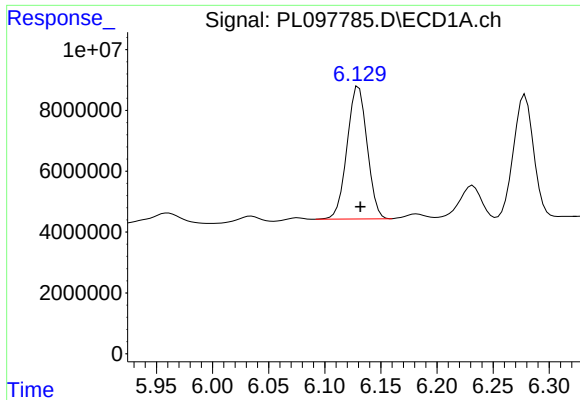

#12 4,4'-DDE


R.T.: 6.130 min
Delta R.T.: -0.001 min
Response: 54199282
Conc: 10.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

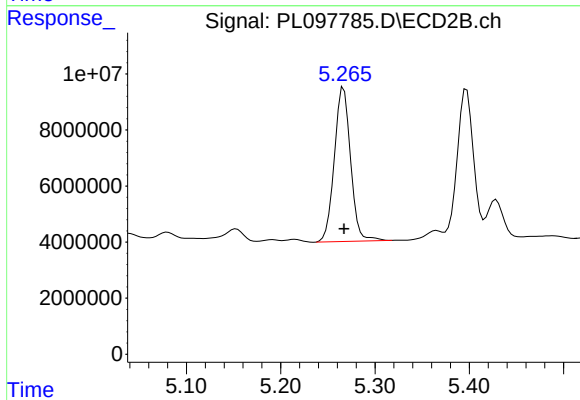


#12 4,4'-DDE

R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 65855026
Conc: 8.09 ng/ml

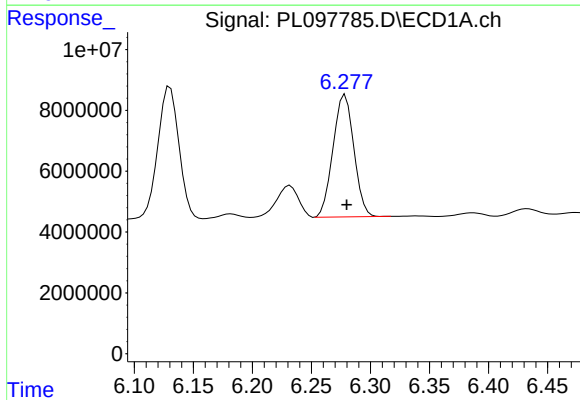


#13 Dieldrin

R.T.: 6.279 min
Delta R.T.: -0.001 min
Response: 49400124
Conc: 8.83 ng/ml

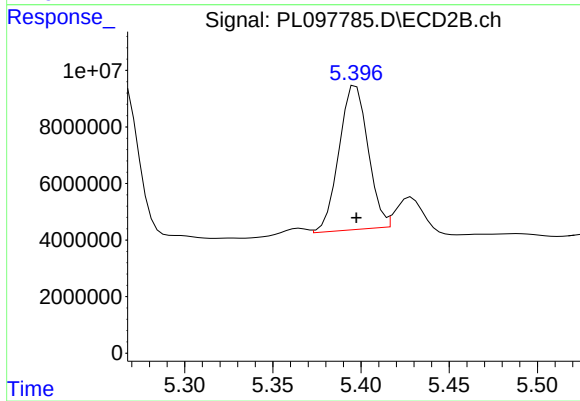

#13 Dieldrin


R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 58239271
Conc: 6.74 ng/ml

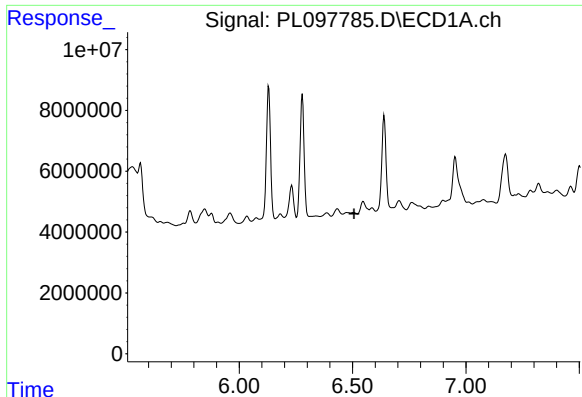

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

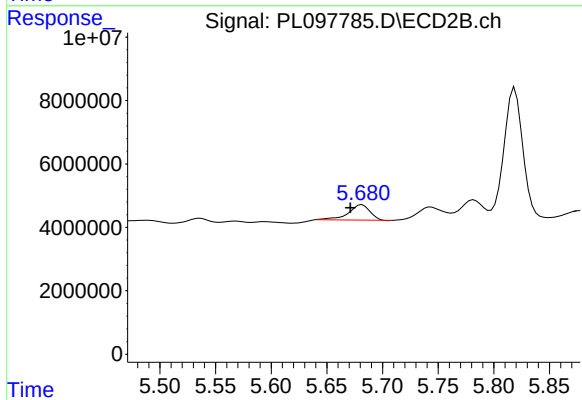


#14 Endrin

R.T.: 5.682 min
Delta R.T.: 0.011 min
Response: 6474255
Conc: 0.84 ng/ml

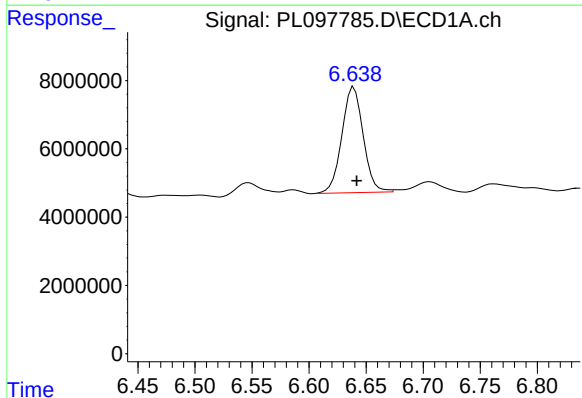


#16 4,4'-DDD

R.T.: 6.639 min
Delta R.T.: -0.002 min
Response: 40238581
Conc: 9.45 ng/ml

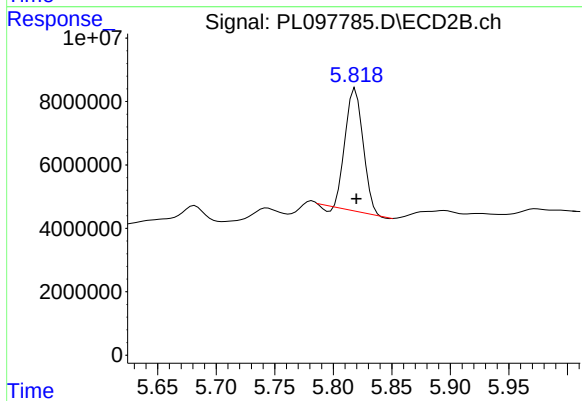

#16 4,4'-DDD


R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 40963934
Conc: 6.06 ng/ml

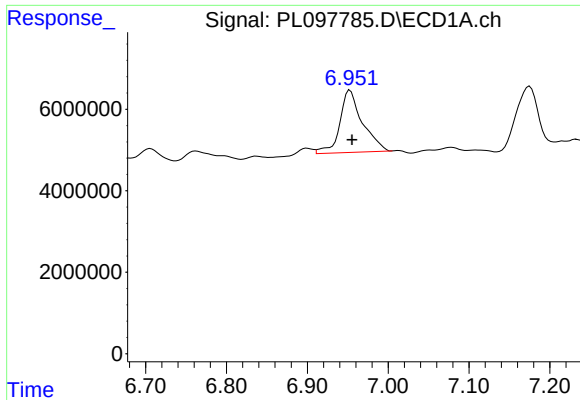

#17 4,4'-DDT


R.T.: 6.953 min
Delta R.T.: -0.002 min
Response: 29574894
Conc: 8.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

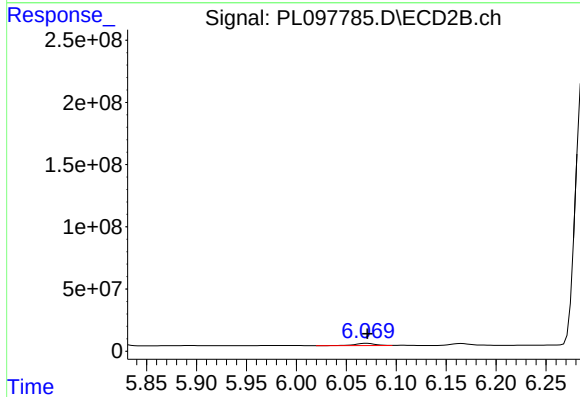


#17 4,4'-DDT

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 25607890
Conc: 5.20 ng/ml

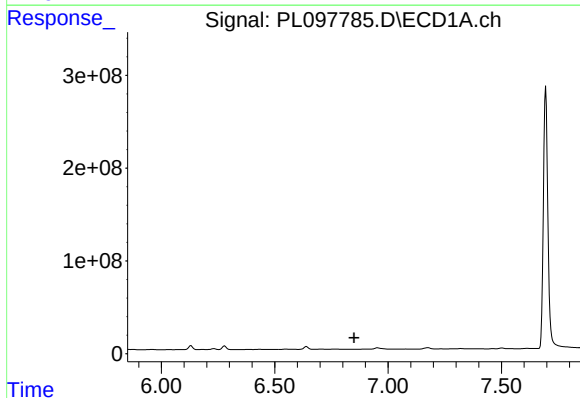


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

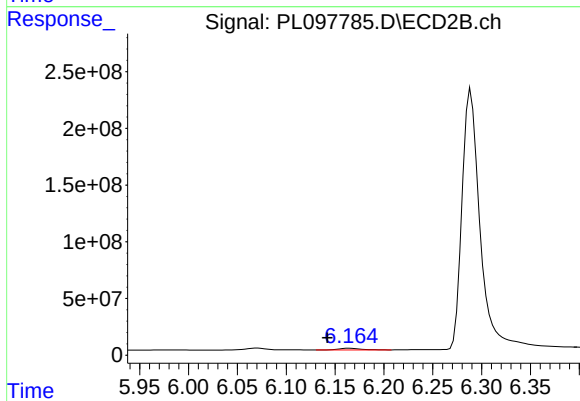

#18 Endrin aldehyde


R.T.: 6.165 min
Delta R.T.: 0.023 min
Response: 23573778
Conc: 0.55 ng/ml

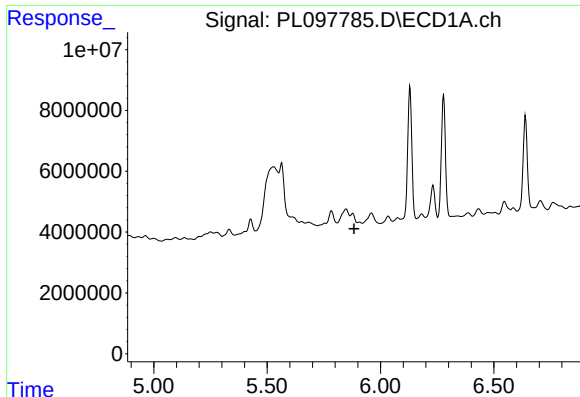

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

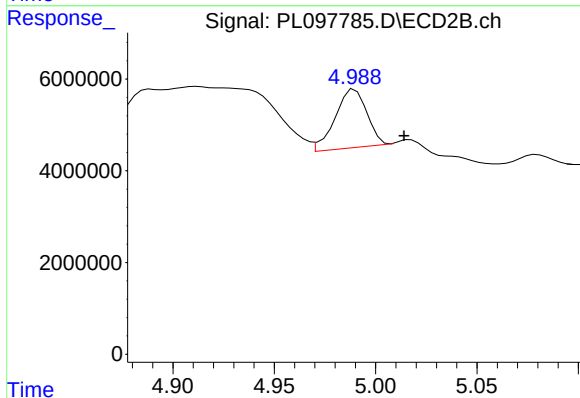


#25 Chlordane-3

R.T.: 4.990 min
Delta R.T.: -0.024 min
Response: 13882631
Conc: 16.97 ng/ml

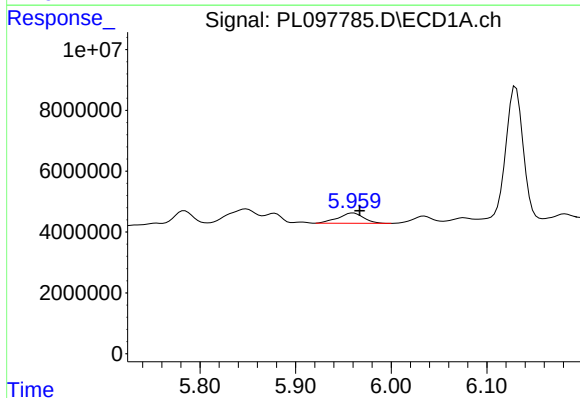


#26 Chlordane-4

R.T.: 5.960 min
Delta R.T.: -0.007 min
Response: 6298222
Conc: 6.62 ng/ml

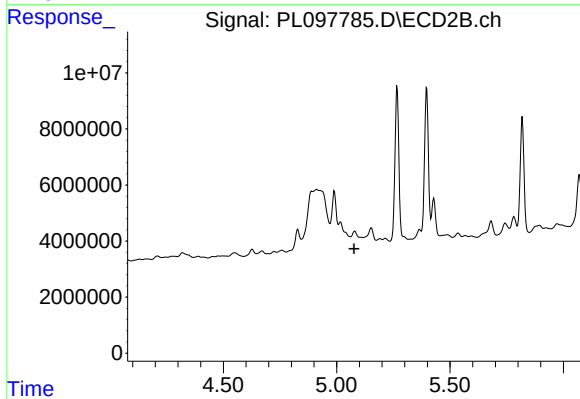

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

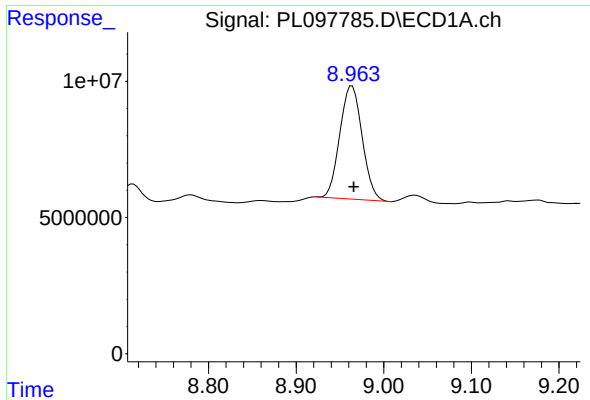

#28 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.002 min
Response: 73662795
Conc: 22.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

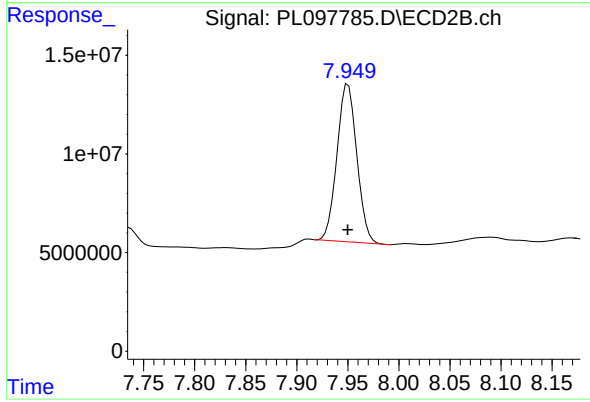

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 108317070
Conc: 23.01 ng/ml