

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120525\
 Data File : PL097789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2025 11:49
 Operator : AR\AJ
 Sample : Q3758-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:18:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 26 07:07:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.510	2.815	52759245	66564317	10.297	9.306
28)	SA Decachlor...	8.964	7.951	61529165	77628381	19.170	16.493
Target Compounds							
7)	B delta-BHC	4.725	0.000	5167939	0	0.740	N.D. #
12)	B 4,4'-DDE	0.000	5.274	0	8158241	N.D.	1.002 #
13)	MA Dieldrin	0.000	5.398	0	19507721	N.D.	2.258 #
14)	MA Endrin	0.000	5.694f	0	6889184	N.D.	0.896 #
15)	B Endosulfa...	6.702f	5.972	18708833	2445164	3.688	0.336 #
16)	A 4,4'-DDD	6.624f	0.000	10650879	0	2.502	N.D. #
19)	B Endosulfa...	0.000	6.383f	0	28642837	N.D.	4.174 #
20)	A Methoxychlor	0.000	6.649	0	8192638	N.D.	3.050 #
21)	B Endrin ke...	0.000	6.855	0	13487146	N.D.	1.851 #
23)	Chlordane-1	4.660	0.000	47712176	0	210.026	N.D. #
24)	Chlordane-2	0.000	4.409f	0	2820805	N.D.	9.577 #
27)	Chlordane-5	6.783f	5.972	6884397	2445164	47.926	9.333 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120525\
Data File : PL097789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2025 11:49
Operator : AR\AJ
Sample : Q3758-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:18:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Wed Nov 26 07:07:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

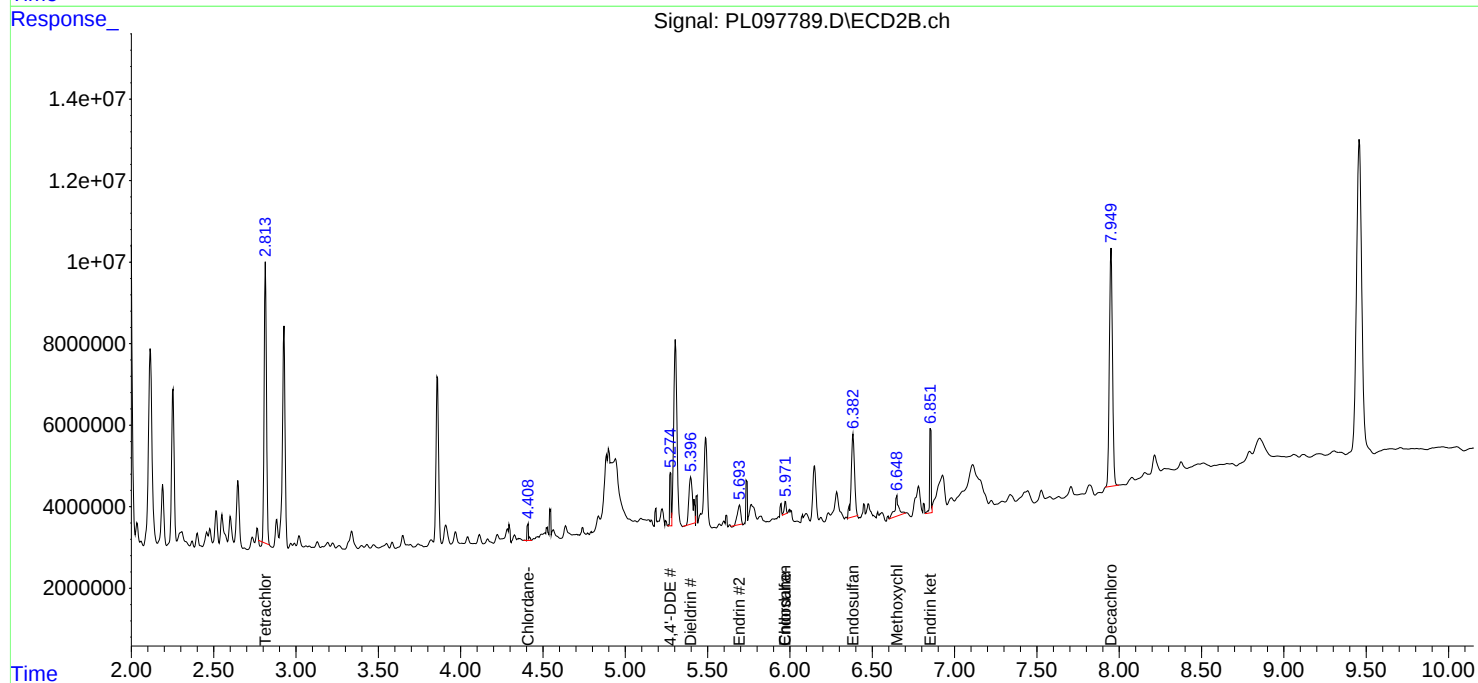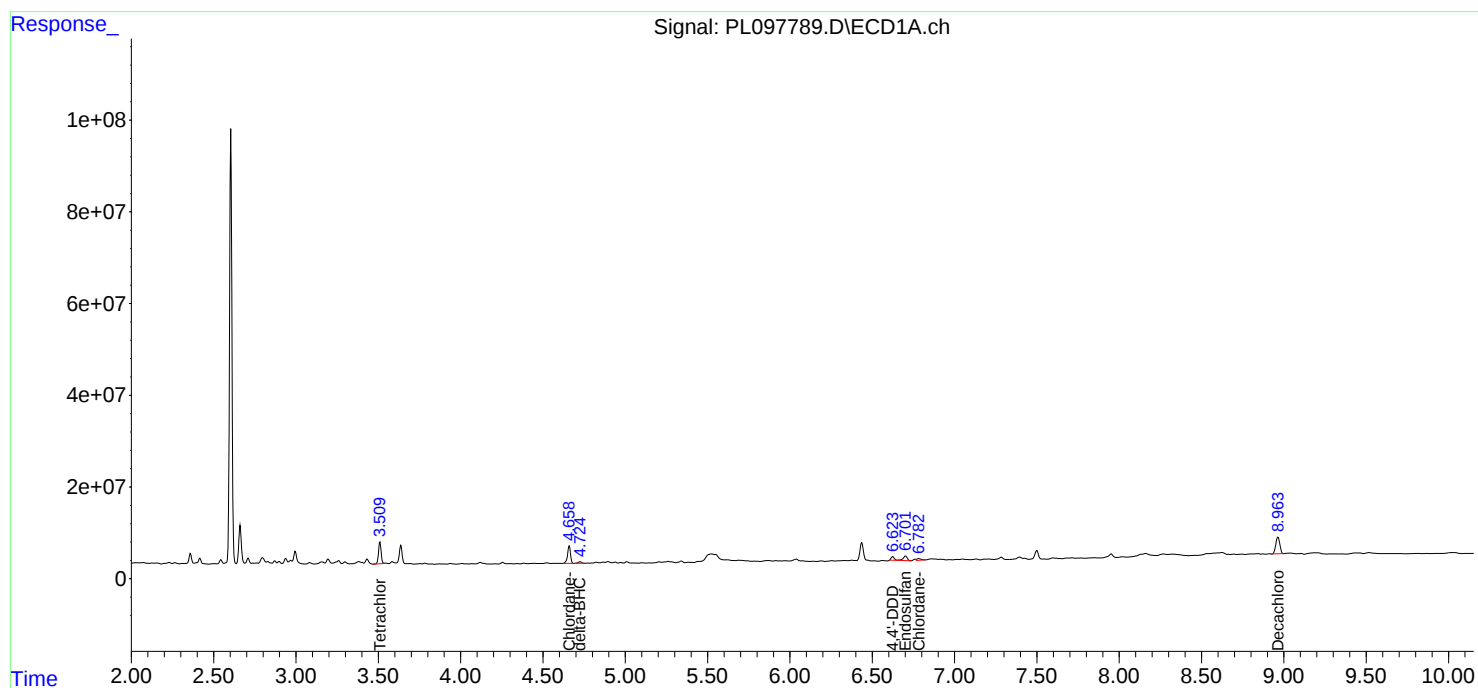


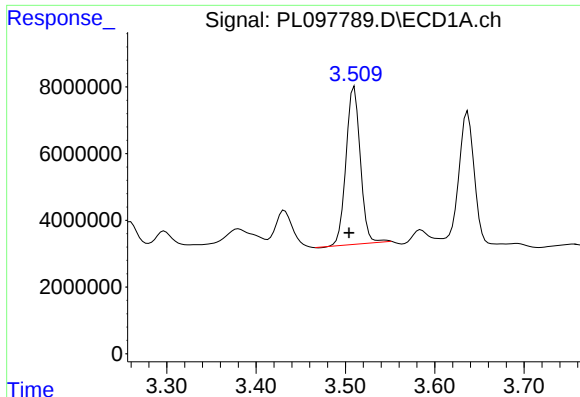

#1 Tetrachloro-m-xylene


R.T.: 3.510 min
Delta R.T.: 0.006 min
Response: 52759245
Conc: 10.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

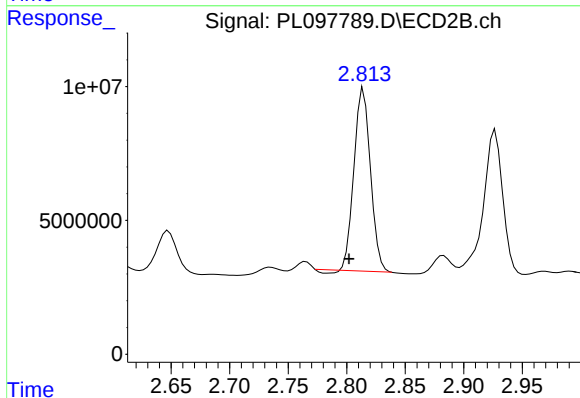


#1 Tetrachloro-m-xylene

R.T.: 2.815 min
Delta R.T.: 0.012 min
Response: 66564317
Conc: 9.31 ng/ml

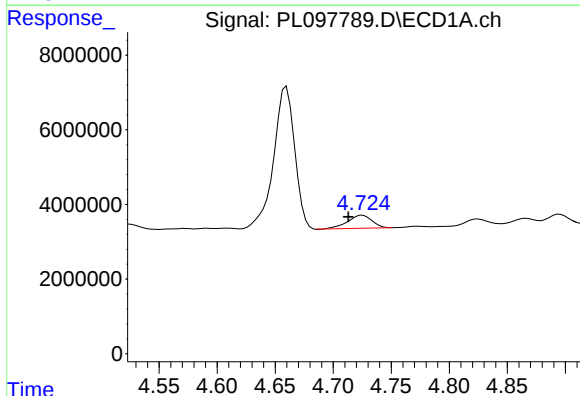


#7 delta-BHC

R.T.: 4.725 min
Delta R.T.: 0.012 min
Response: 5167939
Conc: 0.74 ng/ml

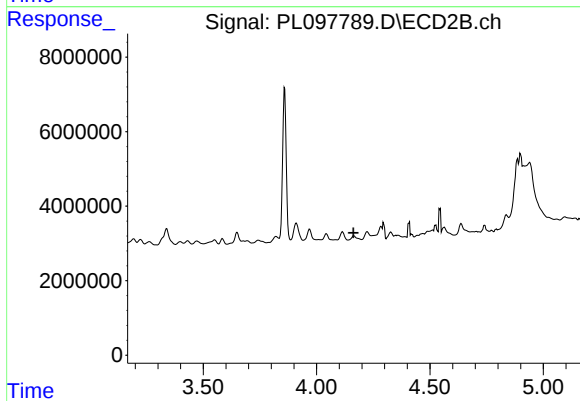

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.163 min
Response: 0
Conc: N.D.

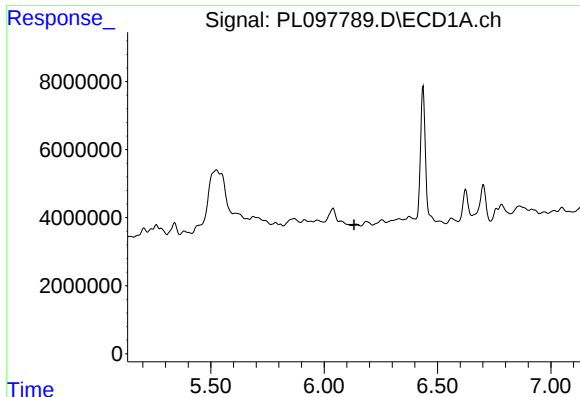

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

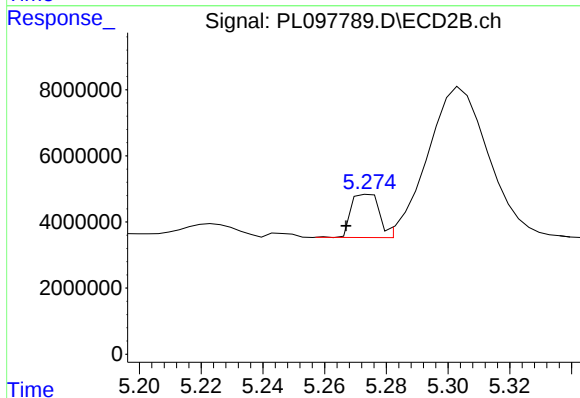


#12 4,4'-DDE

R.T.: 5.274 min
Delta R.T.: 0.007 min
Response: 8158241
Conc: 1.00 ng/ml

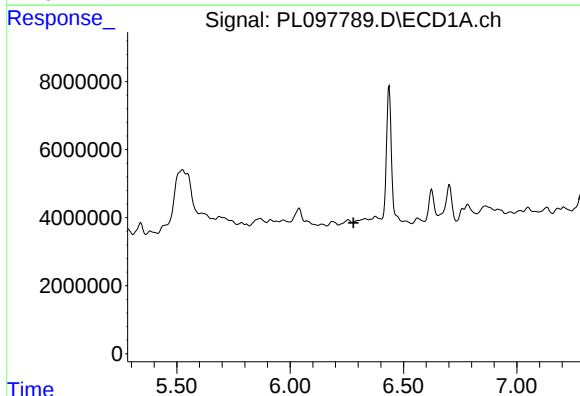


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.280 min
Response: 0
Conc: N.D.

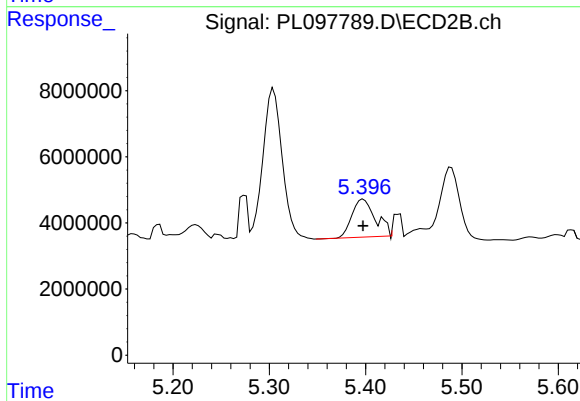

#13 Dieldrin


R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 19507721
Conc: 2.26 ng/ml

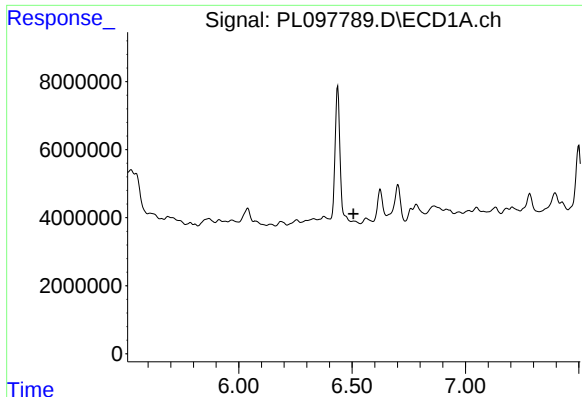

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

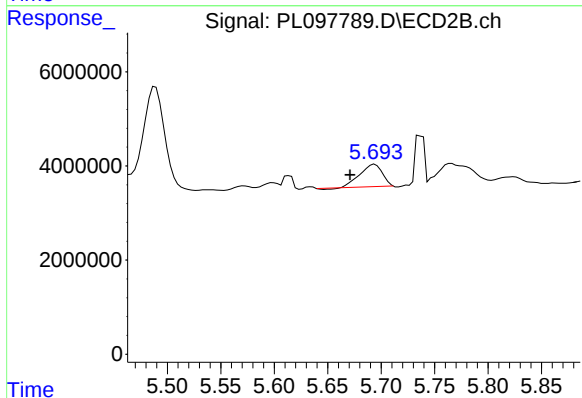


#14 Endrin

R.T.: 5.694 min
Delta R.T.: 0.023 min
Response: 6889184
Conc: 0.90 ng/ml

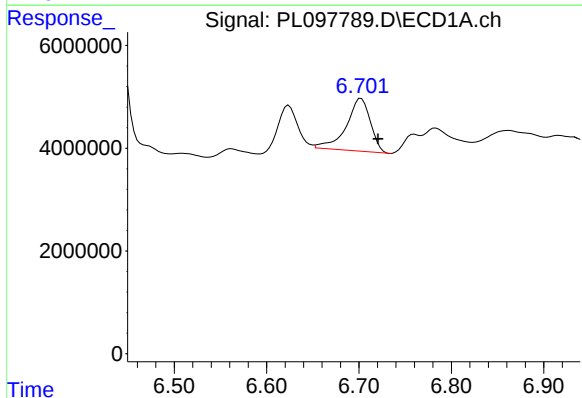


#15 Endosulfan II

R.T.: 6.702 min
Delta R.T.: -0.018 min
Response: 18708833
Conc: 3.69 ng/ml

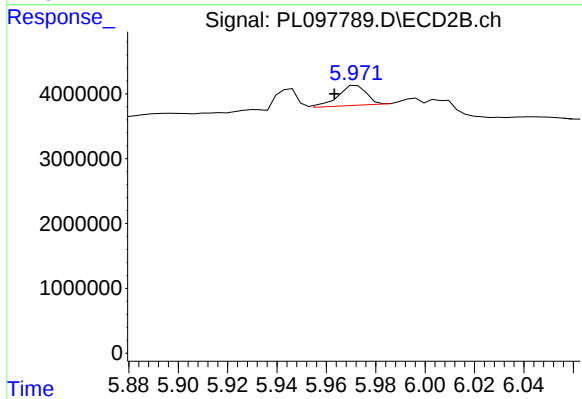

#15 Endosulfan II


R.T.: 5.972 min
Delta R.T.: 0.009 min
Response: 2445164
Conc: 0.34 ng/ml

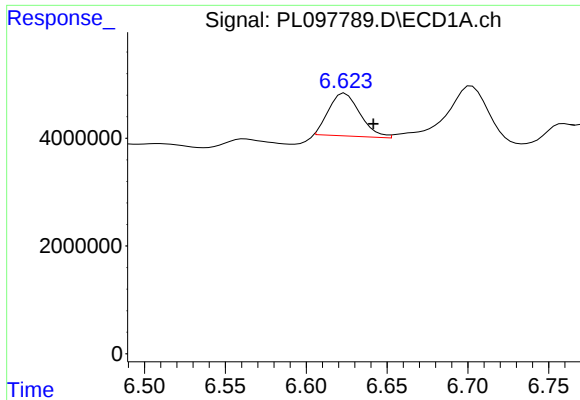

#16 4,4'-DDD


R.T.: 6.624 min
Delta R.T.: -0.018 min
Response: 10650879
Conc: 2.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

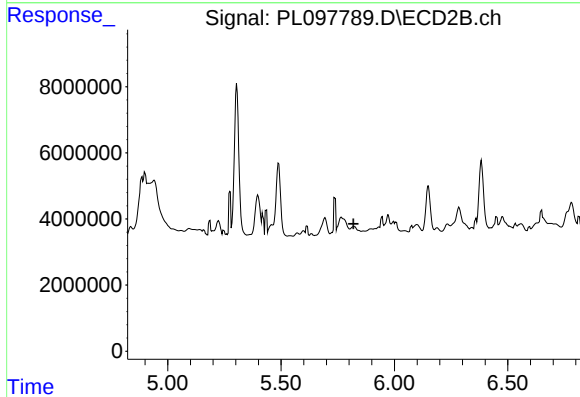


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

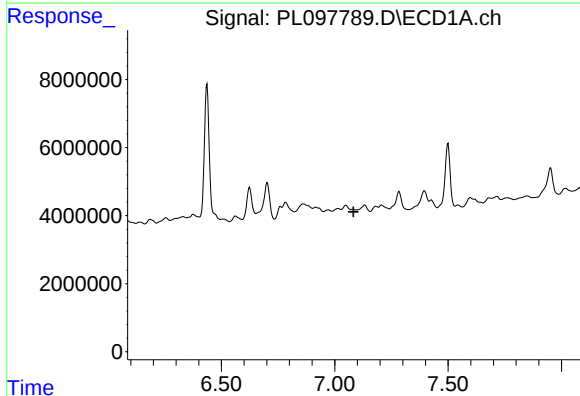


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.083 min
Response: 0
Conc: N.D.

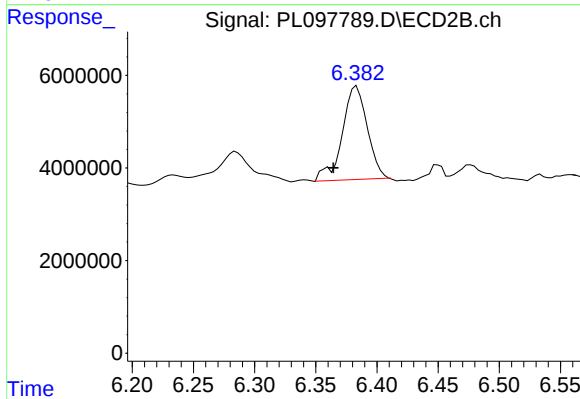

#19 Endosulfan Sulfate


R.T.: 6.383 min
Delta R.T.: 0.019 min
Response: 28642837
Conc: 4.17 ng/ml

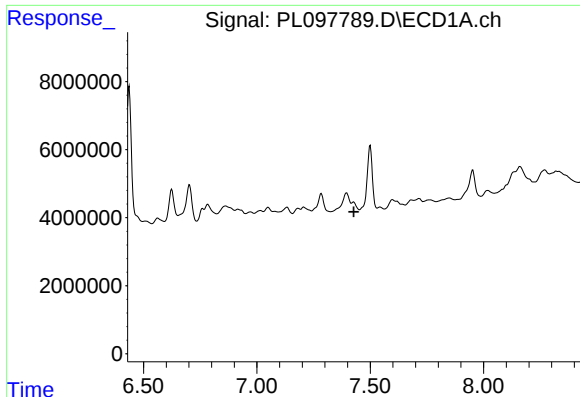

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

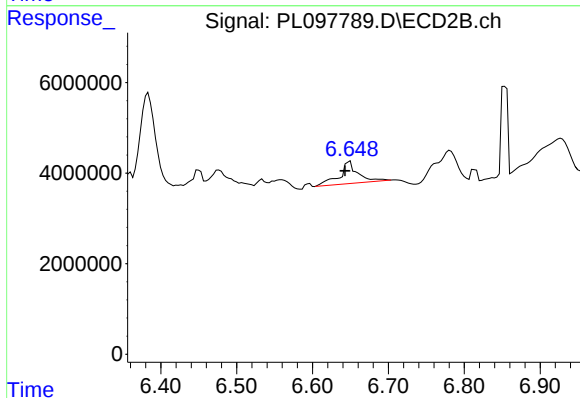


#20 Methoxychlor

R.T.: 6.649 min
Delta R.T.: 0.006 min
Response: 8192638
Conc: 3.05 ng/ml

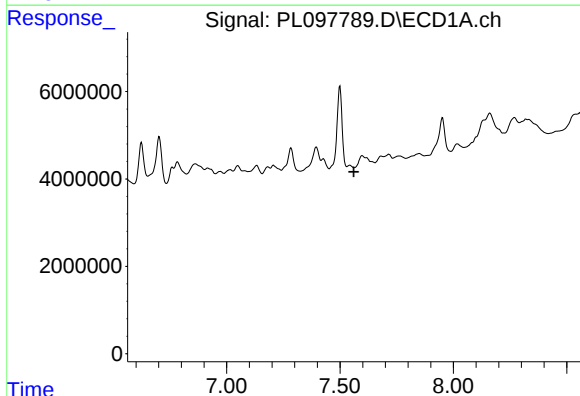


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.561 min
Response: 0
Conc: N.D.

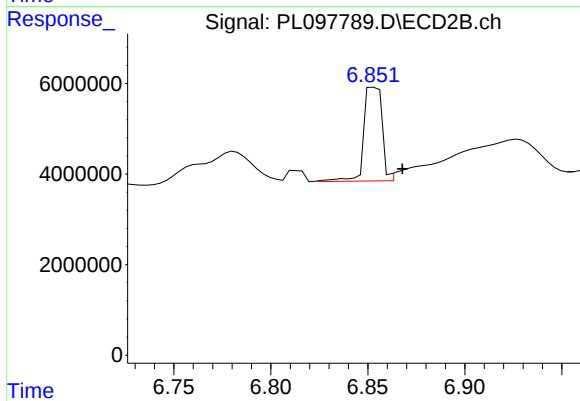

#21 Endrin ketone


R.T.: 6.855 min
Delta R.T.: -0.013 min
Response: 13487146
Conc: 1.85 ng/ml

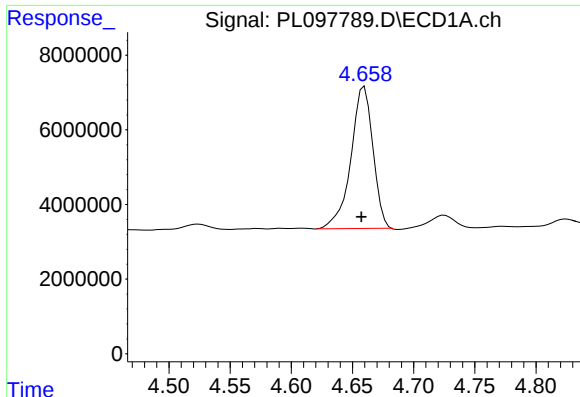

#23 Chlordane-1


R.T.: 4.660 min
Delta R.T.: 0.002 min
Response: 47712176
Conc: 210.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

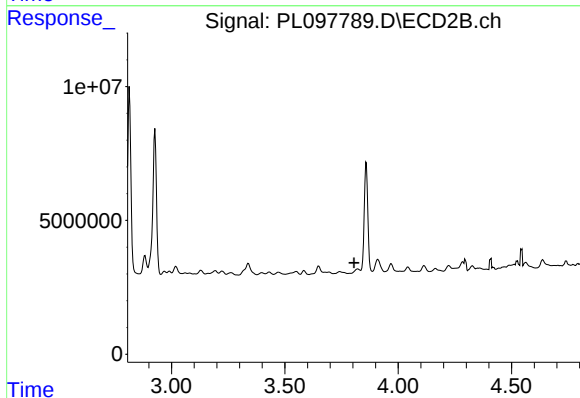


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 3.805 min
Response: 0
Conc: N.D.

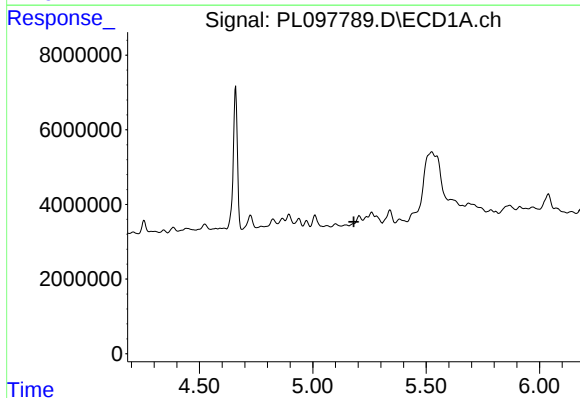


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.181 min
Response: 0
Conc: N.D.

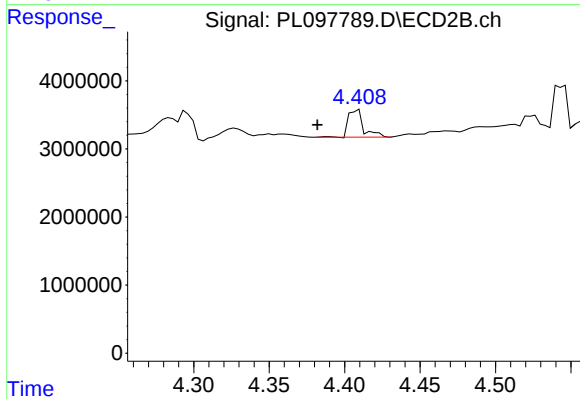

#24 Chlordane-2


R.T.: 4.409 min
Delta R.T.: 0.027 min
Response: 2820805
Conc: 9.58 ng/ml

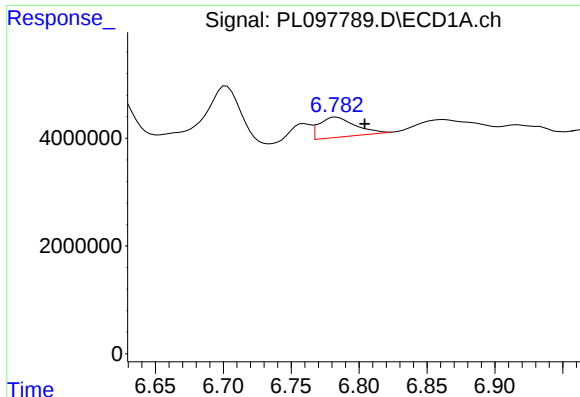

#27 Chlordane-5


R.T.: 6.783 min
Delta R.T.: -0.021 min
Response: 6884397
Conc: 47.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

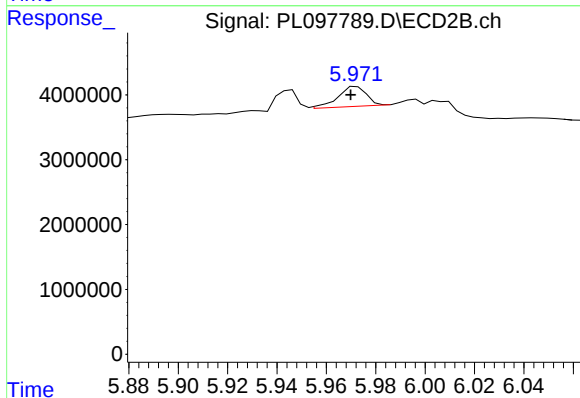


#27 Chlordane-5

R.T.: 5.972 min
Delta R.T.: 0.002 min
Response: 2445164
Conc: 9.33 ng/ml

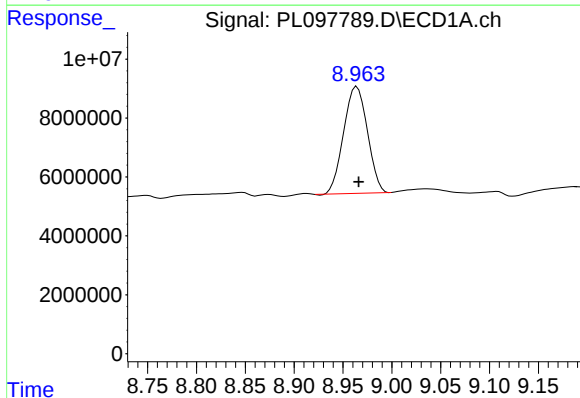

#28 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.002 min
Response: 61529165
Conc: 19.17 ng/ml

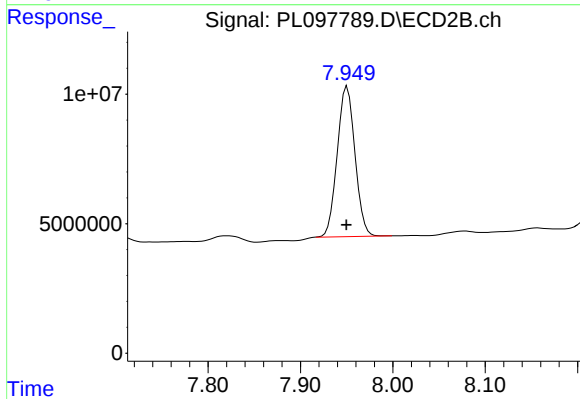

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 77628381
Conc: 16.49 ng/ml