

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120618\
 Data File : PL042850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2018 13:21
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 17:43:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 06 17:17:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.899	0.000	5511696	0	0.583	N.D. #
7) B	delta-BHC	0.000	5.154	0	22639399	N.D.	5.268 #
8) B	Heptachlo...	0.000	5.989	0	10668731	N.D.	2.813 #
10) B	gamma-Chl...	0.000	6.262	0	1616492	N.D.	0.440 #
11) B	alpha-Chl...	0.000	6.262f	0	1616492	N.D.	0.449 #
15) B	Endosulfa...	6.223f	0.000	2649968	0	0.398	N.D. #
23)	Chlordane-1	4.380	5.154	4679801	22639399	17.416	160.185 #
25)	Chlordane-3	0.000	6.262	0	1616492	N.D.	3.292 #
26)	Chlordane-4	0.000	6.262	0	1616492	N.D.	2.832 #
27)	Chlordane-5	6.223	0.000	2649968	0	11.048	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120618\
Data File : PL042850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2018 13:21
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 17:43:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Thu Dec 06 17:17:13 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

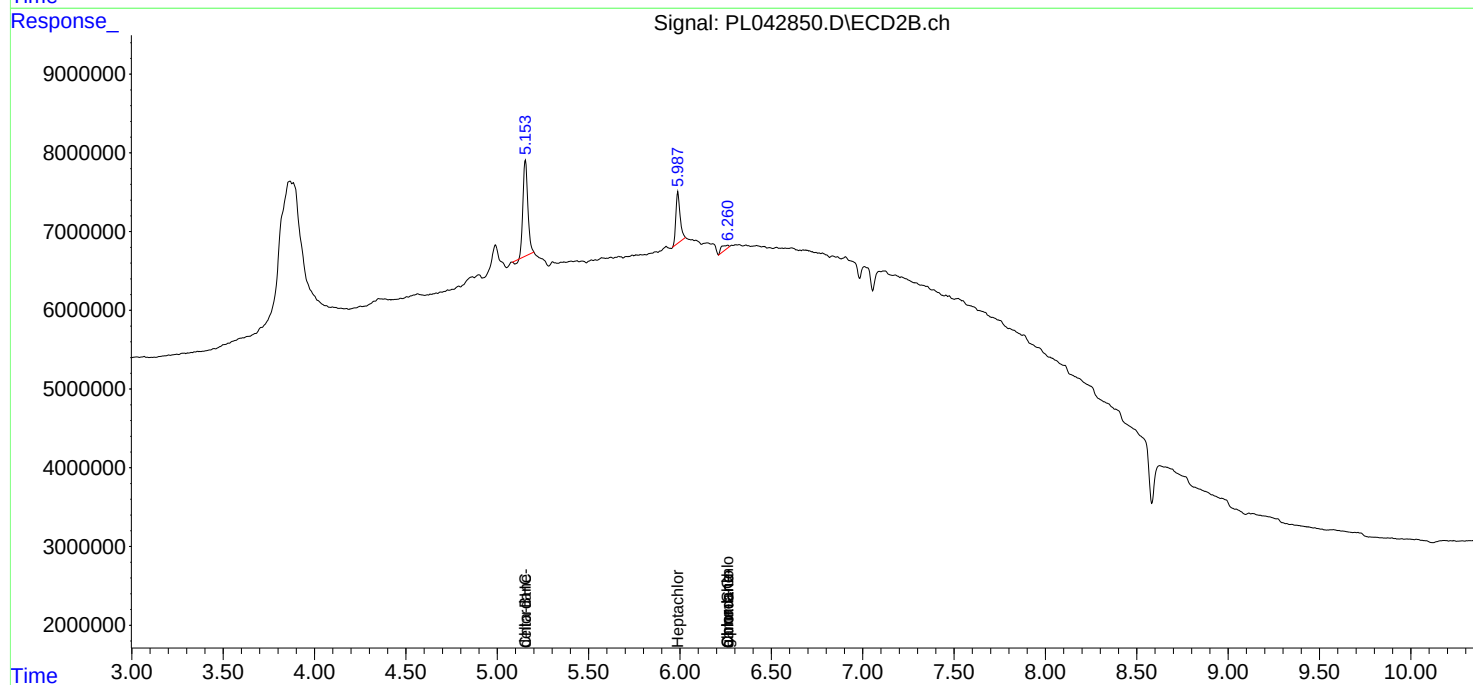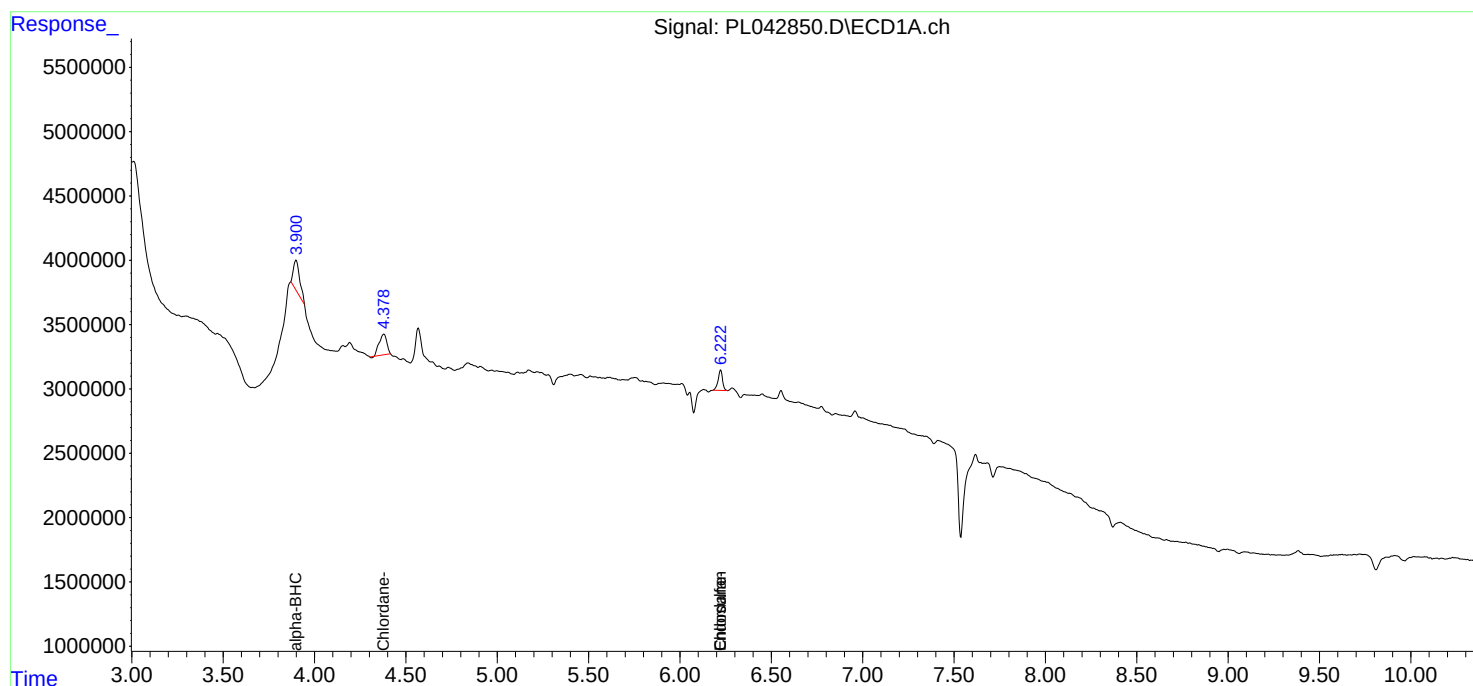


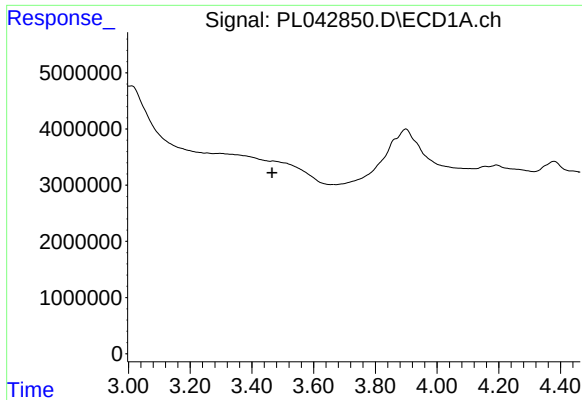

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

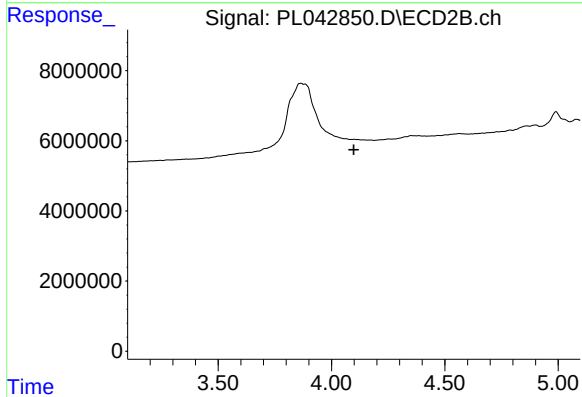


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.099 min
Response: 0
Conc: N.D.

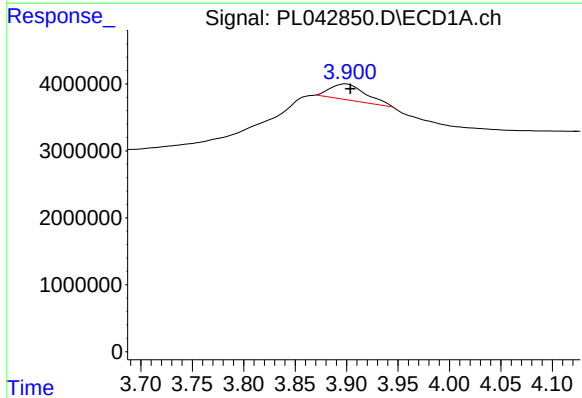


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: -0.004 min
Response: 5511696
Conc: 0.58 ng/ml

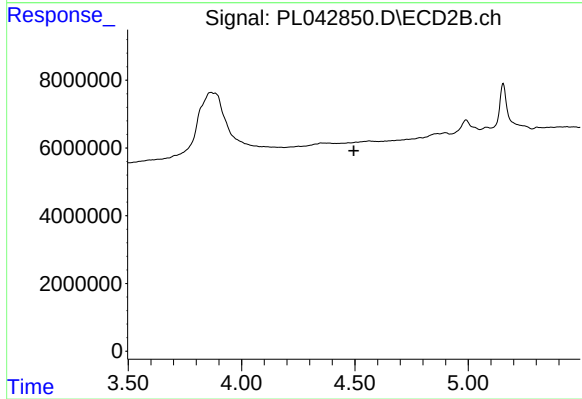

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.495 min
Response: 0
Conc: N.D.

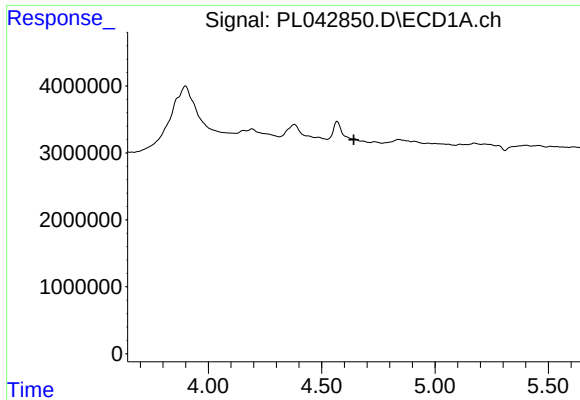

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.641 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

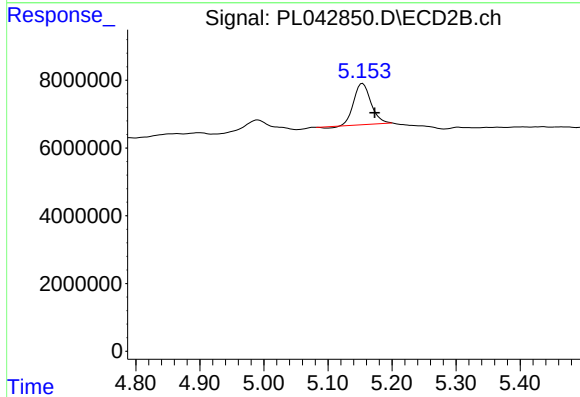


#7 delta-BHC

R.T.: 5.154 min
Delta R.T.: -0.019 min
Response: 22639399
Conc: 5.27 ng/ml

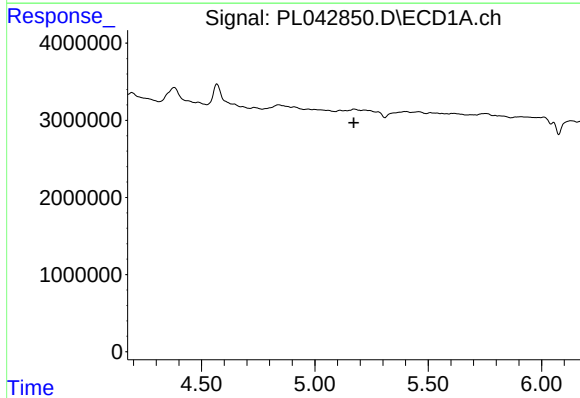


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

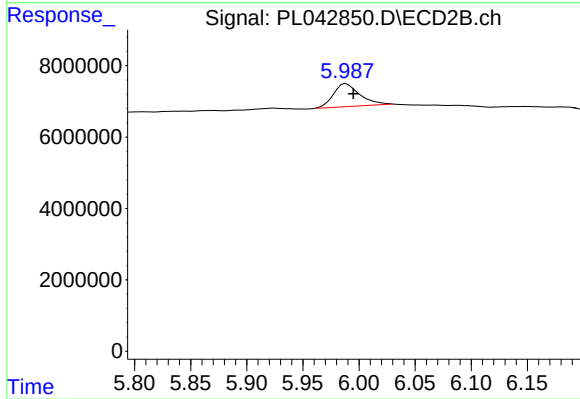

#8 Heptachlor epoxide


R.T.: 5.989 min
Delta R.T.: -0.007 min
Response: 10668731
Conc: 2.81 ng/ml

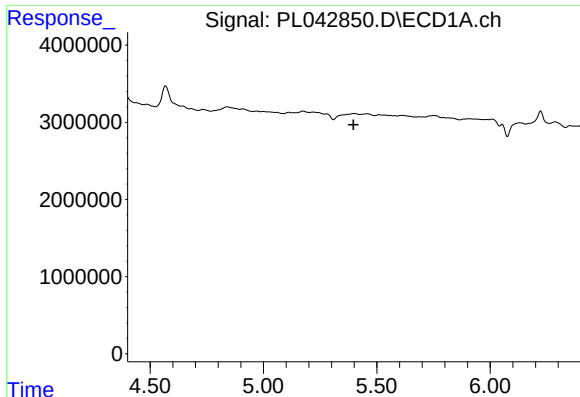

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

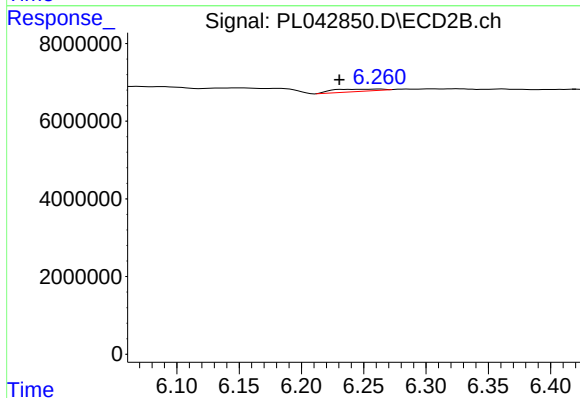


#10 gamma-Chlordane

R.T.: 6.262 min
Delta R.T.: 0.032 min
Response: 1616492
Conc: 0.44 ng/ml

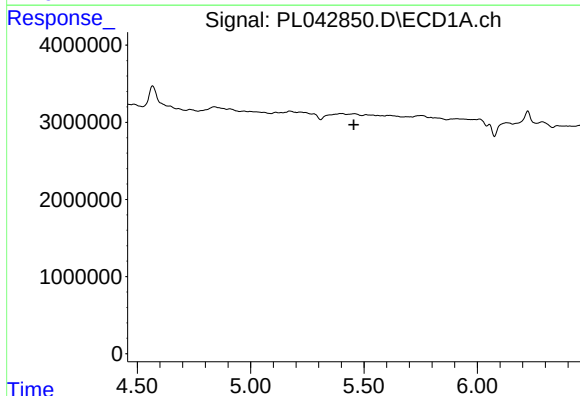


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

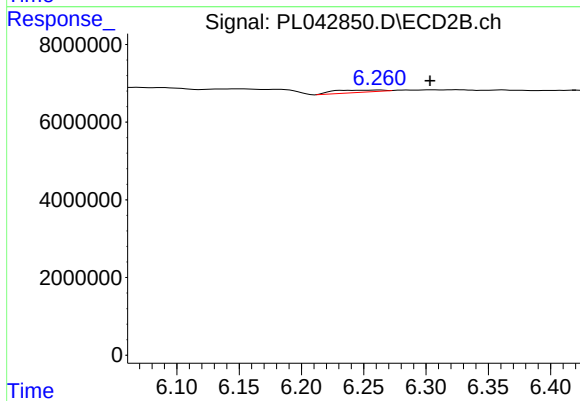

#11 alpha-Chlordane


R.T.: 6.262 min
Delta R.T.: -0.041 min
Response: 1616492
Conc: 0.45 ng/ml

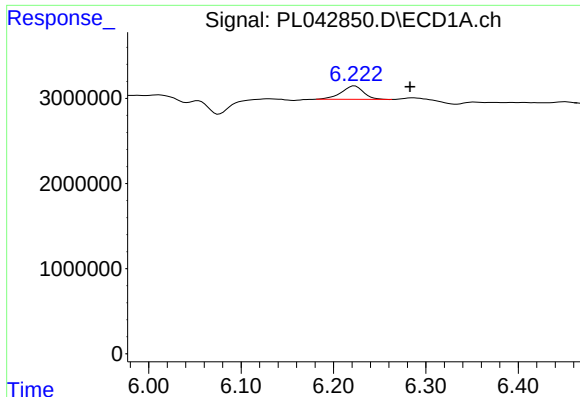

#15 Endosulfan II


R.T.: 6.223 min
Delta R.T.: -0.060 min
Response: 2649968
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

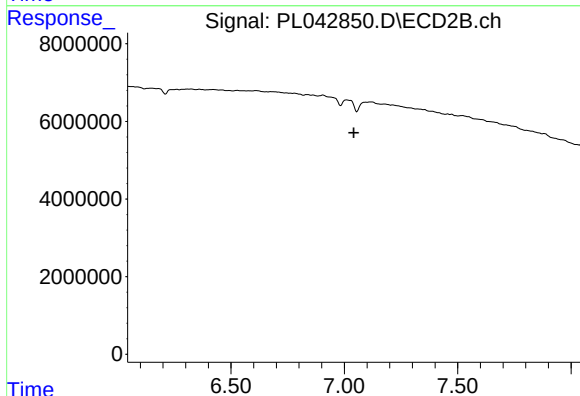


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

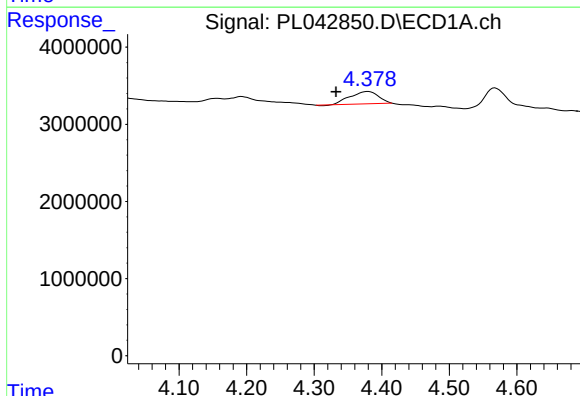


#23 Chlordane-1

R.T.: 4.380 min
Delta R.T.: 0.047 min
Response: 4679801
Conc: 17.42 ng/ml

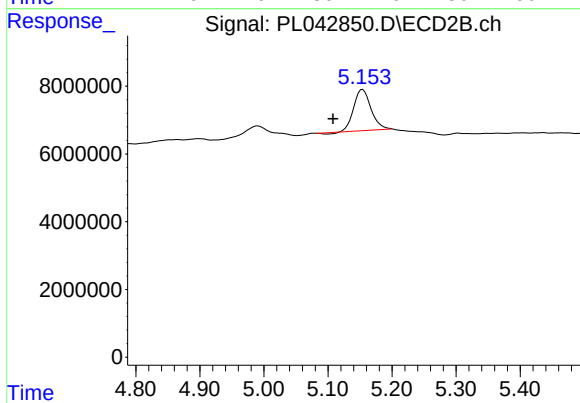

#23 Chlordane-1


R.T.: 5.154 min
Delta R.T.: 0.046 min
Response: 22639399
Conc: 160.18 ng/ml

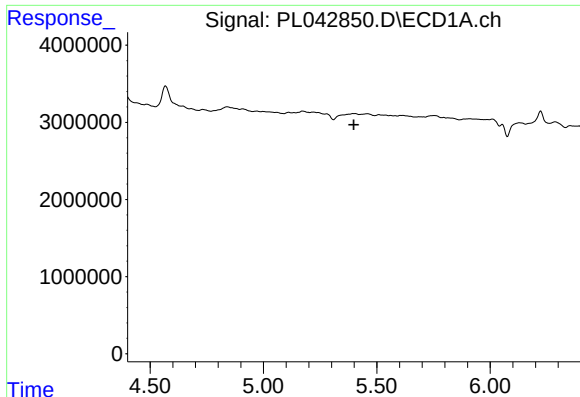

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

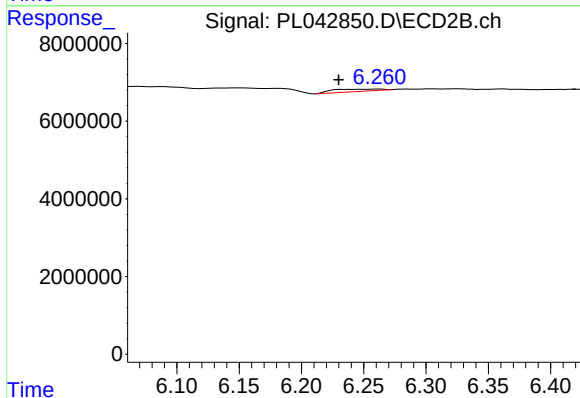


#25 Chlordane-3

R.T.: 6.262 min
Delta R.T.: 0.032 min
Response: 1616492
Conc: 3.29 ng/ml

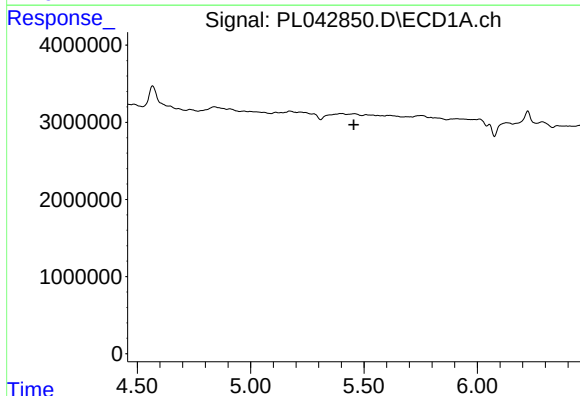


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

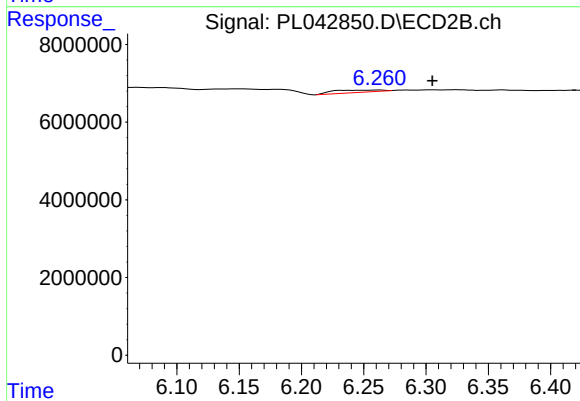

#26 Chlordane-4


R.T.: 6.262 min
Delta R.T.: -0.043 min
Response: 1616492
Conc: 2.83 ng/ml

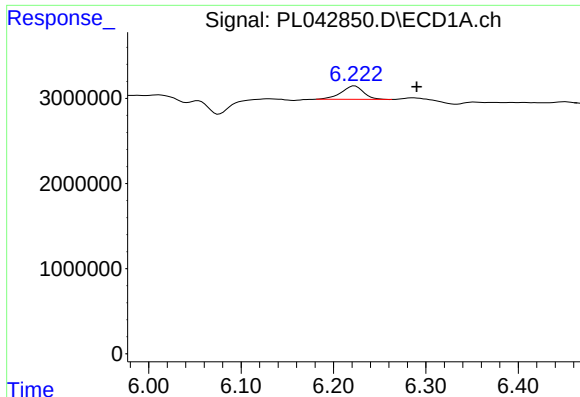

#27 Chlordane-5


R.T.: 6.223 min
Delta R.T.: -0.067 min
Response: 2649968
Conc: 11.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

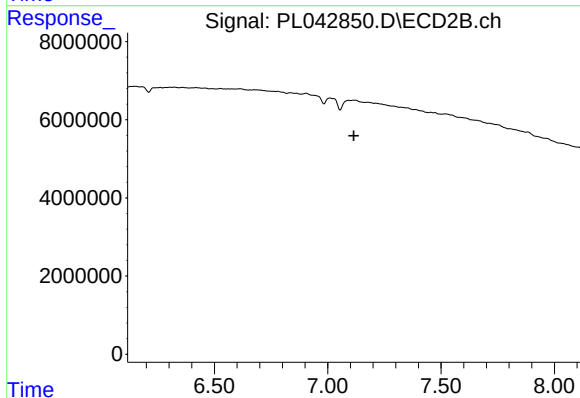


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.115 min
Response: 0
Conc: N.D.

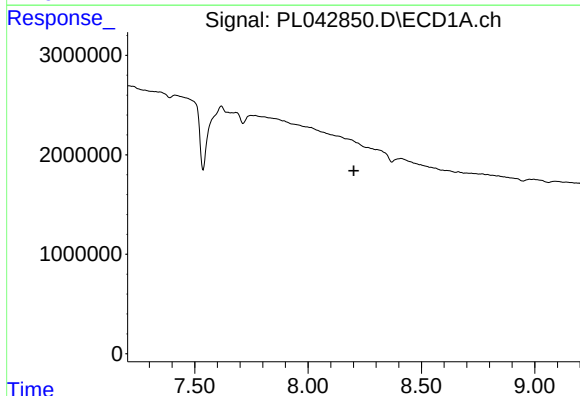

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.201 min
Response: 0
Conc: N.D.

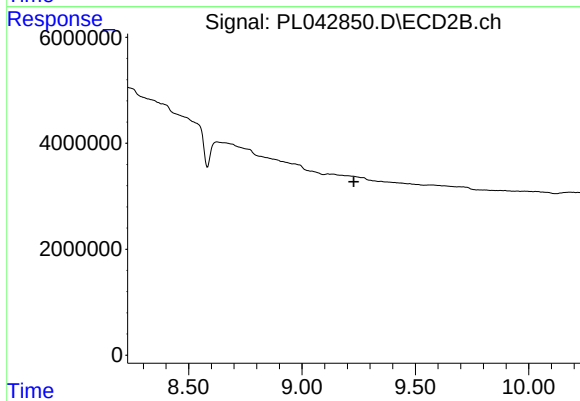

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.228 min
Response: 0
Conc: N.D.