

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120618\
 Data File : PL042859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2018 16:49
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 17:15:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 06 17:15:23 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	303.3E6	140.8E6	50.000	50.000
28)	SA Decachlor...	8.201	9.228	300.4E6	125.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.332	5.108	134.4E6	70666499	500.000	500.000
24)	Chlordane-2	4.832	5.579	143.5E6	71720937	500.000	500.000
25)	Chlordane-3	5.398	6.230	415.5E6	245.5E6	500.000	500.000
26)	Chlordane-4	5.455	6.305	378.0E6	285.4E6	500.000	500.000
27)	Chlordane-5	6.290	7.115	119.9E6	58619530	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120618\
Data File : PL042859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2018 16:49
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 17:15:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Thu Dec 06 17:15:23 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

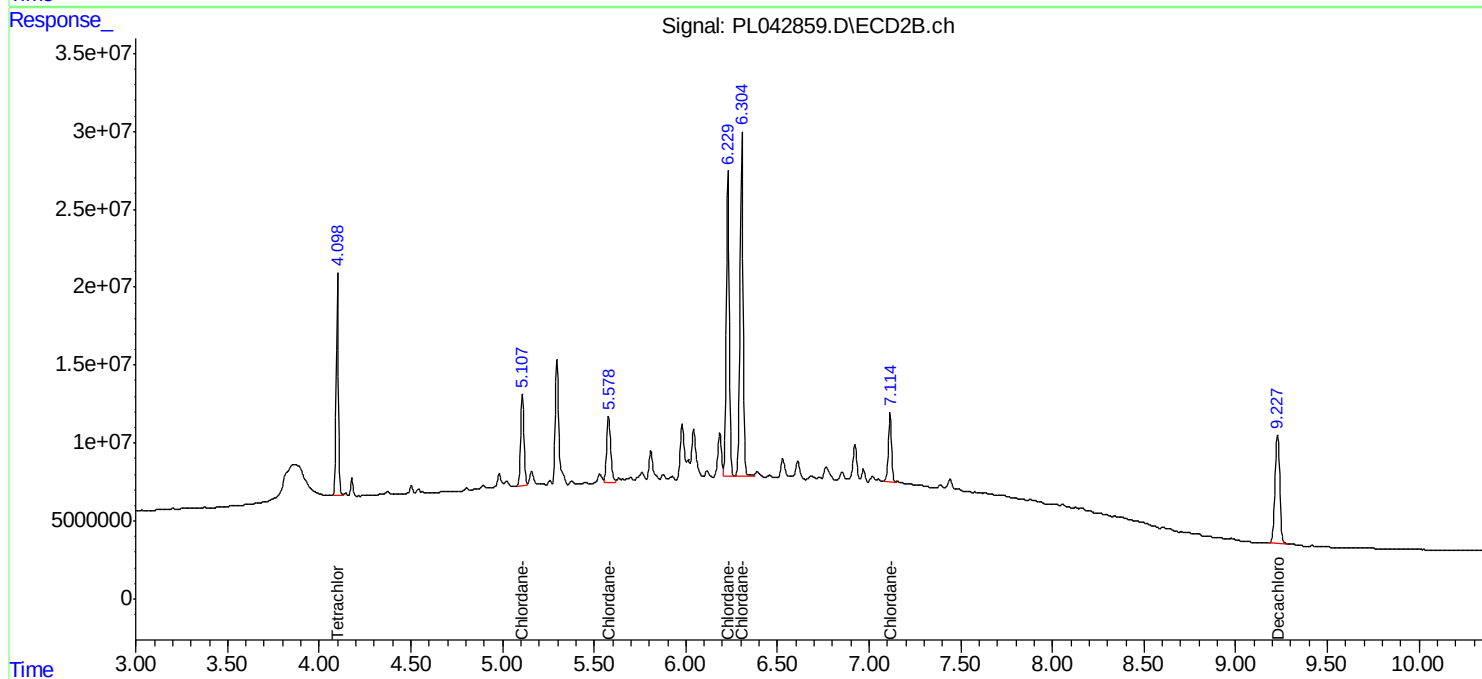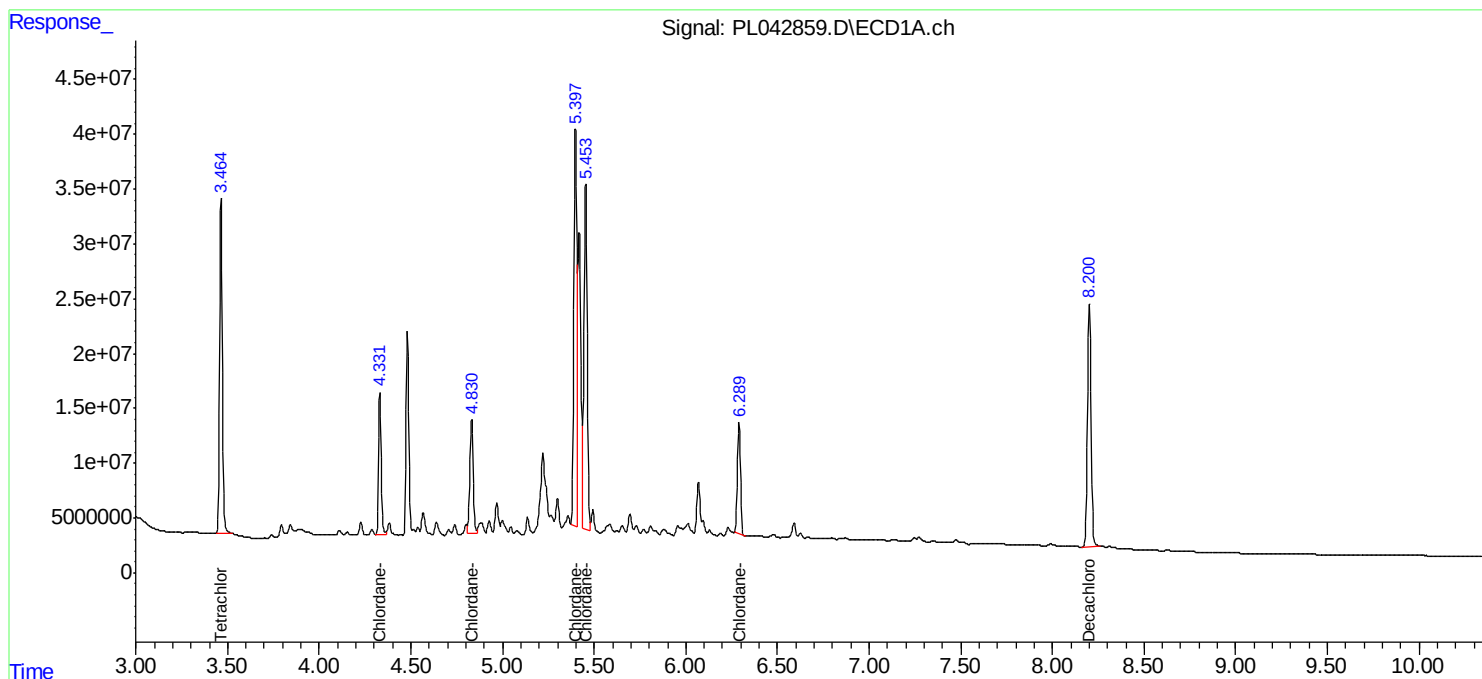


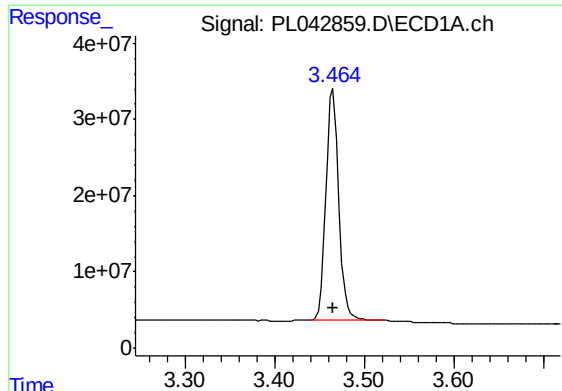

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 303295188
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

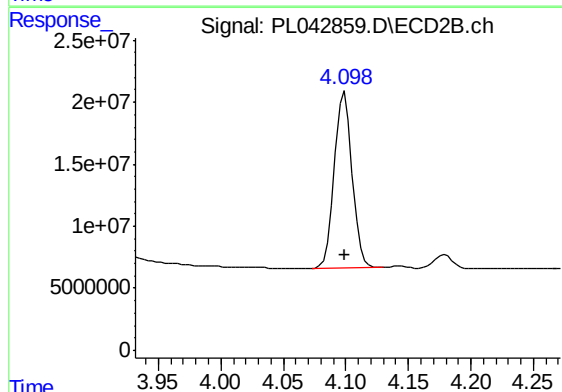


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 140817699
Conc: 50.00 ng/ml

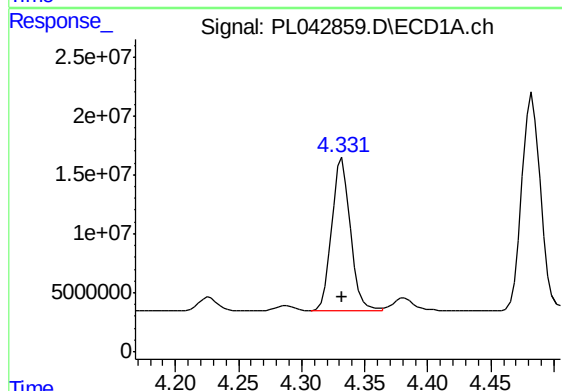


#23 Chlordane-1

R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 134352956
Conc: 500.00 ng/ml

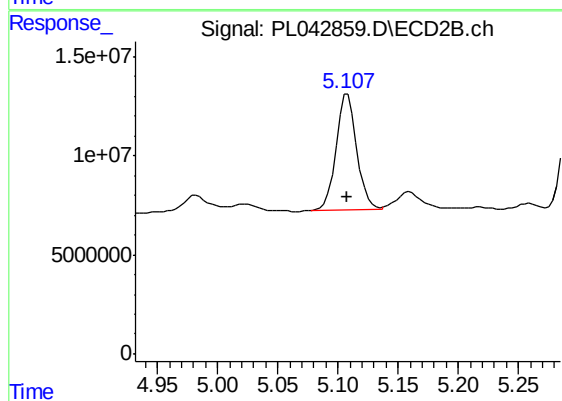

#23 Chlordane-1


R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 70666499
Conc: 500.00 ng/ml

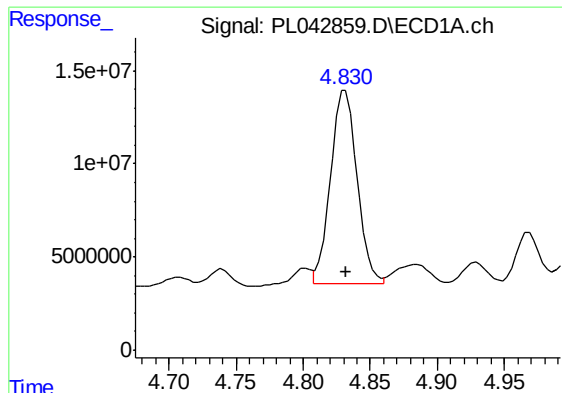

#24 Chlordane-2


R.T.: 4.832 min
Delta R.T.: 0.000 min
Response: 143513644
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

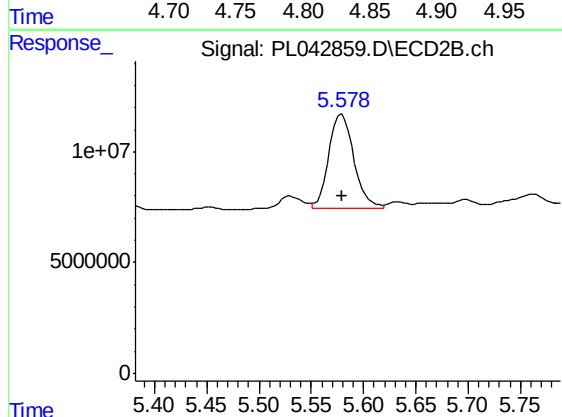


#24 Chlordane-2

R.T.: 5.579 min
Delta R.T.: 0.000 min
Response: 71720937
Conc: 500.00 ng/ml

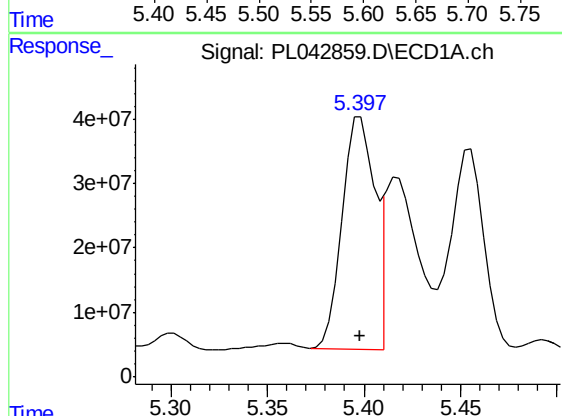


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 415520771
Conc: 500.00 ng/ml

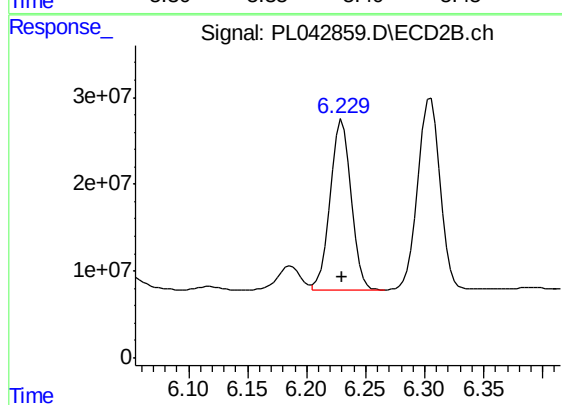

#25 Chlordane-3


R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 245537019
Conc: 500.00 ng/ml

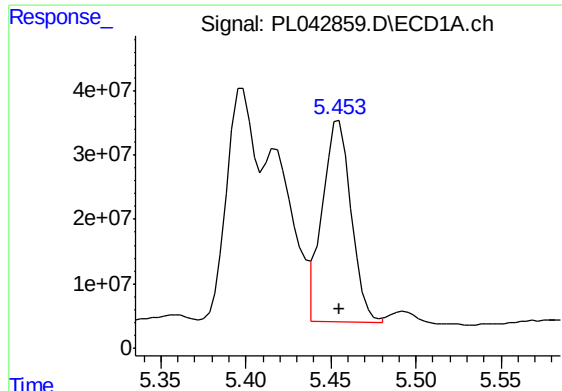

#26 Chlordane-4


R.T.: 5.455 min
Delta R.T.: 0.000 min
Response: 378049121
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

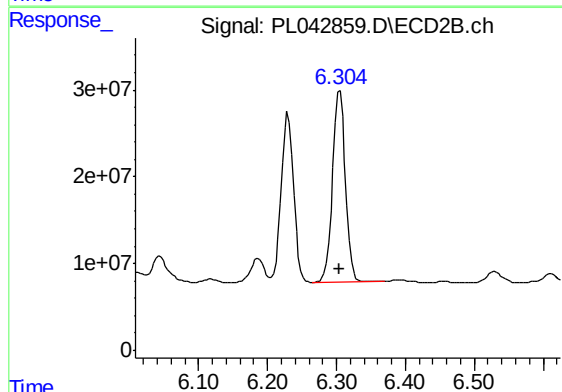


#26 Chlordane-4

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 285374669
Conc: 500.00 ng/ml

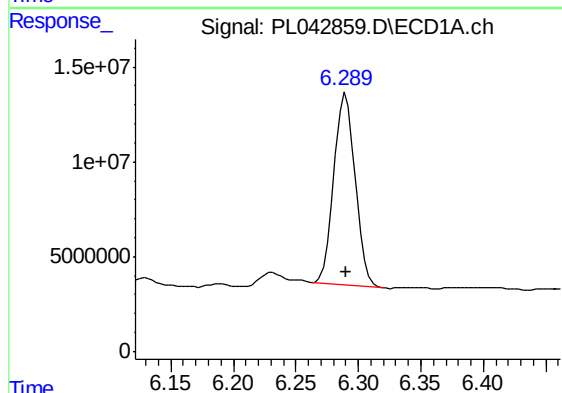


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 119927482
Conc: 500.00 ng/ml

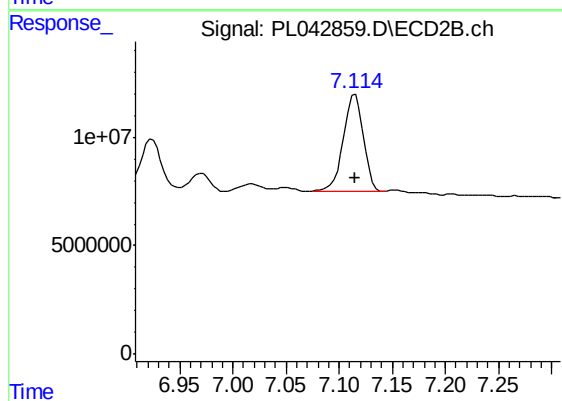

#27 Chlordane-5


R.T.: 7.115 min
Delta R.T.: 0.000 min
Response: 58619530
Conc: 500.00 ng/ml

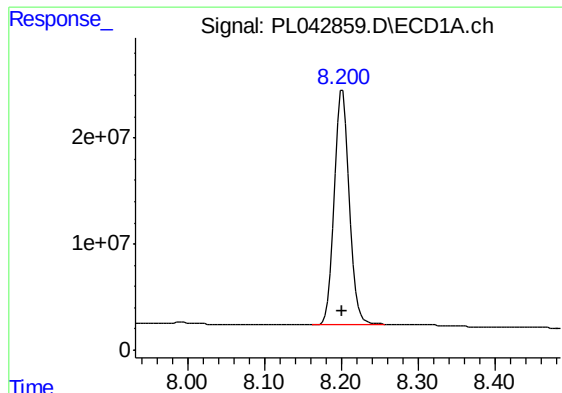

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 300411328
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

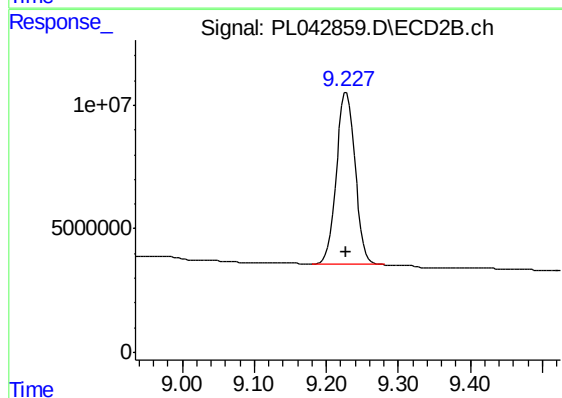

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 125282108
Conc: 50.00 ng/ml