

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120619\
 Data File : PL054830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 14:55
 Operator : SG\AJ
 Sample : PB125294BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB125294BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:06:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	4.051	226.1E6	54377520	19.438	21.309
28)	SA Decachlor...	8.322	9.153	173.4E6	46844521	18.111	19.539
Target Compounds							
15)	B Endosulfa...	0.000	6.982	0	2393267	N.D.	1.018 #
23)	Chlordane-1	4.448f	0.000	6325217	0	16.028	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120619\
Data File : PL054830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 14:55
Operator : SG\AJ
Sample : PB125294BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB125294BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:06:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

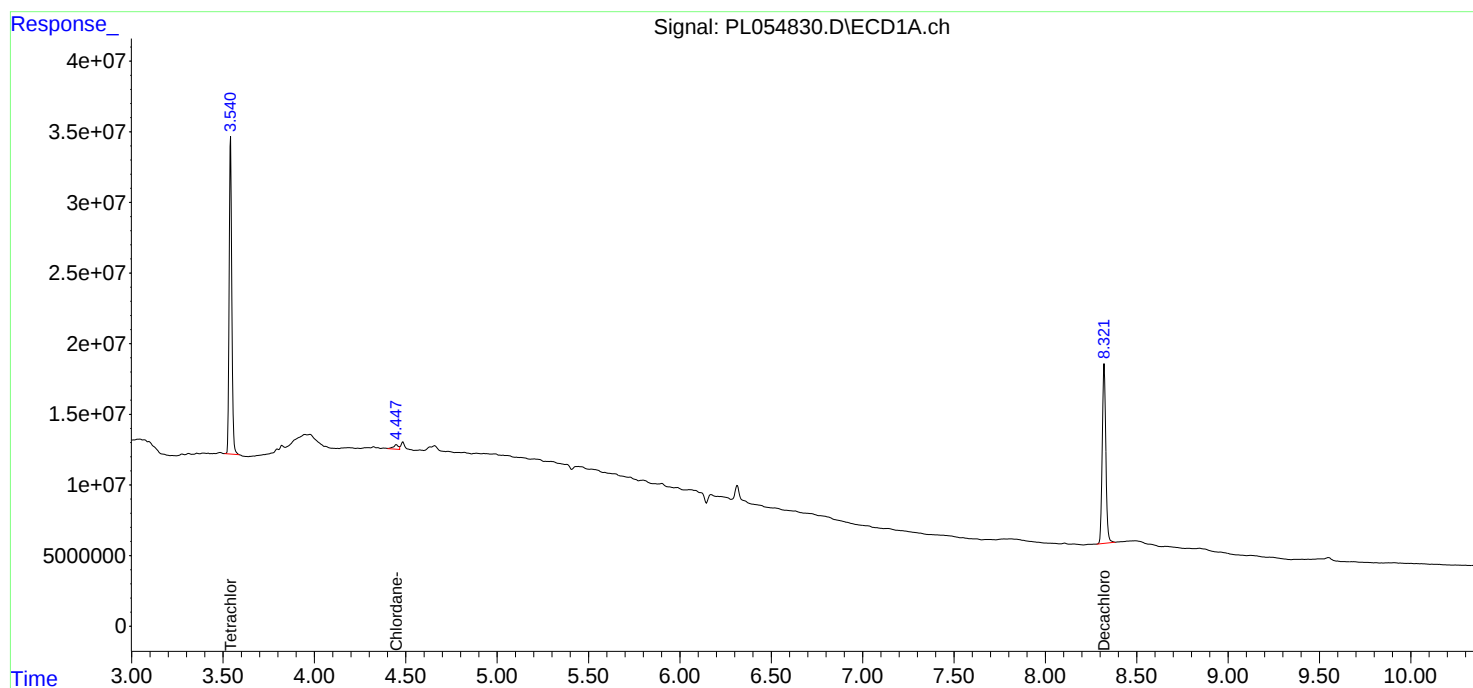


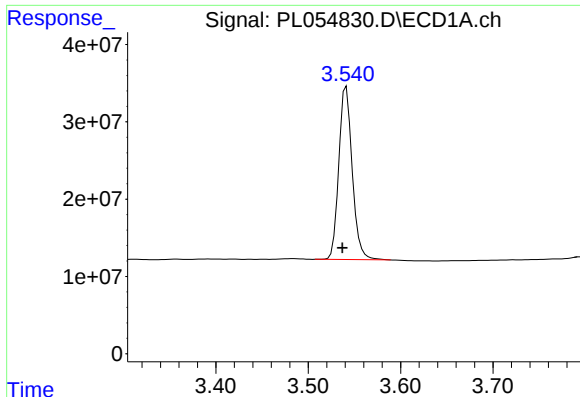

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.004 min
Response: 226145004
Conc: 19.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB125294BL

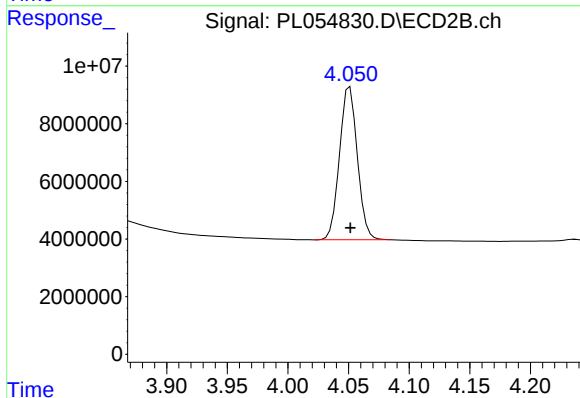


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 54377520
Conc: 21.31 ng/ml

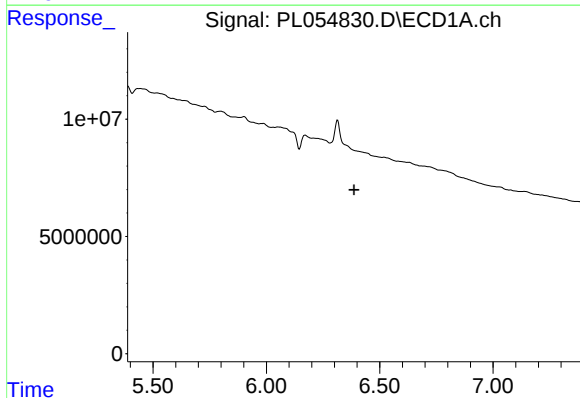


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.388 min
Response: 0
Conc: N.D.

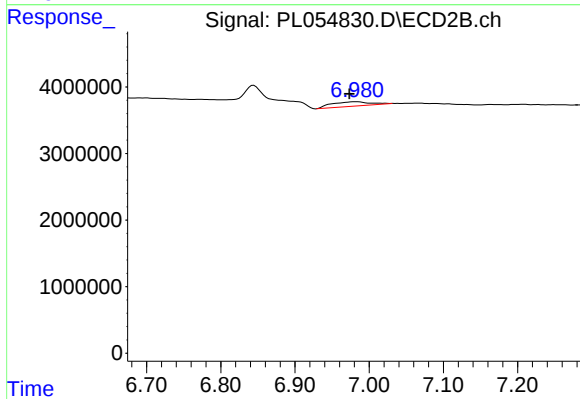

#15 Endosulfan II


R.T.: 6.982 min
Delta R.T.: 0.008 min
Response: 2393267
Conc: 1.02 ng/ml

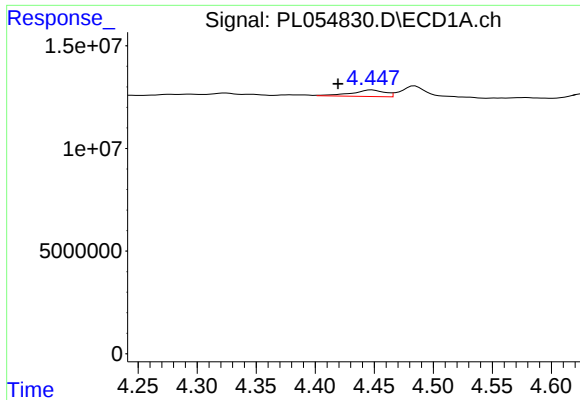

#23 Chlordane-1


R.T.: 4.448 min
Delta R.T.: 0.029 min
Response: 6325217
Conc: 16.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB125294BL

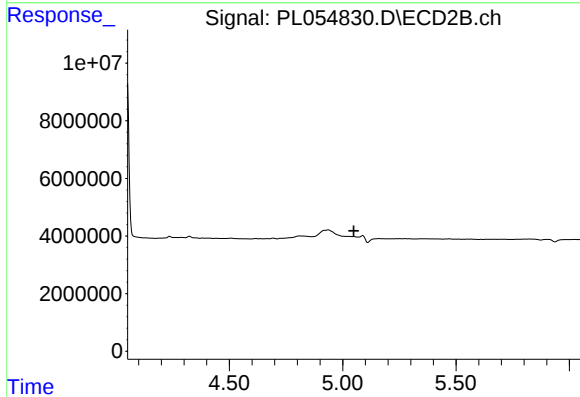


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.049 min
Response: 0
Conc: N.D.

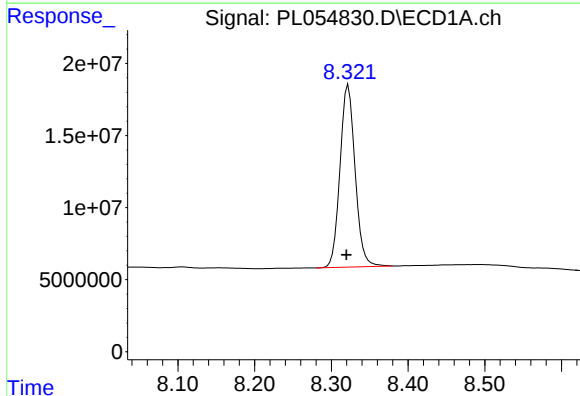

#28 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: 0.002 min
Response: 173431899
Conc: 18.11 ng/ml

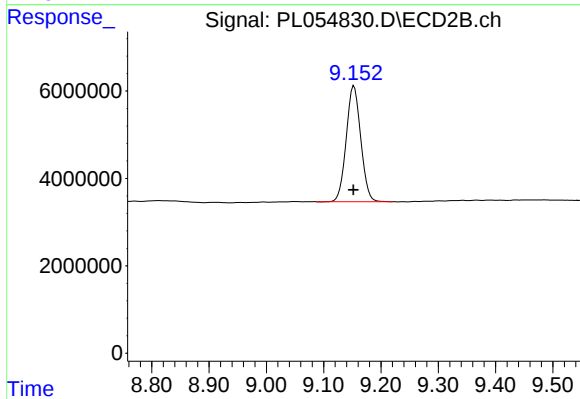

#28 Decachlorobiphenyl

R.T.: 9.153 min
Delta R.T.: 0.001 min
Response: 46844521
Conc: 19.54 ng/ml