

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120619\
 Data File : PL054841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 17:32
 Operator : SG\AJ
 Sample : K6147-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P001-WC003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:08:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.050	221.7E6	56744478	19.052	22.237
28)	SA Decachlor...	8.318	9.150	178.4E6	49252564	18.630	20.544
Target Compounds							
2)	A alpha-BHC	4.008f	0.000	51833890	0	2.730	N.D. #
3)	MA gamma-BHC...	4.296f	0.000	3389238	0	0.199	N.D. #
6)	B beta-BHC	4.492f	0.000	38130279	0	5.141	N.D. #
7)	B delta-BHC	0.000	5.089f	0	7519327	N.D.	2.820 #
9)	A Endosulfan I	5.624	0.000	31278920	0	2.294	N.D. #
12)	B 4,4'-DDE	5.718	6.372f	7908575	1637661	0.594	0.662
19)	B Endosulfa...	0.000	7.348f	0	2401583	N.D.	1.133 #
20)	A Methoxychlor	7.019	0.000	52556352	0	10.487	N.D. #
23)	Chlordane-1	4.449f	0.000	4945826	0	12.533	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120619\
Data File : PL054841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 17:32
Operator : SG\AJ
Sample : K6147-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
P001-WC003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:08:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

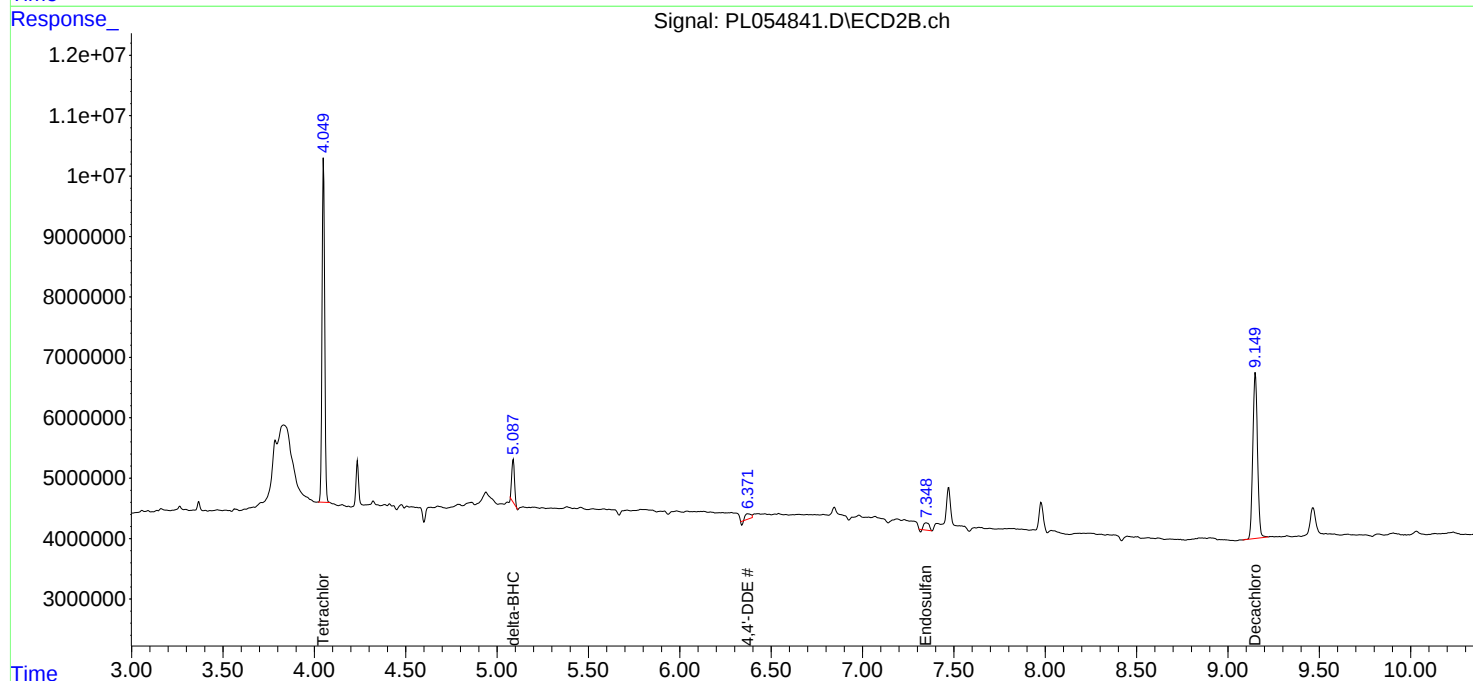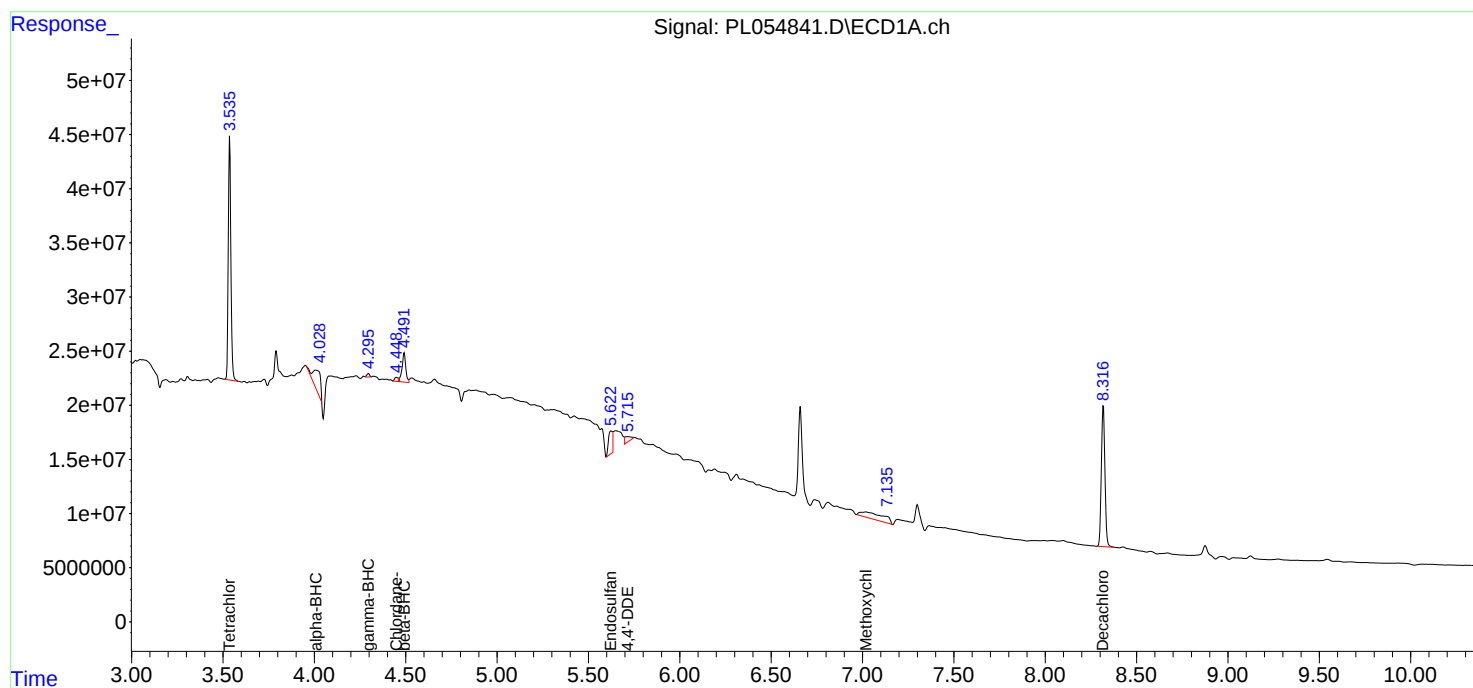


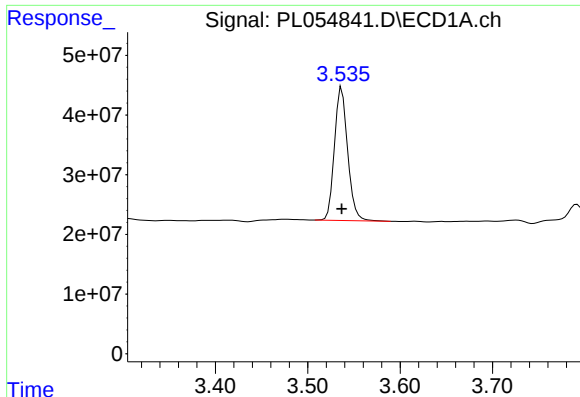

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 221652390
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-WC003

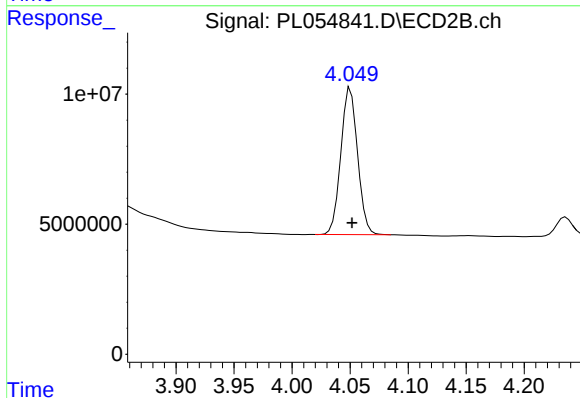


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 56744478
Conc: 22.24 ng/ml

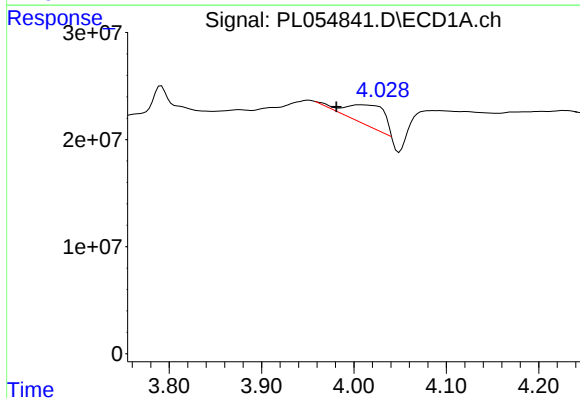


#2 alpha-BHC

R.T.: 4.008 min
Delta R.T.: 0.027 min
Response: 51833890
Conc: 2.73 ng/ml

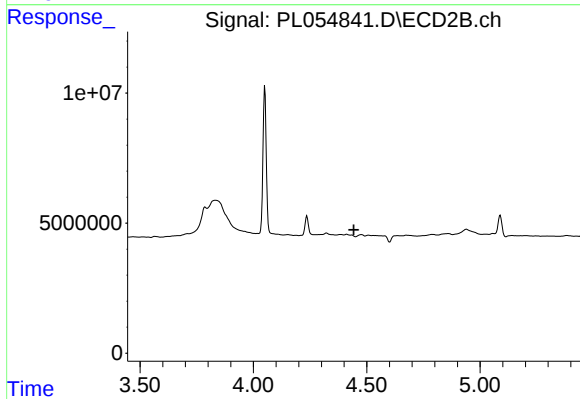

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.443 min
Response: 0
Conc: N.D.

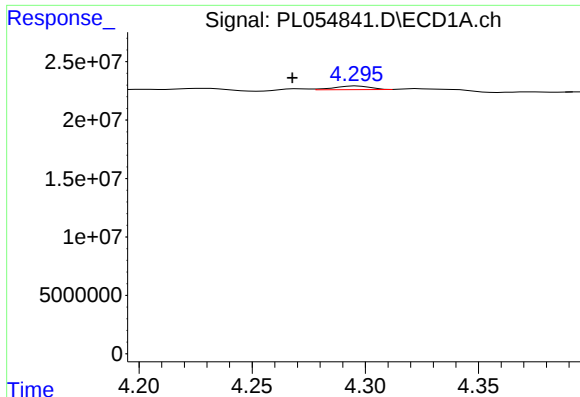

#3 gamma-BHC (Lindane)


R.T.: 4.296 min
Delta R.T.: 0.029 min
Response: 3389238
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-WC003

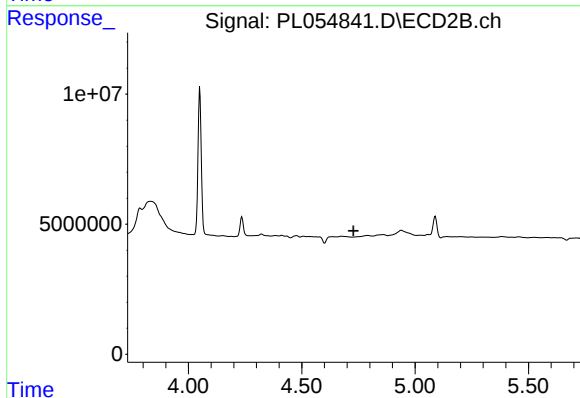


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.729 min
Response: 0
Conc: N.D.

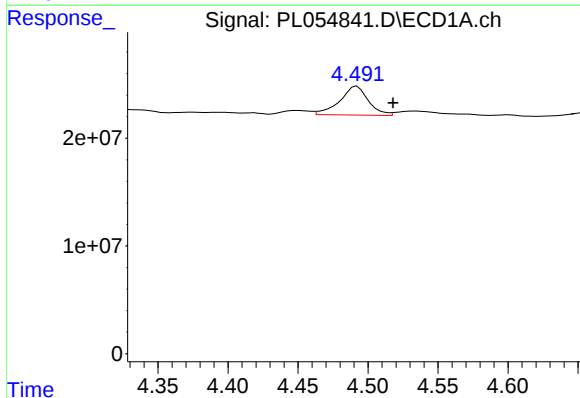


#6 beta-BHC

R.T.: 4.492 min
Delta R.T.: -0.026 min
Response: 38130279
Conc: 5.14 ng/ml

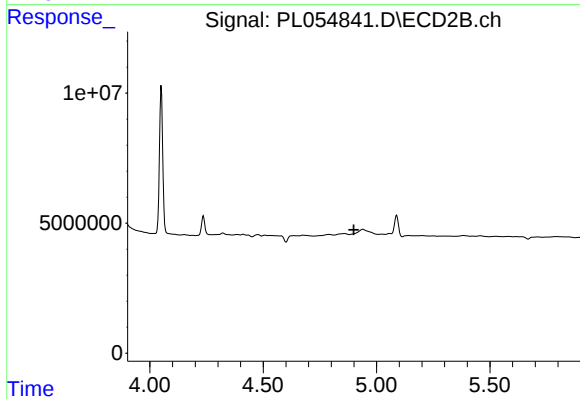

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.899 min
Response: 0
Conc: N.D.

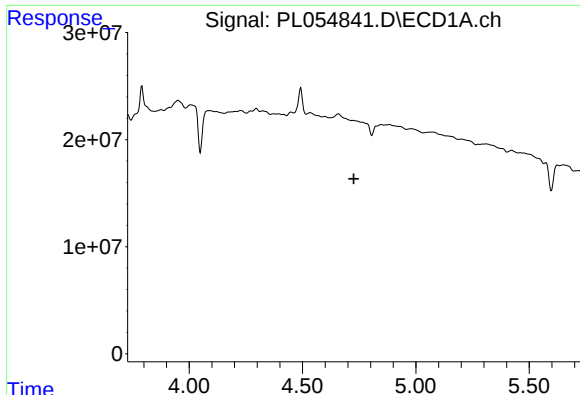

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
P001-WC003

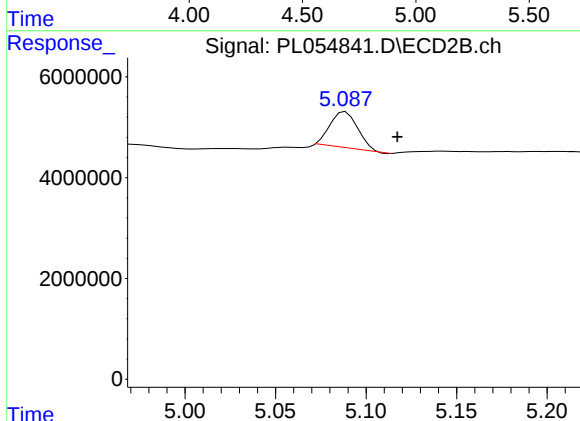


#7 delta-BHC

R.T.: 5.089 min
Delta R.T.: -0.029 min
Response: 7519327
Conc: 2.82 ng/ml

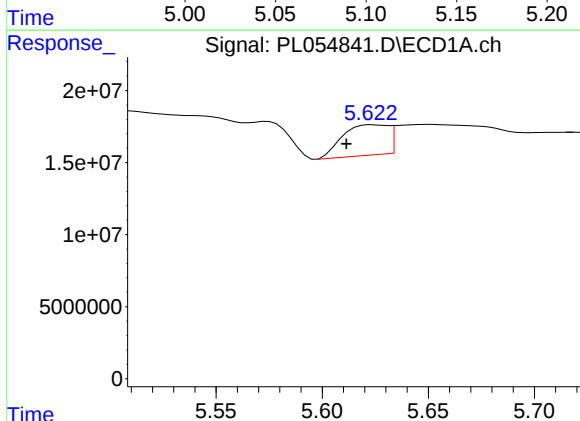


#9 Endosulfan I

R.T.: 5.624 min
Delta R.T.: 0.012 min
Response: 31278920
Conc: 2.29 ng/ml

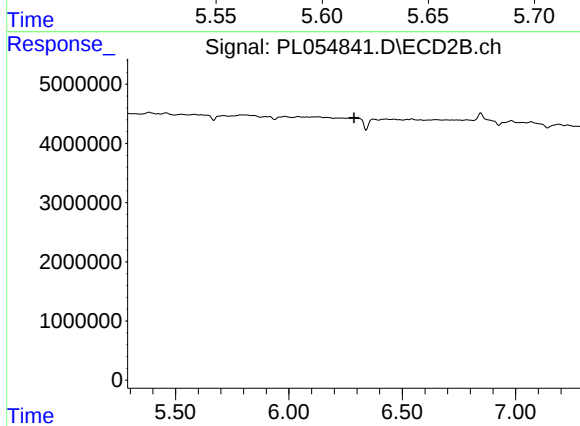

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.288 min
Response: 0
Conc: N.D.

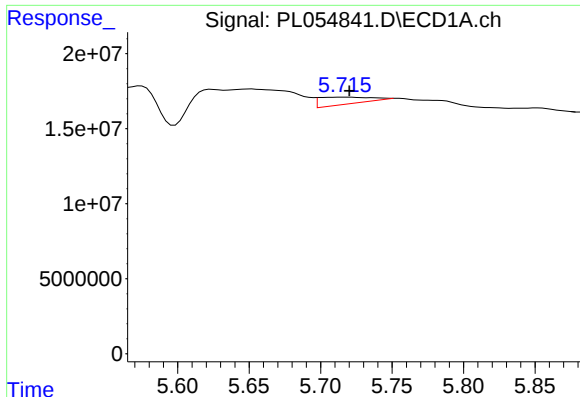

#12 4,4'-DDE


R.T.: 5.718 min
Delta R.T.: -0.003 min
Response: 7908575
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-WC003

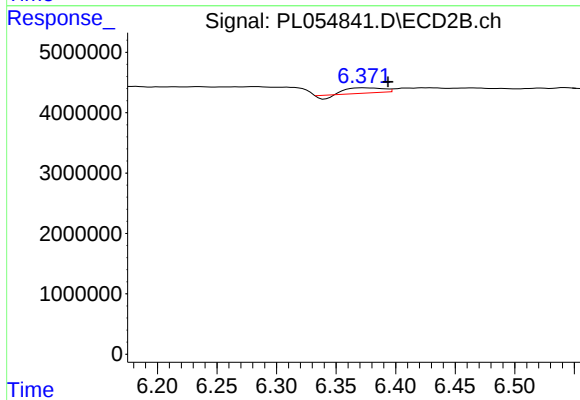


#12 4,4'-DDE

R.T.: 6.372 min
Delta R.T.: -0.022 min
Response: 1637661
Conc: 0.66 ng/ml

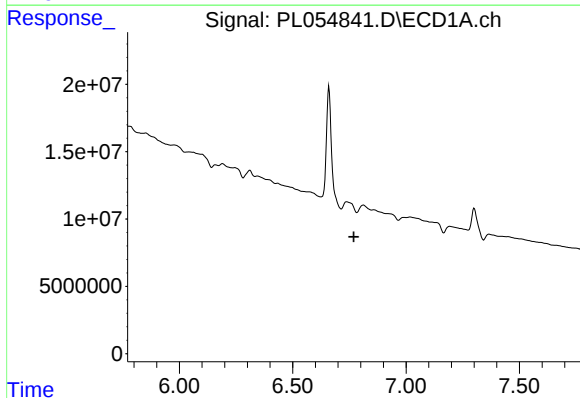


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

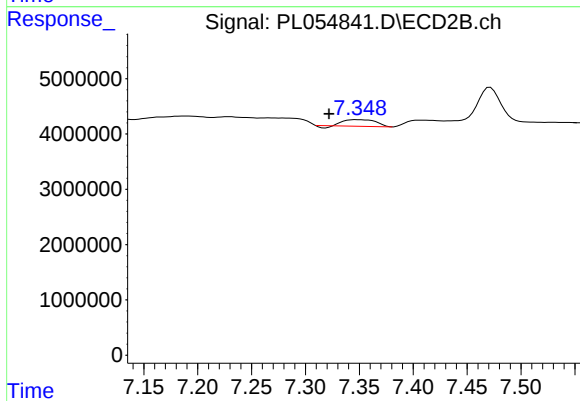

#19 Endosulfan Sulfate


R.T.: 7.348 min
Delta R.T.: 0.026 min
Response: 2401583
Conc: 1.13 ng/ml

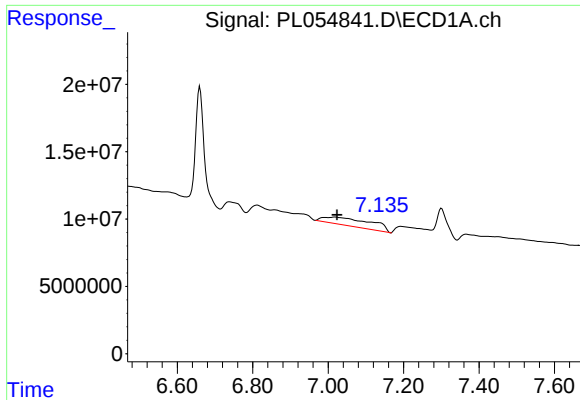

#20 Methoxychlor


R.T.: 7.019 min
Delta R.T.: -0.005 min
Response: 52556352
Conc: 10.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-WC003

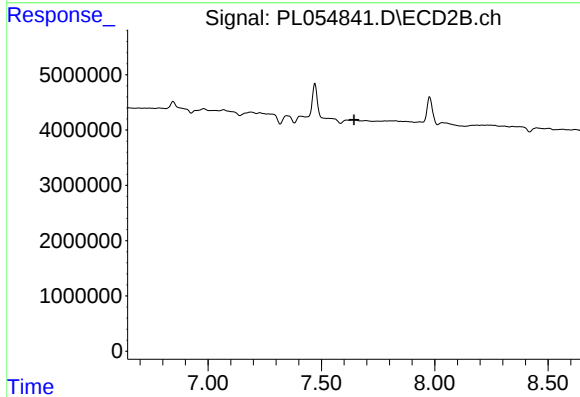


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

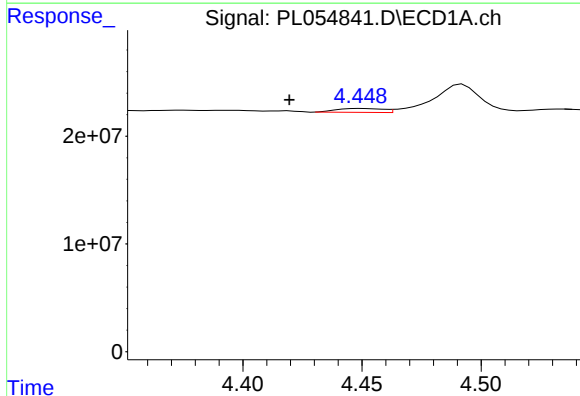


#23 Chlordane-1

R.T.: 4.449 min
Delta R.T.: 0.030 min
Response: 4945826
Conc: 12.53 ng/ml

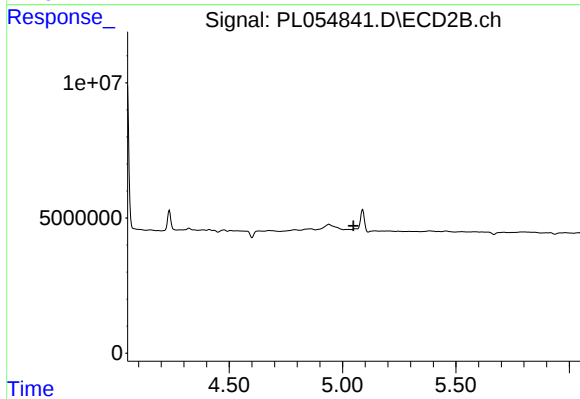

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

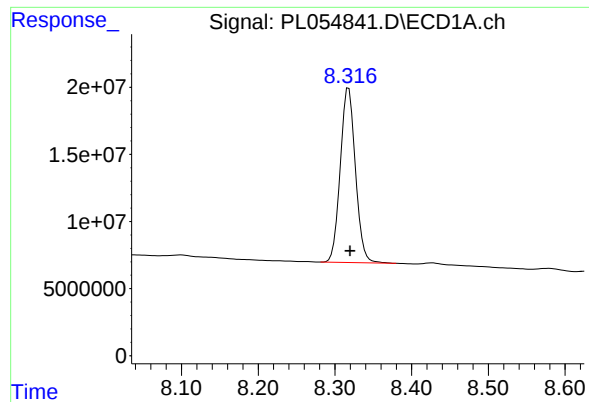

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.002 min
Response: 178405208
Conc: 18.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-WC003

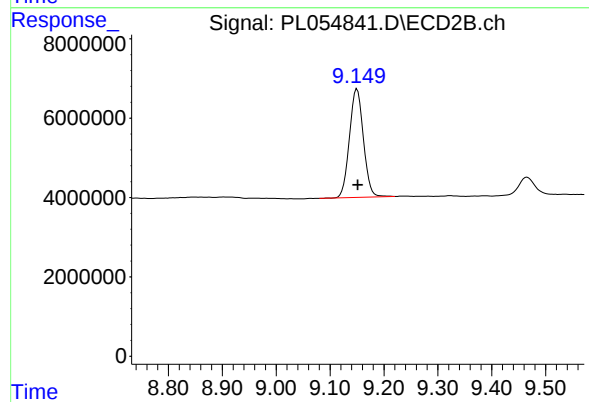

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: -0.002 min
Response: 49252564
Conc: 20.54 ng/ml