

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120619\
 Data File : PL054822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 12:42
 Operator : SG\AJ
 Sample : K6113-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-120519

Manual Integrations
 APPROVED

Ankita
 12/9/2019 10:40:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:04:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	4.050	170.9E6	35570776	14.689	13.939
28) SA Decachlor...	8.318	9.150	103.7E6	28710947	10.833	11.976
Target Compounds						
10) B gamma-Chl...	5.496	6.163	11150849	3189953	0.735m	1.211m#
11) B alpha-Chl...	5.554	6.236	17107875	6756548	1.160m	2.573m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120619\
Data File : PL054822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 12:42
Operator : SG\AJ
Sample : K6113-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-120519


Manual Integrations
APPROVED

Ankita
12/9/2019 10:40:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:04:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

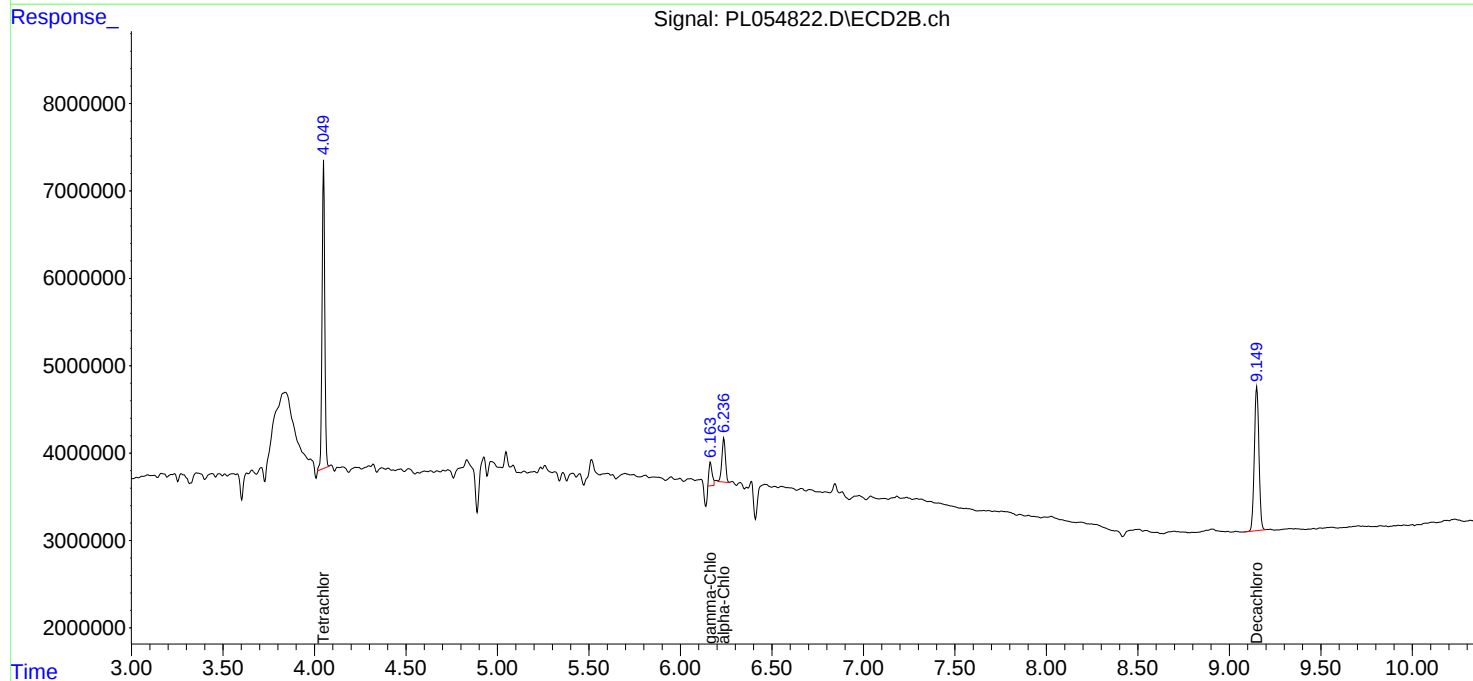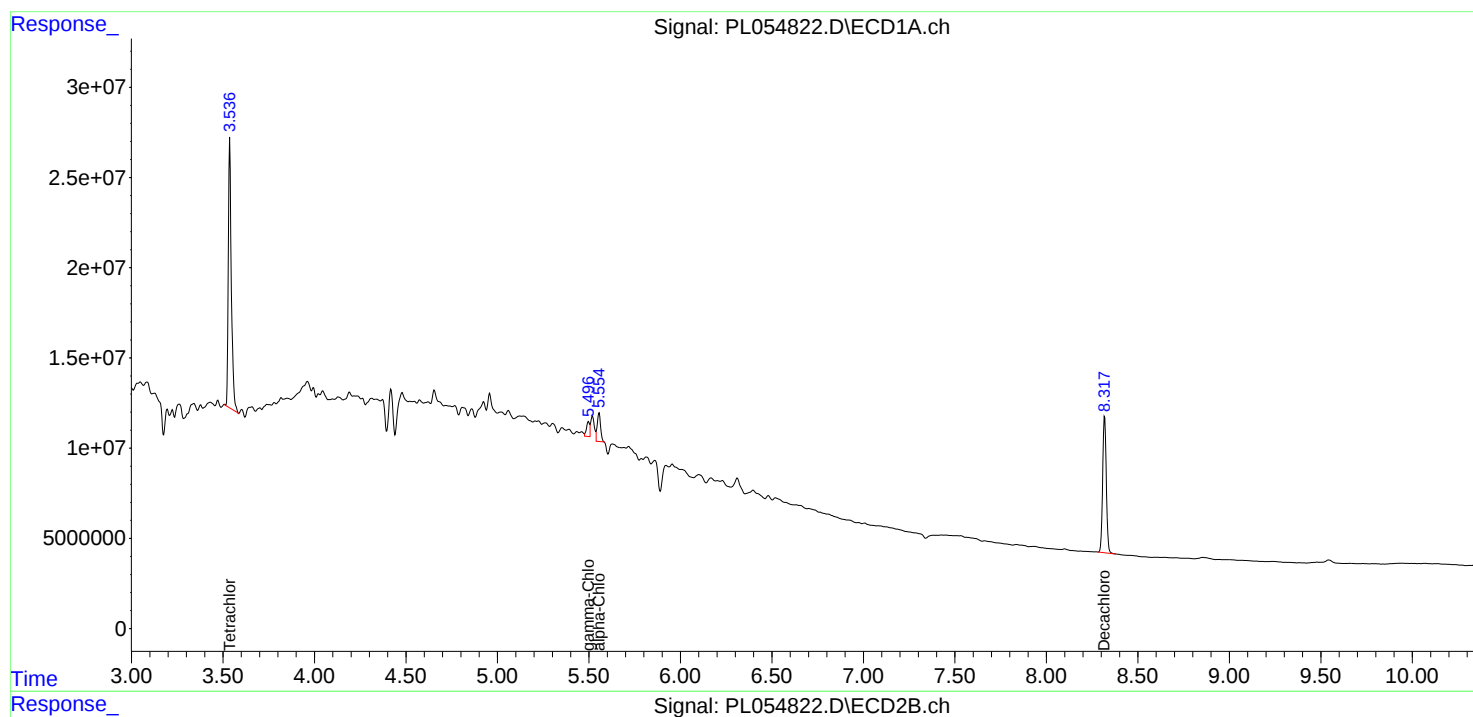

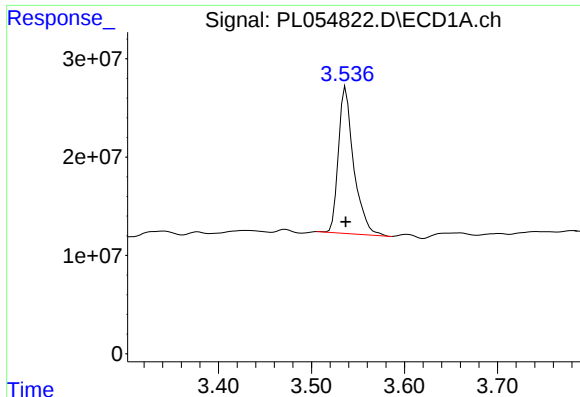


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 170894439
Conc: 14.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-120519


Manual Integrations
APPROVED

Ankita
12/9/2019 10:40:19 AM

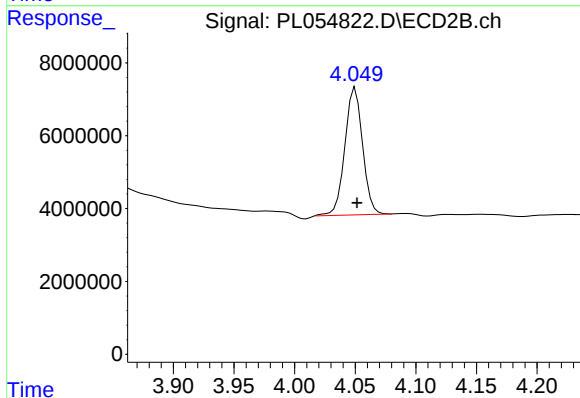


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 35570776
Conc: 13.94 ng/ml

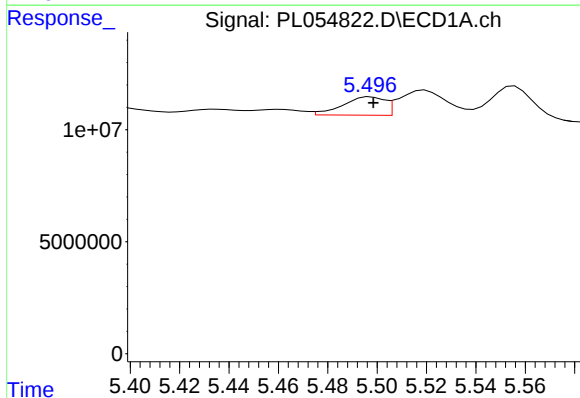


#10 gamma-Chlordane

R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 11150849
Conc: 0.74 ng/ml m

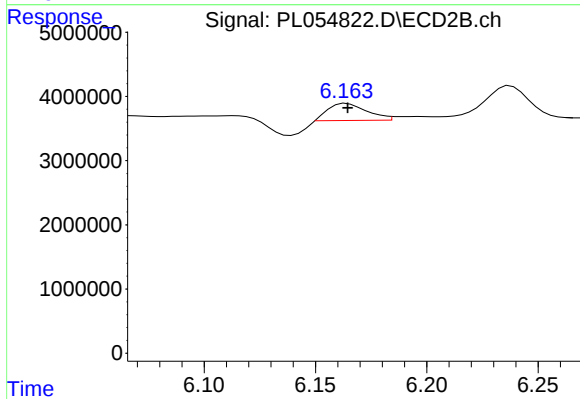

#10 gamma-Chlordane

R.T.: 6.163 min
Delta R.T.: -0.002 min
Response: 3189953
Conc: 1.21 ng/ml m

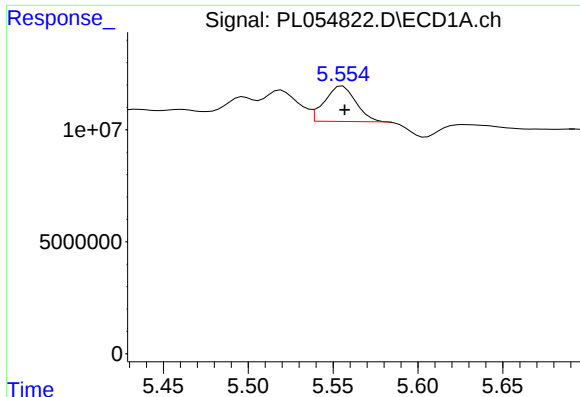


#11 alpha-Chlordane

R.T.: 5.554 min
Delta R.T.: -0.002 min
Response: 17107875
Conc: 1.16 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-03-120519


Manual Integrations
APPROVED

Ankita
12/9/2019 10:40:19 AM

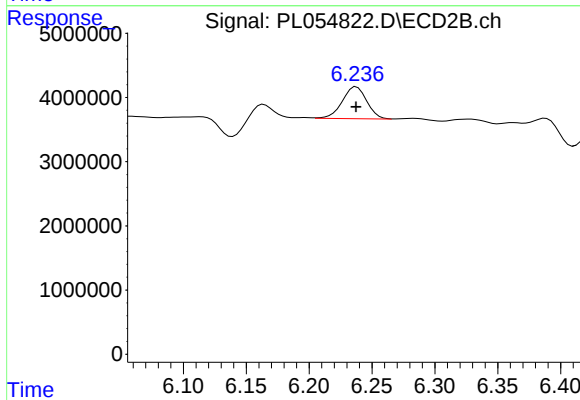


#11 alpha-Chlordane

R.T.: 6.236 min
Delta R.T.: -0.001 min
Response: 6756548
Conc: 2.57 ng/ml m

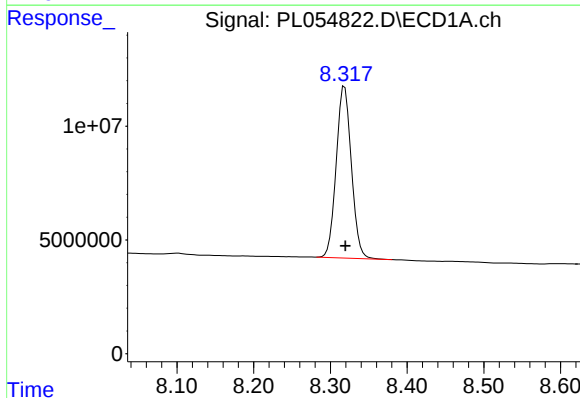

#28 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.001 min
Response: 103738364
Conc: 10.83 ng/ml

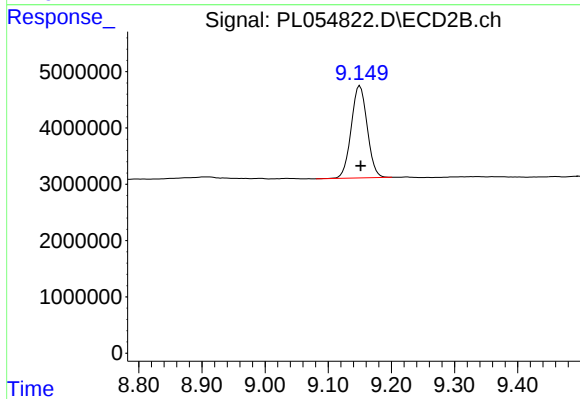

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: -0.001 min
Response: 28710947
Conc: 11.98 ng/ml