

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120621\
 Data File : PL071283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2021 08:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:09:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	7.011	0.000	2581579	0	4.142	N.D. #
10) B	gamma-Chl...	7.268	0.000	148672	0	0.234	N.D. #
20) A	Methoxychlor	9.000	0.000	801857	0	2.219	N.D. #
21) B	Endrin ke...	9.217	0.000	835040	0	1.172	N.D. #
22)	Mirex	0.000	10.451	0	4134559	N.D.	3.791 #
25)	Chlordane-3	7.268	0.000	148672	0	2.397	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120621\
Data File : PL071283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2021 08:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:09:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

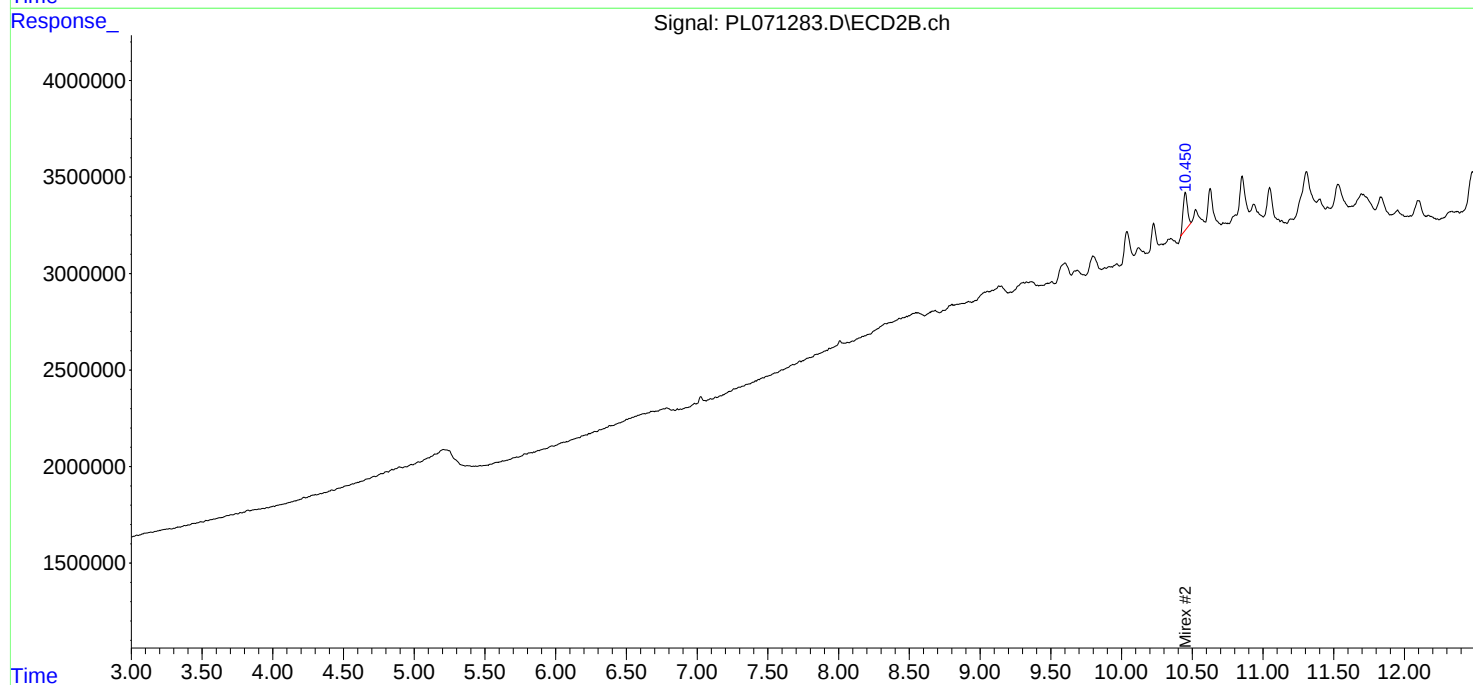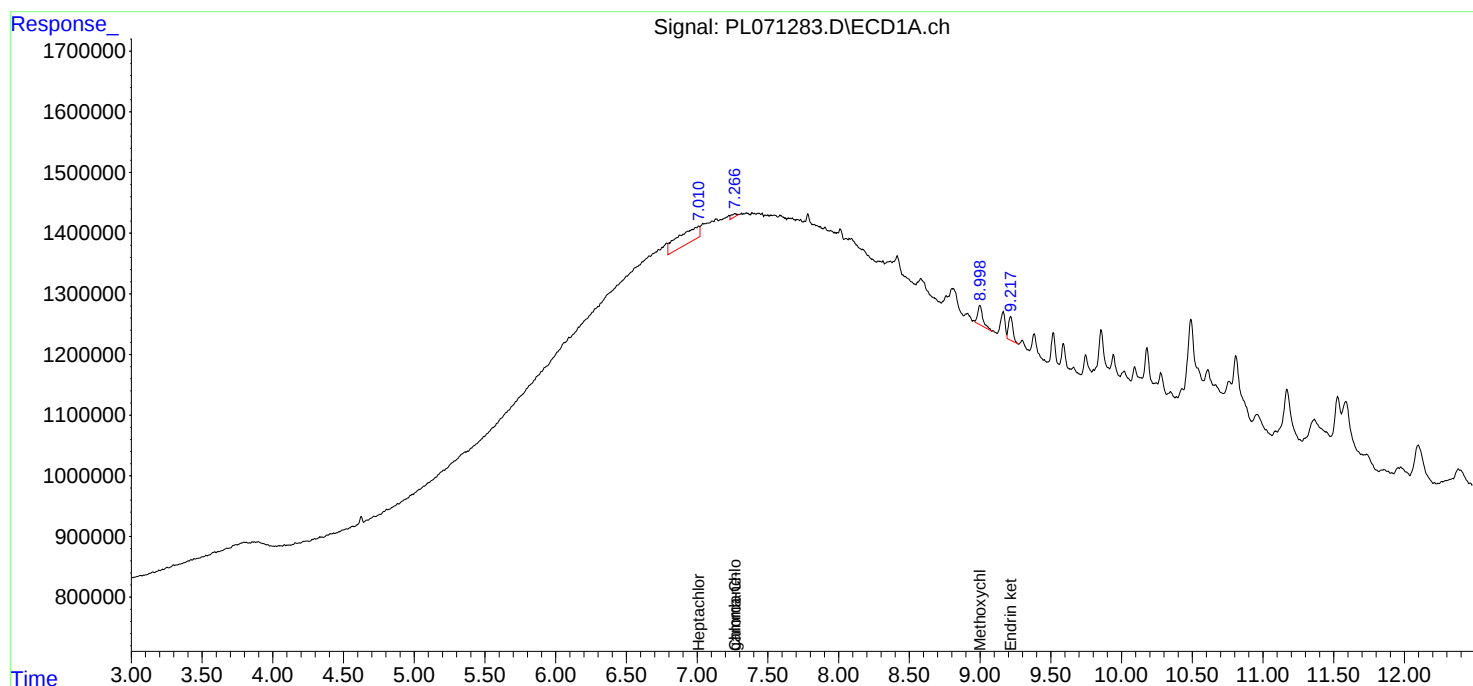


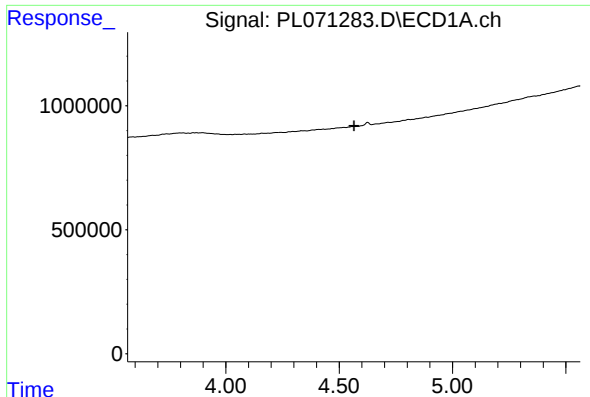

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

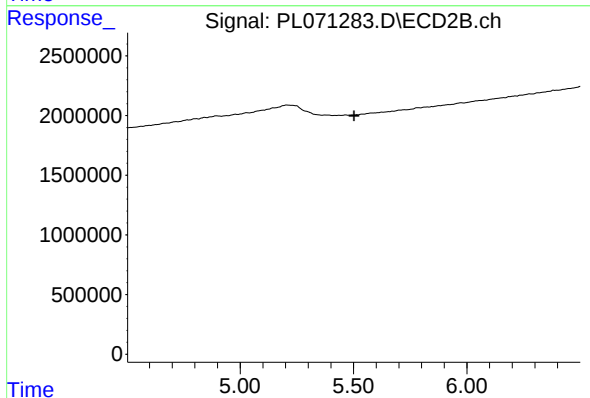


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

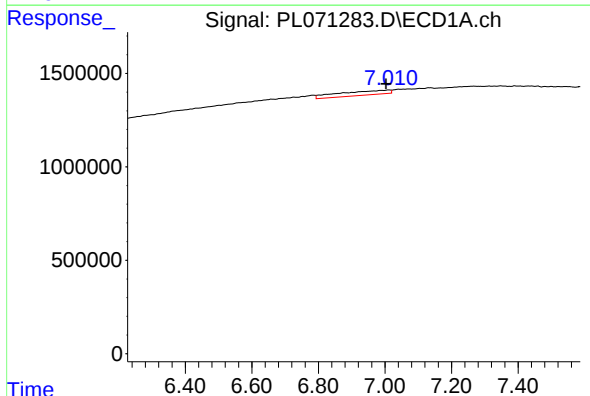


#8 Heptachlor epoxide

R.T.: 7.011 min
Delta R.T.: 0.008 min
Response: 2581579
Conc: 4.14 ng/ml

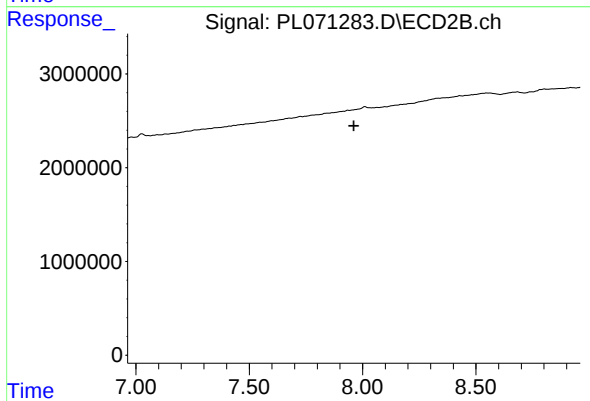

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.961 min
Response: 0
Conc: N.D.

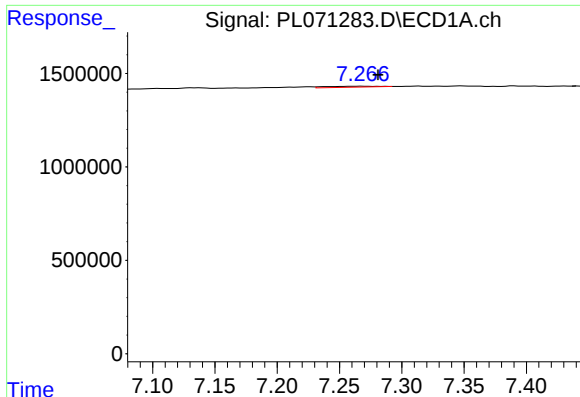

#10 gamma-Chlordane


R.T.: 7.268 min
Delta R.T.: -0.013 min
Response: 148672
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

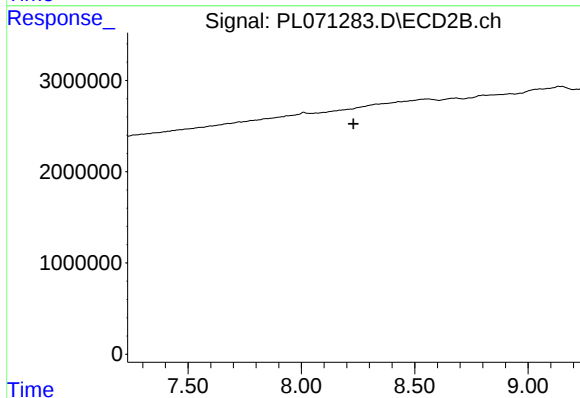


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

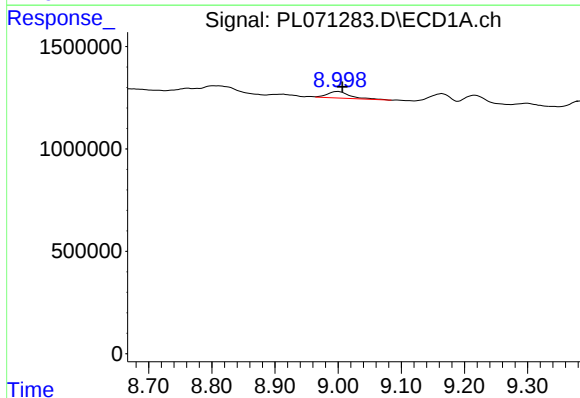


#20 Methoxychlor

R.T.: 9.000 min
Delta R.T.: -0.007 min
Response: 801857
Conc: 2.22 ng/ml

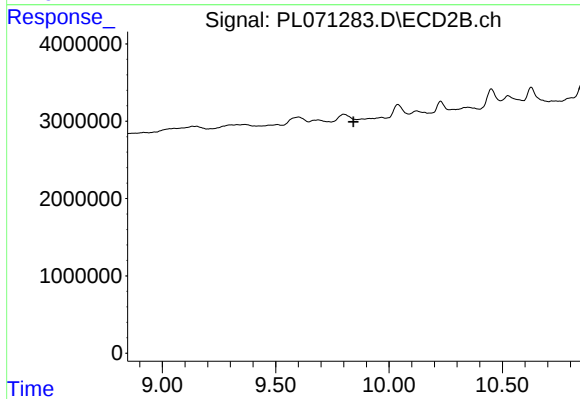

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

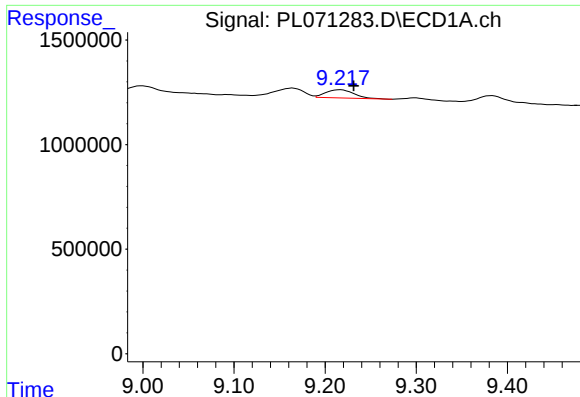

#21 Endrin ketone


R.T.: 9.217 min
Delta R.T.: -0.014 min
Response: 835040
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

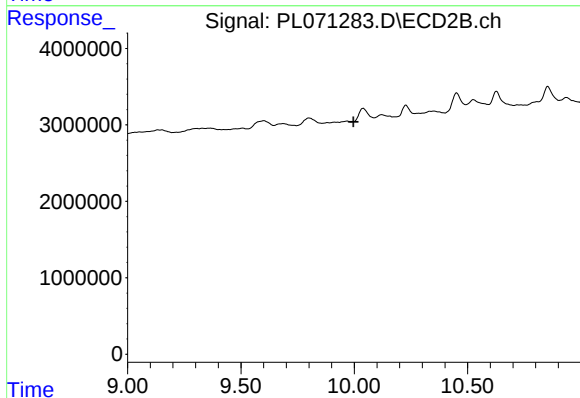


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.997 min
Response: 0
Conc: N.D.

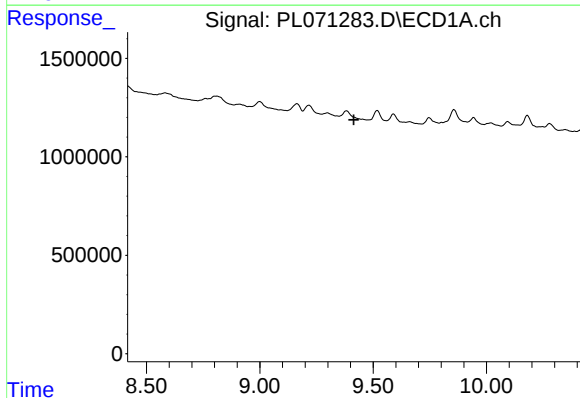


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.415 min
Response: 0
Conc: N.D.

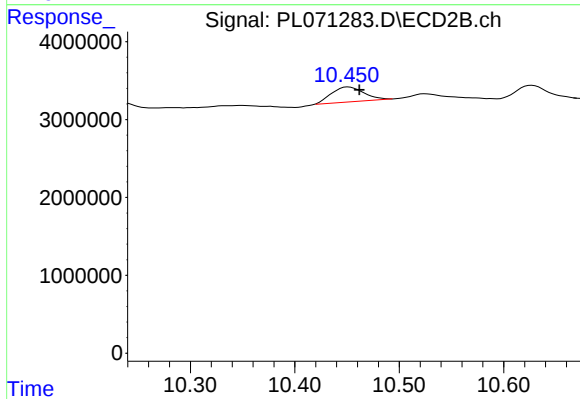

#22 Mirex


R.T.: 10.451 min
Delta R.T.: -0.011 min
Response: 4134559
Conc: 3.79 ng/ml

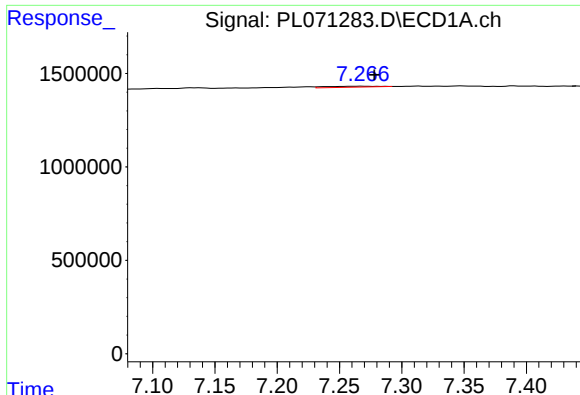

#25 Chlordane-3


R.T.: 7.268 min
Delta R.T.: -0.011 min
Response: 148672
Conc: 2.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

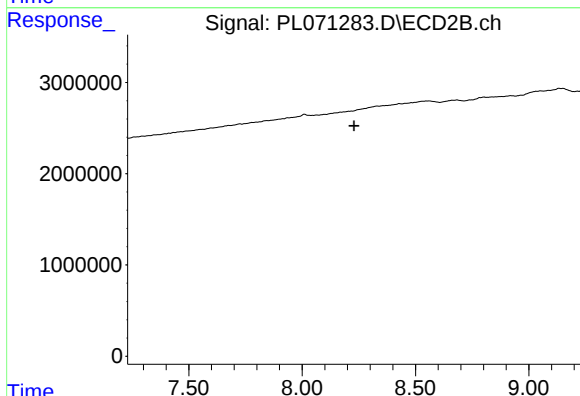


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

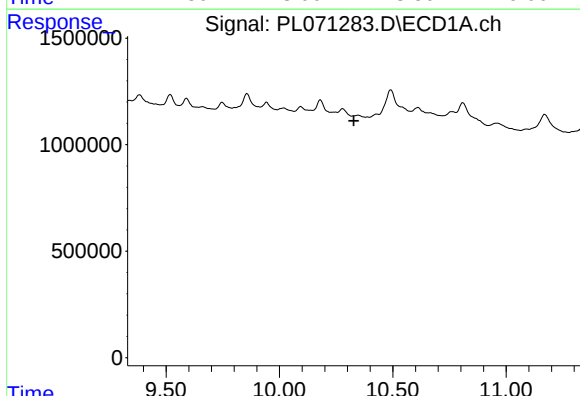

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.328 min
Response: 0
Conc: N.D.

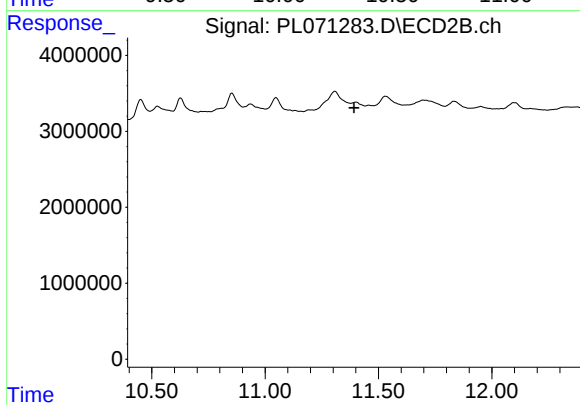

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.