

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120621\
 Data File : PL071290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2021 11:00
 Operator : AR\AJ
 Sample : M4914-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/07/2021
 Supervised By :Ankita Jodhani 12/07/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:10:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.567	5.501	11664782	25014832	24.835	19.933
2) SA Decachlor...	10.328	11.392	7186763	14311801	9.925	10.296
Target Compounds						
10) B gamma-Chl...	7.273	8.224	1831322	13878525	2.884m	8.680 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120621\
Data File : PL071290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2021 11:00
Operator : AR\AJ
Sample : M4914-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/07/2021
Supervised By :Ankita Jodhani 12/07/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:10:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

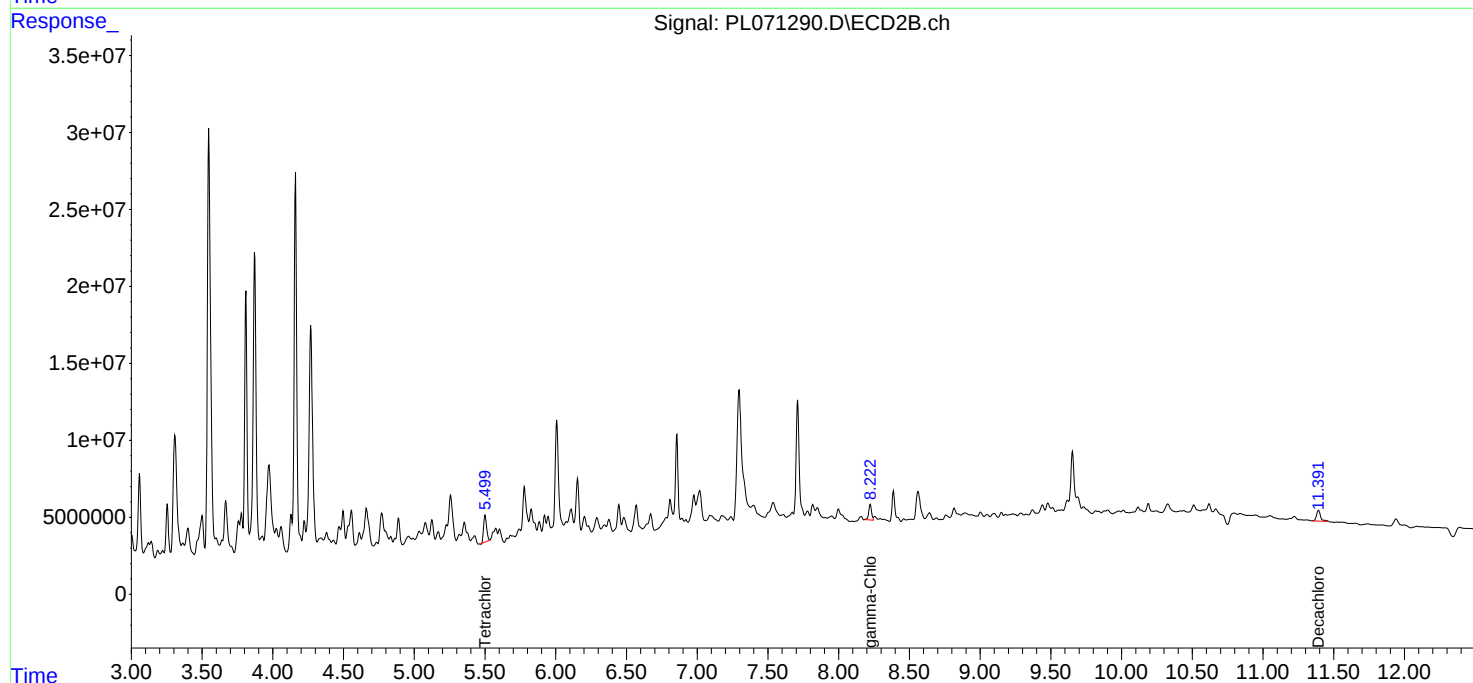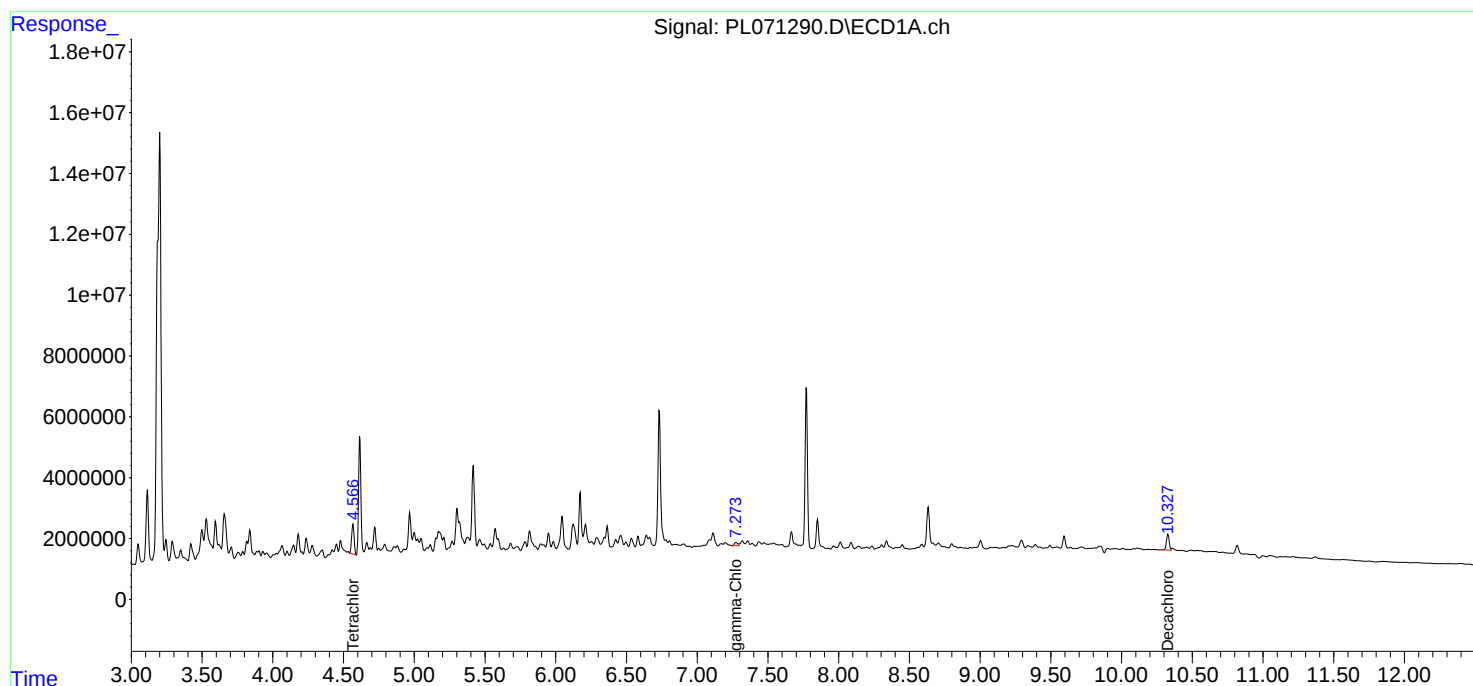

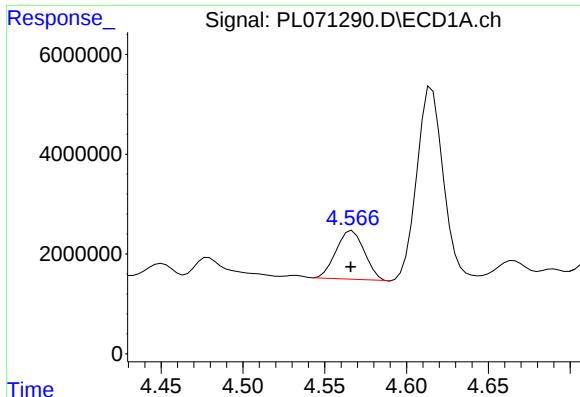


#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 11664782
Conc: 24.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/07/2021
Supervised By :Ankita Jodhani 12/07/2021

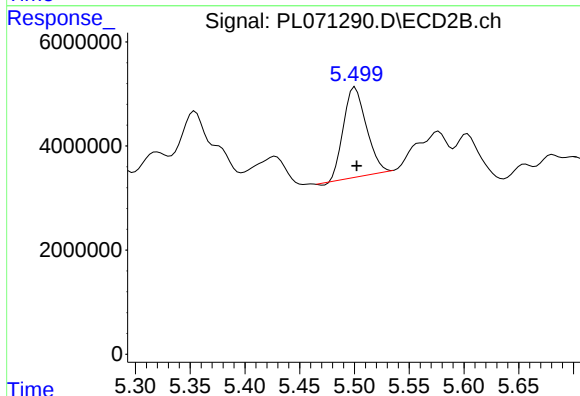


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: -0.001 min
Response: 25014832
Conc: 19.93 ng/ml

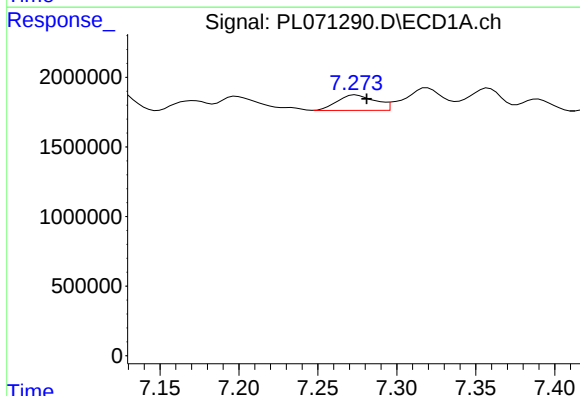


#10 gamma-Chlordane

R.T.: 7.273 min
Delta R.T.: -0.008 min
Response: 1831322
Conc: 2.88 ng/ml m

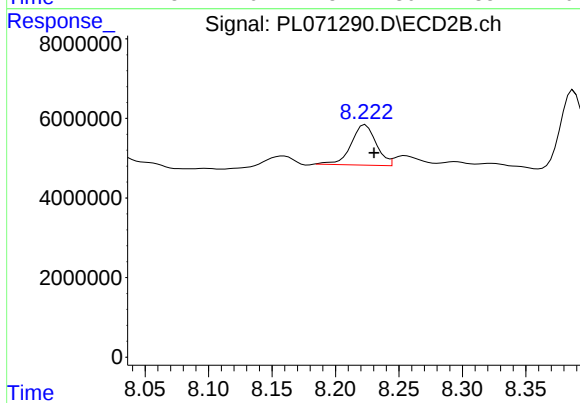

#10 gamma-Chlordane

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 13878525
Conc: 8.68 ng/ml

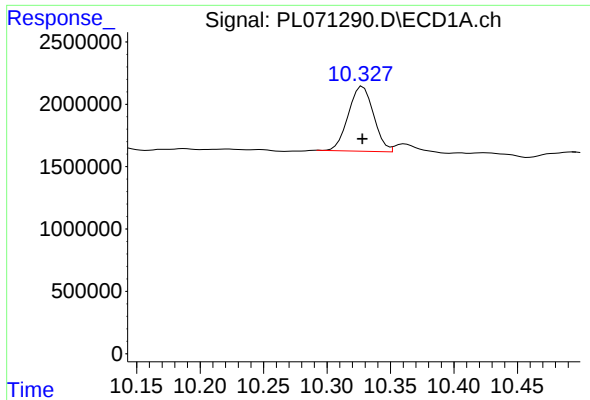


#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 7186763
Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/07/2021
Supervised By :Ankita Jodhani 12/07/2021

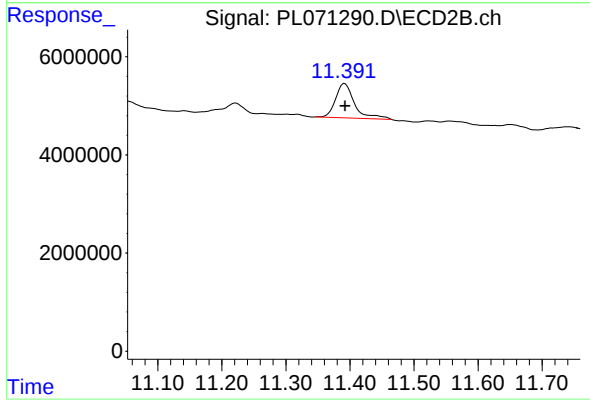

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 14311801
Conc: 10.30 ng/ml