

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120622\
 Data File : PL079602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2022 12:24
 Operator : AR\AJ
 Sample : N5793-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 20:39:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.566	42046569	53518757	18.613	19.661
28)	SA Decachlor...	8.765	7.631	32890304	40720491	16.935	17.333
Target Compounds							
4)	MA Heptachlor	0.000	3.700	0	2771067	N.D.	0.720 #
6)	B beta-BHC	0.000	3.700f	0	2771067	N.D.	1.829 #
7)	B delta-BHC	4.544f	3.891	3171979	235913	1.143	0.061 #
8)	B Heptachlo...	5.467f	0.000	1119296	0	0.392	N.D. #
11)	B alpha-Chl...	0.000	4.746f	0	940542	N.D.	0.281 #
12)	B 4,4'-DDE	5.958	0.000	267558	0	0.107	N.D. #
19)	B Endosulfa...	6.938	0.000	163428	0	0.070	N.D. #
23)	Chlordane-1	0.000	3.546f	0	1140938	N.D.	10.727 #
26)	Chlordane-4	0.000	4.746f	0	940542	N.D.	2.596 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120622\
Data File : PL079602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2022 12:24
Operator : AR\AJ
Sample : N5793-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 20:39:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

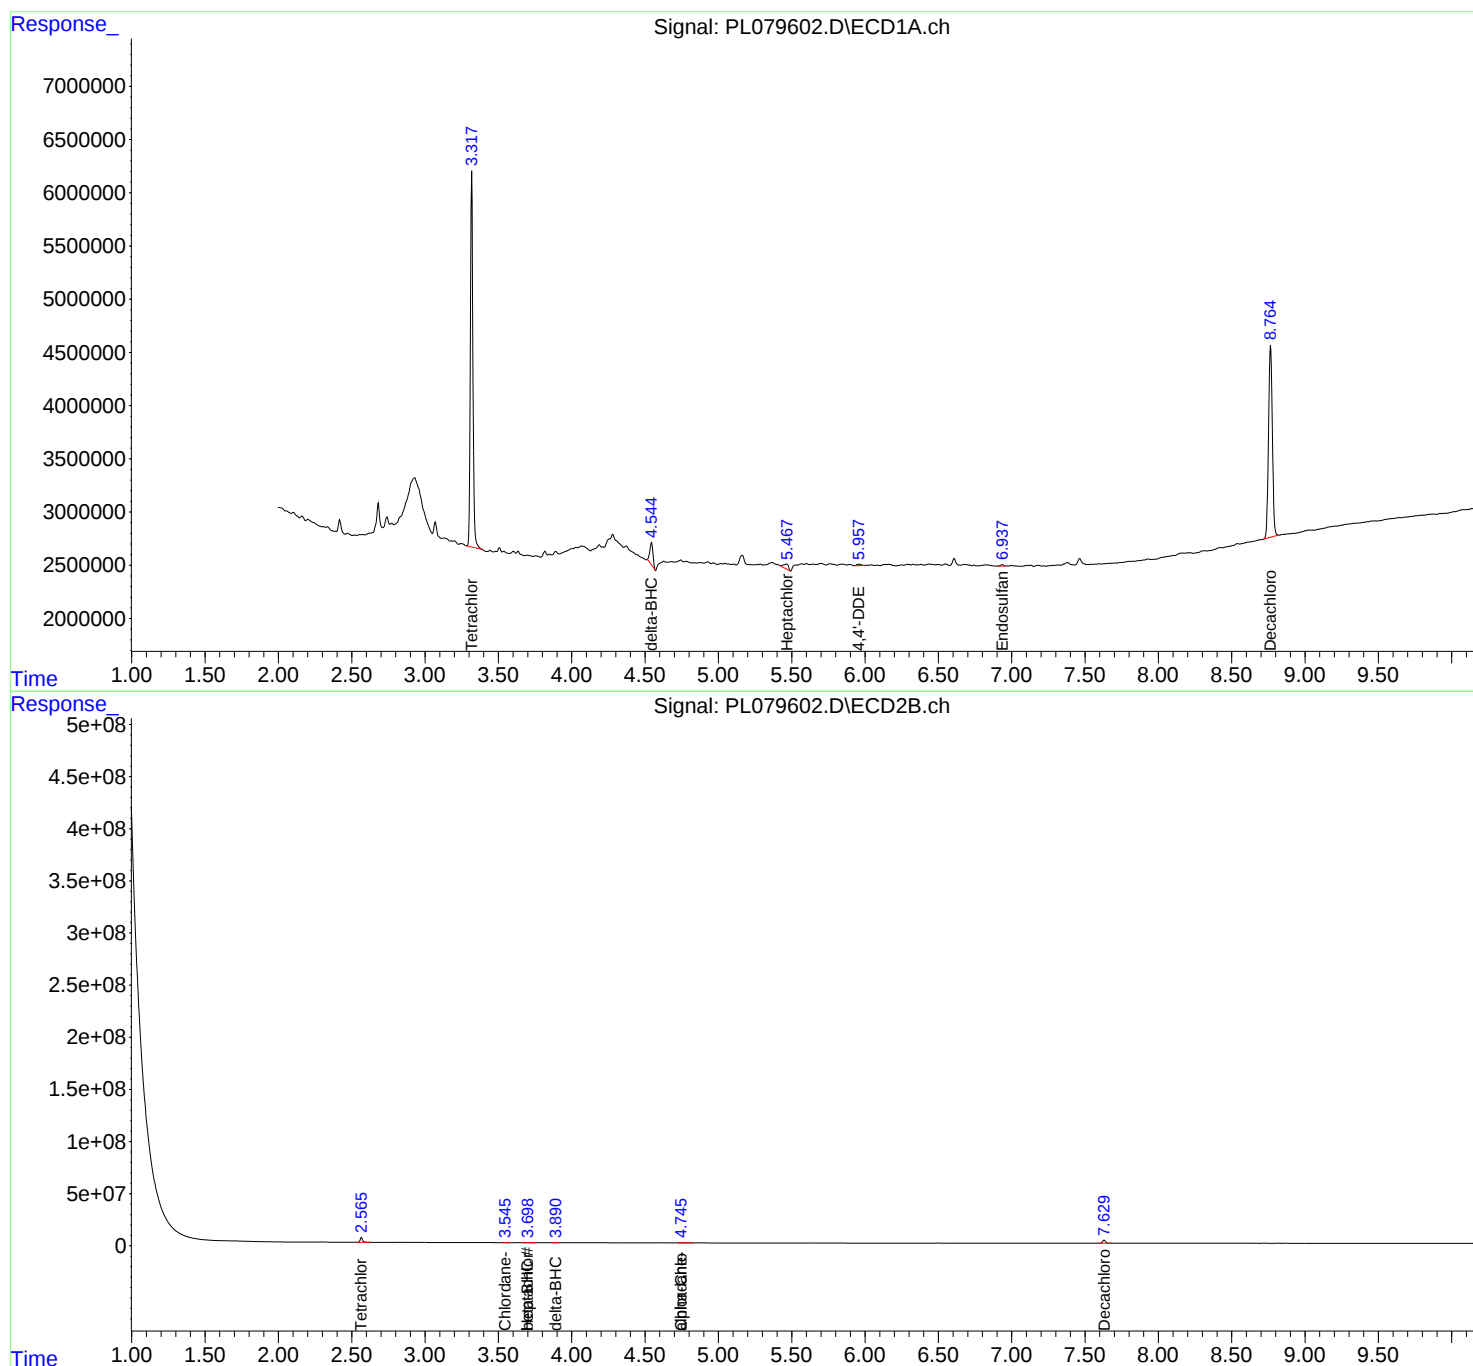


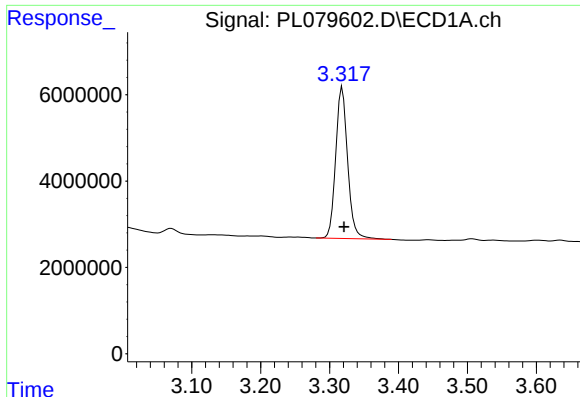

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.003 min
Response: 42046569
Conc: 18.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

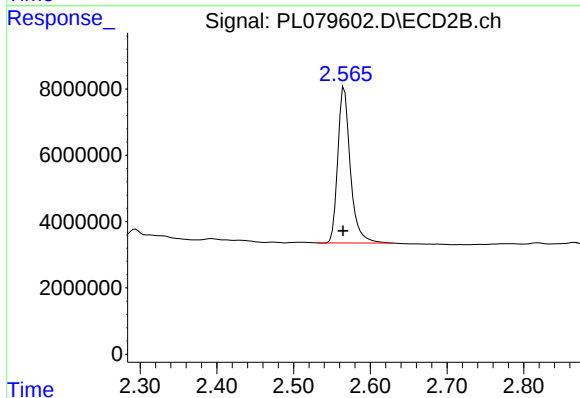


#1 Tetrachloro-m-xylene

R.T.: 2.566 min
Delta R.T.: 0.002 min
Response: 53518757
Conc: 19.66 ng/ml

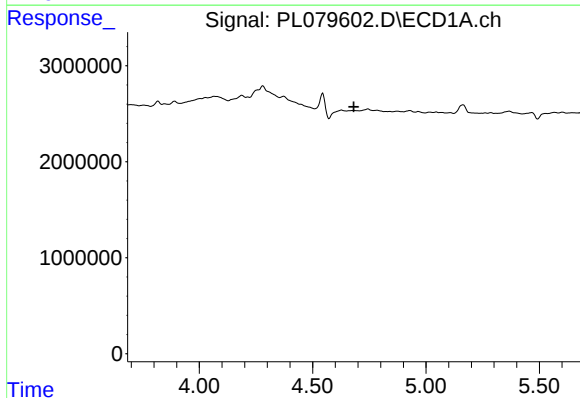


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.681 min
Response: 0
Conc: N.D.

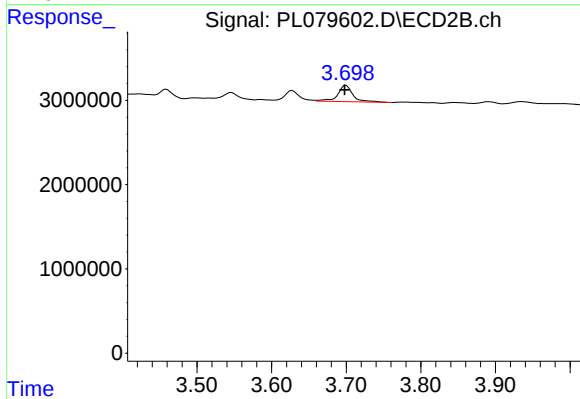

#4 Heptachlor


R.T.: 3.700 min
Delta R.T.: 0.002 min
Response: 2771067
Conc: 0.72 ng/ml

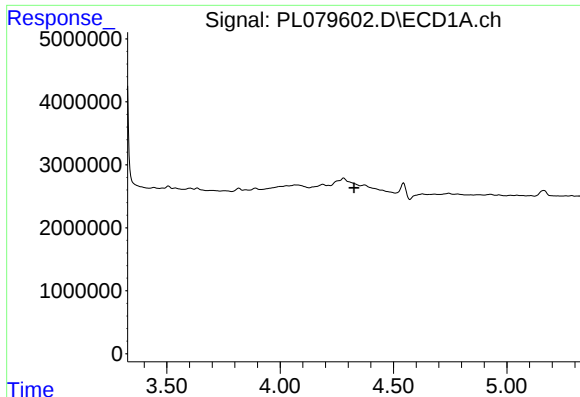

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

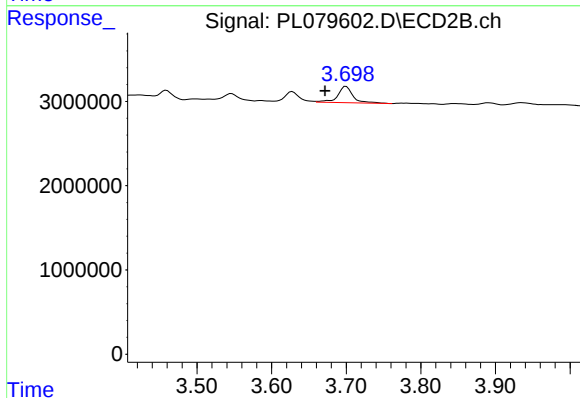


#6 beta-BHC

R.T.: 3.700 min
Delta R.T.: 0.028 min
Response: 2771067
Conc: 1.83 ng/ml

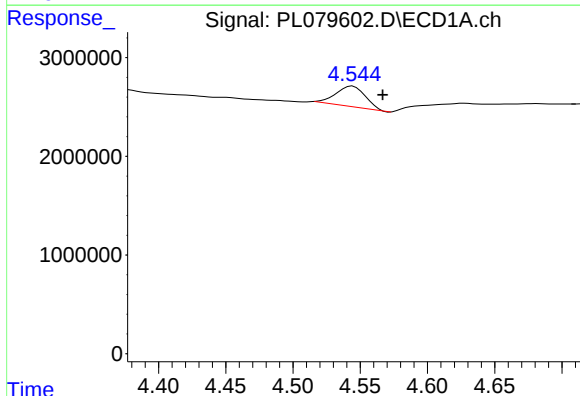


#7 delta-BHC

R.T.: 4.544 min
Delta R.T.: -0.023 min
Response: 3171979
Conc: 1.14 ng/ml

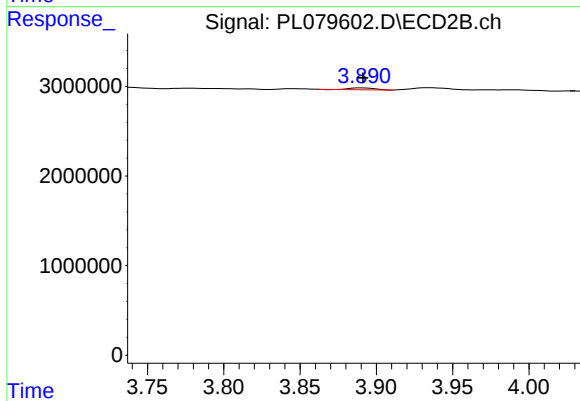

#7 delta-BHC


R.T.: 3.891 min
Delta R.T.: 0.000 min
Response: 235913
Conc: 0.06 ng/ml

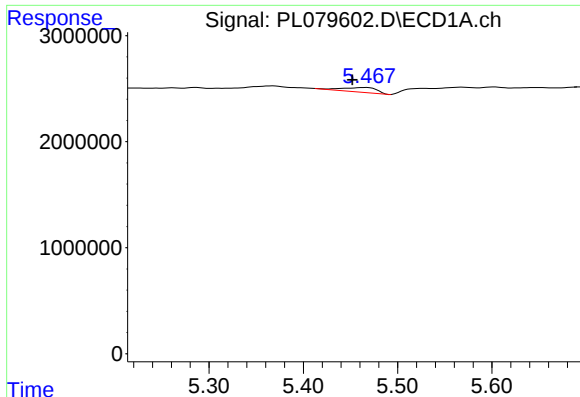

#8 Heptachlor epoxide


R.T.: 5.467 min
Delta R.T.: 0.015 min
Response: 1119296
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

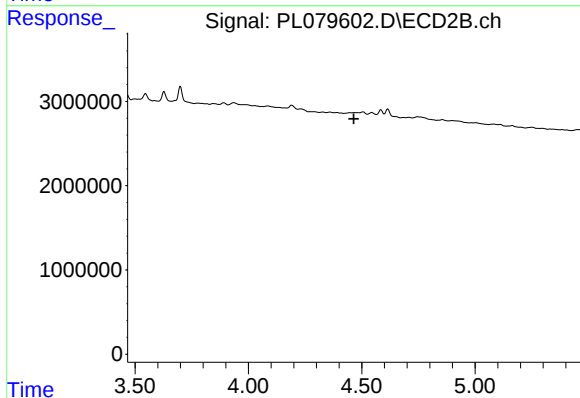


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.465 min
Response: 0
Conc: N.D.

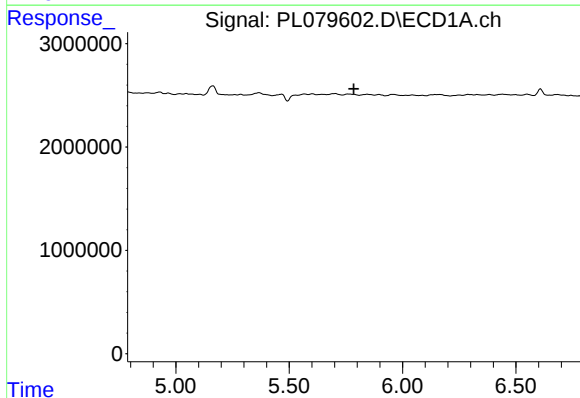


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.784 min
Response: 0
Conc: N.D.

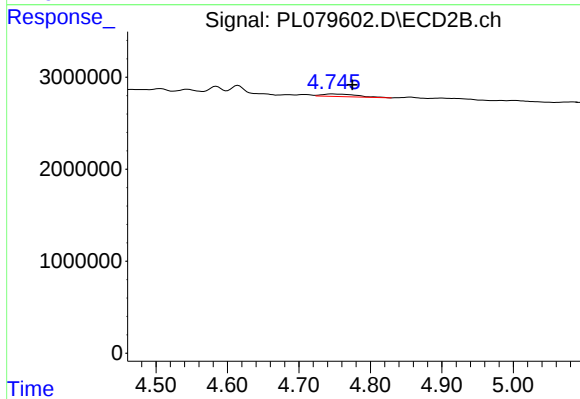

#11 alpha-Chlordane


R.T.: 4.746 min
Delta R.T.: -0.028 min
Response: 940542
Conc: 0.28 ng/ml

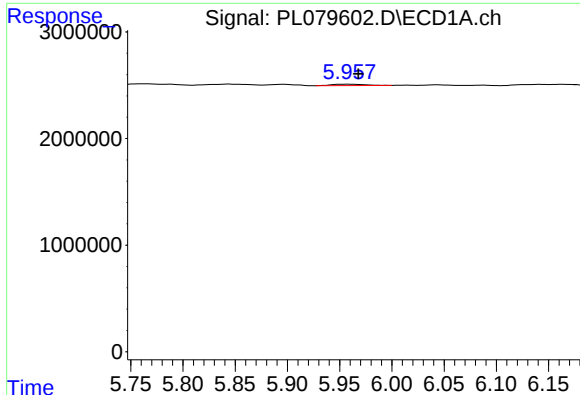

#12 4,4'-DDE


R.T.: 5.958 min
Delta R.T.: -0.010 min
Response: 267558
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

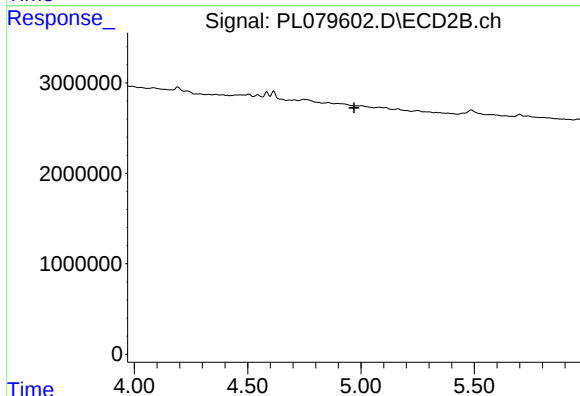


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 4.970 min
Response: 0
Conc: N.D.

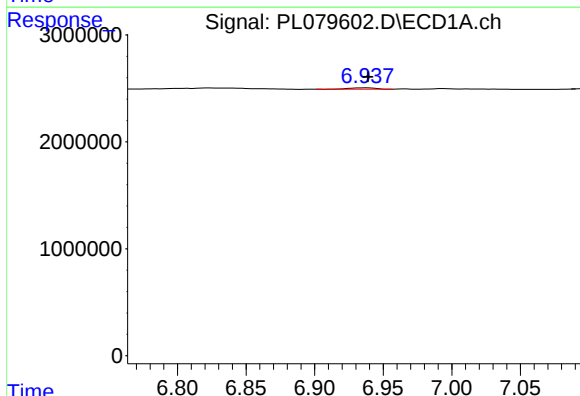


#19 Endosulfan Sulfate

R.T.: 6.938 min
Delta R.T.: -0.001 min
Response: 163428
Conc: 0.07 ng/ml

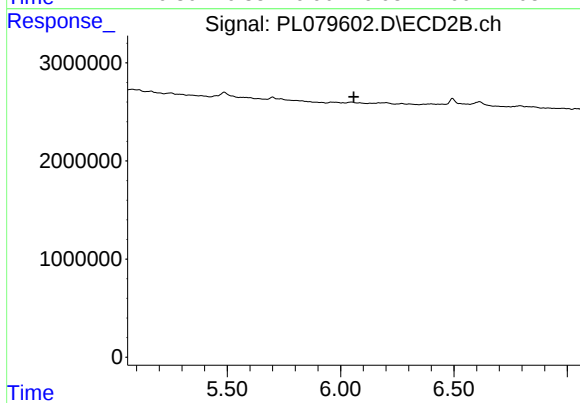

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

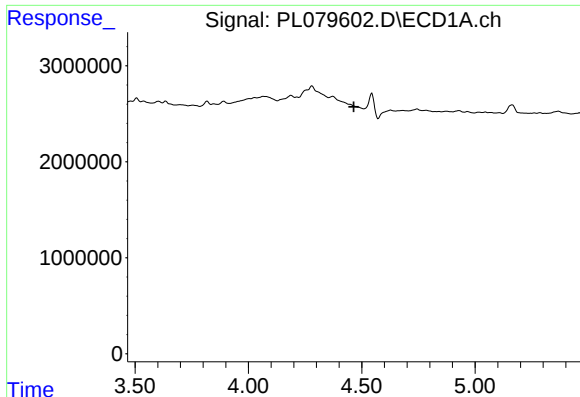

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

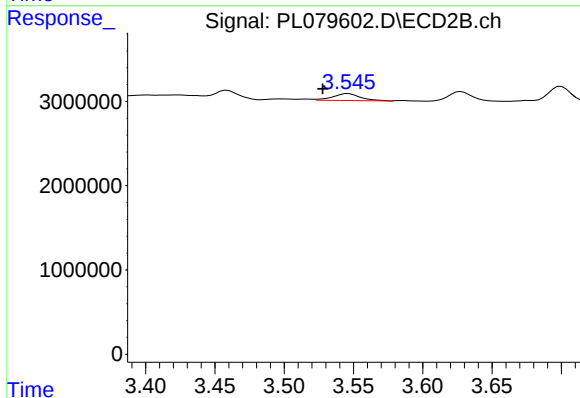


#23 Chlordane-1

R.T.: 3.546 min
Delta R.T.: 0.018 min
Response: 1140938
Conc: 10.73 ng/ml

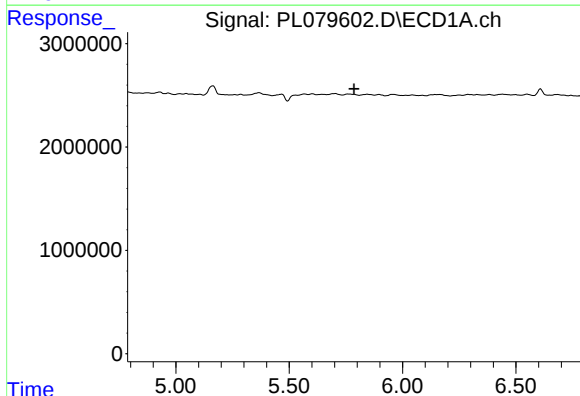


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.786 min
Response: 0
Conc: N.D.

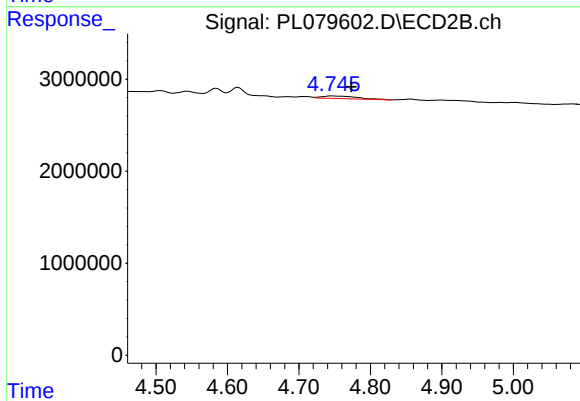

#26 Chlordane-4


R.T.: 4.746 min
Delta R.T.: -0.027 min
Response: 940542
Conc: 2.60 ng/ml

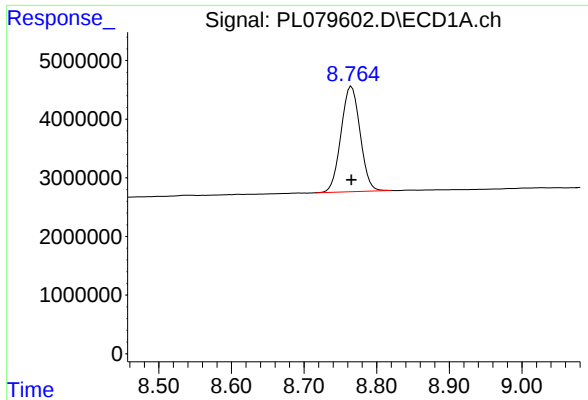

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 32890304
Conc: 16.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

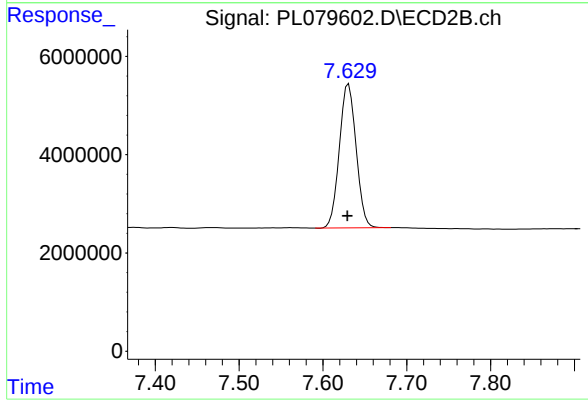

#28 Decachlorobiphenyl

R.T.: 7.631 min
Delta R.T.: 0.002 min
Response: 40720491
Conc: 17.33 ng/ml