

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120623\
 Data File : PL087012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 20:16
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:33:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 07 00:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	2.700	301.2E6	116.3E6	99.837	103.315
28)	SA Decachlor...	9.047	7.900	221.8E6	90781239	99.134	96.638
Target Compounds							
23)	Chlordane-1	4.621	3.707	125.2E6	34585464	996.662	1031.629
24)	Chlordane-2	5.158	4.290	126.4E6	40608906	963.822	996.612
25)	Chlordane-3	5.876	4.926	517.8E6	111.2E6	1035.573	1068.317
26)	Chlordane-4	5.960	4.989	638.0E6	115.9E6	1019.304	1057.356
27)	Chlordane-5	6.816	5.663	91488392	29138895	1020.011	1011.047



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120623\
Data File : PL087012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 20:16
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:33:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
Quant Title : GC Extractables
QLast Update : Thu Dec 07 00:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

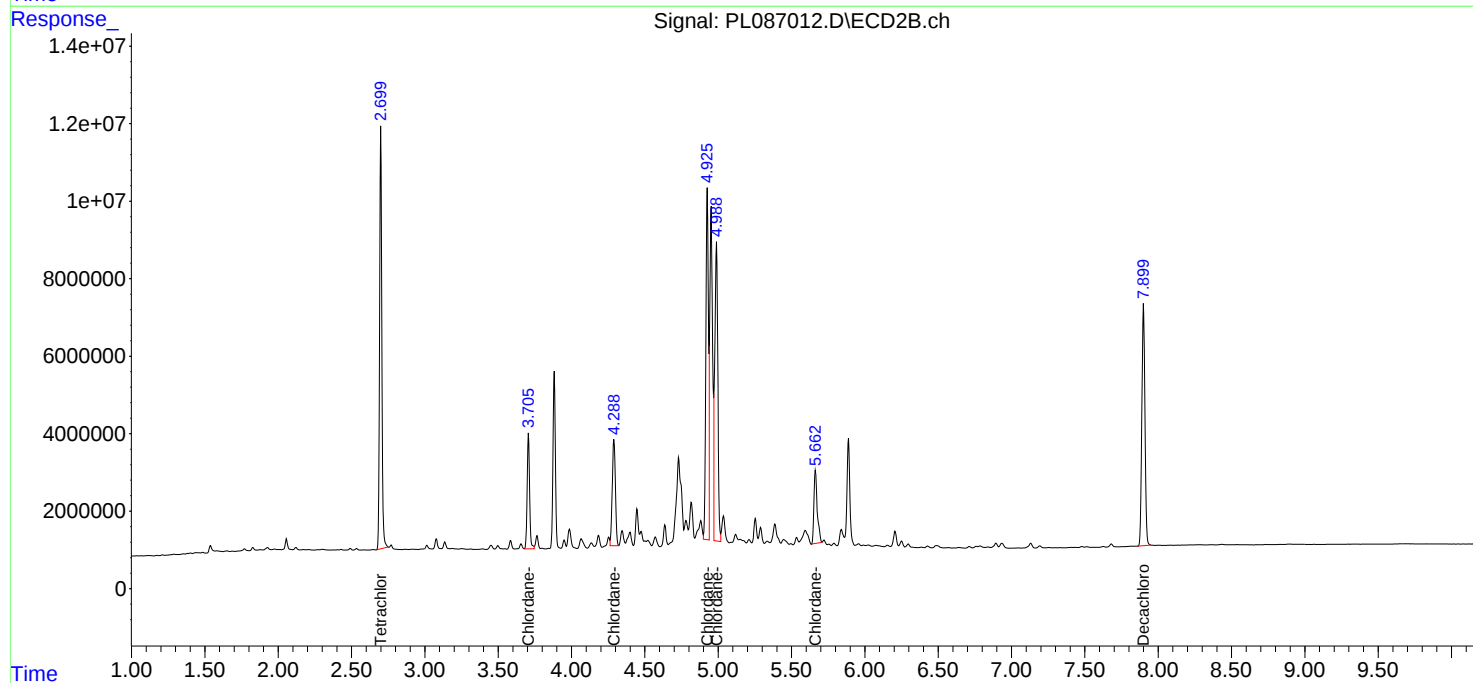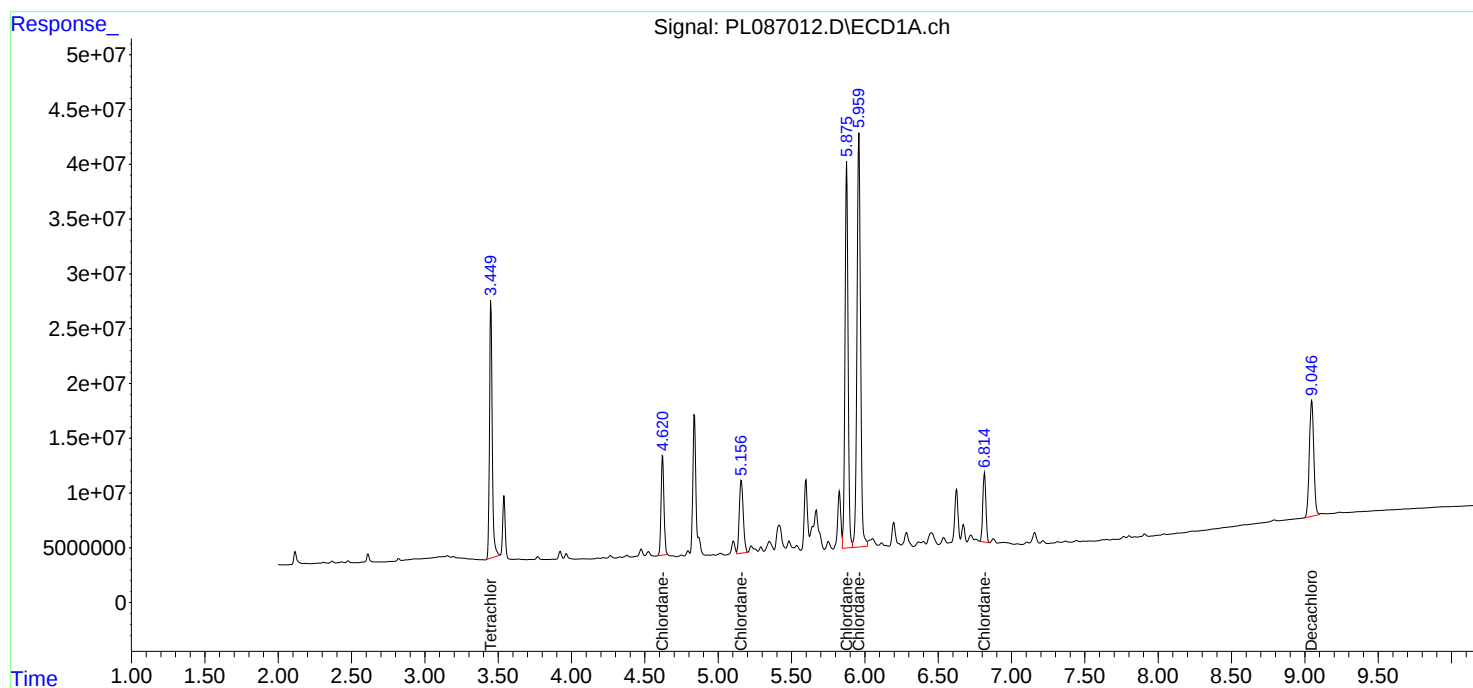


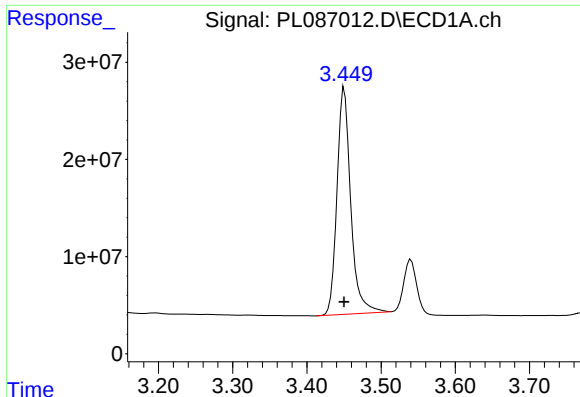

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 301195927
Conc: 99.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

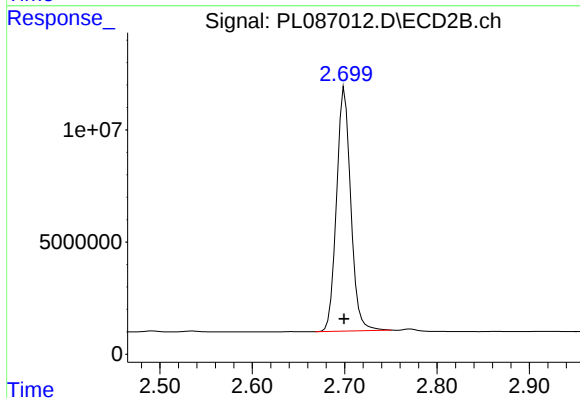


#1 Tetrachloro-m-xylene

R.T.: 2.700 min
Delta R.T.: 0.000 min
Response: 116309129
Conc: 103.32 ng/ml

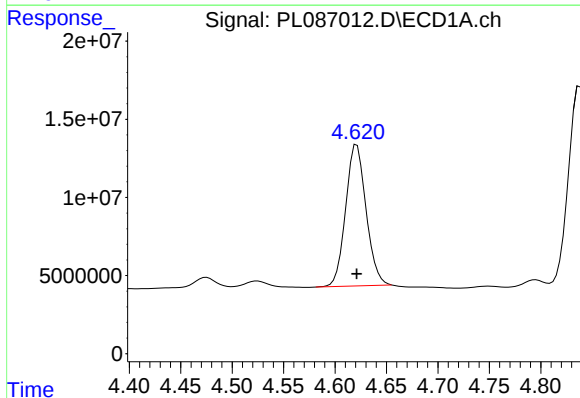


#23 Chlordane-1

R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 125207881
Conc: 996.66 ng/ml

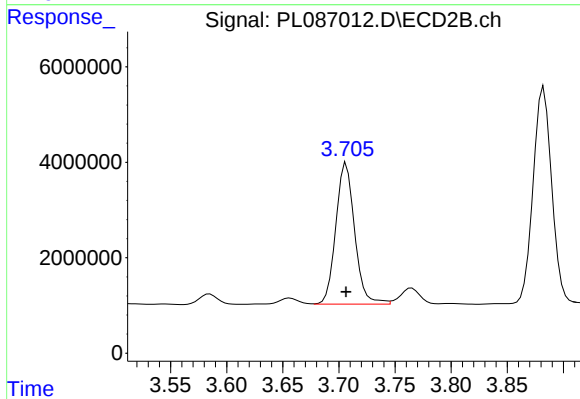

#23 Chlordane-1


R.T.: 3.707 min
Delta R.T.: 0.000 min
Response: 34585464
Conc: 1031.63 ng/ml

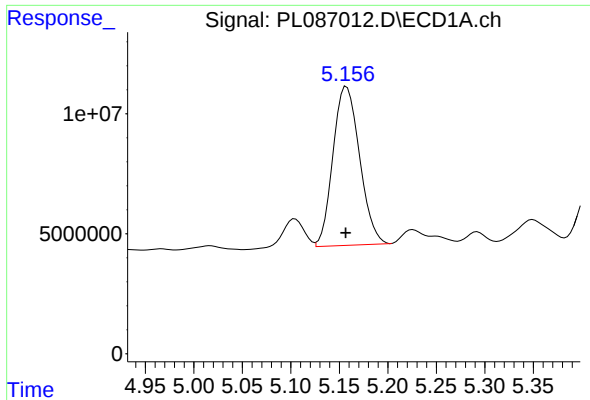

#24 Chlordane-2


R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 126372816
Conc: 963.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

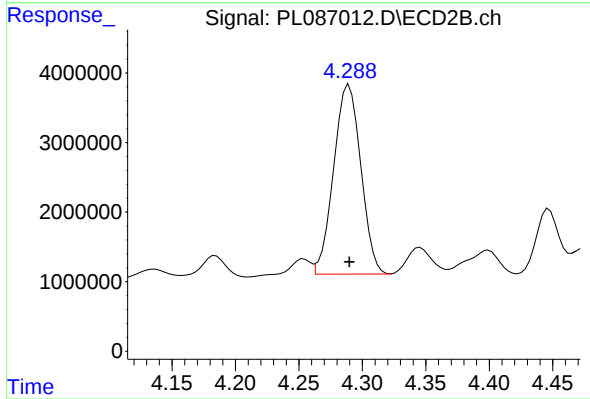


#24 Chlordane-2

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 40608906
Conc: 996.61 ng/ml

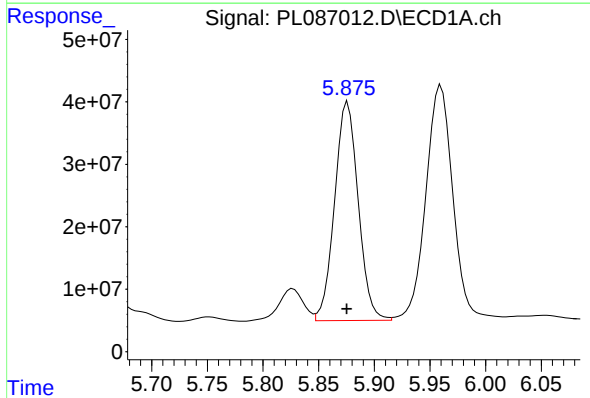


#25 Chlordane-3

R.T.: 5.876 min
Delta R.T.: 0.000 min
Response: 517750831
Conc: 1035.57 ng/ml

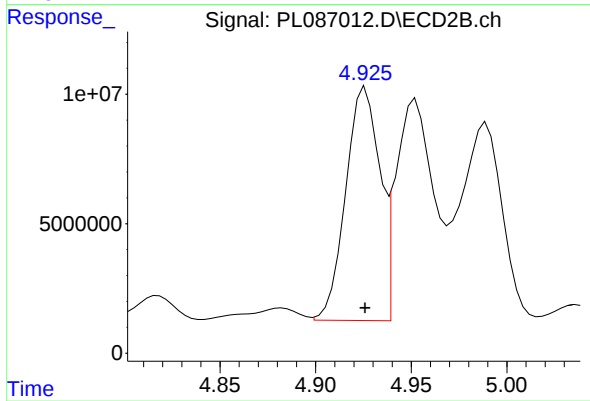

#25 Chlordane-3


R.T.: 4.926 min
Delta R.T.: 0.000 min
Response: 111177052
Conc: 1068.32 ng/ml

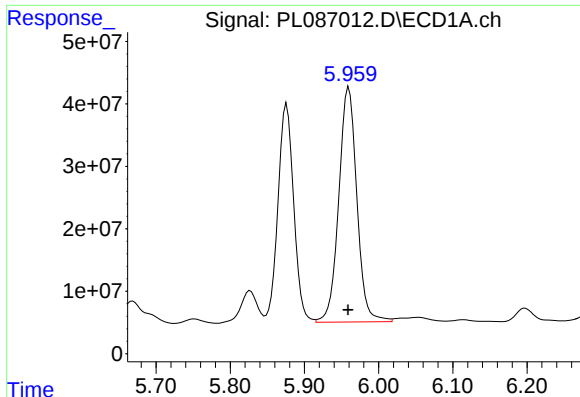

#26 Chlordane-4


R.T.: 5.960 min
Delta R.T.: 0.001 min
Response: 637973757
Conc: 1019.30 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

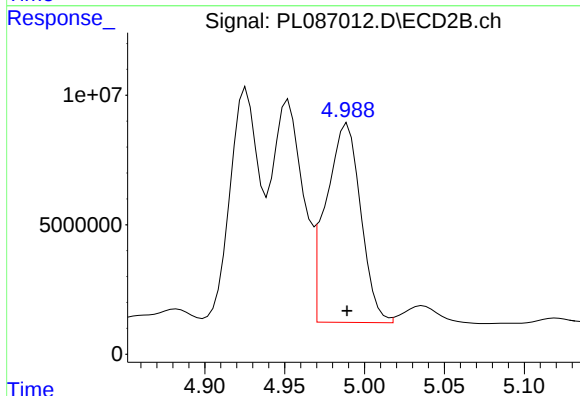


#26 Chlordane-4

R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 115884357
Conc: 1057.36 ng/ml

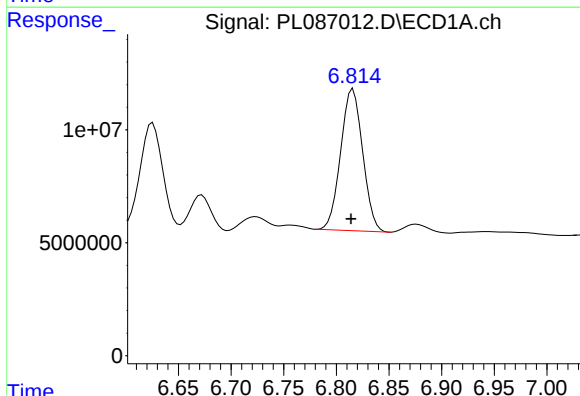


#27 Chlordane-5

R.T.: 6.816 min
Delta R.T.: 0.002 min
Response: 91488392
Conc: 1020.01 ng/ml

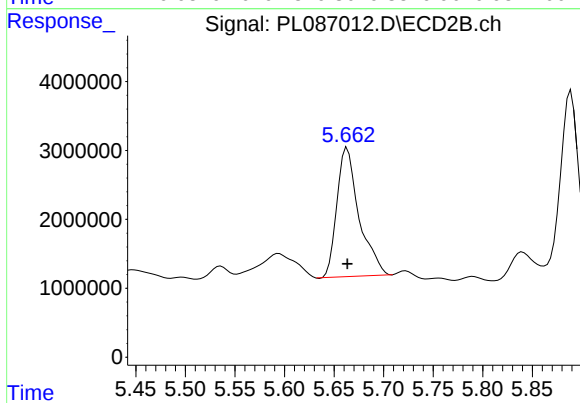

#27 Chlordane-5


R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 29138895
Conc: 1011.05 ng/ml

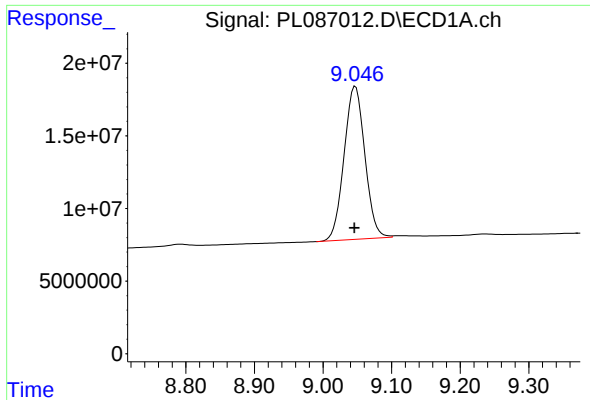

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.002 min
Response: 221839090
Conc: 99.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

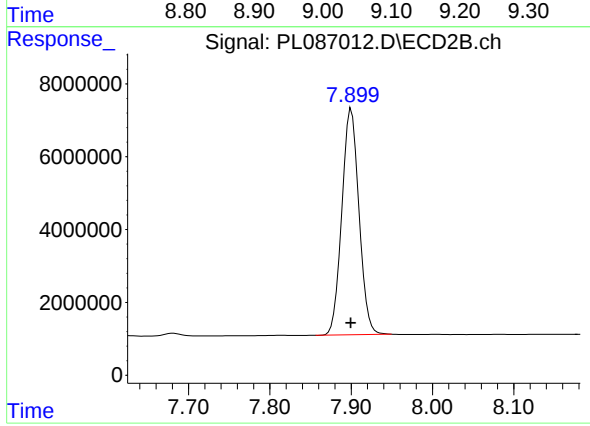

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 90781239
Conc: 96.64 ng/ml