

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120623\
 Data File : PL087013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 20:30
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:34:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 07 00:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	2.699	225.8E6	86285409	74.848	76.646
28)	SA Decachlor...	9.046	7.899	166.6E6	68592456	74.471	73.017
Target Compounds							
23)	Chlordane-1	4.621	3.706	93269665	25689555	742.432	766.278
24)	Chlordane-2	5.157	4.290	95411058	30709499	727.682	753.664
25)	Chlordane-3	5.875	4.925	379.6E6	80622611	759.351	774.715
26)	Chlordane-4	5.959	4.989	470.2E6	84290099	751.269	769.082
27)	Chlordane-5	6.815	5.663	67228997	21556407	749.541	747.953


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120623\
Data File : PL087013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 20:30
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:34:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
Quant Title : GC Extractables
QLast Update : Thu Dec 07 00:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

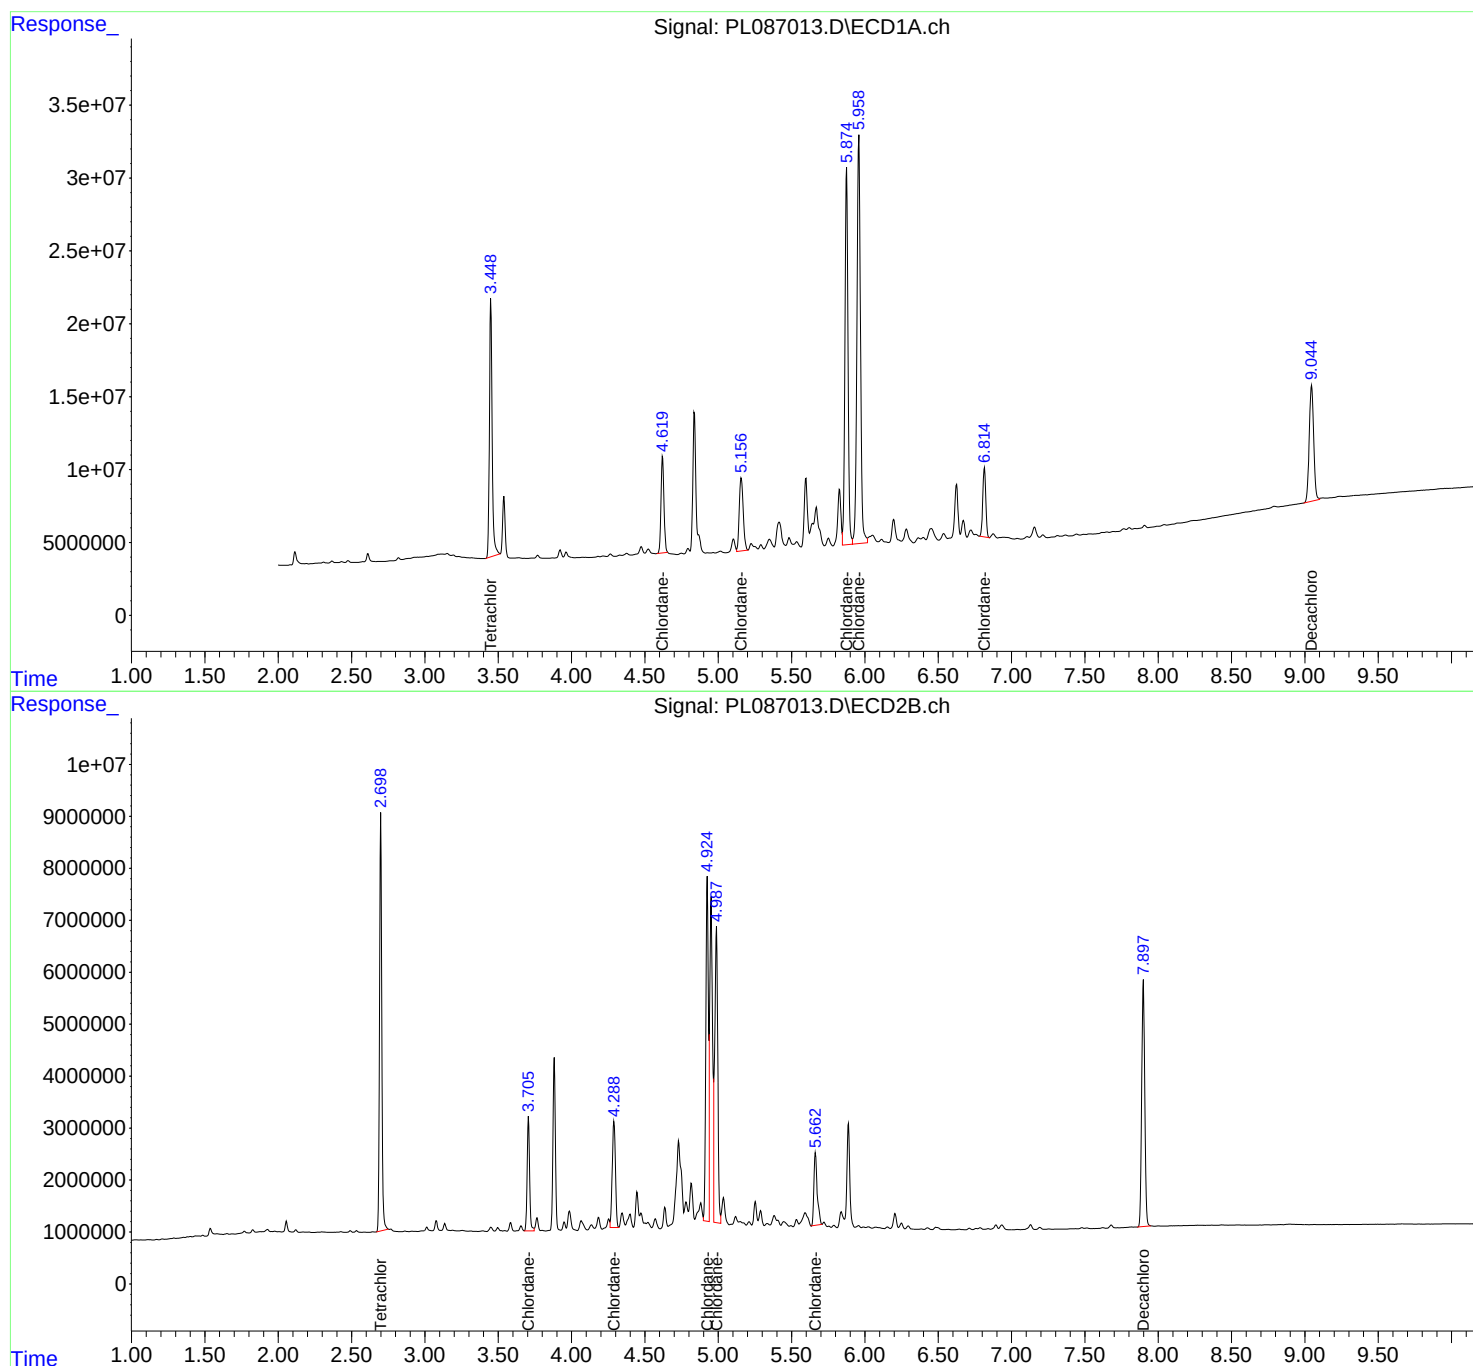


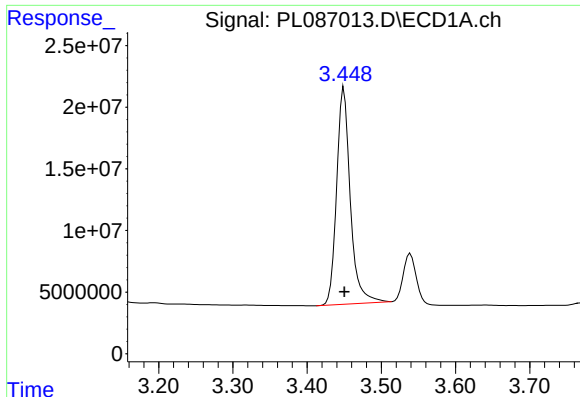

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 225806640
Conc: 74.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

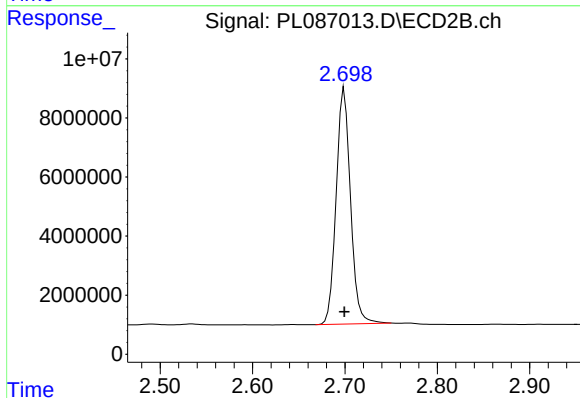


#1 Tetrachloro-m-xylene

R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 86285409
Conc: 76.65 ng/ml

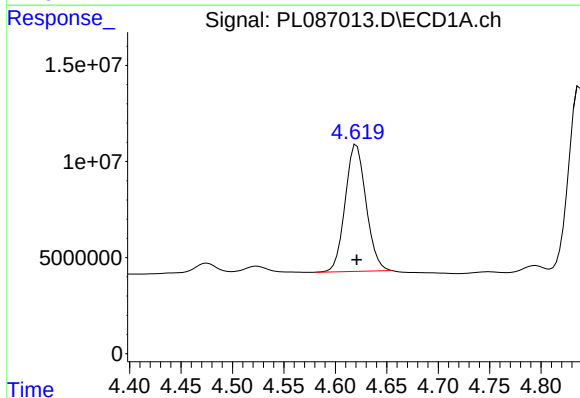


#23 Chlordane-1

R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 93269665
Conc: 742.43 ng/ml

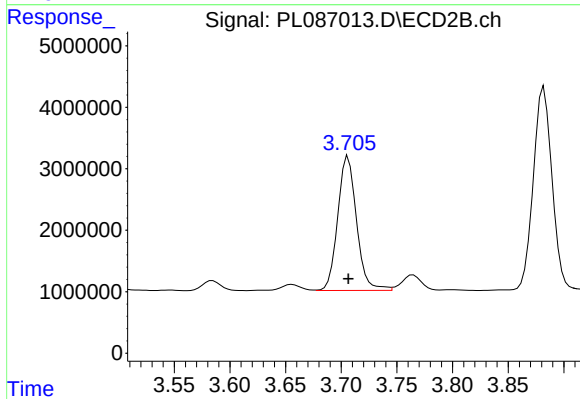

#23 Chlordane-1


R.T.: 3.706 min
Delta R.T.: 0.000 min
Response: 25689555
Conc: 766.28 ng/ml

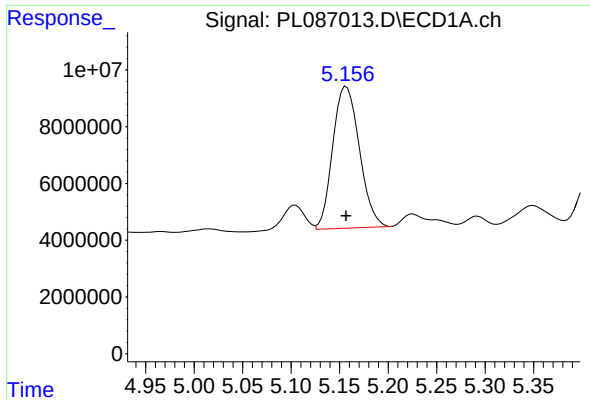

#24 Chlordane-2


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 95411058
Conc: 727.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

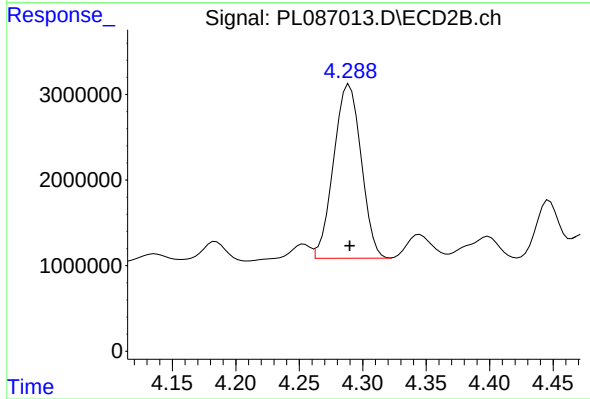


#24 Chlordane-2

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 30709499
Conc: 753.66 ng/ml

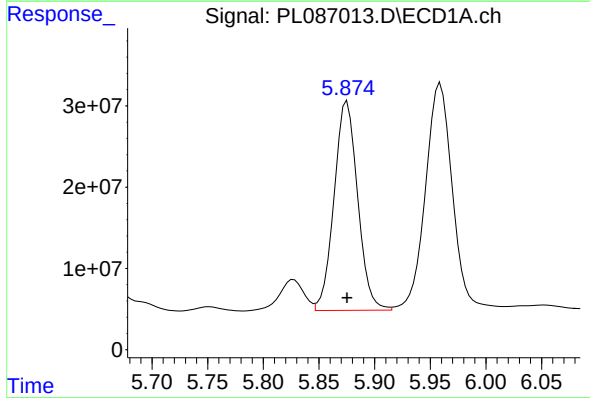


#25 Chlordane-3

R.T.: 5.875 min
Delta R.T.: 0.000 min
Response: 379649416
Conc: 759.35 ng/ml

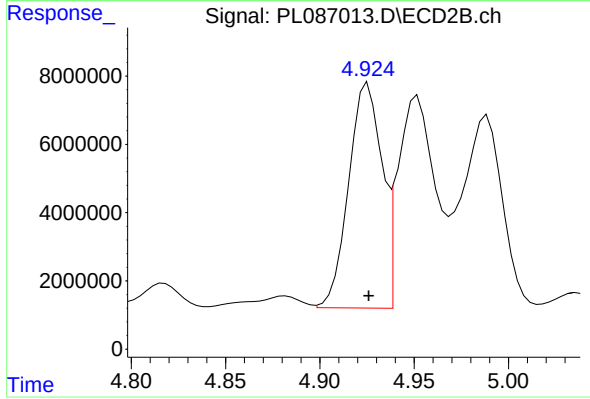

#25 Chlordane-3


R.T.: 4.925 min
Delta R.T.: 0.000 min
Response: 80622611
Conc: 774.71 ng/ml

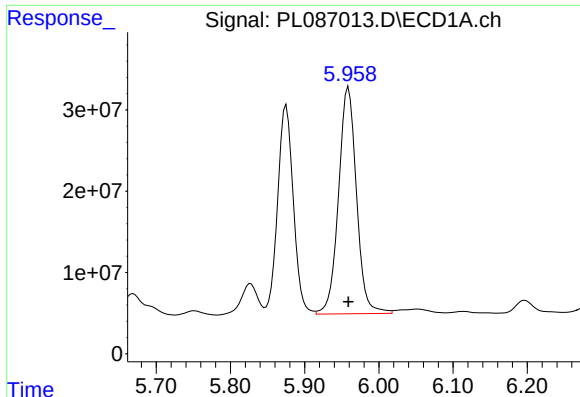

#26 Chlordane-4


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 470213129
Conc: 751.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

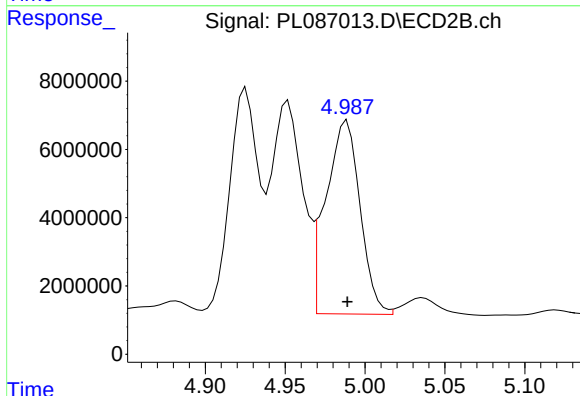


#26 Chlordane-4

R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 84290099
Conc: 769.08 ng/ml

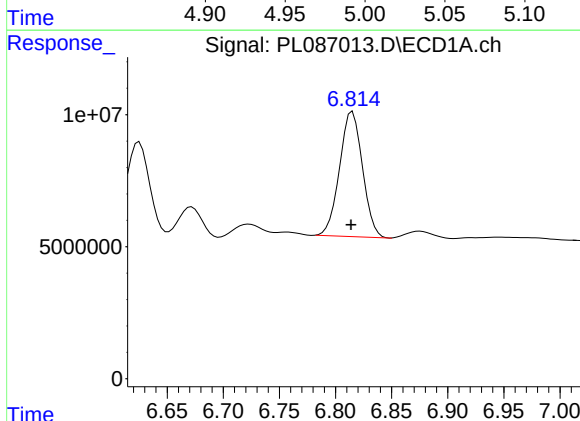


#27 Chlordane-5

R.T.: 6.815 min
Delta R.T.: 0.001 min
Response: 67228997
Conc: 749.54 ng/ml

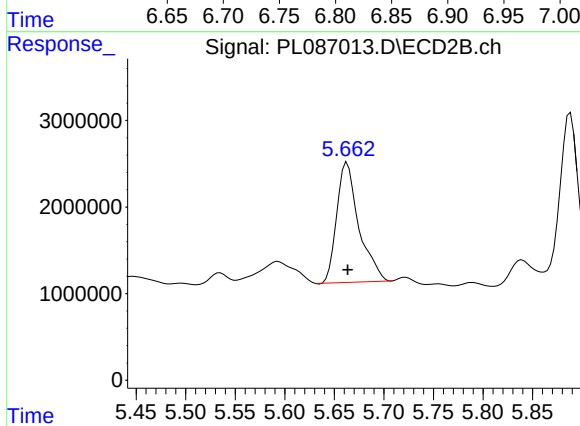

#27 Chlordane-5


R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 21556407
Conc: 747.95 ng/ml

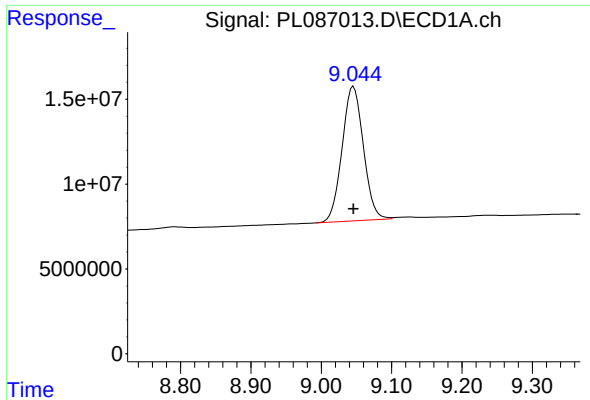

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: 0.000 min
Response: 166649817
Conc: 74.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

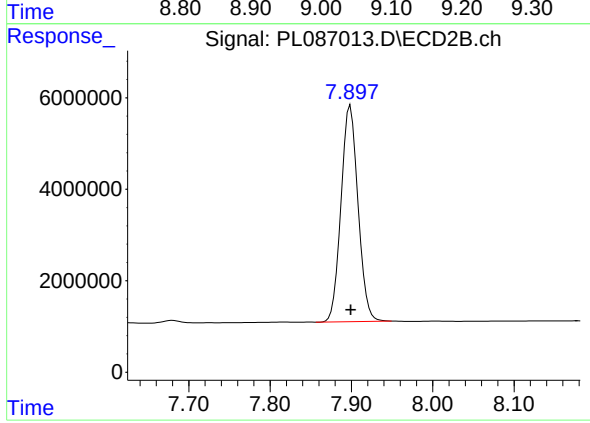

#28 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: 0.000 min
Response: 68592456
Conc: 73.02 ng/ml