

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120623\
 Data File : PL087023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 22:48
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL120623CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:35:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 07 00:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	2.699	154.8E6	56264622	51.322	49.979
28)	SA Decachlor...	9.047	7.900	113.7E6	46803946	50.807	49.823
Target Compounds							
23)	Chlordane-1	4.621	3.706	63815985	16849217	507.979	502.585
24)	Chlordane-2	5.157	4.290	67227730	20399663	512.733	500.643
25)	Chlordane-3	5.875	4.925	257.2E6	52093324	514.403	500.573
26)	Chlordane-4	5.959	4.989	322.2E6	54960715	514.815	501.474
27)	Chlordane-5	6.815	5.663	45992159	14244395	512.770	494.245



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120623\
Data File : PL087023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 22:48
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL120623CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:35:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
Quant Title : GC Extractables
QLast Update : Thu Dec 07 00:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

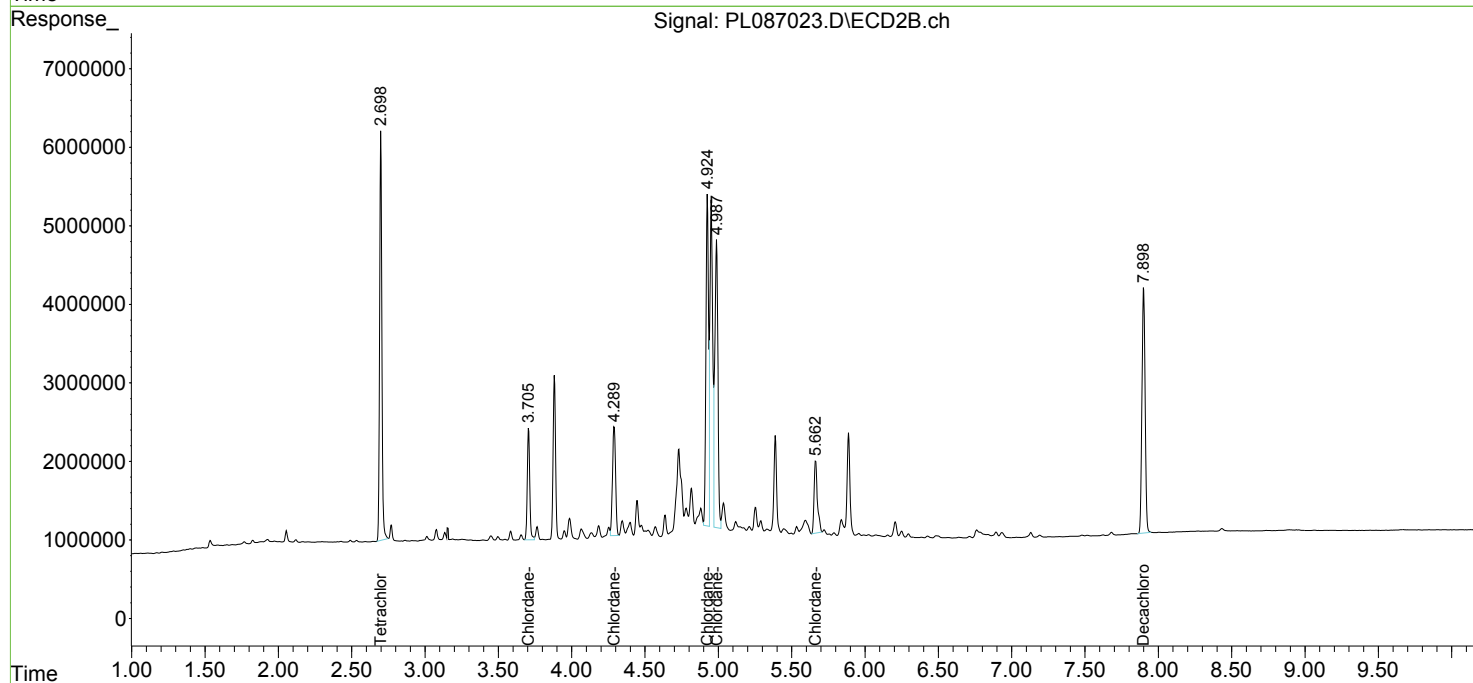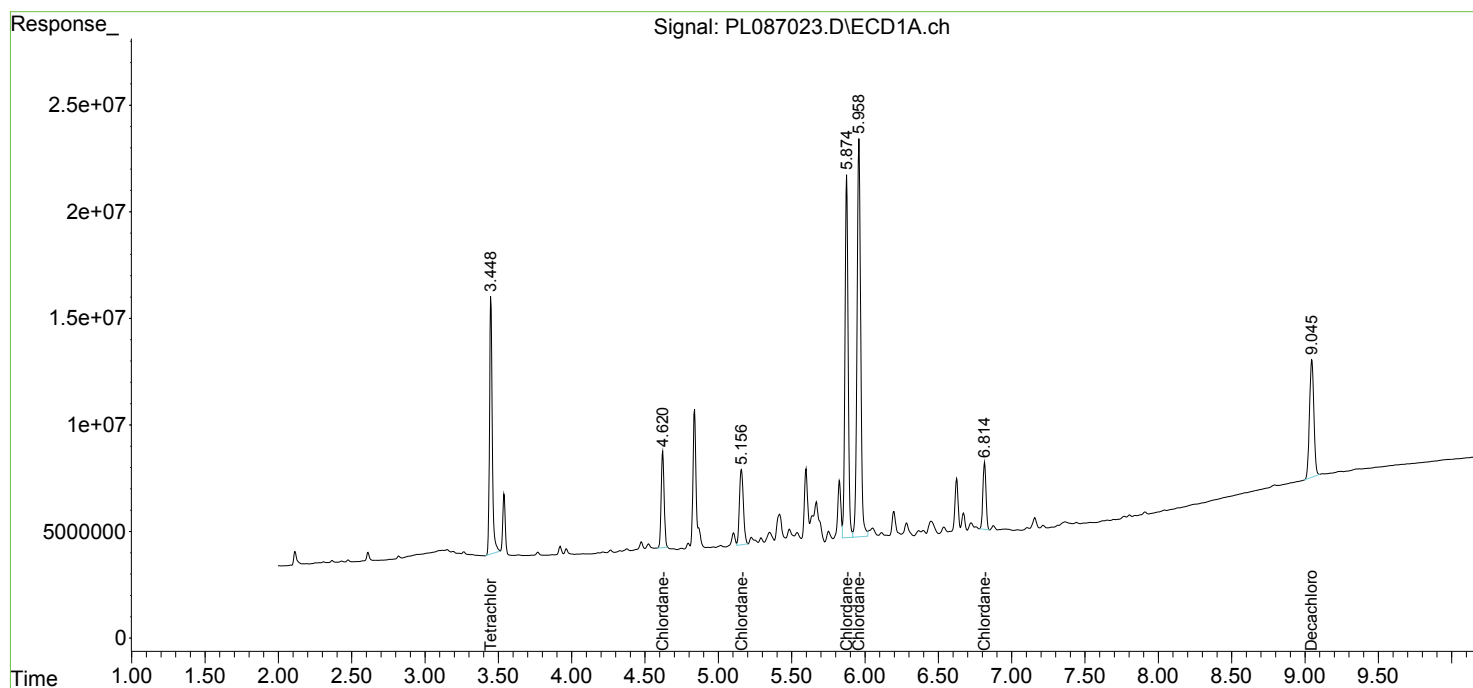


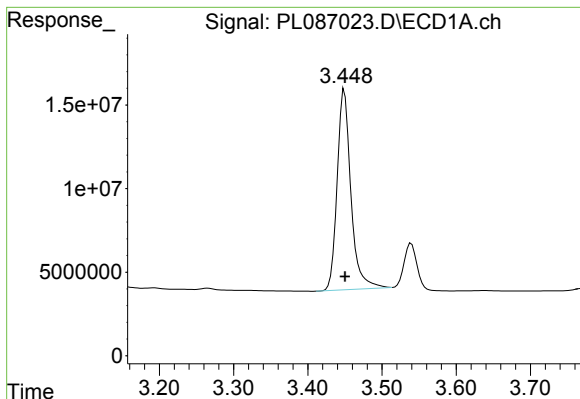

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 154832366
Conc: 51.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120623CHLOR

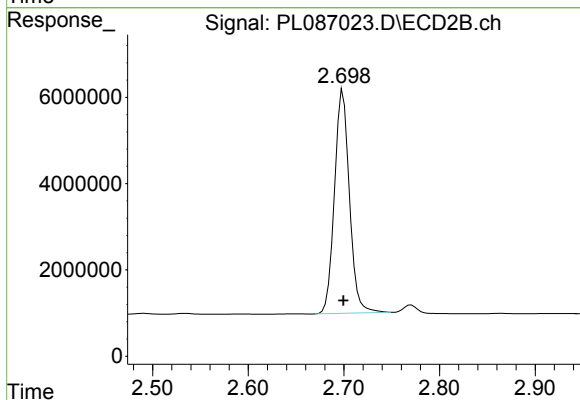


#1 Tetrachloro-m-xylene

R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 56264622
Conc: 49.98 ng/ml

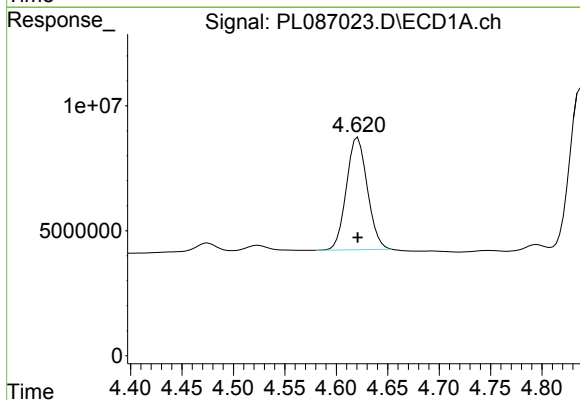


#23 Chlordane-1

R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 63815985
Conc: 507.98 ng/ml

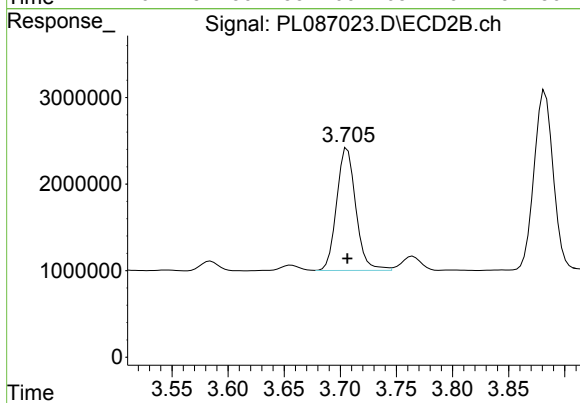

#23 Chlordane-1


R.T.: 3.706 min
Delta R.T.: 0.000 min
Response: 16849217
Conc: 502.59 ng/ml

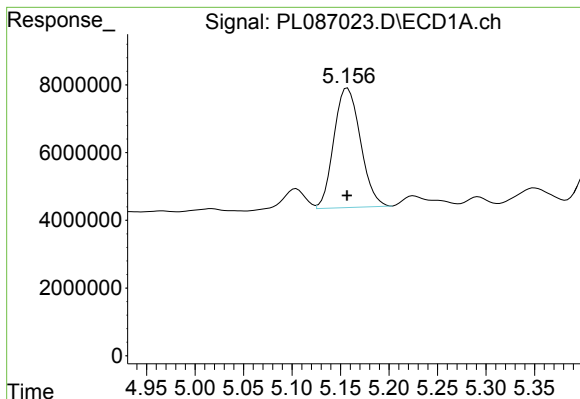

#24 Chlordane-2


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 67227730
Conc: 512.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120623CHLOR

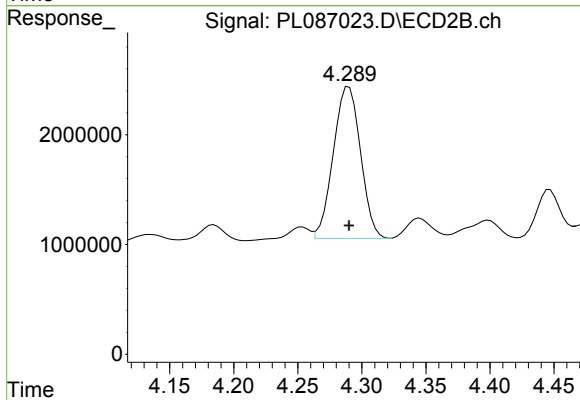


#24 Chlordane-2

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 20399663
Conc: 500.64 ng/ml

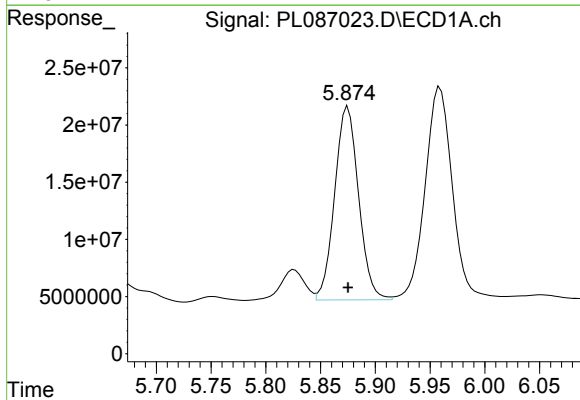


#25 Chlordane-3

R.T.: 5.875 min
Delta R.T.: 0.000 min
Response: 257183924
Conc: 514.40 ng/ml

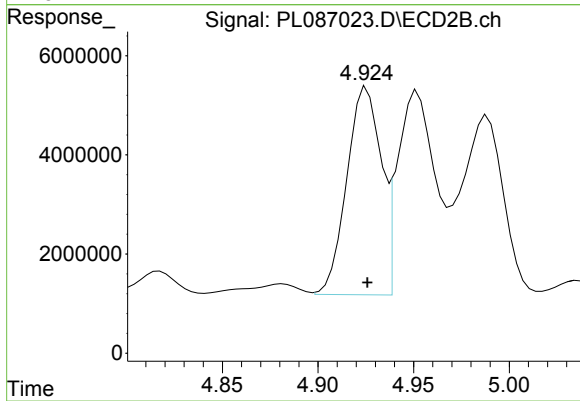

#25 Chlordane-3


R.T.: 4.925 min
Delta R.T.: 0.000 min
Response: 52093324
Conc: 500.57 ng/ml

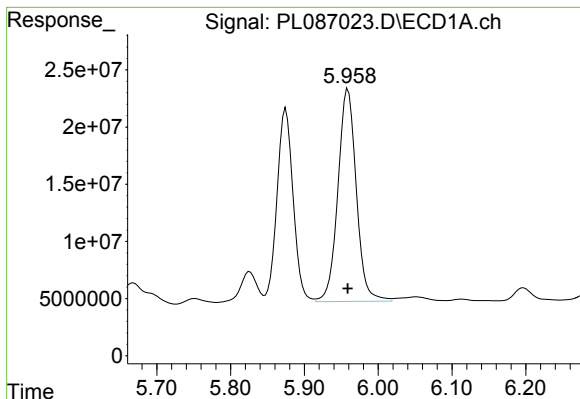

#26 Chlordane-4


R.T.: 5.959 min
Delta R.T.: 0.000 min
Response: 322218250
Conc: 514.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120623CHLOR

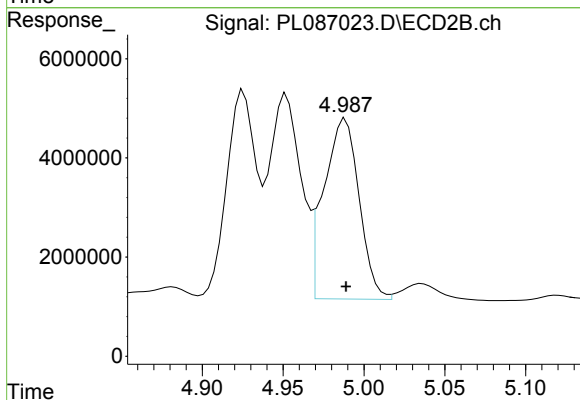


#26 Chlordane-4

R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 54960715
Conc: 501.47 ng/ml

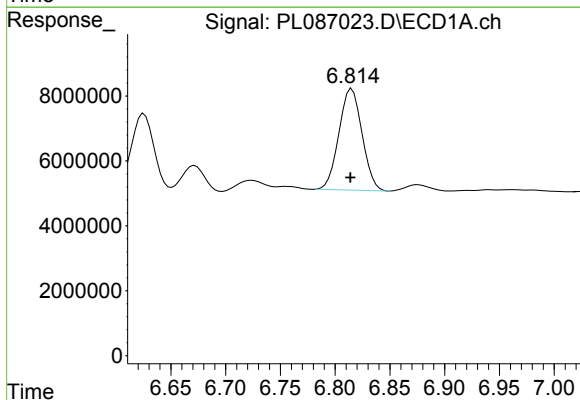


#27 Chlordane-5

R.T.: 6.815 min
Delta R.T.: 0.001 min
Response: 45992159
Conc: 512.77 ng/ml

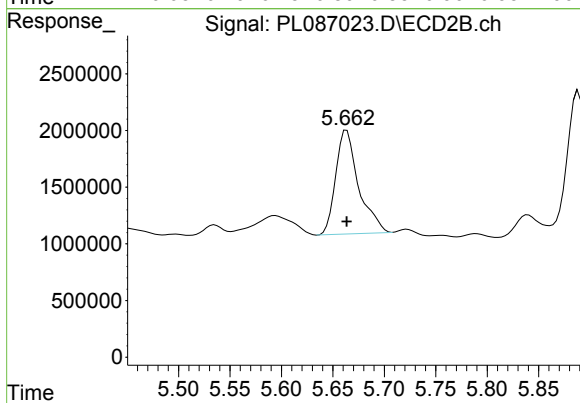

#27 Chlordane-5


R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 14244395
Conc: 494.24 ng/ml

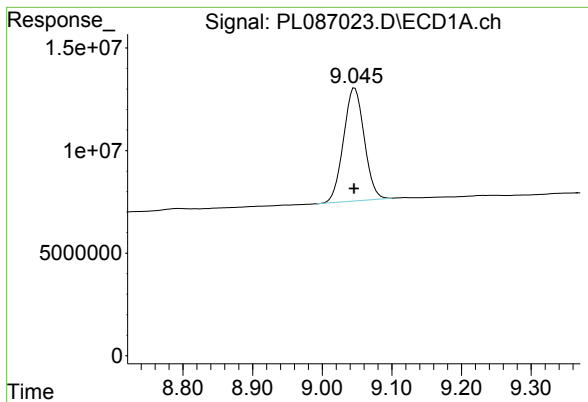

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.001 min
Response: 113693988
Conc: 50.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL120623CHLOR

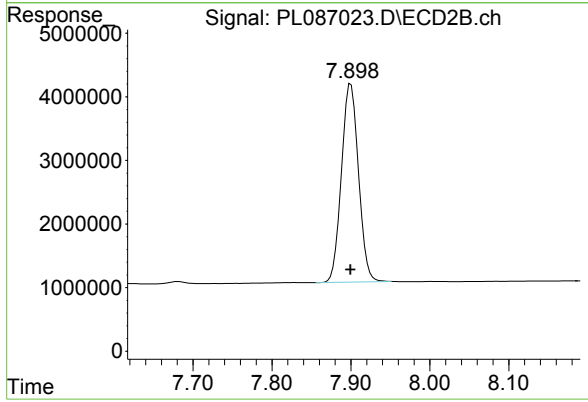

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 46803946
Conc: 49.82 ng/ml