

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120718\
 Data File : PL042871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2018 11:21
 Operator : AJ\SJ
 Sample : J6194-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 13:08:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	123.8E6	62348559	20.185	21.036
28)	SA Decachlor...	8.200	9.226	117.4E6	50154763	17.986	19.227
Target Compounds							
3)	MA gamma-BHC...	4.197	0.000	2324919	0	0.269	N.D. #
6)	B beta-BHC	4.397f	0.000	5194349	0	1.408	N.D. #
7)	B delta-BHC	0.000	5.145f	0	6661441	N.D.	1.550 #
8)	B Heptachlo...	0.000	5.991	0	2183907	N.D.	0.576 #
9)	A Endosulfan I	5.538	0.000	1691127	0	0.231	N.D. #
10)	B gamma-Chl...	0.000	6.232	0	2328488	N.D.	0.634 #
14)	MA Endrin	6.065f	0.000	898664	0	0.125	N.D. #
23)	Chlordane-1	4.362	5.145	2412605	6661441	8.979	47.133 #
25)	Chlordane-3	0.000	6.232	0	2328488	N.D.	4.742 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120718\
Data File : PL042871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2018 11:21
Operator : AJ\SJ
Sample : J6194-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 13:08:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

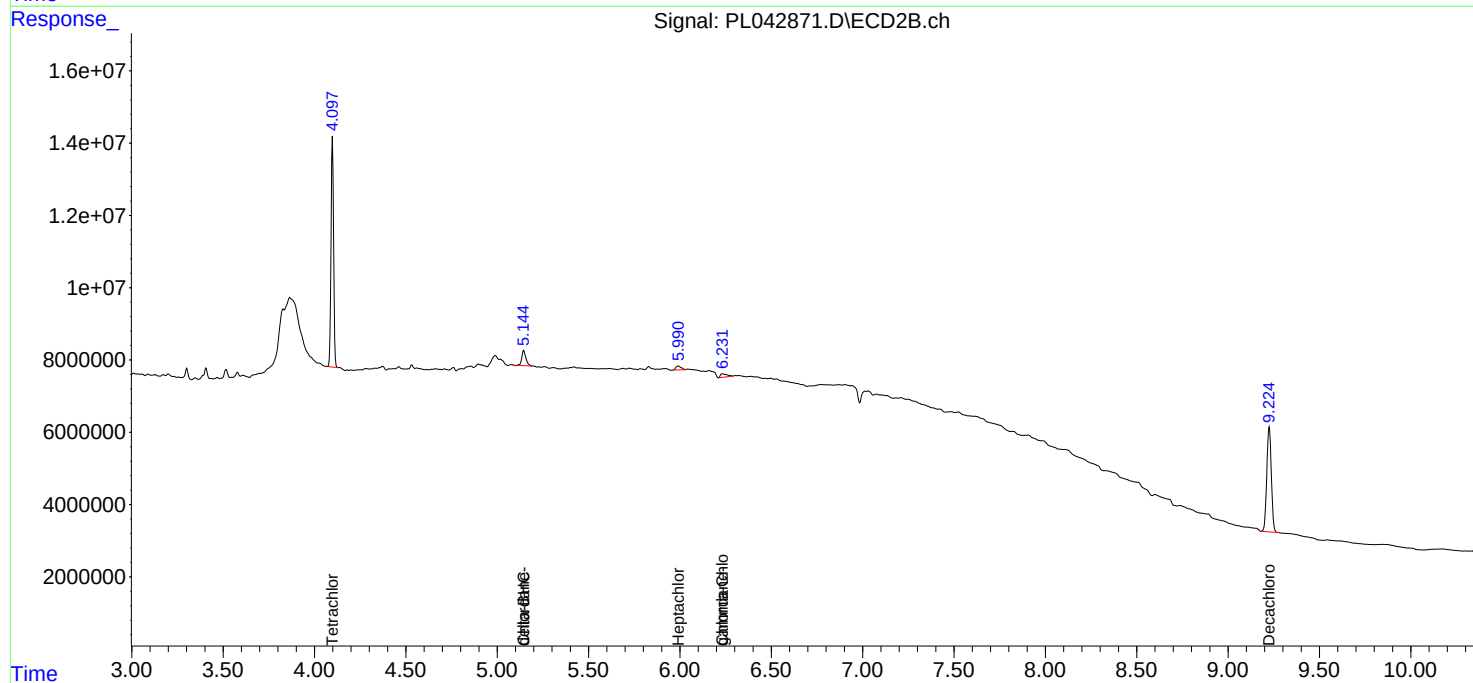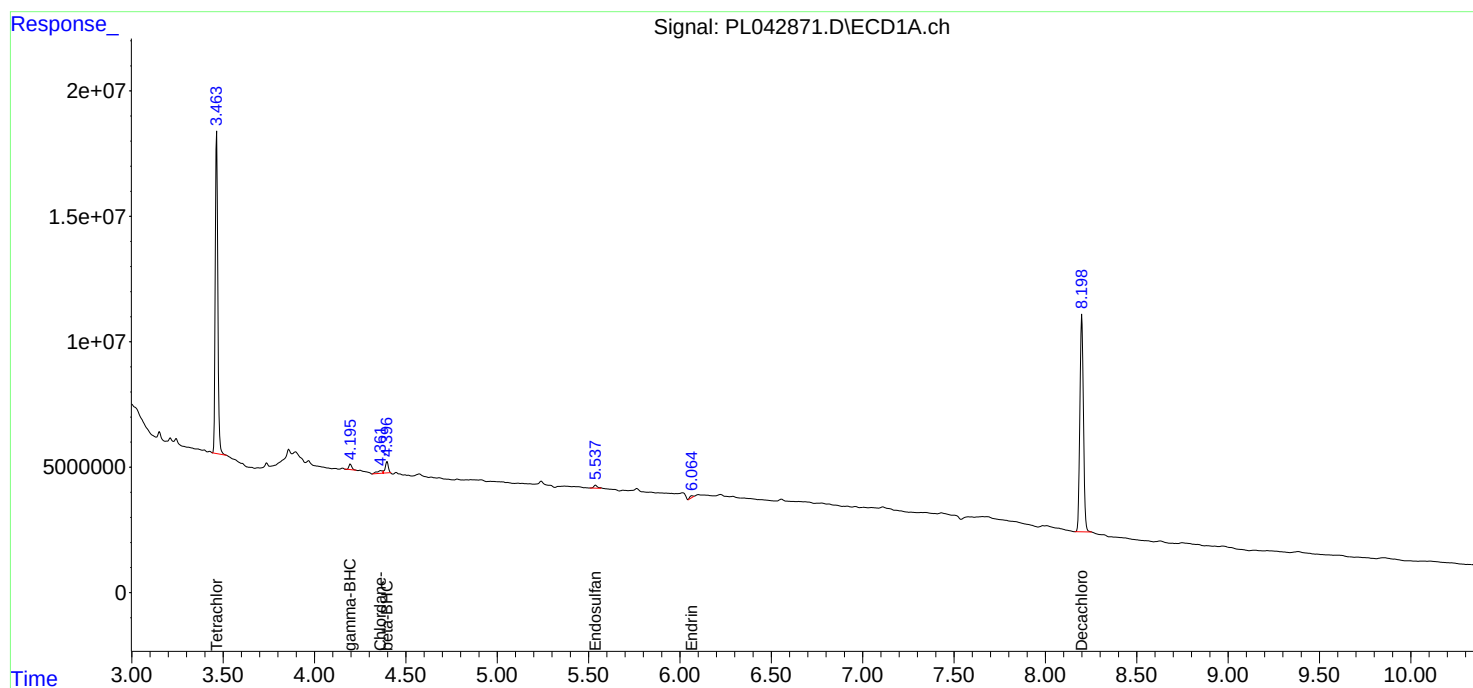


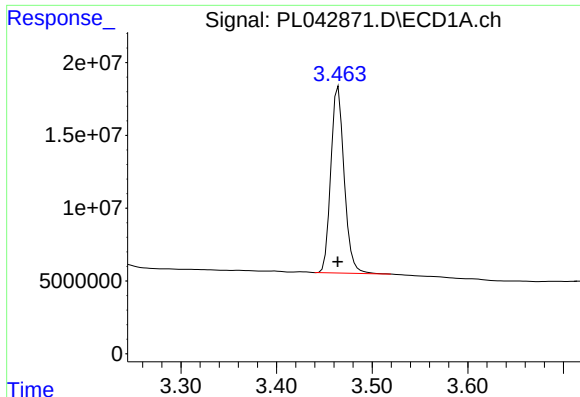

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 123791863
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

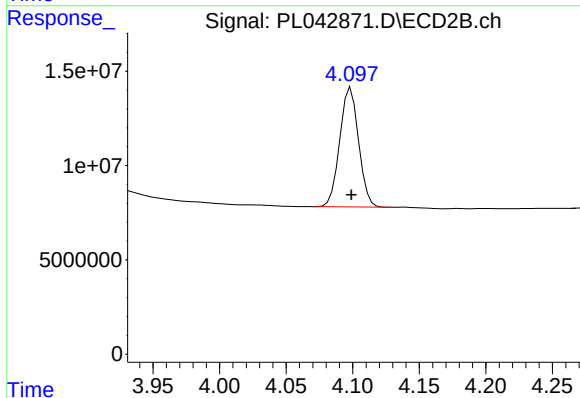


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 62348559
Conc: 21.04 ng/ml

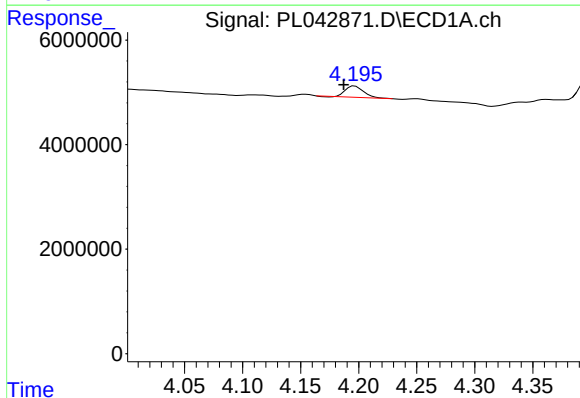


#3 gamma-BHC (Lindane)

R.T.: 4.197 min
Delta R.T.: 0.010 min
Response: 2324919
Conc: 0.27 ng/ml

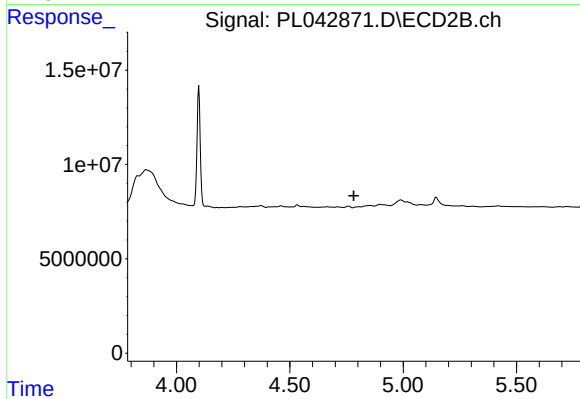

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

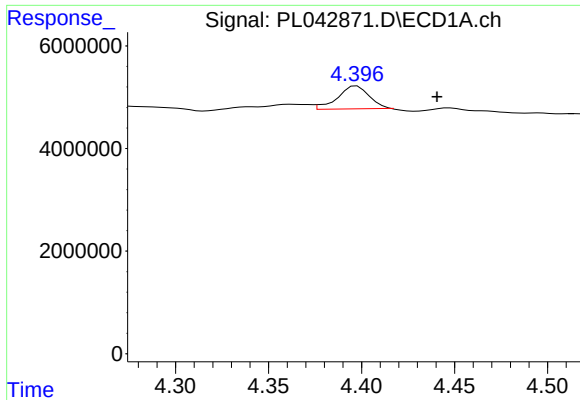

#6 beta-BHC


R.T.: 4.397 min
Delta R.T.: -0.043 min
Response: 5194349
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

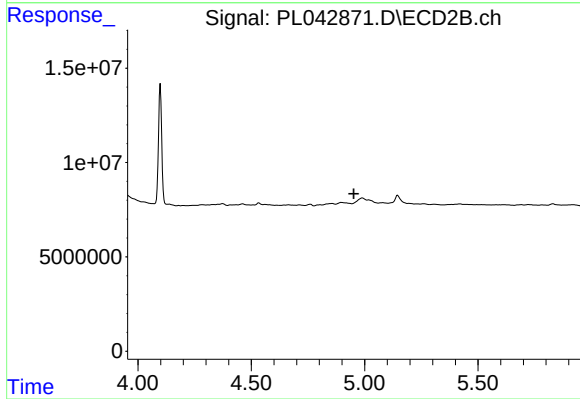


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

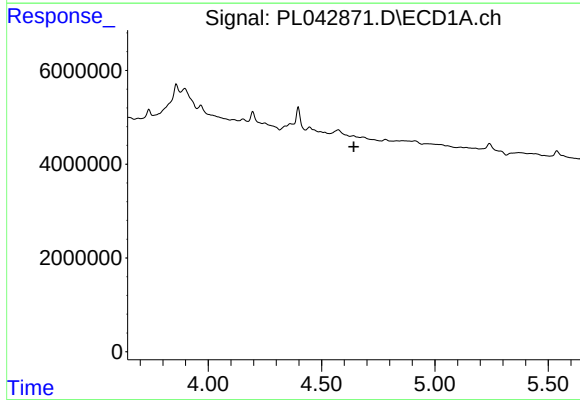


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

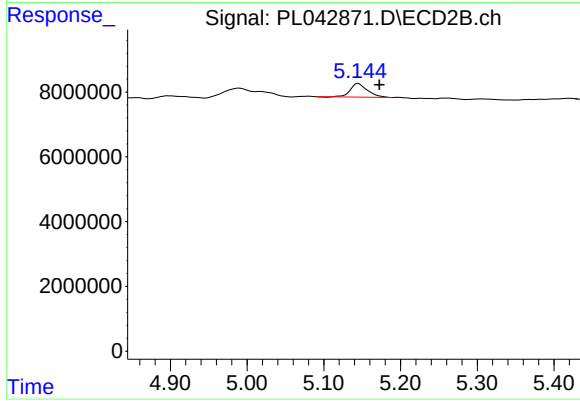

#7 delta-BHC


R.T.: 5.145 min
Delta R.T.: -0.027 min
Response: 6661441
Conc: 1.55 ng/ml

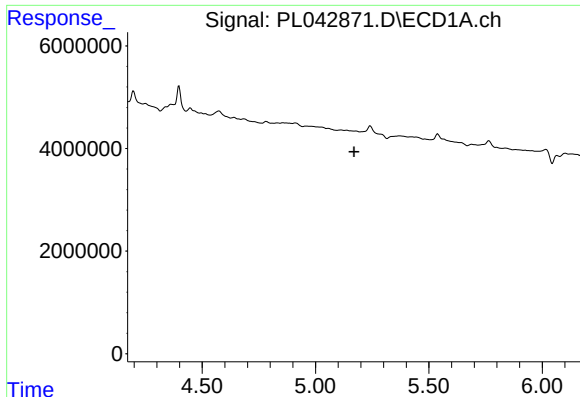

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

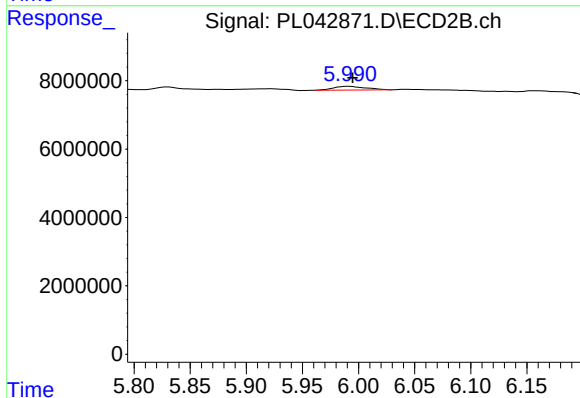


#8 Heptachlor epoxide

R.T.: 5.991 min
Delta R.T.: -0.003 min
Response: 2183907
Conc: 0.58 ng/ml

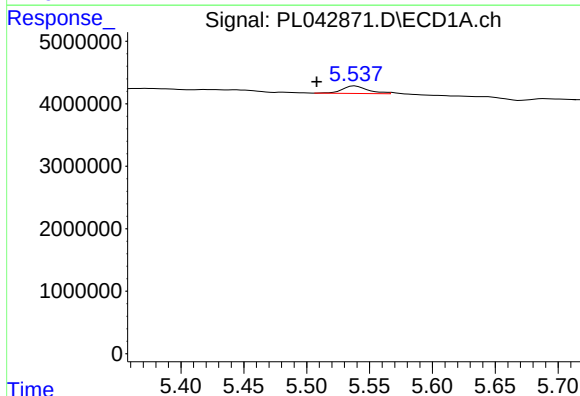


#9 Endosulfan I

R.T.: 5.538 min
Delta R.T.: 0.030 min
Response: 1691127
Conc: 0.23 ng/ml

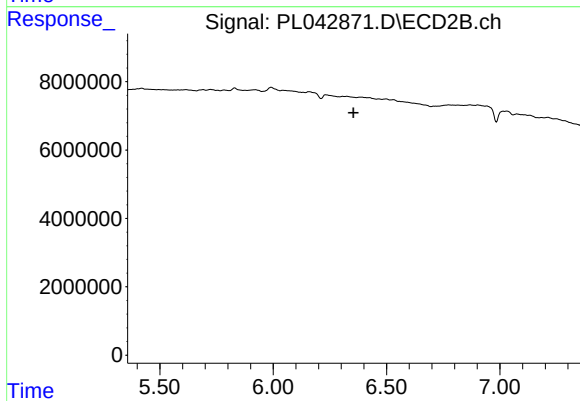

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.354 min
Response: 0
Conc: N.D.

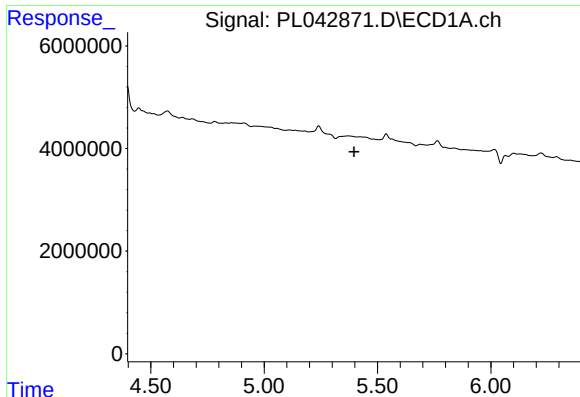

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

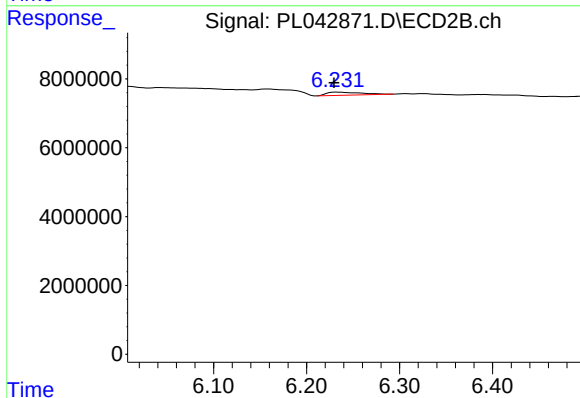


#10 gamma-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.002 min
Response: 2328488
Conc: 0.63 ng/ml

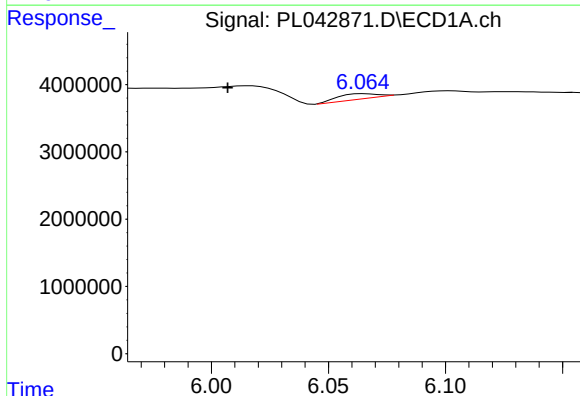


#14 Endrin

R.T.: 6.065 min
Delta R.T.: 0.058 min
Response: 898664
Conc: 0.12 ng/ml

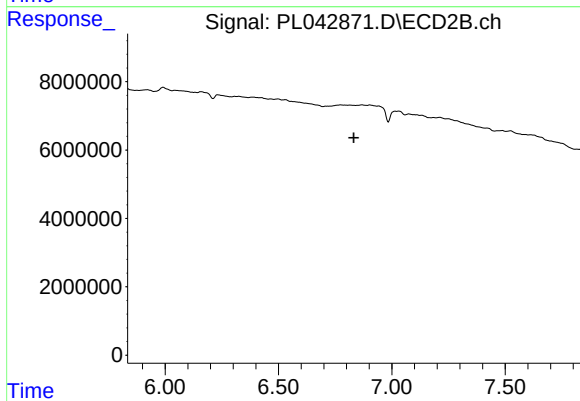

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.832 min
Response: 0
Conc: N.D.

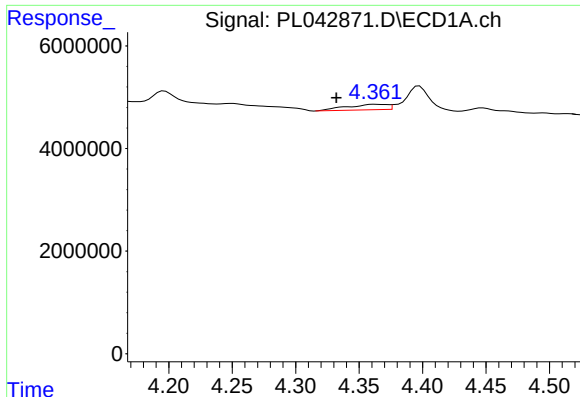

#23 Chlordane-1


R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 2412605
Conc: 8.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

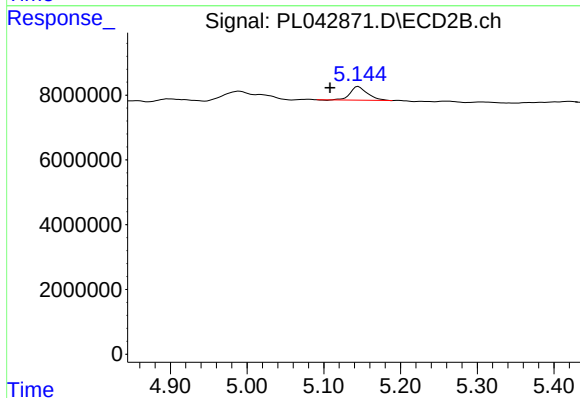


#23 Chlordane-1

R.T.: 5.145 min
Delta R.T.: 0.037 min
Response: 6661441
Conc: 47.13 ng/ml

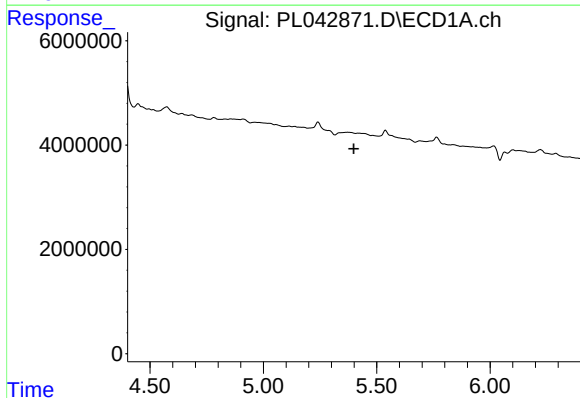


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

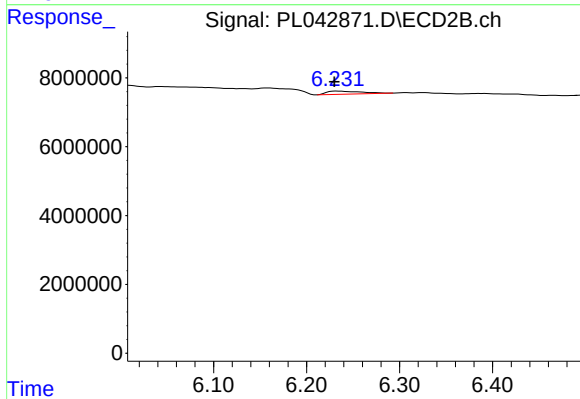

#25 Chlordane-3


R.T.: 6.232 min
Delta R.T.: 0.002 min
Response: 2328488
Conc: 4.74 ng/ml

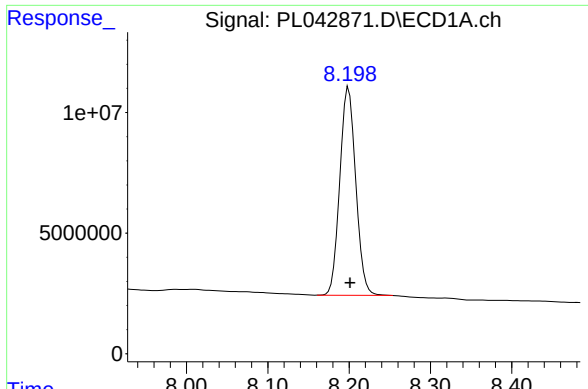

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.002 min
Response: 117446624
Conc: 17.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

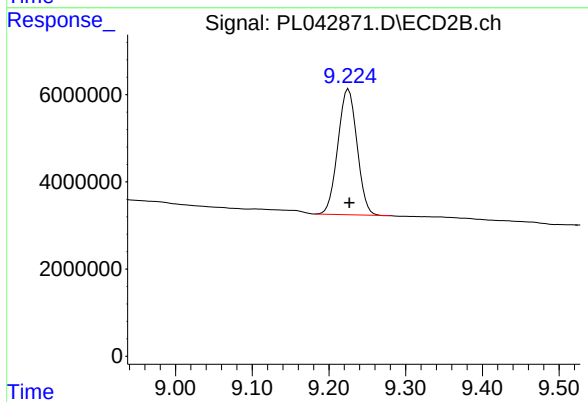

#28 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: -0.001 min
Response: 50154763
Conc: 19.23 ng/ml