

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120718\
 Data File : PL042877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2018 12:46
 Operator : AJ\SJ
 Sample : J6233-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 13:09:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.099	122.8E6	60233261	20.030	20.322
28)	SA Decachlor...	8.201	9.227	134.1E6	55233021	20.531	21.174
Target Compounds							
3)	MA gamma-BHC...	4.154f	0.000	847394	0	0.098	N.D. #
6)	B beta-BHC	4.399f	0.000	4007633	0	1.087	N.D. #
7)	B delta-BHC	0.000	5.146f	0	6391948	N.D.	1.487 #
8)	B Heptachlo...	0.000	5.992	0	3323323	N.D.	0.876 #
10)	B gamma-Chl...	0.000	6.234	0	1503828	N.D.	0.409 #
11)	B alpha-Chl...	0.000	6.234f	0	1503828	N.D.	0.418 #
14)	MA Endrin	6.065f	6.785f	817128	2135265	0.113	0.684 #
23)	Chlordane-1	4.363	5.146	1602783	6391948	5.965	45.226 #
25)	Chlordane-3	0.000	6.234	0	1503828	N.D.	3.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120718\
Data File : PL042877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2018 12:46
Operator : AJ\SJ
Sample : J6233-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 13:09:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

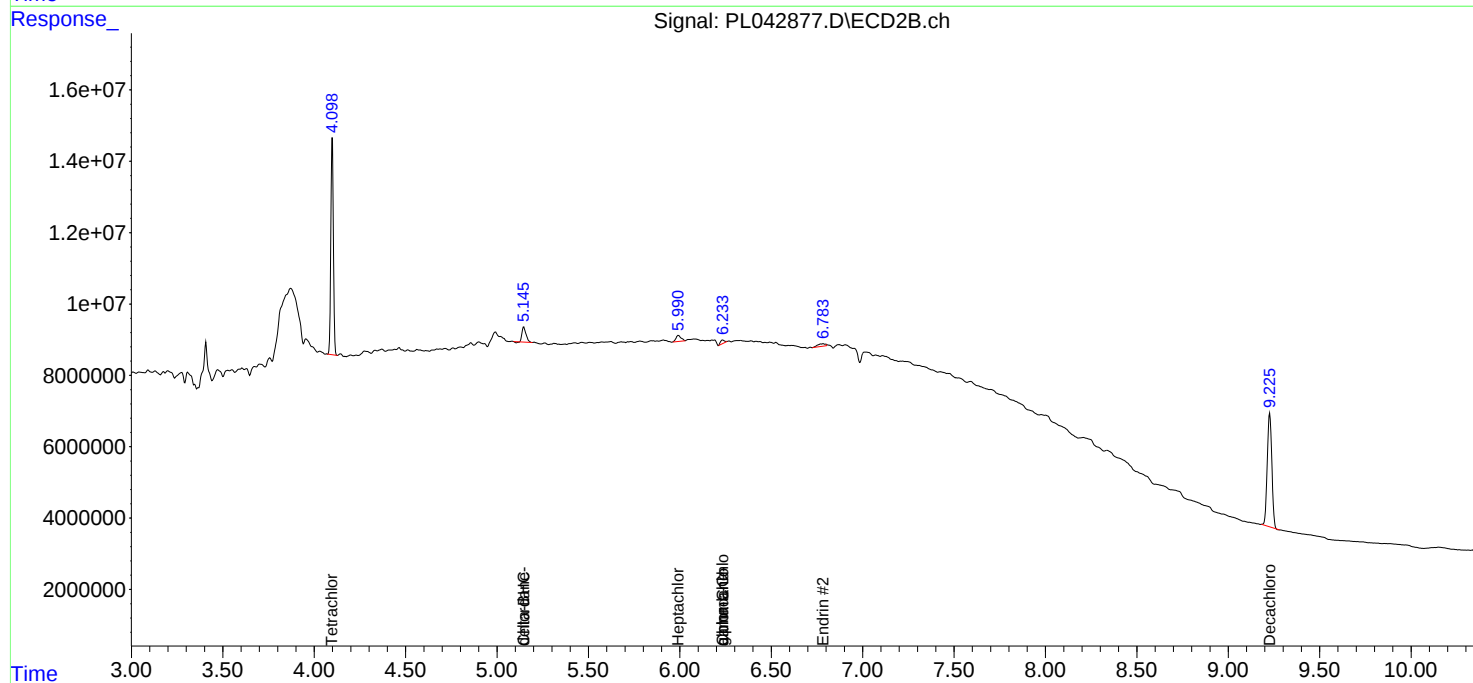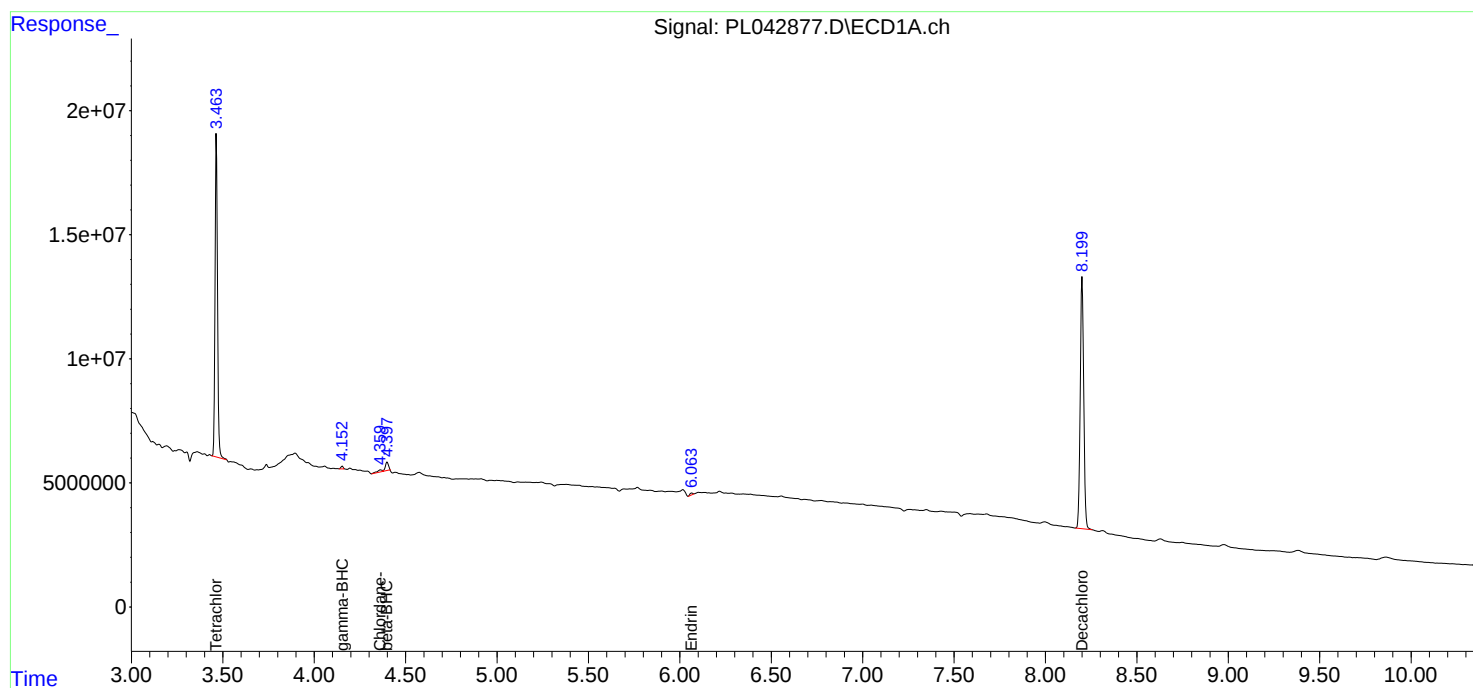


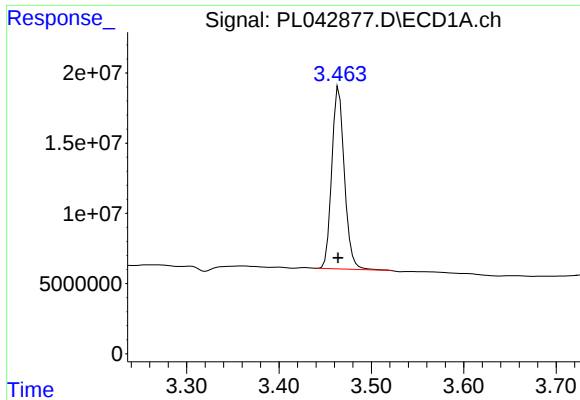

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 122843461
Conc: 20.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

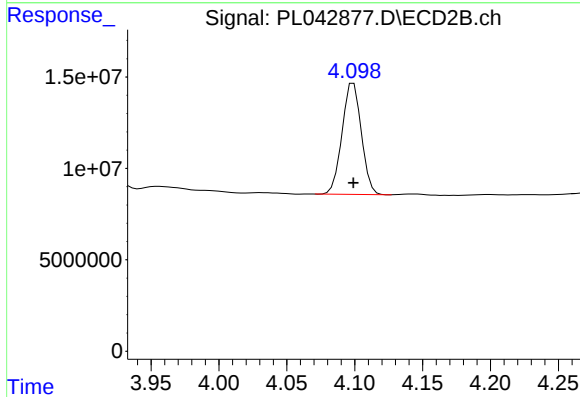


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 60233261
Conc: 20.32 ng/ml

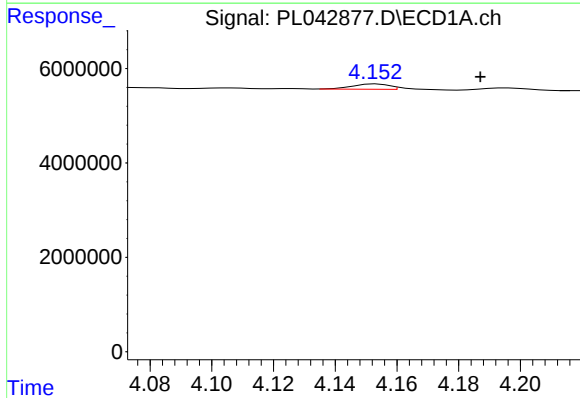


#3 gamma-BHC (Lindane)

R.T.: 4.154 min
Delta R.T.: -0.033 min
Response: 847394
Conc: 0.10 ng/ml

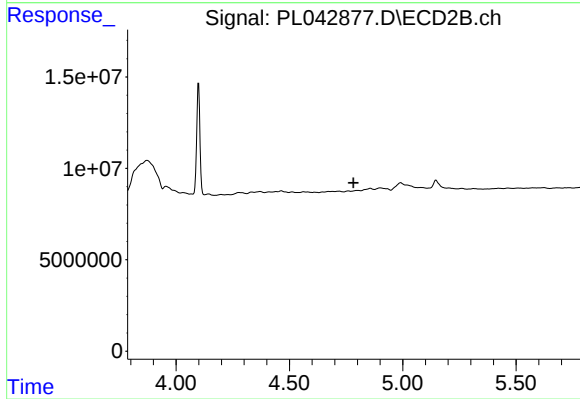

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.783 min
Response: 0
Conc: N.D.

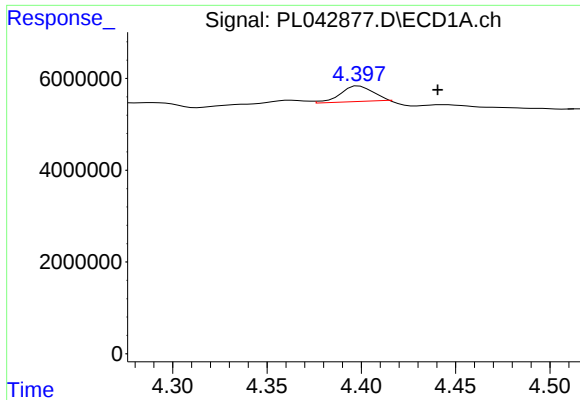

#6 beta-BHC


R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 4007633
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

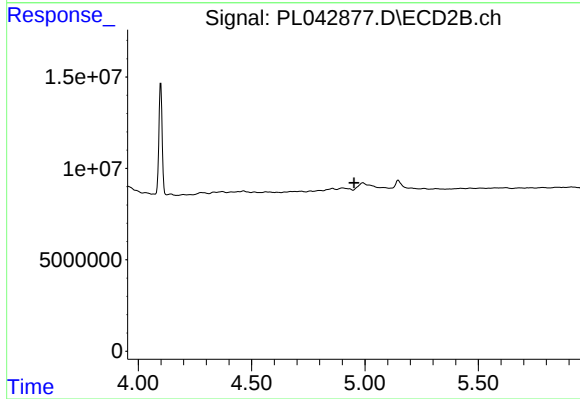


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

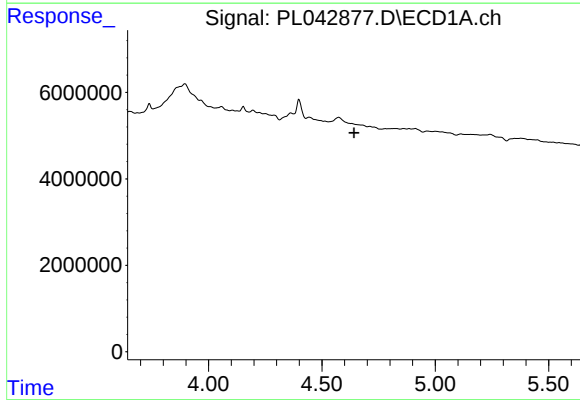


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

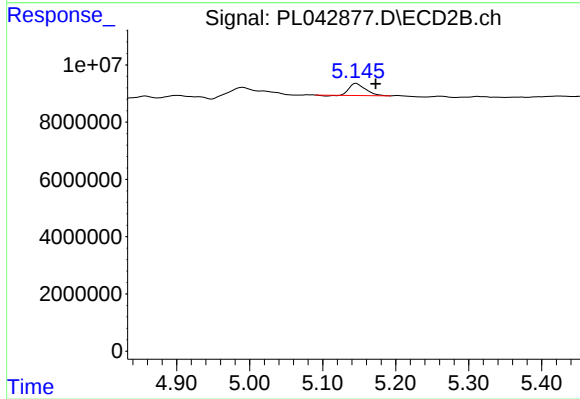

#7 delta-BHC


R.T.: 5.146 min
Delta R.T.: -0.026 min
Response: 6391948
Conc: 1.49 ng/ml

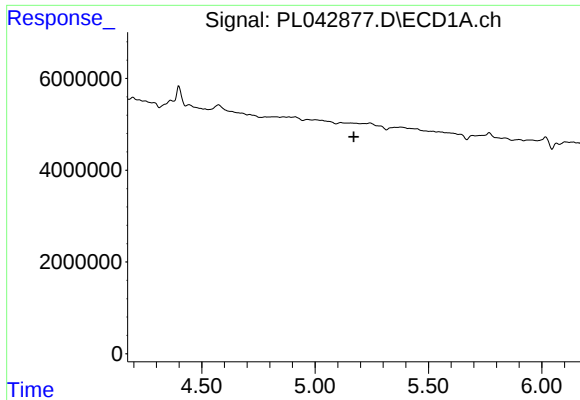

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

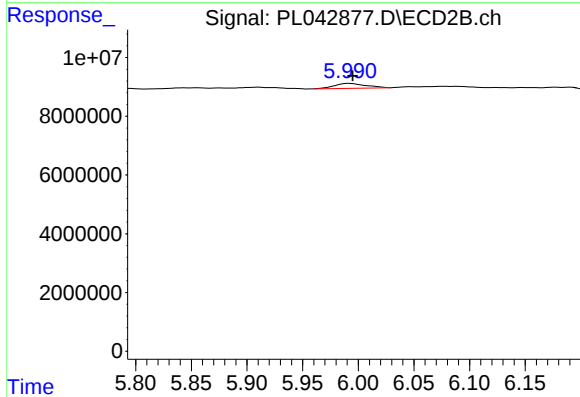


#8 Heptachlor epoxide

R.T.: 5.992 min
Delta R.T.: -0.003 min
Response: 3323323
Conc: 0.88 ng/ml

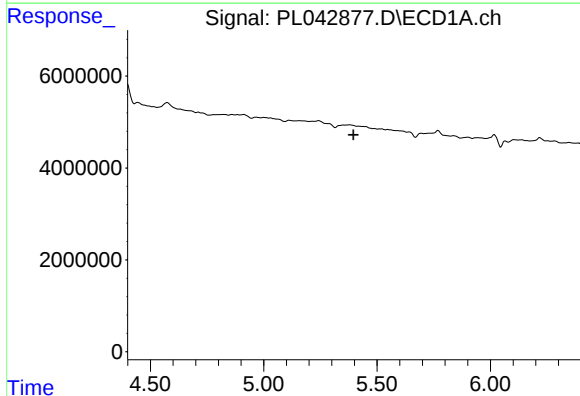


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

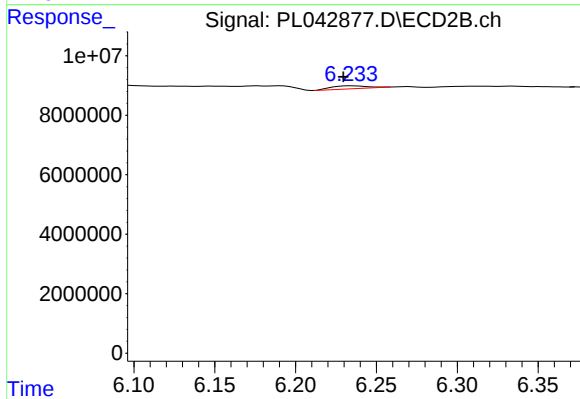

#10 gamma-Chlordane


R.T.: 6.234 min
Delta R.T.: 0.005 min
Response: 1503828
Conc: 0.41 ng/ml

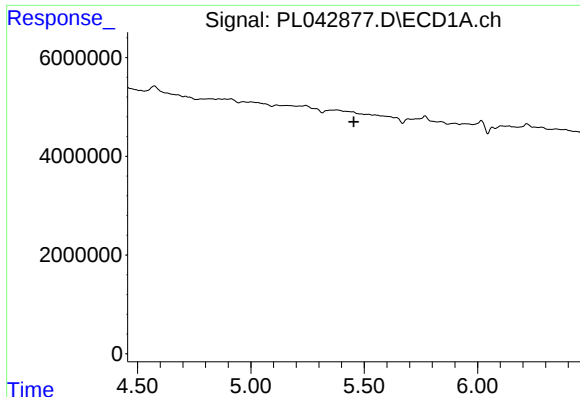

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

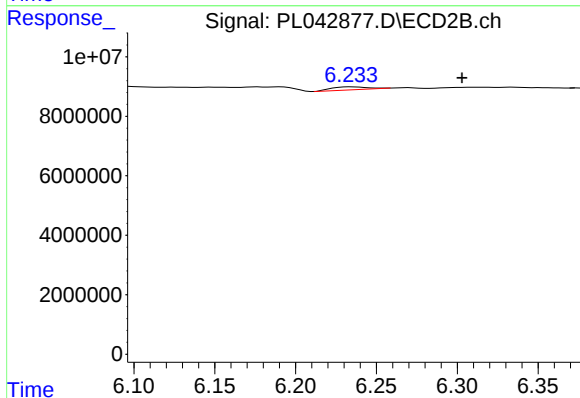


#11 alpha-Chlordane

R.T.: 6.234 min
Delta R.T.: -0.069 min
Response: 1503828
Conc: 0.42 ng/ml

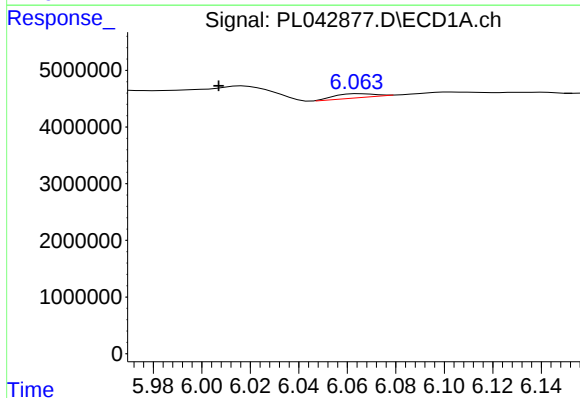


#14 Endrin

R.T.: 6.065 min
Delta R.T.: 0.058 min
Response: 817128
Conc: 0.11 ng/ml

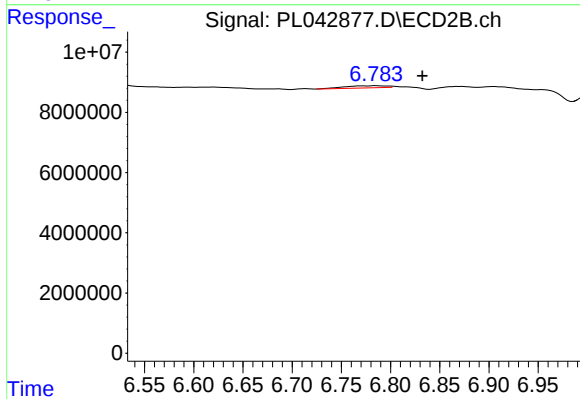

#14 Endrin


R.T.: 6.785 min
Delta R.T.: -0.048 min
Response: 2135265
Conc: 0.68 ng/ml

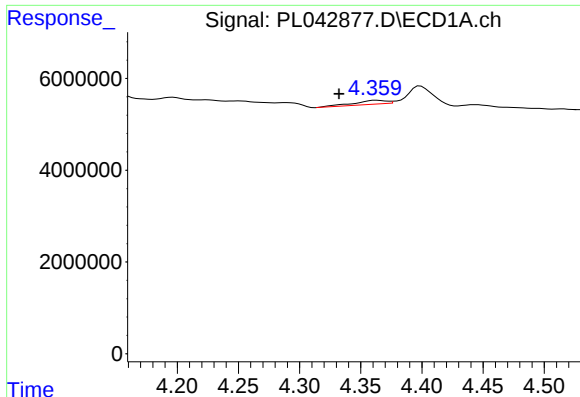

#23 Chlordane-1


R.T.: 4.363 min
Delta R.T.: 0.030 min
Response: 1602783
Conc: 5.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

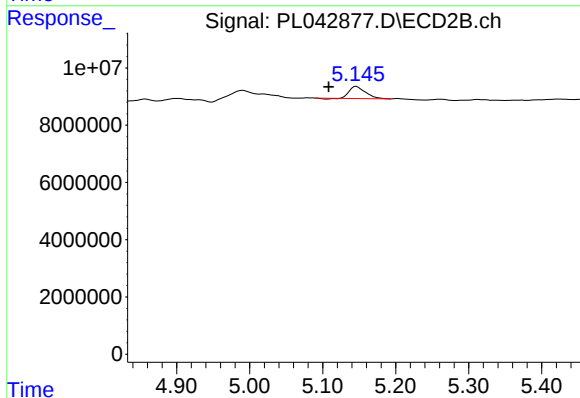


#23 Chlordane-1

R.T.: 5.146 min
Delta R.T.: 0.038 min
Response: 6391948
Conc: 45.23 ng/ml

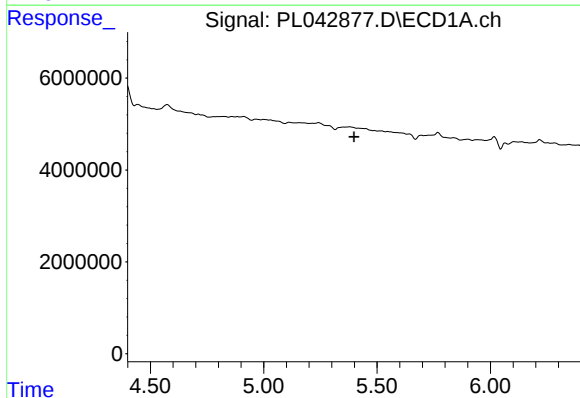


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

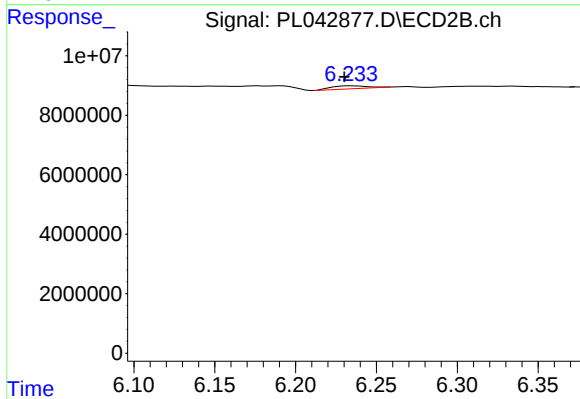

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: 0.004 min
Response: 1503828
Conc: 3.06 ng/ml

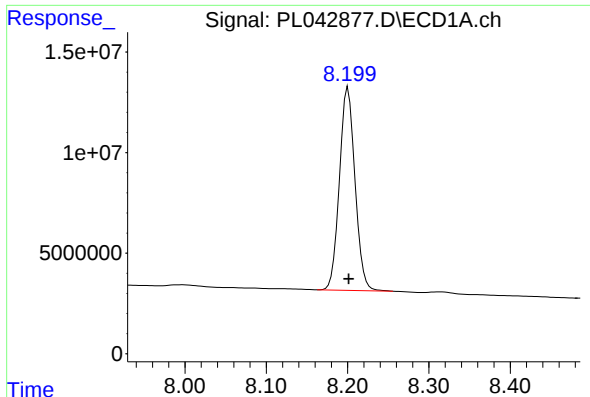

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 134068860
Conc: 20.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

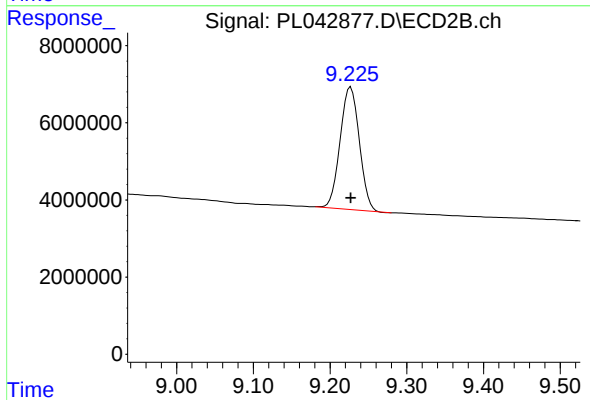

#28 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 55233021
Conc: 21.17 ng/ml