

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120721\
 Data File : PL071293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2021 08:47
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 01:52:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	7.972	0	2007909	N.D. 1.264 #
10) B	gamma-Chl...	7.268	0.000	624364	0	N.D. #
11) B	alpha-Chl...	7.352	0.000	131959	0	N.D. #
12) B	4,4'-DDE	7.551	0.000	39635	0	N.D. #
15) B	Endosulfa...	0.000	9.135	0	1909448	N.D. 1.417 #
17) MA	4,4'-DDT	8.418	9.366	471783	1193658	0.862 0.858
21) B	Endrin ke...	9.204f	0.000	4045244	0	N.D. #
22)	Mirex	0.000	10.455	0	1050326	N.D. 0.963 #
25)	Chlordane-3	7.268	0.000	624364	0	N.D. #
26)	Chlordane-4	7.352	0.000	131959	0	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120721\
Data File : PL071293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2021 08:47
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 01:52:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

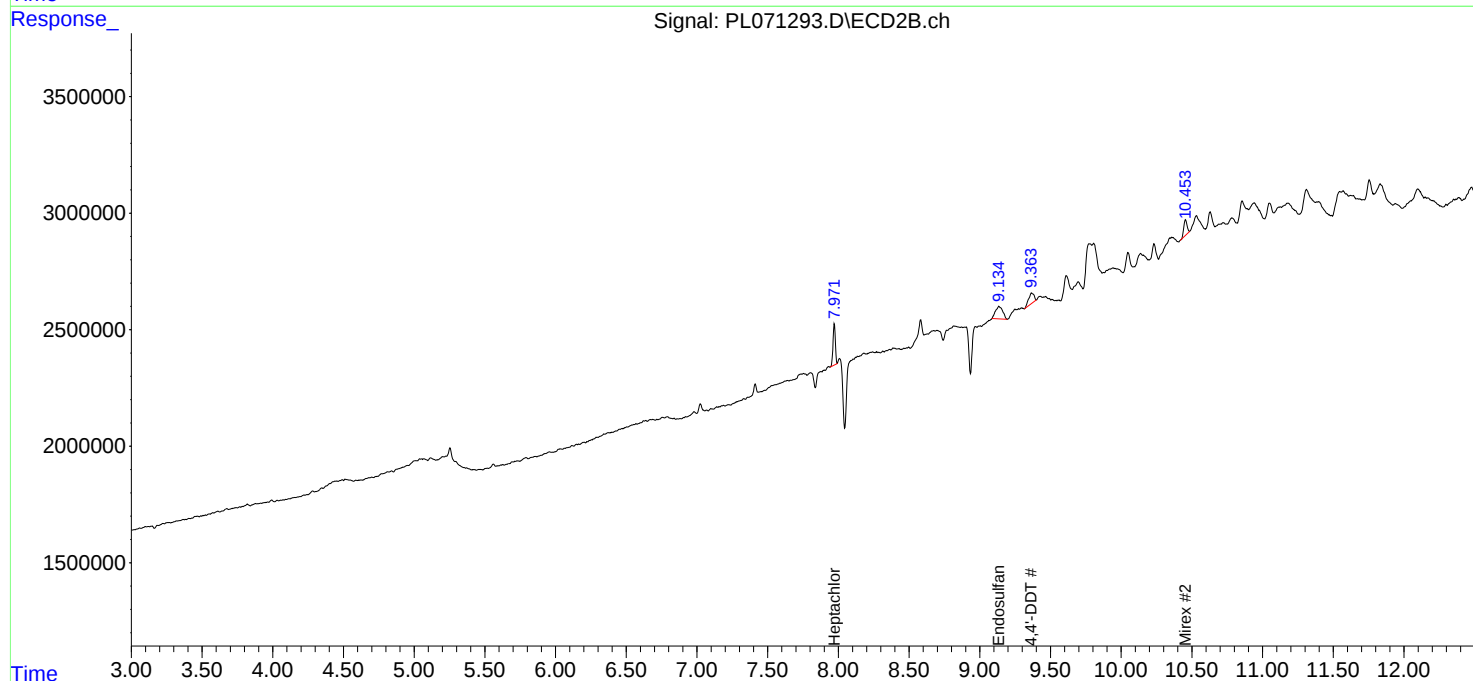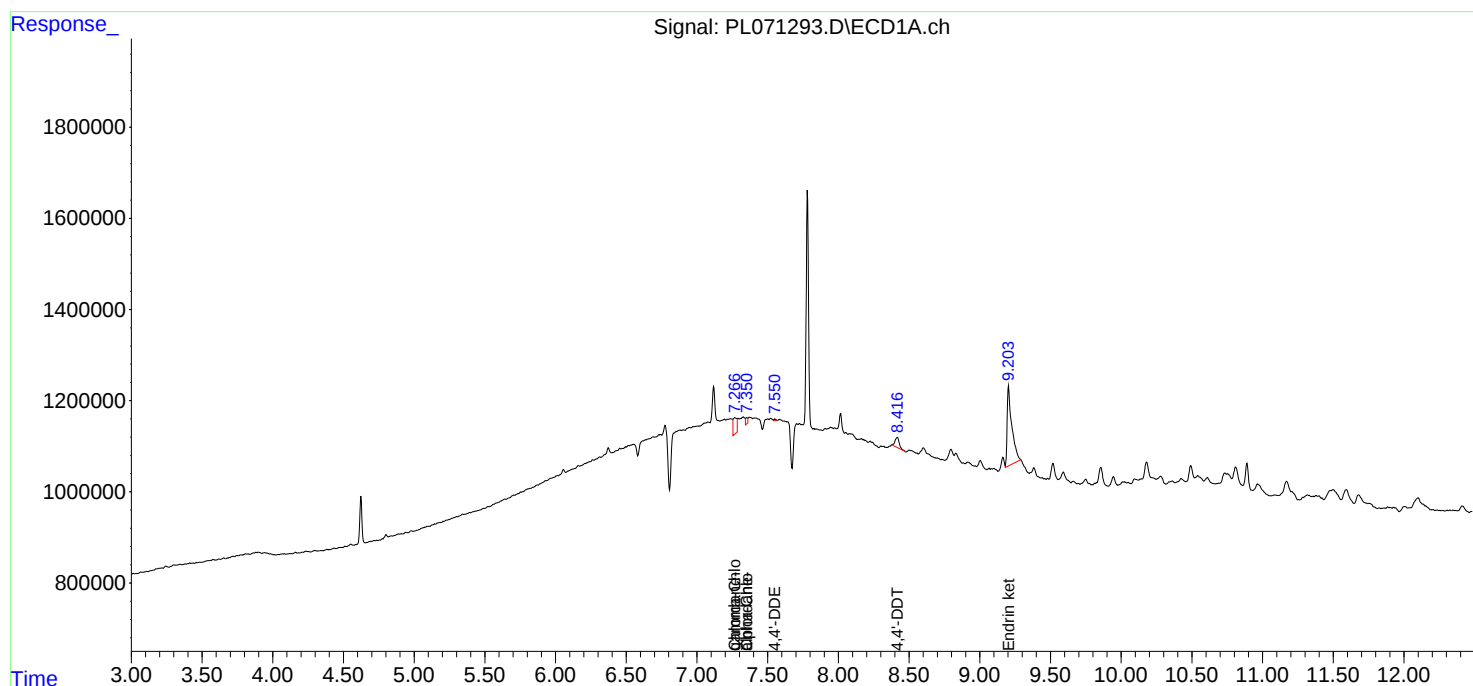


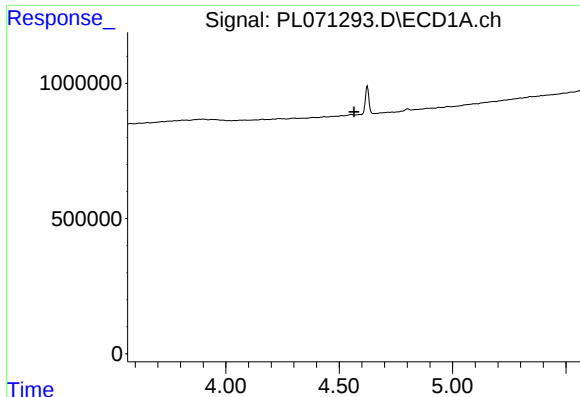

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

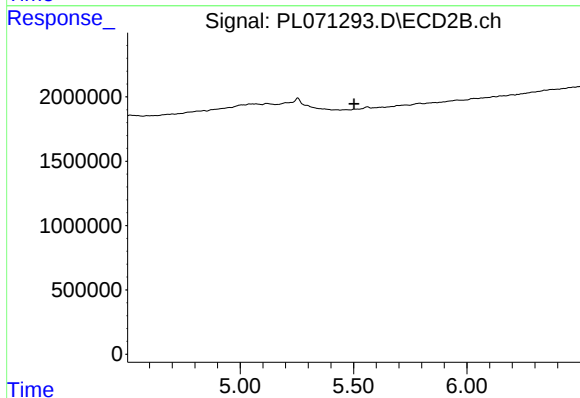


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

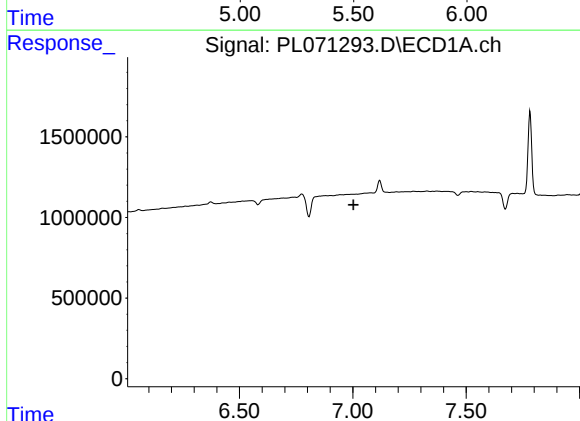


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.003 min
Response: 0
Conc: N.D.

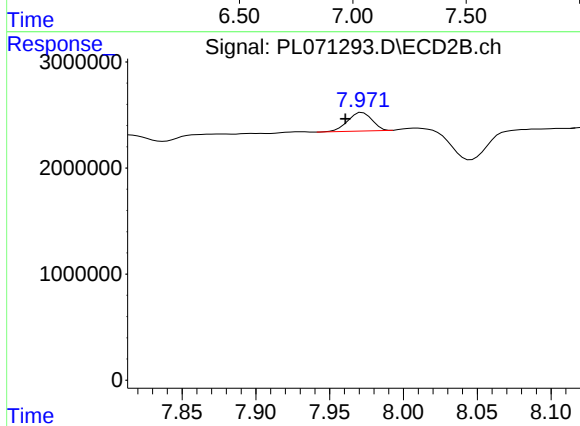

#8 Heptachlor epoxide


R.T.: 7.972 min
Delta R.T.: 0.011 min
Response: 2007909
Conc: 1.26 ng/ml

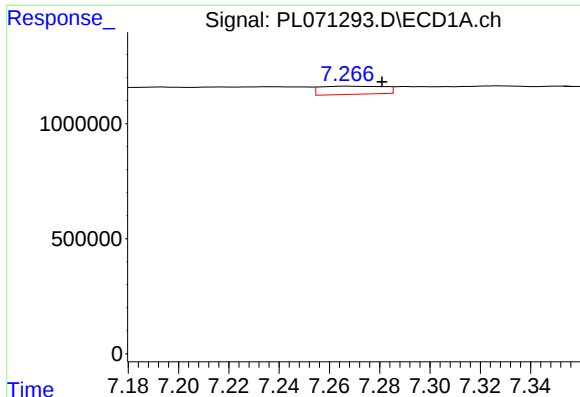

#10 gamma-Chlordane


R.T.: 7.268 min
Delta R.T.: -0.013 min
Response: 624364
Conc: 0.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

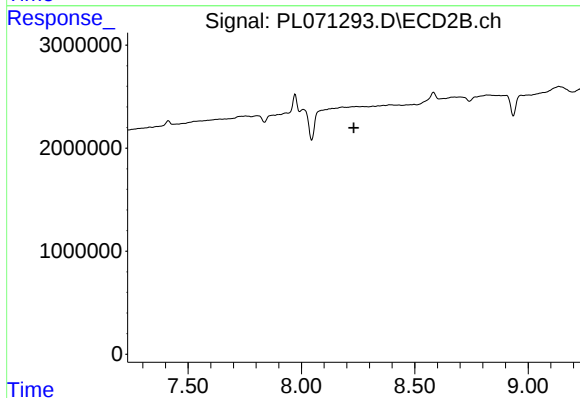


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

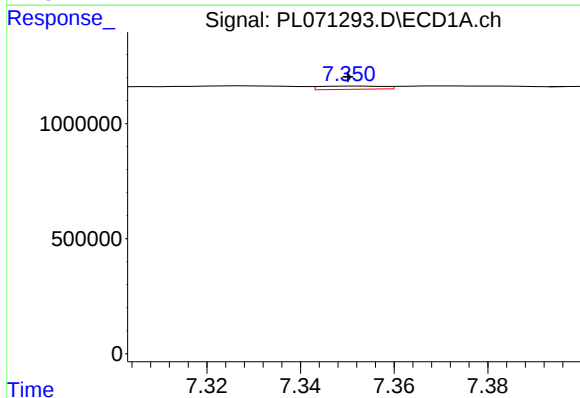


#11 alpha-Chlordane

R.T.: 7.352 min
Delta R.T.: 0.002 min
Response: 131959
Conc: 0.21 ng/ml

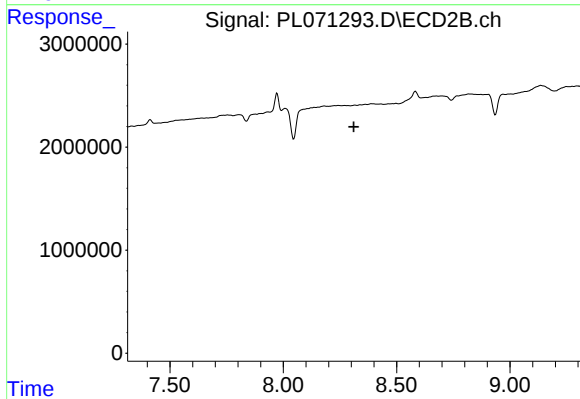

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

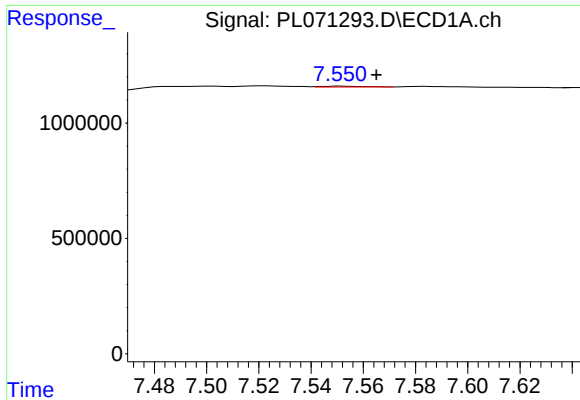

#12 4,4'-DDE


R.T.: 7.551 min
Delta R.T.: -0.014 min
Response: 39635
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

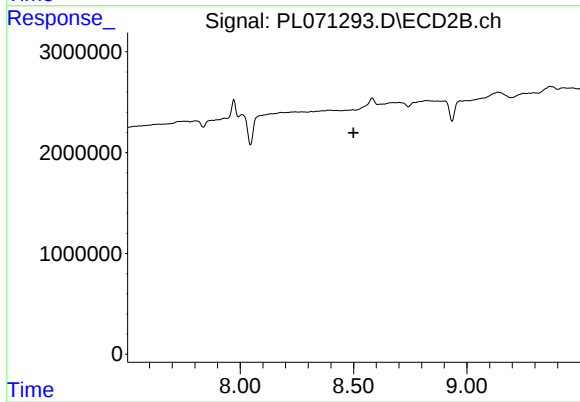


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.500 min
Response: 0
Conc: N.D.

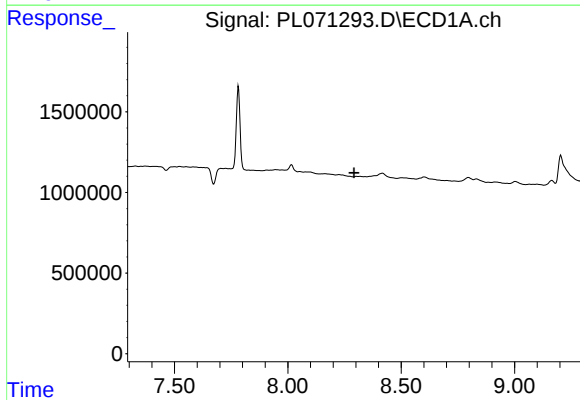


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.293 min
Response: 0
Conc: N.D.

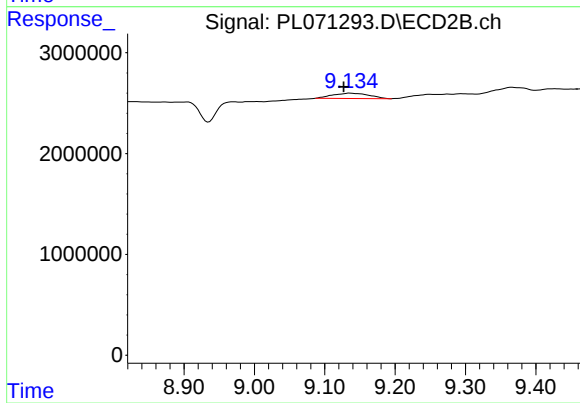

#15 Endosulfan II


R.T.: 9.135 min
Delta R.T.: 0.008 min
Response: 1909448
Conc: 1.42 ng/ml

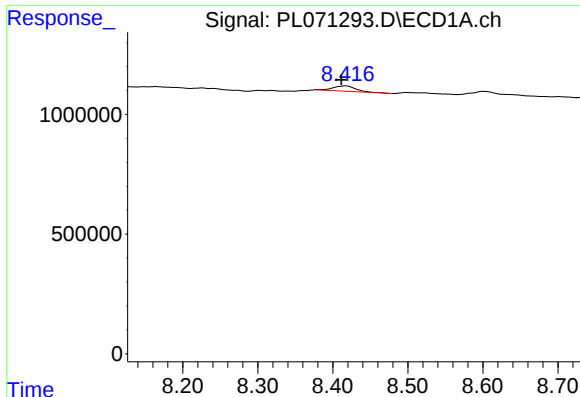

#17 4,4'-DDT


R.T.: 8.418 min
Delta R.T.: 0.006 min
Response: 471783
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

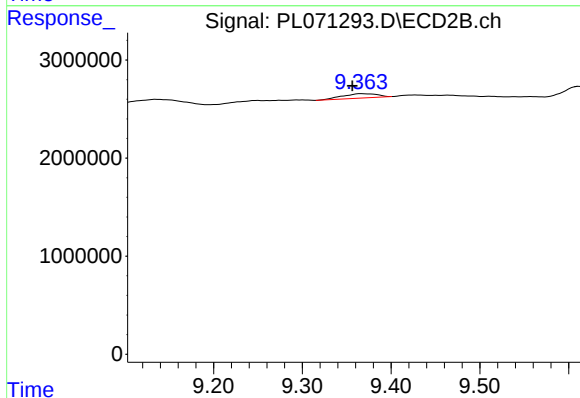


#17 4,4'-DDT

R.T.: 9.366 min
Delta R.T.: 0.010 min
Response: 1193658
Conc: 0.86 ng/ml

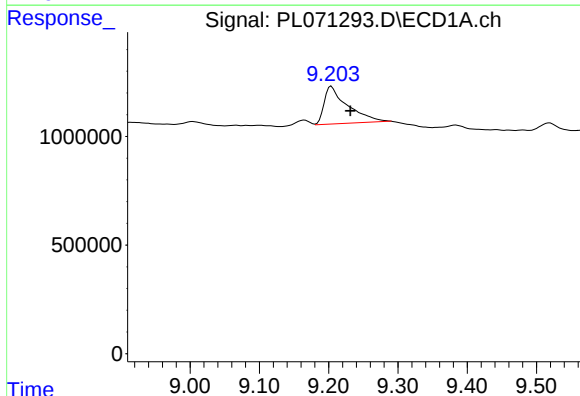


#21 Endrin ketone

R.T.: 9.204 min
Delta R.T.: -0.027 min
Response: 4045244
Conc: 5.68 ng/ml

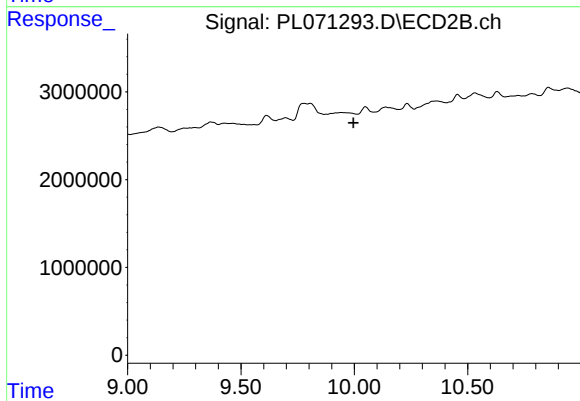

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.997 min
Response: 0
Conc: N.D.

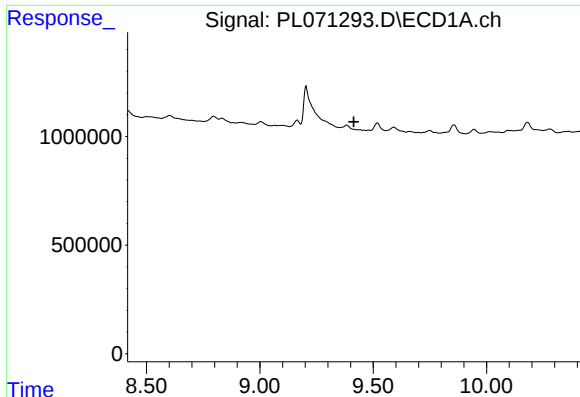

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

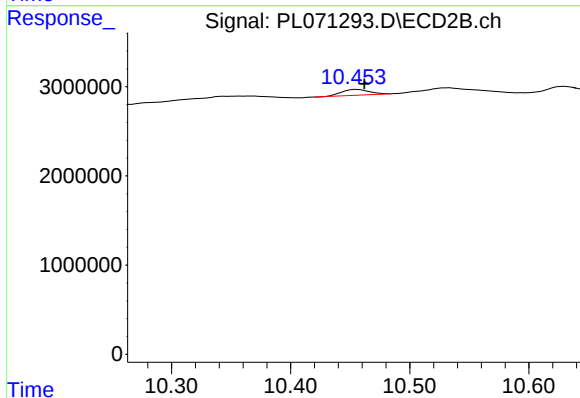


#22 Mirex

R.T.: 10.455 min
Delta R.T.: -0.007 min
Response: 1050326
Conc: 0.96 ng/ml

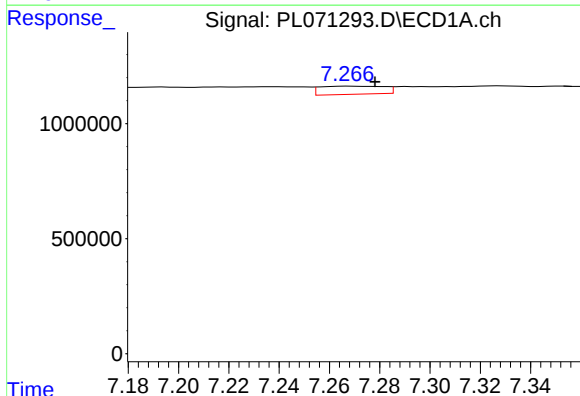


#25 Chlordane-3

R.T.: 7.268 min
Delta R.T.: -0.011 min
Response: 624364
Conc: 10.07 ng/ml

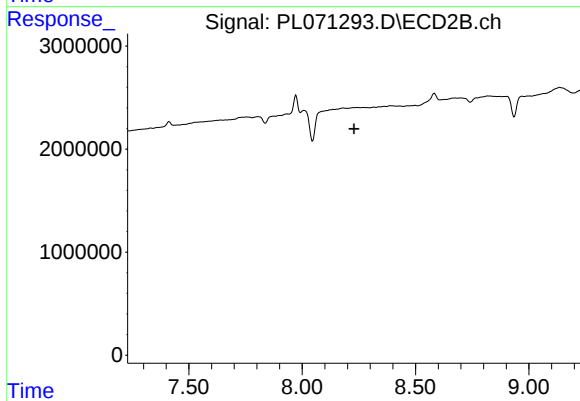

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

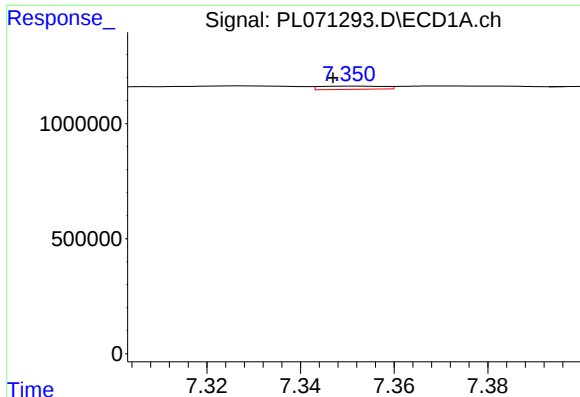

#26 Chlordane-4


R.T.: 7.352 min
Delta R.T.: 0.005 min
Response: 131959
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

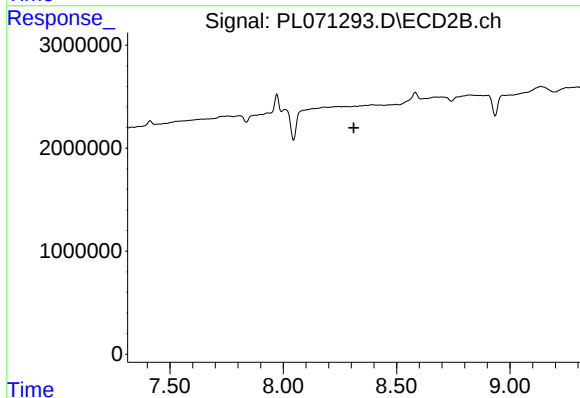


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

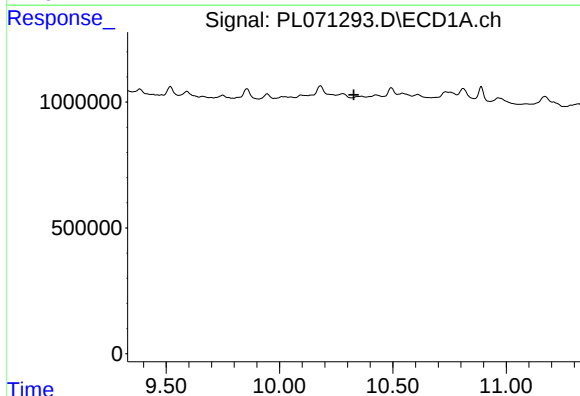

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.328 min
Response: 0
Conc: N.D.

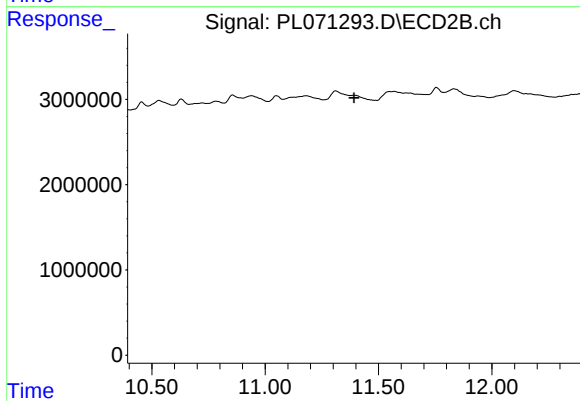

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.