

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120721\
 Data File : PL071300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2021 11:29
 Operator : AR\AJ
 Sample : M4920-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 01:53:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.500	10593022	26798356	22.553	21.355
28)	SA Decachlor...	10.328	11.391	15731929	26907843	21.726	19.358
Target Compounds							
7)	B delta-BHC	0.000	7.019f	0	5477525	N.D.	3.222 #
14)	MA Endrin	0.000	8.915f	0	437133	N.D.	0.326 #
15)	B Endosulfa...	0.000	9.152f	0	1484220	N.D.	1.102 #
18)	B Endrin al...	0.000	9.271	0	445041	N.D.	0.431 #
19)	B Endosulfa...	0.000	9.500	0	2570620	N.D.	1.967 #
27)	Chlordane-5	0.000	9.217f	0	652583	N.D.	13.842 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120721\
Data File : PL071300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2021 11:29
Operator : AR\AJ
Sample : M4920-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 01:53:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

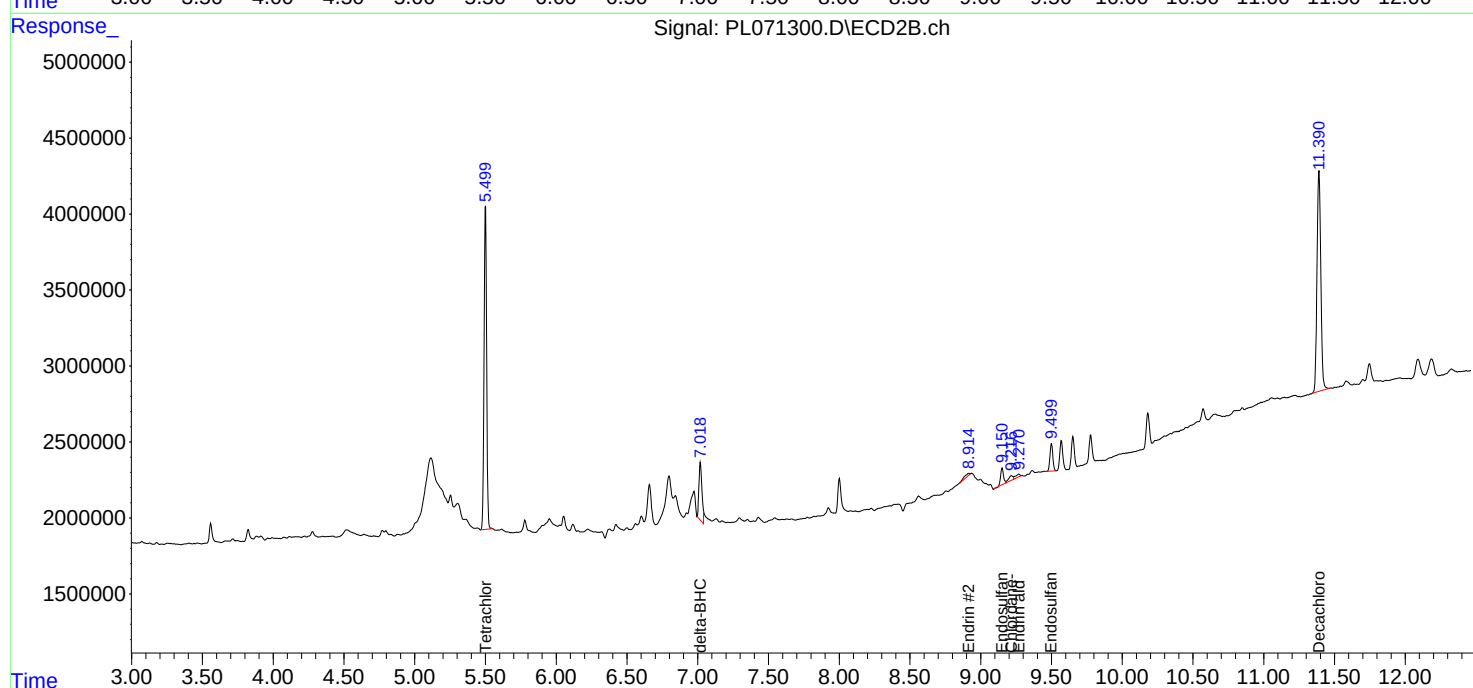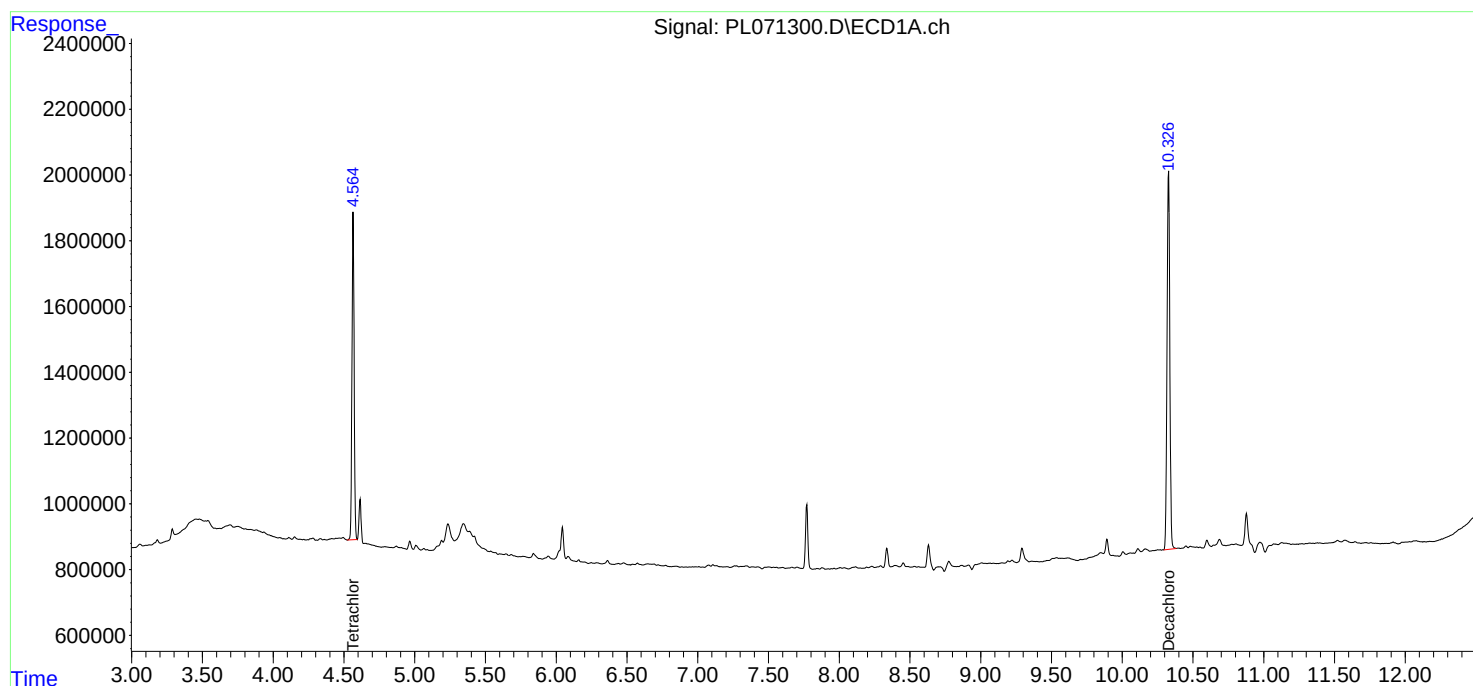


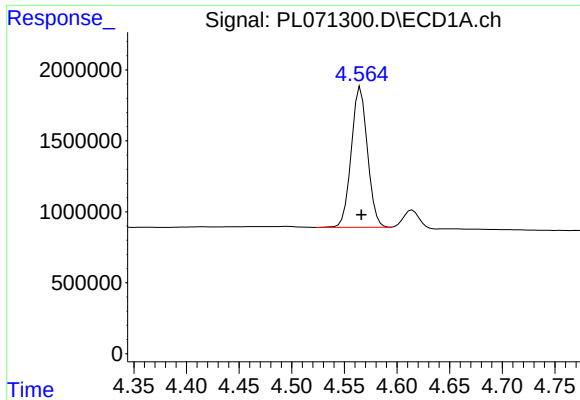

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: 0.000 min
Response: 10593022
Conc: 22.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

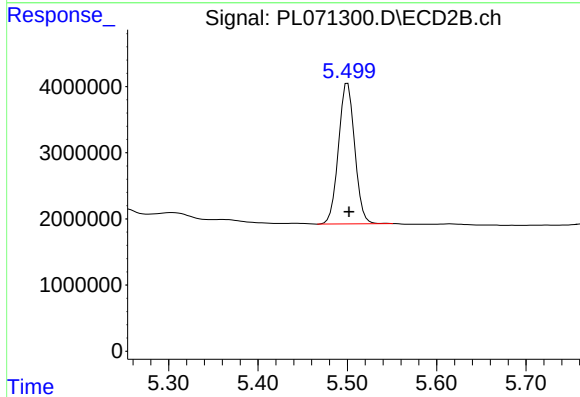


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 26798356
Conc: 21.35 ng/ml

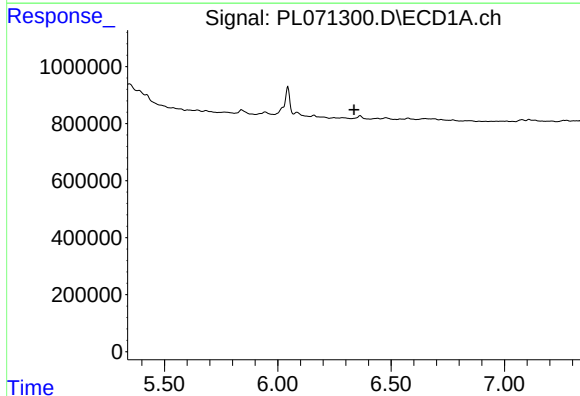


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

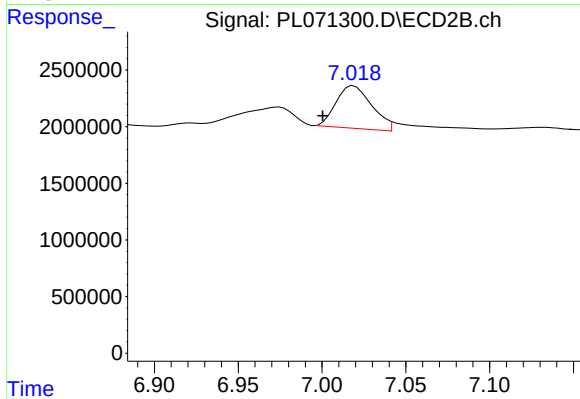

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.019 min
Response: 5477525
Conc: 3.22 ng/ml

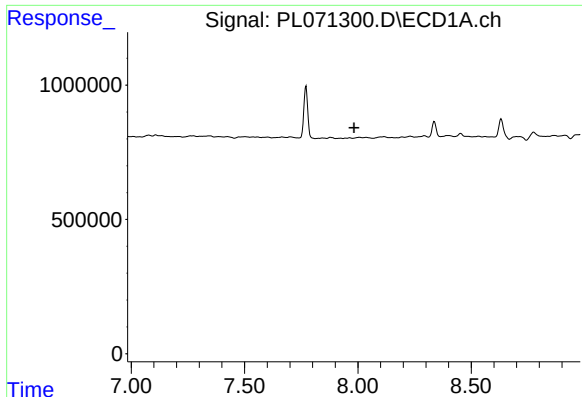

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.983 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

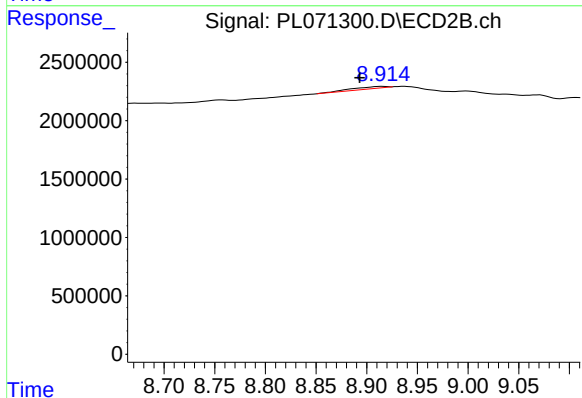


#14 Endrin

R.T.: 8.915 min
Delta R.T.: 0.022 min
Response: 437133
Conc: 0.33 ng/ml

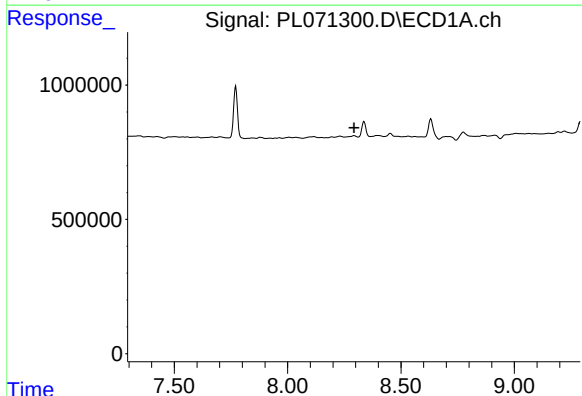


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

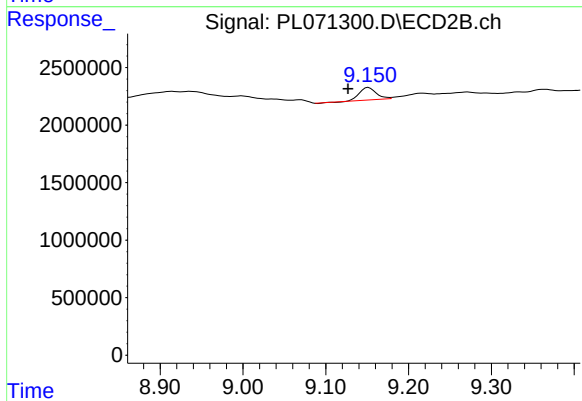

#15 Endosulfan II


R.T.: 9.152 min
Delta R.T.: 0.024 min
Response: 1484220
Conc: 1.10 ng/ml

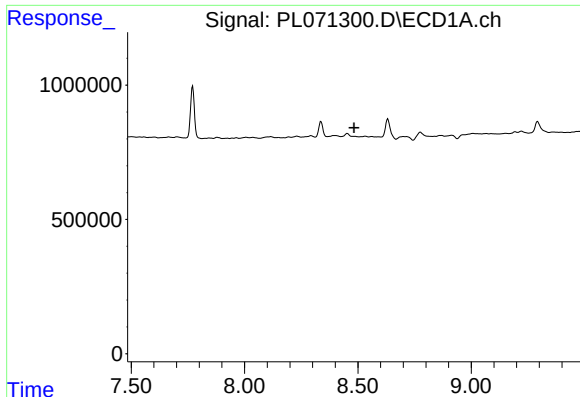

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

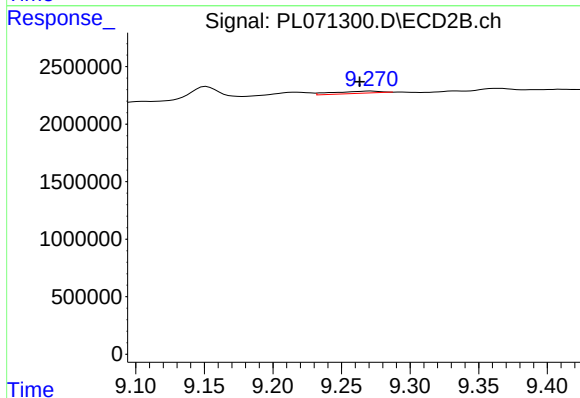


#18 Endrin aldehyde

R.T.: 9.271 min
Delta R.T.: 0.008 min
Response: 445041
Conc: 0.43 ng/ml

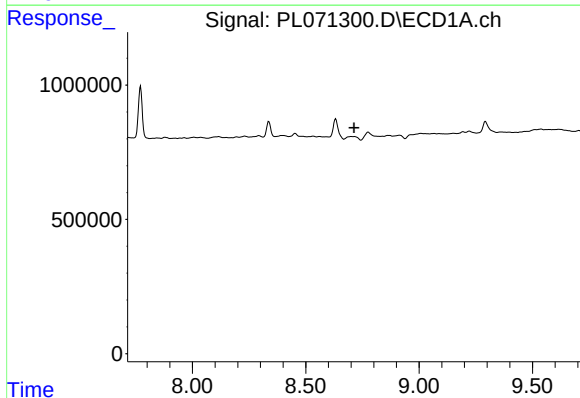


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.714 min
Response: 0
Conc: N.D.

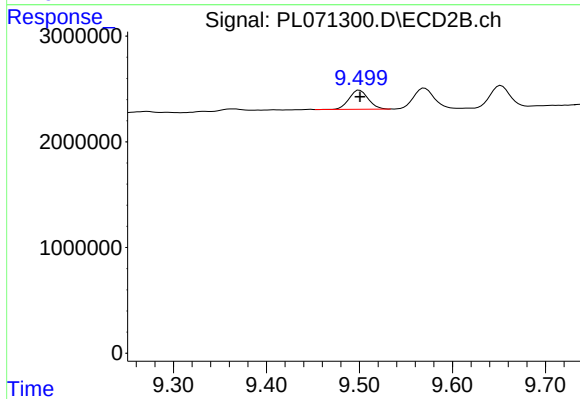

#19 Endosulfan Sulfate


R.T.: 9.500 min
Delta R.T.: 0.000 min
Response: 2570620
Conc: 1.97 ng/ml

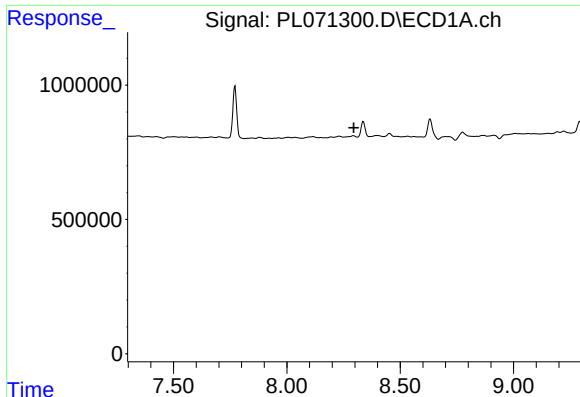

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

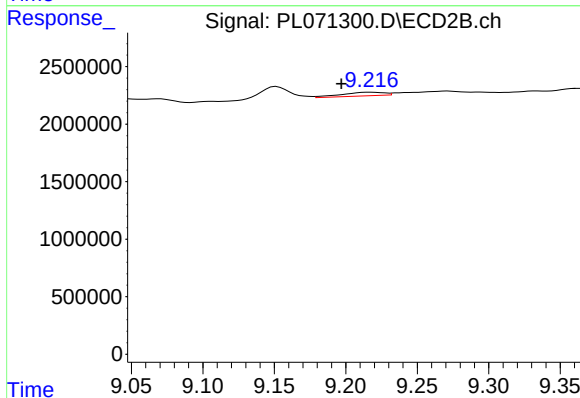


#27 Chlordane-5

R.T.: 9.217 min
Delta R.T.: 0.020 min
Response: 652583
Conc: 13.84 ng/ml

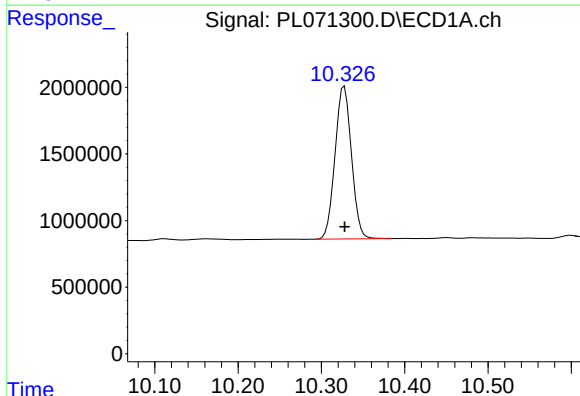

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 15731929
Conc: 21.73 ng/ml

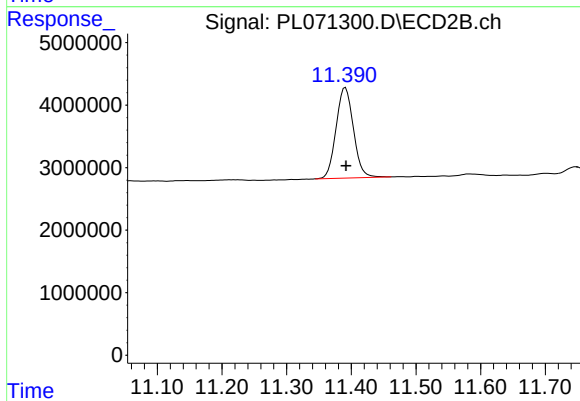

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: -0.001 min
Response: 26907843
Conc: 19.36 ng/ml