

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120721\
 Data File : PL071304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2021 12:36
 Operator : AR\AJ
 Sample : M4936-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 01:54:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	10694013	26423546	22.768	21.056
28)	SA Decachlor...	10.325	11.389	16082916	28481055	22.211	20.490
Target Compounds							
6)	B beta-BHC	0.000	6.742	0	1702702	N.D.	1.935 #
7)	B delta-BHC	0.000	7.020f	0	1553722	N.D.	0.914 #
15)	B Endosulfa...	0.000	9.150f	0	6143043	N.D.	4.559 #
17)	MA 4,4'-DDT	0.000	9.342	0	349335	N.D.	0.251 #
23)	Chlordane-1	0.000	6.872	0	3649417	N.D.	68.776 #
27)	Chlordane-5	0.000	9.215f	0	1204217	N.D.	25.543 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120721\
Data File : PL071304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2021 12:36
Operator : AR\AJ
Sample : M4936-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 01:54:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

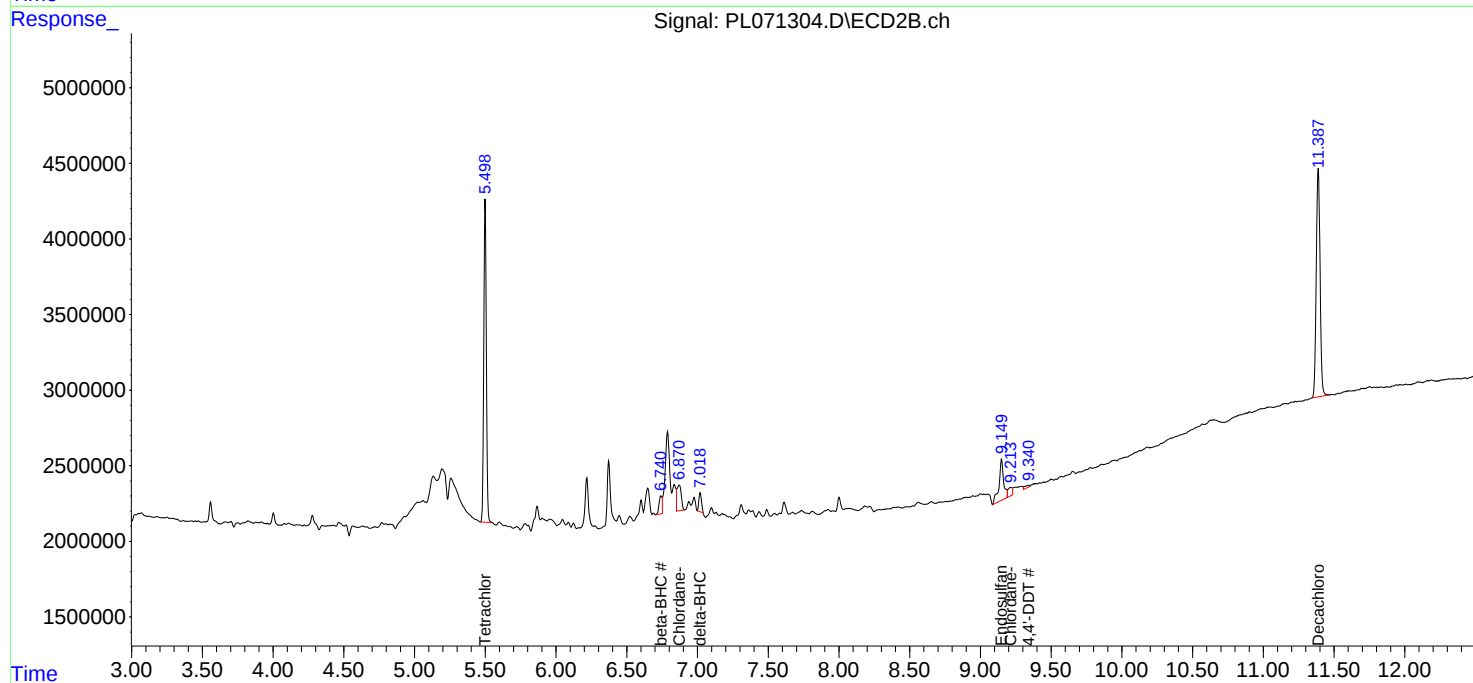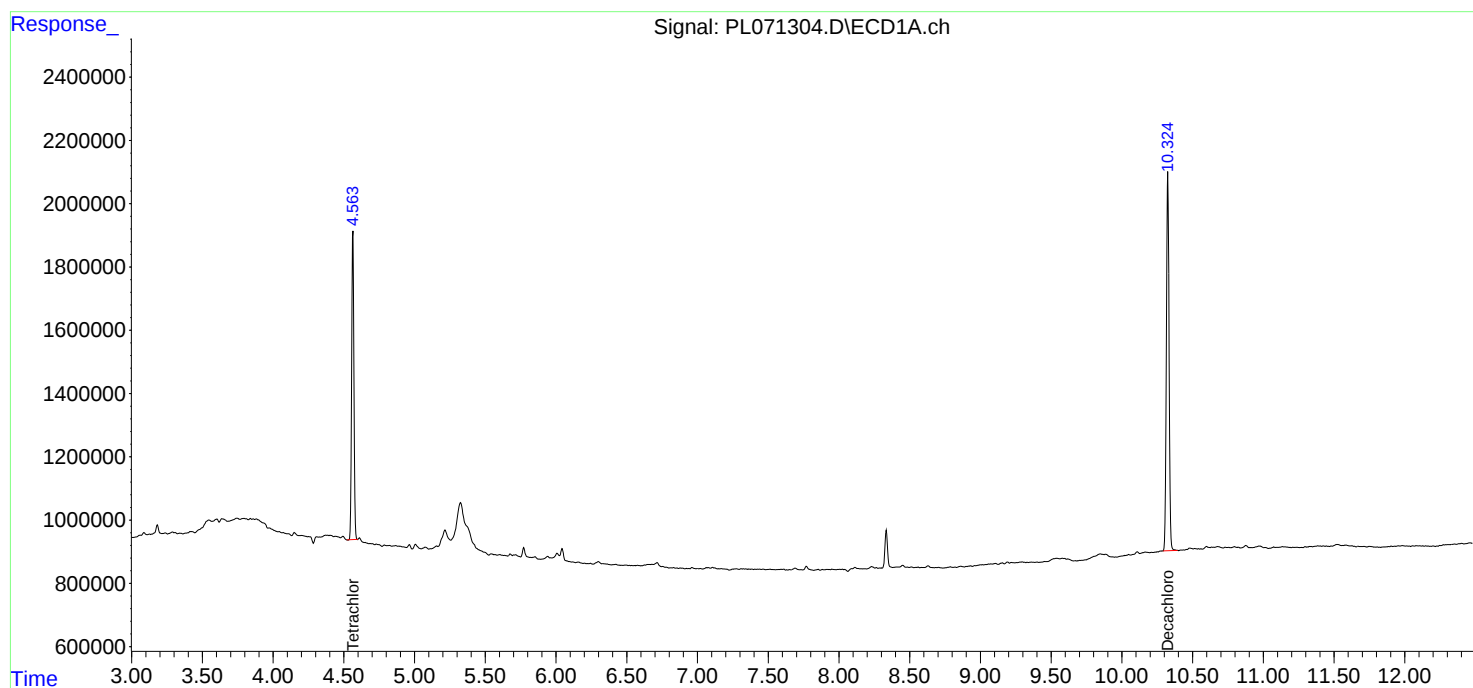


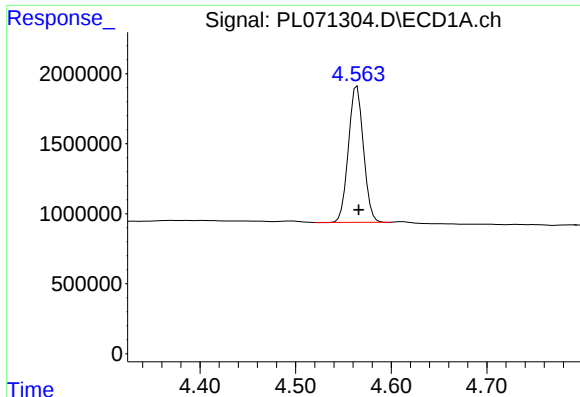

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: -0.002 min
Response: 10694013
Conc: 22.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

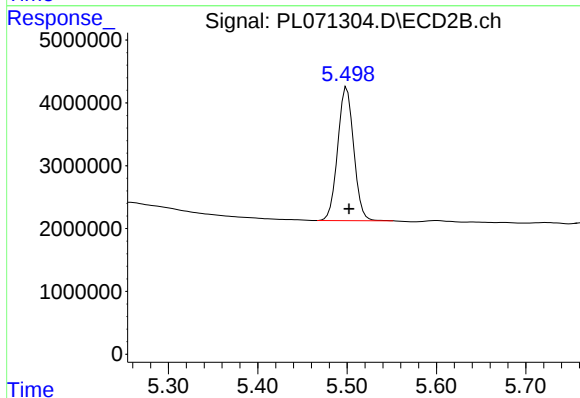


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 26423546
Conc: 21.06 ng/ml

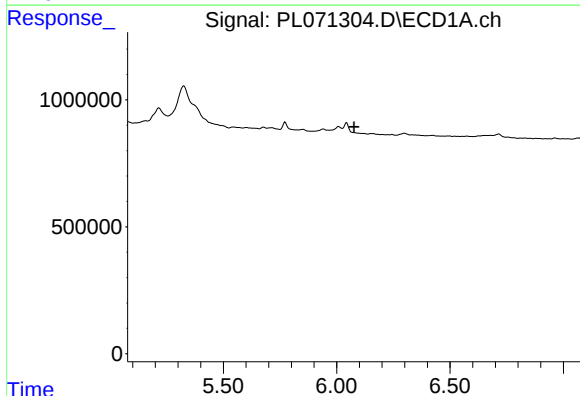


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

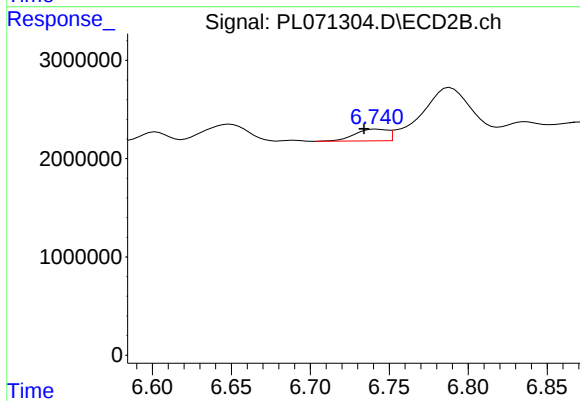

#6 beta-BHC


R.T.: 6.742 min
Delta R.T.: 0.008 min
Response: 1702702
Conc: 1.93 ng/ml

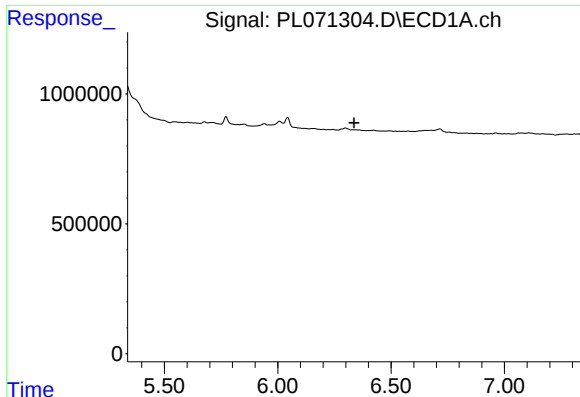

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

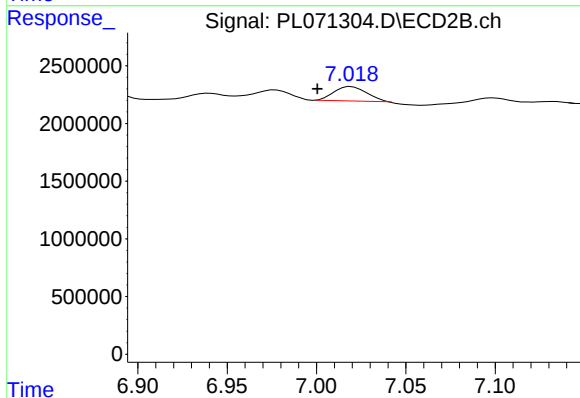


#7 delta-BHC

R.T.: 7.020 min
Delta R.T.: 0.019 min
Response: 1553722
Conc: 0.91 ng/ml

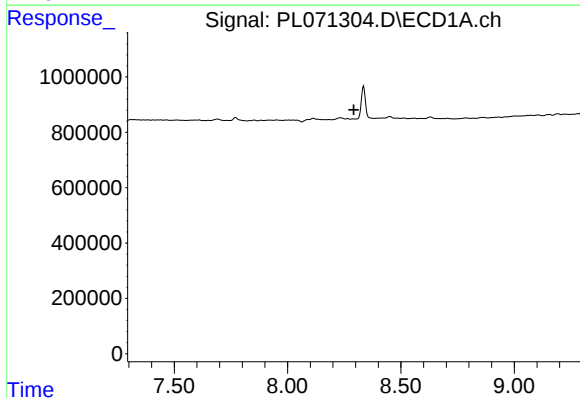


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.293 min
Response: 0
Conc: N.D.

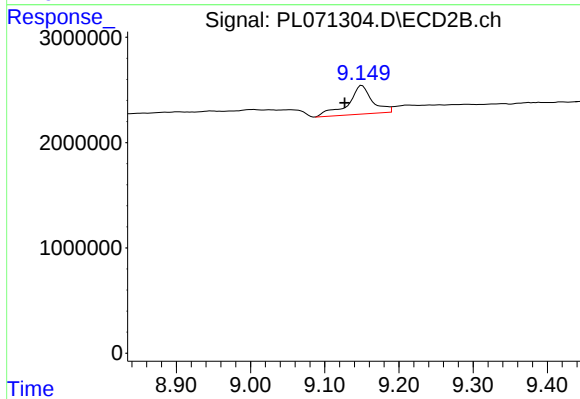

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.023 min
Response: 6143043
Conc: 4.56 ng/ml

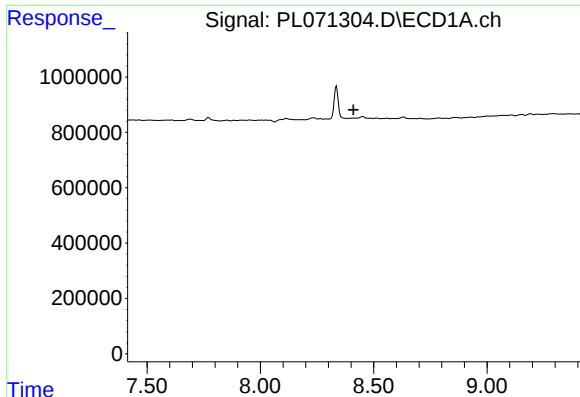

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

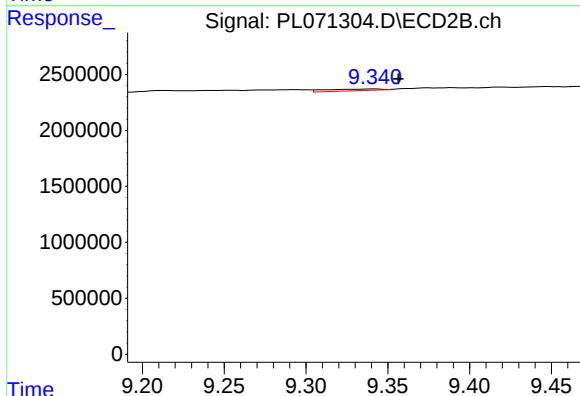


#17 4,4'-DDT

R.T.: 9.342 min
Delta R.T.: -0.015 min
Response: 349335
Conc: 0.25 ng/ml

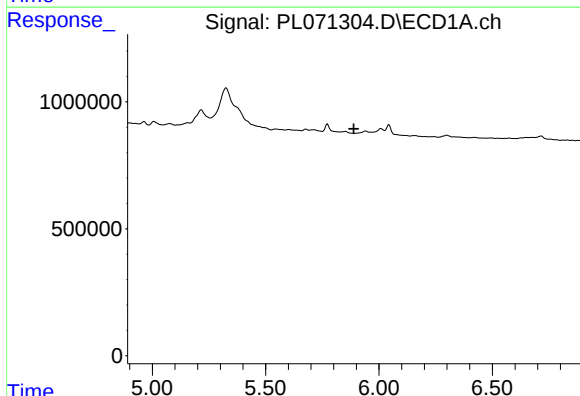


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.889 min
Response: 0
Conc: N.D.

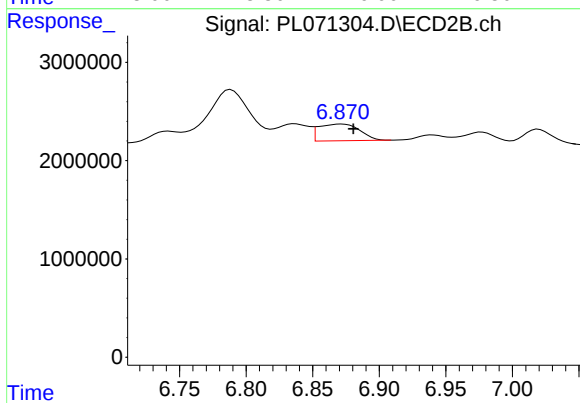

#23 Chlordane-1


R.T.: 6.872 min
Delta R.T.: -0.008 min
Response: 3649417
Conc: 68.78 ng/ml

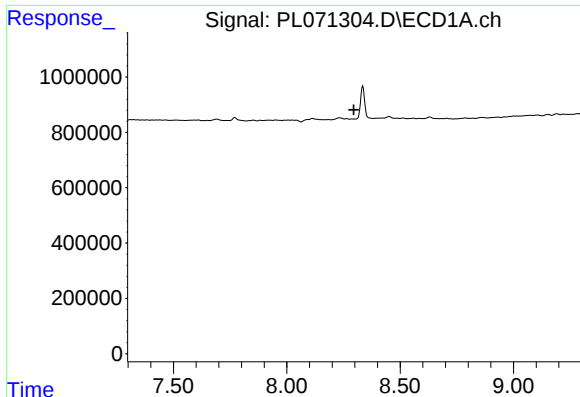

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

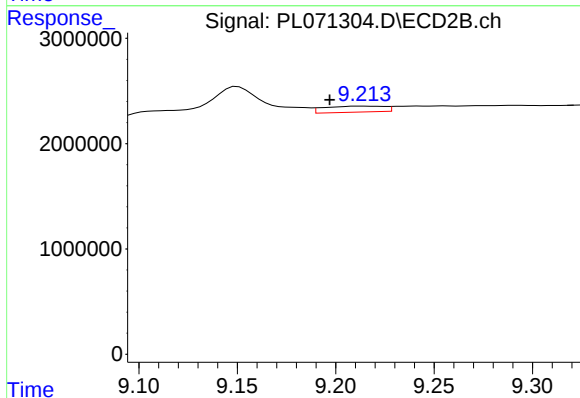


#27 Chlordane-5

R.T.: 9.215 min
Delta R.T.: 0.018 min
Response: 1204217
Conc: 25.54 ng/ml

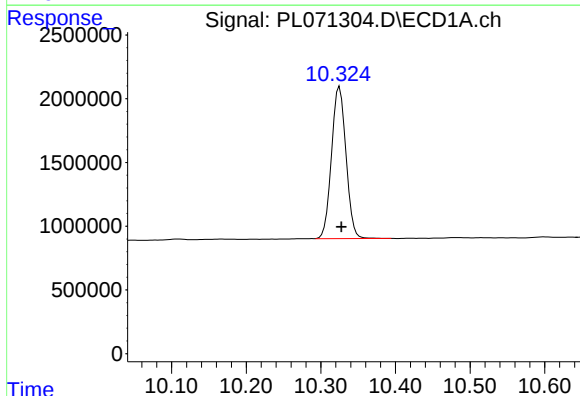

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: -0.003 min
Response: 16082916
Conc: 22.21 ng/ml

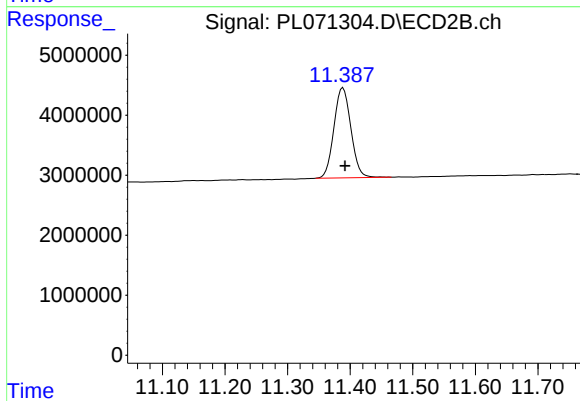

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.004 min
Response: 28481055
Conc: 20.49 ng/ml