

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
 Data File : PL063372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2020 12:50
 Operator : DD\AJ
 Sample : L4969-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NORTH-BRANFORD-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:12:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.951	35060278	66393550	20.586	20.343
28)	SA Decachlor...	8.129	8.993	38892720	51059215	20.827	21.460
Target Compounds							
9)	A Endosulfan I	5.459f	0.000	2985636	0	1.764	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
Data File : PL063372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2020 12:50
Operator : DD\AJ
Sample : L4969-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NORTH-BRANFORD-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:12:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

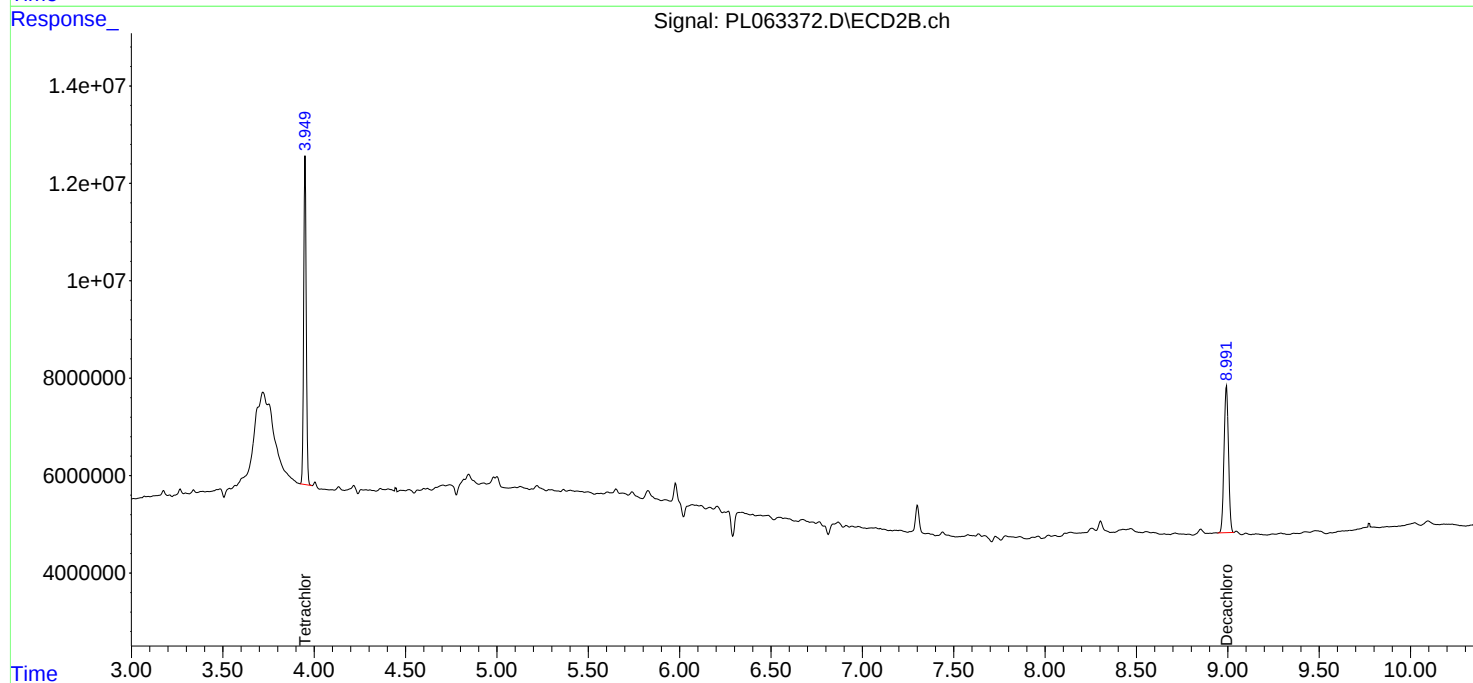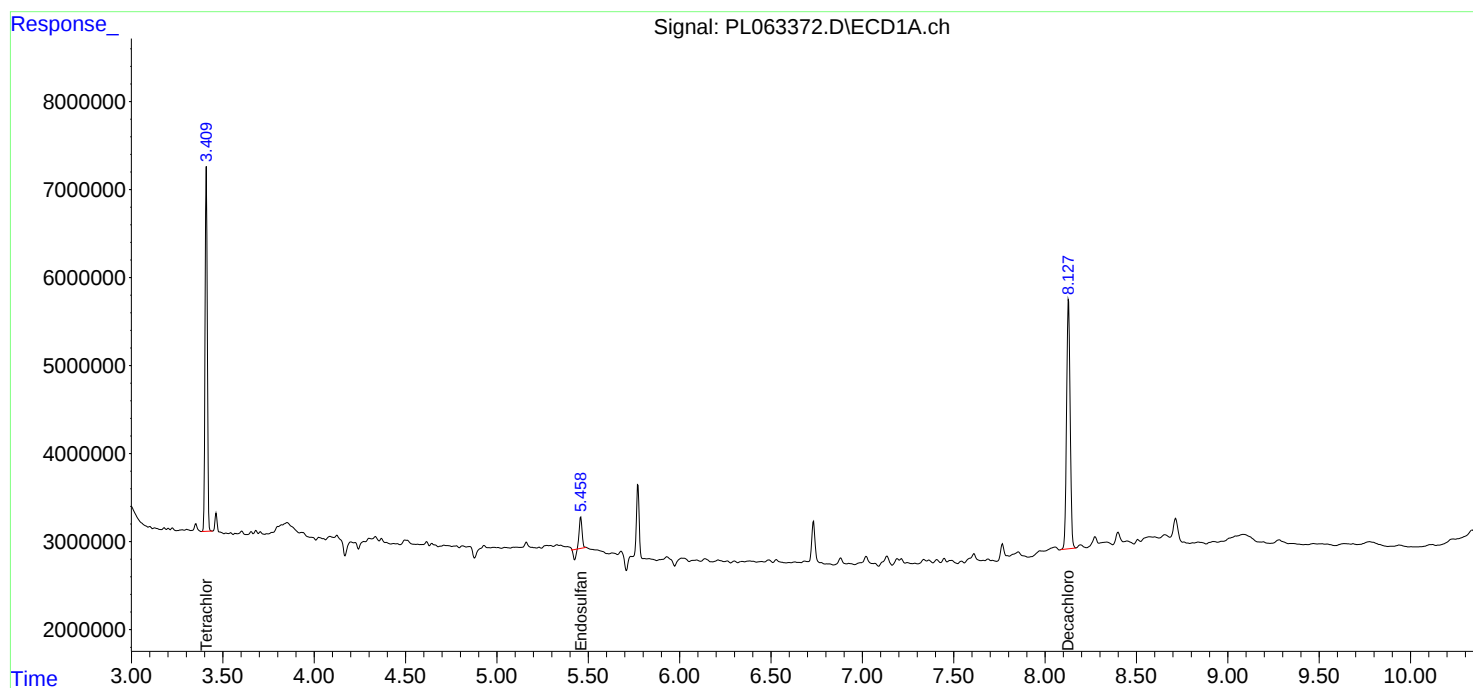


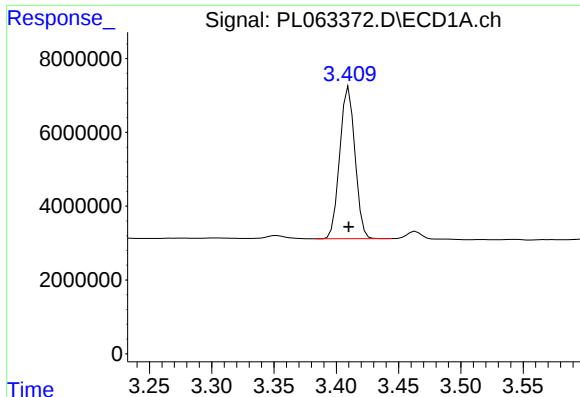

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 35060278
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
NORTH-BRANFORD-03

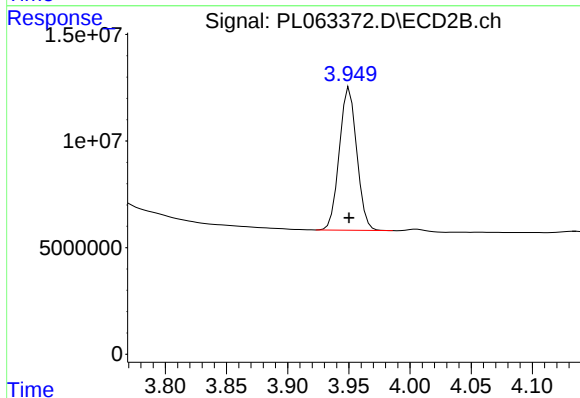


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 66393550
Conc: 20.34 ng/ml

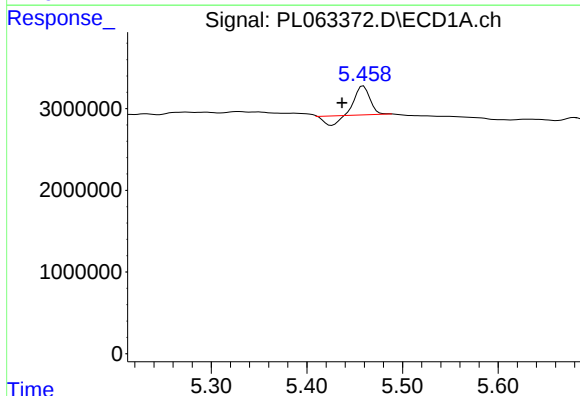


#9 Endosulfan I

R.T.: 5.459 min
Delta R.T.: 0.022 min
Response: 2985636
Conc: 1.76 ng/ml

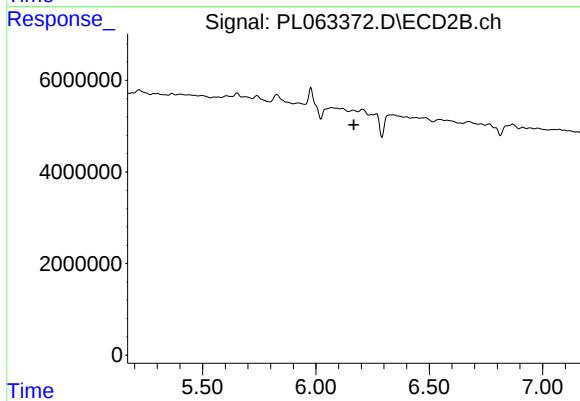

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.167 min
Response: 0
Conc: N.D.

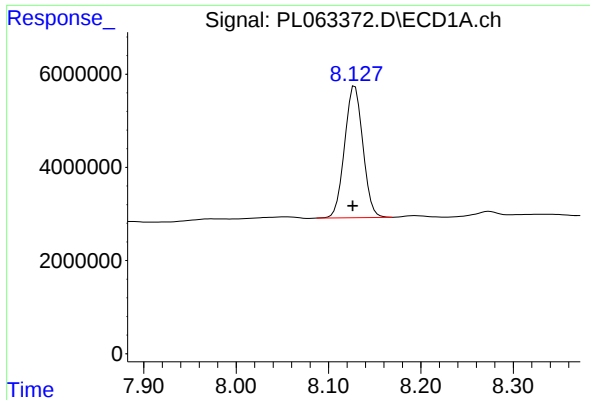

#28 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.003 min
Response: 38892720
Conc: 20.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
NORTH-BRANFORD-03

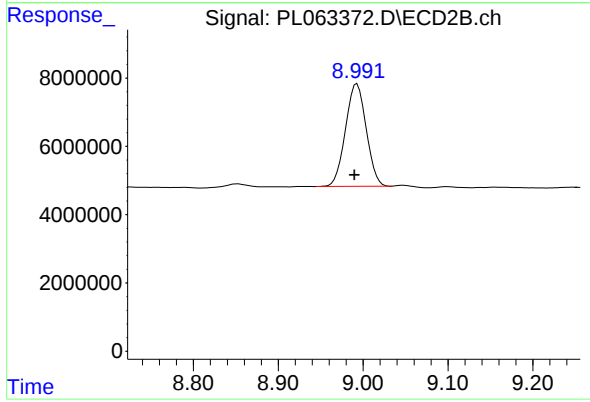

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.003 min
Response: 51059215
Conc: 21.46 ng/ml