

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
 Data File : PL063380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2020 14:52
 Operator : DD\AJ
 Sample : L4965-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:14:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	3.951	35586524	59408486	20.895	18.202
28)	SA Decachlor...	8.135	8.998	35334197	43839424	18.921	18.426
Target Compounds							
6)	B beta-BHC	0.000	4.816f	0	6849724	N.D.	3.359 #
8)	B Heptachlo...	0.000	5.827f	0	9313079	N.D.	2.673 #
9)	A Endosulfan I	5.466f	0.000	10760360	0	6.357	N.D. #
10)	B gamma-Chl...	0.000	6.040	0	13176282	N.D.	3.724 #
11)	B alpha-Chl...	0.000	6.126	0	14854232	N.D.	4.117 #
12)	B 4,4'-DDE	5.557	6.280	6160467	15254455	3.717	4.348
14)	MA Endrin	0.000	6.636	0	10183534	N.D.	3.449 #
17)	MA 4,4'-DDT	6.308	7.071	6525569	14524276	4.852	5.687
25)	Chlordane-3	0.000	6.040	0	13176282	N.D.	29.711 #
26)	Chlordane-4	0.000	6.126	0	14854232	N.D.	27.695 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
Data File : PL063380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2020 14:52
Operator : DD\AJ
Sample : L4965-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CRT002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:14:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

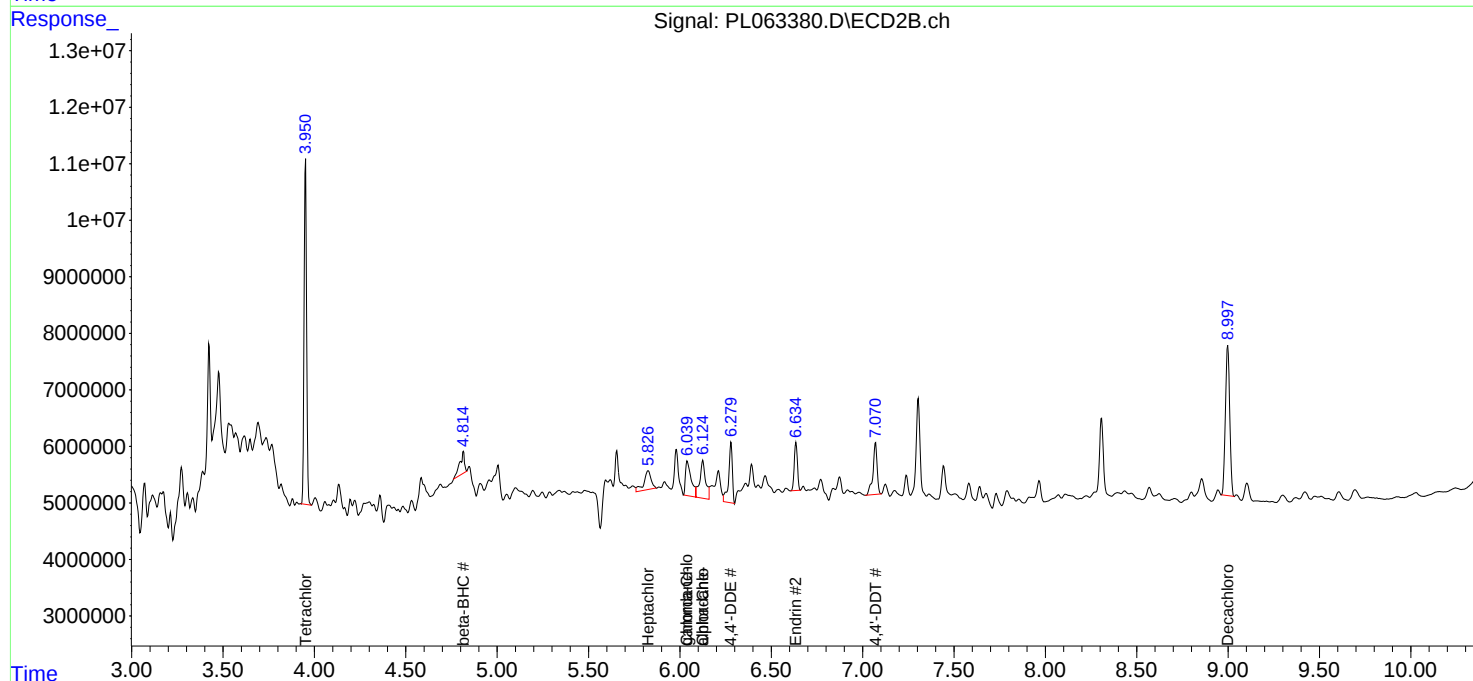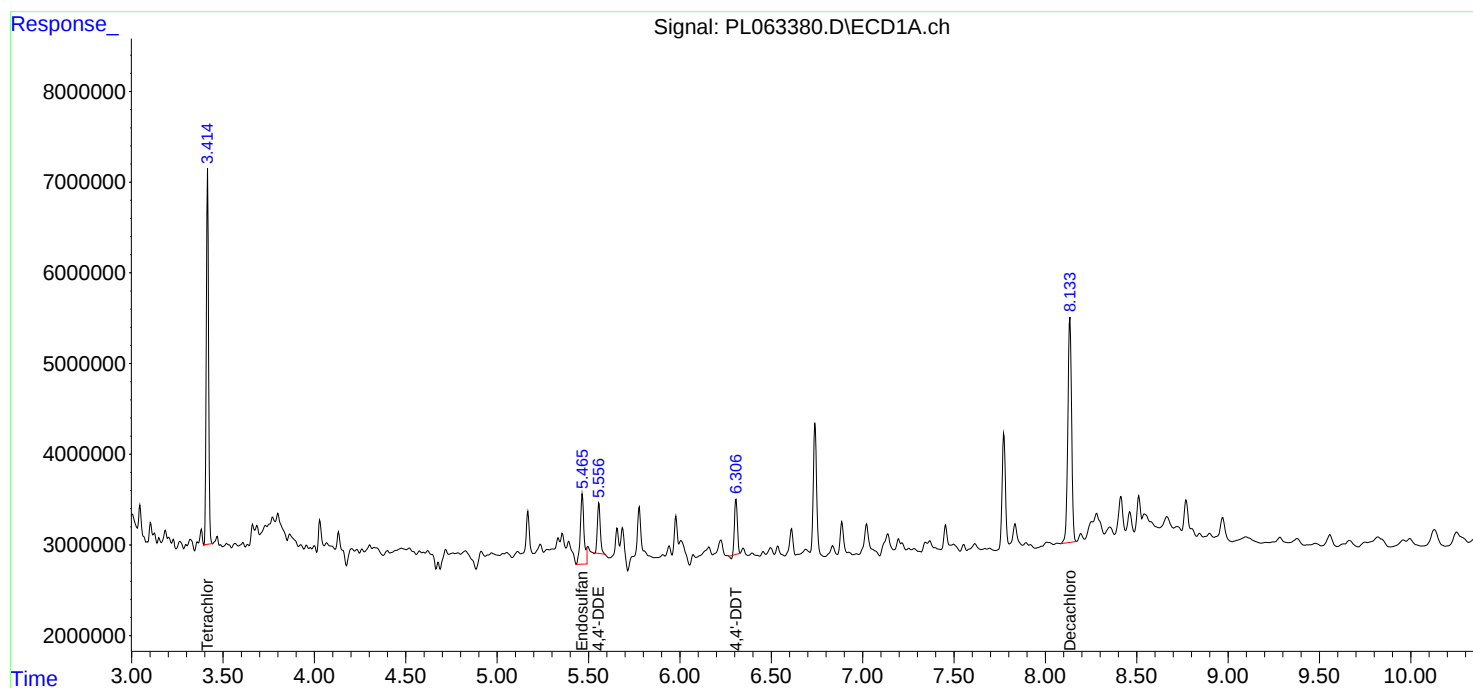


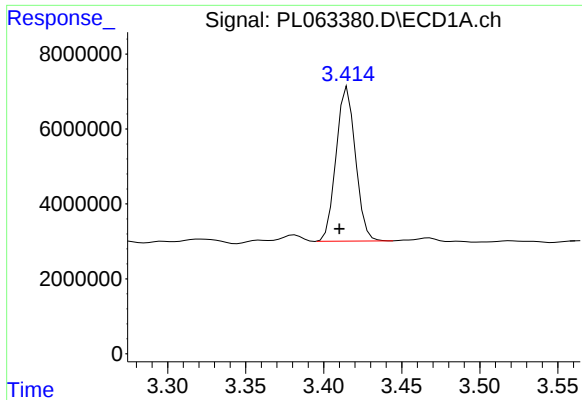

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.005 min
Response: 35586524
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT002

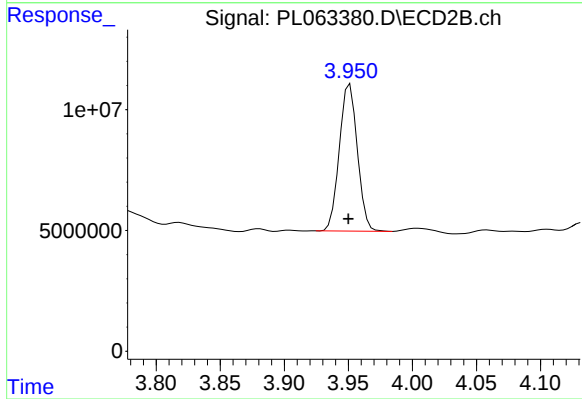


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.001 min
Response: 59408486
Conc: 18.20 ng/ml

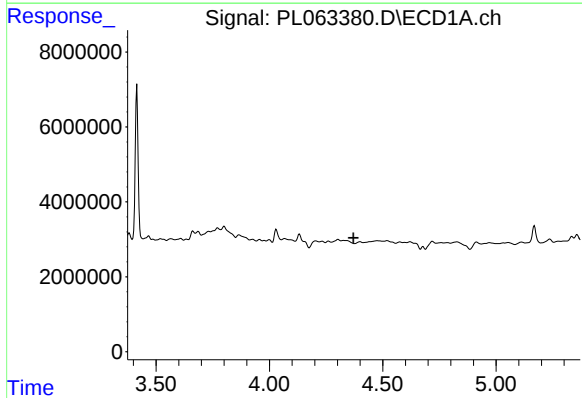


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

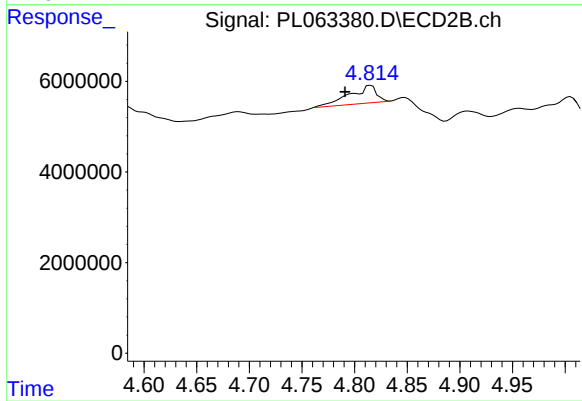

#6 beta-BHC


R.T.: 4.816 min
Delta R.T.: 0.025 min
Response: 6849724
Conc: 3.36 ng/ml

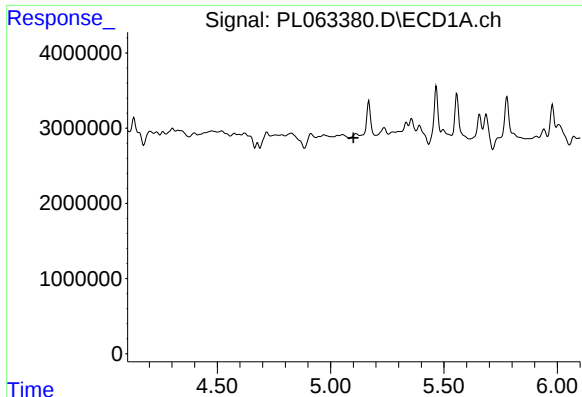

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT002

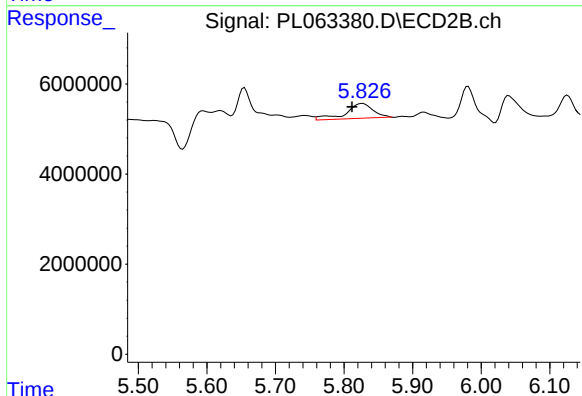


#8 Heptachlor epoxide

R.T.: 5.827 min
Delta R.T.: 0.016 min
Response: 9313079
Conc: 2.67 ng/ml

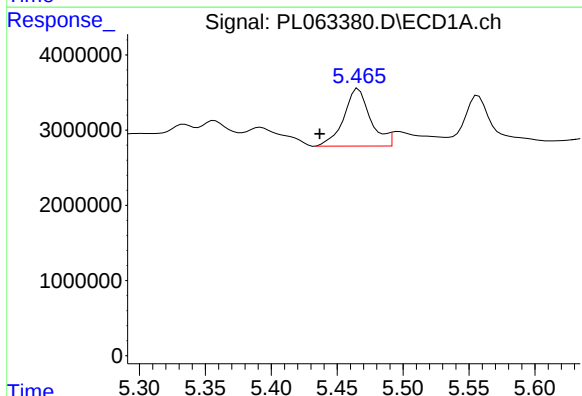


#9 Endosulfan I

R.T.: 5.466 min
Delta R.T.: 0.029 min
Response: 10760360
Conc: 6.36 ng/ml

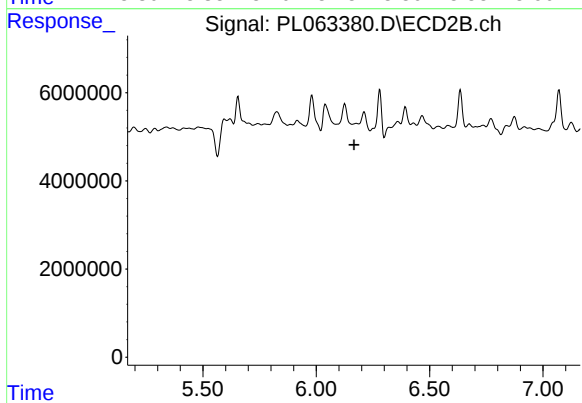

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.167 min
Response: 0
Conc: N.D.

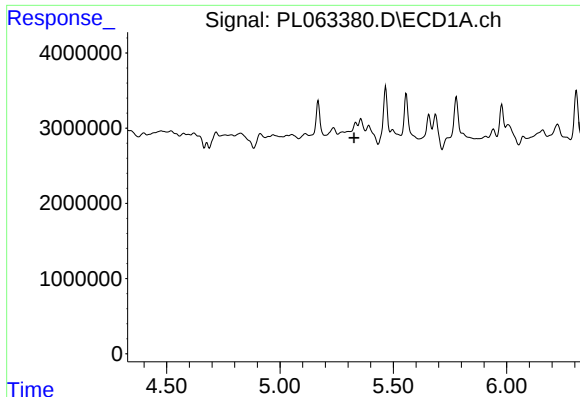

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT002

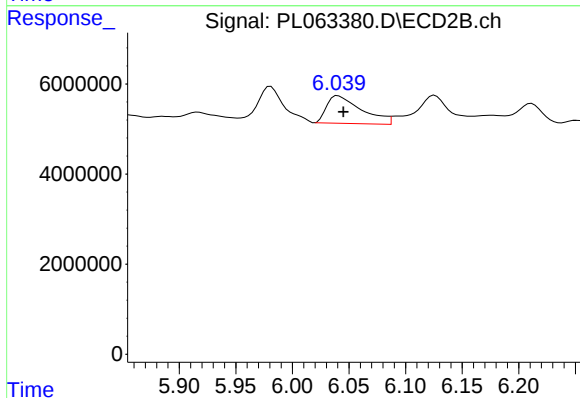


#10 gamma-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.005 min
Response: 13176282
Conc: 3.72 ng/ml

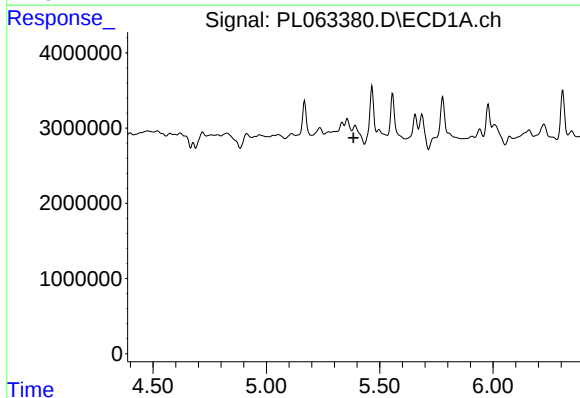


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.384 min
Response: 0
Conc: N.D.

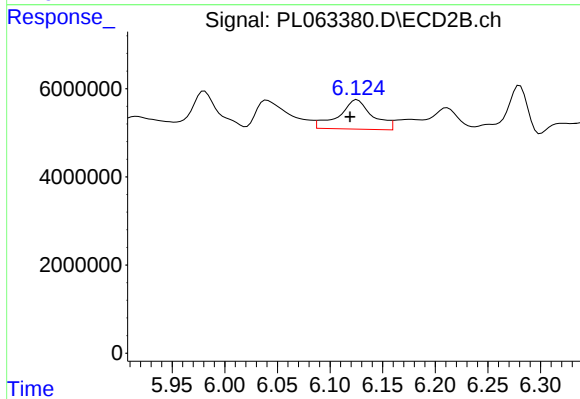

#11 alpha-Chlordane


R.T.: 6.126 min
Delta R.T.: 0.007 min
Response: 14854232
Conc: 4.12 ng/ml

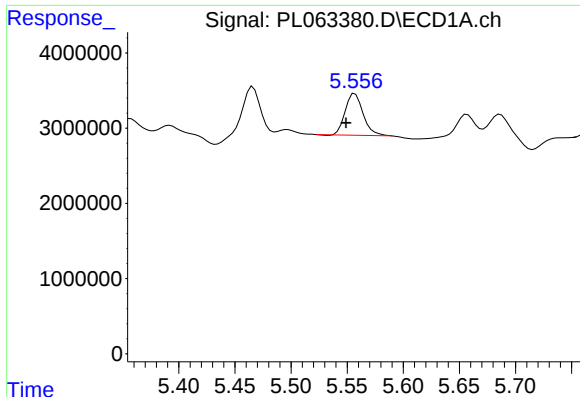

#12 4,4'-DDE


R.T.: 5.557 min
Delta R.T.: 0.008 min
Response: 6160467
Conc: 3.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT002

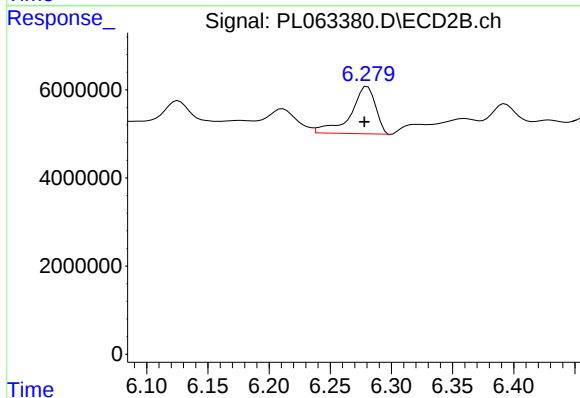


#12 4,4'-DDE

R.T.: 6.280 min
Delta R.T.: 0.002 min
Response: 15254455
Conc: 4.35 ng/ml

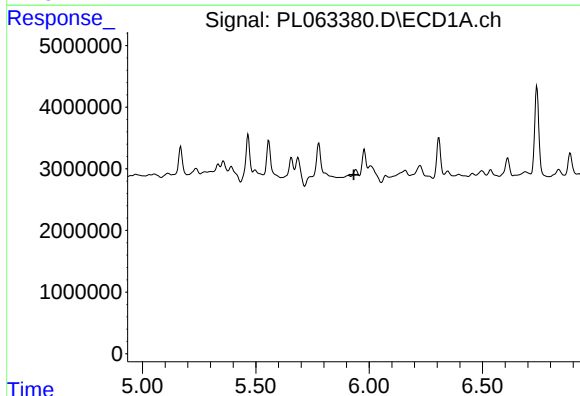


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.932 min
Response: 0
Conc: N.D.

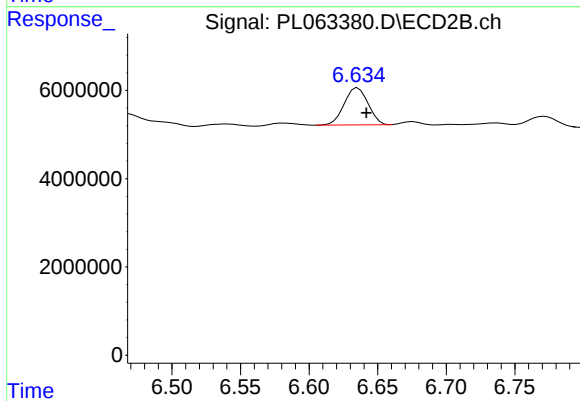

#14 Endrin


R.T.: 6.636 min
Delta R.T.: -0.006 min
Response: 10183534
Conc: 3.45 ng/ml

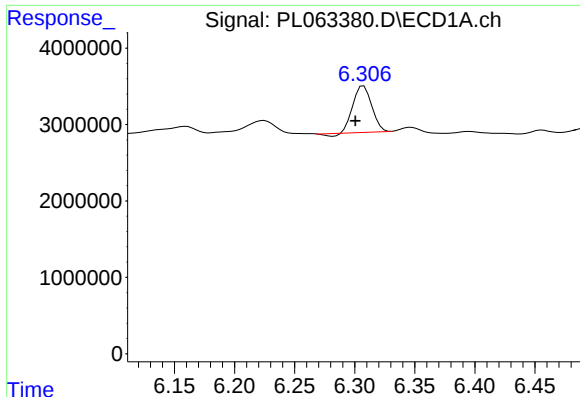

#17 4,4'-DDT


R.T.: 6.308 min
Delta R.T.: 0.007 min
Response: 6525569
Conc: 4.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT002

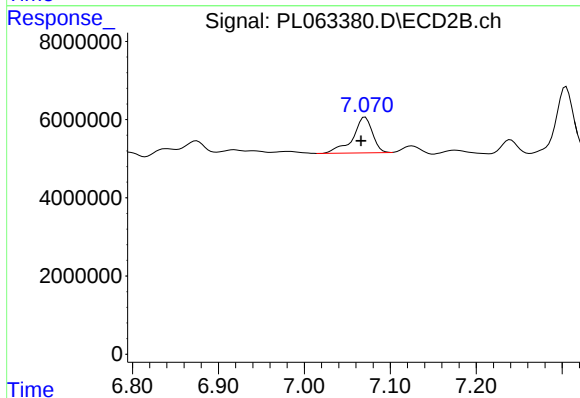


#17 4,4'-DDT

R.T.: 7.071 min
Delta R.T.: 0.005 min
Response: 14524276
Conc: 5.69 ng/ml

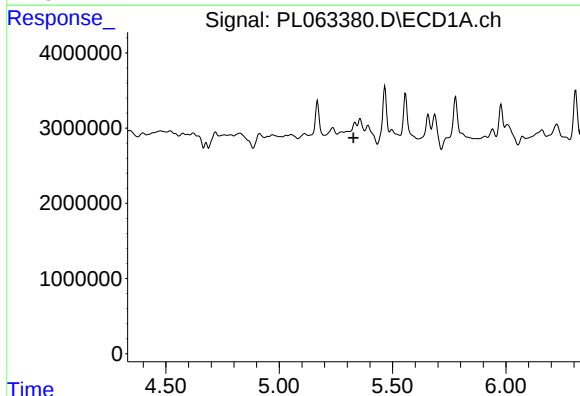


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

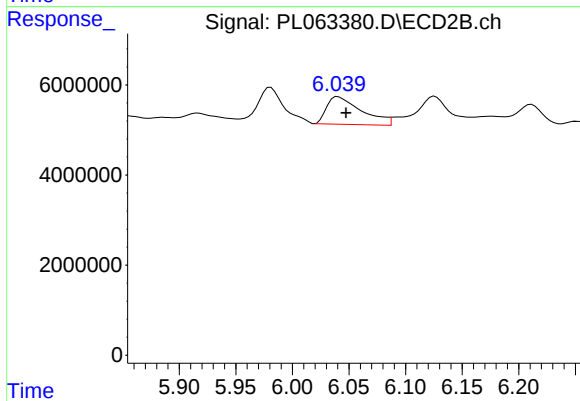

#25 Chlordane-3


R.T.: 6.040 min
Delta R.T.: -0.007 min
Response: 13176282
Conc: 29.71 ng/ml

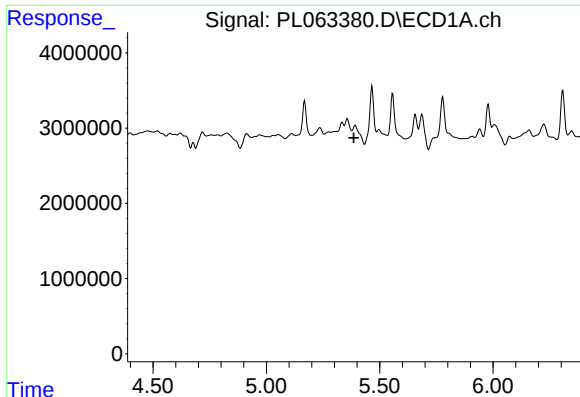

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT002

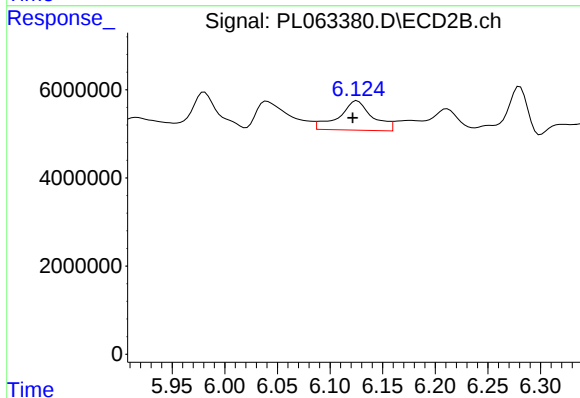


#26 Chlordane-4

R.T.: 6.126 min
Delta R.T.: 0.004 min
Response: 14854232
Conc: 27.70 ng/ml

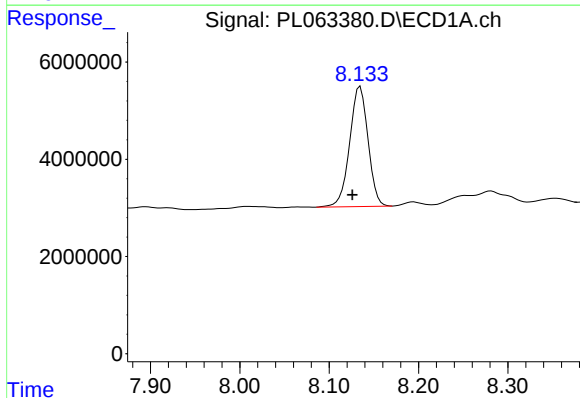

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.009 min
Response: 35334197
Conc: 18.92 ng/ml

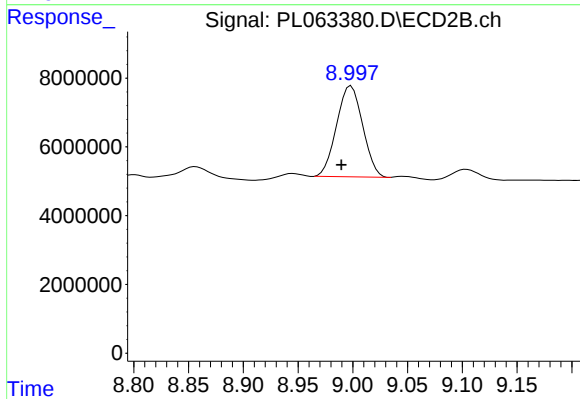

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.009 min
Response: 43839424
Conc: 18.43 ng/ml