

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
 Data File : PL063387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2020 16:32
 Operator : DD\AJ
 Sample : L4971-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 5S2-A-D-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:16:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.951	20565141	38341655	12.075	11.748
28)	SA Decachlor...	8.129	8.993	30722174	37813425	16.451	15.893
Target Compounds							
20)	A Methoxychlor	6.830	0.000	8648183	0	10.094	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
Data File : PL063387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2020 16:32
Operator : DD\AJ
Sample : L4971-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
5S2-A-D-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:16:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

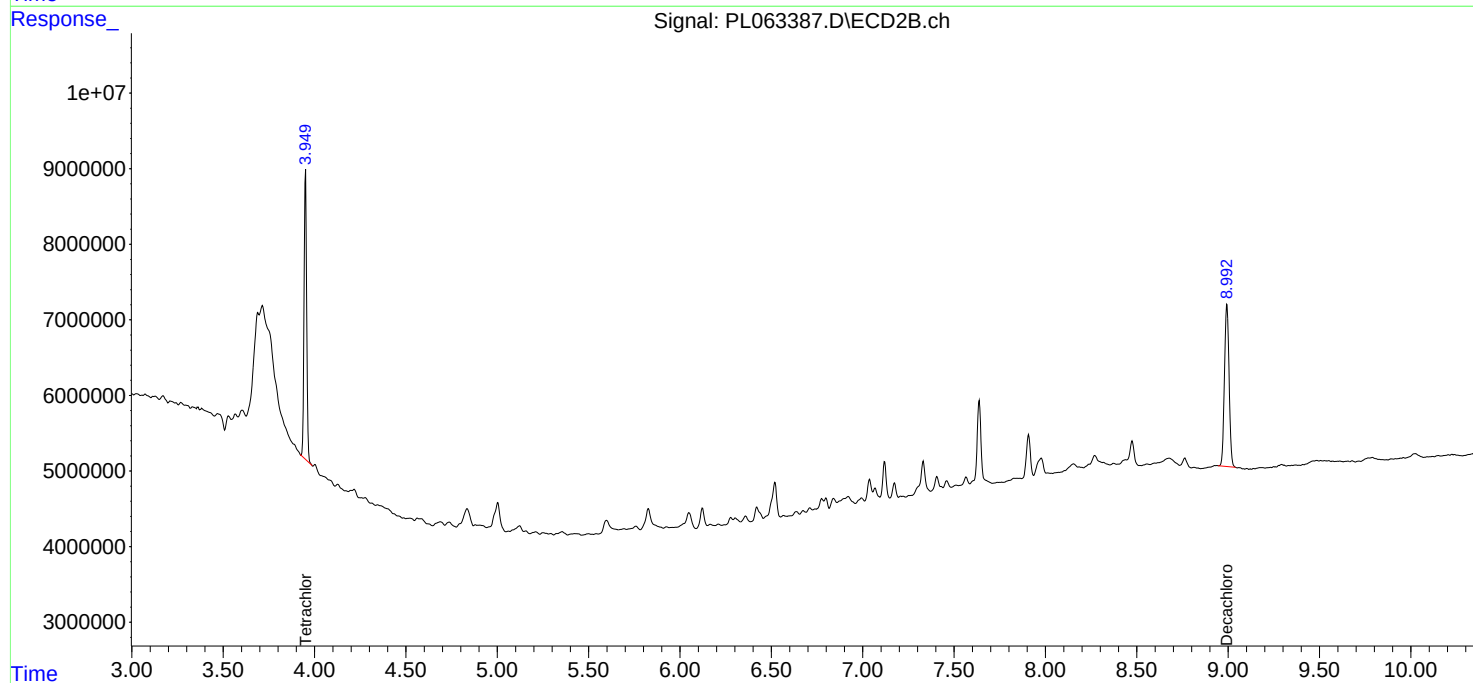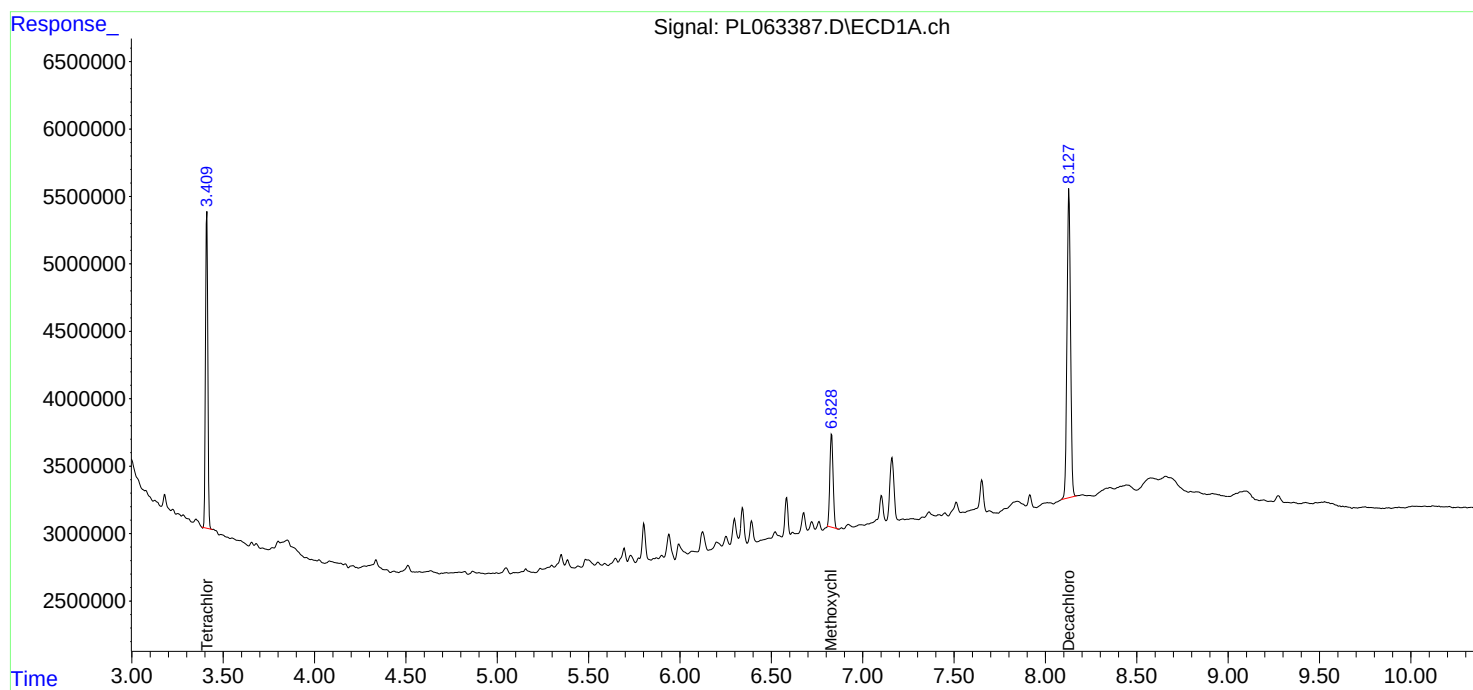


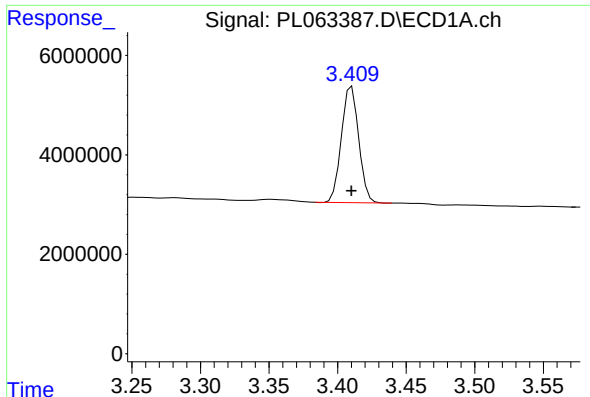

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 20565141
Conc: 12.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
5S2-A-D-COMP

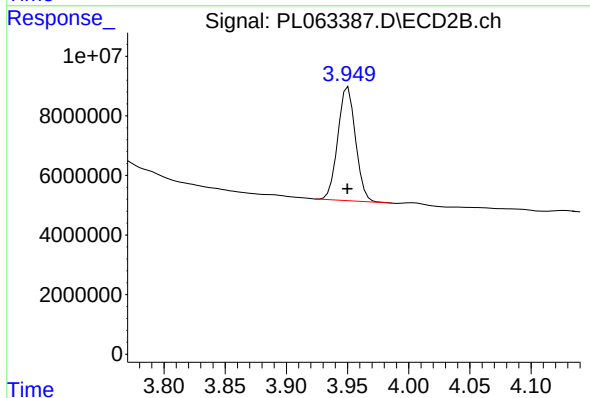


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 38341655
Conc: 11.75 ng/ml

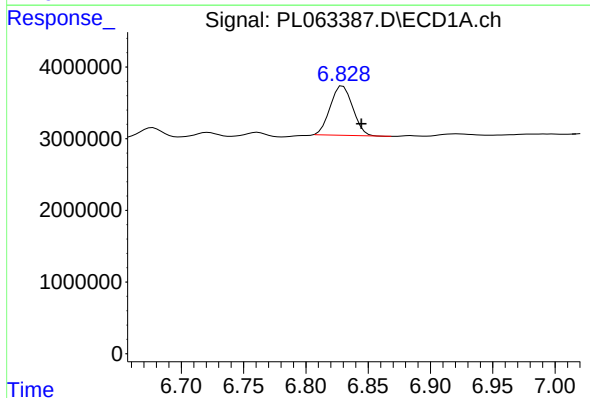


#20 Methoxychlor

R.T.: 6.830 min
Delta R.T.: -0.015 min
Response: 8648183
Conc: 10.09 ng/ml

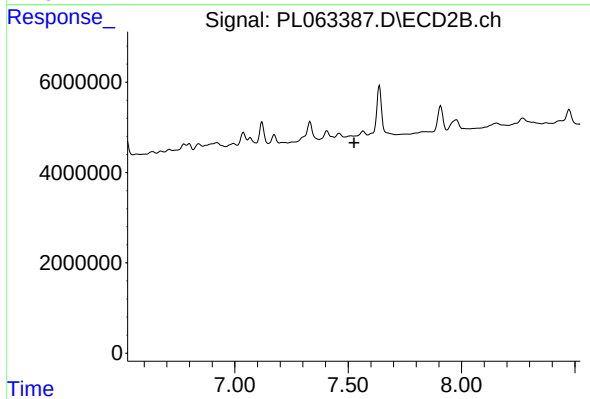

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.526 min
Response: 0
Conc: N.D.

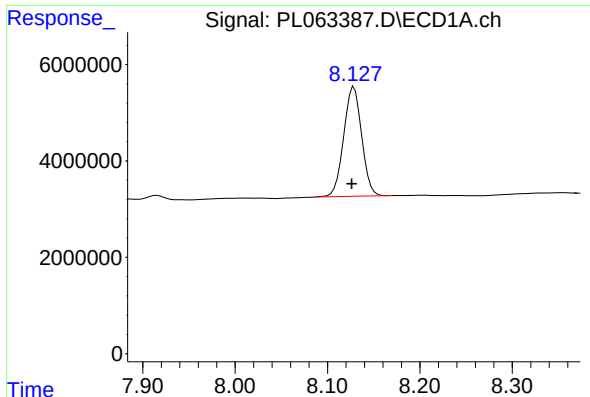

#28 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.003 min
Response: 30722174
Conc: 16.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
5S2-A-D-COMP

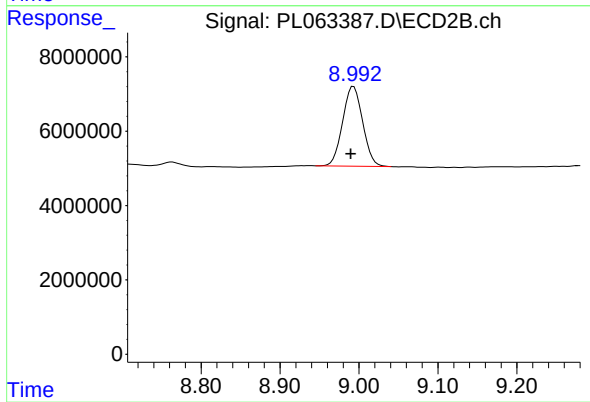

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.004 min
Response: 37813425
Conc: 15.89 ng/ml