

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
 Data File : PL063394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2020 18:11
 Operator : DD\AJ
 Sample : L4965-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT012

Manual Integrations
 APPROVED

Ankita
 12/9/2020 3:09:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:18:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.970f	35359334	69289964	20.762	21.230m
28)	SA Decachlor...	8.127	9.012f	36244790	47594041	19.409	20.004m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120820\
Data File : PL063394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2020 18:11
Operator : DD\AJ
Sample : L4965-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT012


Manual Integrations
APPROVED

Ankita
12/9/2020 3:09:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:18:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

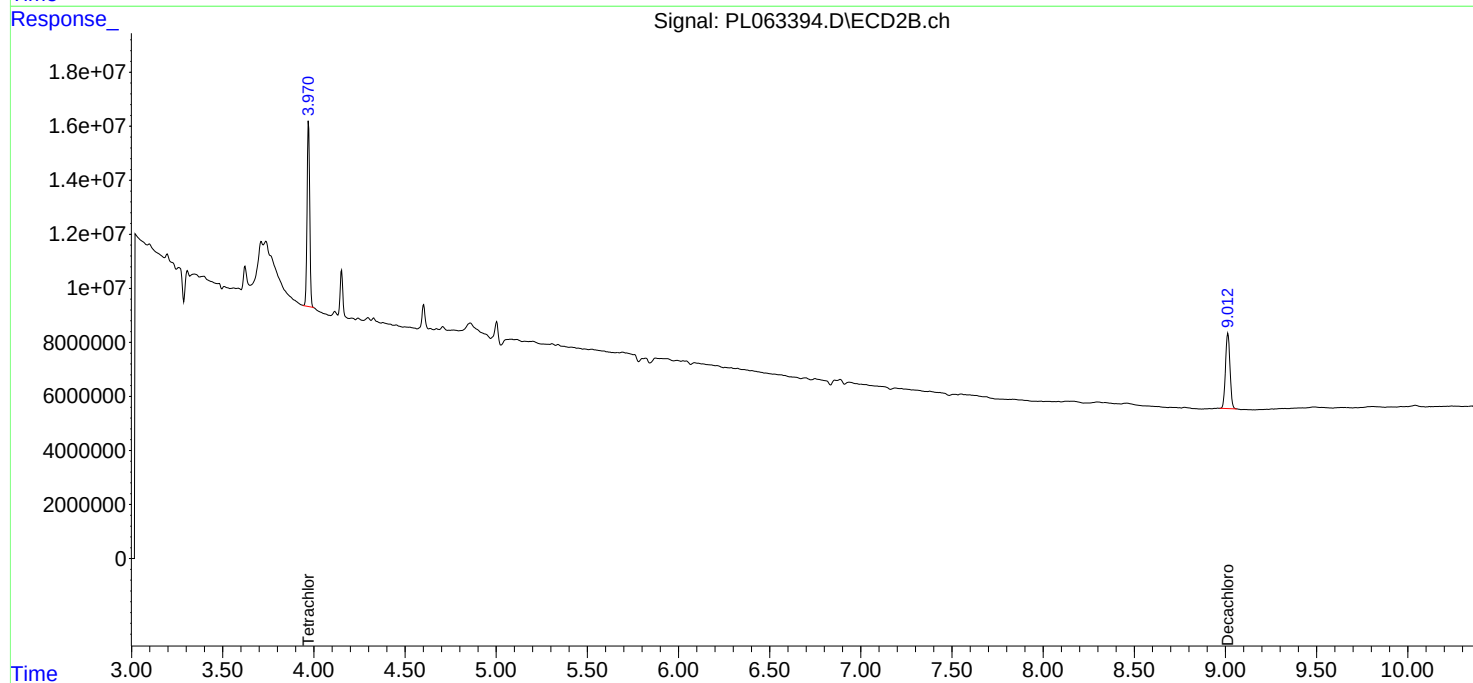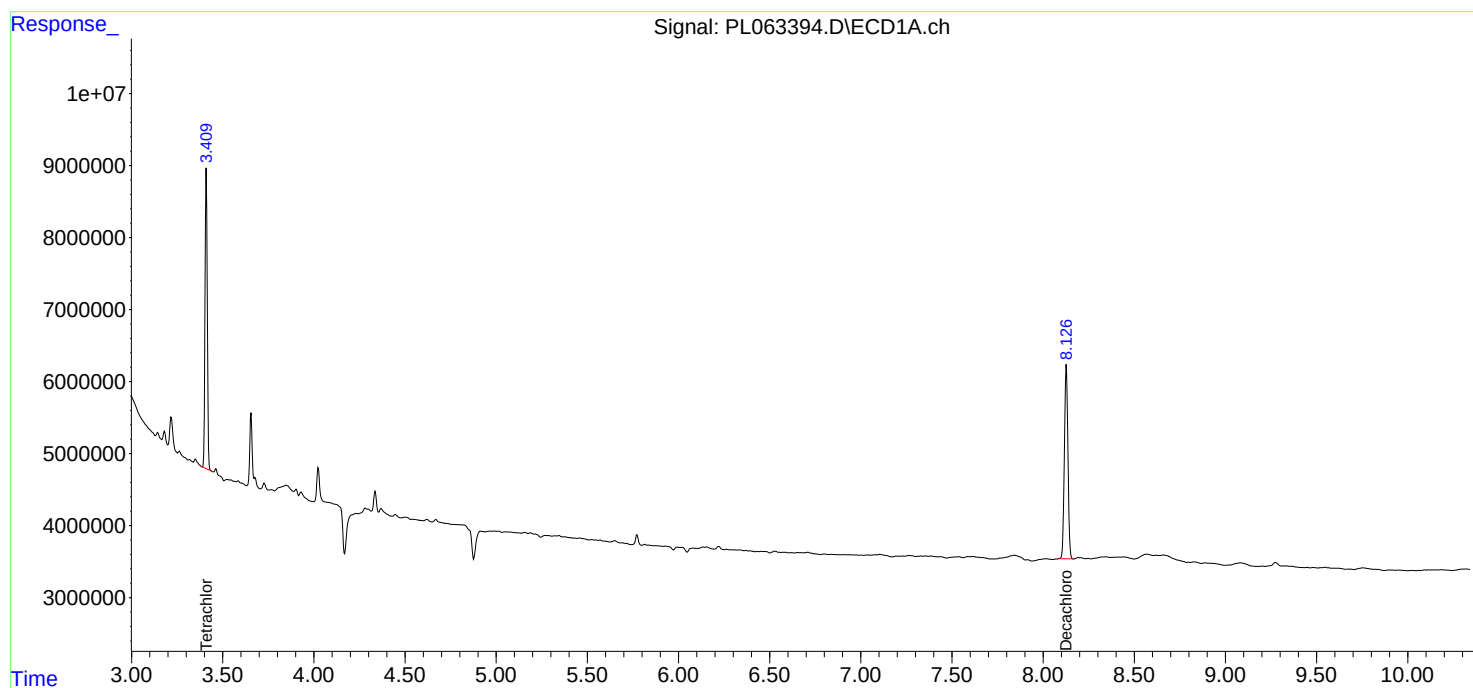

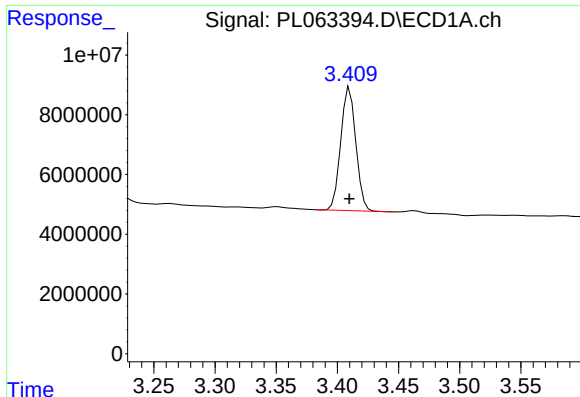


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 35359334
Conc: 20.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT012


Manual Integrations
APPROVED

Ankita
12/9/2020 3:09:22 PM

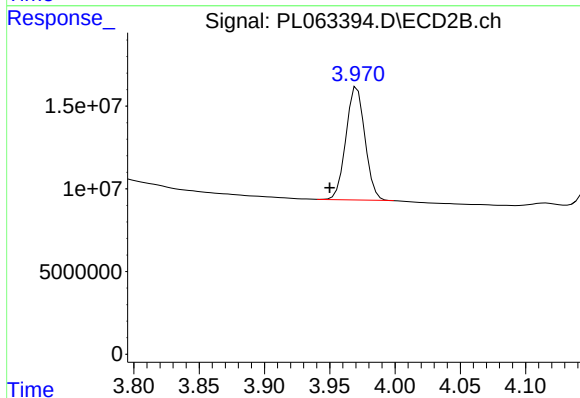


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.020 min
Response: 69289964
Conc: 21.23 ng/ml m

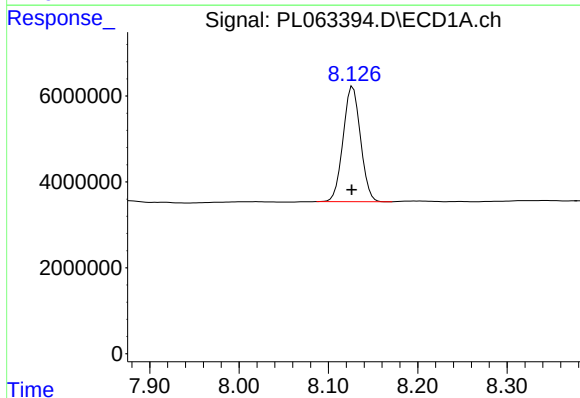

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 36244790
Conc: 19.41 ng/ml

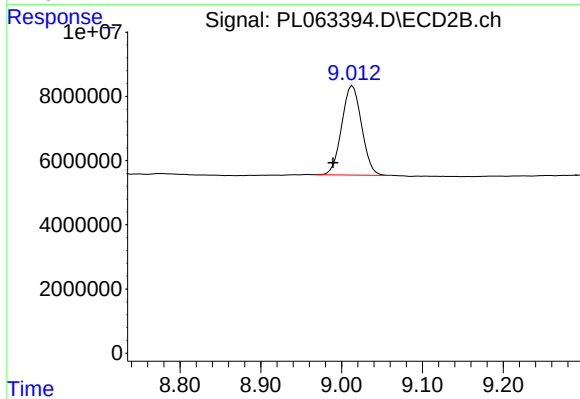

#28 Decachlorobiphenyl

R.T.: 9.012 min
Delta R.T.: 0.023 min
Response: 47594041
Conc: 20.00 ng/ml m