

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120821\
 Data File : PL071328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2021 13:49
 Operator : AR\AJ
 Sample : M4959-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 05:08:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.500	9450599	23788592	20.121	18.956
28)	SA Decachlor...	10.327	11.392	12491914	22406469	17.252	16.120
Target Compounds							
7)	B delta-BHC	0.000	7.022f	0	1003763	N.D.	0.590 #
9)	A Endosulfan I	7.429f	0.000	576024	0	0.969	N.D. #
11)	B alpha-Chl...	7.363	8.308	444552	905787	0.695	0.570
13)	MA Dieldrin	7.699	0.000	374383	0	0.619	N.D. #
17)	MA 4,4'-DDT	8.408	9.357	431679	880568	0.789	0.633
20)	A Methoxychlor	9.026f	0.000	392624	0	1.087	N.D. #
21)	B Endrin ke...	0.000	9.968f	0	464388	N.D.	0.317 #
26)	Chlordane-4	7.363f	8.308	444552	905787	6.703	3.414 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120821\
Data File : PL071328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2021 13:49
Operator : AR\AJ
Sample : M4959-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 05:08:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

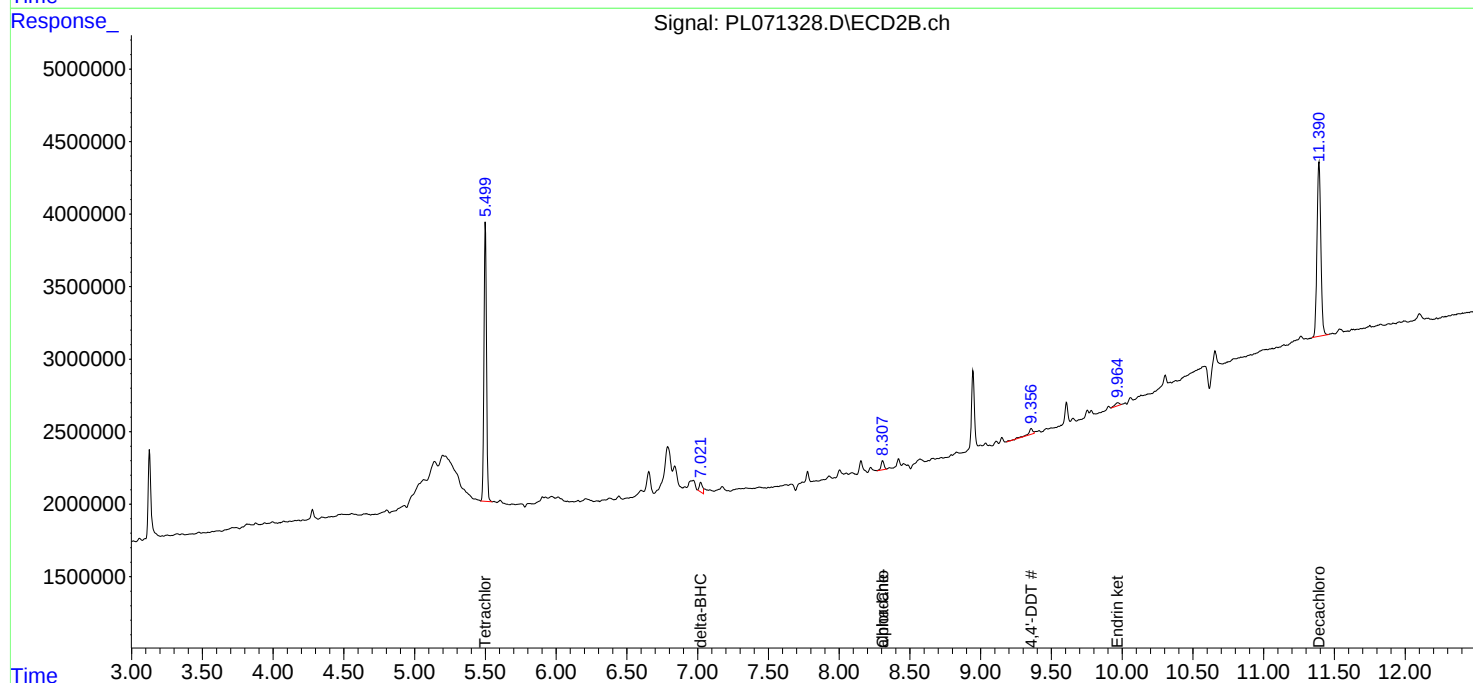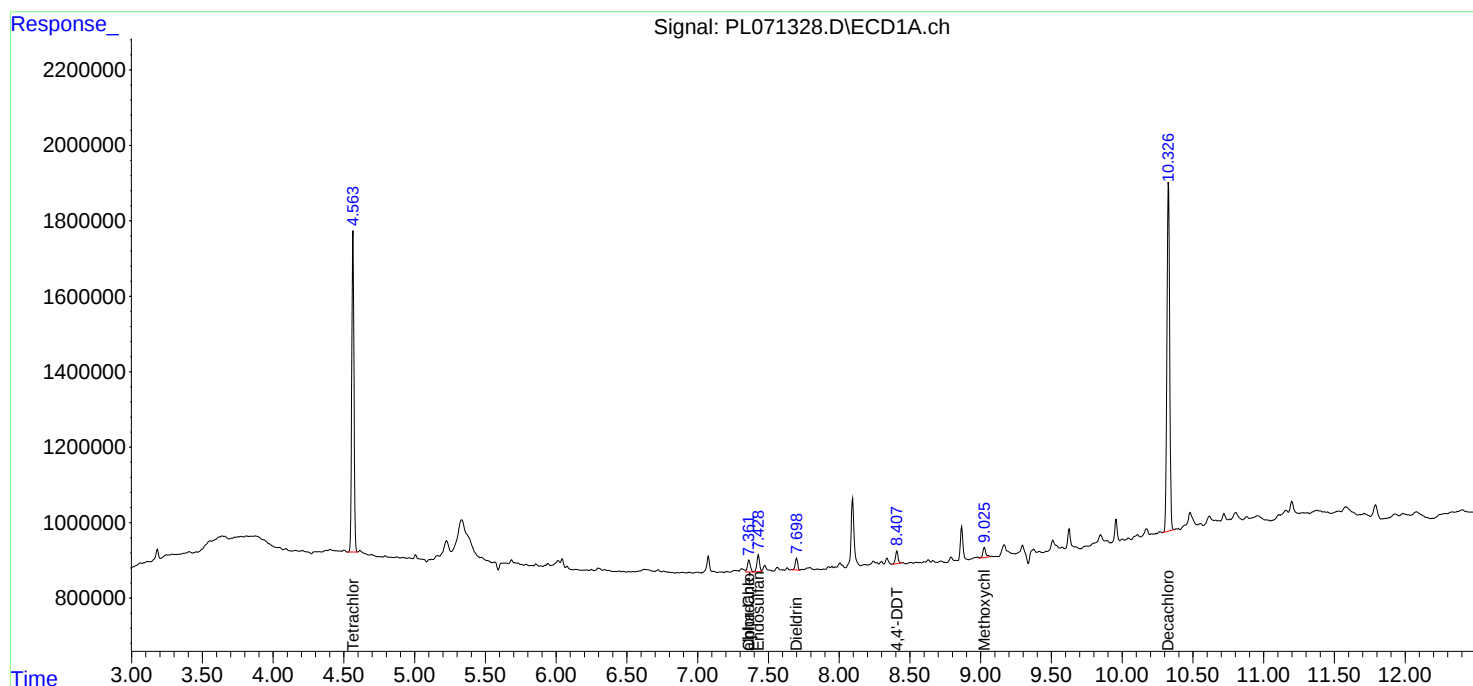


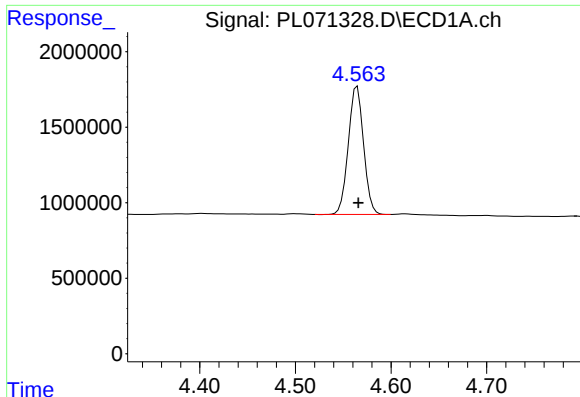

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: -0.001 min
Response: 9450599
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

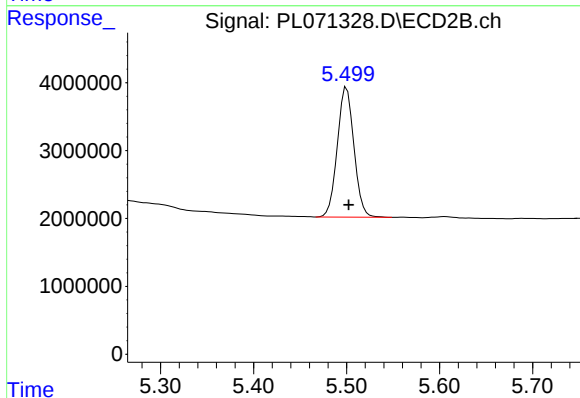


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 23788592
Conc: 18.96 ng/ml

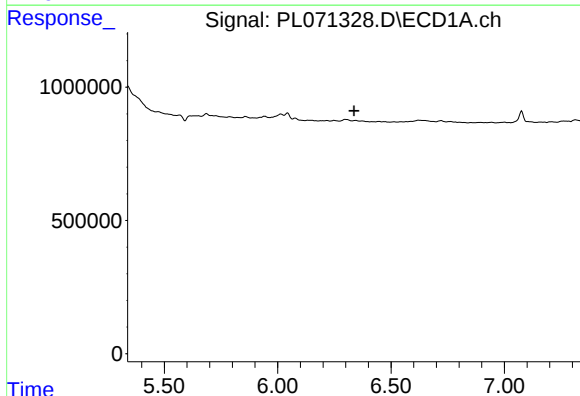


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

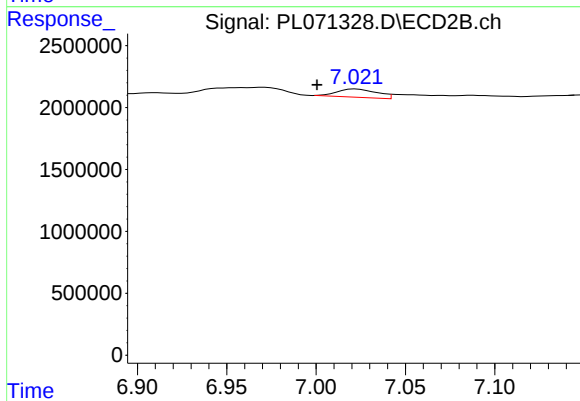

#7 delta-BHC


R.T.: 7.022 min
Delta R.T.: 0.022 min
Response: 1003763
Conc: 0.59 ng/ml

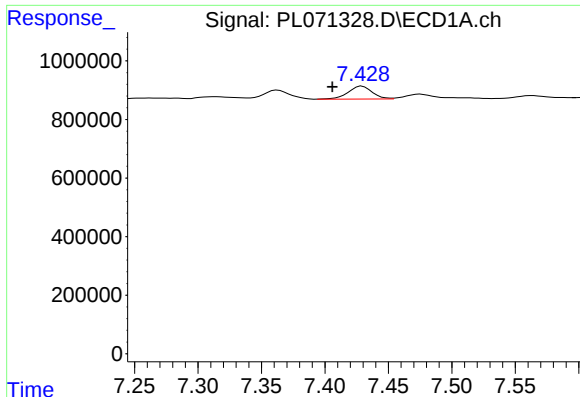

#9 Endosulfan I


R.T.: 7.429 min
Delta R.T.: 0.024 min
Response: 576024
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

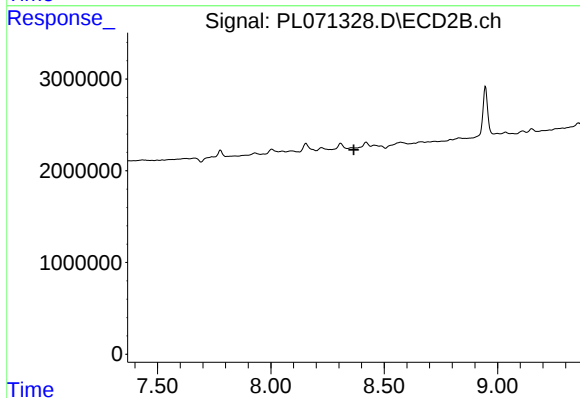


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.366 min
Response: 0
Conc: N.D.

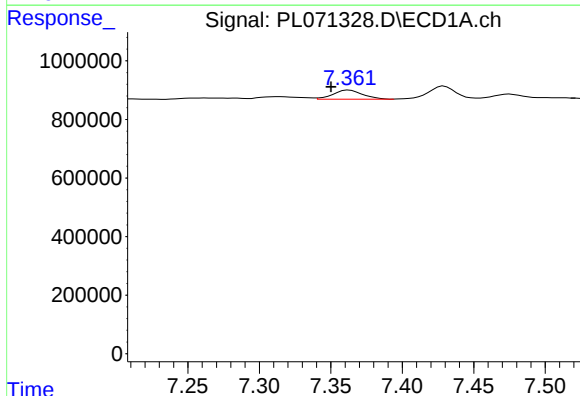


#11 alpha-Chlordane

R.T.: 7.363 min
Delta R.T.: 0.013 min
Response: 444552
Conc: 0.69 ng/ml

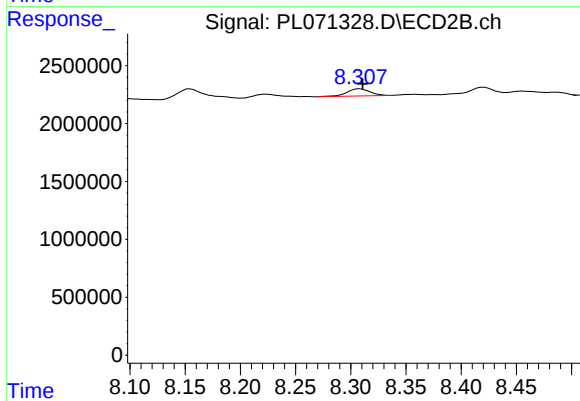

#11 alpha-Chlordane


R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 905787
Conc: 0.57 ng/ml

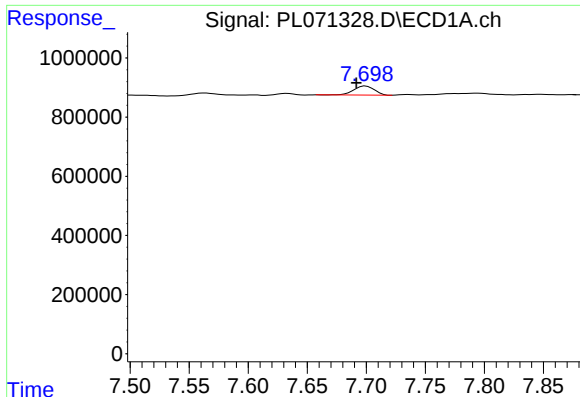

#13 Dieldrin


R.T.: 7.699 min
Delta R.T.: 0.008 min
Response: 374383
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

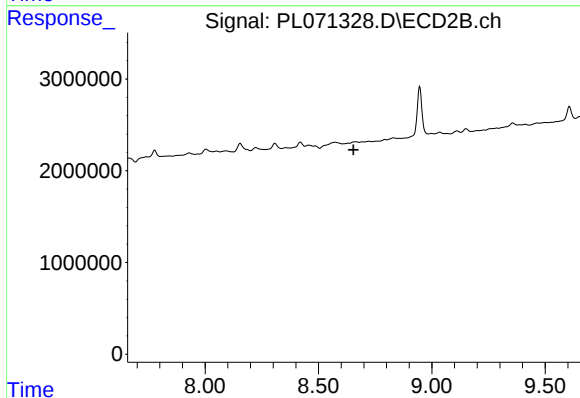


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.655 min
Response: 0
Conc: N.D.

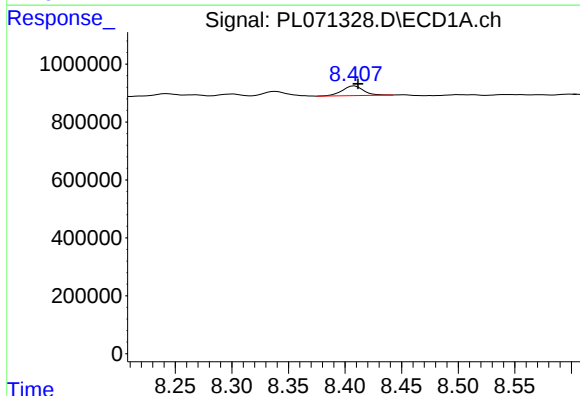


#17 4,4'-DDT

R.T.: 8.408 min
Delta R.T.: -0.003 min
Response: 431679
Conc: 0.79 ng/ml

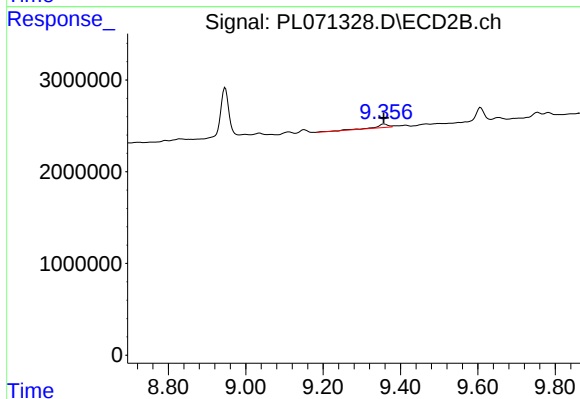

#17 4,4'-DDT


R.T.: 9.357 min
Delta R.T.: 0.000 min
Response: 880568
Conc: 0.63 ng/ml

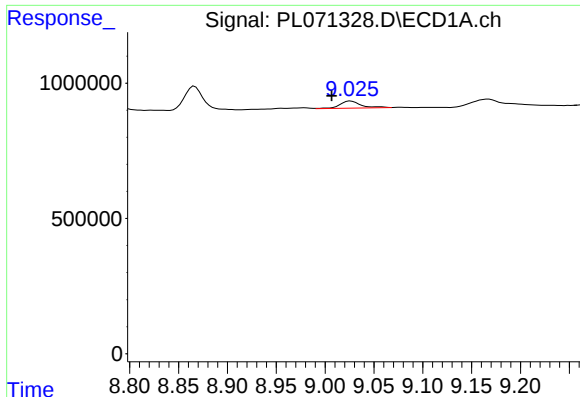

#20 Methoxychlor


R.T.: 9.026 min
Delta R.T.: 0.020 min
Response: 392624
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

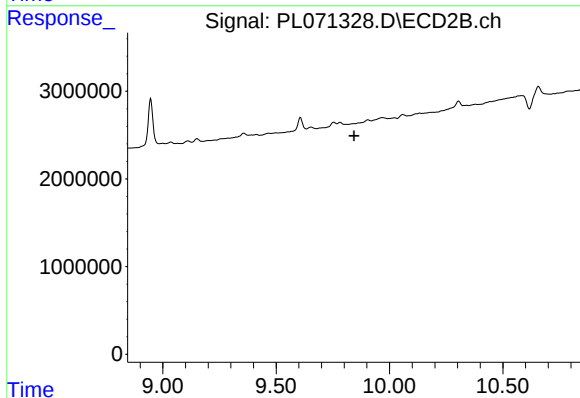


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

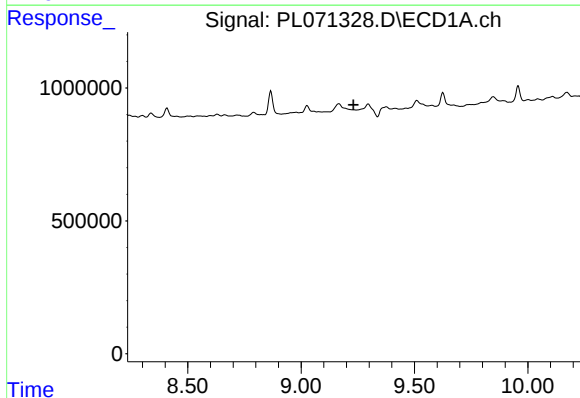


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

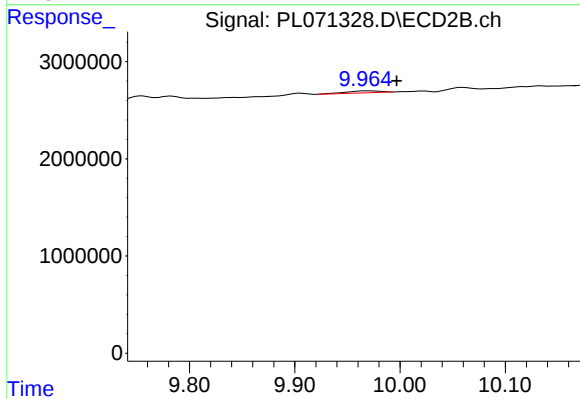

#21 Endrin ketone


R.T.: 9.968 min
Delta R.T.: -0.029 min
Response: 464388
Conc: 0.32 ng/ml

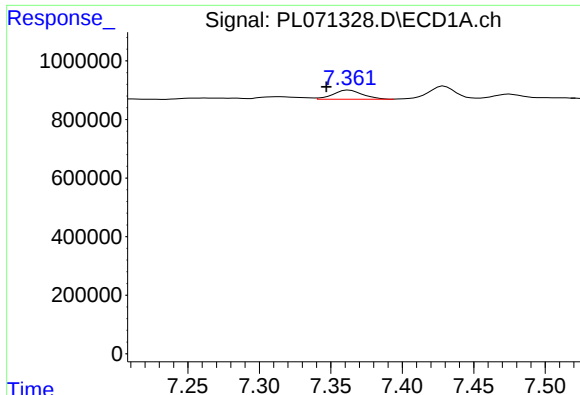

#26 Chlordane-4


R.T.: 7.363 min
Delta R.T.: 0.016 min
Response: 444552
Conc: 6.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

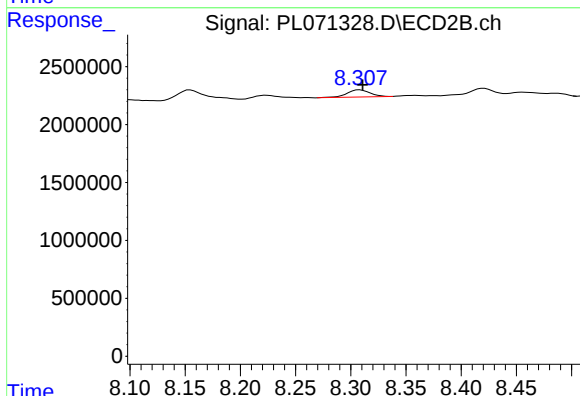


#26 Chlordane-4

R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 905787
Conc: 3.41 ng/ml

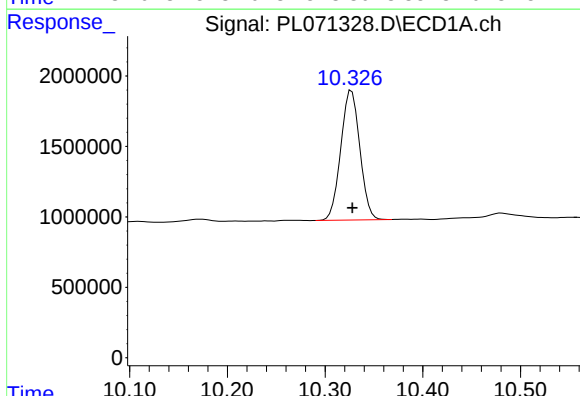

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.000 min
Response: 12491914
Conc: 17.25 ng/ml

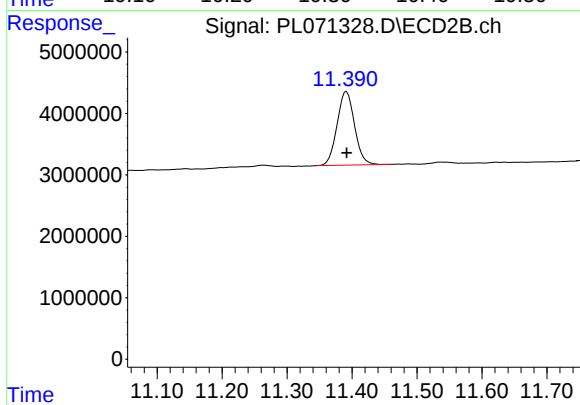

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 22406469
Conc: 16.12 ng/ml