

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120821\
 Data File : PL071337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2021 16:23
 Operator : AR\AJ
 Sample : M4959-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 05:09:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	9951431	24838371	21.187	19.793
28)	SA Decachlor...	10.328	11.392	13361019	22685698	18.452	16.321
Target Compounds							
15)	B Endosulfa...	8.264f	9.154f	257030	475825	0.440	0.353
20)	A Methoxychlor	8.985f	0.000	129483	0	0.358	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120821\
Data File : PL071337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2021 16:23
Operator : AR\AJ
Sample : M4959-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 05:09:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

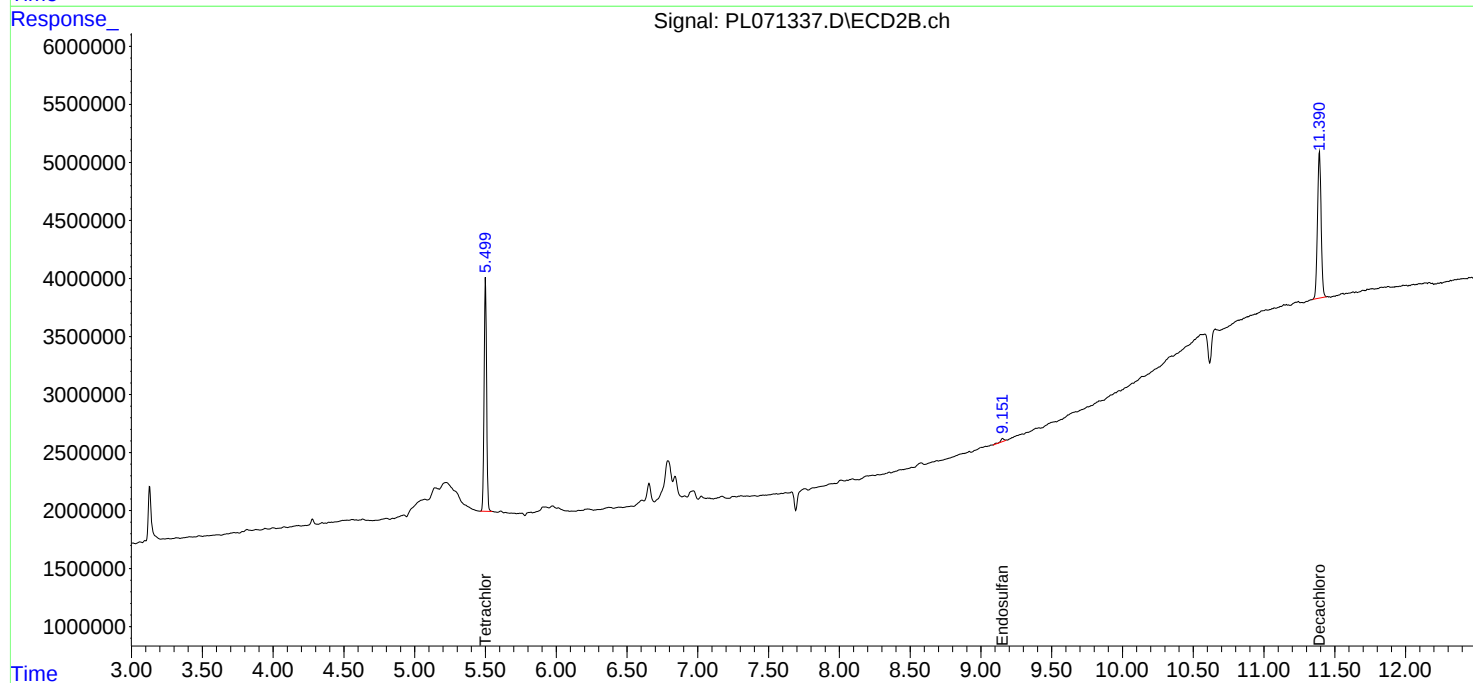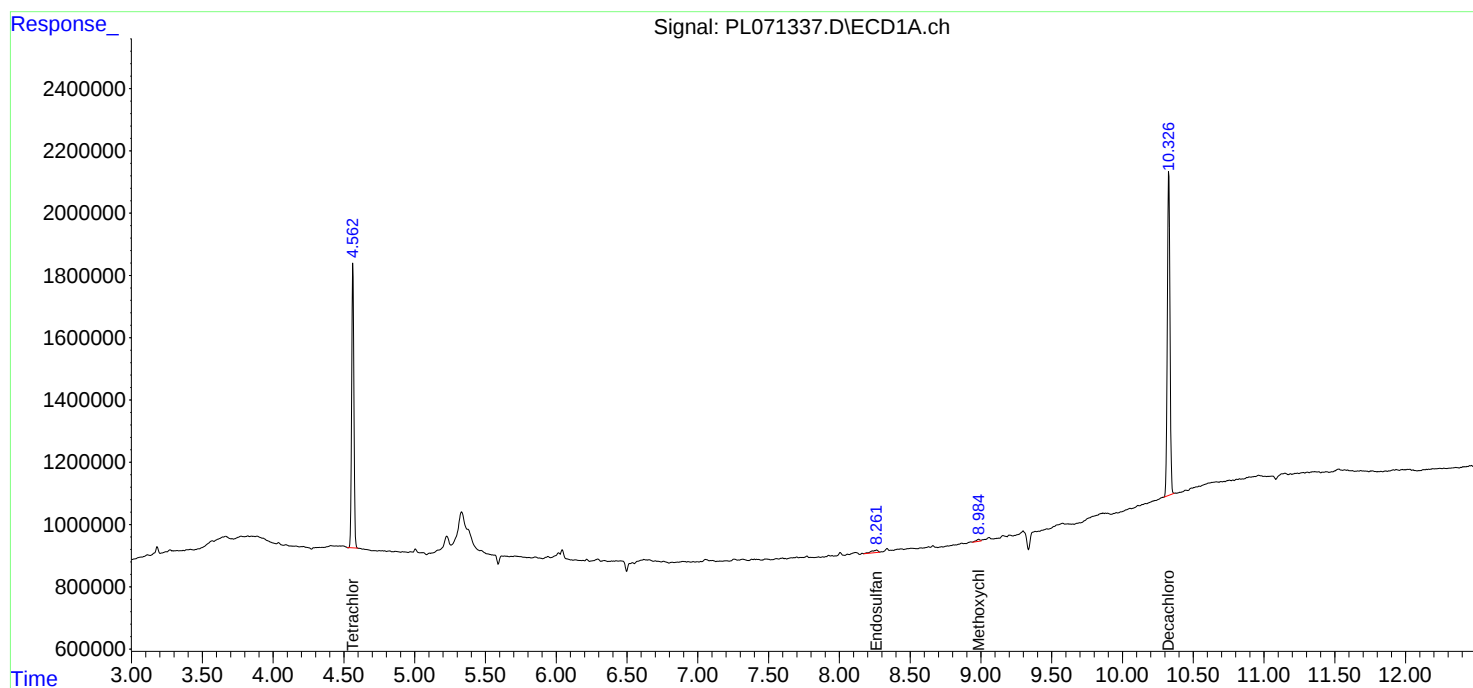


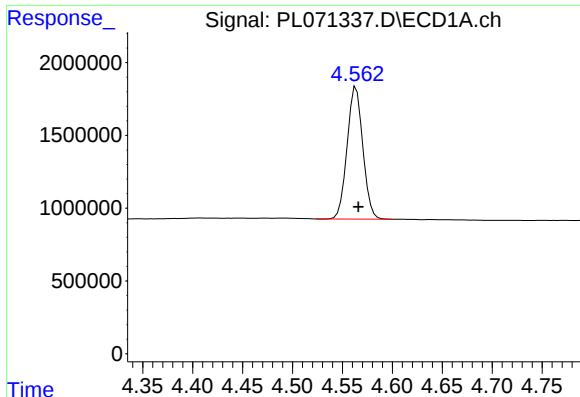

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: -0.002 min
Response: 9951431
Conc: 21.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

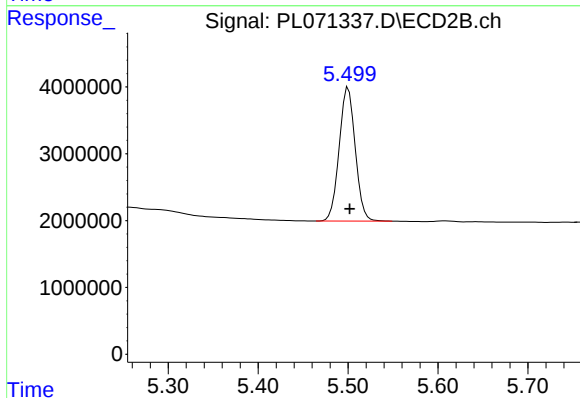


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 24838371
Conc: 19.79 ng/ml

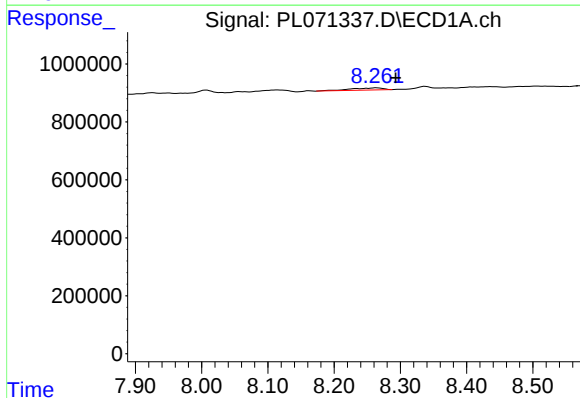


#15 Endosulfan II

R.T.: 8.264 min
Delta R.T.: -0.029 min
Response: 257030
Conc: 0.44 ng/ml

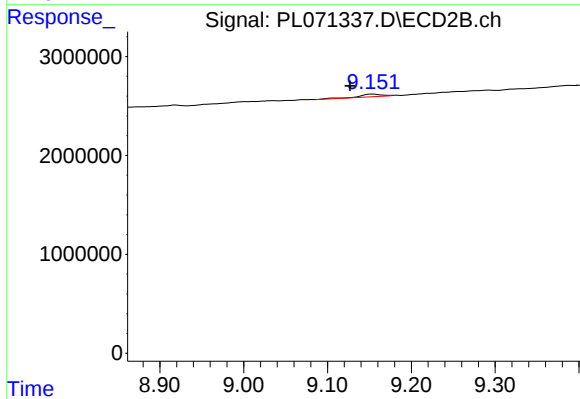

#15 Endosulfan II

R.T.: 9.154 min
Delta R.T.: 0.027 min
Response: 475825
Conc: 0.35 ng/ml

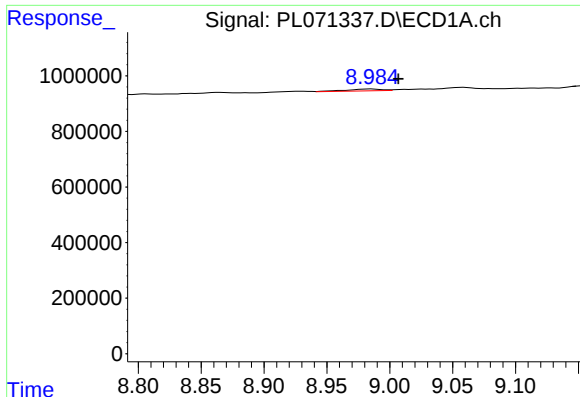


#20 Methoxychlor

R.T.: 8.985 min
Delta R.T.: -0.022 min
Response: 129483
Conc: 0.36 ng/ml

Instrument :


ECD_L

ClientSampleId :

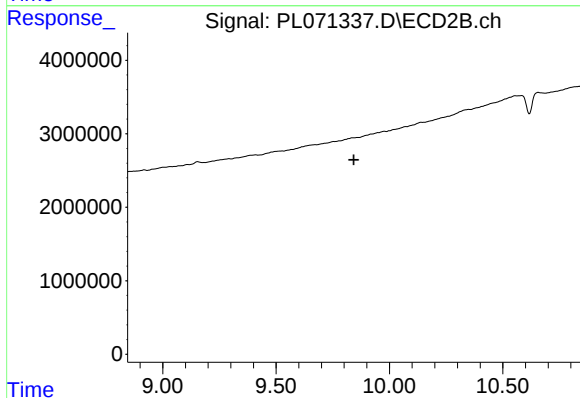


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

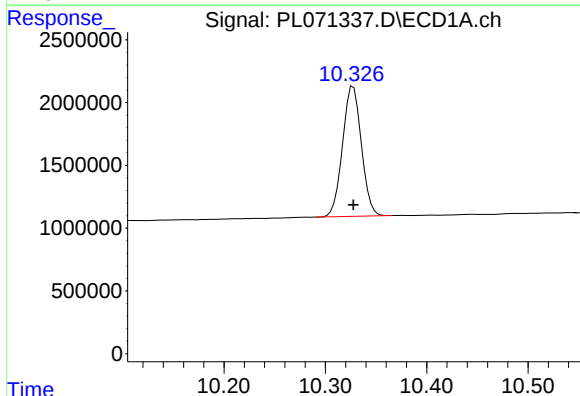

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 13361019
Conc: 18.45 ng/ml

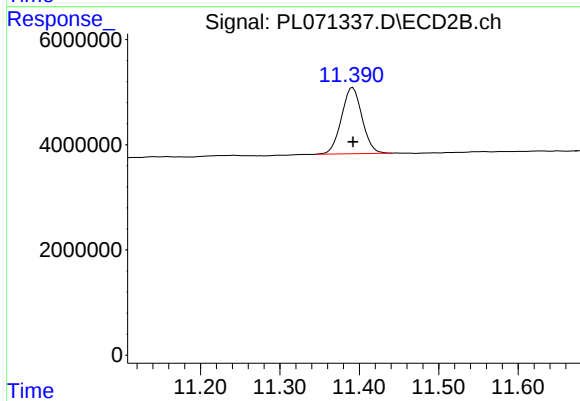

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 22685698
Conc: 16.32 ng/ml