

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120821\
 Data File : PL071339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2021 16:56
 Operator : AR\AJ
 Sample : M4953-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 05:10:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.500	10268195	27224867	21.861	21.694
28)	SA Decachlor...	10.328	11.392	3489035	5981405	4.818	4.303
Target Compounds							
7)	B delta-BHC	0.000	7.021f	0	227866	N.D.	0.134 #
9)	A Endosulfan I	7.408	0.000	425284	0	0.715	N.D. #
11)	B alpha-Chl...	7.357	0.000	416261	0	0.650	N.D. #
15)	B Endosulfa...	0.000	9.152f	0	946262	N.D.	0.702 #
18)	B Endrin al...	0.000	9.275	0	892401	N.D.	0.864 #
20)	A Methoxychlor	8.981f	0.000	10051	0	0.028	N.D. #
21)	B Endrin ke...	0.000	10.025f	0	566483	N.D.	0.387 #
26)	Chlordane-4	7.357	0.000	416261	0	6.276	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120821\
Data File : PL071339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2021 16:56
Operator : AR\AJ
Sample : M4953-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 05:10:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

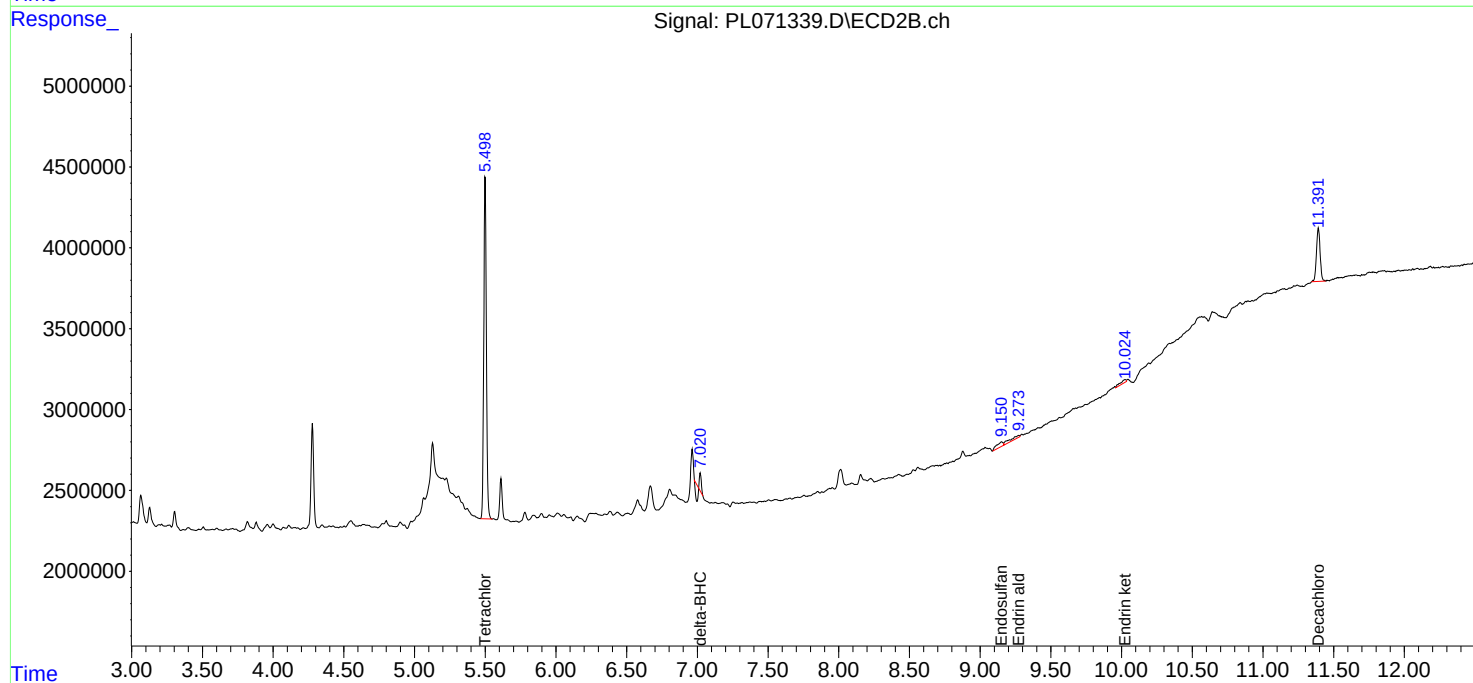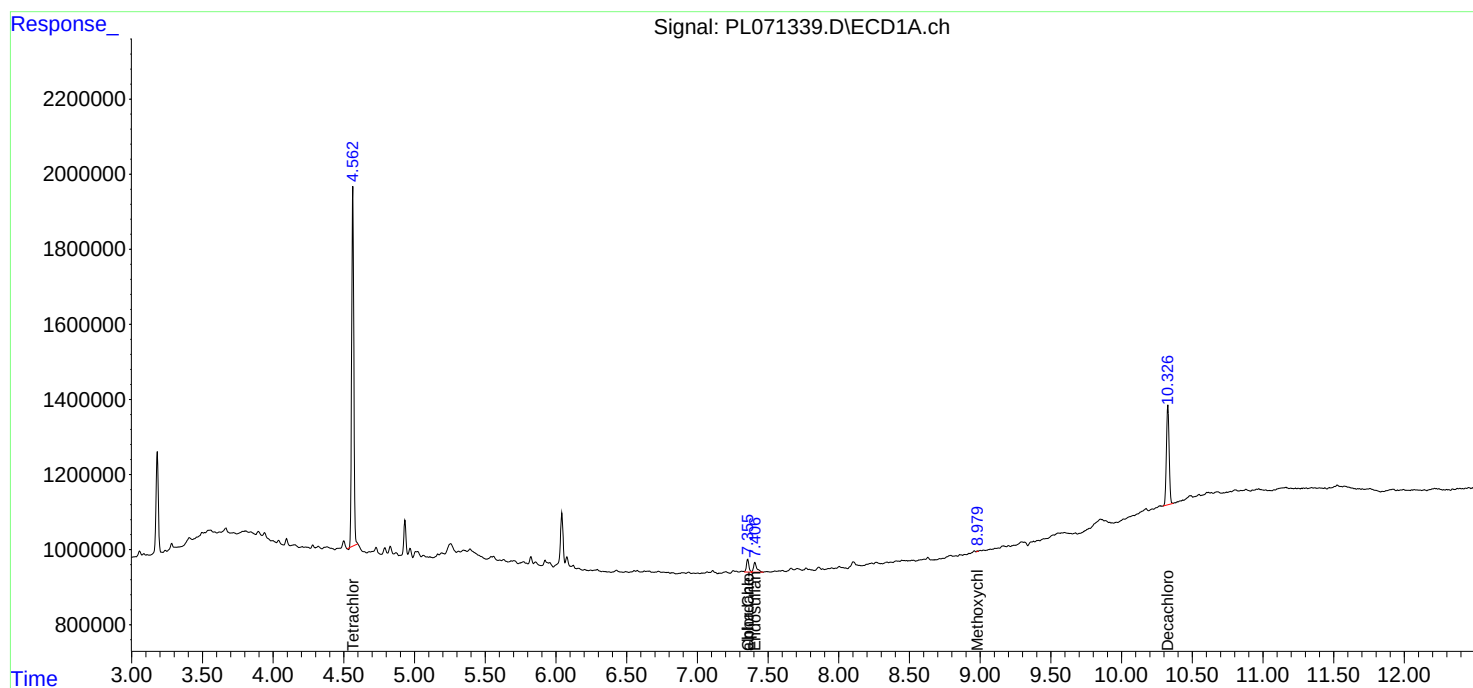


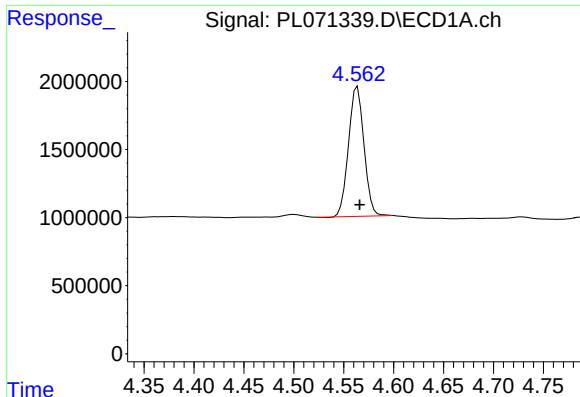

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: -0.002 min
Response: 10268195
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

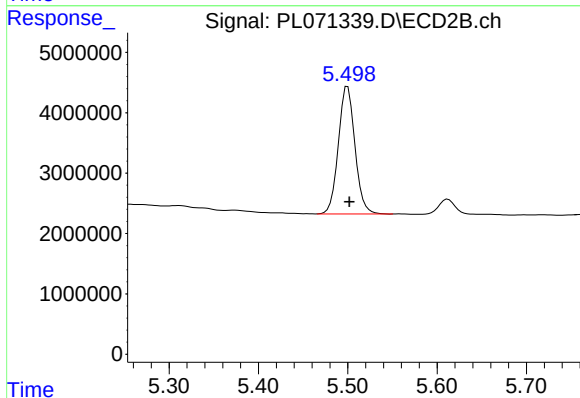


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 27224867
Conc: 21.69 ng/ml

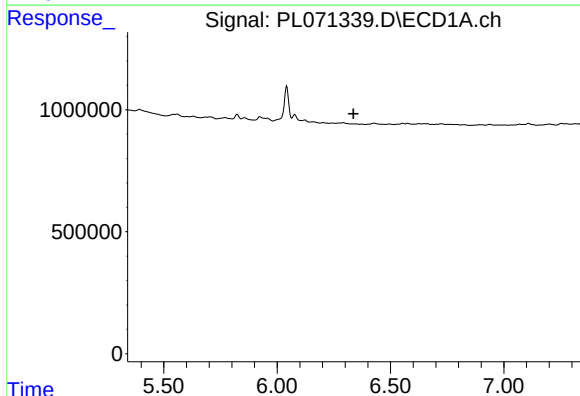


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

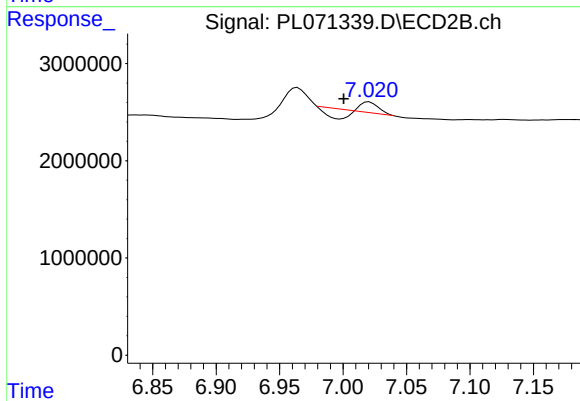

#7 delta-BHC


R.T.: 7.021 min
Delta R.T.: 0.020 min
Response: 227866
Conc: 0.13 ng/ml

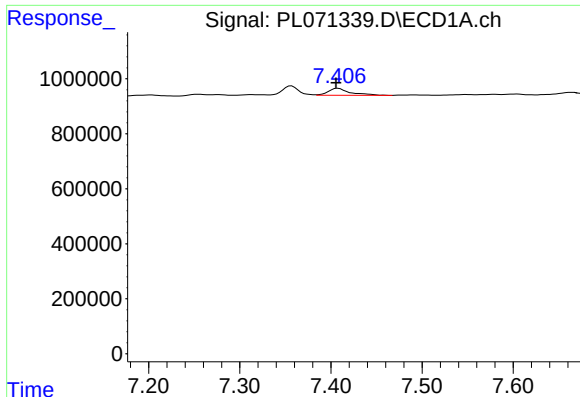

#9 Endosulfan I


R.T.: 7.408 min
Delta R.T.: 0.002 min
Response: 425284
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

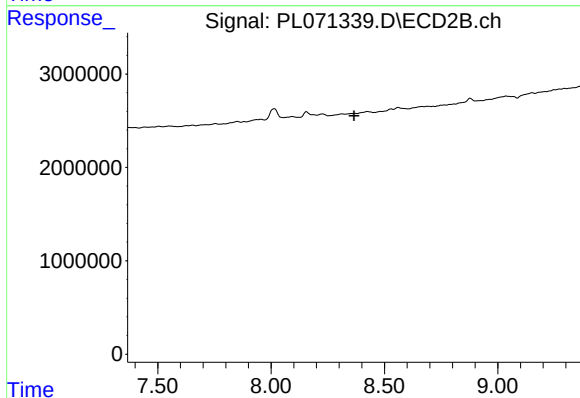


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.366 min
Response: 0
Conc: N.D.

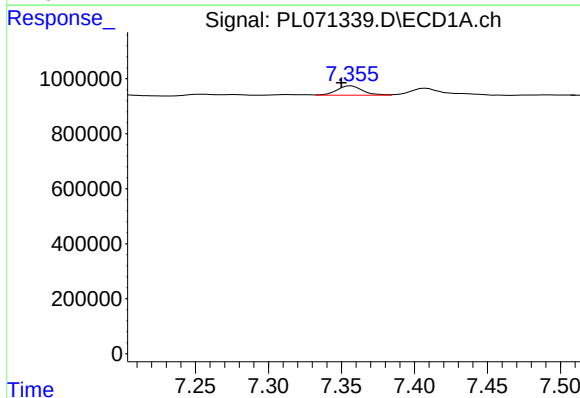


#11 alpha-Chlordane

R.T.: 7.357 min
Delta R.T.: 0.007 min
Response: 416261
Conc: 0.65 ng/ml

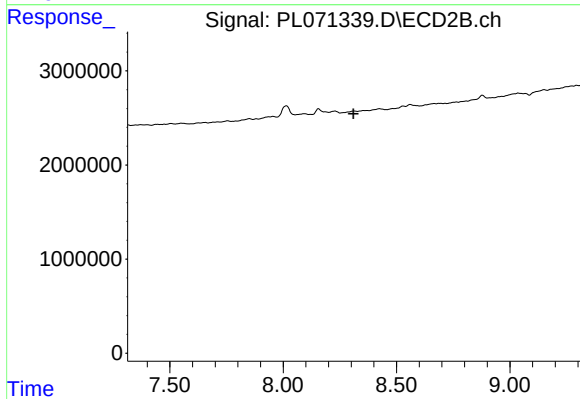

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

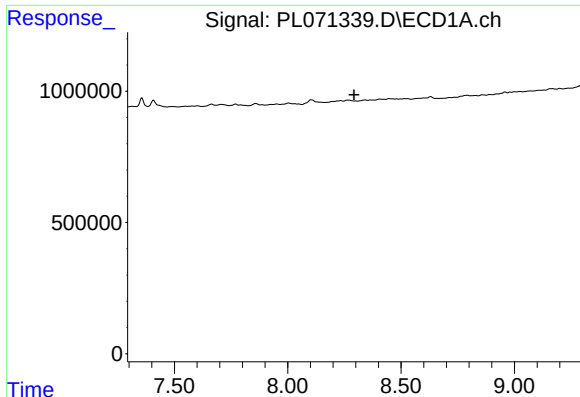

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

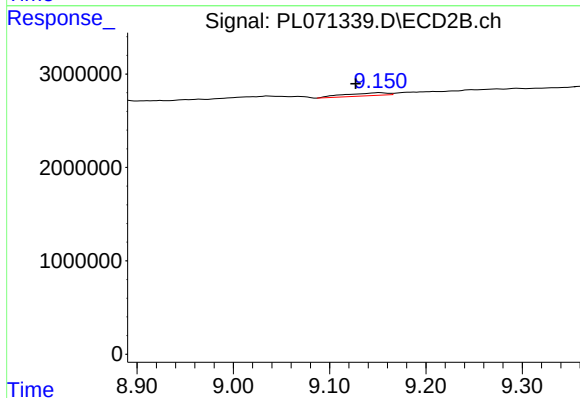


#15 Endosulfan II

R.T.: 9.152 min
Delta R.T.: 0.025 min
Response: 946262
Conc: 0.70 ng/ml

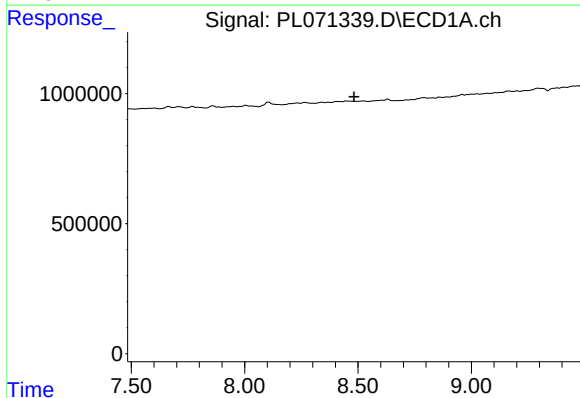


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.483 min
Response: 0
Conc: N.D.

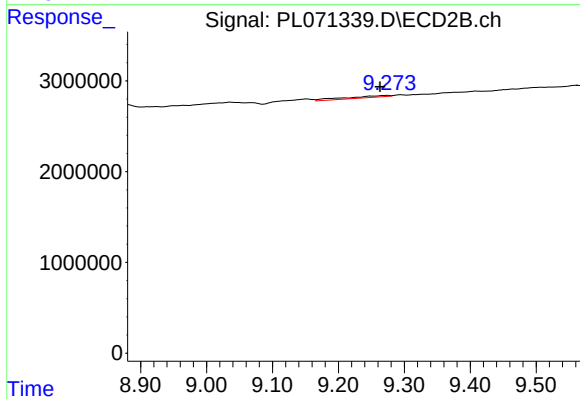

#18 Endrin aldehyde


R.T.: 9.275 min
Delta R.T.: 0.012 min
Response: 892401
Conc: 0.86 ng/ml

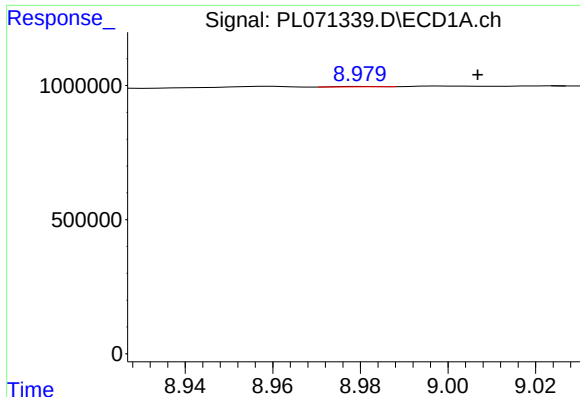

#20 Methoxychlor


R.T.: 8.981 min
Delta R.T.: -0.026 min
Response: 10051
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

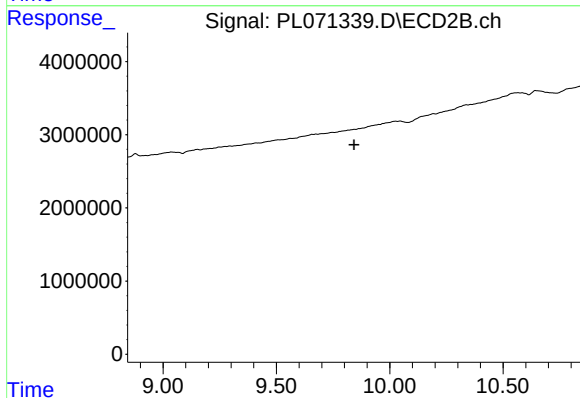


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

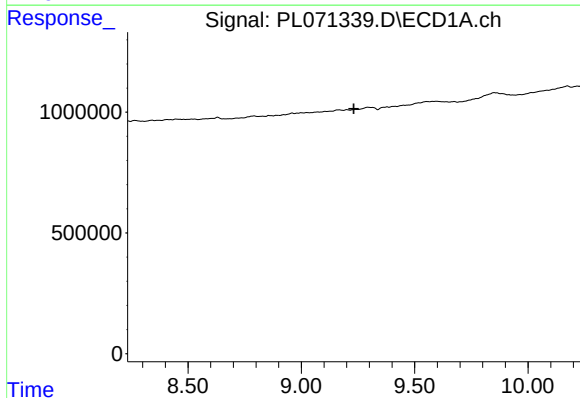


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

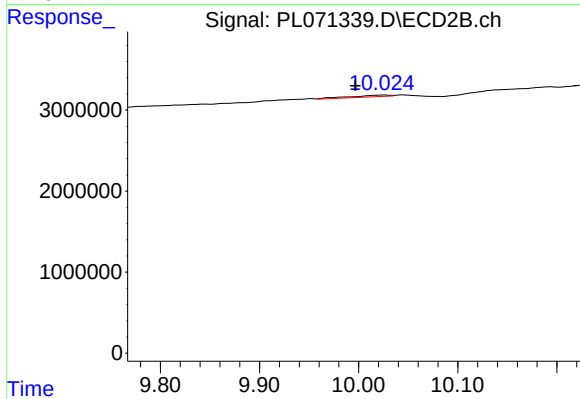

#21 Endrin ketone


R.T.: 10.025 min
Delta R.T.: 0.029 min
Response: 566483
Conc: 0.39 ng/ml

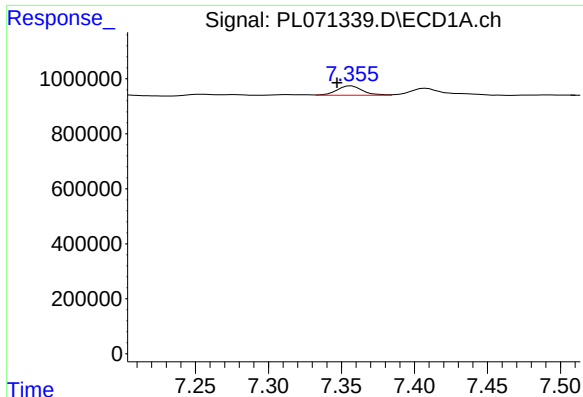

#26 Chlordane-4


R.T.: 7.357 min
Delta R.T.: 0.010 min
Response: 416261
Conc: 6.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

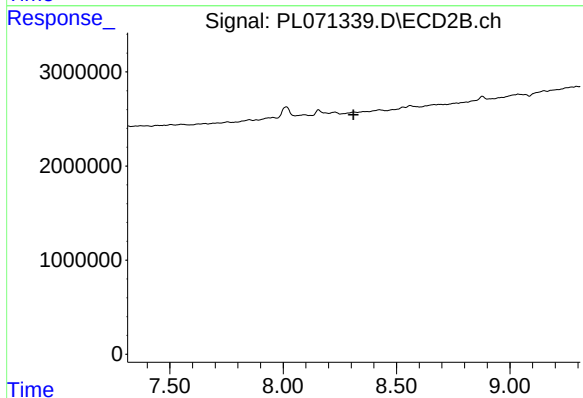


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

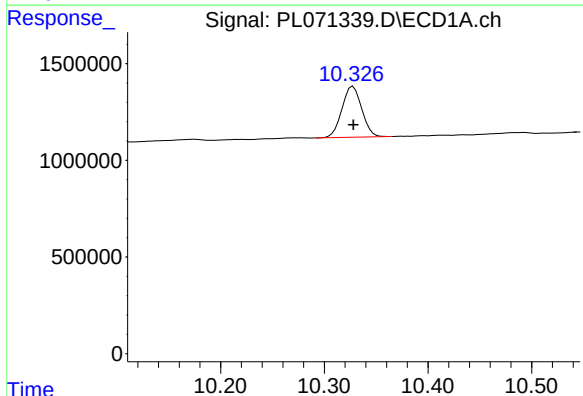

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 3489035
Conc: 4.82 ng/ml

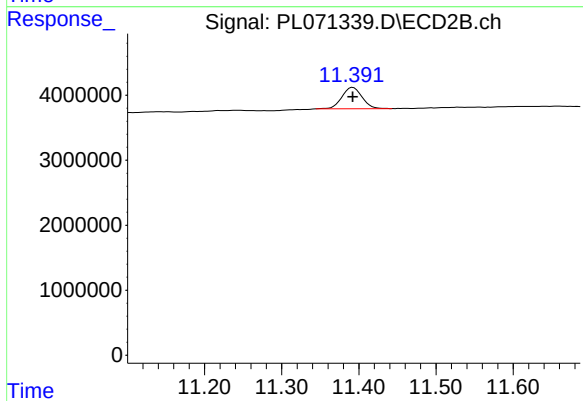

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 5981405
Conc: 4.30 ng/ml