

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120822\
 Data File : PL079641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2022 17:44
 Operator : AR\AJ
 Sample : N5932-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/09/2022
 Supervised By :Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 20:22:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.316	2.565	29076953	38815325	12.871m	14.260
28) SA Decachlor...	8.765	7.630	25994801	36138112	13.385	15.383

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120822\
Data File : PL079641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2022 17:44
Operator : AR\AJ
Sample : N5932-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/09/2022
Supervised By : Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 20:22:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

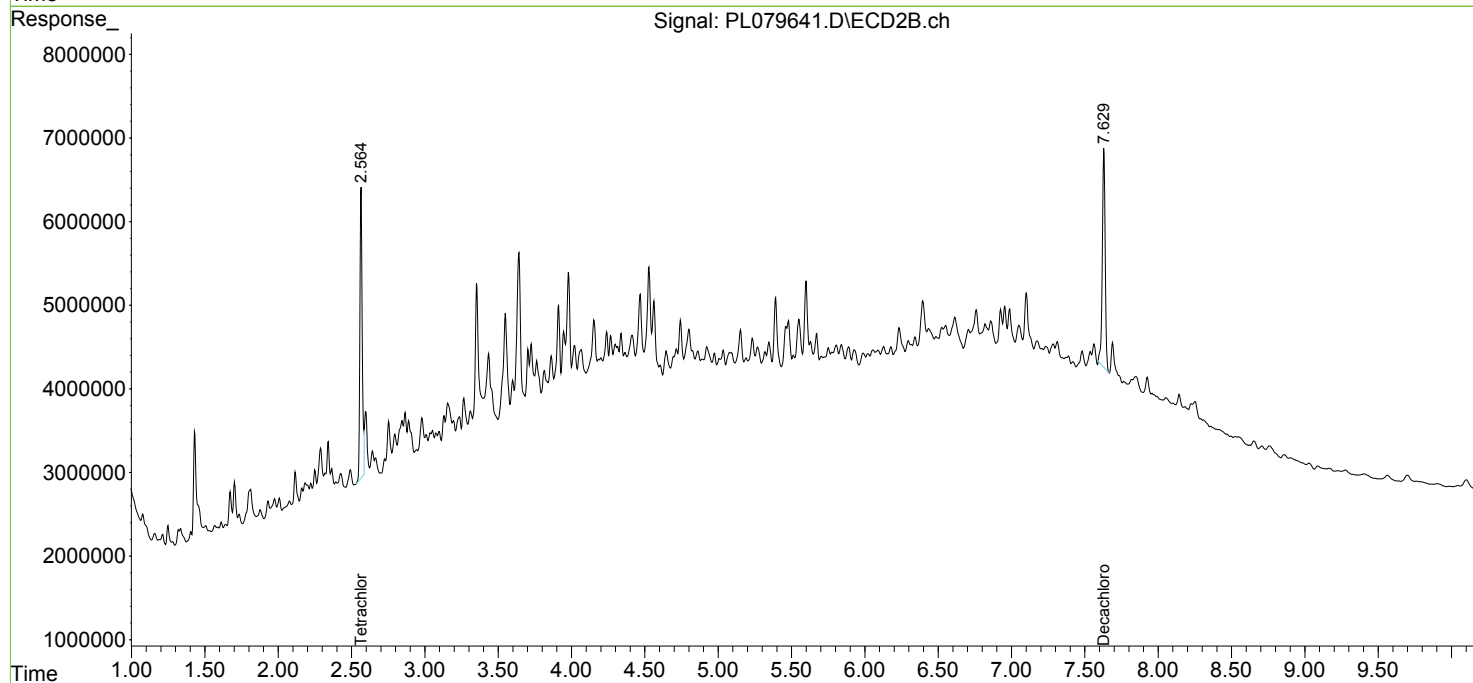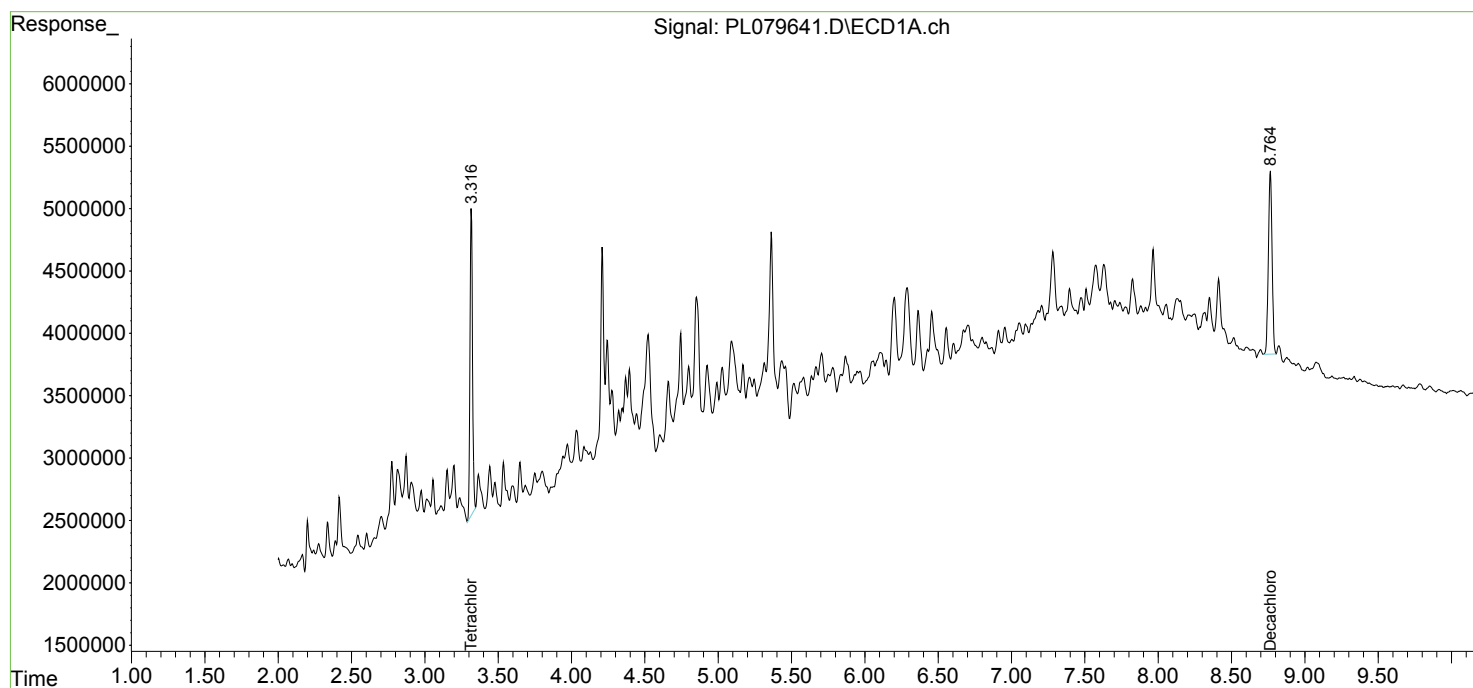

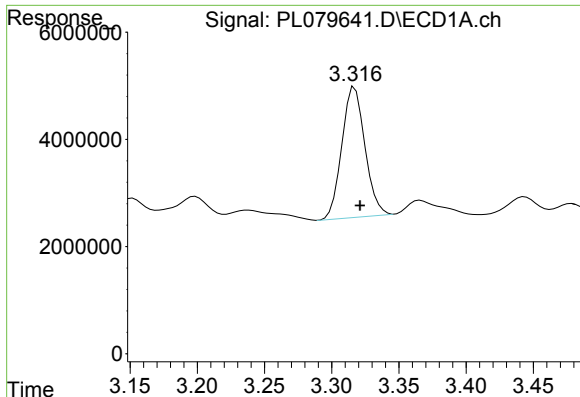


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.005 min
Response: 29076953
Conc: 12.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

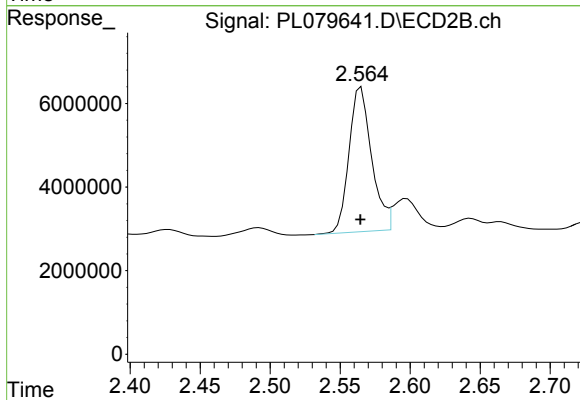


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: 0.000 min
Response: 38815325
Conc: 14.26 ng/ml

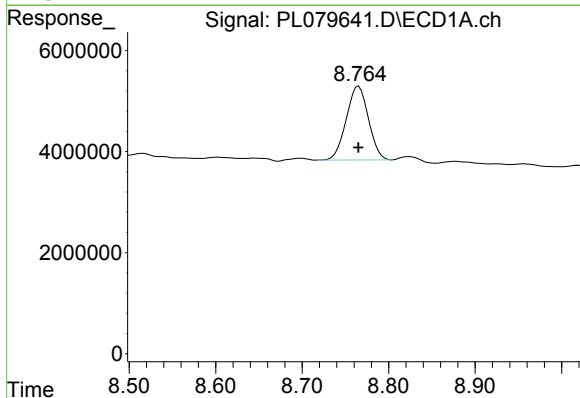

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 25994801
Conc: 13.38 ng/ml

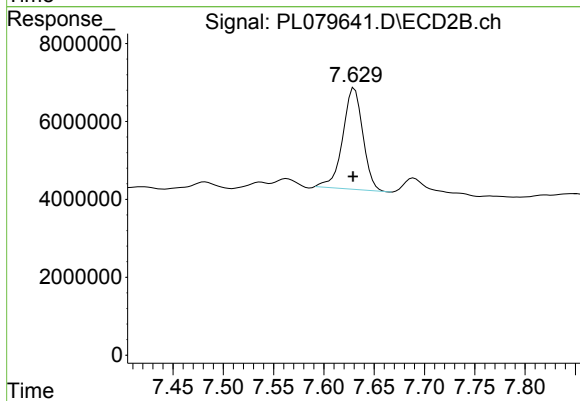

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.001 min
Response: 36138112
Conc: 15.38 ng/ml