

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120822\
 Data File : PL079643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2022 18:12
 Operator : AR\AJ
 Sample : N5936-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MONTHLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/09/2022
 Supervised By :Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 20:23:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.317	2.565	30372011	41295007	13.445	15.171
2) SA Decachlor...	8.763	7.630	26067324	37664209	13.422m	16.032

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120822\
Data File : PL079643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2022 18:12
Operator : AR\AJ
Sample : N5936-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/09/2022
Supervised By : Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 20:23:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

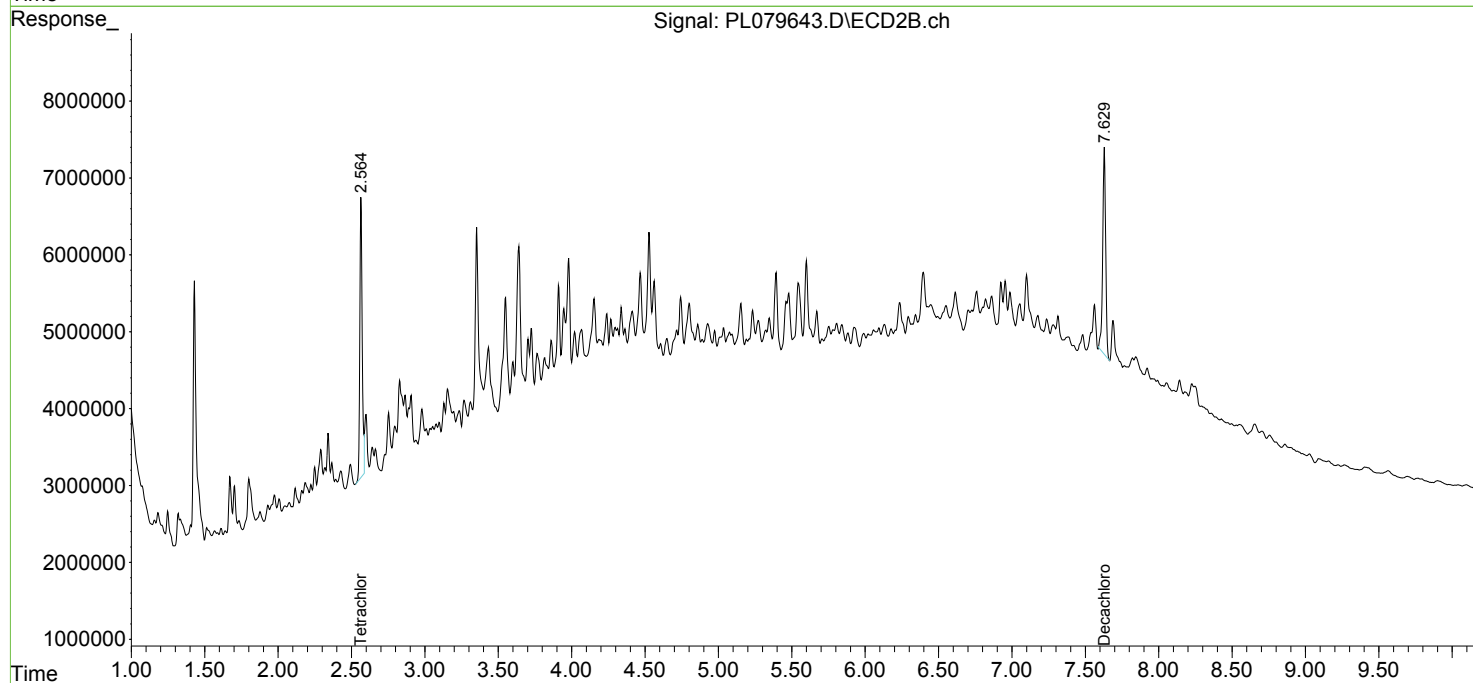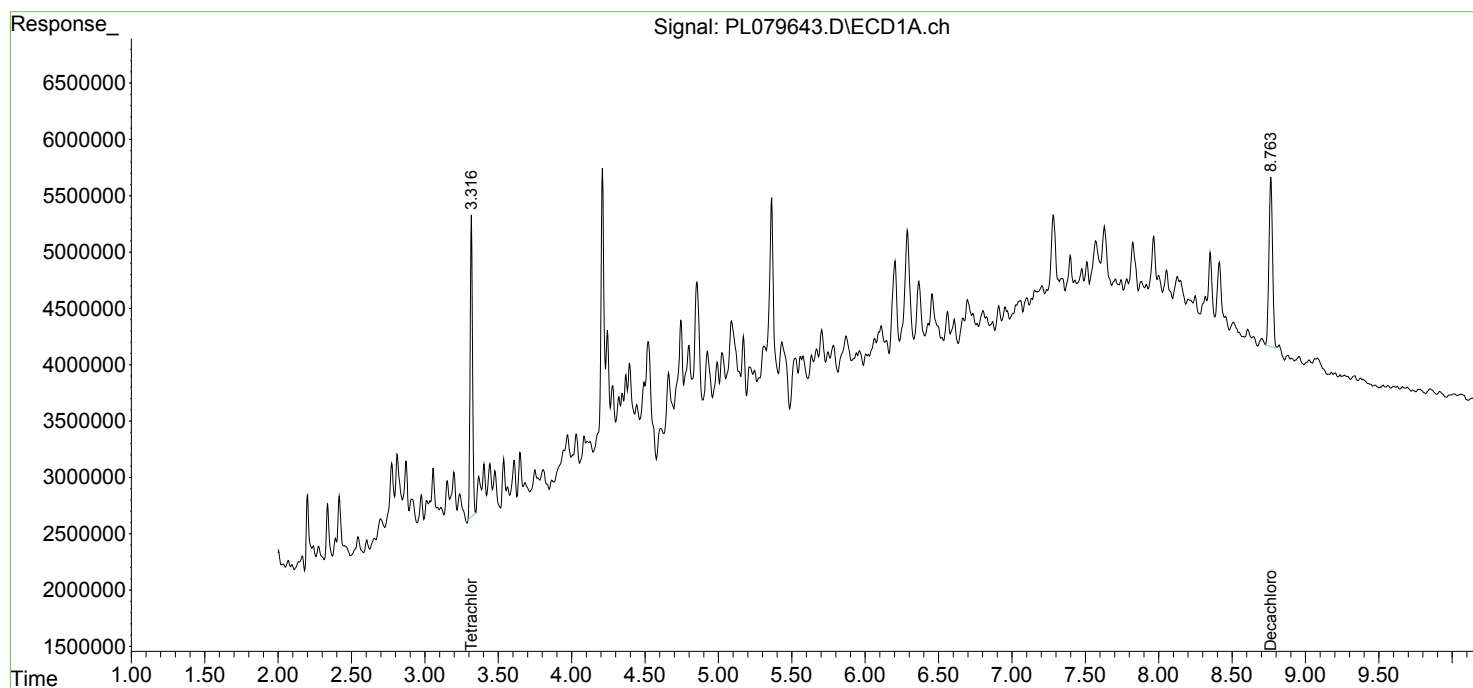

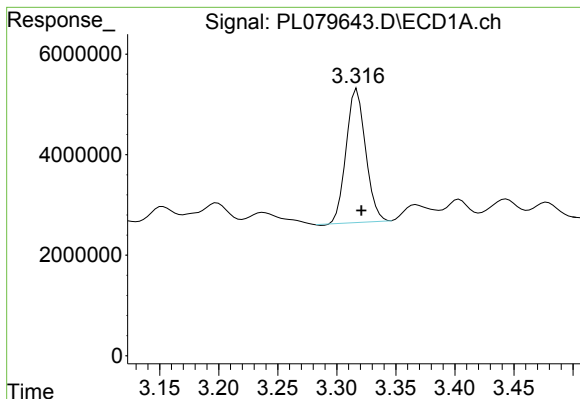


#1 Tetrachloro-m-xylene

R.T.: 3.317 min
Delta R.T.: -0.004 min
Response: 30372011
Conc: 13.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

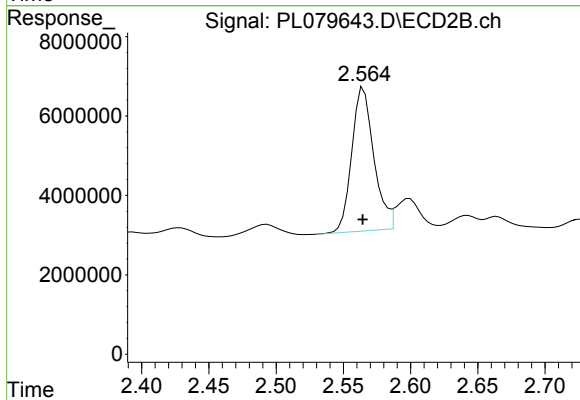


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: 0.000 min
Response: 41295007
Conc: 15.17 ng/ml

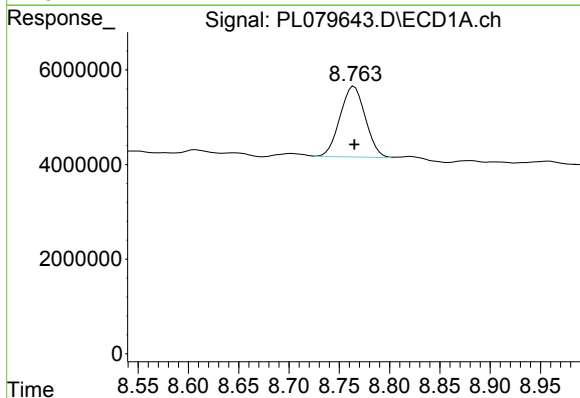

#28 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: -0.002 min
Response: 26067324
Conc: 13.42 ng/ml m

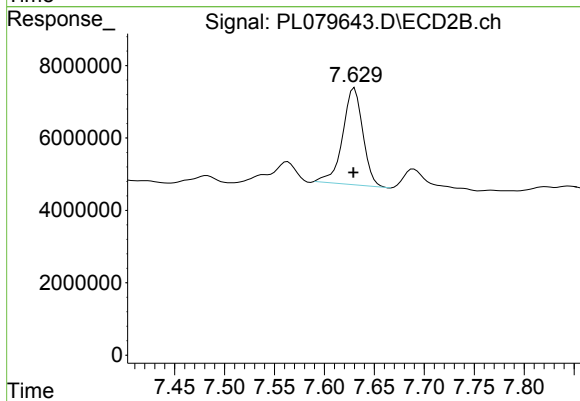

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 37664209
Conc: 16.03 ng/ml