

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120823\
 Data File : PL087043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2023 17:06
 Operator : AR\AJ
 Sample : 05665-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MONTHLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/11/2023
 Supervised By : Ankita Jodhani 12/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 01:12:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 07 00:53:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.452	2.702	44704592	18669223	13.852	19.085 #
2)	SA Decachlor...	9.043	7.893	35050708	15351064	15.334m	15.953

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120823\
Data File : PL087043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2023 17:06
Operator : AR\AJ
Sample : 05665-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 01:12:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120623.M
Quant Title : GC Extractables
QLast Update : Thu Dec 07 00:53:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

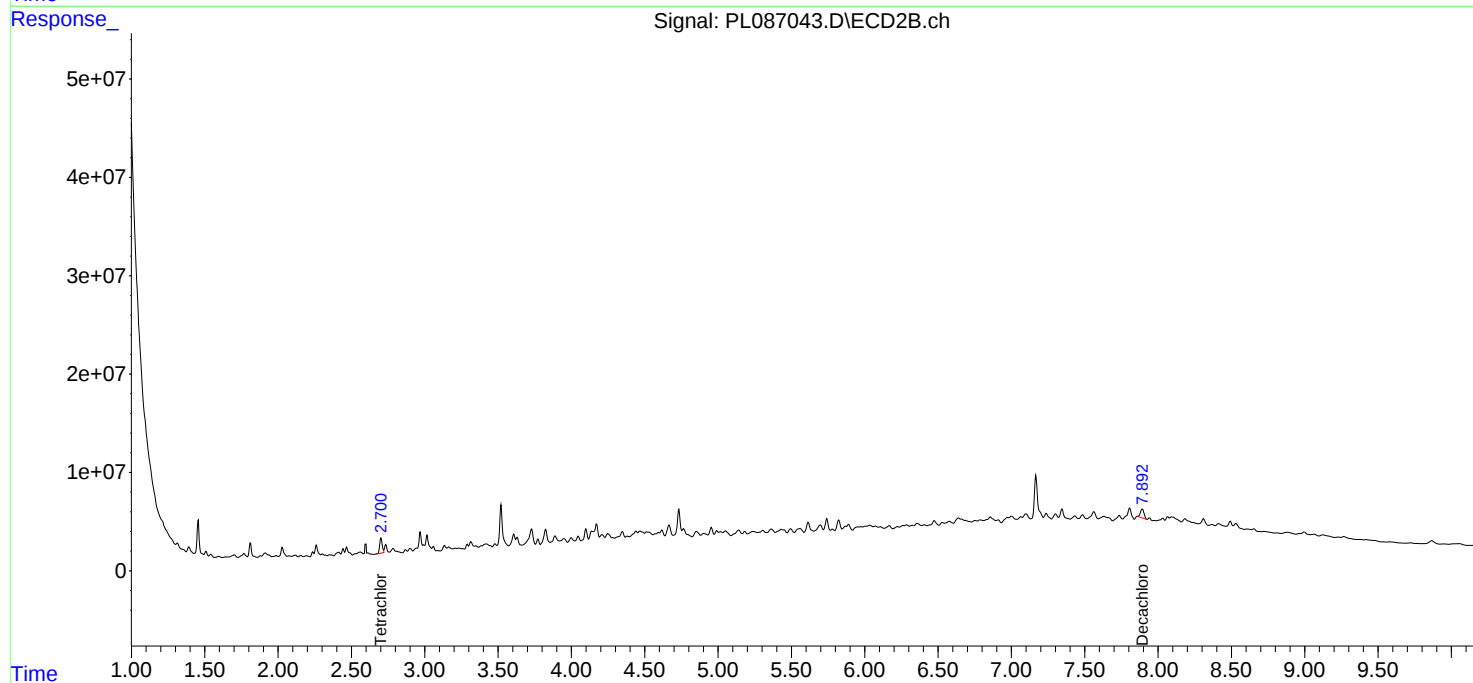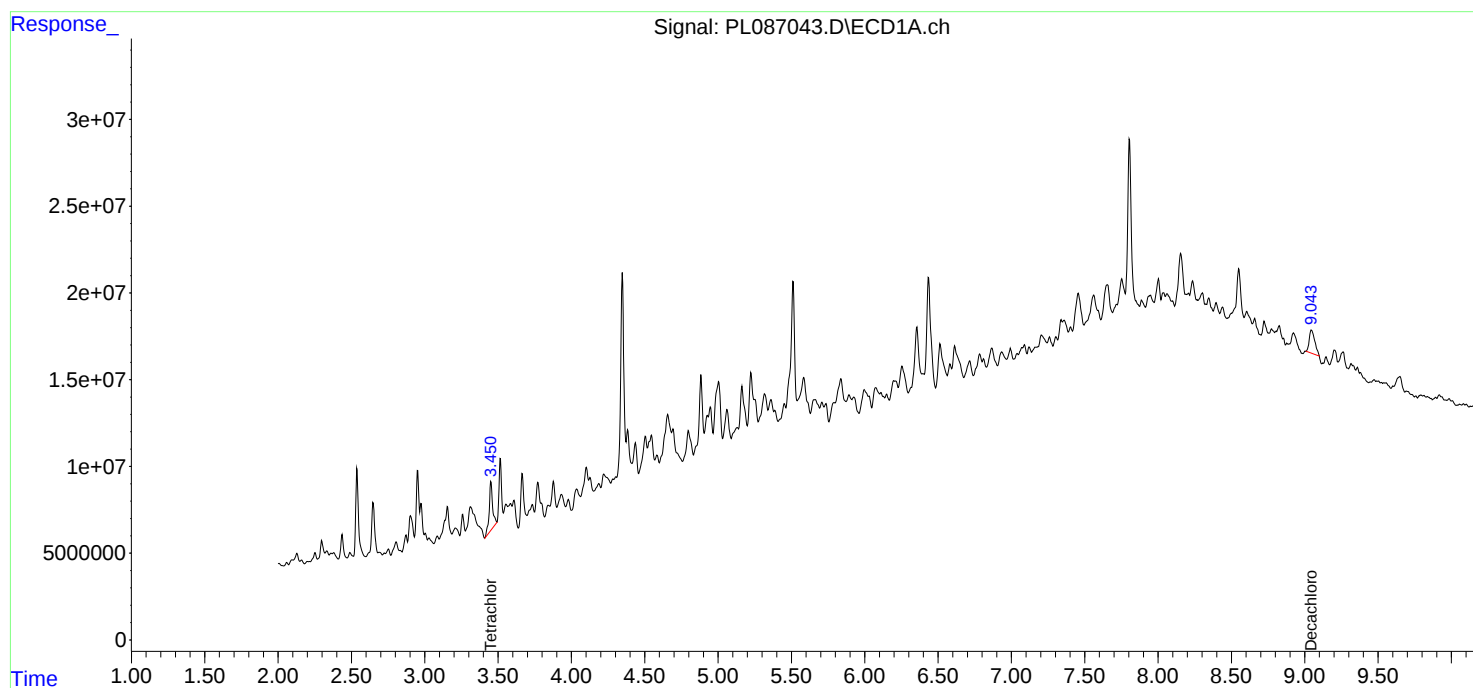

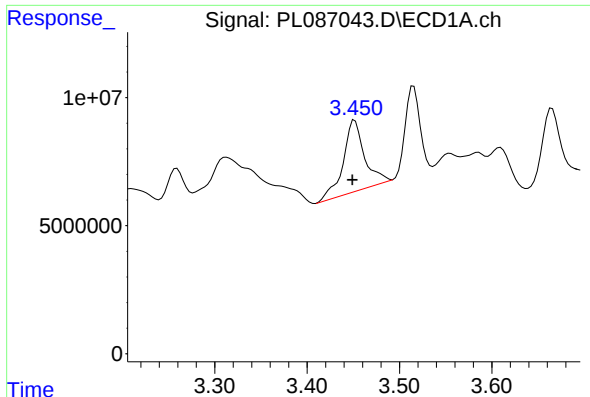


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: 0.003 min
Response: 44704592
Conc: 13.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

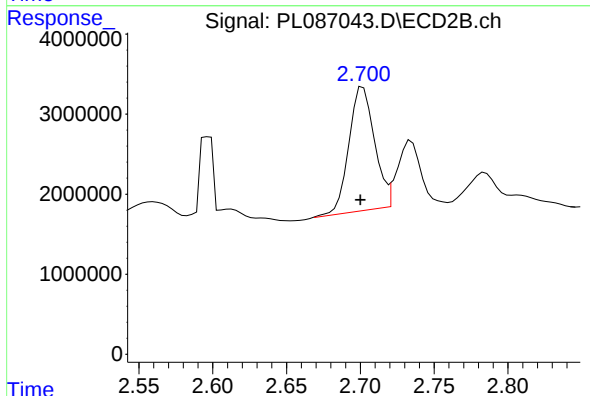


#1 Tetrachloro-m-xylene

R.T.: 2.702 min
Delta R.T.: 0.002 min
Response: 18669223
Conc: 19.09 ng/ml

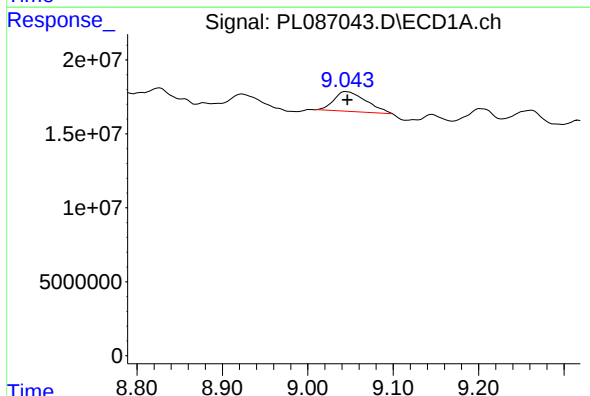

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: -0.003 min
Response: 35050708
Conc: 15.33 ng/ml m

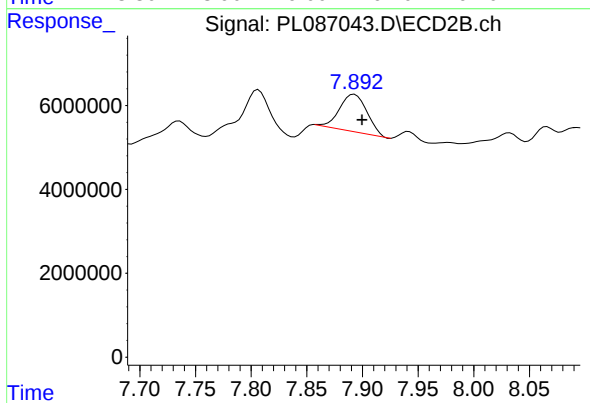

#28 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: -0.007 min
Response: 15351064
Conc: 15.95 ng/ml