

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120919\
 Data File : PL054860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2019 10:40
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:28:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.051	277.9E6	64221537	23.889	25.167
28)	SA Decachlor...	8.317	9.149	205.8E6	52253138	21.493	21.795
Target Compounds							
2)	A alpha-BHC	3.979	0.000	15171570	0	0.799	N.D. #
23)	Chlordane-1	4.448f	0.000	9458572	0	23.968	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120919\
Data File : PL054860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2019 10:40
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:28:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

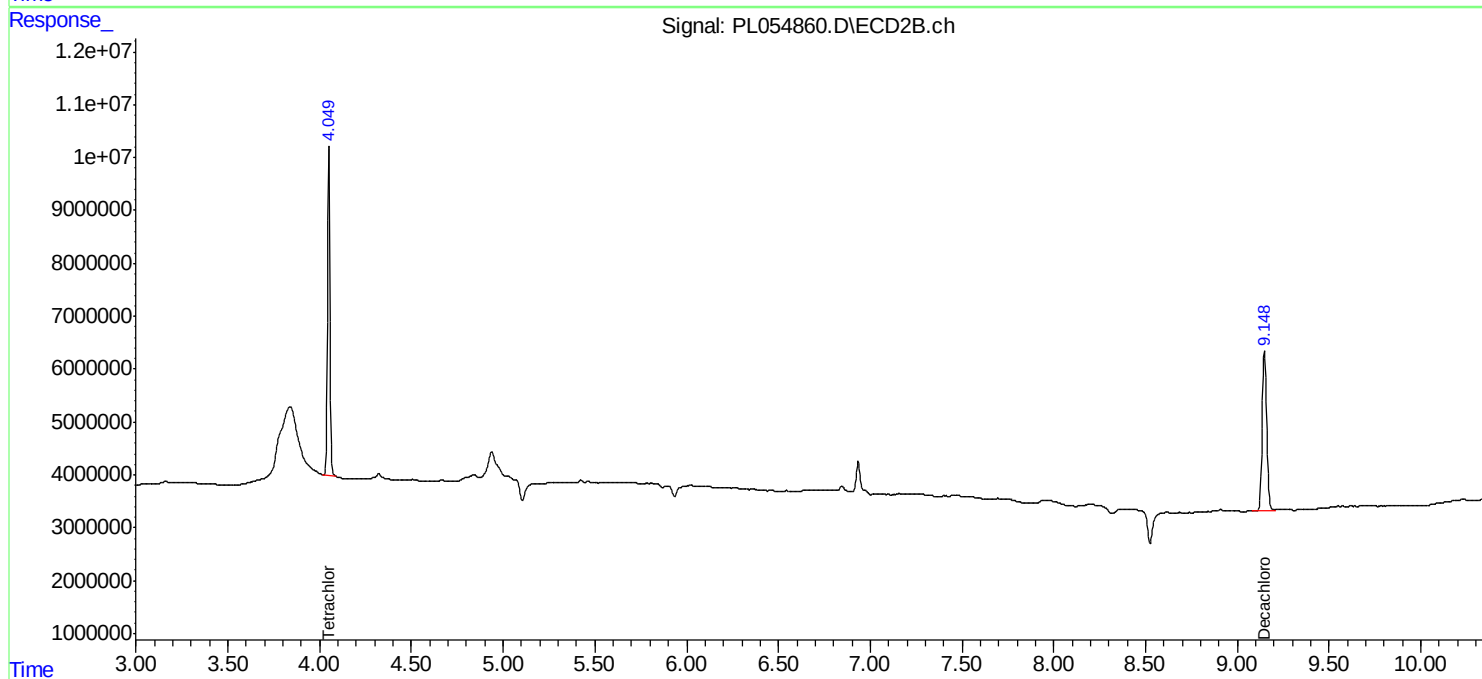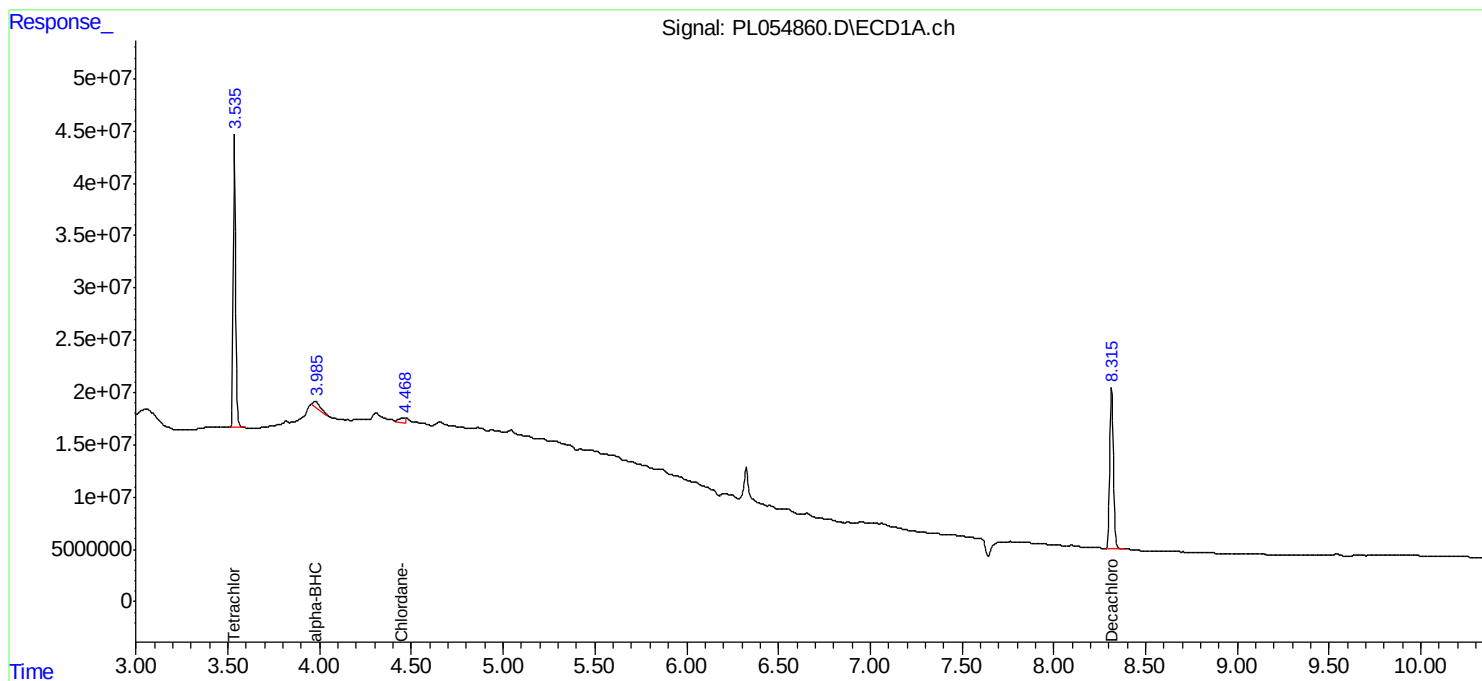


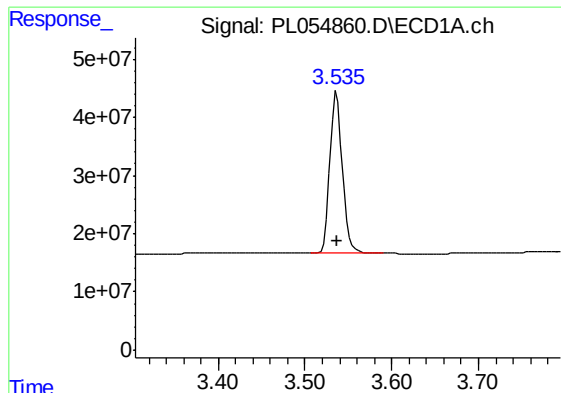

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 277923973
Conc: 23.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

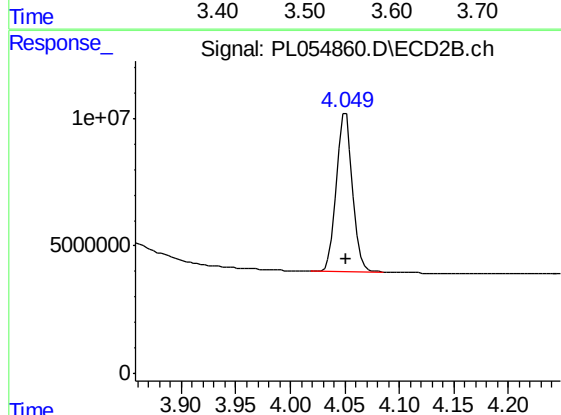


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 64221537
Conc: 25.17 ng/ml

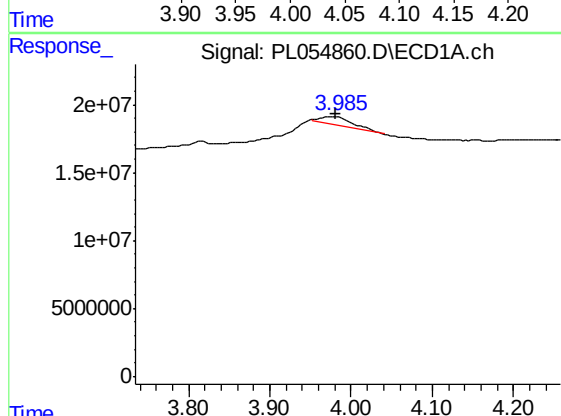


#2 alpha-BHC

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 15171570
Conc: 0.80 ng/ml

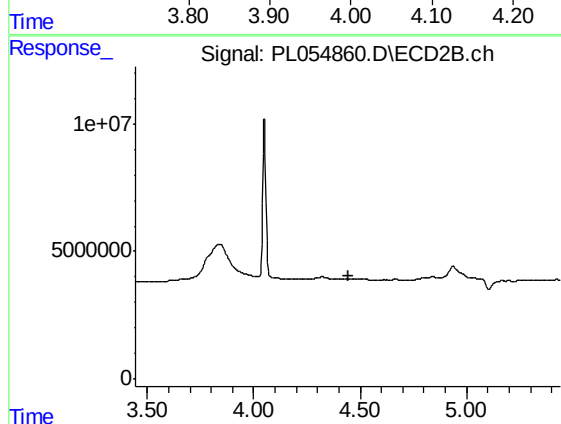

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.443 min
Response: 0
Conc: N.D.

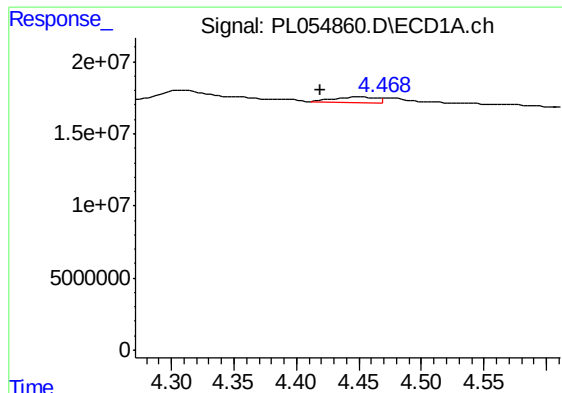

#23 Chlordane-1


R.T.: 4.448 min
Delta R.T.: 0.029 min
Response: 9458572
Conc: 23.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

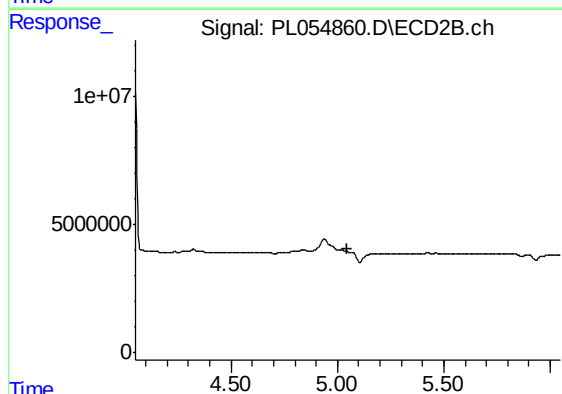


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.049 min
Response: 0
Conc: N.D.

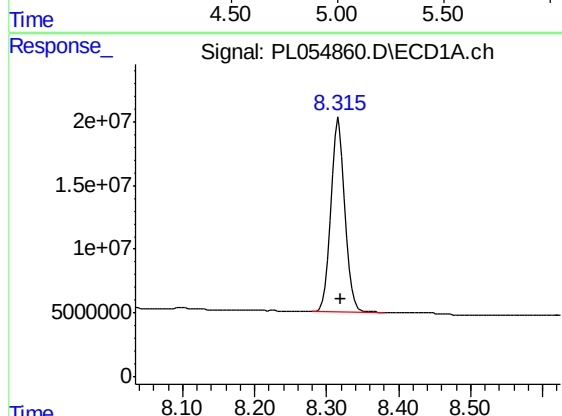

#28 Decachlorobiphenyl

R.T.: 8.317 min
Delta R.T.: -0.003 min
Response: 205819419
Conc: 21.49 ng/ml

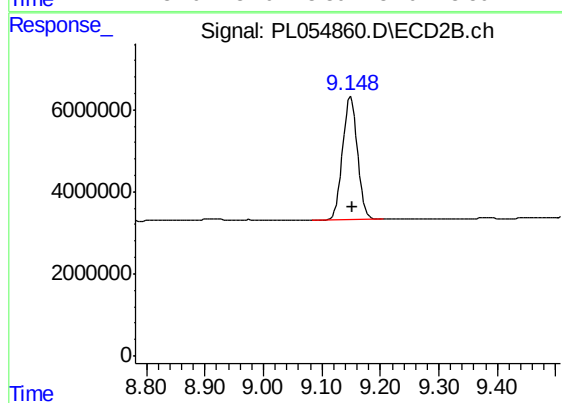

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.002 min
Response: 52253138
Conc: 21.80 ng/ml