

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
 Data File : PL063412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 10:13
 Operator : DD\AJ
 Sample : L4965-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:02:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	20883421	39047944	12.262	11.964
28)	SA Decachlor...	8.128	8.992	20538953	25523466	10.998	10.728
Target Compounds							
8)	B Heptachlo...	0.000	5.810	0	41032410	N.D.	11.779 #
11)	B alpha-Chl...	0.000	6.119	0	6540051	N.D.	1.812 #
12)	B 4,4'-DDE	0.000	6.278	0	8362930	N.D.	2.384 #
14)	MA Endrin	5.937	0.000	13244978	0	7.887	N.D. #
17)	MA 4,4'-DDT	0.000	7.068	0	7864614	N.D.	3.080 #
26)	Chlordane-4	0.000	6.119	0	6540051	N.D.	12.194 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
Data File : PL063412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 10:13
Operator : DD\AJ
Sample : L4965-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CRT014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:02:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

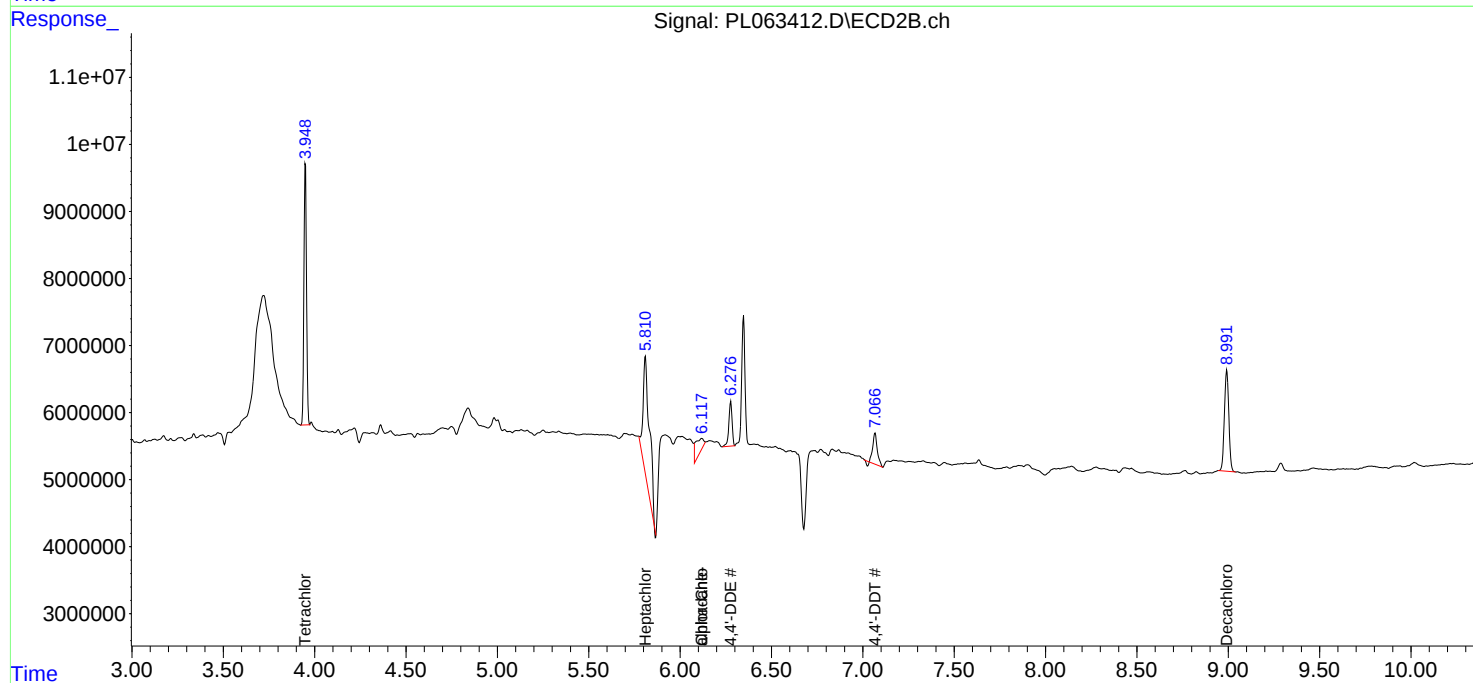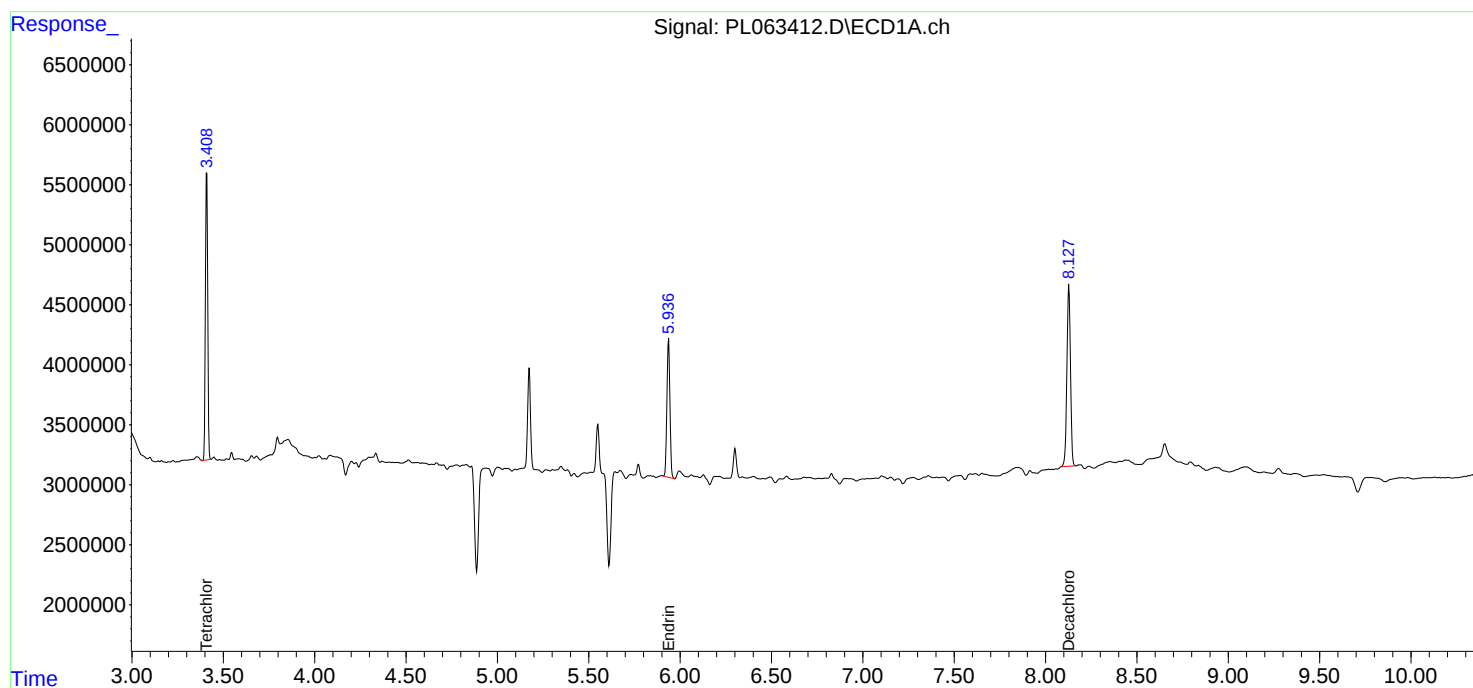


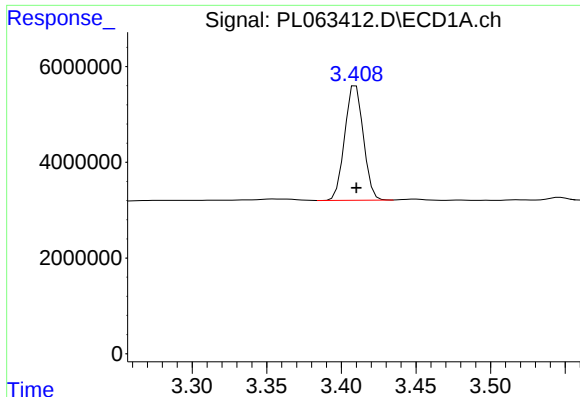

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 20883421
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT014

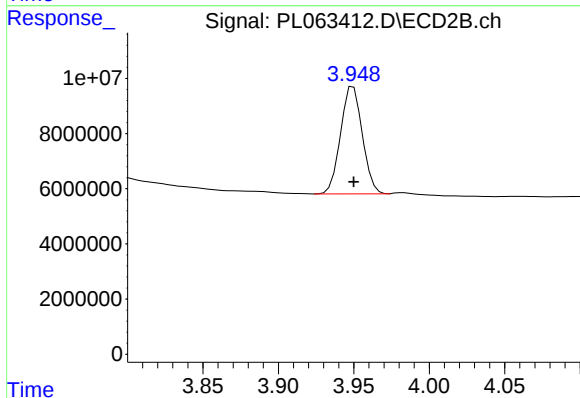


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 39047944
Conc: 11.96 ng/ml

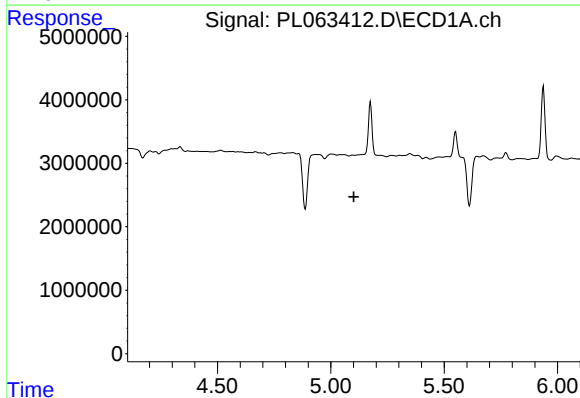


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.101 min
Response: 0
Conc: N.D.

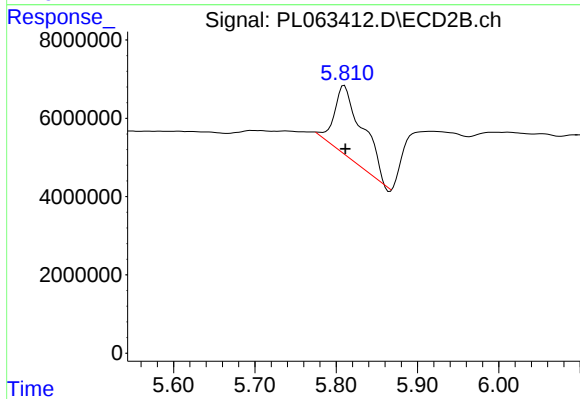

#8 Heptachlor epoxide


R.T.: 5.810 min
Delta R.T.: -0.001 min
Response: 41032410
Conc: 11.78 ng/ml

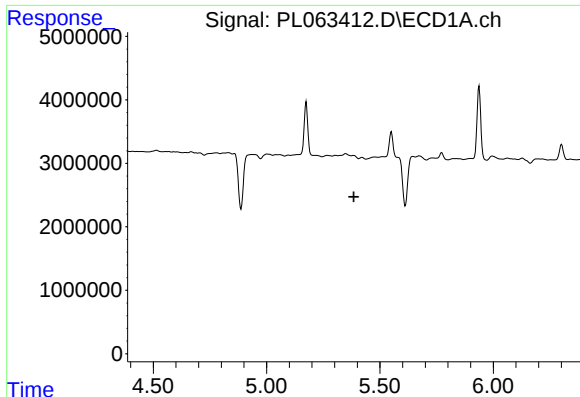

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.384 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT014

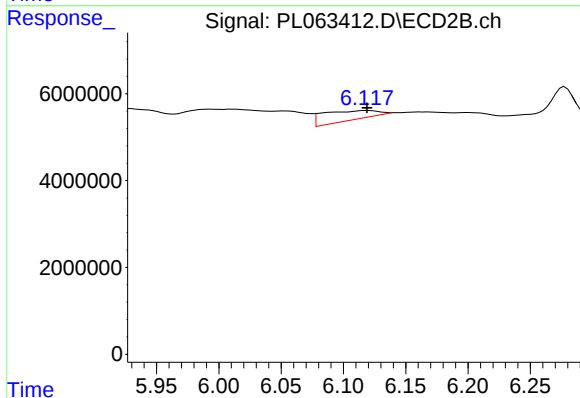


#11 alpha-Chlordane

R.T.: 6.119 min
Delta R.T.: 0.000 min
Response: 6540051
Conc: 1.81 ng/ml

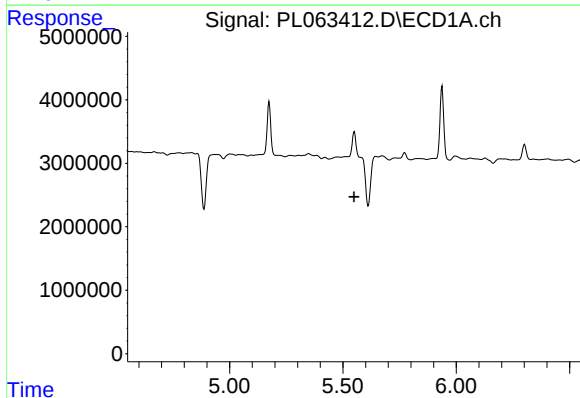


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

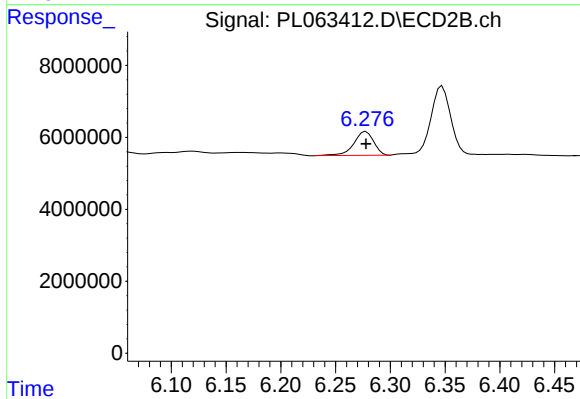

#12 4,4'-DDE


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 8362930
Conc: 2.38 ng/ml

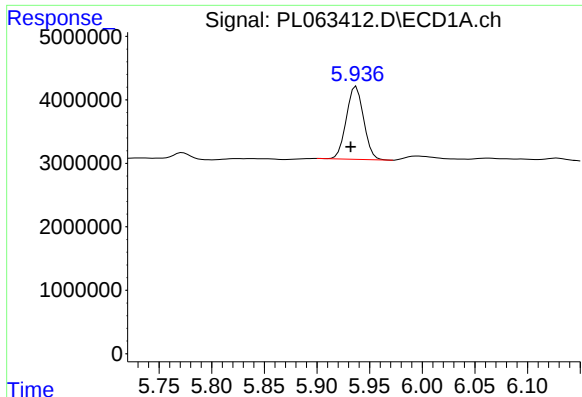

#14 Endrin


R.T.: 5.937 min
Delta R.T.: 0.005 min
Response: 13244978
Conc: 7.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT014

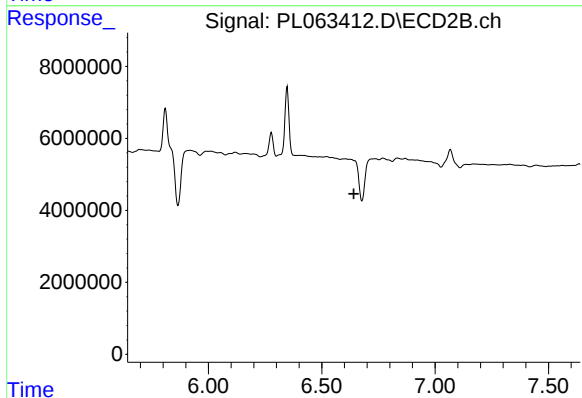


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

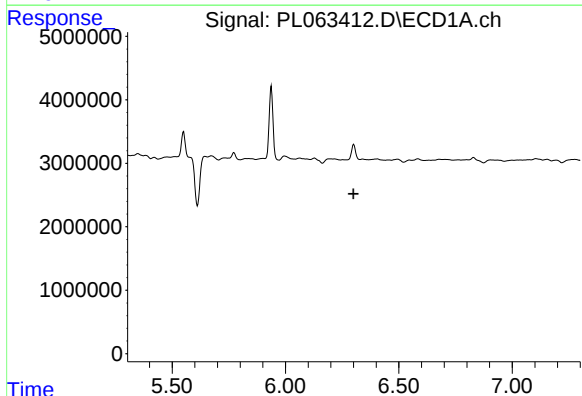


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

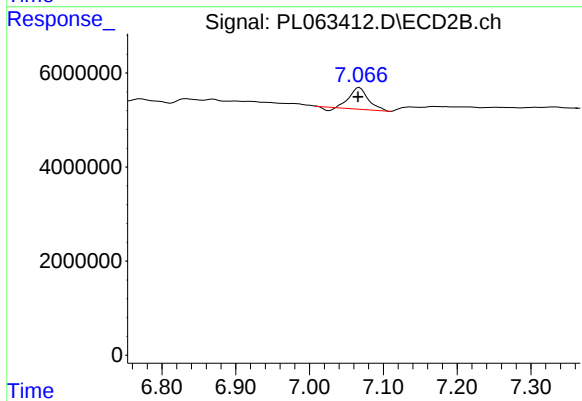

#17 4,4'-DDT


R.T.: 7.068 min
Delta R.T.: 0.002 min
Response: 7864614
Conc: 3.08 ng/ml

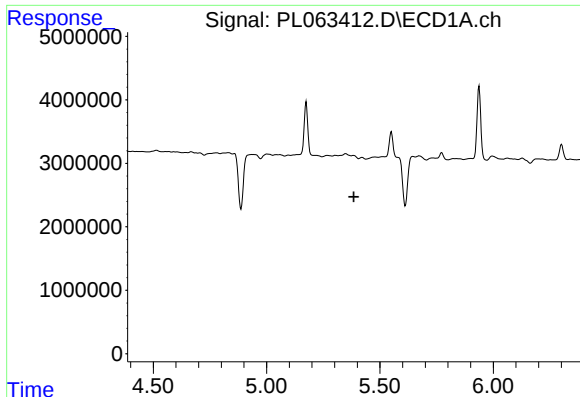

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CRT014

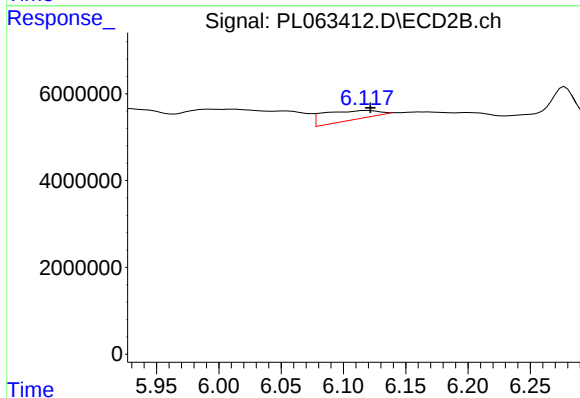


#26 Chlordane-4

R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 6540051
Conc: 12.19 ng/ml

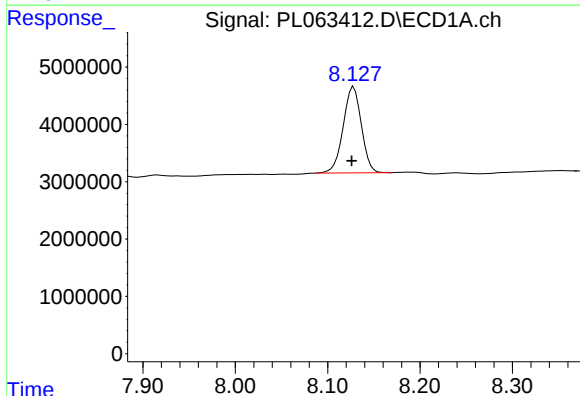

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 20538953
Conc: 11.00 ng/ml

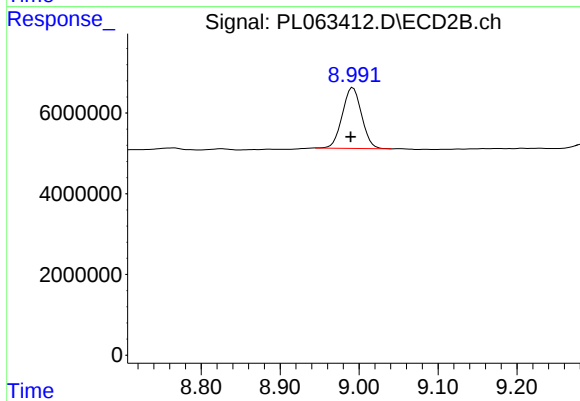

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 25523466
Conc: 10.73 ng/ml