

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
 Data File : PL063413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 10:27
 Operator : DD\AJ
 Sample : L4968-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:03:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.951	38590949	72478086	22.660	22.207
28)	SA Decachlor...	8.128	8.993	36951065	46110912	19.787	19.381
Target Compounds							
10)	B gamma-Chl...	0.000	6.032	0	9106553	N.D.	2.574 #
11)	B alpha-Chl...	0.000	6.121	0	9058145	N.D.	2.510 #
14)	MA Endrin	5.938	0.000	24896003	0	14.825	N.D. #
15)	B Endosulfa...	0.000	6.871f	0	7528653	N.D.	2.277 #
25)	Chlordane-3	0.000	6.032f	0	9106553	N.D.	20.534 #
26)	Chlordane-4	0.000	6.121	0	9058145	N.D.	16.889 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
Data File : PL063413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 10:27
Operator : DD\AJ
Sample : L4968-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:03:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

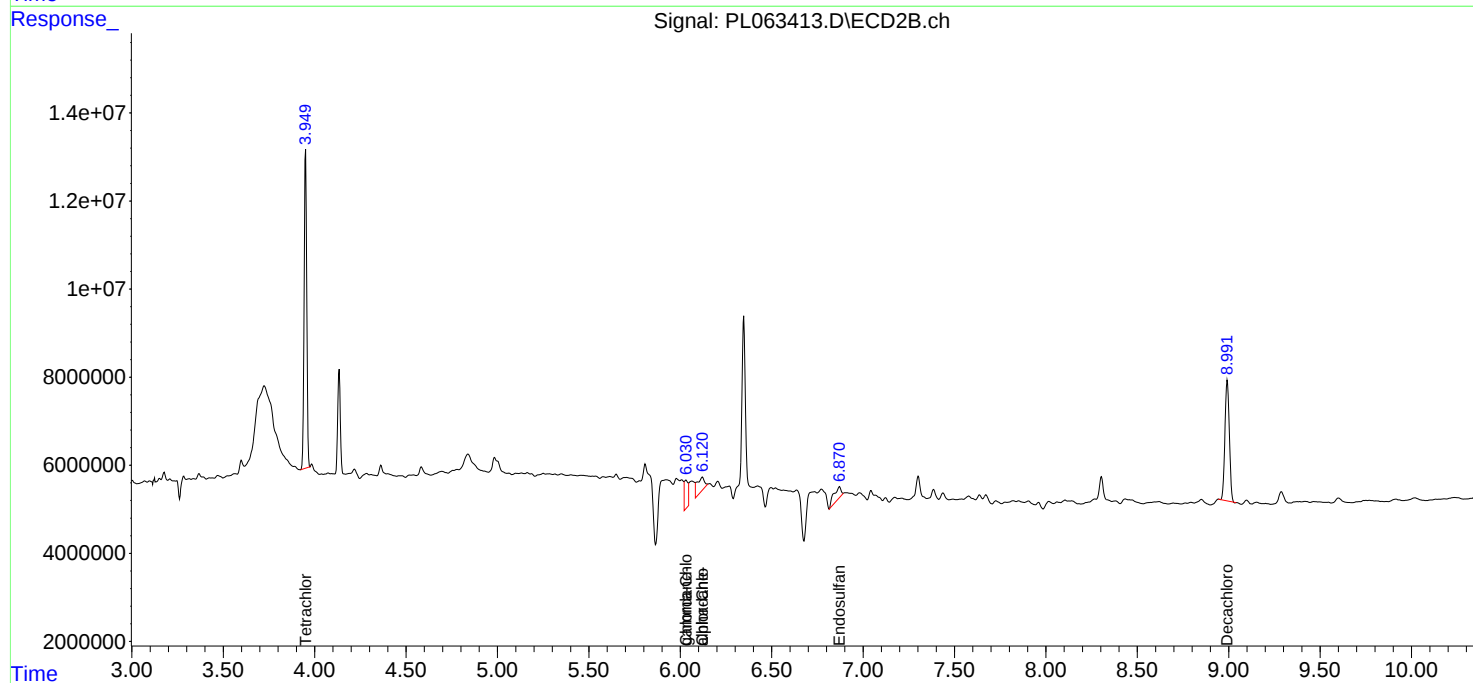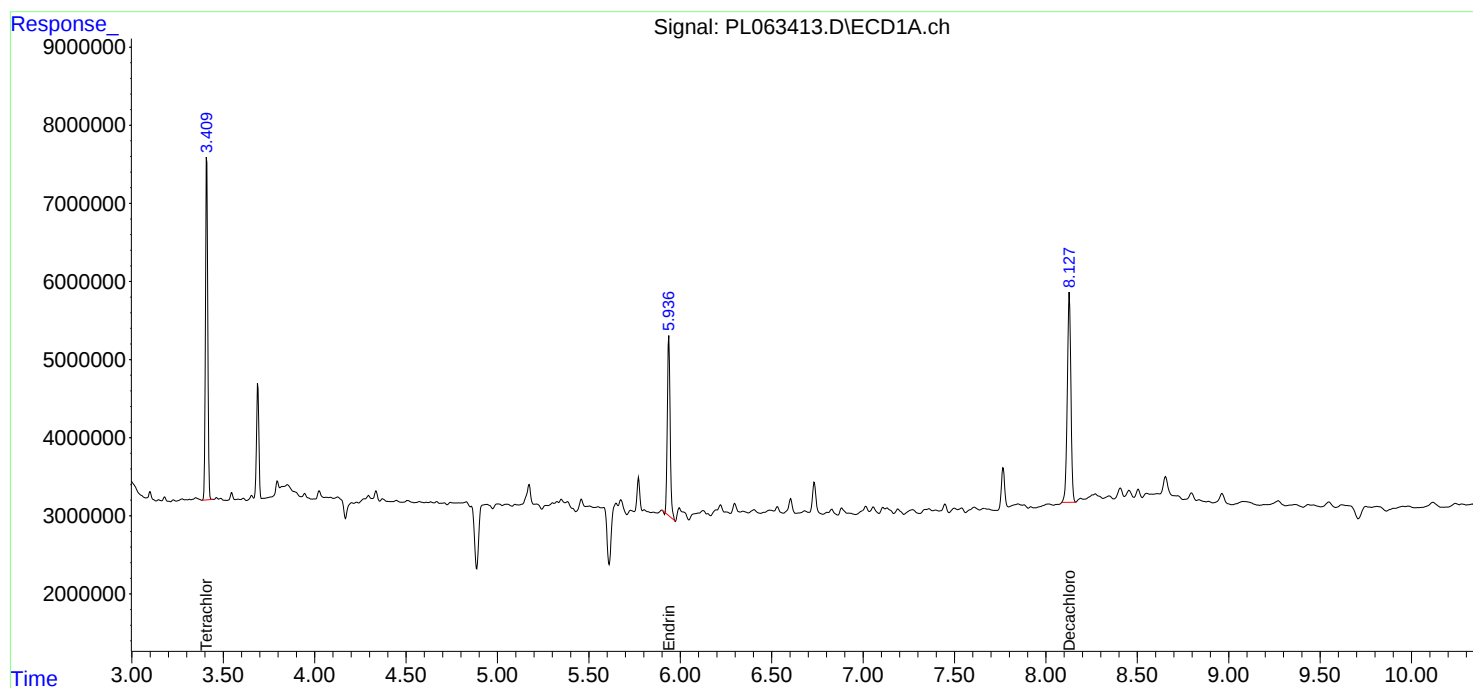


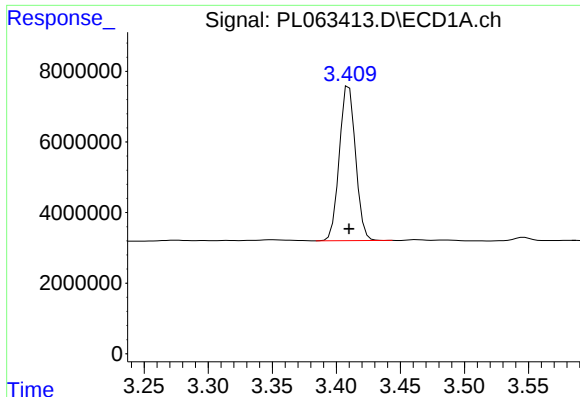

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 38590949
Conc: 22.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

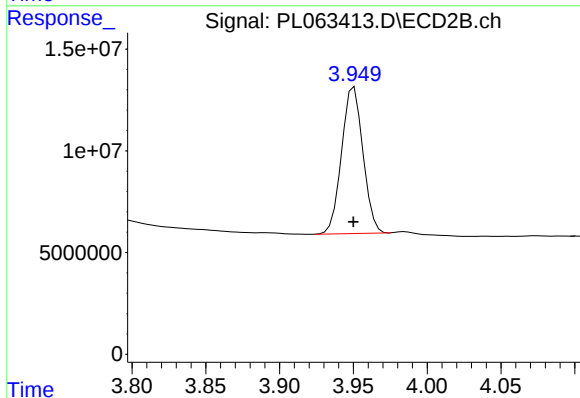


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 72478086
Conc: 22.21 ng/ml

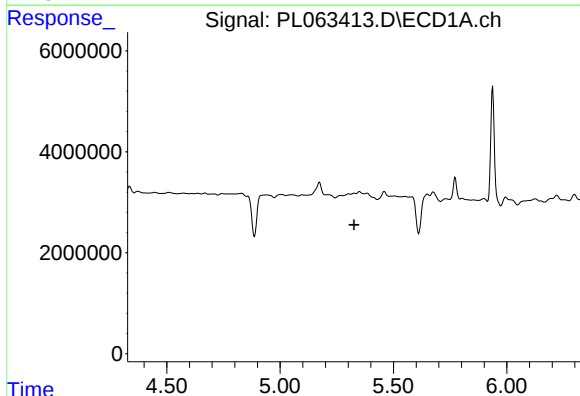


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.327 min
Response: 0
Conc: N.D.

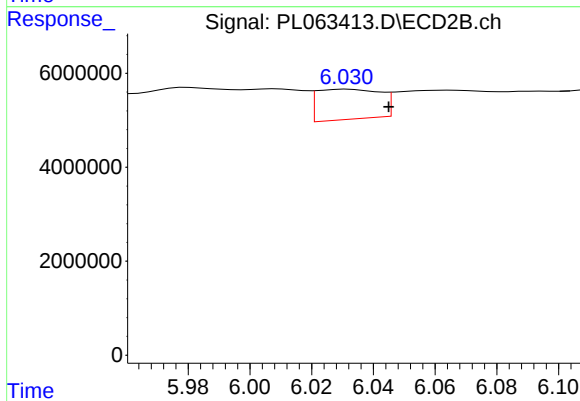

#10 gamma-Chlordane


R.T.: 6.032 min
Delta R.T.: -0.013 min
Response: 9106553
Conc: 2.57 ng/ml

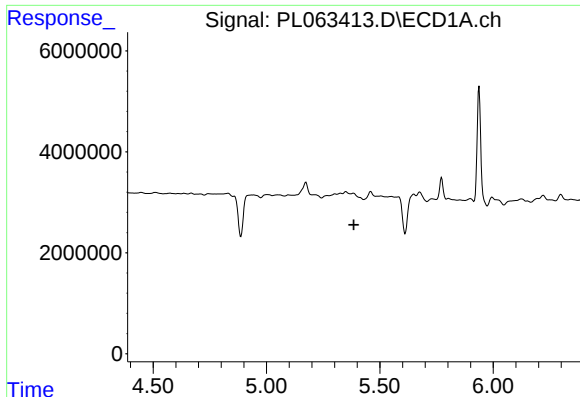

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.384 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

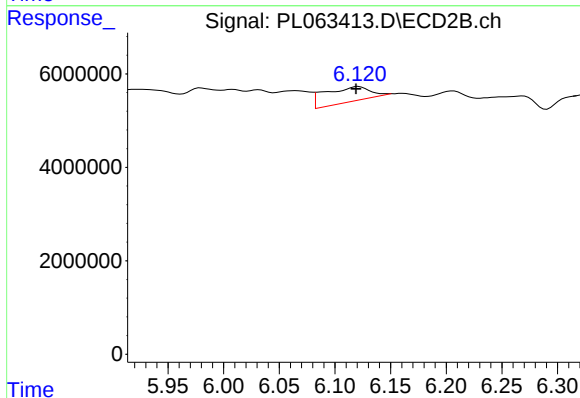


#11 alpha-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.002 min
Response: 9058145
Conc: 2.51 ng/ml

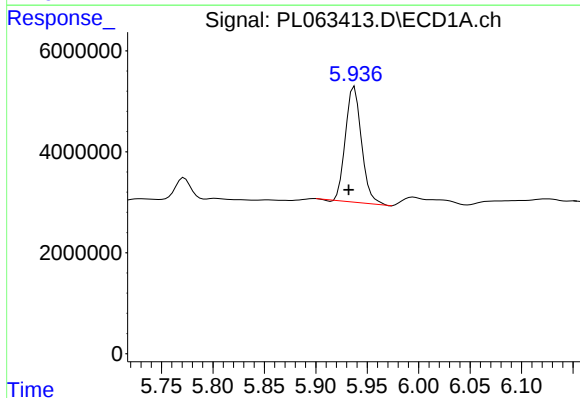


#14 Endrin

R.T.: 5.938 min
Delta R.T.: 0.005 min
Response: 24896003
Conc: 14.82 ng/ml

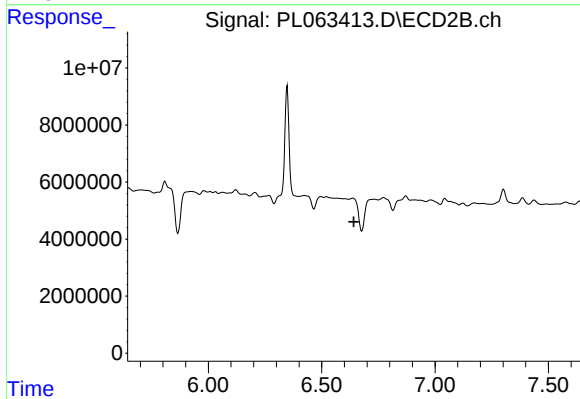

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

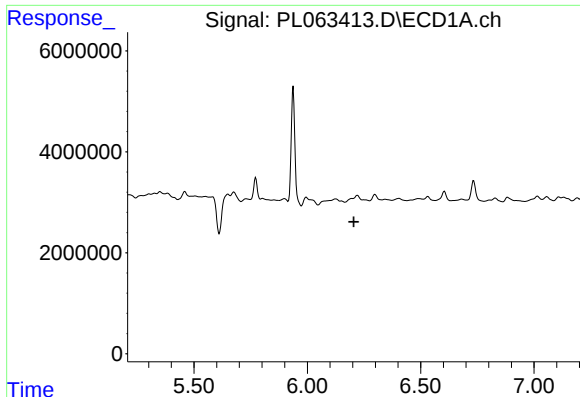

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

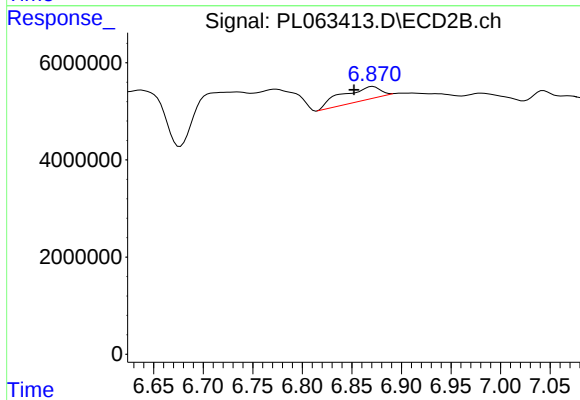


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.019 min
Response: 7528653
Conc: 2.28 ng/ml

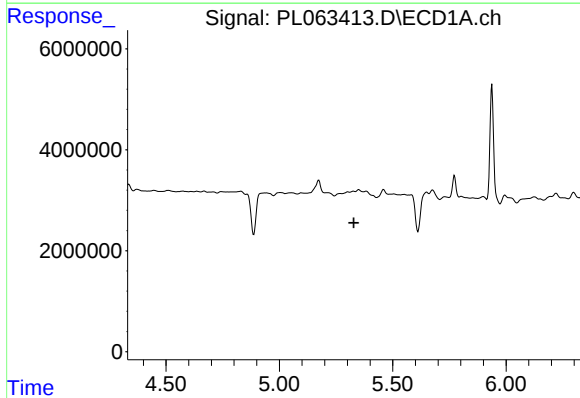


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

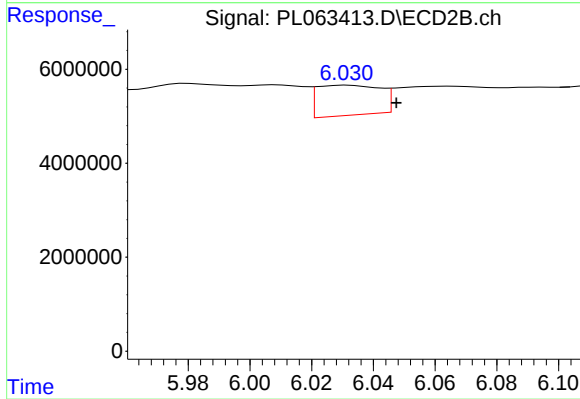

#25 Chlordane-3


R.T.: 6.032 min
Delta R.T.: -0.016 min
Response: 9106553
Conc: 20.53 ng/ml

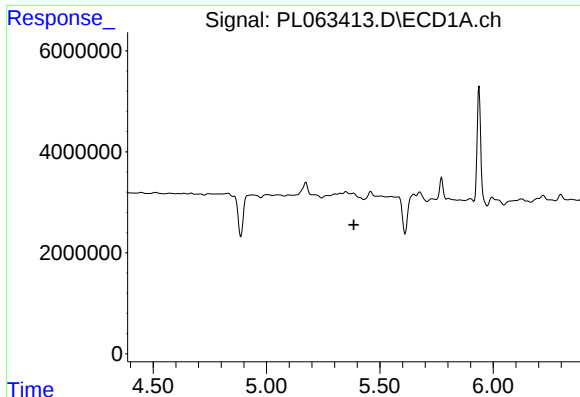

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

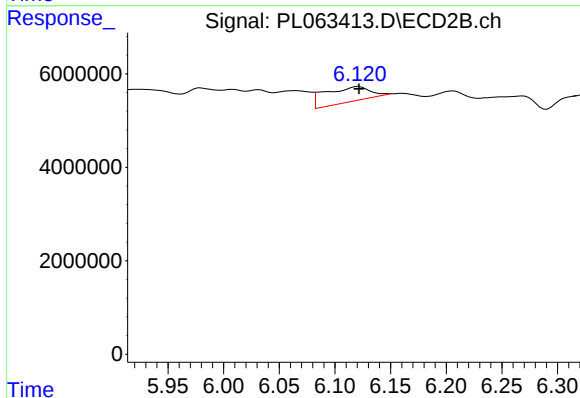


#26 Chlordane-4

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 9058145
Conc: 16.89 ng/ml

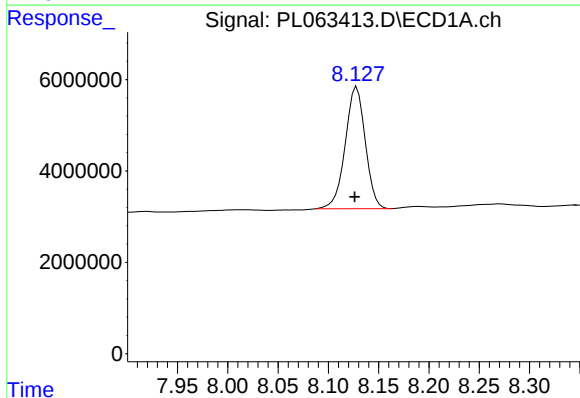

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 36951065
Conc: 19.79 ng/ml

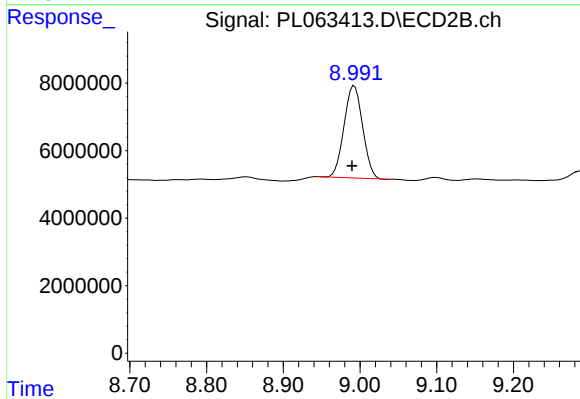

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.003 min
Response: 46110912
Conc: 19.38 ng/ml