

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
 Data File : PL063411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 09:59
 Operator : DD\AJ
 Sample : L4965-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT012

Manual Integrations
 APPROVED

Ankita
 12/10/2020 1:40:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:02:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	23787277	44756926	13.967	13.713
28)	SA Decachlor...	8.129	8.993	23356151	29941545	12.507	12.585
Target Compounds							
17)	MA 4,4'-DDT	6.299	7.067	1724338	4378429	1.282m	1.715m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
Data File : PL063411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 09:59
Operator : DD\AJ
Sample : L4965-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT012


Manual Integrations
APPROVED

Ankita
12/10/2020 1:40:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:02:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

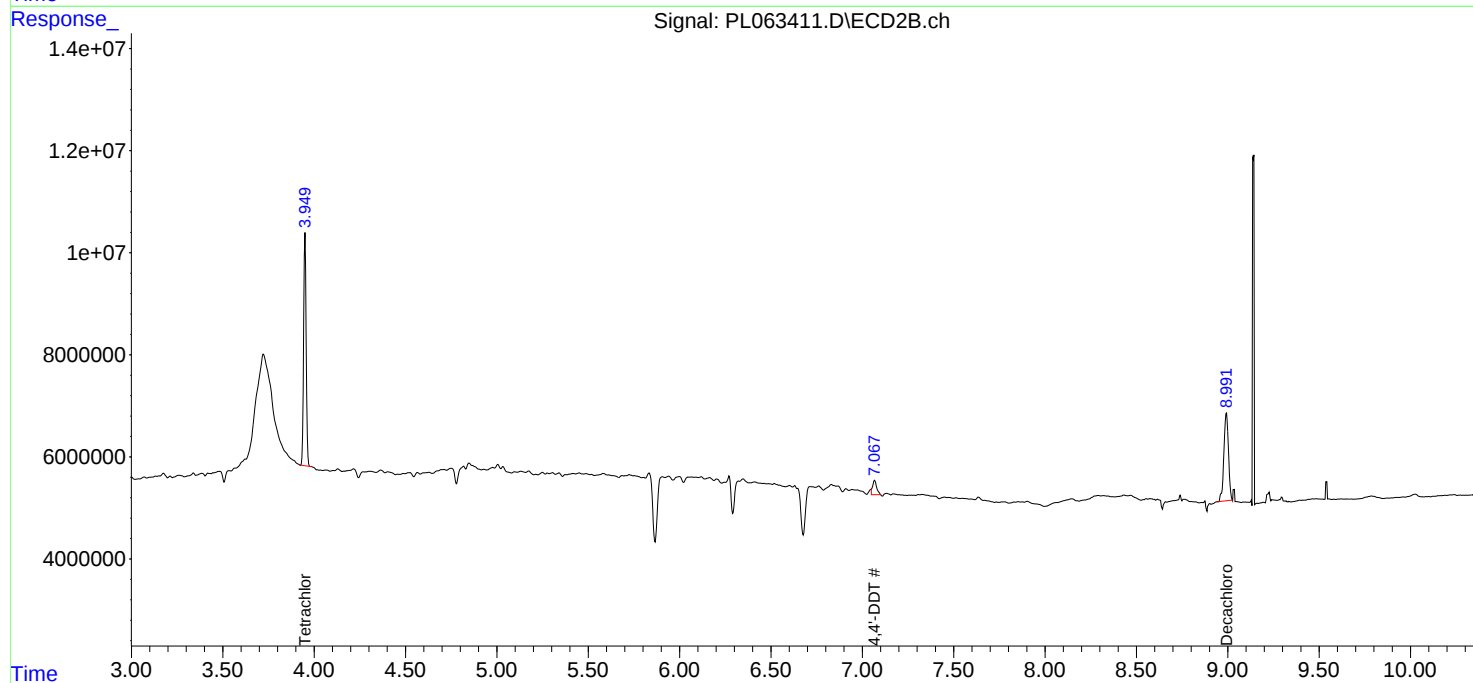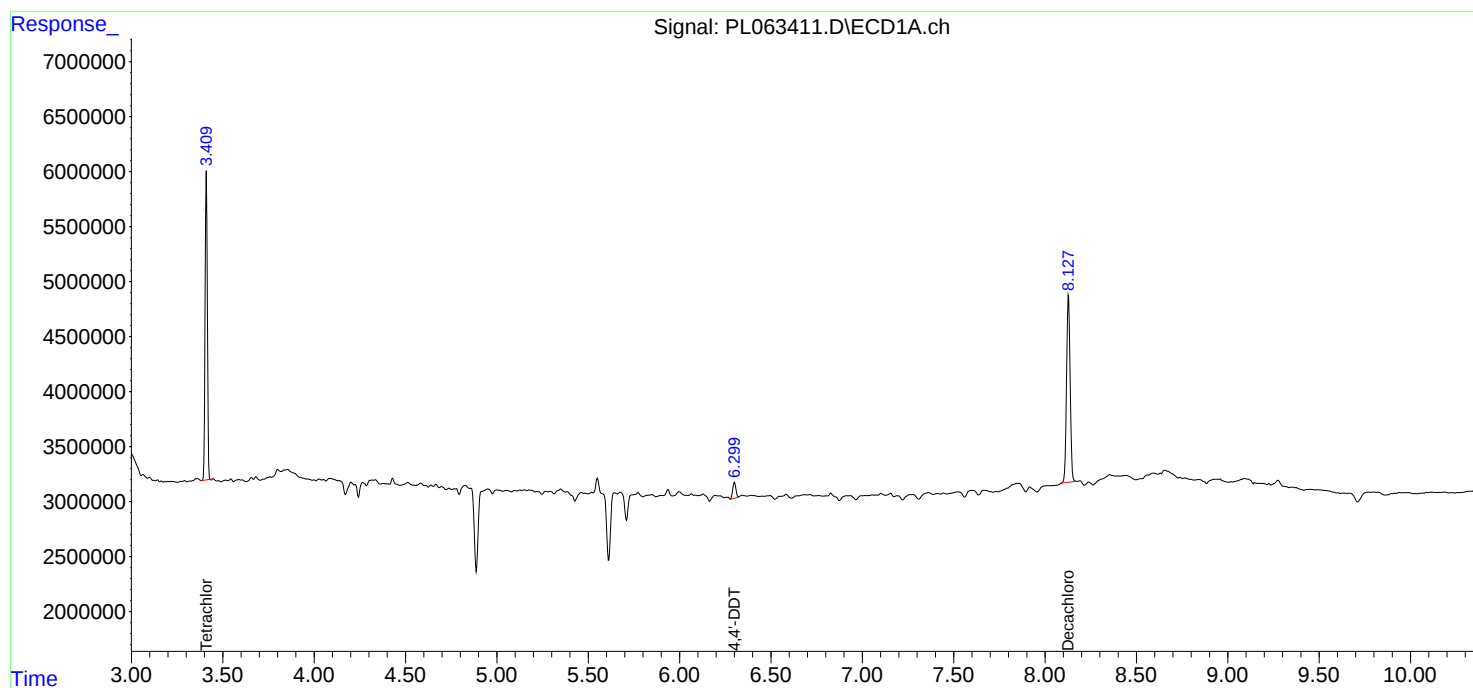

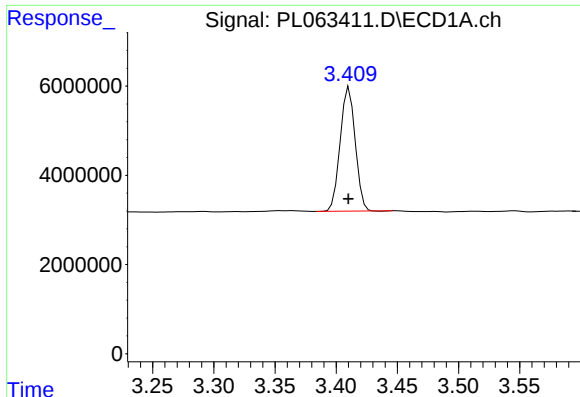


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 23787277
Conc: 13.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT012


Manual Integrations
APPROVED

Ankita
12/10/2020 1:40:42 PM

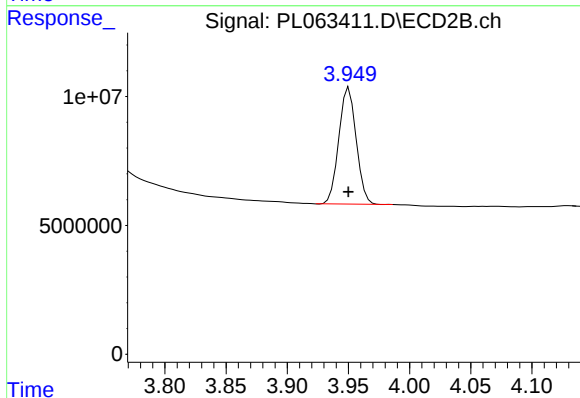


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 44756926
Conc: 13.71 ng/ml

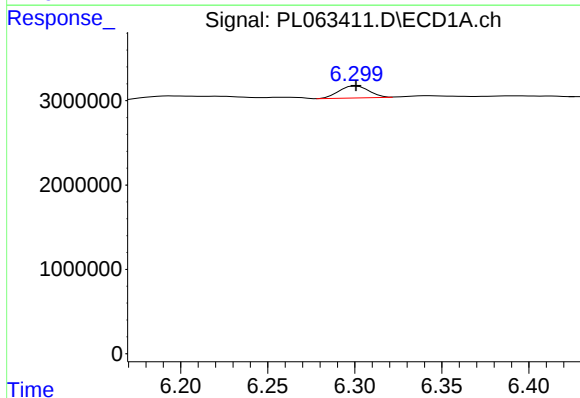


#17 4,4'-DDT

R.T.: 6.299 min
Delta R.T.: -0.001 min
Response: 1724338
Conc: 1.28 ng/ml m

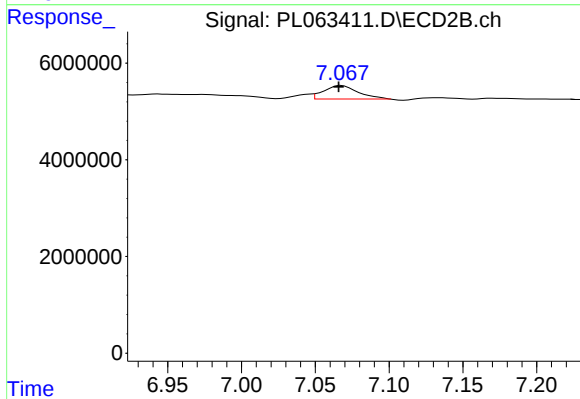

#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 4378429
Conc: 1.71 ng/ml m

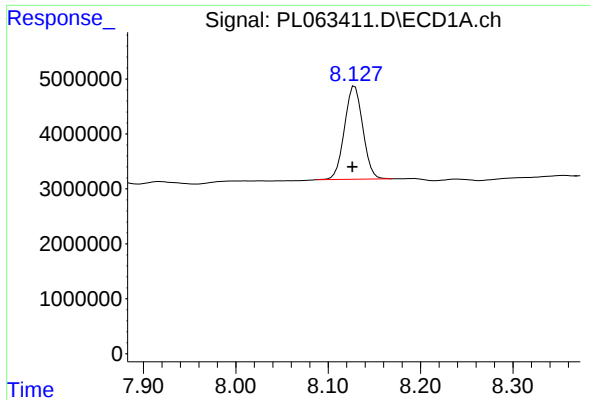


#28 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.003 min
Response: 23356151
Conc: 12.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT012

Manual Integrations
APPROVED

Ankita
12/10/2020 1:40:42 PM

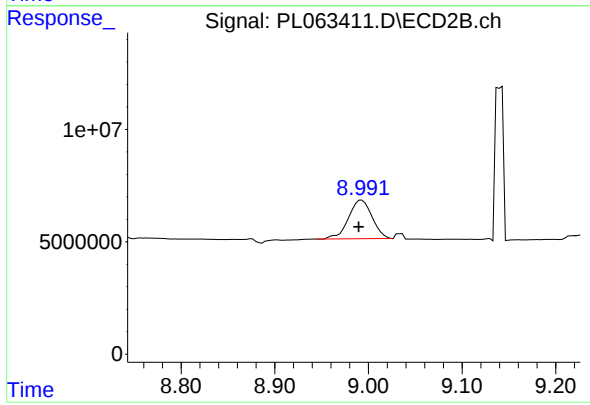

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.003 min
Response: 29941545
Conc: 12.58 ng/ml