

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
 Data File : PL063412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 10:13
 Operator : DD\AJ
 Sample : L4965-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT014

Manual Integrations
 APPROVED

Ankita
 12/10/2020 1:40:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 08:05:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	20883421	39047944	12.262	11.964
28)	SA Decachlor...	8.128	8.992	20538953	25523466	10.998	10.728
Target Compounds							
12)	B 4,4'-DDE	5.549	6.278	4629580	8362930	2.794m	2.384
17)	MA 4,4'-DDT	6.300	7.066	2914530	9833670	2.167m	3.851m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120920\
Data File : PL063412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 10:13
Operator : DD\AJ
Sample : L4965-11
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT014


Manual Integrations
APPROVED

Ankita
12/10/2020 1:40:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 08:05:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

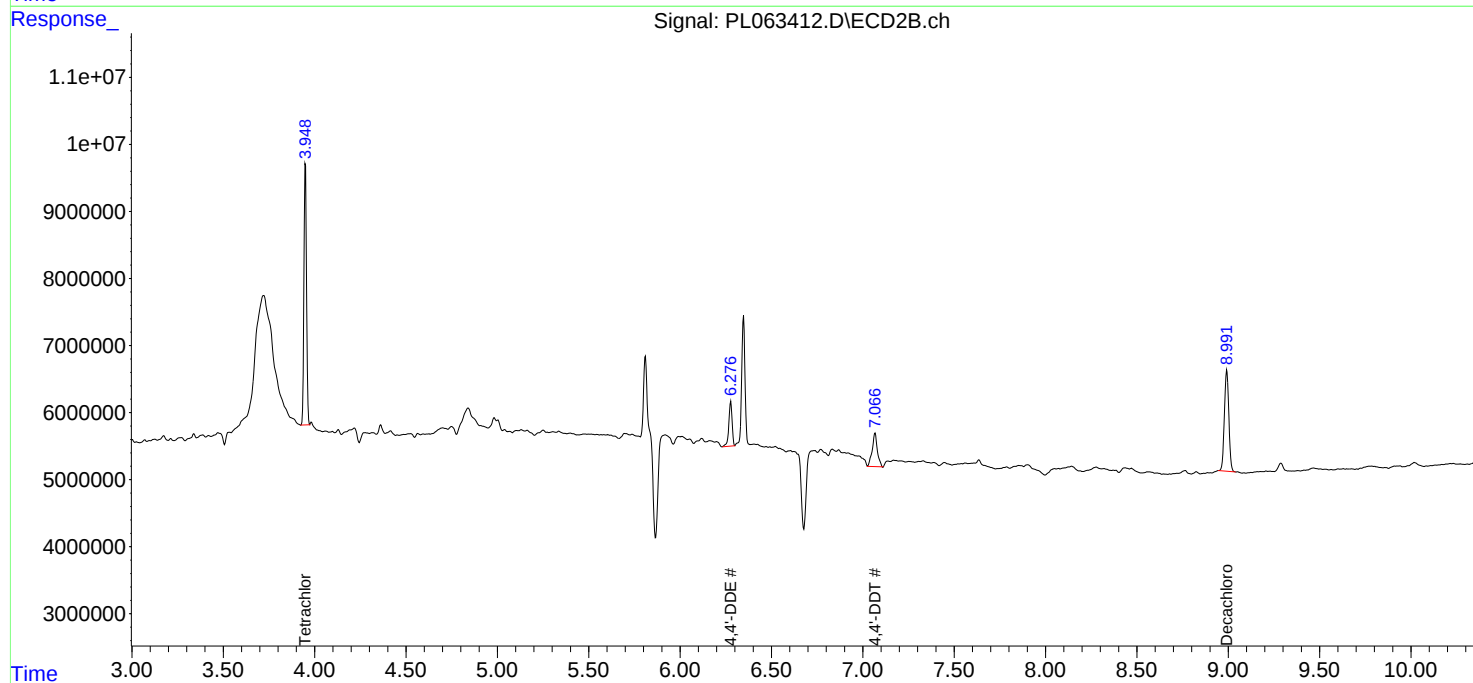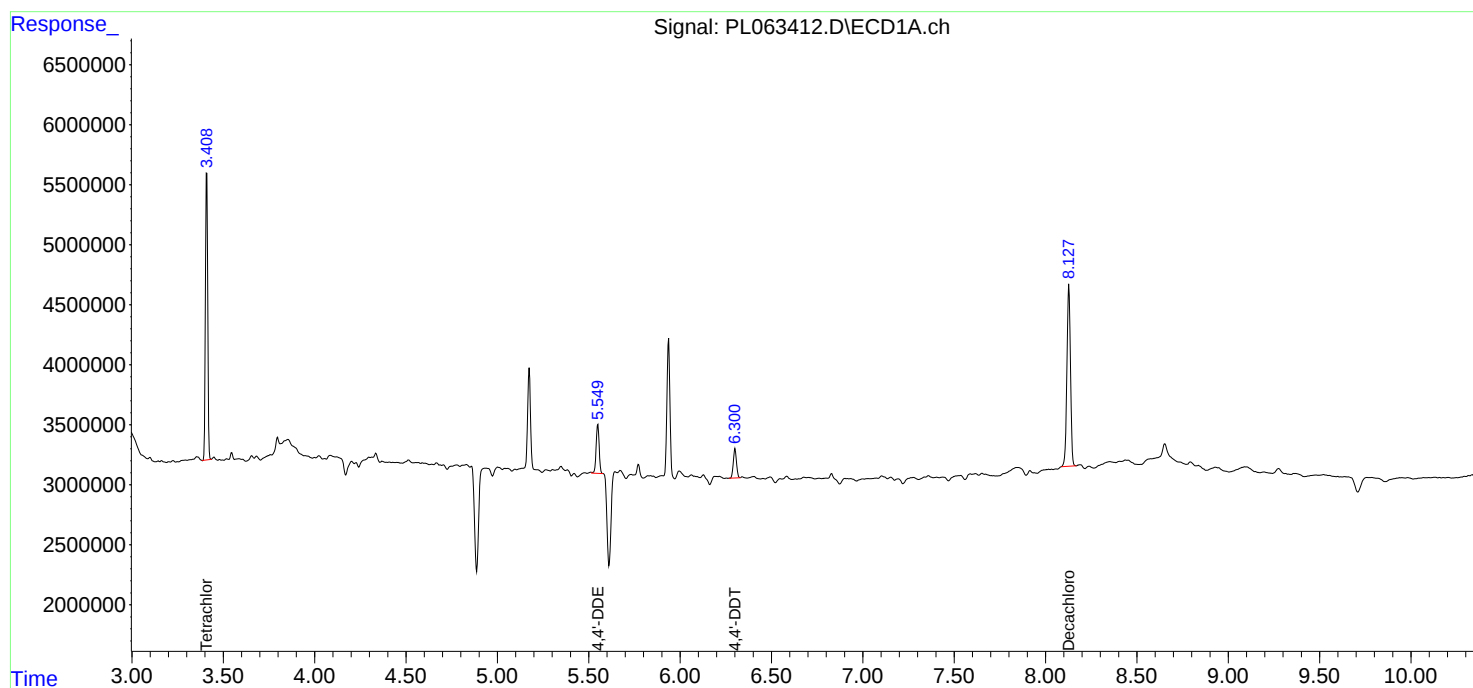

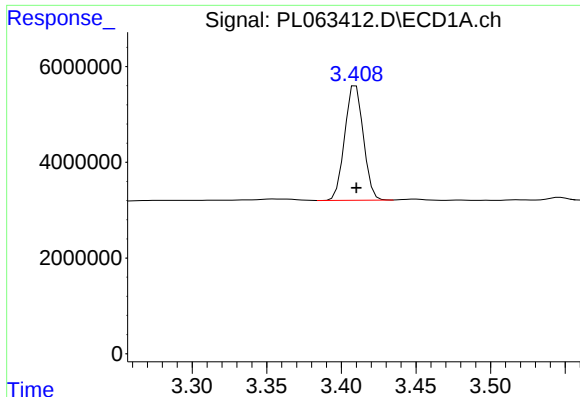


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 20883421
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT014


Manual Integrations
APPROVED

Ankita
12/10/2020 1:40:43 PM

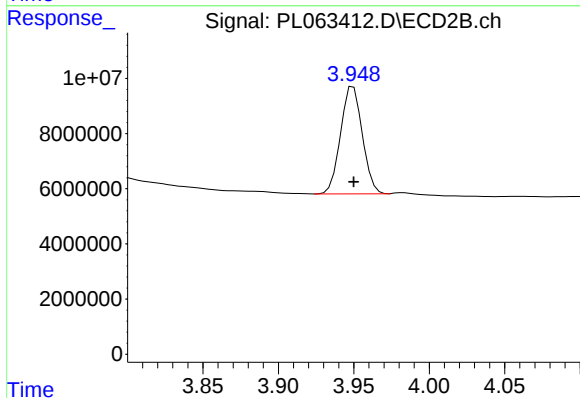


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 39047944
Conc: 11.96 ng/ml

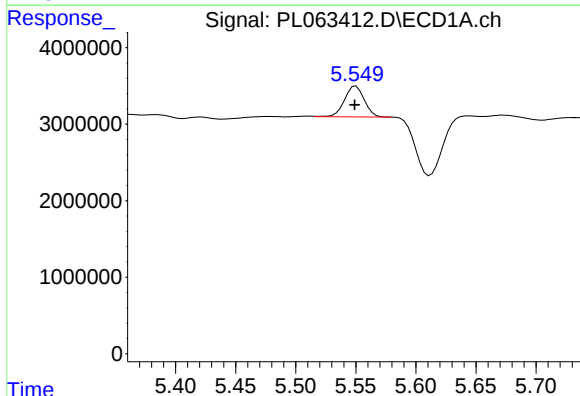


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: 0.000 min
Response: 4629580
Conc: 2.79 ng/ml m

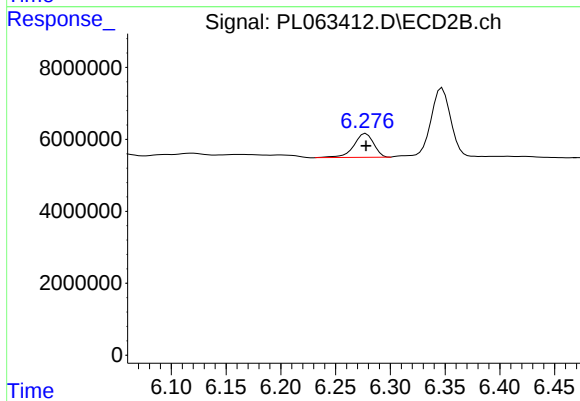

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 8362930
Conc: 2.38 ng/ml

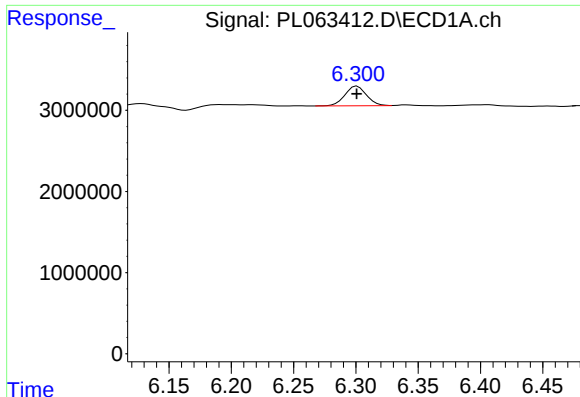


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 2914530
Conc: 2.17 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CRT014


Manual Integrations
APPROVED

Ankita
12/10/2020 1:40:43 PM

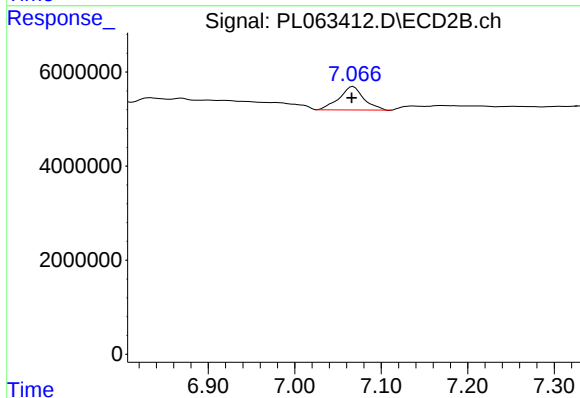


#17 4,4'-DDT

R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 9833670
Conc: 3.85 ng/ml m

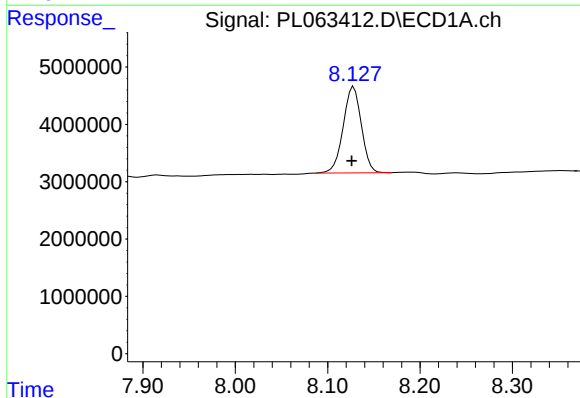

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 20538953
Conc: 11.00 ng/ml

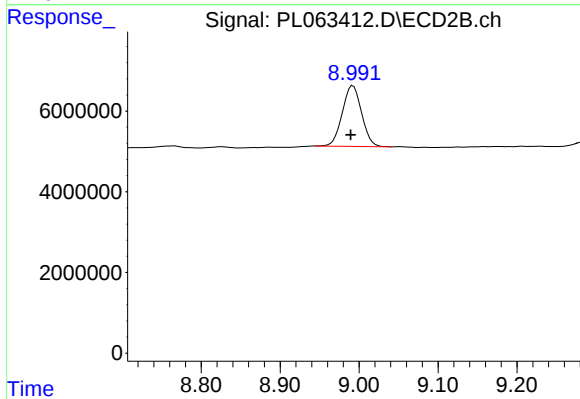

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 25523466
Conc: 10.73 ng/ml