

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
 Data File : PL071350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2021 10:49
 Operator : AR\AJ
 Sample : M4953-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 12:12:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.568	5.502	9879632	25975370	21.034	20.699
28)	SA Decachlor...	10.330	11.396	3417511	5778895	4.720	4.157
Target Compounds							
9)	A Endosulfan I	7.411	0.000	418052	0	0.703	N.D. #
11)	B alpha-Chl...	7.361	0.000	382045	0	0.597	N.D. #
20)	A Methoxychlor	9.018	0.000	103748	0	0.287	N.D. #
26)	Chlordane-4	7.361	0.000	382045	0	5.760	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
Data File : PL071350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2021 10:49
Operator : AR\AJ
Sample : M4953-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 12:12:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

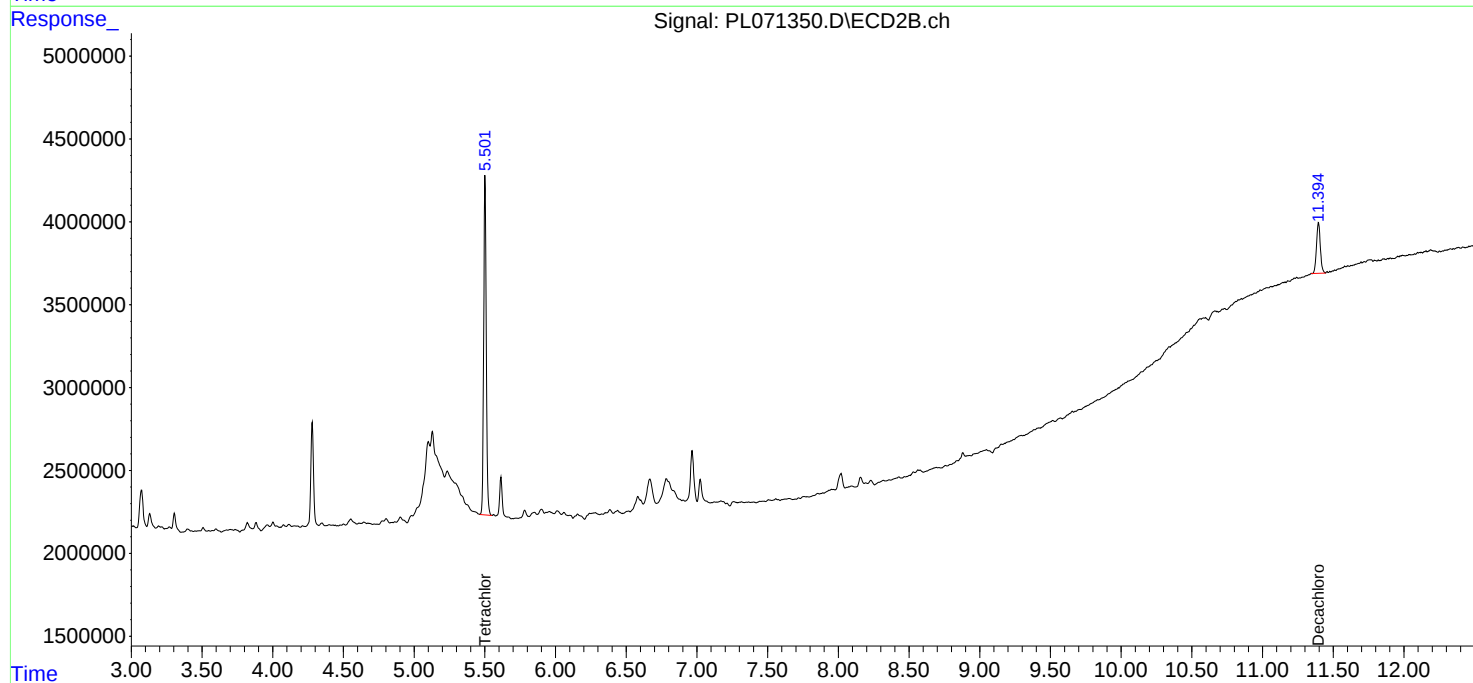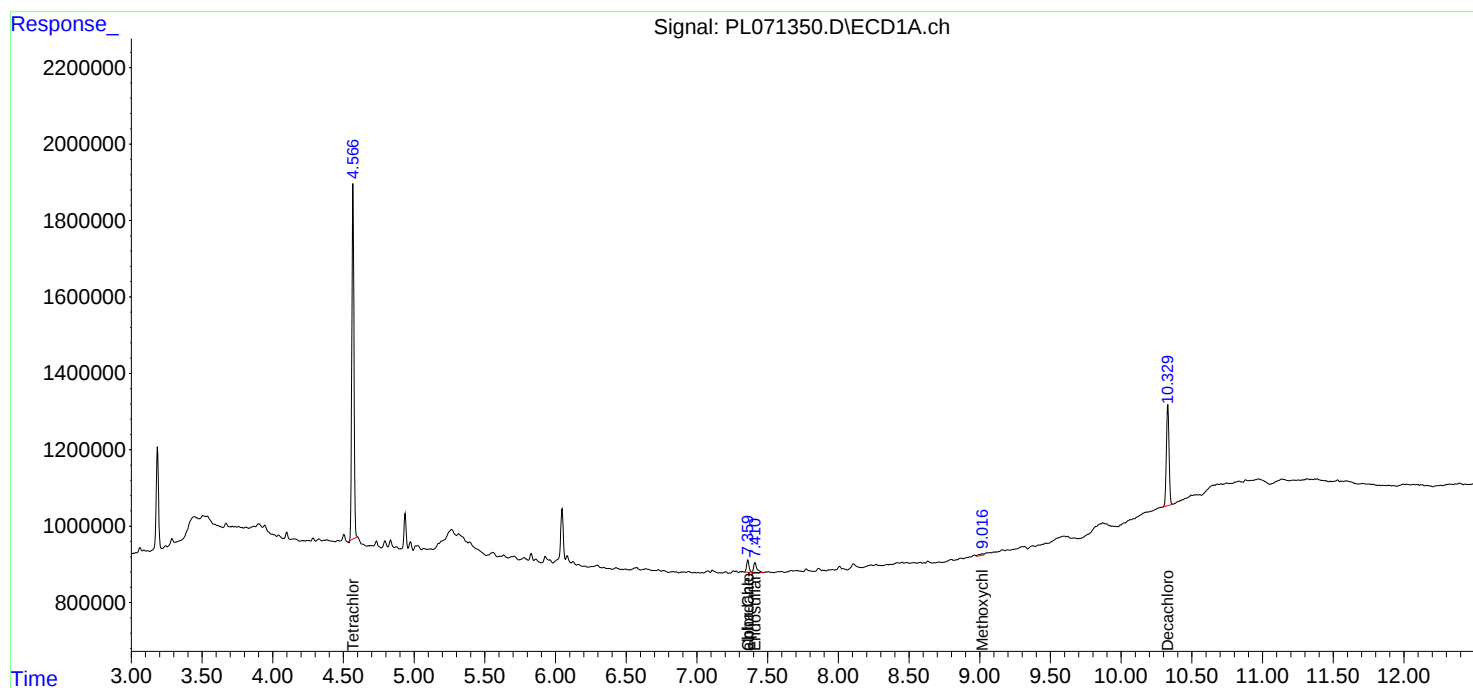


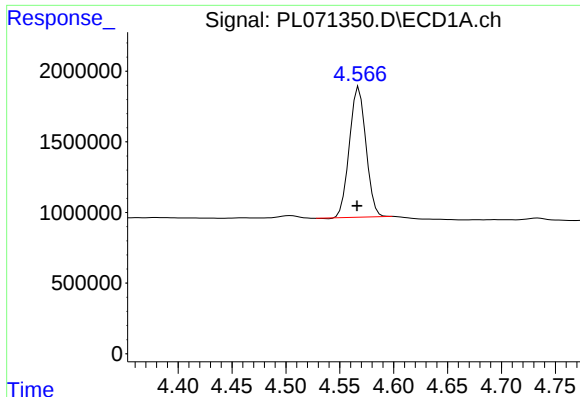

#1 Tetrachloro-m-xylene


R.T.: 4.568 min
Delta R.T.: 0.002 min
Response: 9879632
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

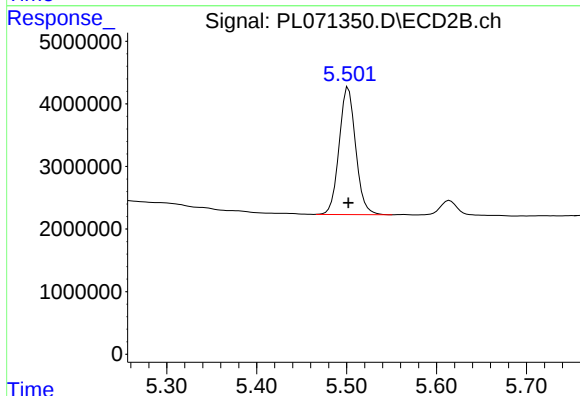


#1 Tetrachloro-m-xylene

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 25975370
Conc: 20.70 ng/ml

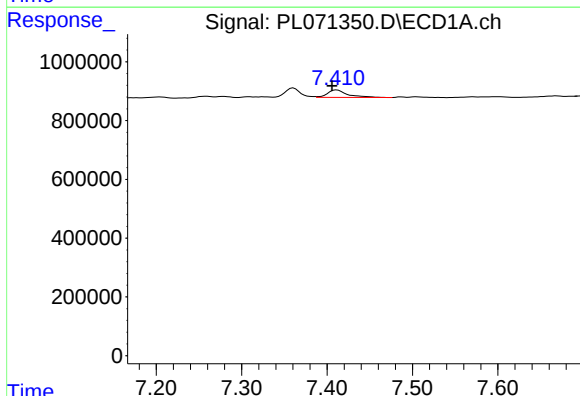


#9 Endosulfan I

R.T.: 7.411 min
Delta R.T.: 0.006 min
Response: 418052
Conc: 0.70 ng/ml

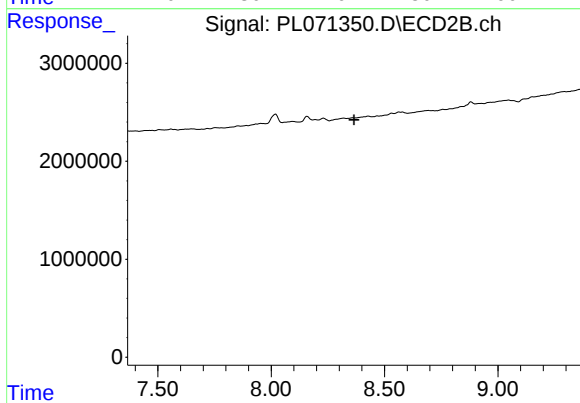

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.366 min
Response: 0
Conc: N.D.

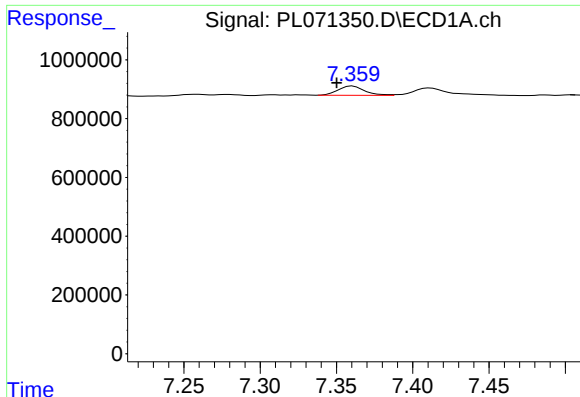

#11 alpha-Chlordane


R.T.: 7.361 min
Delta R.T.: 0.011 min
Response: 382045
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

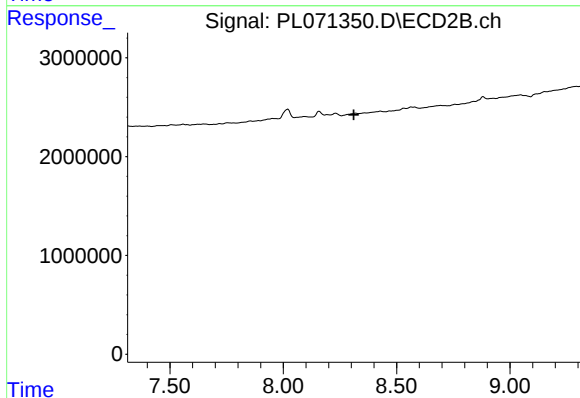


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

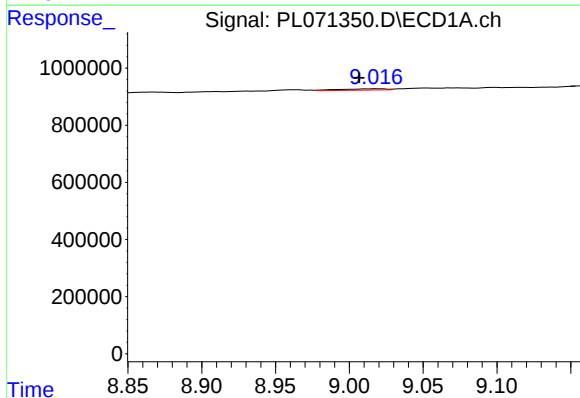


#20 Methoxychlor

R.T.: 9.018 min
Delta R.T.: 0.011 min
Response: 103748
Conc: 0.29 ng/ml

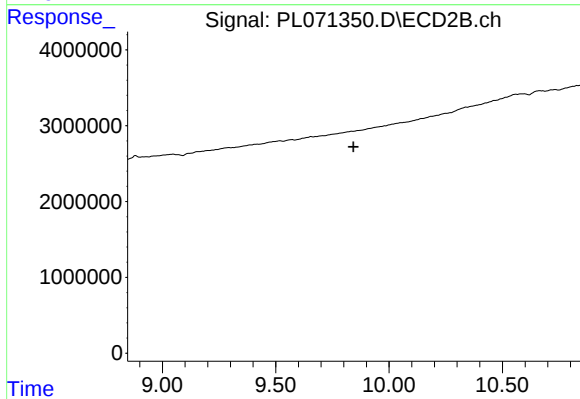

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

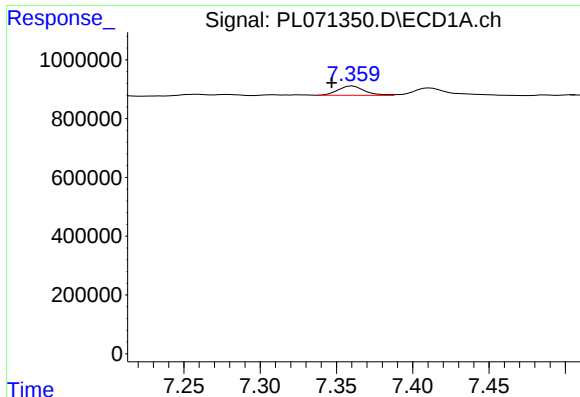

#26 Chlordane-4


R.T.: 7.361 min
Delta R.T.: 0.014 min
Response: 382045
Conc: 5.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

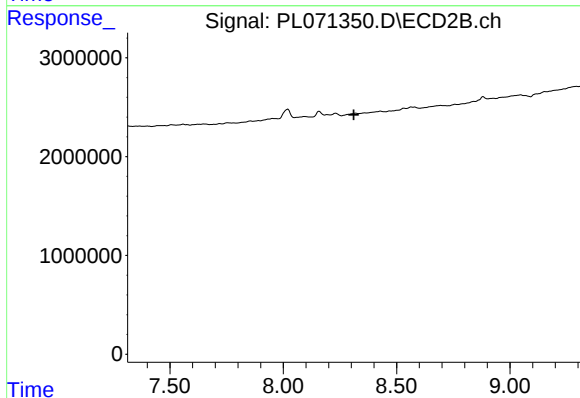


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

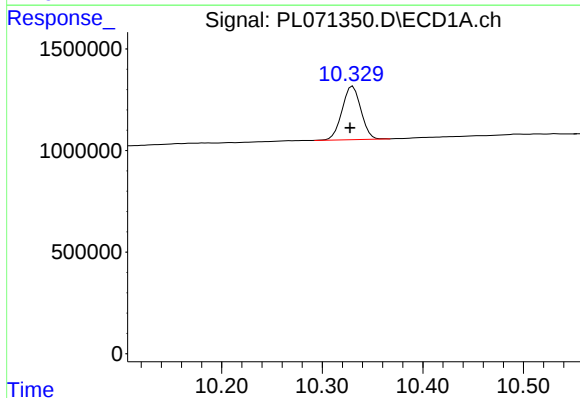

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.003 min
Response: 3417511
Conc: 4.72 ng/ml

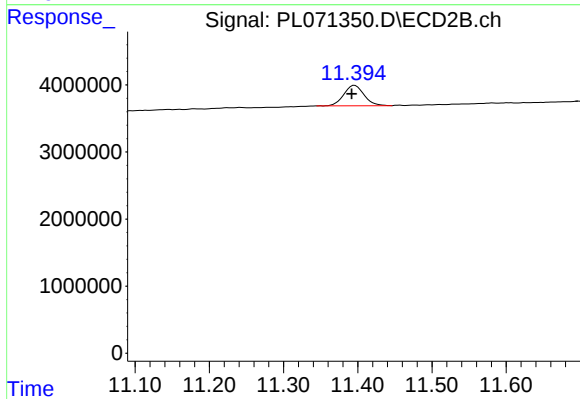

#28 Decachlorobiphenyl

R.T.: 11.396 min
Delta R.T.: 0.004 min
Response: 5778895
Conc: 4.16 ng/ml