

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
 Data File : PL071351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2021 11:06
 Operator : AR\AJ
 Sample : M4953-03RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 12:12:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.502	9697404	24538459	20.646	19.554
28)	SA Decachlor...	10.328	11.394	2266091	3514140	3.130	2.528
Target Compounds							
4)	MA Heptachlor	6.122f	0.000	435781	0	0.629	N.D. #
11)	B alpha-Chl...	7.359	0.000	214131	0	0.335	N.D. #
13)	MA Dieldrin	0.000	8.680f	0	1604323	N.D.	1.033 #
21)	B Endrin ke...	9.246	0.000	23684	0	0.033	N.D. #
26)	Chlordane-4	7.359	0.000	214131	0	3.228	N.D. #
27)	Chlordane-5	0.000	9.192	0	1125729	N.D.	23.879 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120921\
Data File : PL071351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2021 11:06
Operator : AR\AJ
Sample : M4953-03RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 12:12:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

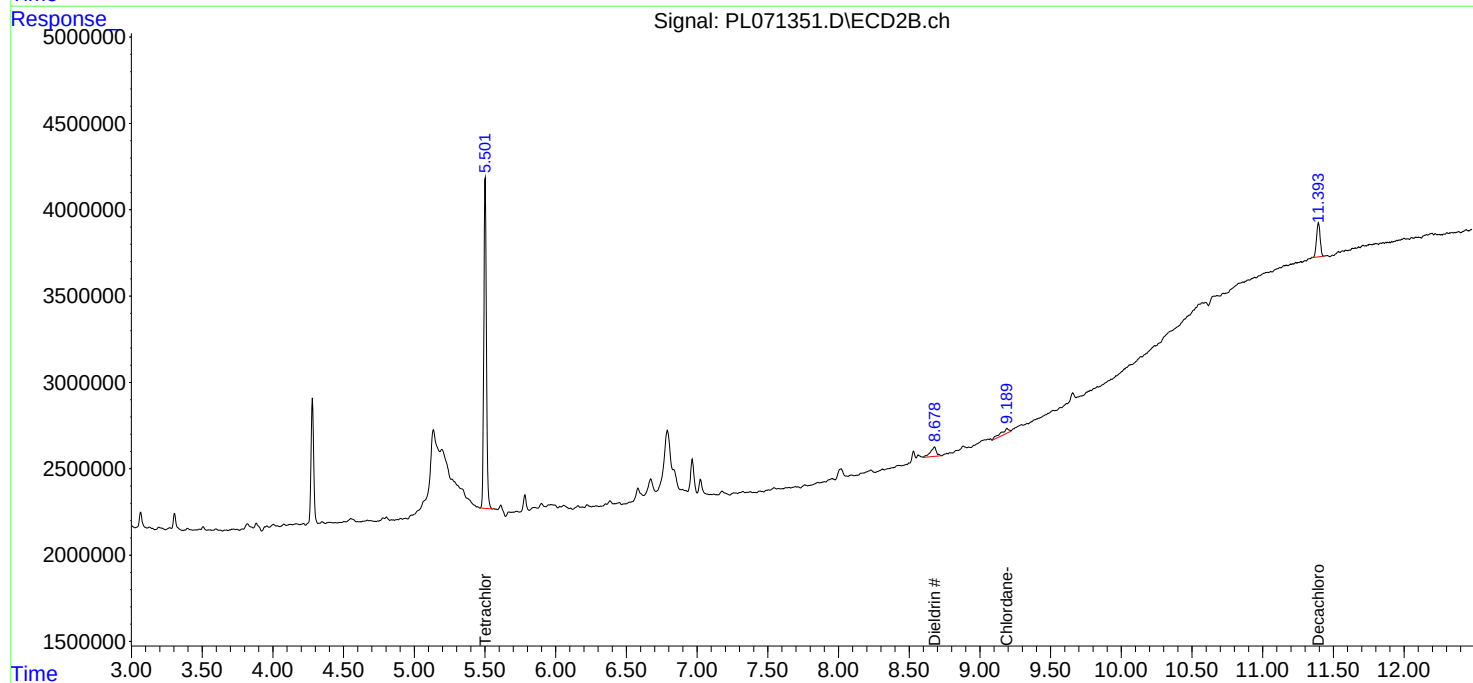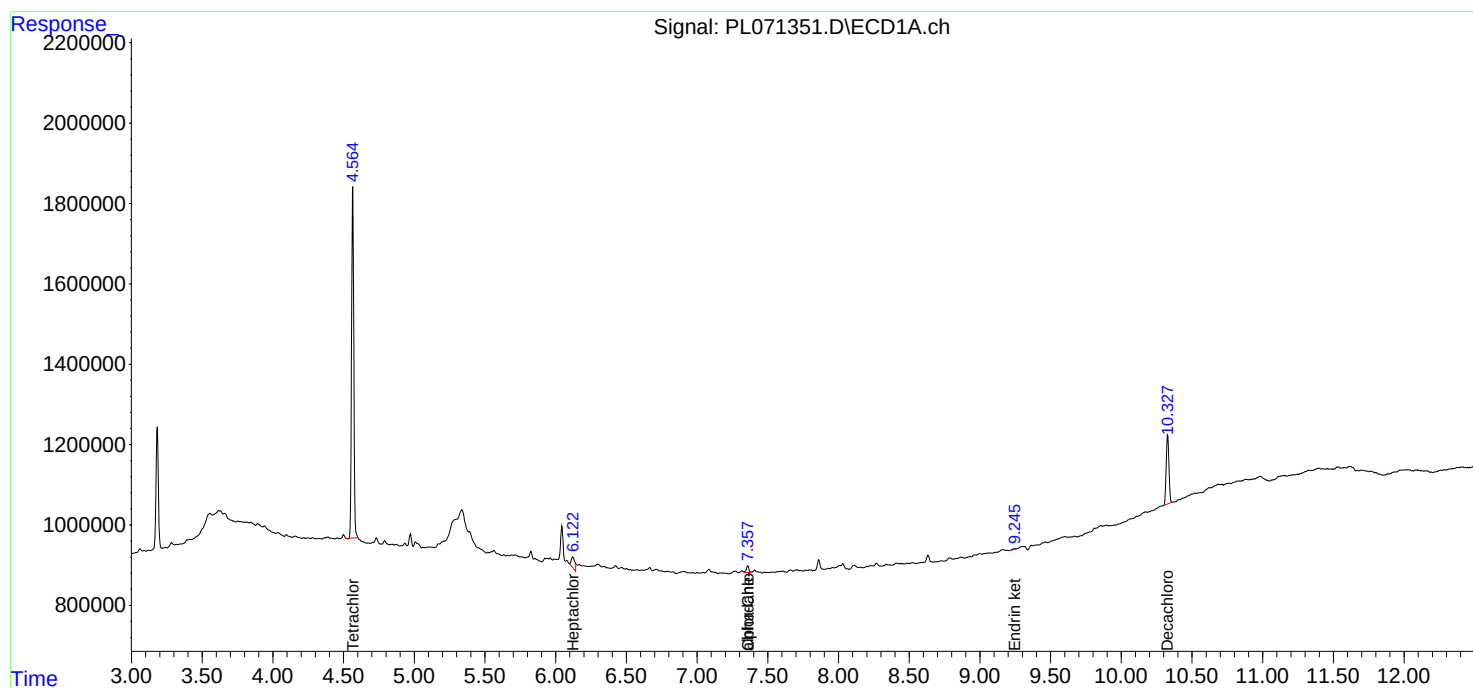


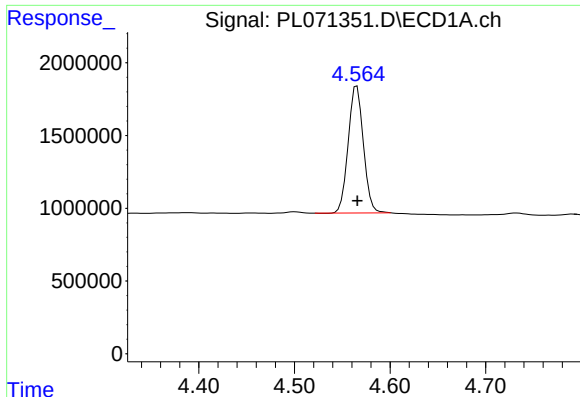

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: 0.000 min
Response: 9697404
Conc: 20.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

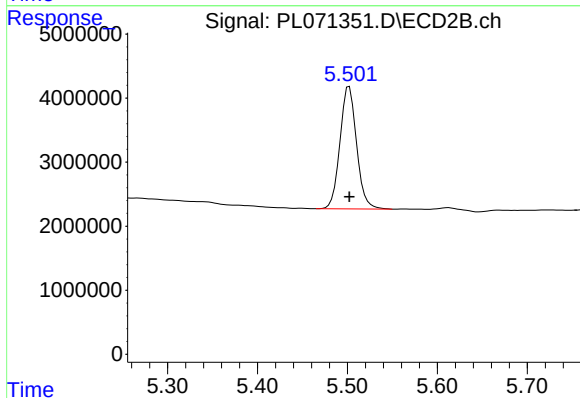


#1 Tetrachloro-m-xylene

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 24538459
Conc: 19.55 ng/ml

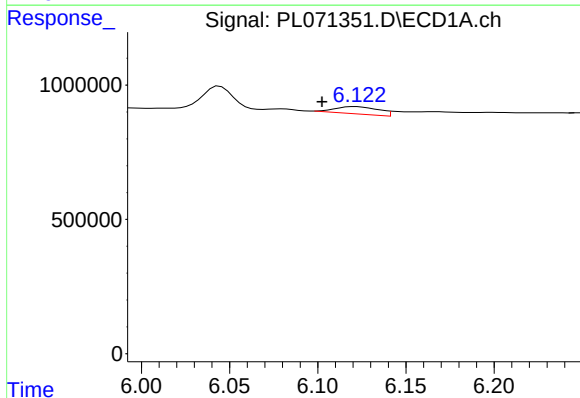


#4 Heptachlor

R.T.: 6.122 min
Delta R.T.: 0.019 min
Response: 435781
Conc: 0.63 ng/ml

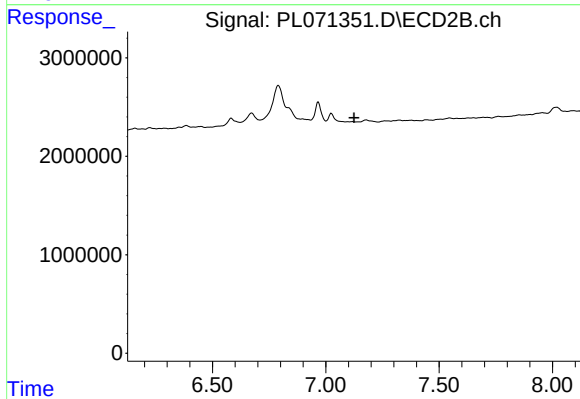

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.124 min
Response: 0
Conc: N.D.

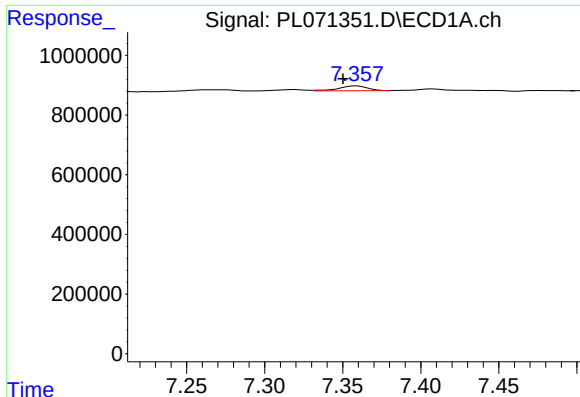

#11 alpha-Chlordane


R.T.: 7.359 min
Delta R.T.: 0.009 min
Response: 214131
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

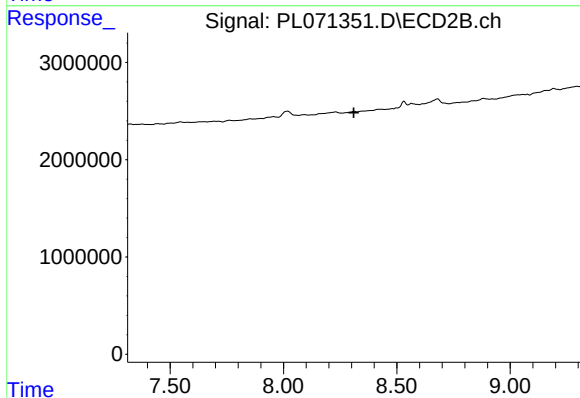


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

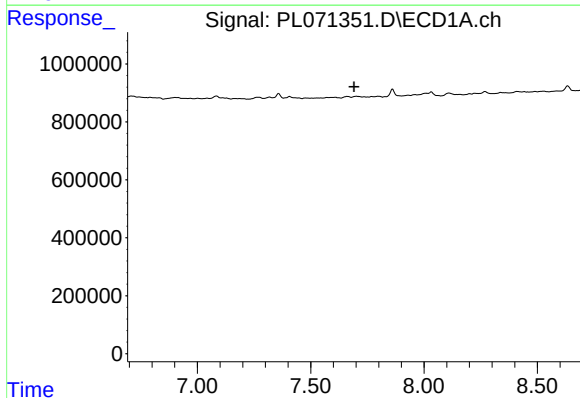


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.692 min
Response: 0
Conc: N.D.

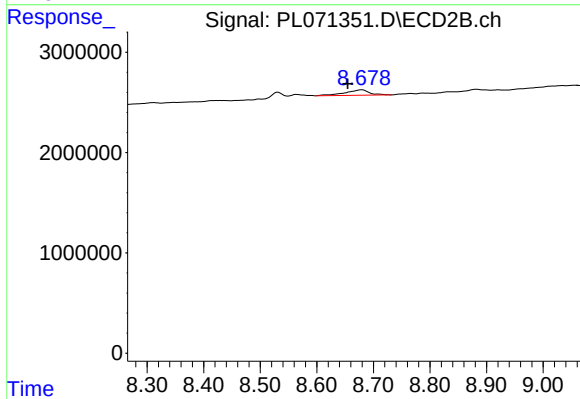

#13 Dieldrin


R.T.: 8.680 min
Delta R.T.: 0.025 min
Response: 1604323
Conc: 1.03 ng/ml

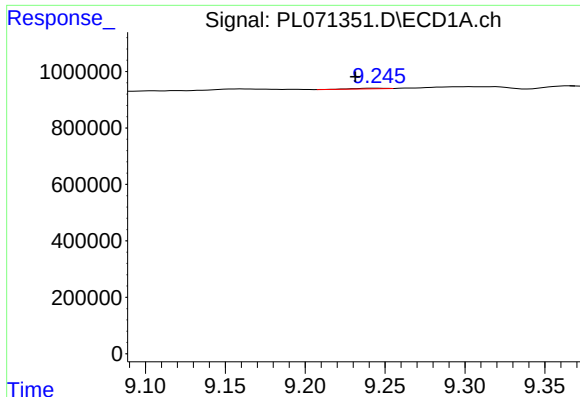

#21 Endrin ketone


R.T.: 9.246 min
Delta R.T.: 0.015 min
Response: 23684
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

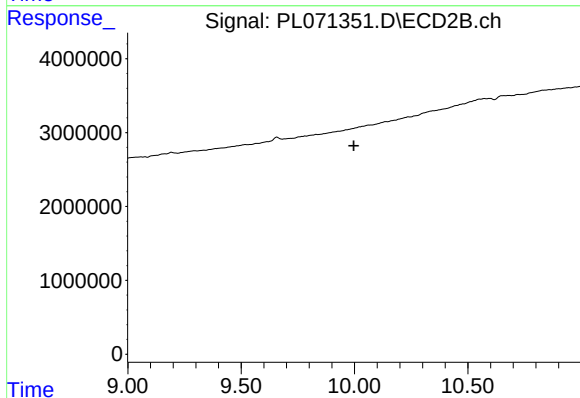


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.997 min
Response: 0
Conc: N.D.

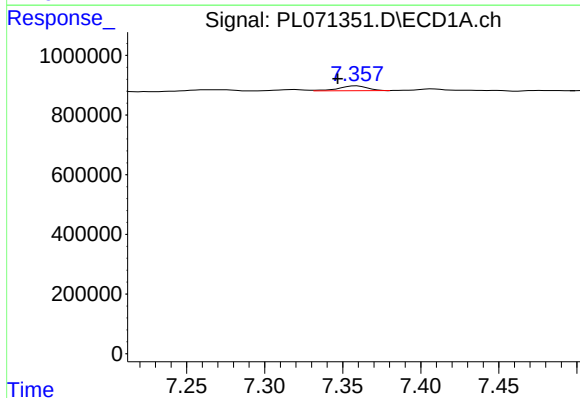


#26 Chlordane-4

R.T.: 7.359 min
Delta R.T.: 0.012 min
Response: 214131
Conc: 3.23 ng/ml

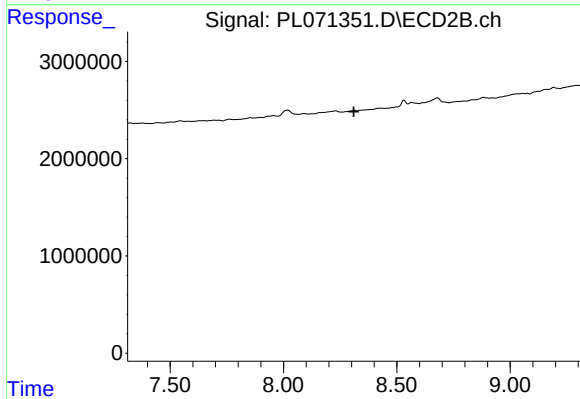

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.311 min
Response: 0
Conc: N.D.

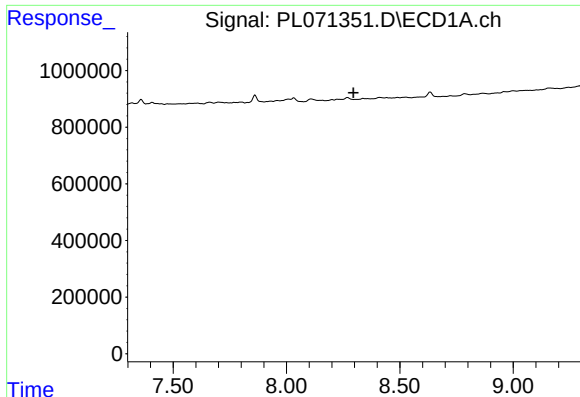

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

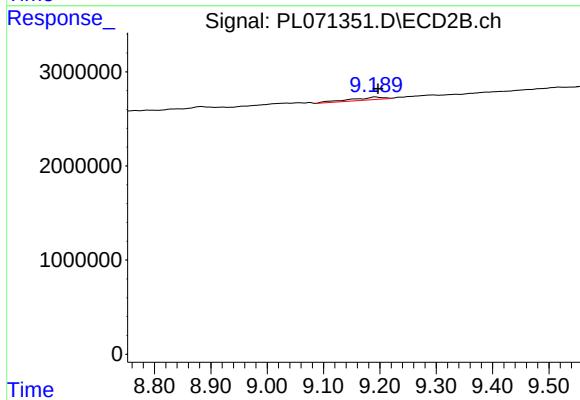


#27 Chlordane-5

R.T.: 9.192 min
Delta R.T.: -0.005 min
Response: 1125729
Conc: 23.88 ng/ml

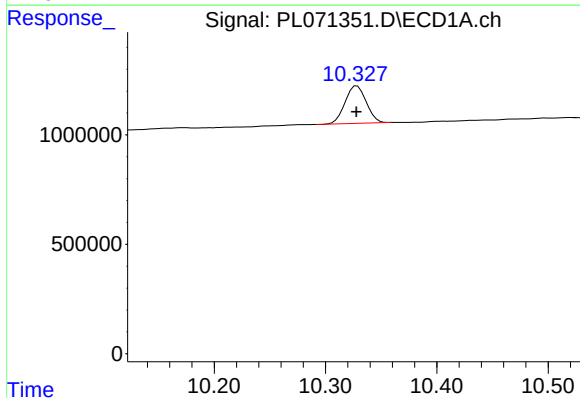

#28 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 2266091
Conc: 3.13 ng/ml

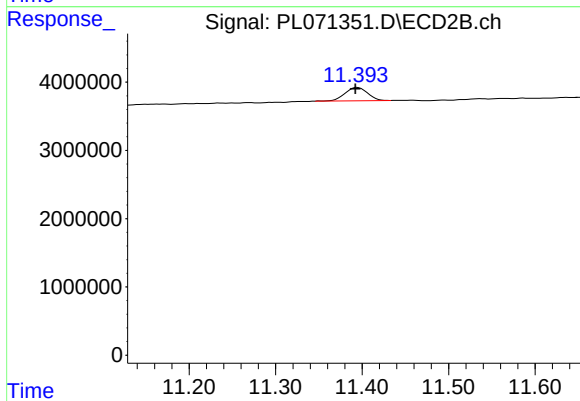

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.002 min
Response: 3514140
Conc: 2.53 ng/ml